

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072919\
 Data File : P0058503.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Jul 2019 15:35
 Operator : SM/AJ
 Sample : K4032-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S14-07-S

Manual Integrations
 APPROVED

Ankita
 7/29/2019 8:53:21 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 28 03:29:48 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jul 27 06:49:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.177	3.523	778231	722196	18.440	18.077
2) SA Decachlor...	9.671	8.413	2196383	845898	40.557m	21.430 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072919\
Data File : P0058503.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Jul 2019 15:35
Operator : SM/AJ
Sample : K4032-07
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
S14-07-S


Manual Integrations
APPROVED

Ankita
7/29/2019 8:53:21 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 28 03:29:48 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 27 06:49:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

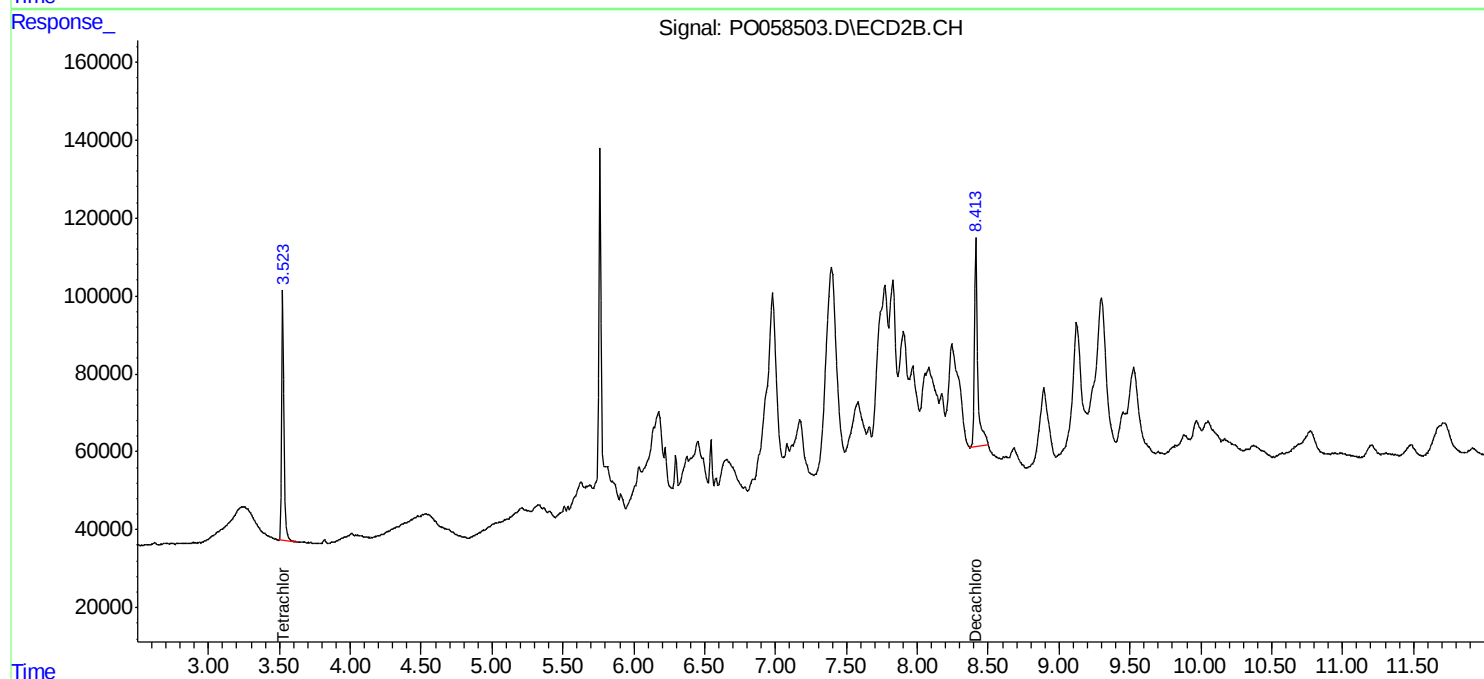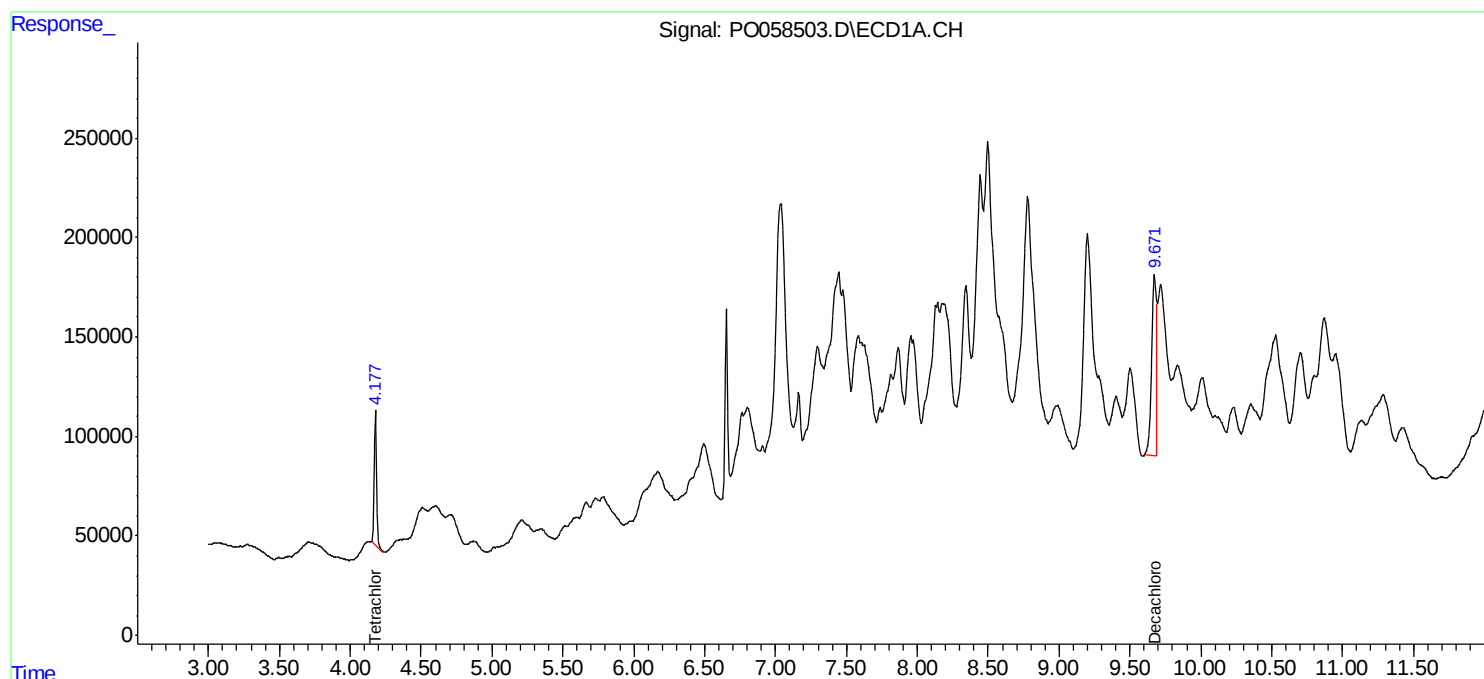

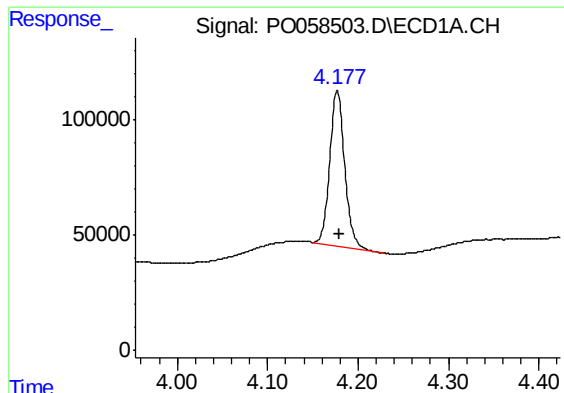


#1 Tetrachloro-m-xylene

R.T.: 4.177 min
Delta R.T.: -0.002 min
Response: 778231
Conc: 18.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
S14-07-S


Manual Integrations
APPROVED

Ankita
7/29/2019 8:53:21 AM

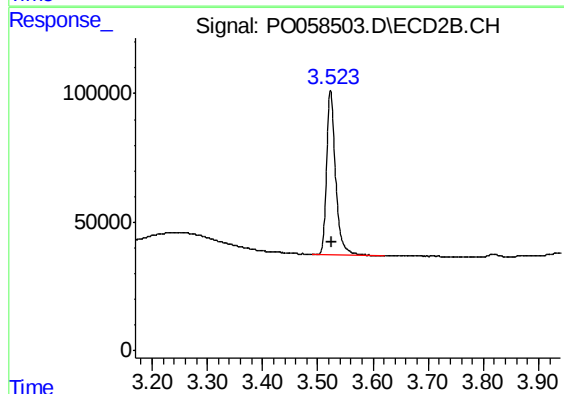


#1 Tetrachloro-m-xylene

R.T.: 3.523 min
Delta R.T.: -0.002 min
Response: 722196
Conc: 18.08 ng/ml

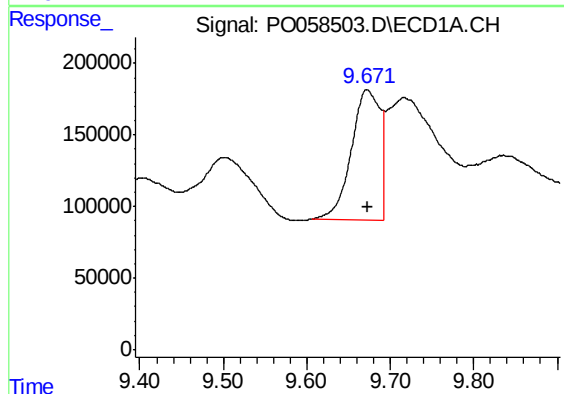

#2 Decachlorobiphenyl

R.T.: 9.671 min
Delta R.T.: -0.001 min
Response: 2196383
Conc: 40.56 ng/ml m

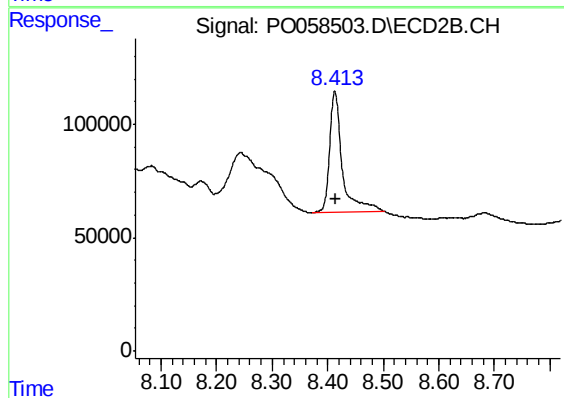

#2 Decachlorobiphenyl

R.T.: 8.413 min
Delta R.T.: -0.001 min
Response: 845898
Conc: 21.43 ng/ml