

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072920\
 Data File : P0070176.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Jul 2020 11:52
 Operator : DD\AJ
 Sample : L3436-13
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 13

Manual Integrations
 APPROVED

Ankita
 7/30/2020 1:41:27 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 29 14:14:11 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 29 12:02:56 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.378	3.561	629136	970846	17.183m	25.601m#
2) SA Decachlor...	10.015	8.757	728158	680530	12.167	13.020

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072920\
Data File : P0070176.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Jul 2020 11:52
Operator : DD\AJ
Sample : L3436-13
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
13


Manual Integrations
APPROVED

Ankita
7/30/2020 1:41:27 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 29 14:14:11 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072720.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 29 12:02:56 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

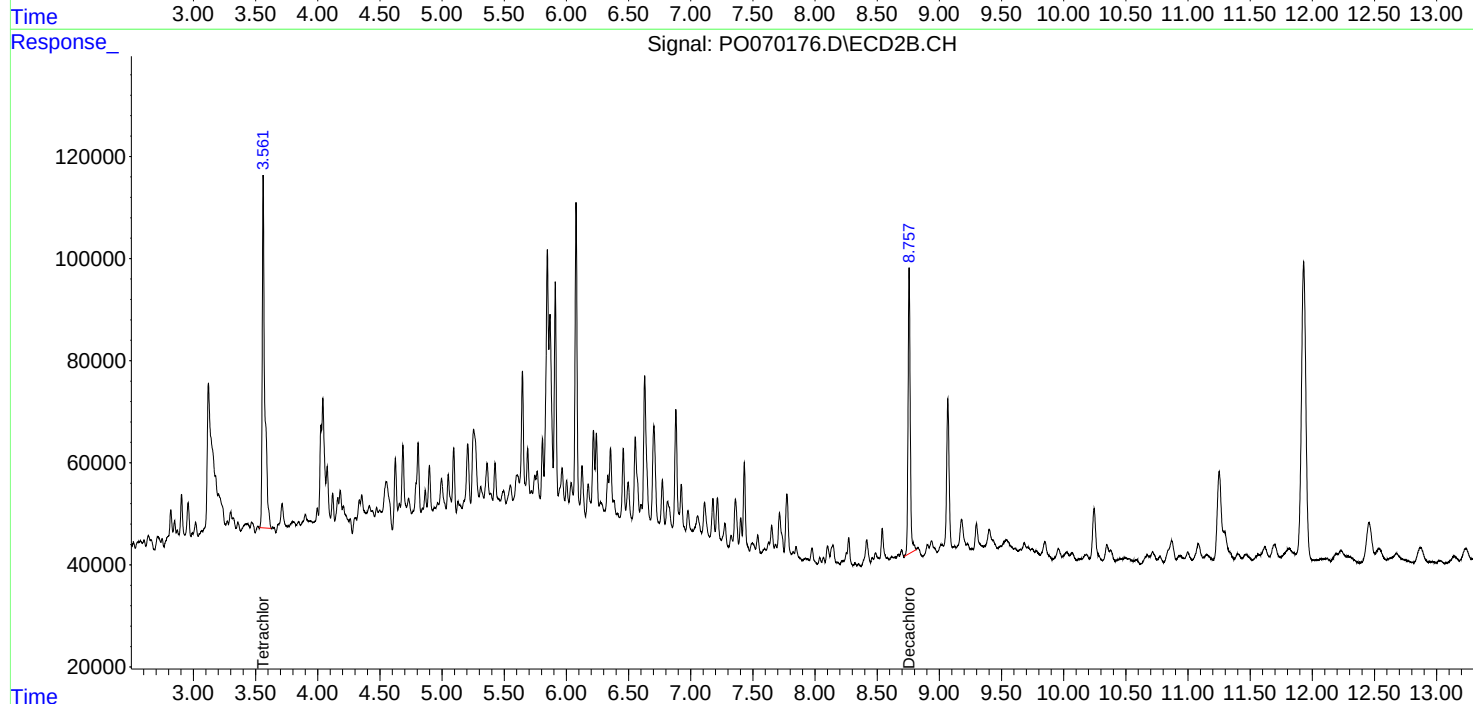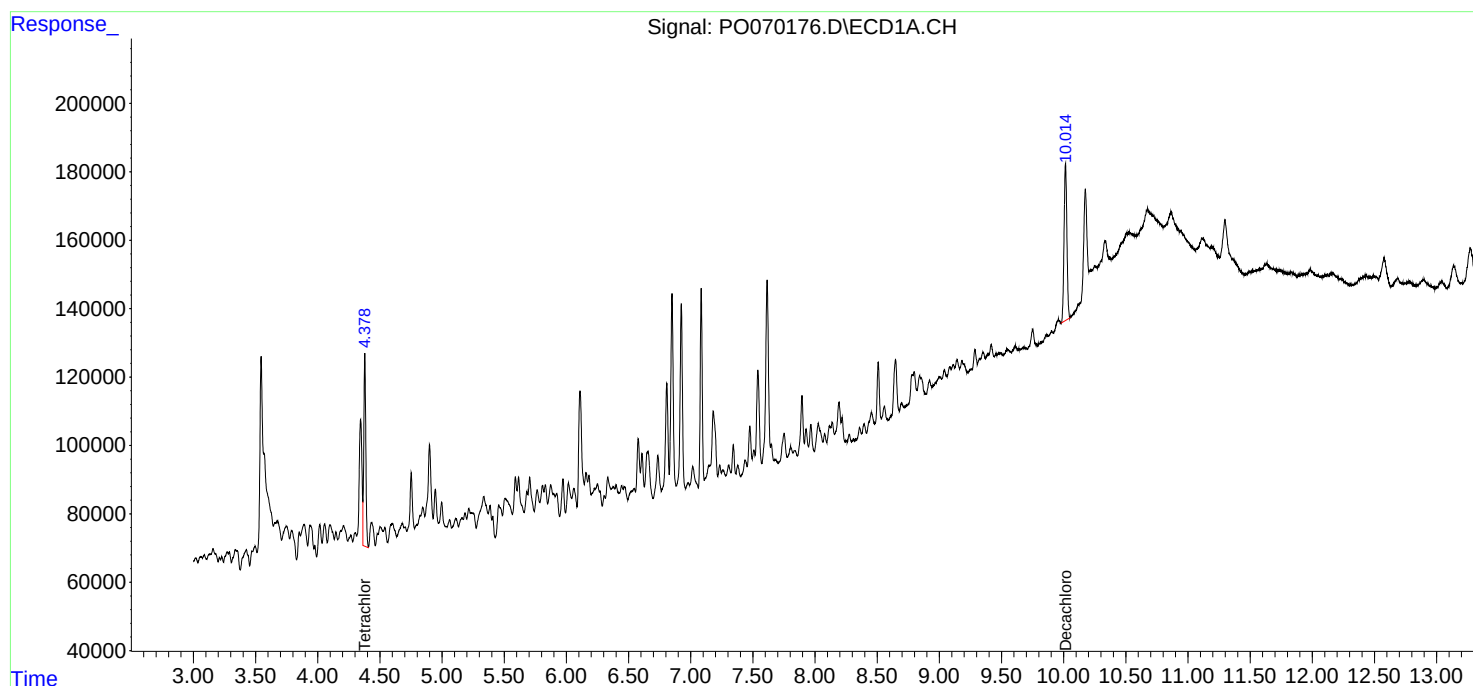

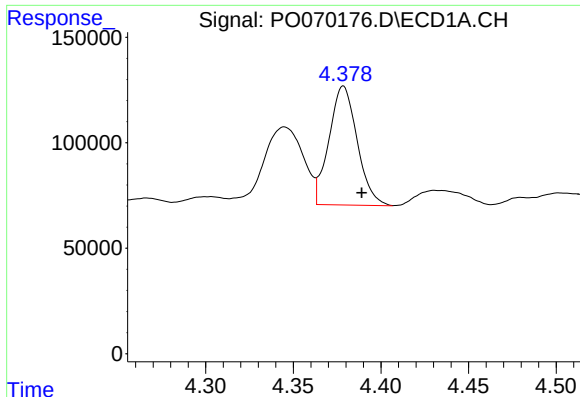


#1 Tetrachloro-m-xylene

R.T.: 4.378 min
Delta R.T.: -0.011 min
Response: 629136
Conc: 17.18 ng/ml m

Instrument :
ECD_O
ClientSampleId :
13


Manual Integrations
APPROVED

Ankita
7/30/2020 1:41:27 PM

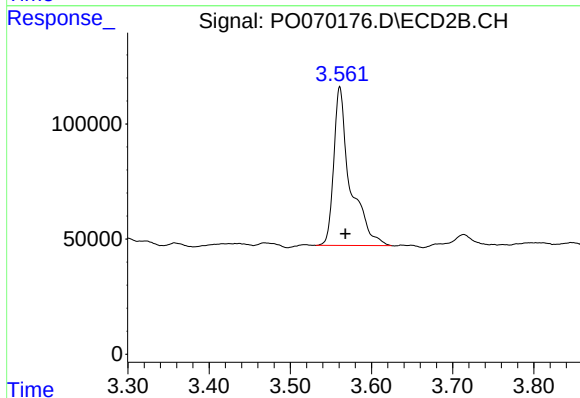


#1 Tetrachloro-m-xylene

R.T.: 3.561 min
Delta R.T.: -0.007 min
Response: 970846
Conc: 25.60 ng/ml m

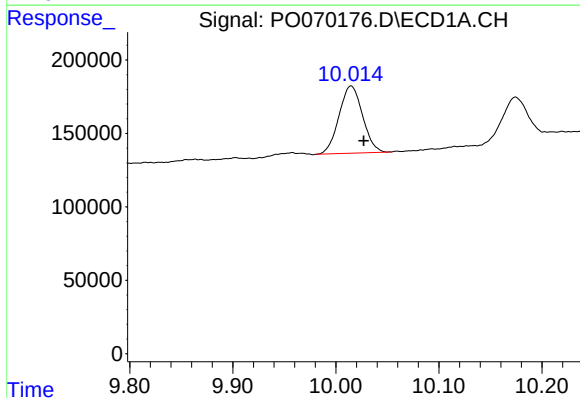

#2 Decachlorobiphenyl

R.T.: 10.015 min
Delta R.T.: -0.012 min
Response: 728158
Conc: 12.17 ng/ml

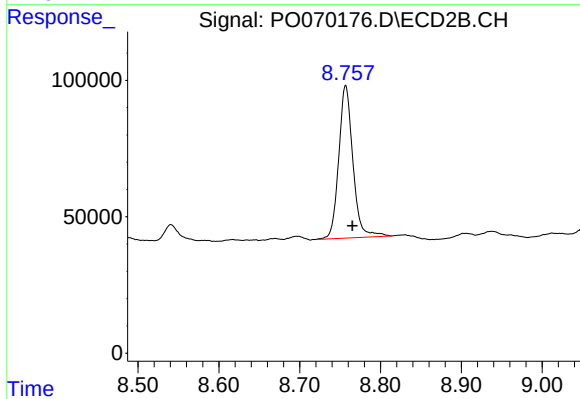

#2 Decachlorobiphenyl

R.T.: 8.757 min
Delta R.T.: -0.008 min
Response: 680530
Conc: 13.02 ng/ml