

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072921\
 Data File : P0079947.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Jul 2021 16:05
 Operator : DD\AJ
 Sample : M3210-04
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-4(1.0-2.0)

Manual Integrations
 APPROVED

mohammad
 7/30/2021 2:25:06 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 30 02:56:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 28 18:45:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.001	4.119	1492036	552068	24.761	24.107
2) SA Decachlor...	11.111	9.527	1162038	513070	24.772m	24.689m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072921\
Data File : P0079947.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Jul 2021 16:05
Operator : DD\AJ
Sample : M3210-04
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB-4(1.0-2.0)


Manual Integrations
APPROVED

mohammad
7/30/2021 2:25:06 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 30 02:56:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072821.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 28 18:45:36 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

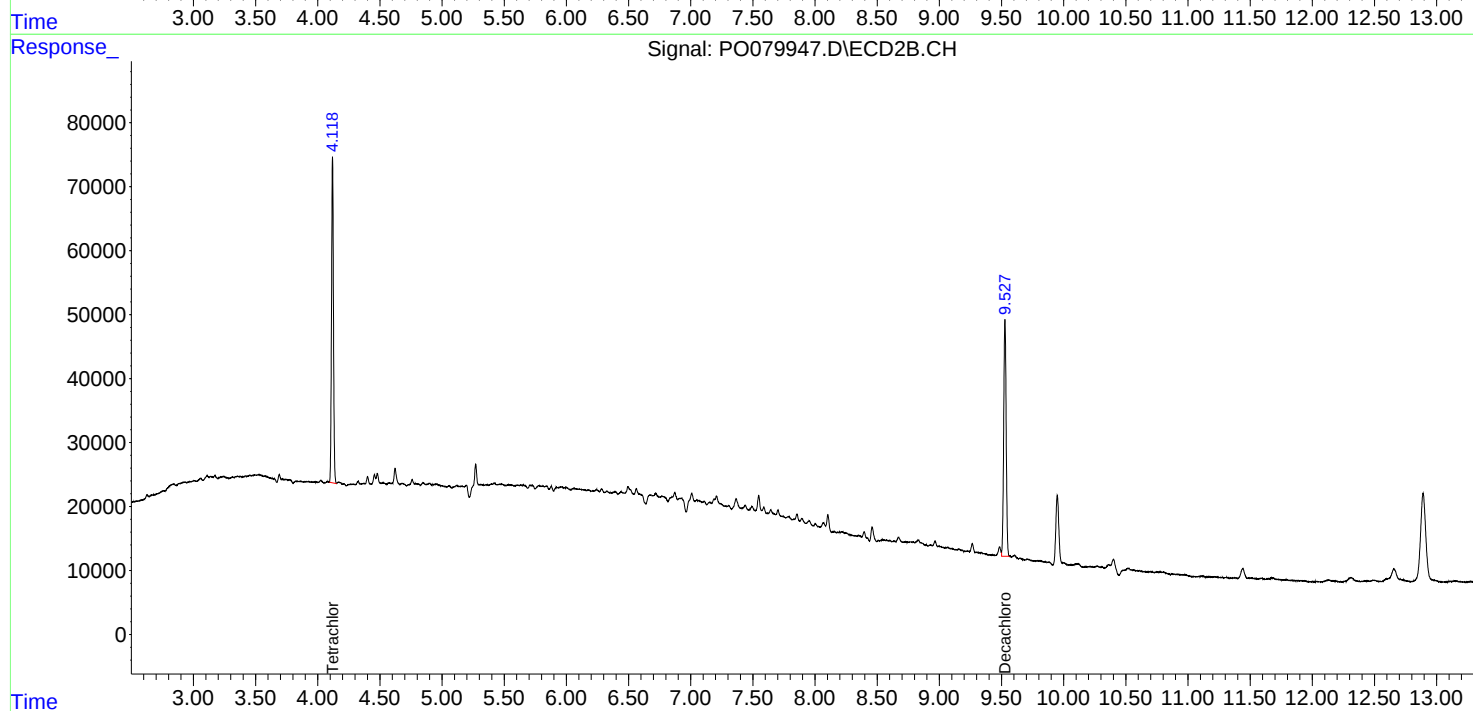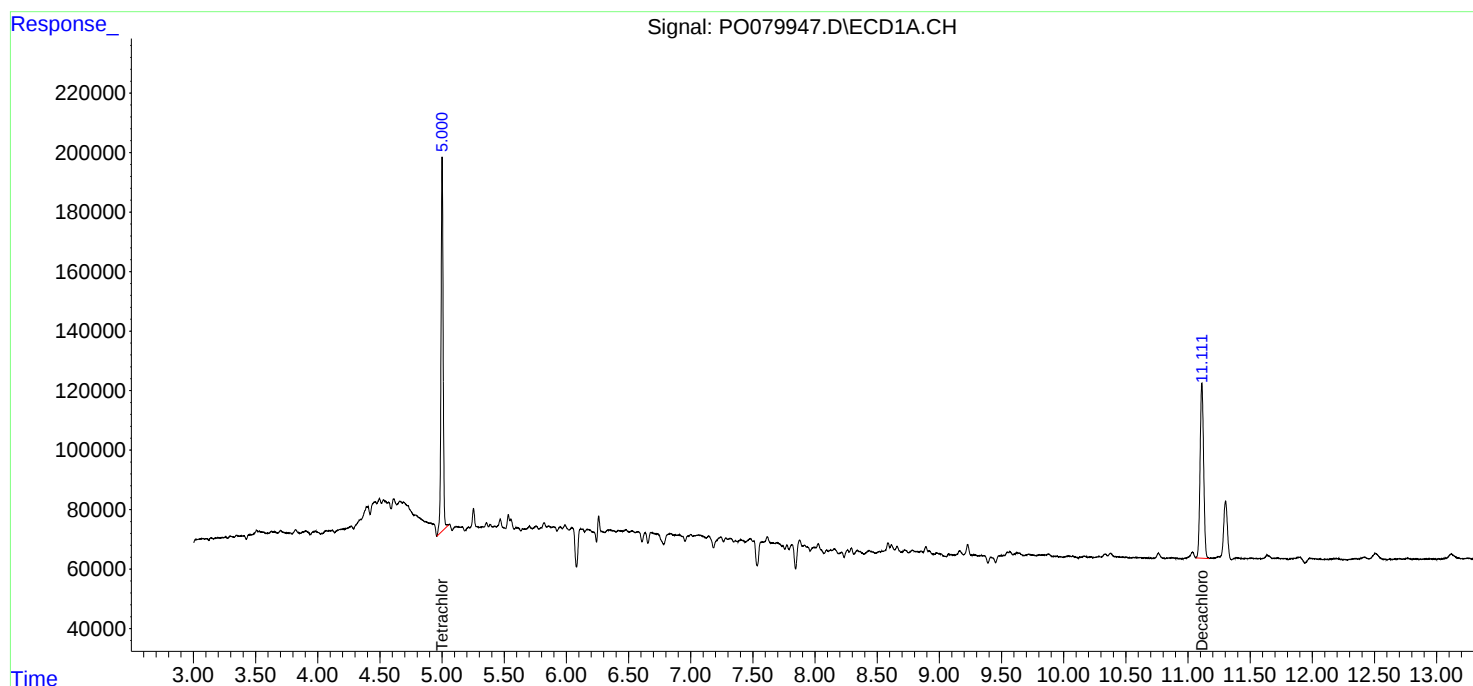

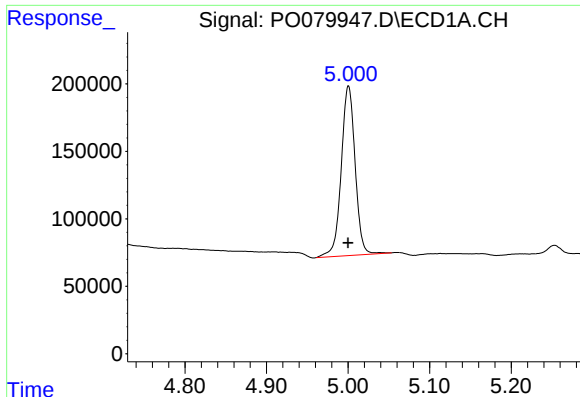


#1 Tetrachloro-m-xylene

R.T.: 5.001 min
Delta R.T.: 0.000 min
Response: 1492036
Conc: 24.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-4(1.0-2.0)


Manual Integrations
APPROVED

mohammad
7/30/2021 2:25:06 PM

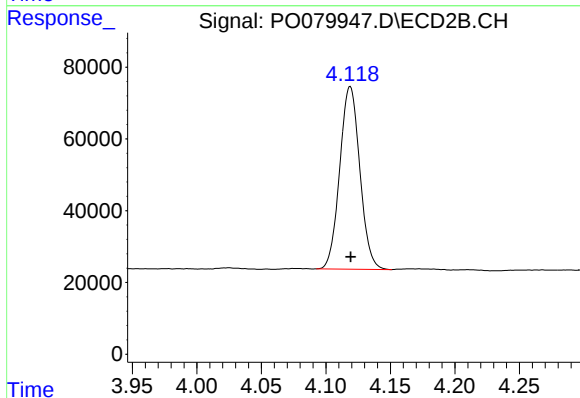


#1 Tetrachloro-m-xylene

R.T.: 4.119 min
Delta R.T.: 0.000 min
Response: 552068
Conc: 24.11 ng/ml

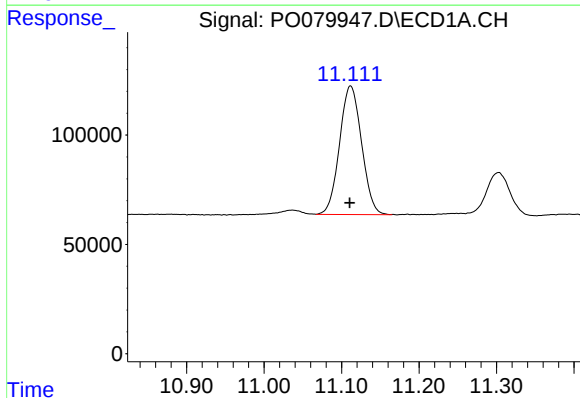

#2 Decachlorobiphenyl

R.T.: 11.111 min
Delta R.T.: 0.000 min
Response: 1162038
Conc: 24.77 ng/ml m

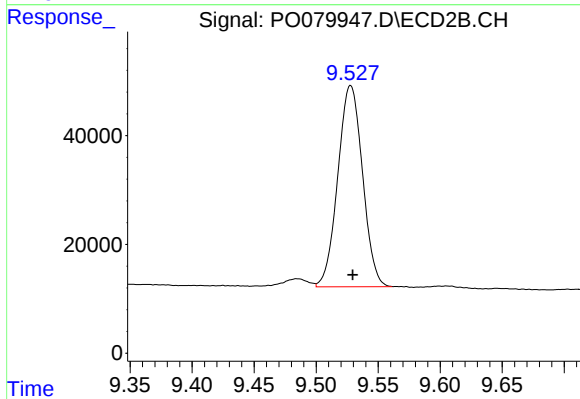

#2 Decachlorobiphenyl

R.T.: 9.527 min
Delta R.T.: -0.002 min
Response: 513070
Conc: 24.69 ng/ml m