

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072921\
 Data File : P0079964.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Jul 2021 21:17
 Operator : DD\AJ
 Sample : M3222-01
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MH-458-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 30 03:03:40 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 28 18:45:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.001	4.119	1409048	601596	23.384	26.269
2) SA Decachlor...	11.114	9.528	944493	402635	20.134	19.375

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072921\
Data File : P0079964.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Jul 2021 21:17
Operator : DD\AJ
Sample : M3222-01
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MH-458-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 30 03:03:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072821.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 28 18:45:36 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

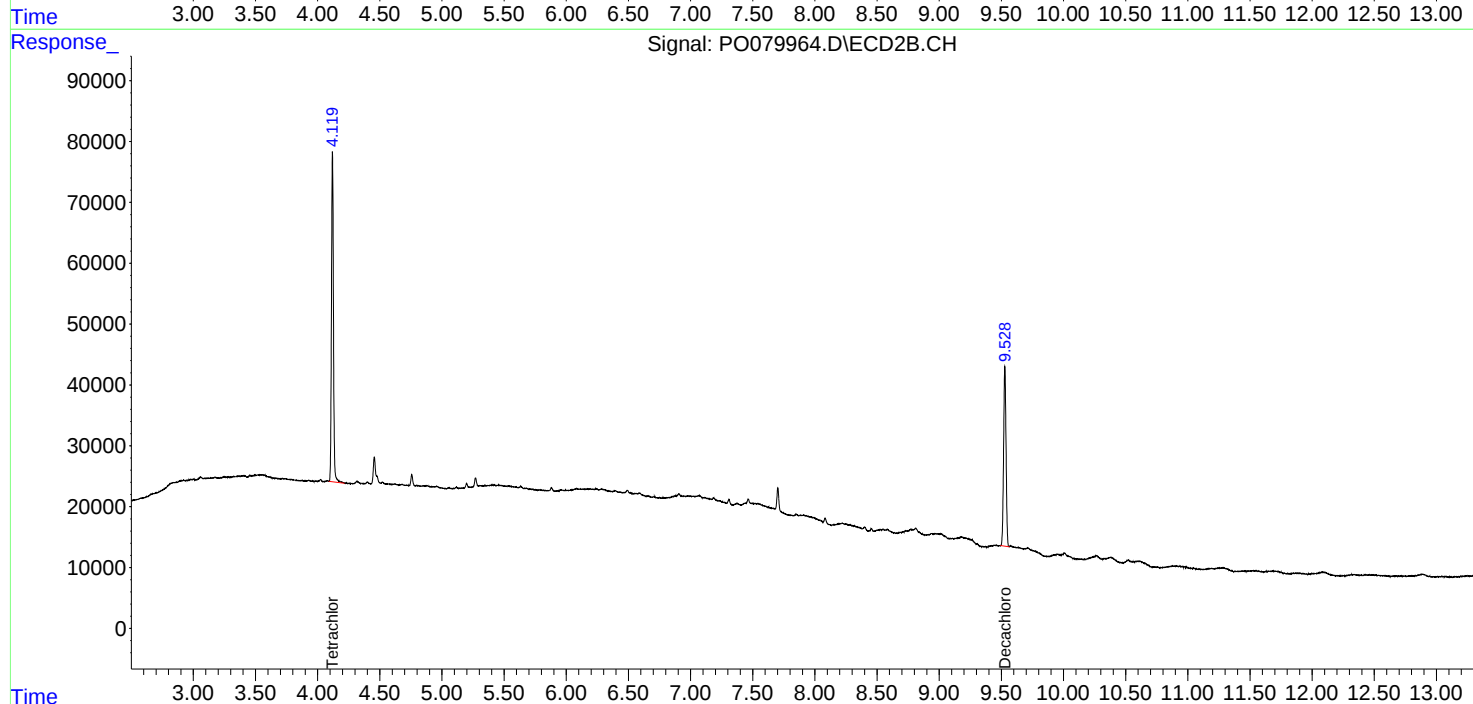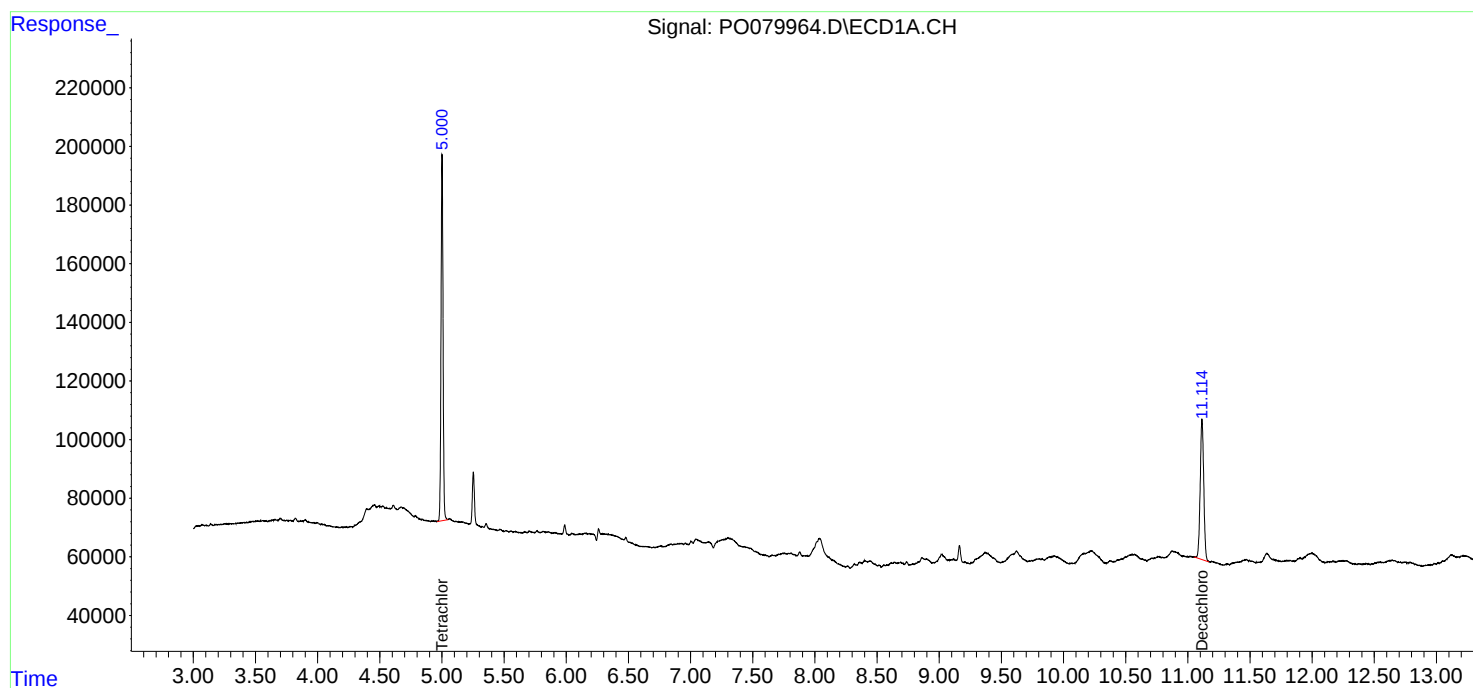


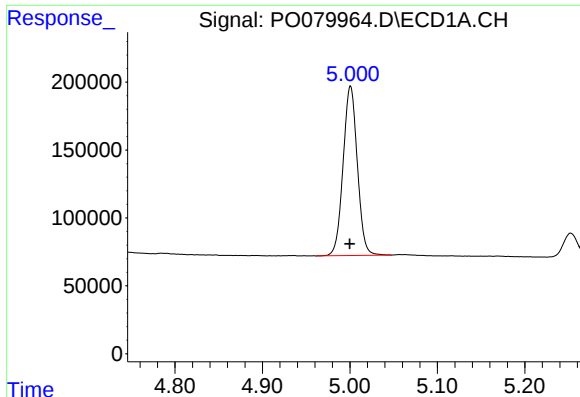

#1 Tetrachloro-m-xylene


R.T.: 5.001 min
Delta R.T.: 0.000 min
Response: 1409048
Conc: 23.38 ng/ml

Instrument :
ECD_O
ClientSampleId :
MH-458-COMP

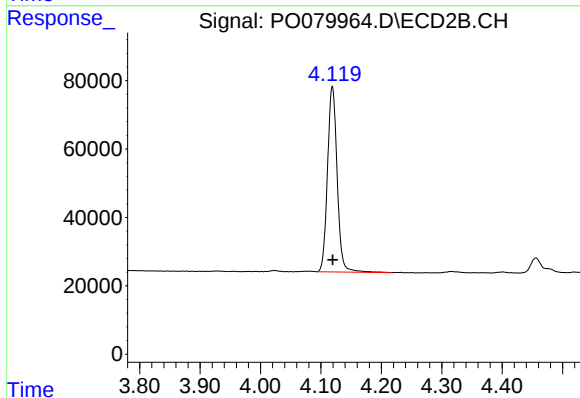


#1 Tetrachloro-m-xylene

R.T.: 4.119 min
Delta R.T.: 0.000 min
Response: 601596
Conc: 26.27 ng/ml

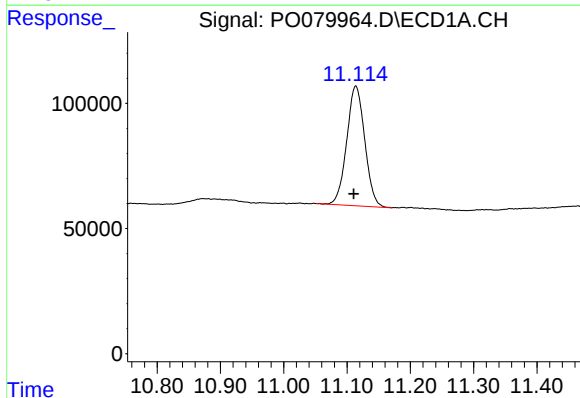

#2 Decachlorobiphenyl

R.T.: 11.114 min
Delta R.T.: 0.003 min
Response: 944493
Conc: 20.13 ng/ml

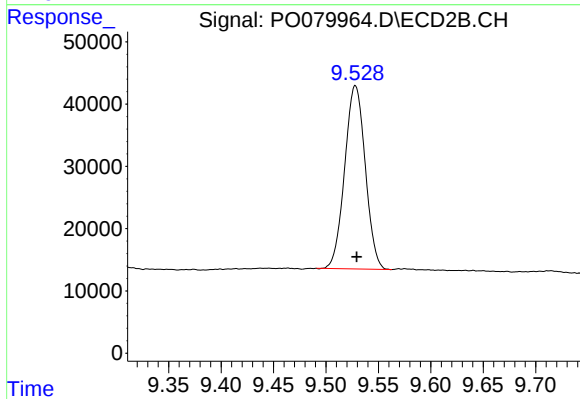

#2 Decachlorobiphenyl

R.T.: 9.528 min
Delta R.T.: -0.001 min
Response: 402635
Conc: 19.37 ng/ml