

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072921\
 Data File : P0079971.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Jul 2021 23:18
 Operator : DD\AJ
 Sample : M3216-11
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SPLP-LEACHATE-AMENDED-COM-

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 30 03:06:16 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 28 18:45:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.001	4.119	1369134	527107	22.721	23.017
2)	SA Decachlor...	11.114	9.528	694987	308447	14.815	14.842

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072921\
Data File : P0079971.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Jul 2021 23:18
Operator : DD\AJ
Sample : M3216-11
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SPLP-LEACHATE-AMENDED-COM-

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 30 03:06:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072821.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 28 18:45:36 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

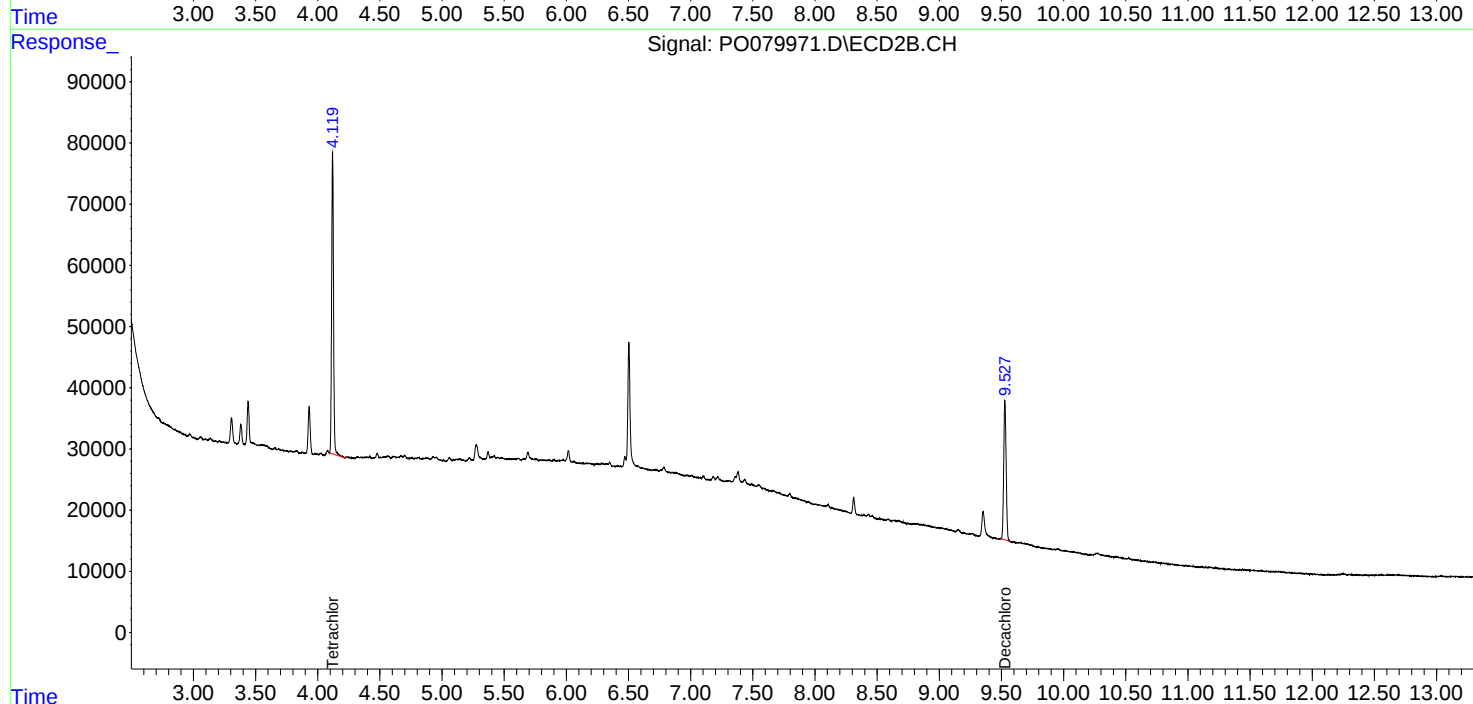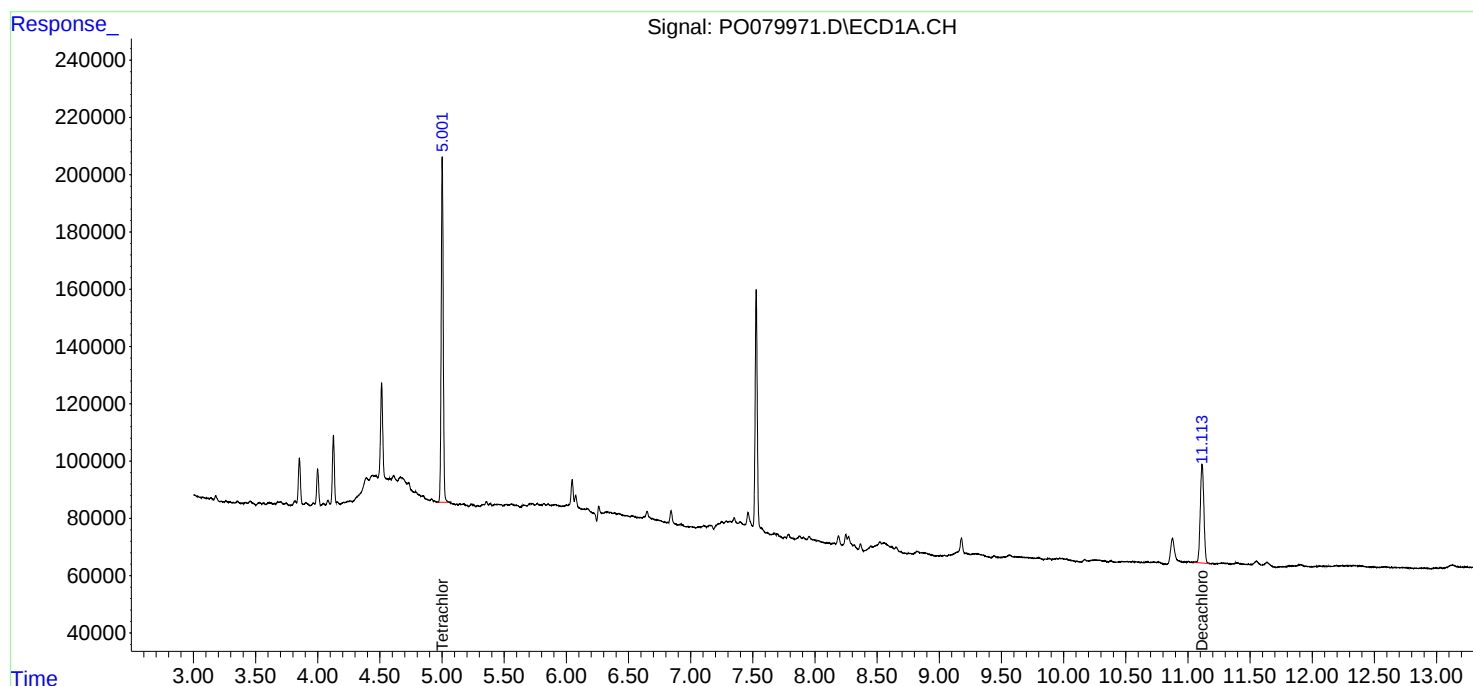


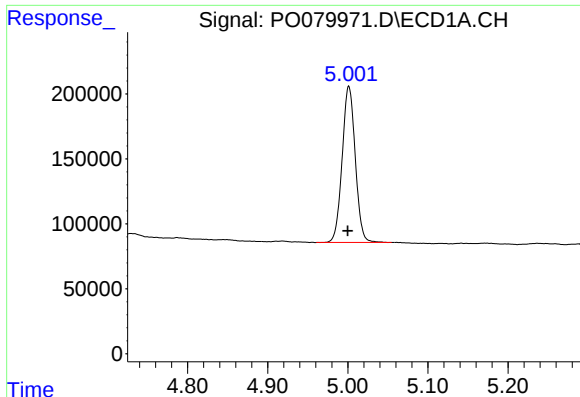

#1 Tetrachloro-m-xylene


R.T.: 5.001 min
Delta R.T.: 0.001 min
Response: 1369134
Conc: 22.72 ng/ml

Instrument :
ECD_O
ClientSampleId :
SPLP-LEACHATE-AMENDED-COM-

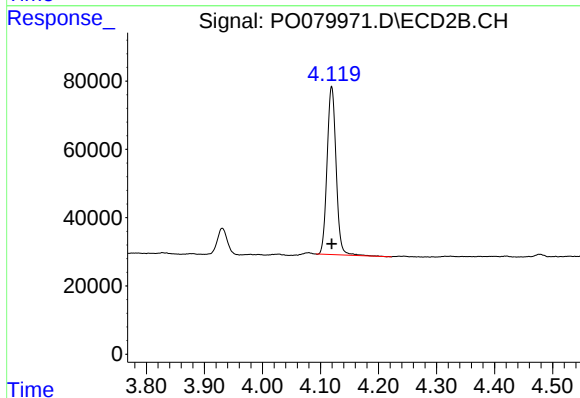


#1 Tetrachloro-m-xylene

R.T.: 4.119 min
Delta R.T.: 0.000 min
Response: 527107
Conc: 23.02 ng/ml

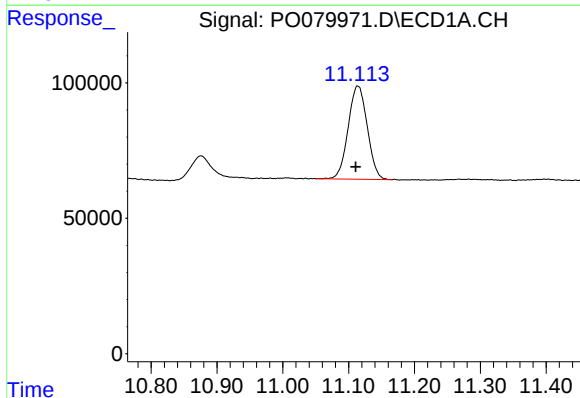

#2 Decachlorobiphenyl

R.T.: 11.114 min
Delta R.T.: 0.003 min
Response: 694987
Conc: 14.82 ng/ml

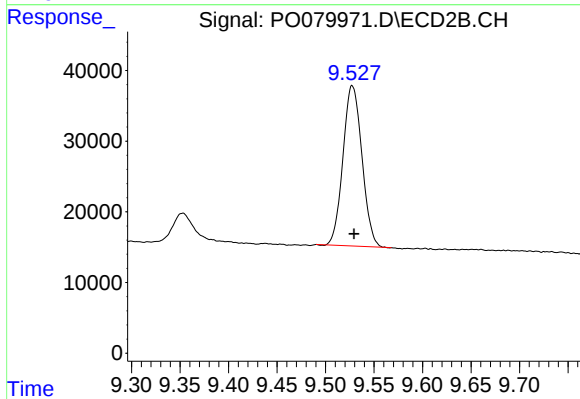

#2 Decachlorobiphenyl

R.T.: 9.528 min
Delta R.T.: -0.002 min
Response: 308447
Conc: 14.84 ng/ml