

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072922\
 Data File : P0088440.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jul 2022 14:59
 Operator : YP/AJ
 Sample : N3927-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 RVE-80

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/01/2022
 Supervised By :Ankita Jodhani 08/01/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 29 22:27:17 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 26 11:20:17 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.444	3.603	83494065	30219817	32.728	32.030m
2) SA Decachlor...	10.286	8.596	57140532	34390507	26.906	32.909

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072922\
Data File : P0088440.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jul 2022 14:59
Operator : YP/AJ
Sample : N3927-07
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
RVE-80


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/01/2022
Supervised By :Ankita Jodhani 08/01/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 29 22:27:17 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071422.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 26 11:20:17 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

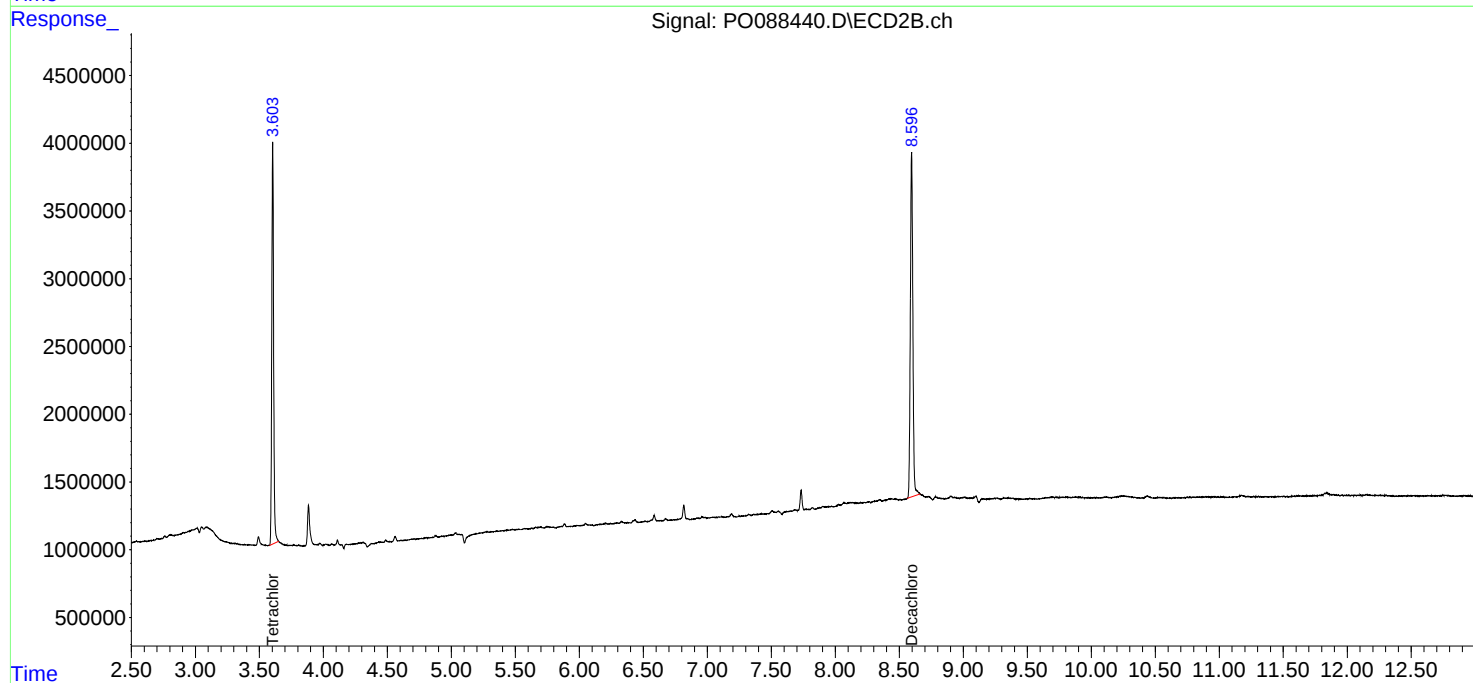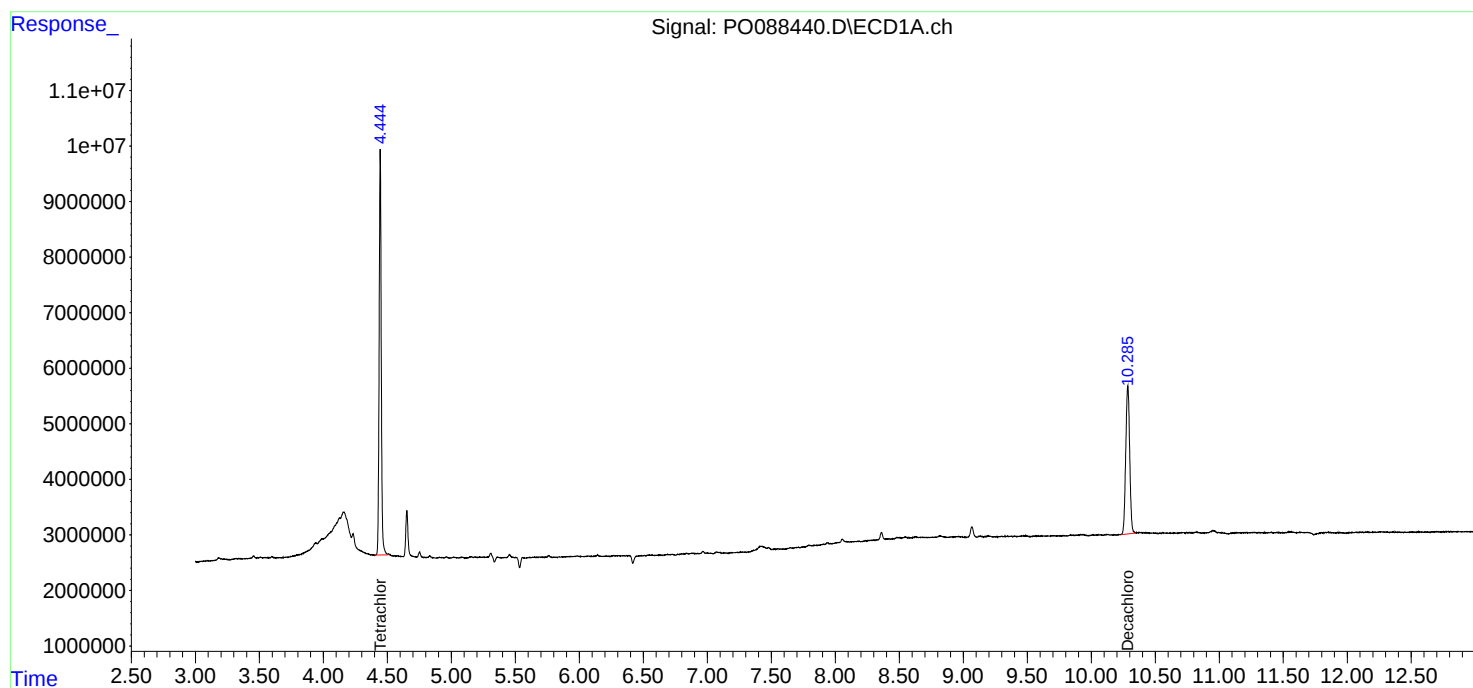

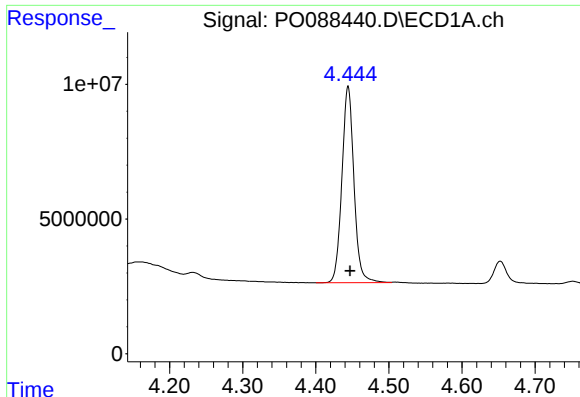


#1 Tetrachloro-m-xylene

R.T.: 4.444 min
Delta R.T.: -0.003 min
Response: 83494065
Conc: 32.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
RVE-80


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/01/2022
Supervised By :Ankita Jodhani 08/01/2022

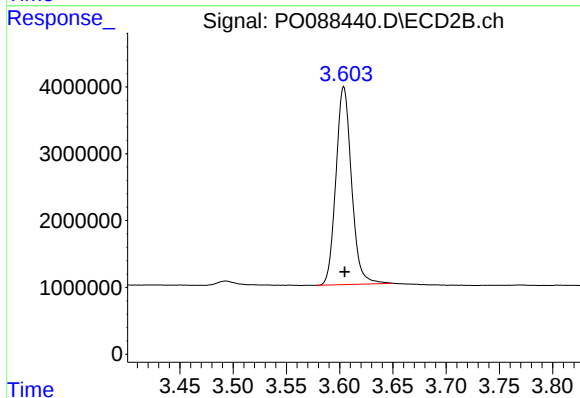


#1 Tetrachloro-m-xylene

R.T.: 3.603 min
Delta R.T.: -0.001 min
Response: 30219817
Conc: 32.03 ng/ml m

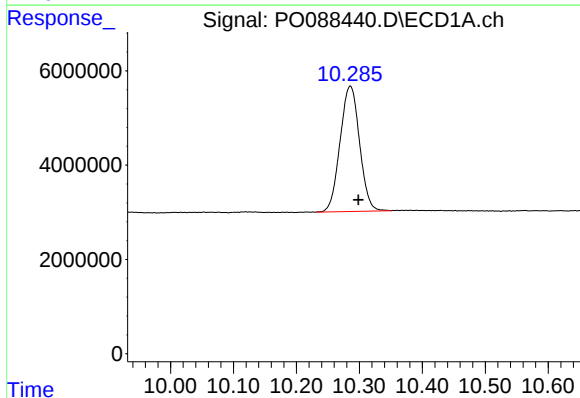

#2 Decachlorobiphenyl

R.T.: 10.286 min
Delta R.T.: -0.013 min
Response: 57140532
Conc: 26.91 ng/ml

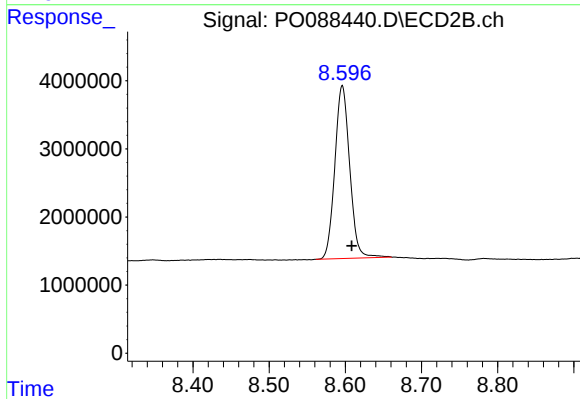

#2 Decachlorobiphenyl

R.T.: 8.596 min
Delta R.T.: -0.012 min
Response: 34390507
Conc: 32.91 ng/ml