

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072925\
 Data File : P0112571.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jul 2025 10:28
 Operator : YP/AJ
 Sample : DDT ANALOG
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 DDT ANALOG

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 30 01:45:02 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 24 04:54:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	0.000	3.661	0	17181	N.D.	0.003 #
2)	SA Decachlor...	8.693	8.638	177479	125054	0.024	0.071 #
Target Compounds							
3)	L1 AR-1016-1	4.765	4.741	122448	202806	0.456	1.159 #
4)	L1 AR-1016-2	4.765	4.755	122448	223580	0.302	0.858 #
5)	L1 AR-1016-3	4.825	4.936	425863	417529	1.627	3.071 #
6)	L1 AR-1016-4	4.947	4.975	1180702	832856	5.574	7.497 #
7)	L1 AR-1016-5	5.200	5.186	2147070	519755	9.783	3.627 #
8)	L2 AR-1221-1	0.000	3.866	0	103098	N.D.	1.533 #
9)	L2 AR-1221-2	0.000	3.961	0	255905	N.D.	5.045 #
10)	L2 AR-1221-3	4.100f	4.036	1322166	103228	5.562	0.651 #
11)	L3 AR-1232-1	4.100f	4.036	1322166	103228	7.071	0.816 #
12)	L3 AR-1232-2	4.548	4.755	619083	223580	5.752	1.705 #
13)	L3 AR-1232-3	4.765	4.936	122448	417529	0.592	6.214 #
14)	L3 AR-1232-4	4.947	5.022	1180702	553201	11.273	9.246
15)	L3 AR-1232-5	4.957f	5.186	2016670	519755	29.709	7.971 #
16)	L4 AR-1242-1	4.765	4.741	122448	202806	0.495	1.280 #
17)	L4 AR-1242-2	4.765	4.755	122448	223580	0.331	0.957 #
18)	L4 AR-1242-3	4.825	4.936	425863	417529	1.799	3.445 #
19)	L4 AR-1242-4	4.947	5.022	1180702	553201	6.077	4.507 #
20)	L4 AR-1242-5	5.595	5.520	2722397	2101046	12.727	13.052
21)	L5 AR-1248-1	4.765	4.741	122448	202806	0.654	1.669 #
22)	L5 AR-1248-2	4.957f	4.975	2016670	832856	7.905	4.920 #
23)	L5 AR-1248-3	5.200	5.022	2147070	553201	6.247	3.114 #
24)	L5 AR-1248-4	5.550	5.186	7427466	519755	14.619	2.495 #
25)	L5 AR-1248-5	5.595	5.580	2722397	3702513	7.787	17.240 #
26)	L6 AR-1254-1	5.550	5.520	7427466	2101046	13.530	6.394 #
27)	L6 AR-1254-2	5.700	5.702	1932863	12528348	3.978	43.277 #
28)	L6 AR-1254-3	6.104	6.099	108739	14547739	0.146	34.033 #
29)	L6 AR-1254-4	6.354	6.327	1170561	1624652	2.129	5.952 #
30)	L6 AR-1254-5	6.759	6.724	4207.1E6	2028.3E6	5943.653	6072.541
31)	L7 AR-1260-1	6.247	6.209	208047	1206884	0.474	4.856 #
32)	L7 AR-1260-2	6.438	6.403	5250397	3418437	7.633	10.375 #
33)	L7 AR-1260-3	6.759f	0.000	4207.1E6	0	7154.629	N.D. #
34)	L7 AR-1260-4	7.066	7.032	1964458	2451628	4.356	12.815 #
35)	L7 AR-1260-5	7.301	7.246	4587768	1679653	3.702	4.075
36)	L8 AR-1262-1	6.759f	6.724f	4207.1E6	2028.3E6	4527.579	4889.612
37)	L8 AR-1262-2	7.301	7.246	4587768	1679653	3.085	3.258
38)	L8 AR-1262-3	7.588	7.561	103658	525394	0.176	2.817 #
39)	L8 AR-1262-4	7.680	7.632	486306	59258	0.489	0.206 #
40)	L8 AR-1262-5	8.135	0.000	3963645	0	9.132	N.D. #
41)	L9 AR-1268-1	7.588	7.561	103658	525394	0.059	1.015 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072925\
 Data File : P0112571.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jul 2025 10:28
 Operator : YP/AJ
 Sample : DDT ANALOG
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DDT ANALOG

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 30 01:45:02 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 24 04:54:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	7.680	7.632	486306	59258	0.330	0.139 #
43) L9	AR-1268-3	7.838	7.856f	220578	17726	0.176	0.055 #
44) L9	AR-1268-4	8.135	0.000	3963645	0	8.226	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO072925\
Data File : PO112571.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jul 2025 10:28
Operator : YP/AJ
Sample : DDT ANALOG
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 30 01:45:02 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072325.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 24 04:54:06 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

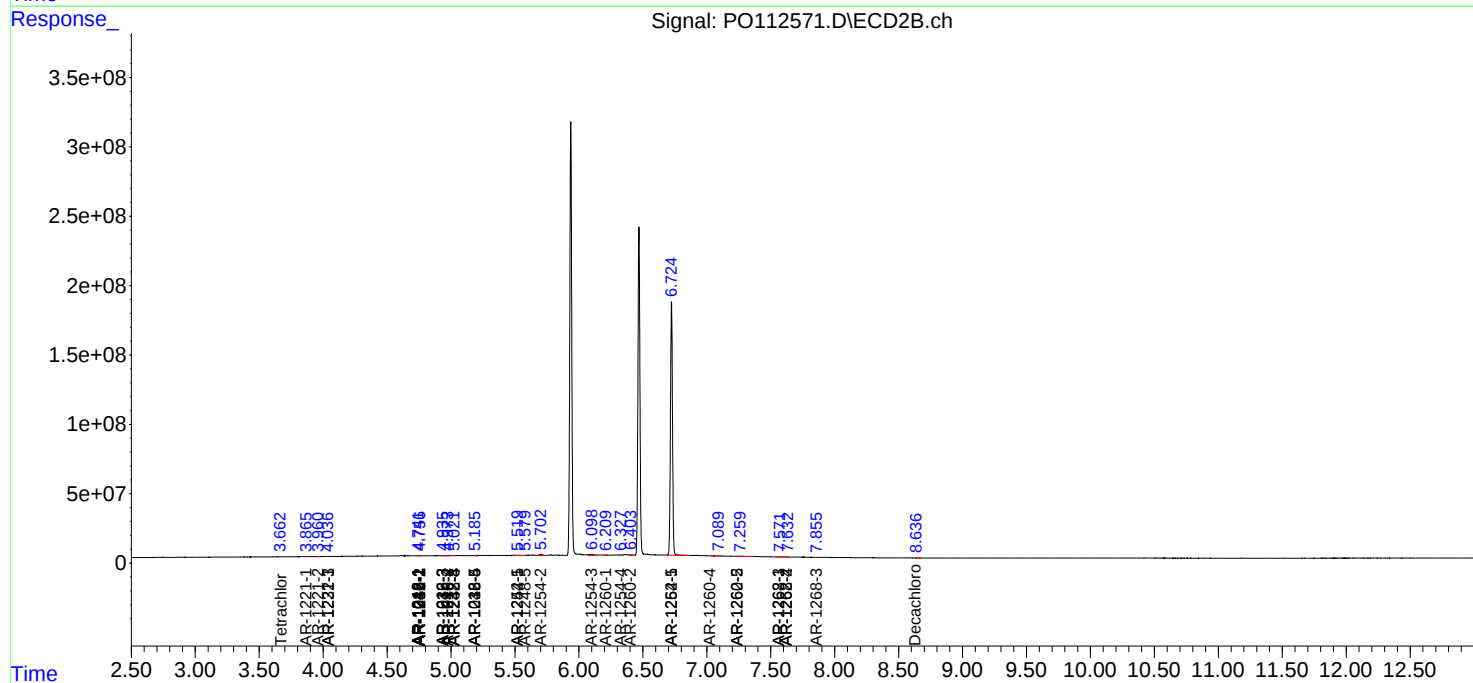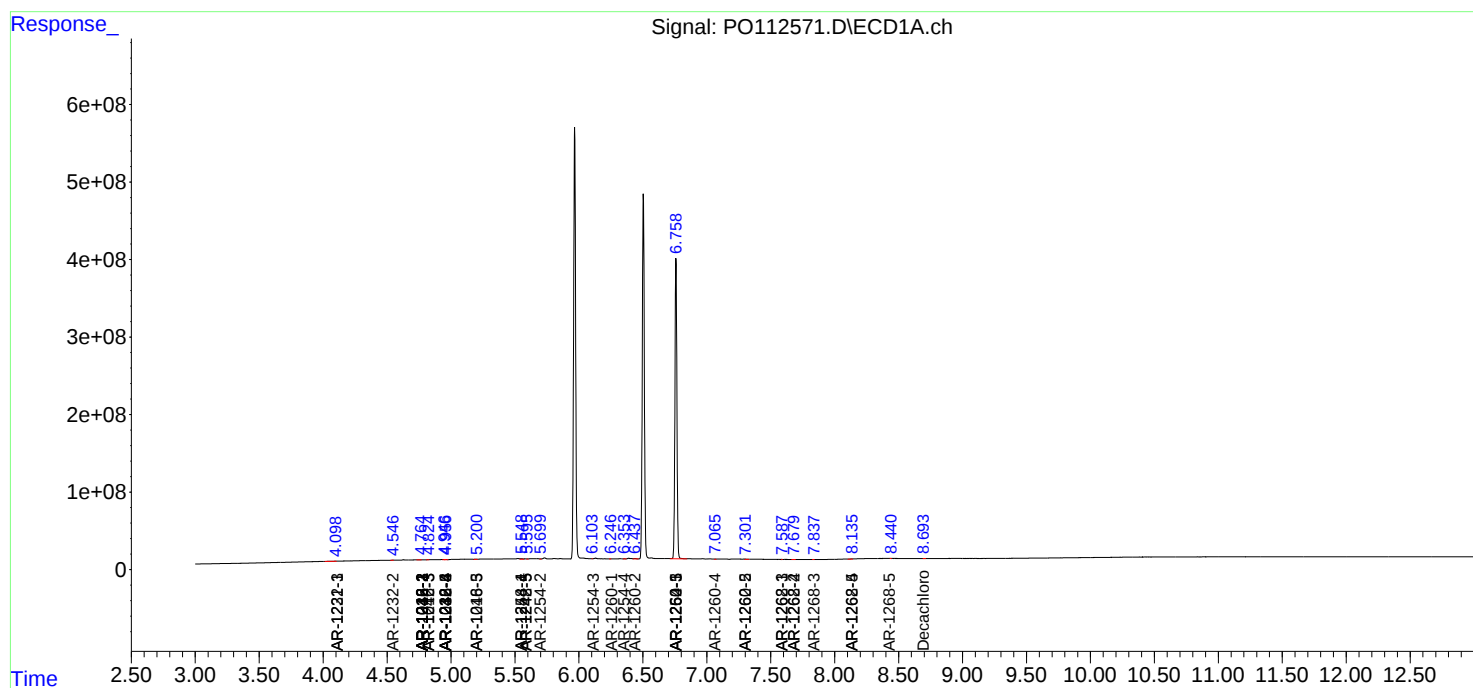


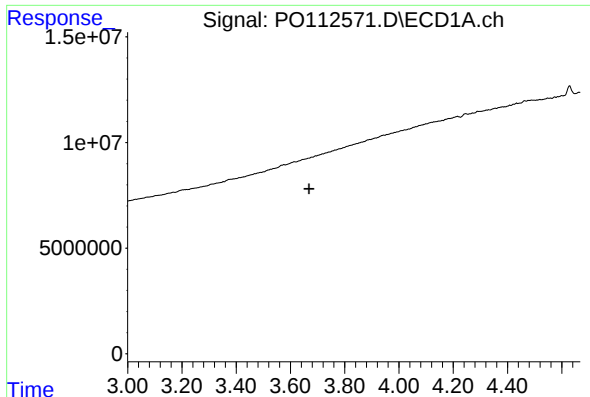

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.669 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

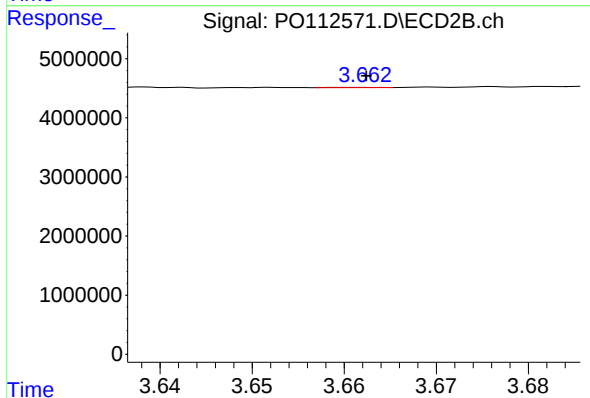


#1 Tetrachloro-m-xylene

R.T.: 3.661 min
Delta R.T.: -0.001 min
Response: 17181
Conc: 0.00 ng/ml

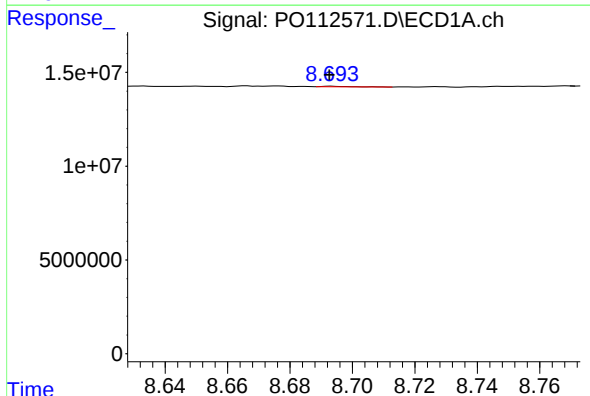


#2 Decachlorobiphenyl

R.T.: 8.693 min
Delta R.T.: 0.000 min
Response: 177479
Conc: 0.02 ng/ml

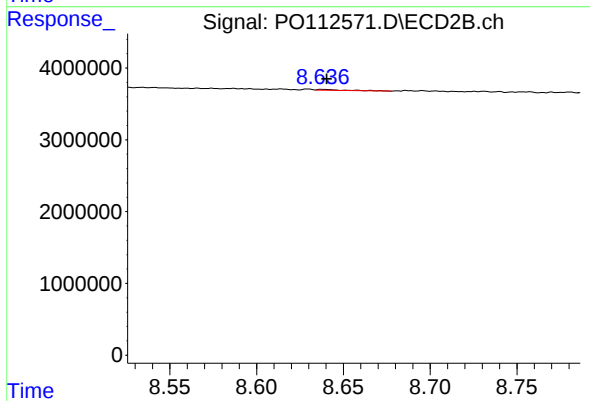

#2 Decachlorobiphenyl


R.T.: 8.638 min
Delta R.T.: -0.002 min
Response: 125054
Conc: 0.07 ng/ml

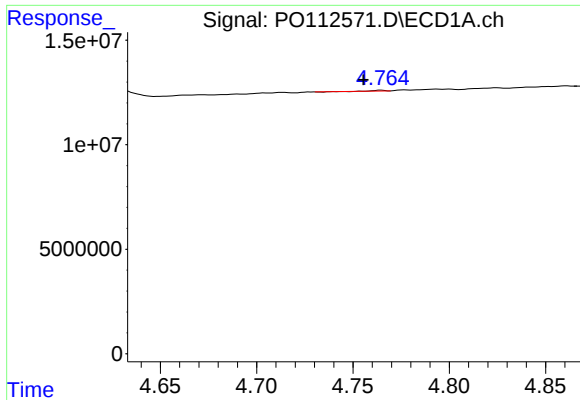

#3 AR-1016-1


R.T.: 4.765 min
Delta R.T.: 0.009 min
Response: 122448
Conc: 0.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

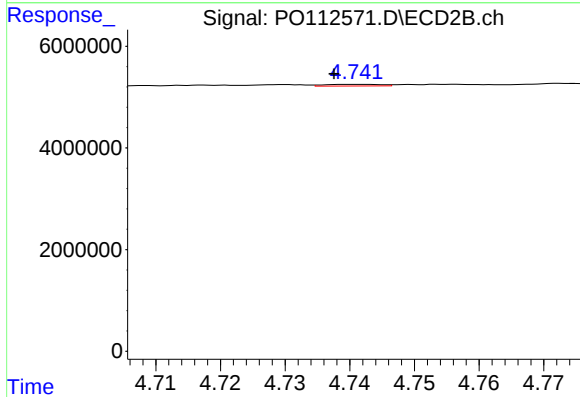


#3 AR-1016-1

R.T.: 4.741 min
Delta R.T.: 0.004 min
Response: 202806
Conc: 1.16 ng/ml

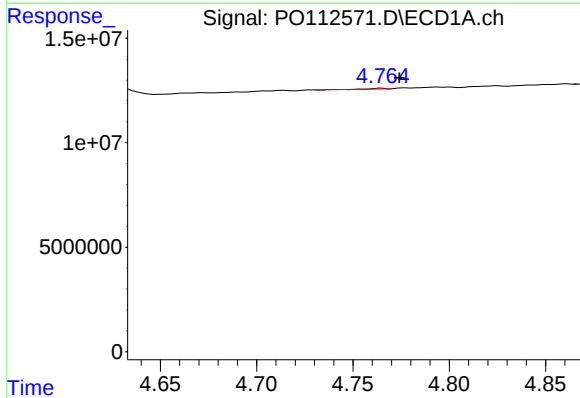


#4 AR-1016-2

R.T.: 4.765 min
Delta R.T.: -0.009 min
Response: 122448
Conc: 0.30 ng/ml

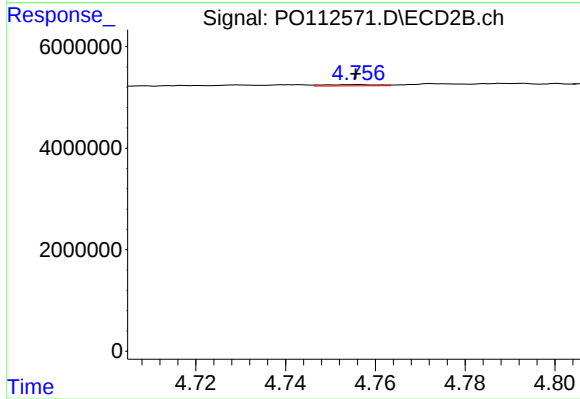

#4 AR-1016-2


R.T.: 4.755 min
Delta R.T.: 0.000 min
Response: 223580
Conc: 0.86 ng/ml

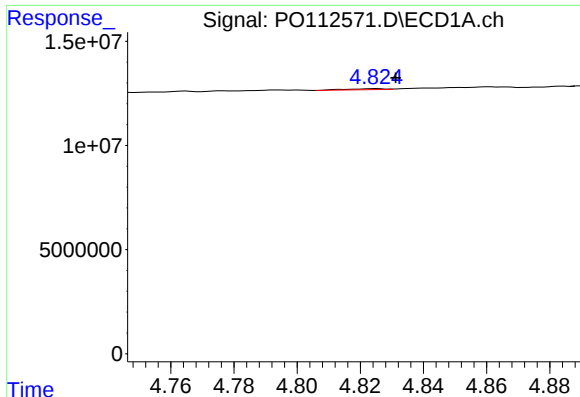

#5 AR-1016-3


R.T.: 4.825 min
Delta R.T.: -0.006 min
Response: 425863
Conc: 1.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

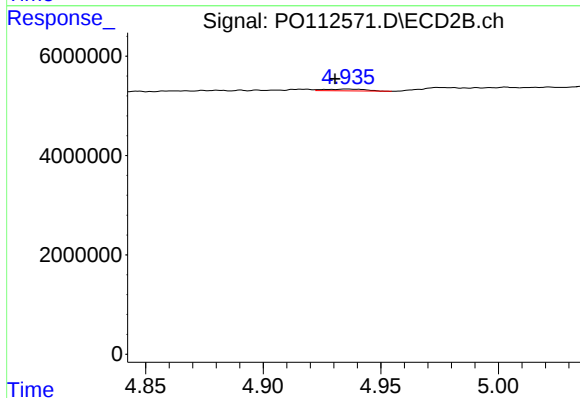


#5 AR-1016-3

R.T.: 4.936 min
Delta R.T.: 0.005 min
Response: 417529
Conc: 3.07 ng/ml

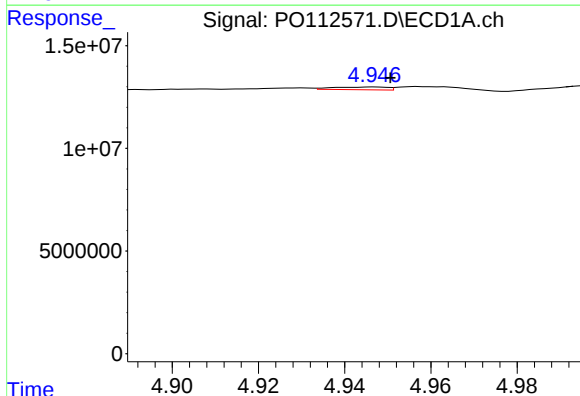


#6 AR-1016-4

R.T.: 4.947 min
Delta R.T.: -0.004 min
Response: 1180702
Conc: 5.57 ng/ml

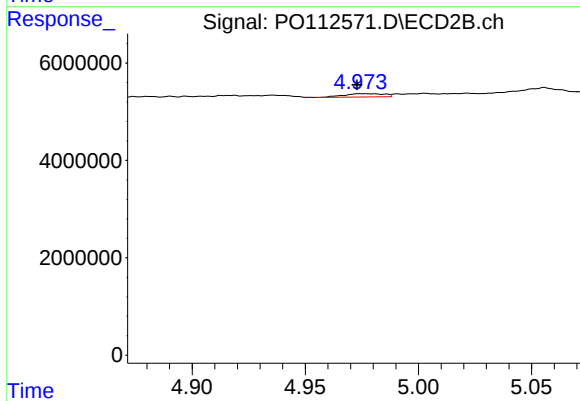

#6 AR-1016-4


R.T.: 4.975 min
Delta R.T.: 0.002 min
Response: 832856
Conc: 7.50 ng/ml

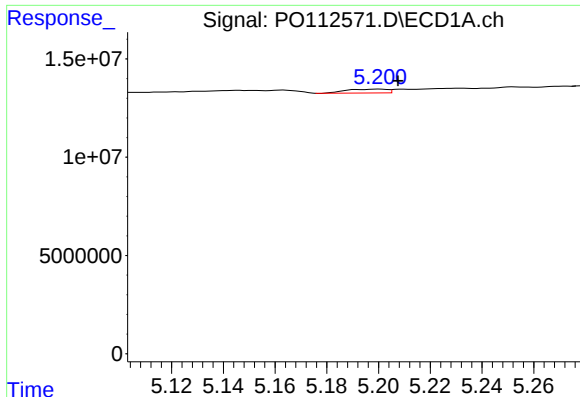

#7 AR-1016-5


R.T.: 5.200 min
Delta R.T.: -0.007 min
Response: 2147070
Conc: 9.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

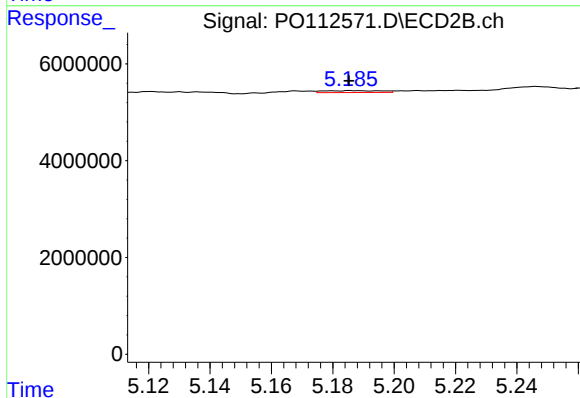


#7 AR-1016-5

R.T.: 5.186 min
Delta R.T.: 0.001 min
Response: 519755
Conc: 3.63 ng/ml

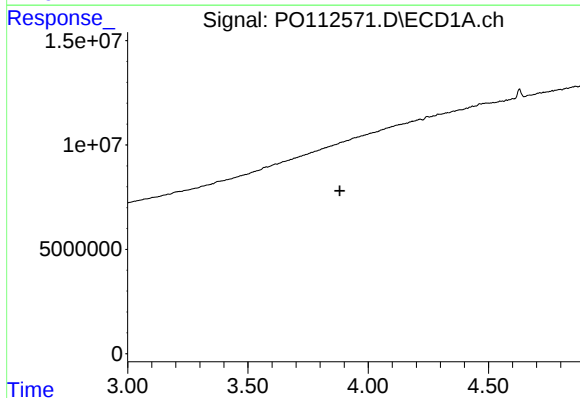


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 3.882 min
Response: 0
Conc: N.D.

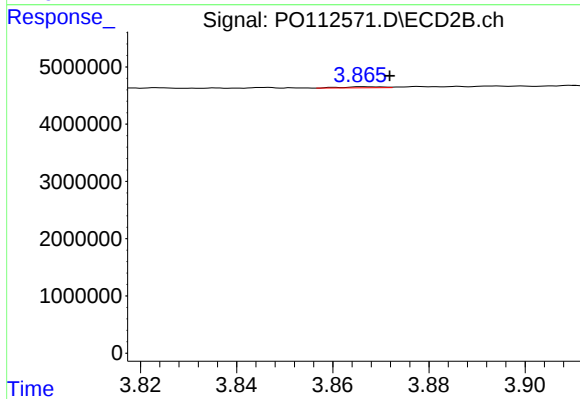

#8 AR-1221-1


R.T.: 3.866 min
Delta R.T.: -0.006 min
Response: 103098
Conc: 1.53 ng/ml

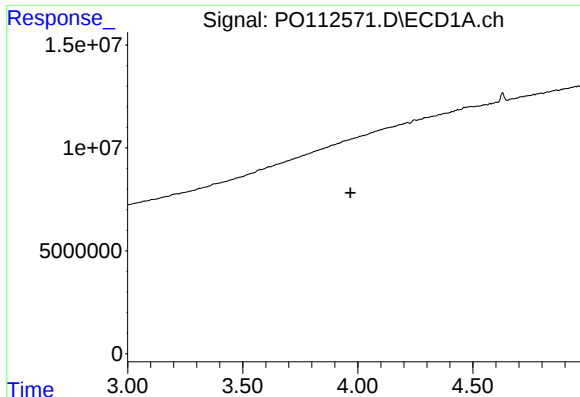

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T.: 3.967 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

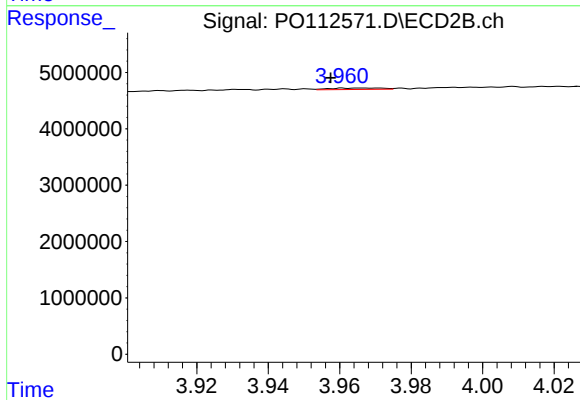


#9 AR-1221-2

R.T.: 3.961 min
Delta R.T.: 0.003 min
Response: 255905
Conc: 5.04 ng/ml

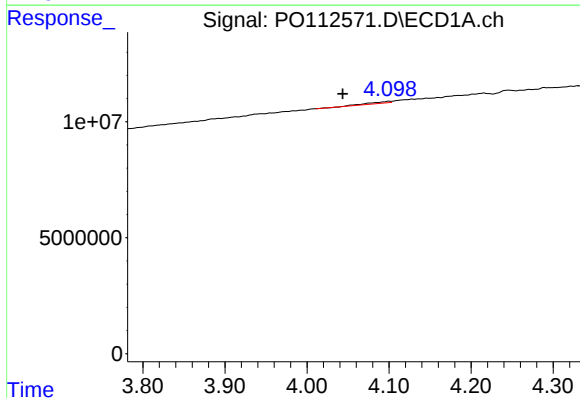


#10 AR-1221-3

R.T.: 4.100 min
Delta R.T.: 0.056 min
Response: 1322166
Conc: 5.56 ng/ml

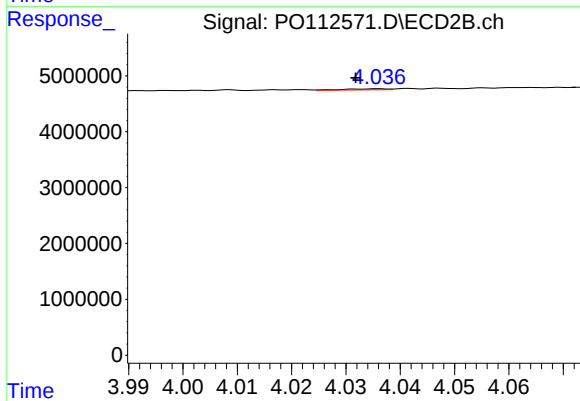

#10 AR-1221-3


R.T.: 4.036 min
Delta R.T.: 0.004 min
Response: 103228
Conc: 0.65 ng/ml

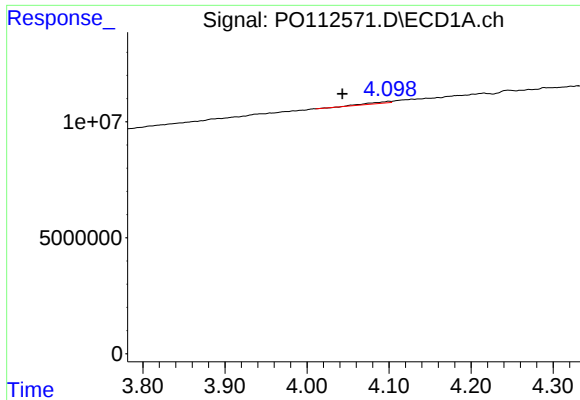

#11 AR-1232-1


R.T.: 4.100 min
Delta R.T.: 0.057 min
Response: 1322166
Conc: 7.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

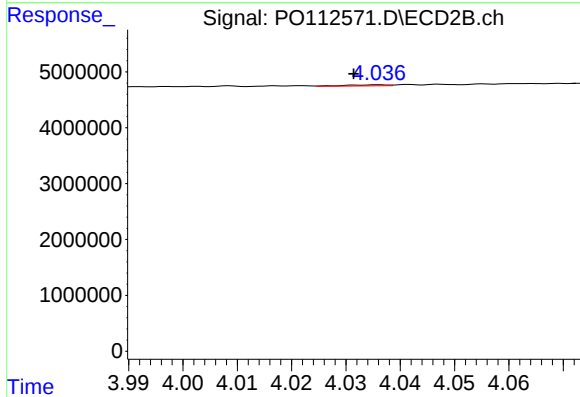


#11 AR-1232-1

R.T.: 4.036 min
Delta R.T.: 0.005 min
Response: 103228
Conc: 0.82 ng/ml

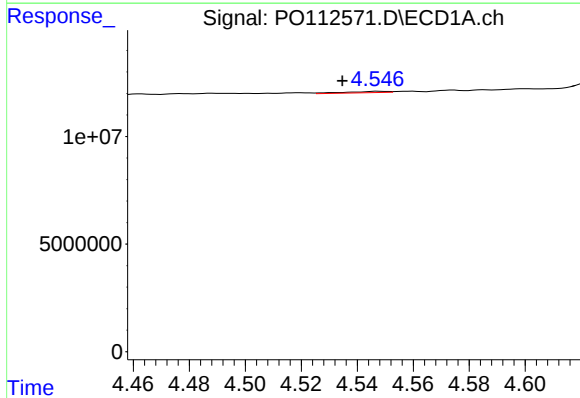


#12 AR-1232-2

R.T.: 4.548 min
Delta R.T.: 0.013 min
Response: 619083
Conc: 5.75 ng/ml

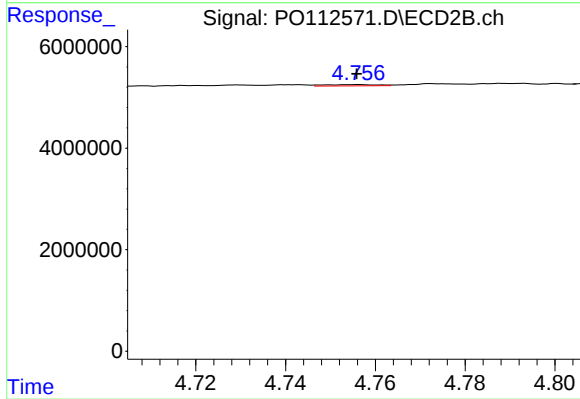

#12 AR-1232-2


R.T.: 4.755 min
Delta R.T.: 0.000 min
Response: 223580
Conc: 1.70 ng/ml

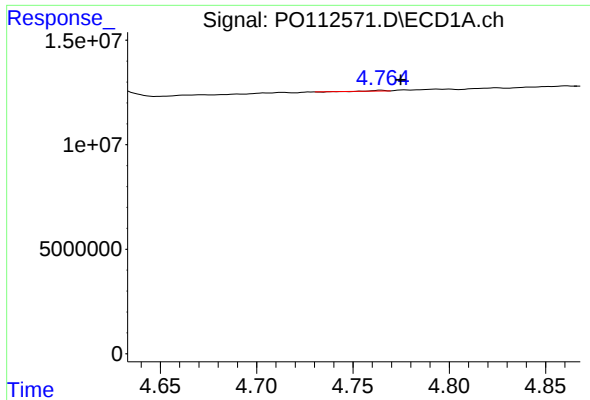

#13 AR-1232-3


R.T.: 4.765 min
Delta R.T.: -0.010 min
Response: 122448
Conc: 0.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

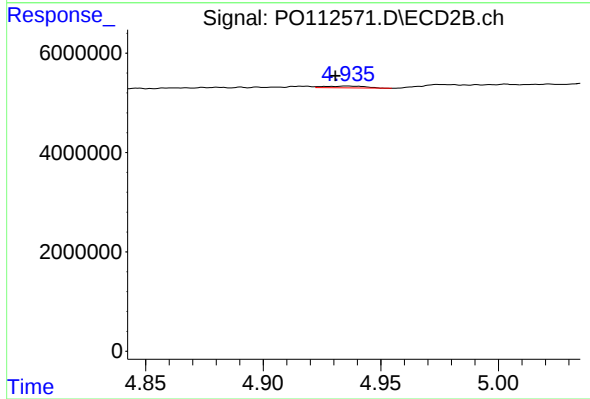


#13 AR-1232-3

R.T.: 4.936 min
Delta R.T.: 0.005 min
Response: 417529
Conc: 6.21 ng/ml

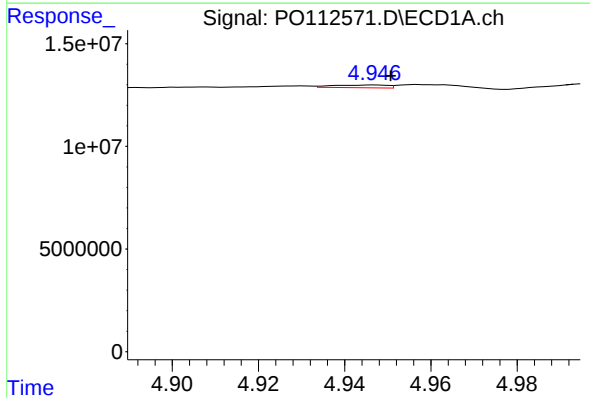


#14 AR-1232-4

R.T.: 4.947 min
Delta R.T.: -0.004 min
Response: 1180702
Conc: 11.27 ng/ml

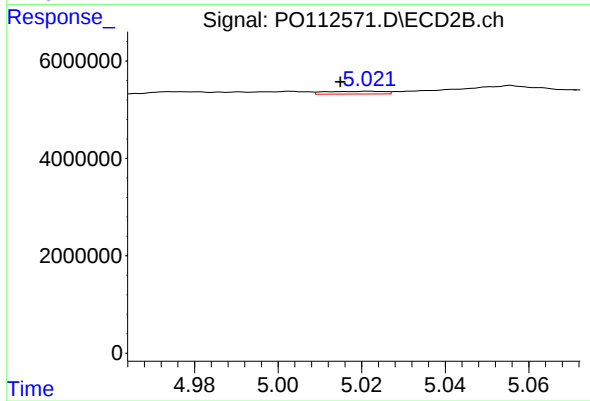

#14 AR-1232-4


R.T.: 5.022 min
Delta R.T.: 0.007 min
Response: 553201
Conc: 9.25 ng/ml

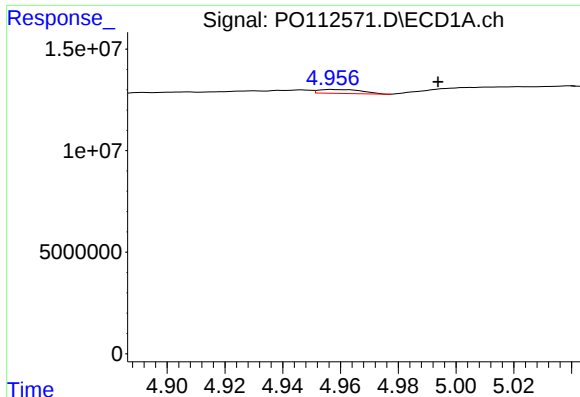

#15 AR-1232-5


R.T.: 4.957 min
Delta R.T.: -0.036 min
Response: 2016670
Conc: 29.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

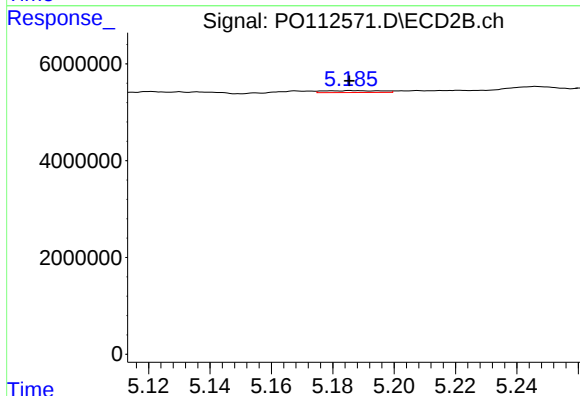


#15 AR-1232-5

R.T.: 5.186 min
Delta R.T.: 0.000 min
Response: 519755
Conc: 7.97 ng/ml

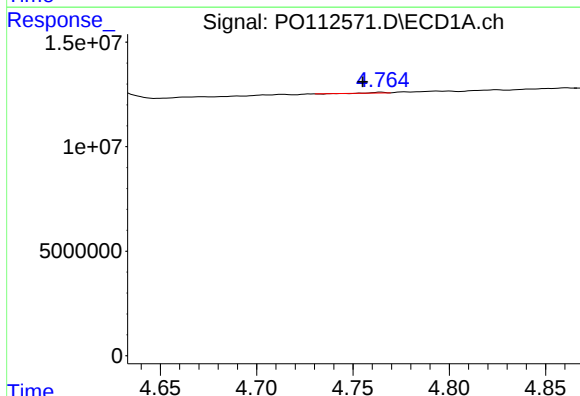


#16 AR-1242-1

R.T.: 4.765 min
Delta R.T.: 0.010 min
Response: 122448
Conc: 0.49 ng/ml

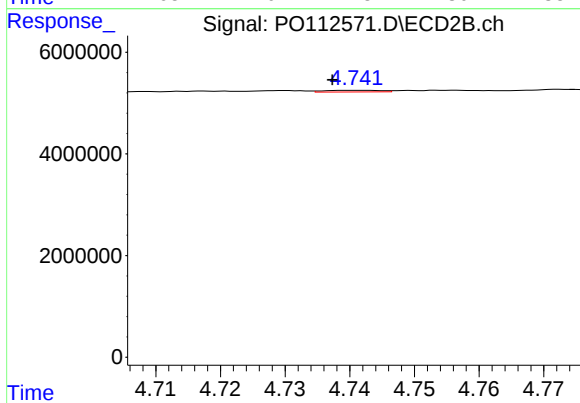

#16 AR-1242-1


R.T.: 4.741 min
Delta R.T.: 0.004 min
Response: 202806
Conc: 1.28 ng/ml

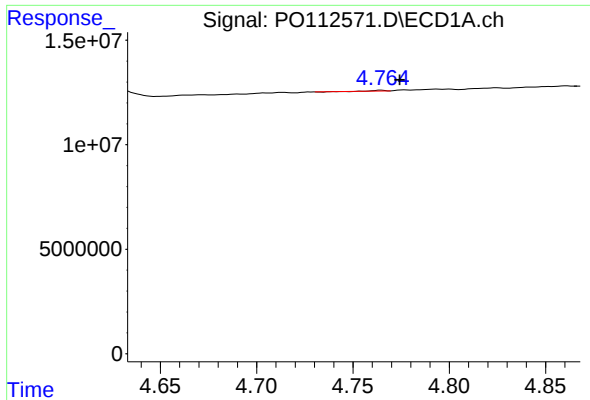

#17 AR-1242-2


R.T.: 4.765 min
Delta R.T.: -0.010 min
Response: 122448
Conc: 0.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

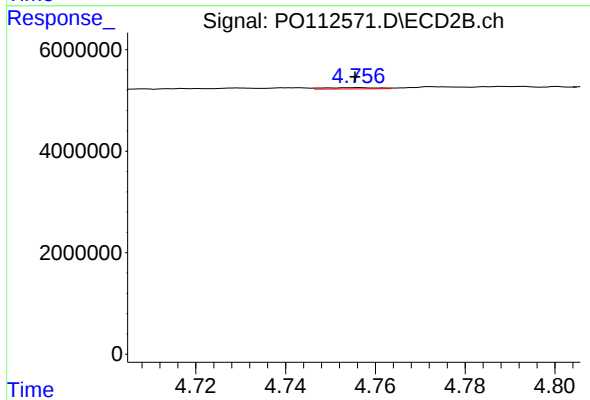


#17 AR-1242-2

R.T.: 4.755 min
Delta R.T.: 0.000 min
Response: 223580
Conc: 0.96 ng/ml

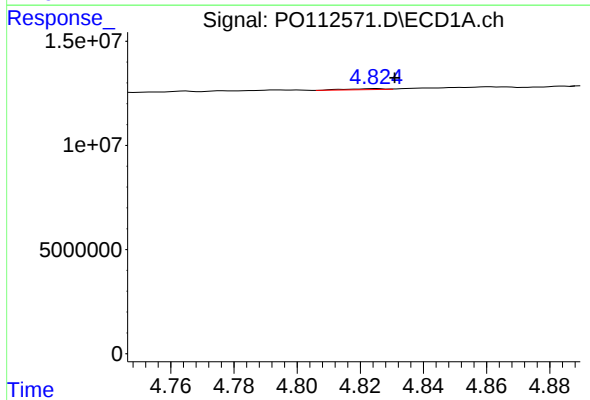


#18 AR-1242-3

R.T.: 4.825 min
Delta R.T.: -0.006 min
Response: 425863
Conc: 1.80 ng/ml

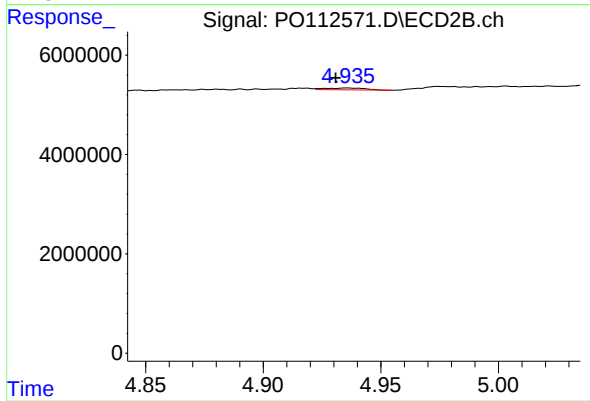

#18 AR-1242-3


R.T.: 4.936 min
Delta R.T.: 0.005 min
Response: 417529
Conc: 3.45 ng/ml

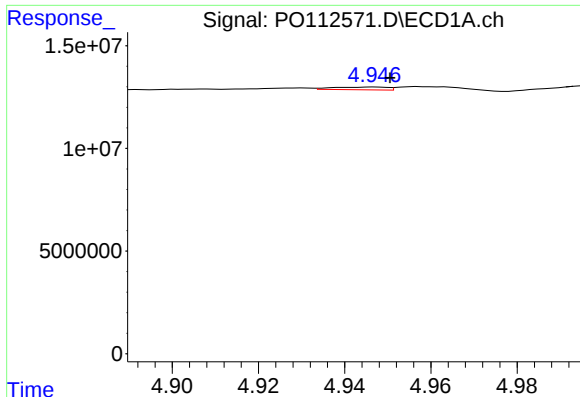

#19 AR-1242-4


R.T.: 4.947 min
Delta R.T.: -0.004 min
Response: 1180702
Conc: 6.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

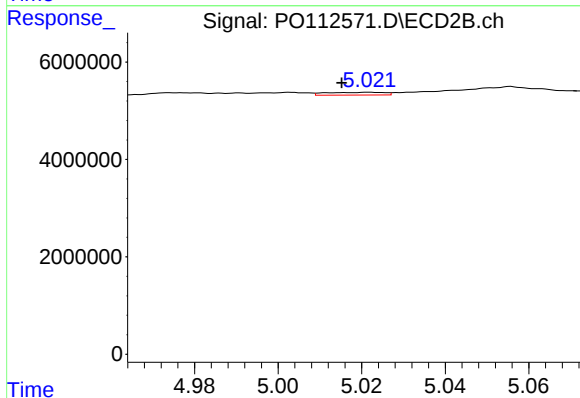


#19 AR-1242-4

R.T.: 5.022 min
Delta R.T.: 0.006 min
Response: 553201
Conc: 4.51 ng/ml

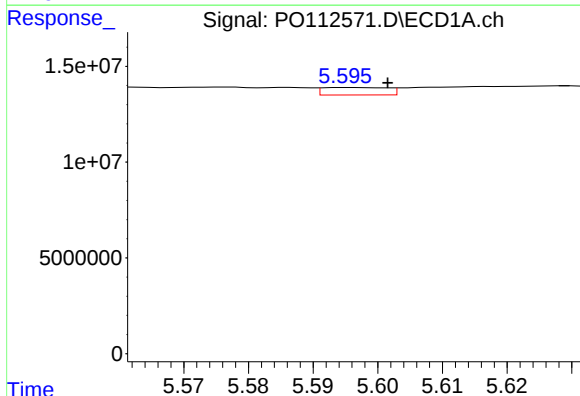


#20 AR-1242-5

R.T.: 5.595 min
Delta R.T.: -0.006 min
Response: 2722397
Conc: 12.73 ng/ml

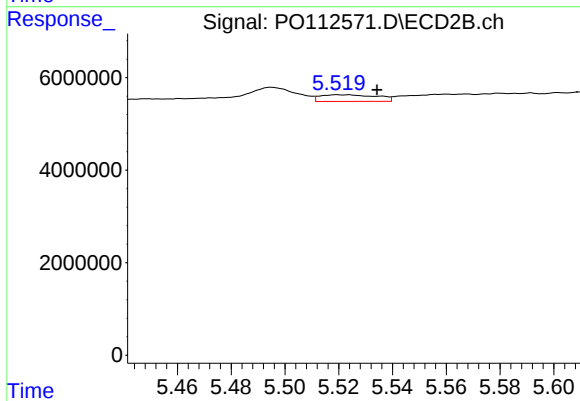

#20 AR-1242-5


R.T.: 5.520 min
Delta R.T.: -0.014 min
Response: 2101046
Conc: 13.05 ng/ml

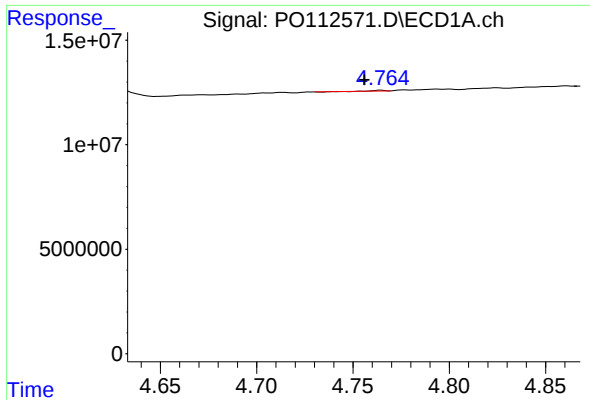

#21 AR-1248-1


R.T.: 4.765 min
Delta R.T.: 0.009 min
Response: 122448
Conc: 0.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

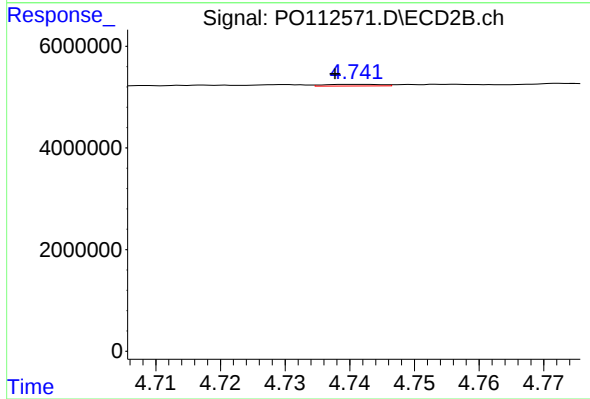


#21 AR-1248-1

R.T.: 4.741 min
Delta R.T.: 0.003 min
Response: 202806
Conc: 1.67 ng/ml

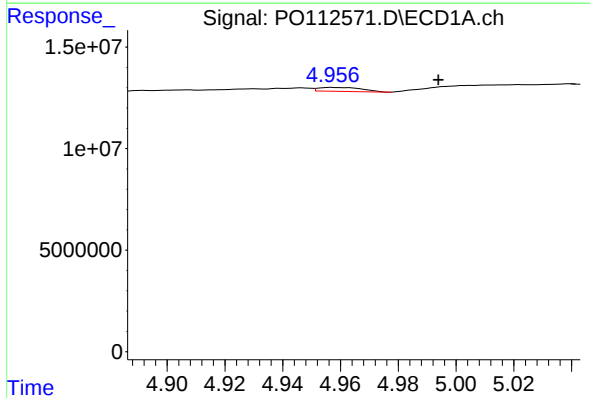


#22 AR-1248-2

R.T.: 4.957 min
Delta R.T.: -0.037 min
Response: 2016670
Conc: 7.91 ng/ml

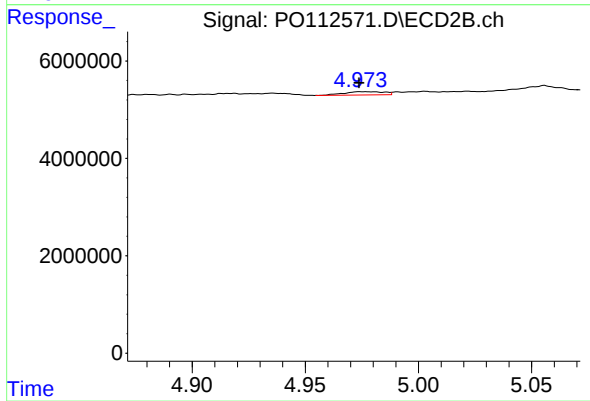

#22 AR-1248-2


R.T.: 4.975 min
Delta R.T.: 0.001 min
Response: 832856
Conc: 4.92 ng/ml

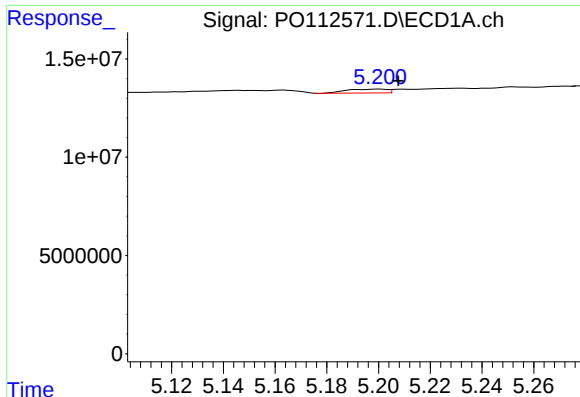

#23 AR-1248-3


R.T.: 5.200 min
Delta R.T.: -0.007 min
Response: 2147070
Conc: 6.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

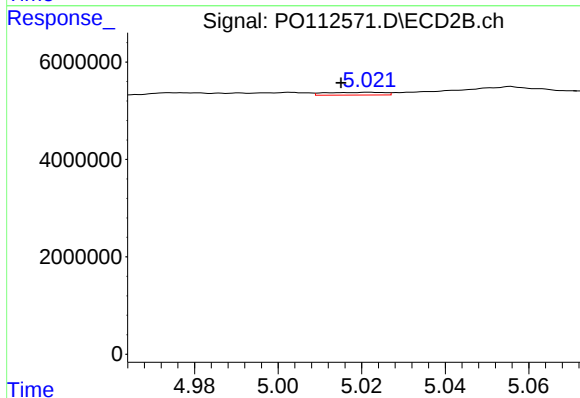


#23 AR-1248-3

R.T.: 5.022 min
Delta R.T.: 0.007 min
Response: 553201
Conc: 3.11 ng/ml

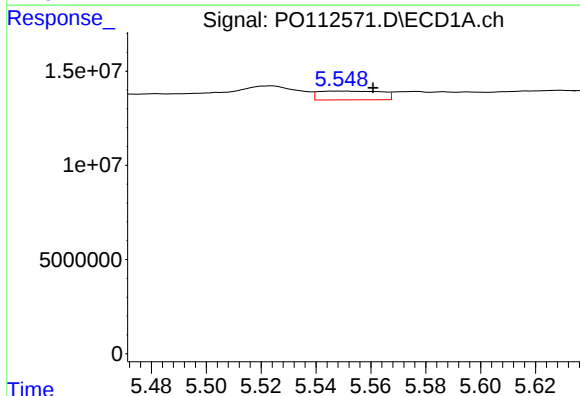


#24 AR-1248-4

R.T.: 5.550 min
Delta R.T.: -0.011 min
Response: 7427466
Conc: 14.62 ng/ml

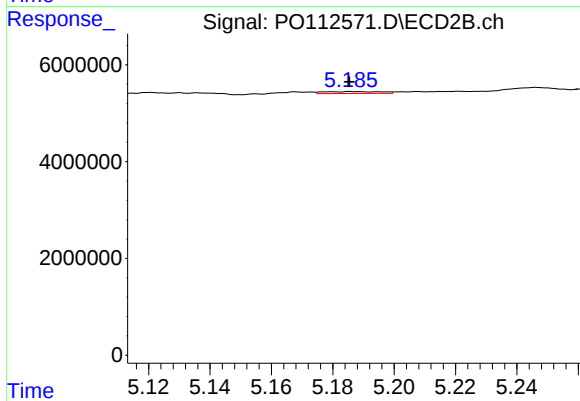

#24 AR-1248-4


R.T.: 5.186 min
Delta R.T.: 0.000 min
Response: 519755
Conc: 2.49 ng/ml

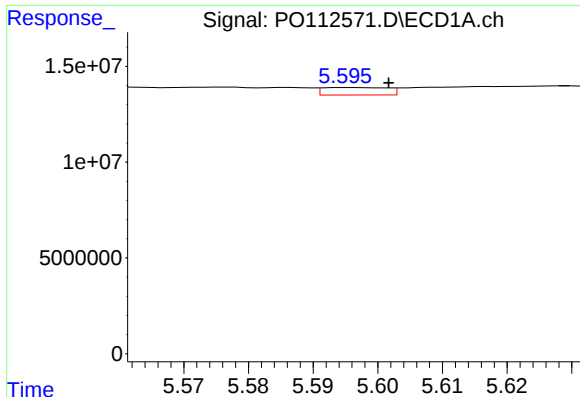

#25 AR-1248-5


R.T.: 5.595 min
Delta R.T.: -0.006 min
Response: 2722397
Conc: 7.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

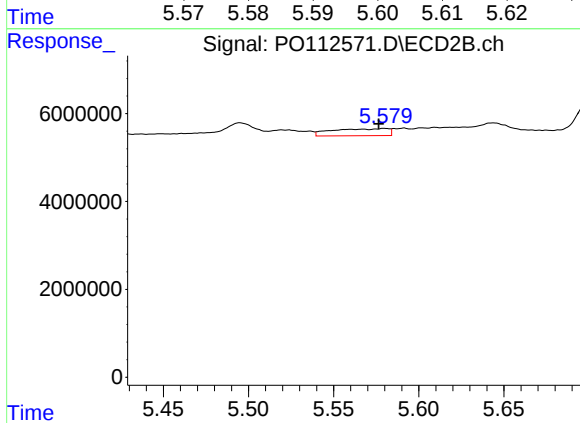


#25 AR-1248-5

R.T.: 5.580 min
Delta R.T.: 0.004 min
Response: 3702513
Conc: 17.24 ng/ml

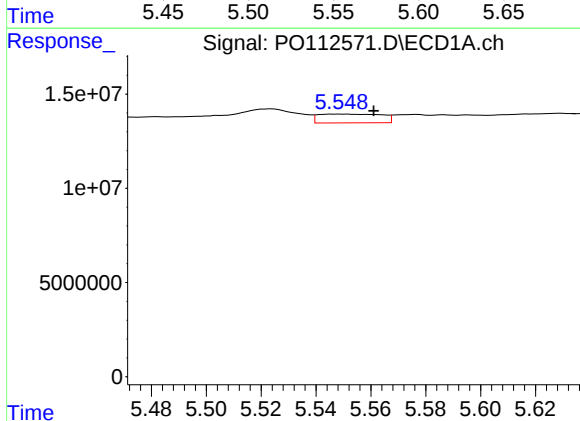


#26 AR-1254-1

R.T.: 5.550 min
Delta R.T.: -0.011 min
Response: 7427466
Conc: 13.53 ng/ml

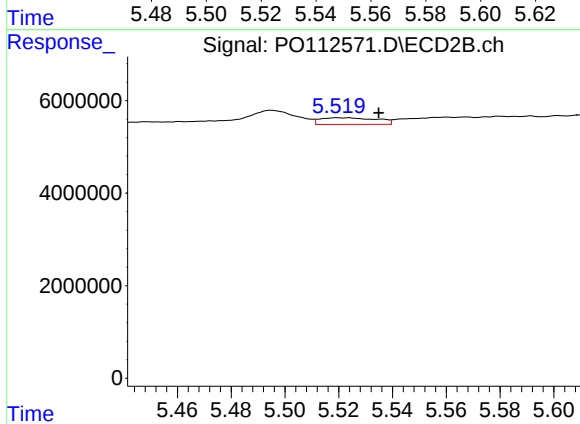

#26 AR-1254-1


R.T.: 5.520 min
Delta R.T.: -0.015 min
Response: 2101046
Conc: 6.39 ng/ml

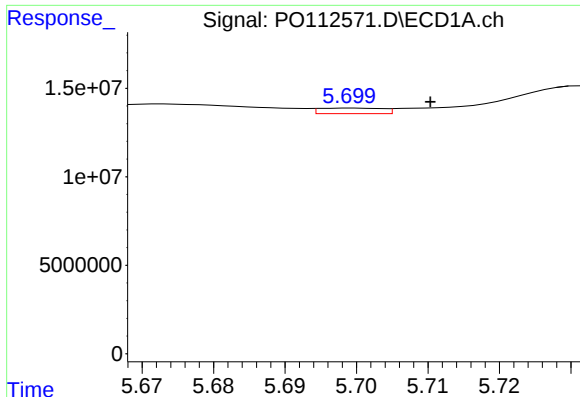

#27 AR-1254-2


R.T.: 5.700 min
Delta R.T.: -0.011 min
Response: 1932863
Conc: 3.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

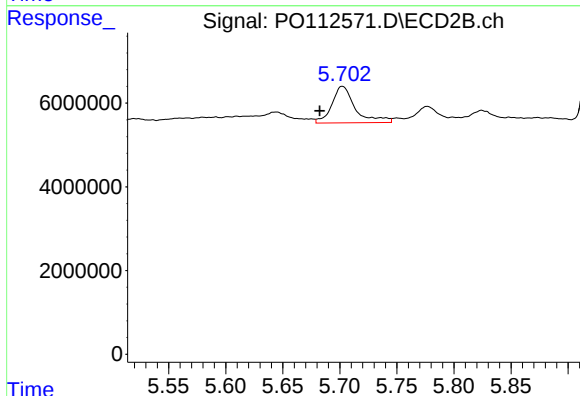


#27 AR-1254-2

R.T.: 5.702 min
Delta R.T.: 0.020 min
Response: 12528348
Conc: 43.28 ng/ml

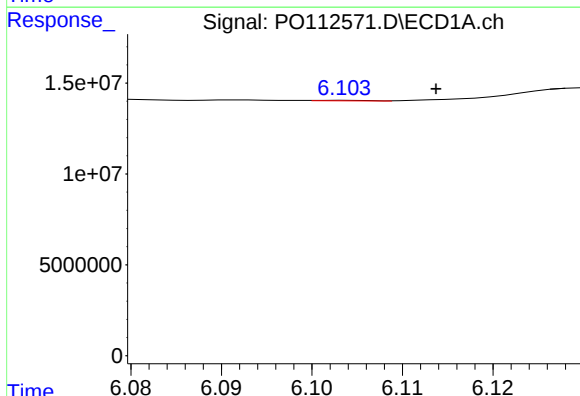


#28 AR-1254-3

R.T.: 6.104 min
Delta R.T.: -0.010 min
Response: 108739
Conc: 0.15 ng/ml

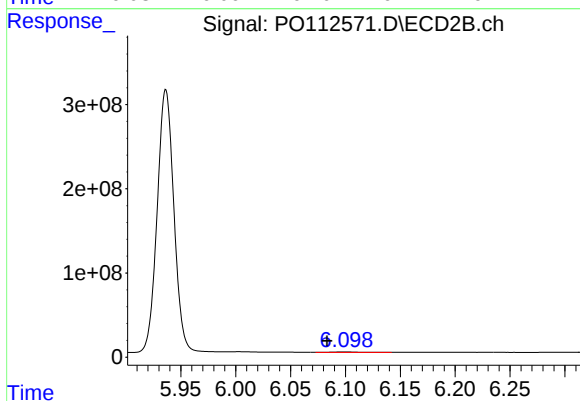

#28 AR-1254-3


R.T.: 6.099 min
Delta R.T.: 0.016 min
Response: 14547739
Conc: 34.03 ng/ml

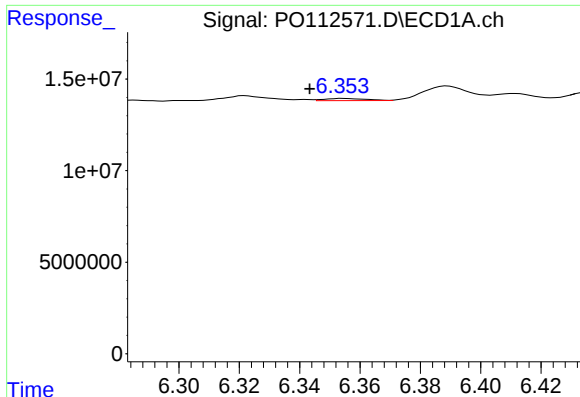

#29 AR-1254-4


R.T.: 6.354 min
Delta R.T.: 0.011 min
Response: 1170561
Conc: 2.13 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

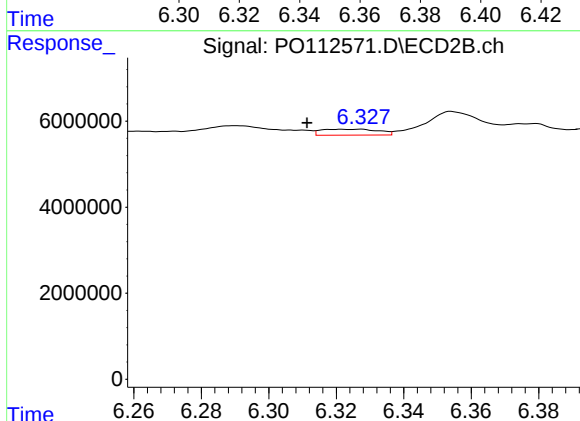


#29 AR-1254-4

R.T.: 6.327 min
Delta R.T.: 0.016 min
Response: 1624652
Conc: 5.95 ng/ml

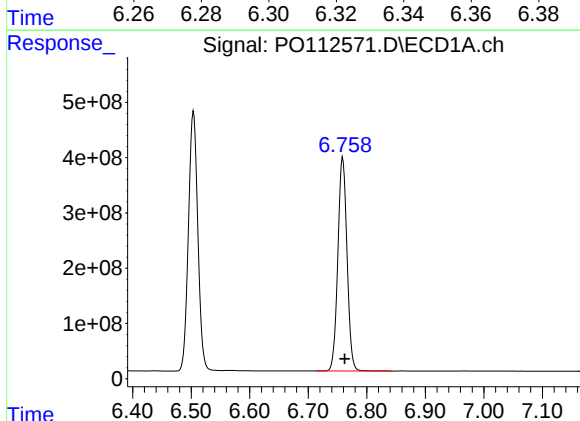


#30 AR-1254-5

R.T.: 6.759 min
Delta R.T.: -0.003 min
Response: 4207061805
Conc: 5943.65 ng/ml

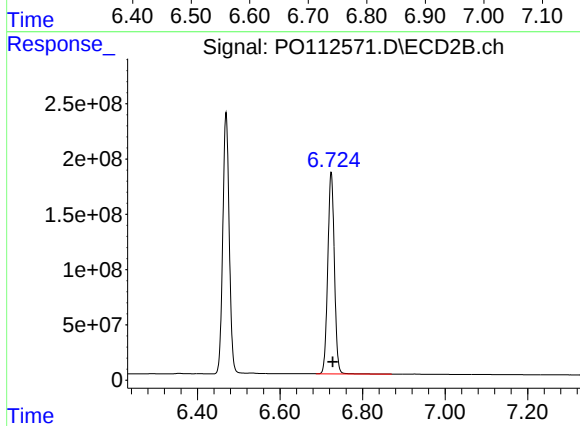

#30 AR-1254-5


R.T.: 6.724 min
Delta R.T.: -0.003 min
Response: 2028347915
Conc: 6072.54 ng/ml

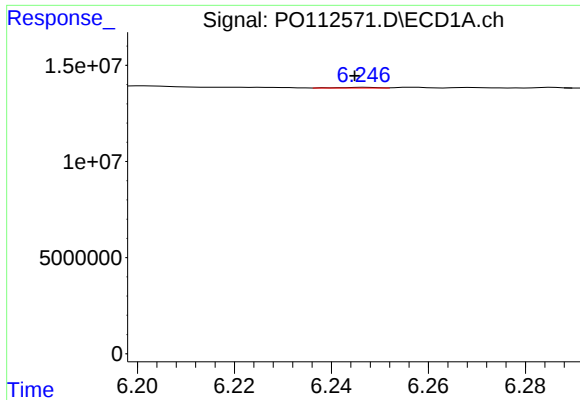

#31 AR-1260-1


R.T.: 6.247 min
Delta R.T.: 0.002 min
Response: 208047
Conc: 0.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

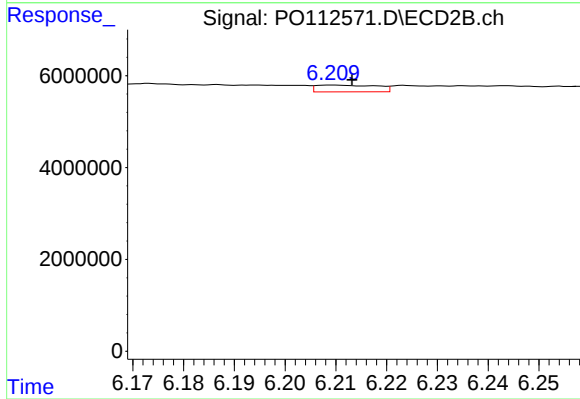


#31 AR-1260-1

R.T.: 6.209 min
Delta R.T.: -0.004 min
Response: 1206884
Conc: 4.86 ng/ml

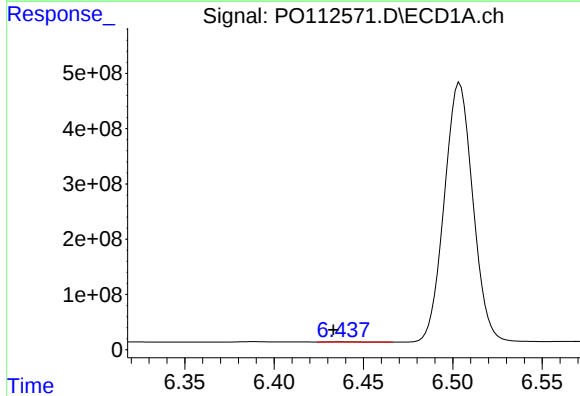


#32 AR-1260-2

R.T.: 6.438 min
Delta R.T.: 0.004 min
Response: 5250397
Conc: 7.63 ng/ml

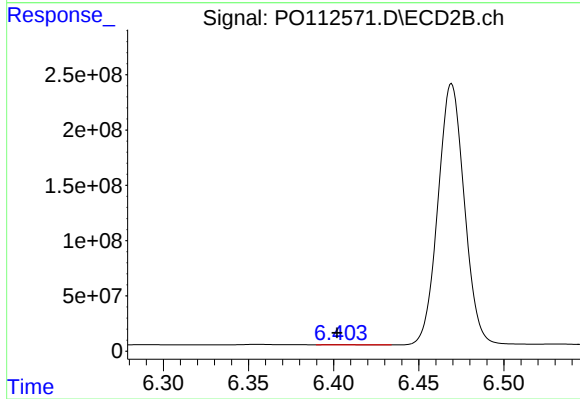

#32 AR-1260-2


R.T.: 6.403 min
Delta R.T.: 0.001 min
Response: 3418437
Conc: 10.37 ng/ml

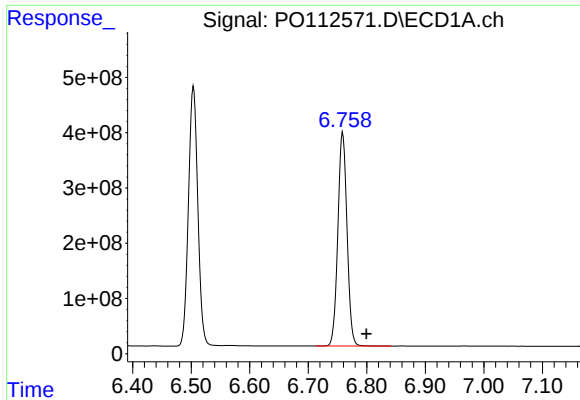

#33 AR-1260-3


R.T.: 6.759 min
Delta R.T.: -0.041 min
Response: 4207061805
Conc: 7154.63 ng/m

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

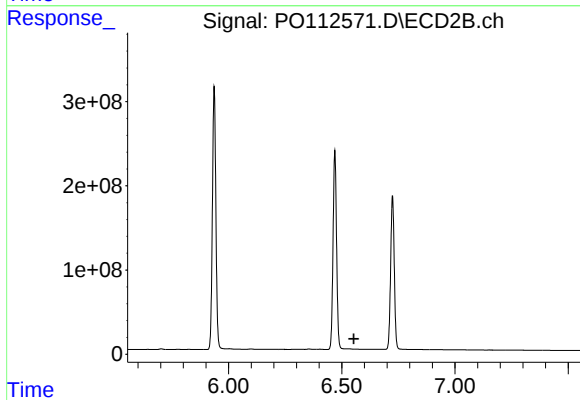


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 6.553 min
Response: 0
Conc: N.D.

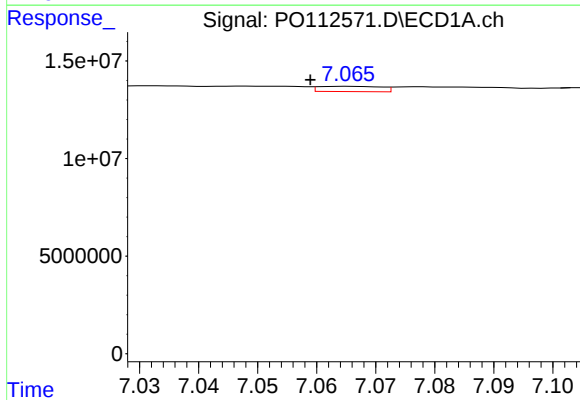


#34 AR-1260-4

R.T.: 7.066 min
Delta R.T.: 0.007 min
Response: 1964458
Conc: 4.36 ng/ml

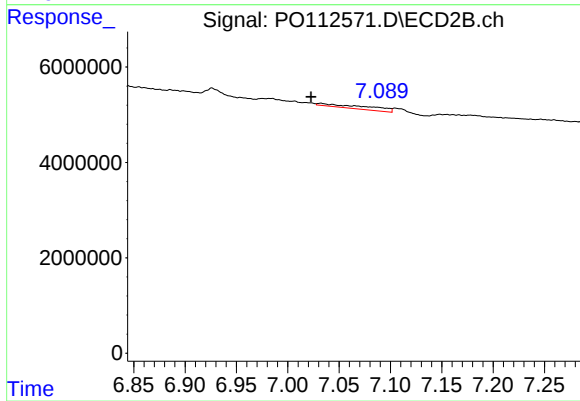

#34 AR-1260-4


R.T.: 7.032 min
Delta R.T.: 0.009 min
Response: 2451628
Conc: 12.81 ng/ml

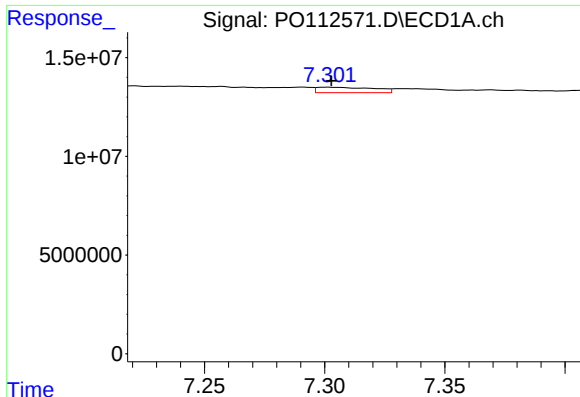

#35 AR-1260-5


R.T.: 7.301 min
Delta R.T.: -0.001 min
Response: 4587768
Conc: 3.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

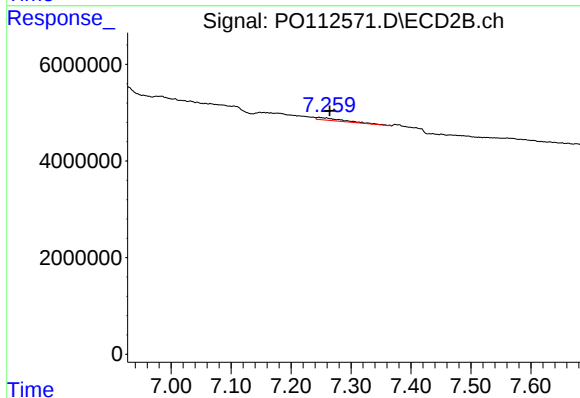


#35 AR-1260-5

R.T.: 7.246 min
Delta R.T.: -0.018 min
Response: 1679653
Conc: 4.07 ng/ml

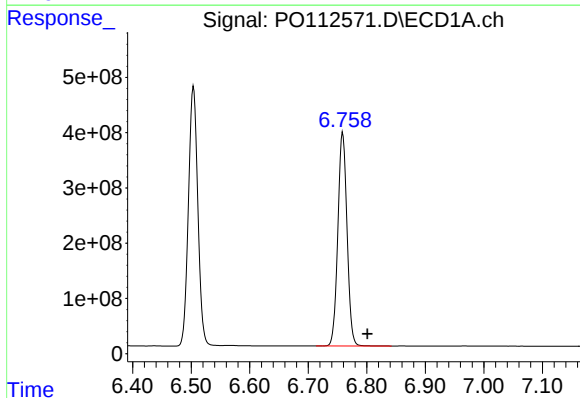


#36 AR-1262-1

R.T.: 6.759 min
Delta R.T.: -0.042 min
Response: 4207061805
Conc: 4527.58 ng/ml

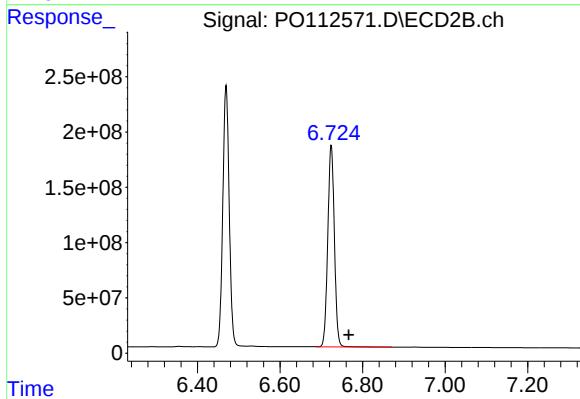

#36 AR-1262-1


R.T.: 6.724 min
Delta R.T.: -0.042 min
Response: 2028347915
Conc: 4889.61 ng/ml

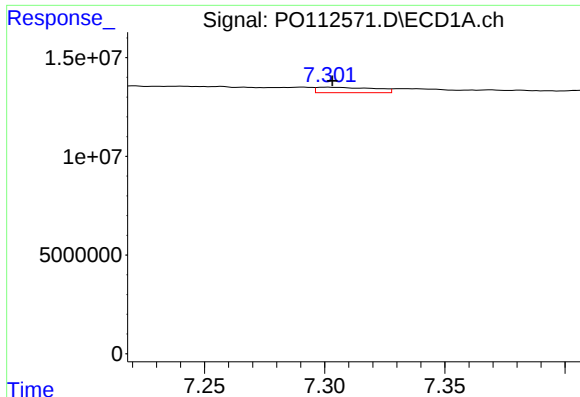

#37 AR-1262-2


R.T.: 7.301 min
Delta R.T.: -0.002 min
Response: 4587768
Conc: 3.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

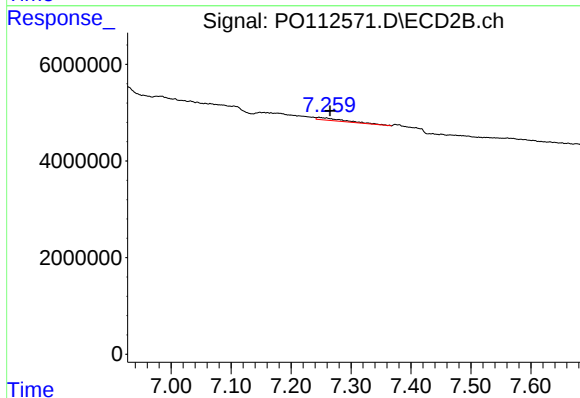


#37 AR-1262-2

R.T.: 7.246 min
Delta R.T.: -0.019 min
Response: 1679653
Conc: 3.26 ng/ml

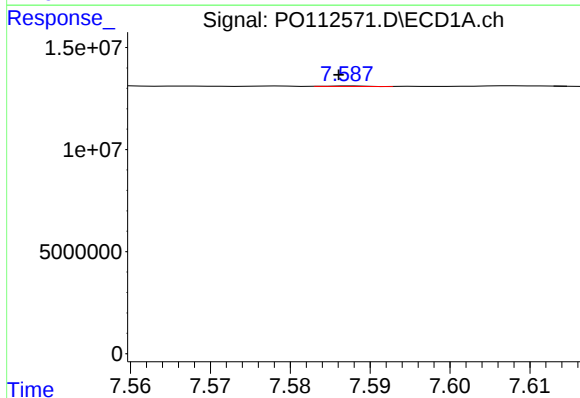


#38 AR-1262-3

R.T.: 7.588 min
Delta R.T.: 0.002 min
Response: 103658
Conc: 0.18 ng/ml

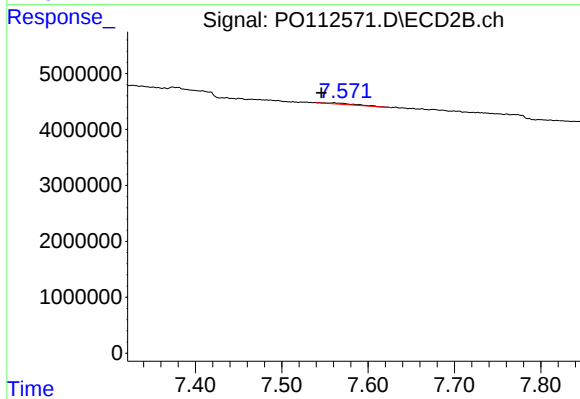

#38 AR-1262-3


R.T.: 7.561 min
Delta R.T.: 0.015 min
Response: 525394
Conc: 2.82 ng/ml

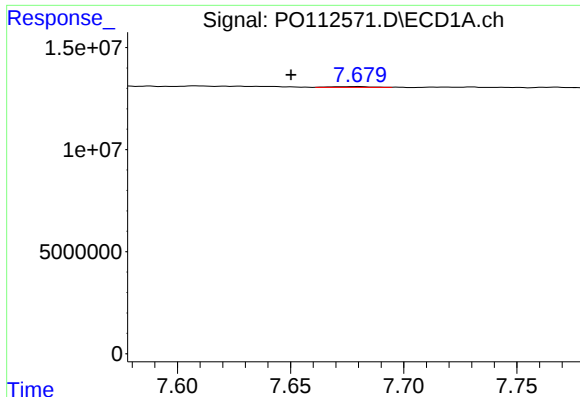

#39 AR-1262-4


R.T.: 7.680 min
Delta R.T.: 0.029 min
Response: 486306
Conc: 0.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

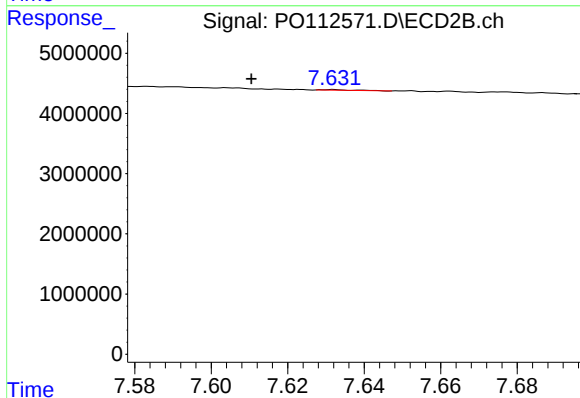


#39 AR-1262-4

R.T.: 7.632 min
Delta R.T.: 0.021 min
Response: 59258
Conc: 0.21 ng/ml

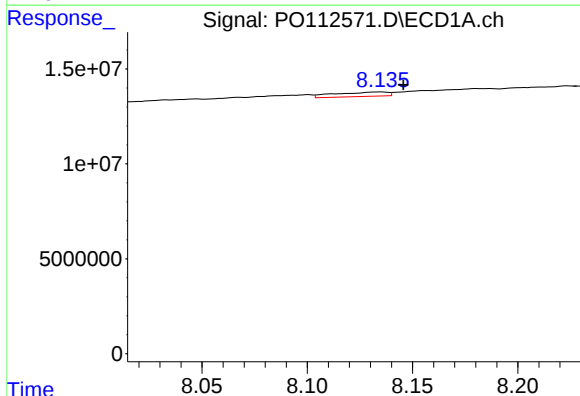


#40 AR-1262-5

R.T.: 8.135 min
Delta R.T.: -0.011 min
Response: 3963645
Conc: 9.13 ng/ml

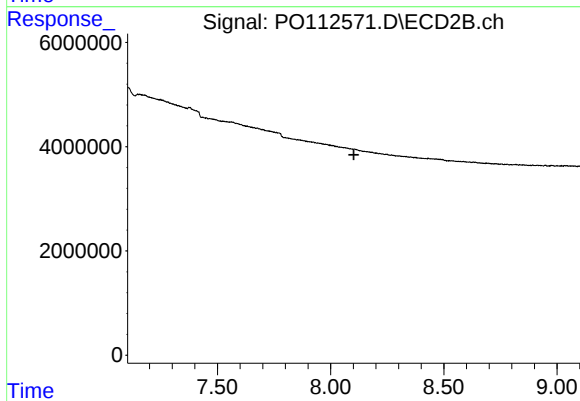

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T.: 8.103 min
Response: 0
Conc: N.D.

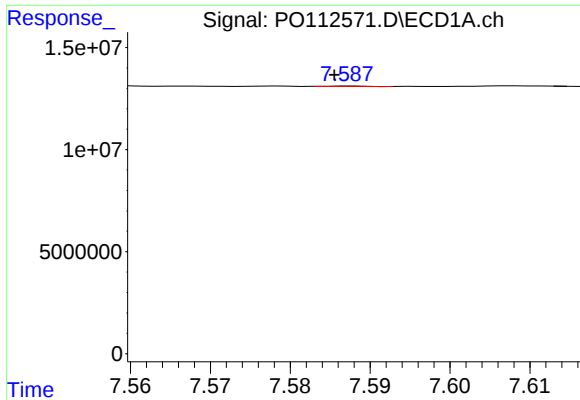

#41 AR-1268-1


R.T.: 7.588 min
Delta R.T.: 0.002 min
Response: 103658
Conc: 0.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

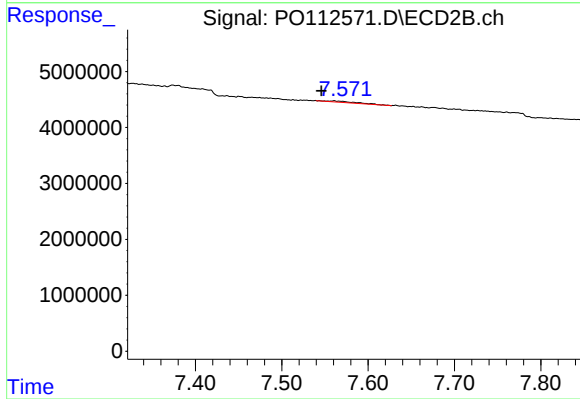


#41 AR-1268-1

R.T.: 7.561 min
Delta R.T.: 0.015 min
Response: 525394
Conc: 1.01 ng/ml

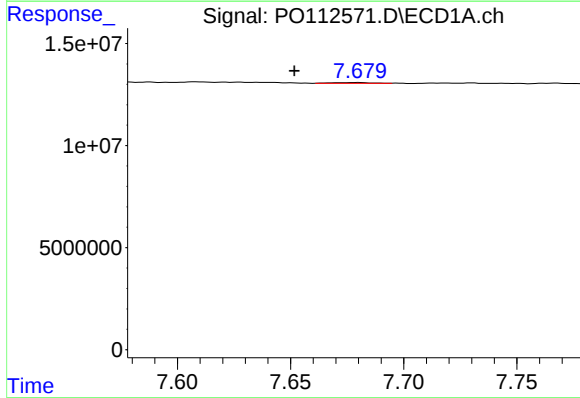


#42 AR-1268-2

R.T.: 7.680 min
Delta R.T.: 0.028 min
Response: 486306
Conc: 0.33 ng/ml

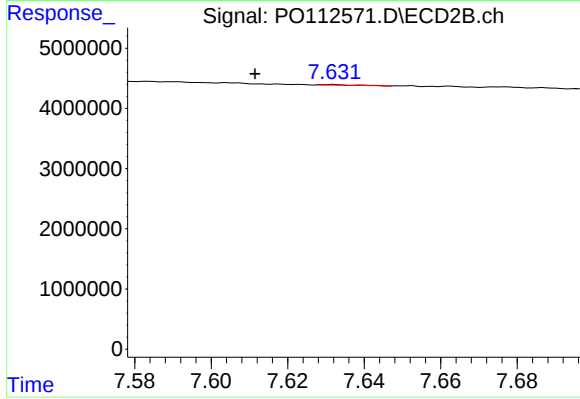

#42 AR-1268-2


R.T.: 7.632 min
Delta R.T.: 0.020 min
Response: 59258
Conc: 0.14 ng/ml

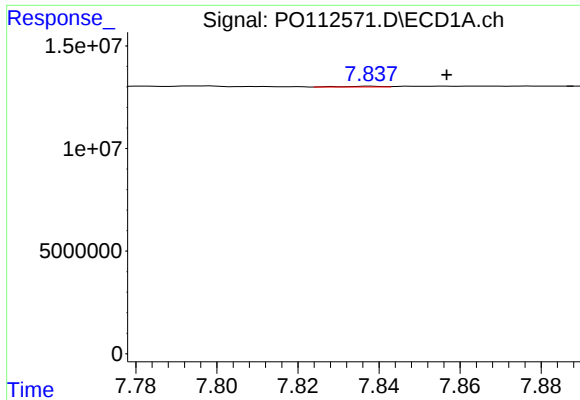

#43 AR-1268-3


R.T.: 7.838 min
Delta R.T.: -0.019 min
Response: 220578
Conc: 0.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

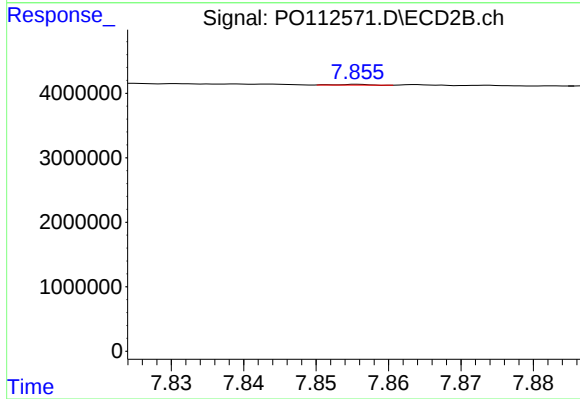


#43 AR-1268-3

R.T.: 7.856 min
Delta R.T.: 0.040 min
Response: 17726
Conc: 0.06 ng/ml

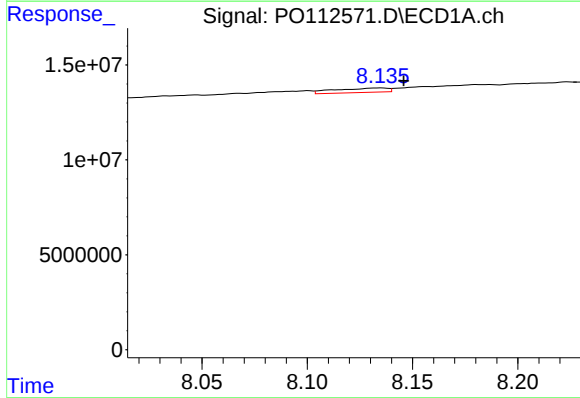


#44 AR-1268-4

R.T.: 8.135 min
Delta R.T.: -0.011 min
Response: 3963645
Conc: 8.23 ng/ml

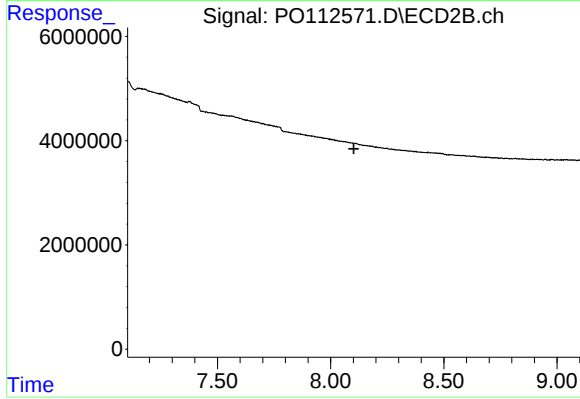

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T. : 8.103 min
Response: 0
Conc: N.D.

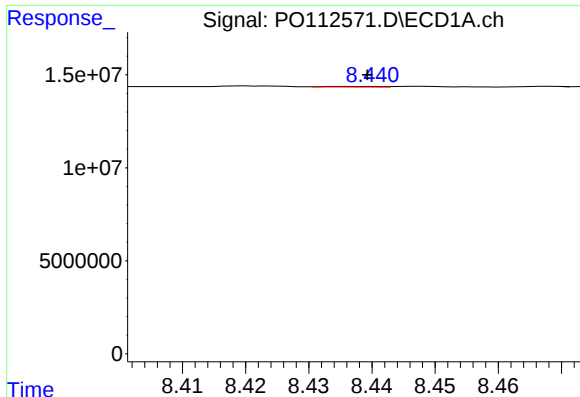

#45 AR-1268-5

R.T.: 8.435 min
Delta R.T.: -0.004 min
Response: 184139
Conc: 0.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

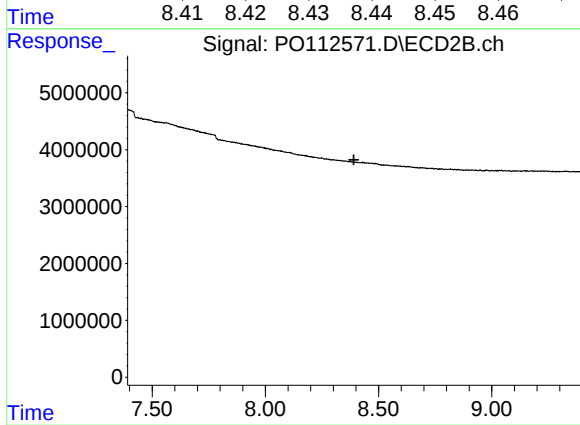

#45 AR-1268-5

R.T.: 8.372 min
Delta R.T.: -0.019 min
Response: -50957
Conc: N.D.