

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072925\
 Data File : P0112587.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jul 2025 20:11
 Operator : YP/AJ
 Sample : Q2720-03 10X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 M4A

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/30/2025
 Supervised By :mohammad ahmed 07/31/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 30 01:50:35 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 24 04:54:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.670	3.662	7600084	4500374	0.935	0.906
2) SA Decachlor...	8.693	8.639	7046306	1933241	0.964m	1.094

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO072925\
Data File : PO112587.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jul 2025 20:11
Operator : YP/AJ
Sample : Q2720-03 10X
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
M4A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/30/2025
Supervised By :mohammad ahmed 07/31/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 30 01:50:35 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072325.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 24 04:54:06 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

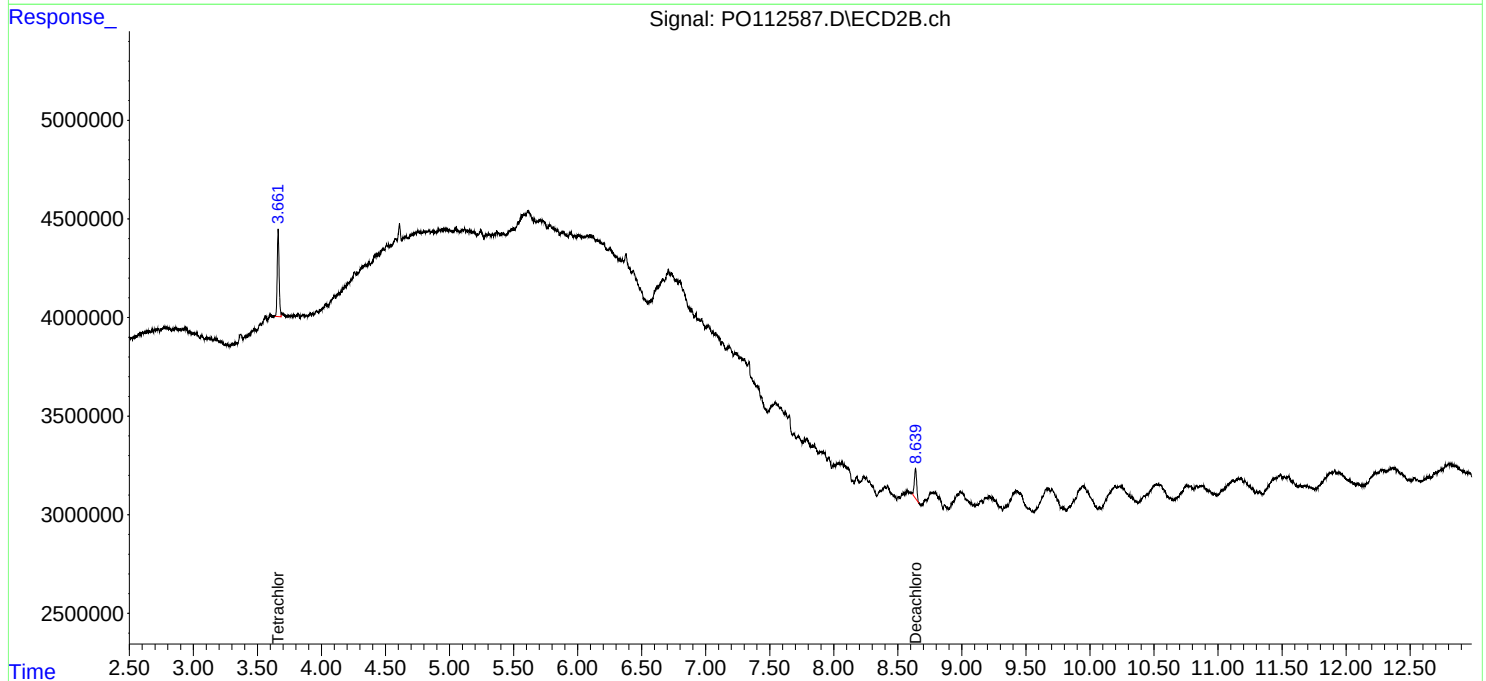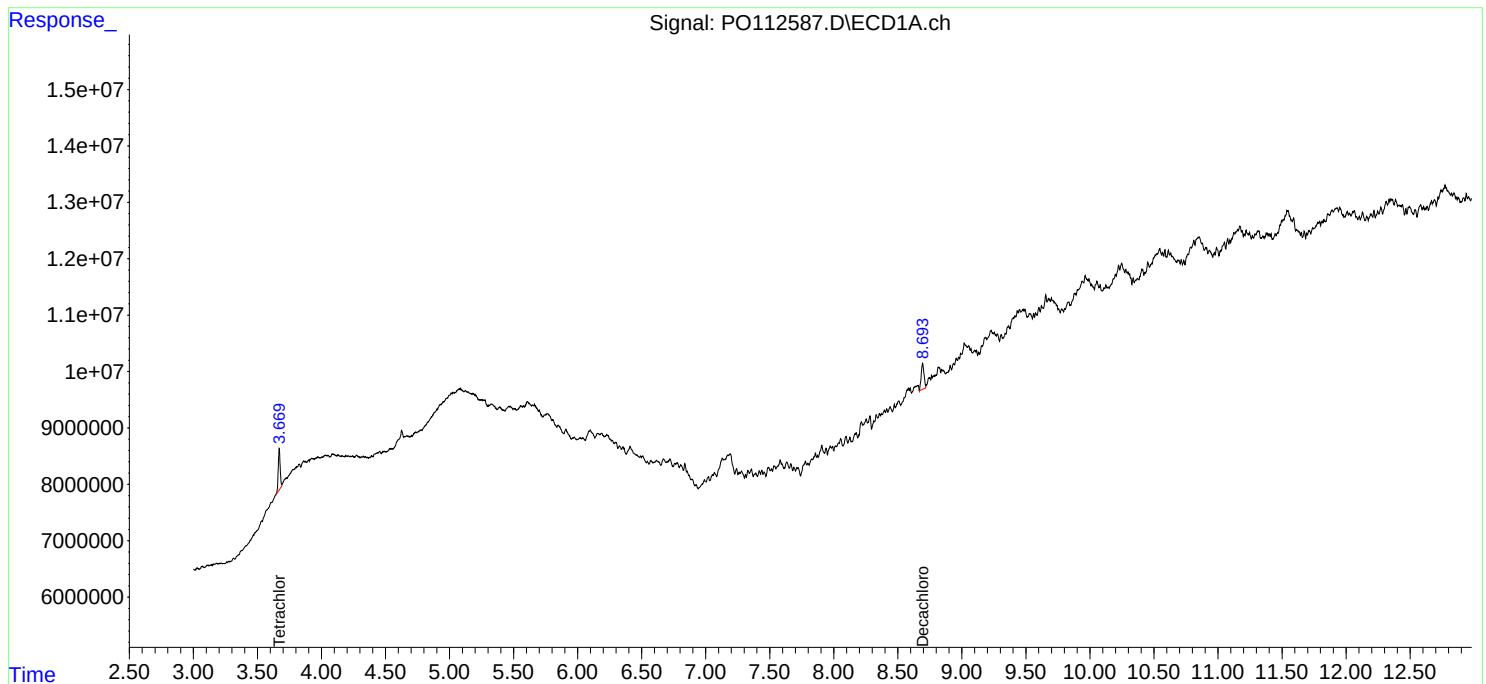

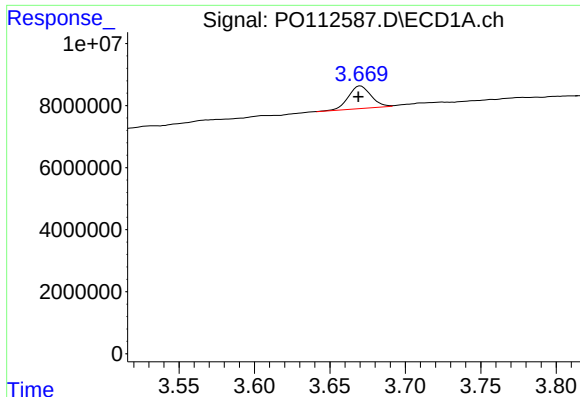


#1 Tetrachloro-m-xylene

R.T.: 3.670 min
Delta R.T.: 0.001 min
Response: 7600084
Conc: 0.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
M4A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/30/2025
Supervised By :mohammad ahmed 07/31/2025

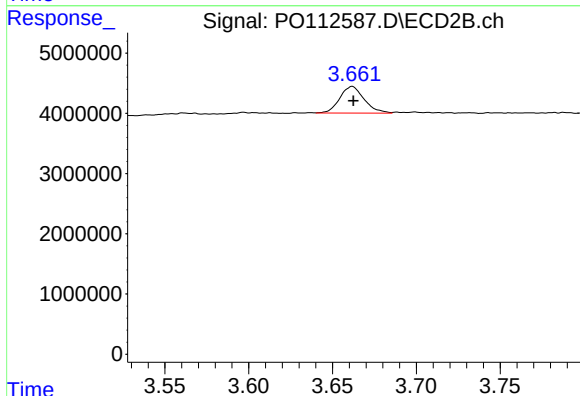


#1 Tetrachloro-m-xylene

R.T.: 3.662 min
Delta R.T.: 0.000 min
Response: 4500374
Conc: 0.91 ng/ml

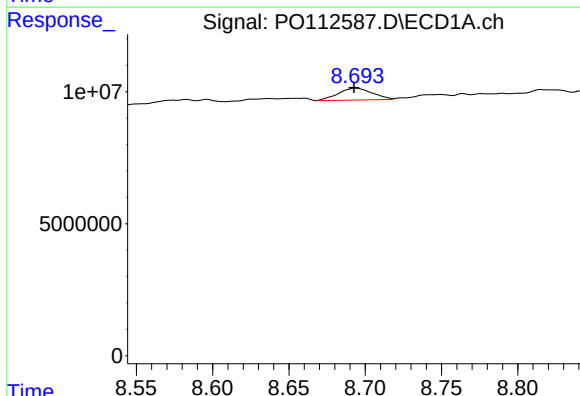

#2 Decachlorobiphenyl

R.T.: 8.693 min
Delta R.T.: 0.000 min
Response: 7046306
Conc: 0.96 ng/ml m

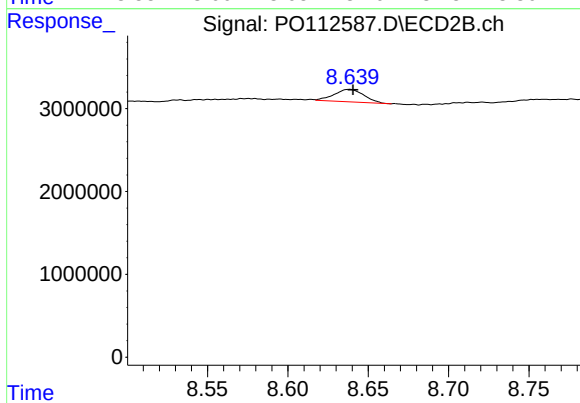

#2 Decachlorobiphenyl

R.T.: 8.639 min
Delta R.T.: -0.002 min
Response: 1933241
Conc: 1.09 ng/ml