

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0073018\
 Data File : P0047347.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Jul 2018 10:34
 Operator : SM/SJ
 Sample : J3762-07
 Misc : AR1660 25PPB LOD WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2018

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 31 03:48:40 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jul 27 02:33:29 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.398	3.644	3777159	4022939	18.708	16.372
2) SA Decachlor...	10.090	8.637	2843424	2831664	17.434	18.014
Target Compounds						
3) L1 AR-1016-1	5.299	4.508	159912	154723	33.479	27.064
4) L1 AR-1016-2	5.650	4.923	188524	130581	32.024	24.870
5) L1 AR-1016-3	5.749	4.963	150439	117436	30.335	26.746
6) L1 AR-1016-4	6.042	5.005	165644	135469	35.612	26.125 #
7) L1 AR-1016-5	6.181	5.177	154395	170467	29.617	29.062
8) L2 AR-1221-1	4.606	3.853	23902	21133	10.808	8.956
9) L2 AR-1221-2	4.703	3.944	85292	87907	52.160	48.459
10) L2 AR-1221-3	4.769	4.020	115552	115302	22.382	19.946
11) L3 AR-1232-1	5.105	4.317	146425	244128	68.088	103.808 #
12) L3 AR-1232-2	5.566	4.728	215501	198935	73.238	65.099
13) L3 AR-1232-3	5.588	4.747	292155	309250	68.003	66.969
14) L3 AR-1232-4	5.650	4.802	188524	158624	68.111	51.312
15) L3 AR-1232-5	5.749	4.963	150439	117436	67.367	65.617
16) L4 AR-1242-1	5.588	4.747	292155	309250	39.748	38.616
17) L4 AR-1242-2	5.650	4.923	188524	130581	40.732	31.697
18) L4 AR-1242-3	5.749	5.005	150439	135469	39.156	32.302
19) L4 AR-1242-4	6.042	5.177	165644	170467	43.089	36.099
20) L4 AR-1242-5	6.181	5.325	154395	163314	36.069	42.181
21) L5 AR-1248-1	6.042	5.177	165644	170467	26.490	22.850
22) L5 AR-1248-2	6.181	5.325	154395	163314	28.342	30.526
23) L5 AR-1248-3	6.444	5.528	57550	175128	8.178	17.600 #
24) L5 AR-1248-4	6.486	5.567	33742	51797	5.026	7.391 #
25) L5 AR-1248-5	6.634	6.091	128636	314624	18.175	66.017 #
26) L6 AR-1254-1	6.634	5.528	128636	175128	10.519	14.232 #
27) L6 AR-1254-2	6.915	5.673	40623	127164	5.447	12.216 #
28) L6 AR-1254-3	7.009	6.091	529126	314624	40.573	18.128 #
29) L6 AR-1254-4	7.287	6.304	45812	41143	4.700	3.797
30) L6 AR-1254-5	7.548	6.627	147744	26163	19.998	3.421 #
31) L7 AR-1260-1	7.163	6.207	226963	359272	24.204	32.513 #
32) L7 AR-1260-2	7.419	6.385	283347	880967	25.410	65.704 #
33) L7 AR-1260-3	7.702	6.720	408173	397180	31.725	27.320
34) L7 AR-1260-4	8.317	7.257	428766	536356	24.104	24.376
35) L7 AR-1260-5	8.639	7.603	287179	364195	25.148	23.346
36) L8 AR-1262-1	7.163	6.385	226963	880967	27.396	77.700 #
37) L8 AR-1262-2	7.419	6.547	283347	318681	29.236	28.241
38) L8 AR-1262-3	7.776	6.758	211108	226420	17.202	15.003

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0073018\
 Data File : P0047347.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Jul 2018 10:34
 Operator : SM/SJ
 Sample : J3762-07
 Misc : AR1660 25PPB LOD WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2018

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 31 03:48:40 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072718.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jul 27 02:33:29 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
39)	L8 AR-1262-4	8.002	7.017	218145	222734	18.525	16.915
40)	L8 AR-1262-5	8.317	7.257	428766	536356	19.956	20.766
41)	L9 AR-1268-1	8.639	7.541	287179	95027	12.373	3.655 #
42)	L9 AR-1268-2	8.692	7.603	167351	364195	7.810	14.619 #
43)	L9 AR-1268-3	8.943	7.810	13066	15557	0.724	0.788
44)	L9 AR-1268-4	9.357	8.096	137564	111647	17.252	13.310
45)	L9 AR-1268-5	9.757	8.384	63681	48996	1.169	0.897



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0073018\
Data File : P0047347.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Jul 2018 10:34
Operator : SM/SJ
Sample : J3762-07
Misc : AR1660 25PPB LOD WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2018

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 31 03:48:40 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072718.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 27 02:33:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

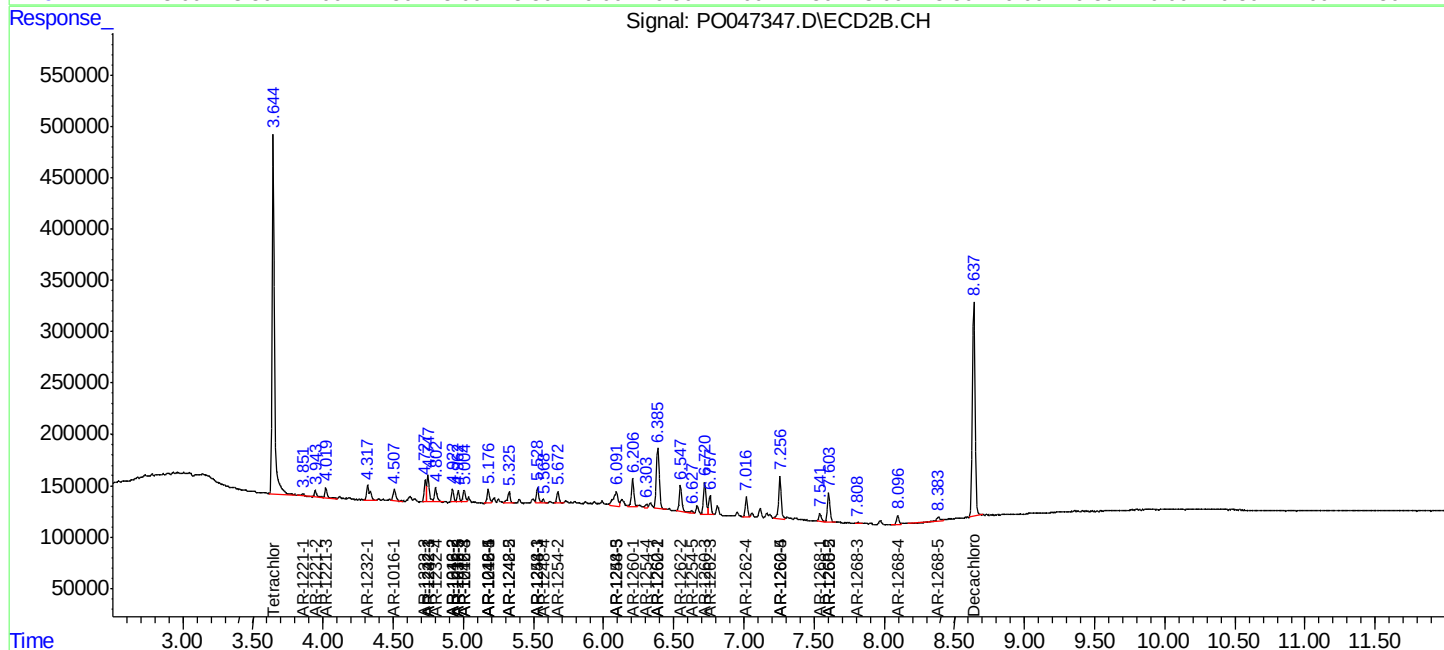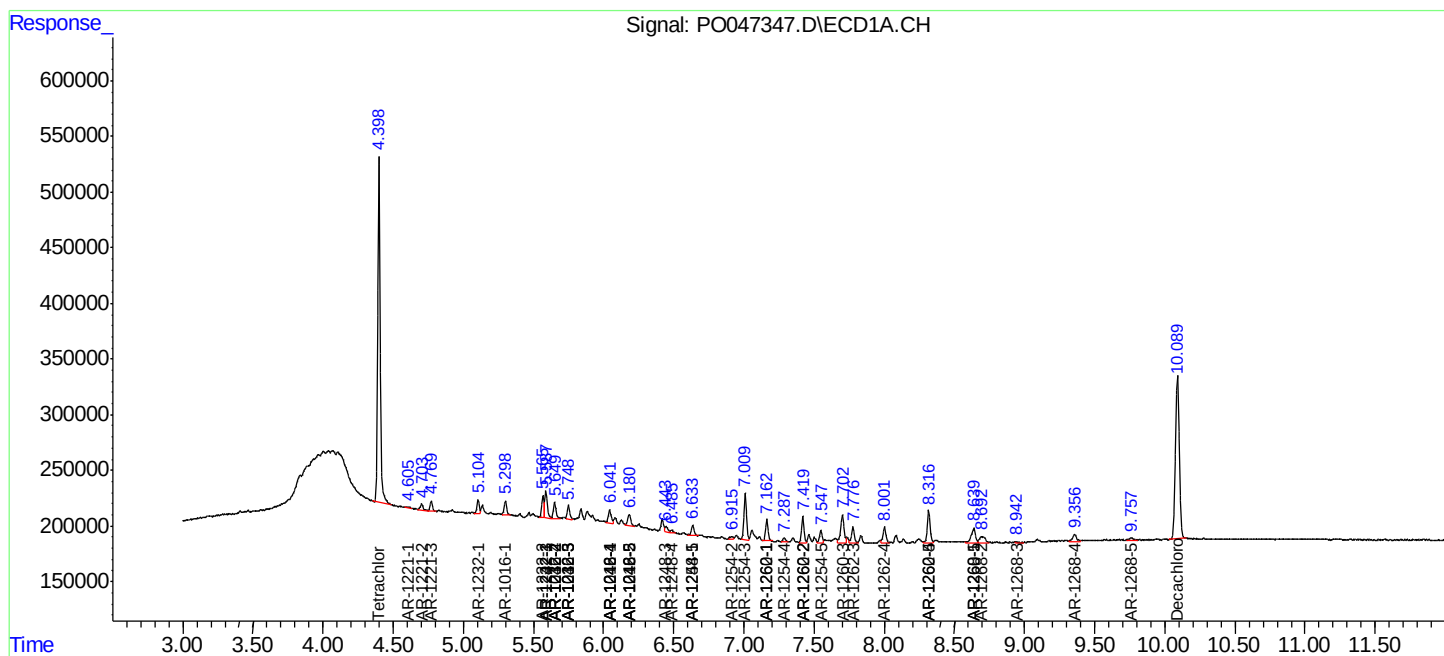


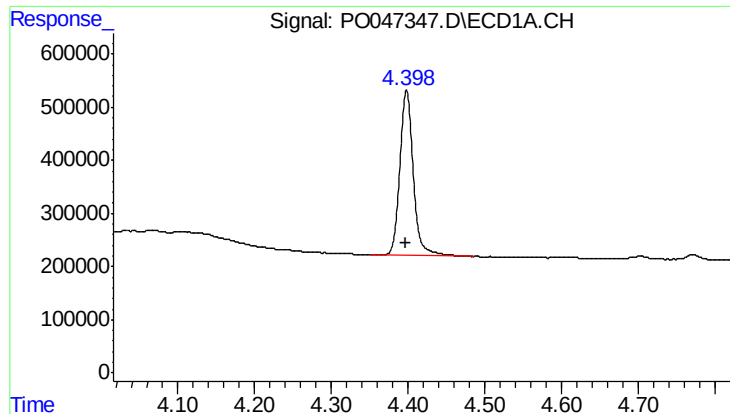

#1 Tetrachloro-m-xylene


R.T.: 4.398 min
Delta R.T.: 0.000 min
Response: 3777159
Conc: 18.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2018

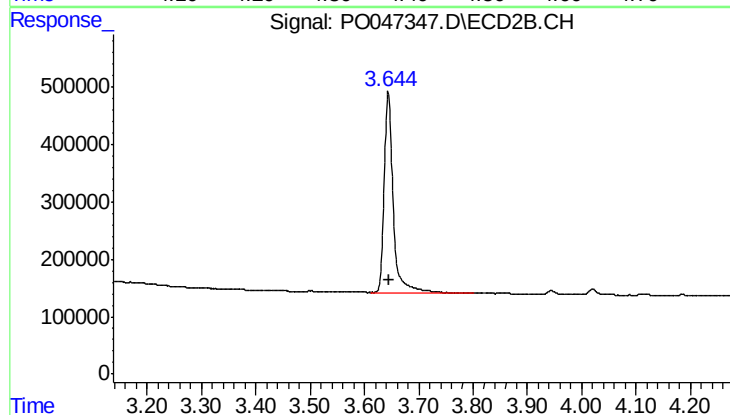


#1 Tetrachloro-m-xylene

R.T.: 3.644 min
Delta R.T.: -0.001 min
Response: 4022939
Conc: 16.37 ng/ml

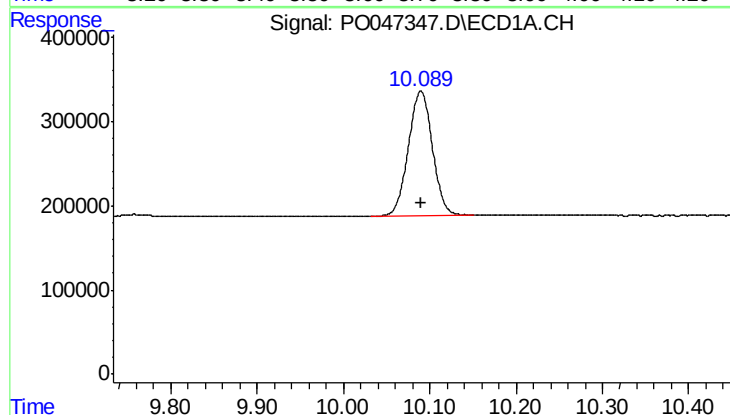


#2 Decachlorobiphenyl

R.T.: 10.090 min
Delta R.T.: 0.000 min
Response: 2843424
Conc: 17.43 ng/ml

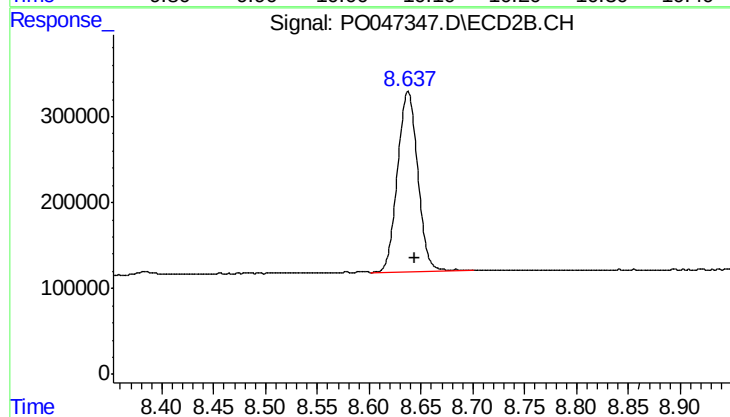

#2 Decachlorobiphenyl


R.T.: 8.637 min
Delta R.T.: -0.007 min
Response: 2831664
Conc: 18.01 ng/ml

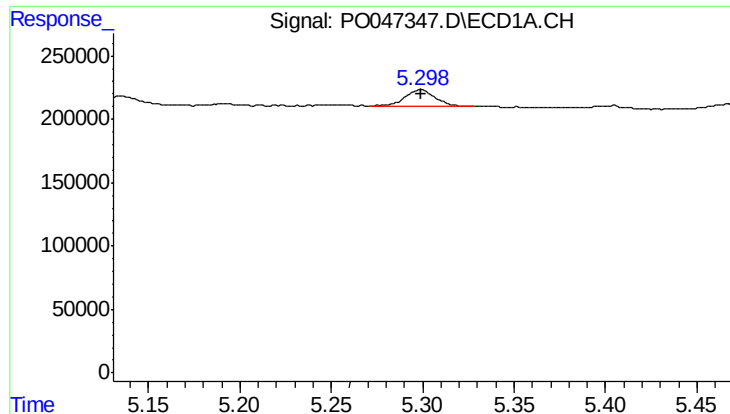

#3 AR-1016-1


R.T.: 5.299 min
Delta R.T.: 0.000 min
Response: 159912
Conc: 33.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2018

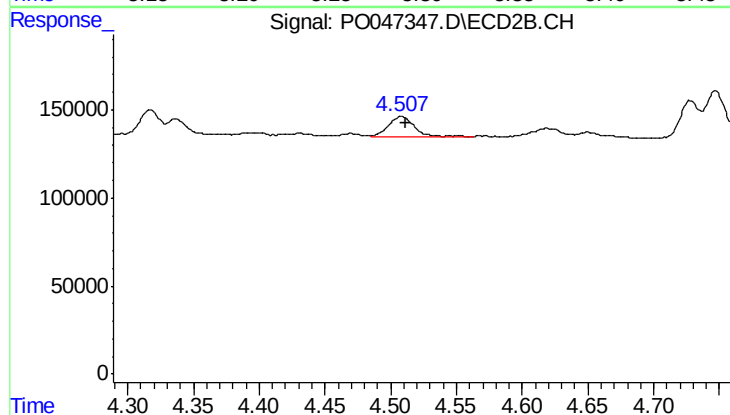


#3 AR-1016-1

R.T.: 4.508 min
Delta R.T.: -0.003 min
Response: 154723
Conc: 27.06 ng/ml

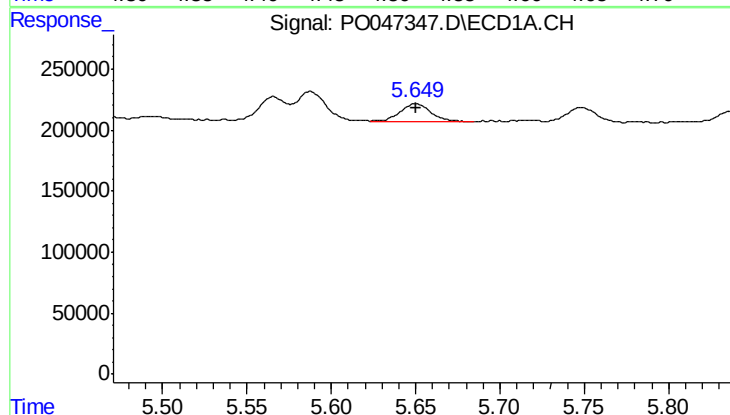


#4 AR-1016-2

R.T.: 5.650 min
Delta R.T.: 0.000 min
Response: 188524
Conc: 32.02 ng/ml

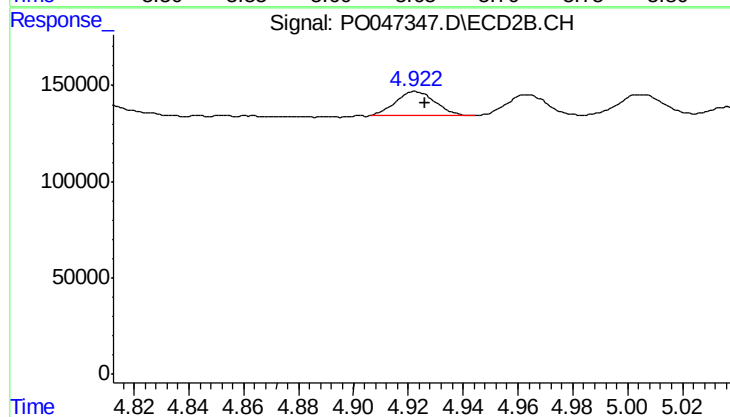

#4 AR-1016-2


R.T.: 4.923 min
Delta R.T.: -0.003 min
Response: 130581
Conc: 24.87 ng/ml

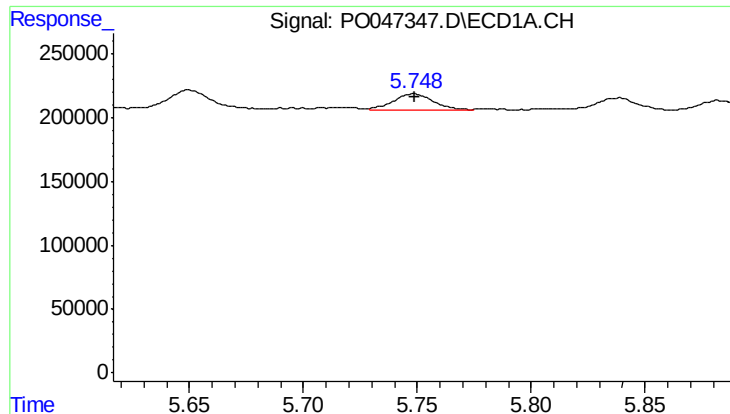

#5 AR-1016-3


R.T.: 5.749 min
Delta R.T.: 0.000 min
Response: 150439
Conc: 30.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2018

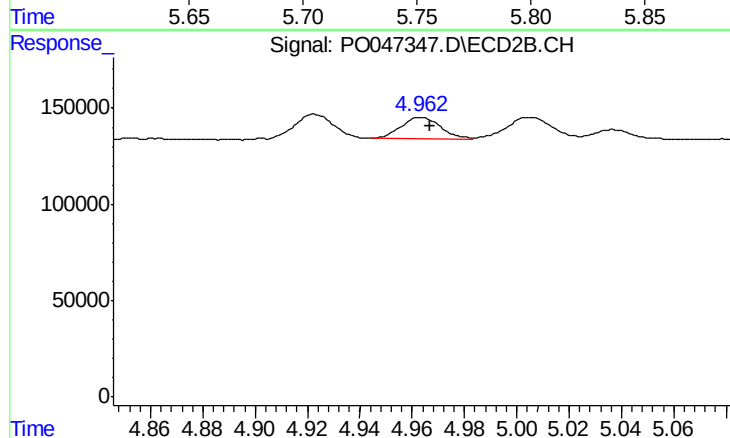


#5 AR-1016-3

R.T.: 4.963 min
Delta R.T.: -0.004 min
Response: 117436
Conc: 26.75 ng/ml

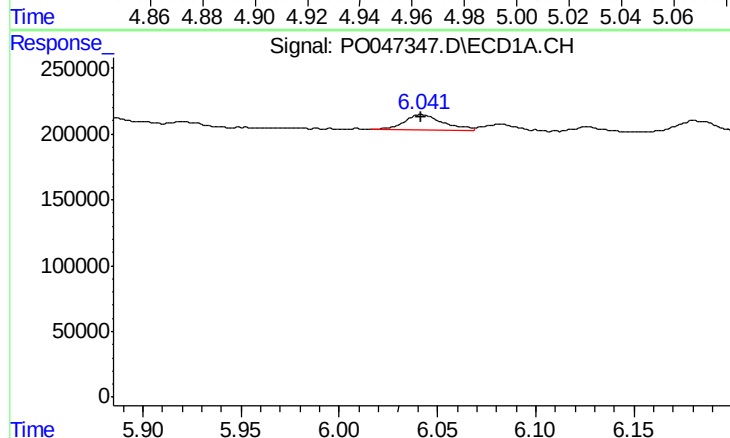


#6 AR-1016-4

R.T.: 6.042 min
Delta R.T.: 0.000 min
Response: 165644
Conc: 35.61 ng/ml

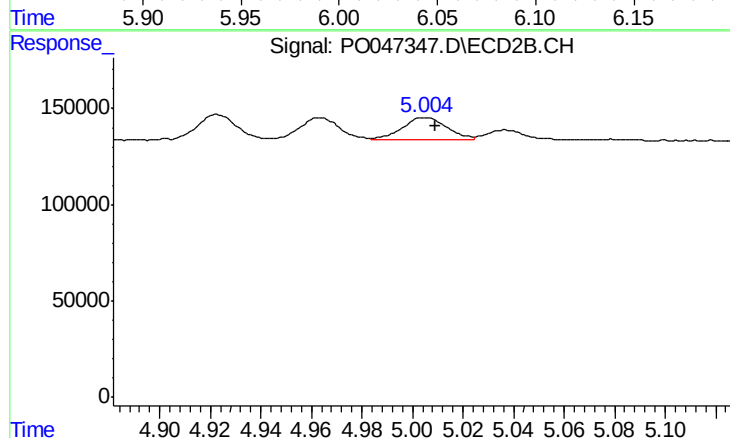

#6 AR-1016-4


R.T.: 5.005 min
Delta R.T.: -0.004 min
Response: 135469
Conc: 26.12 ng/ml

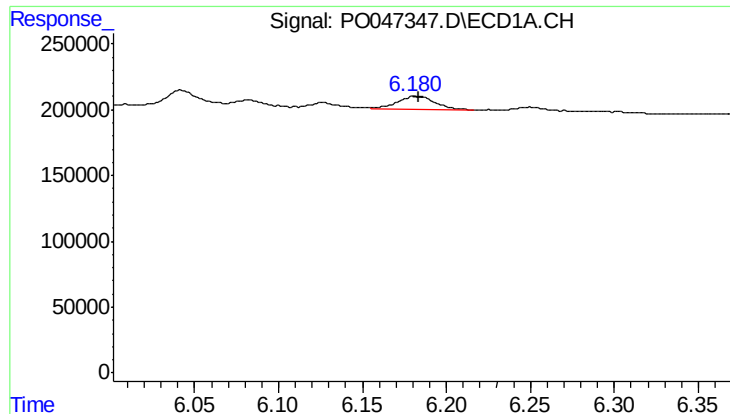

#7 AR-1016-5


R.T.: 6.181 min
Delta R.T.: -0.003 min
Response: 154395
Conc: 29.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2018

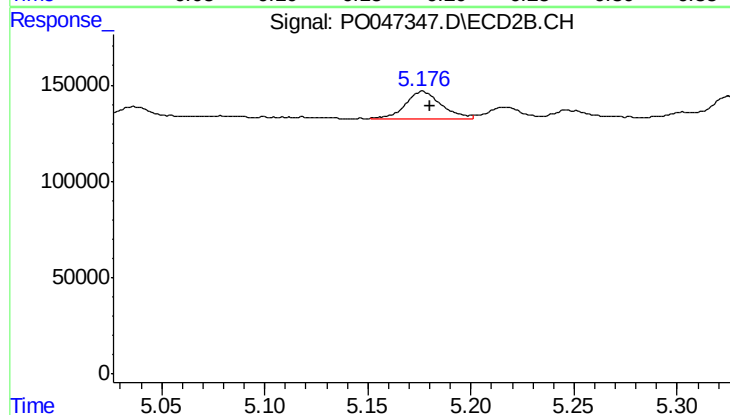


#7 AR-1016-5

R.T.: 5.177 min
Delta R.T.: -0.004 min
Response: 170467
Conc: 29.06 ng/ml

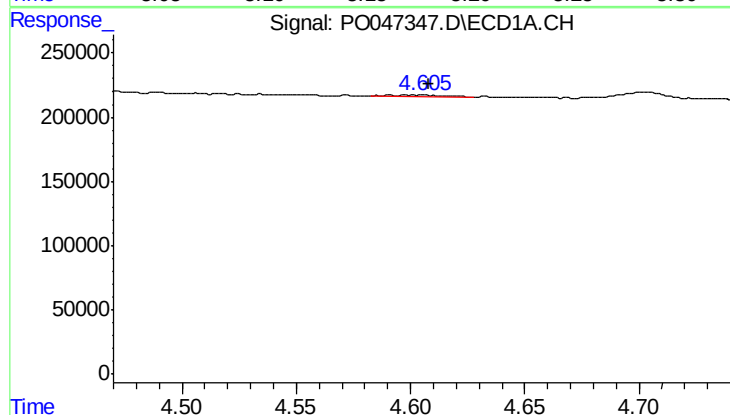


#8 AR-1221-1

R.T.: 4.606 min
Delta R.T.: -0.003 min
Response: 23902
Conc: 10.81 ng/ml

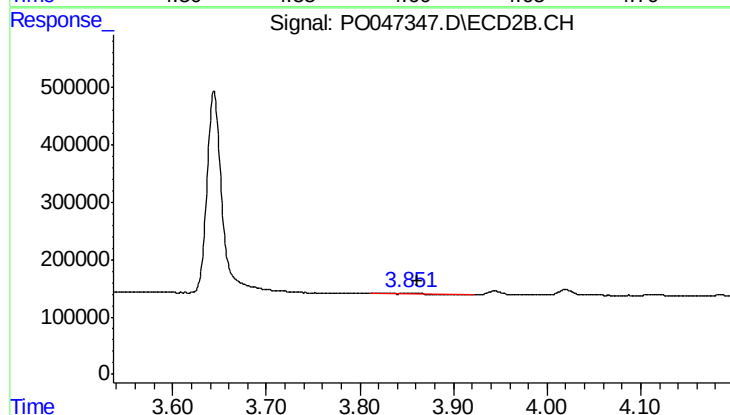

#8 AR-1221-1


R.T.: 3.853 min
Delta R.T.: -0.008 min
Response: 21133
Conc: 8.96 ng/ml

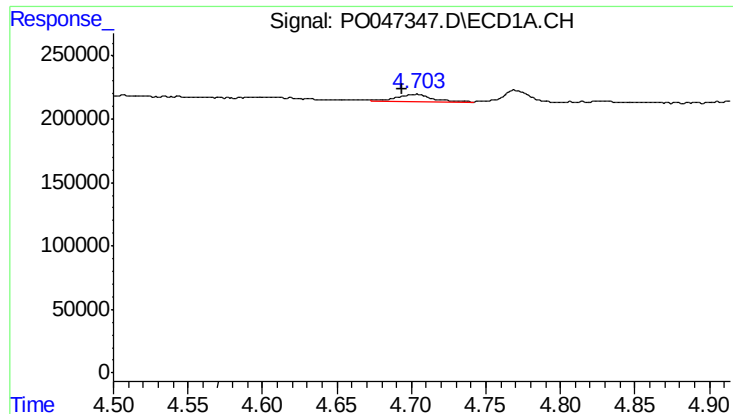

#9 AR-1221-2


R.T.: 4.703 min
Delta R.T.: 0.009 min
Response: 85292
Conc: 52.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2018

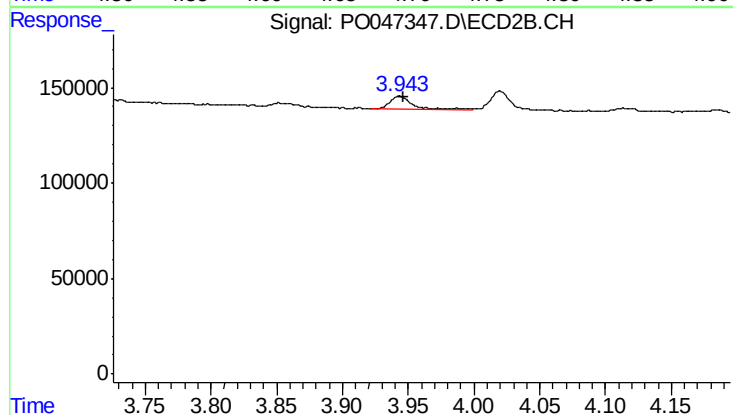


#9 AR-1221-2

R.T.: 3.944 min
Delta R.T.: -0.002 min
Response: 87907
Conc: 48.46 ng/ml

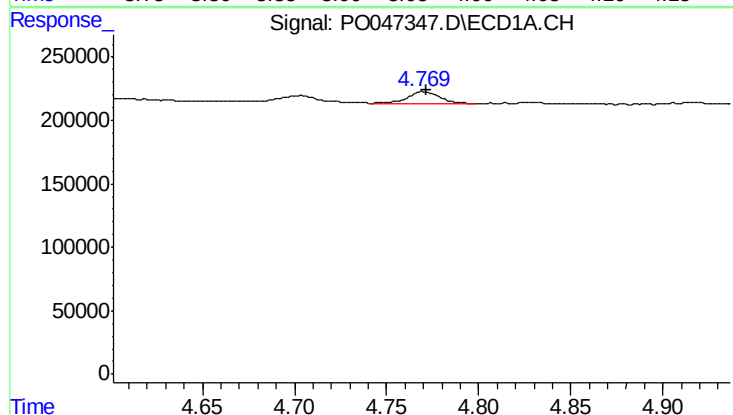


#10 AR-1221-3

R.T.: 4.769 min
Delta R.T.: -0.002 min
Response: 115552
Conc: 22.38 ng/ml

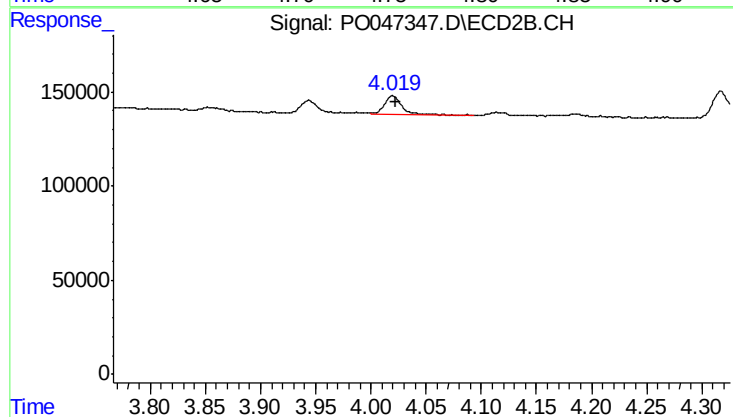

#10 AR-1221-3


R.T.: 4.020 min
Delta R.T.: -0.003 min
Response: 115302
Conc: 19.95 ng/ml

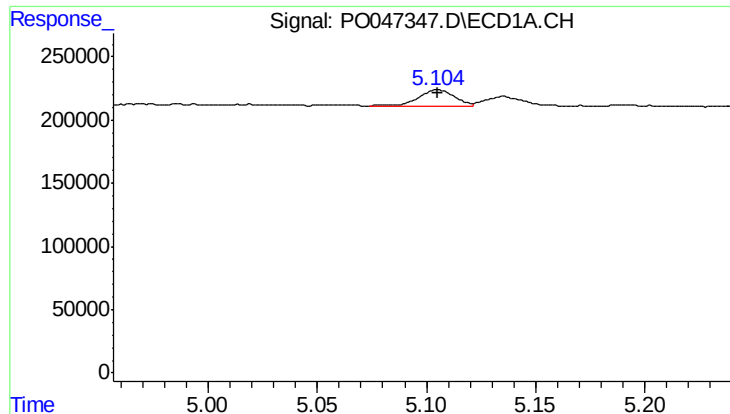

#11 AR-1232-1


R.T.: 5.105 min
Delta R.T.: 0.000 min
Response: 146425
Conc: 68.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2018

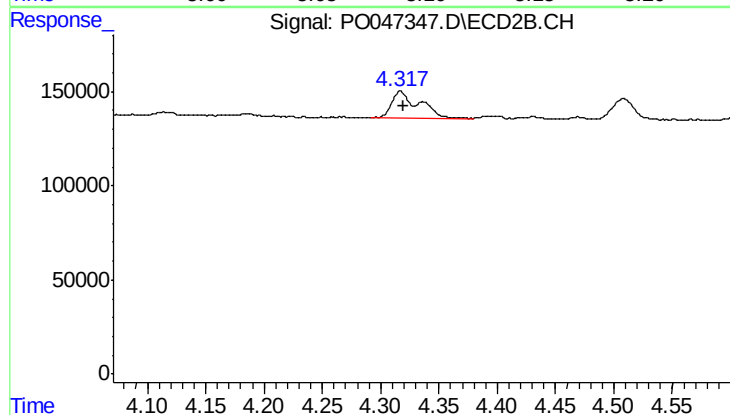


#11 AR-1232-1

R.T.: 4.317 min
Delta R.T.: -0.003 min
Response: 244128
Conc: 103.81 ng/ml

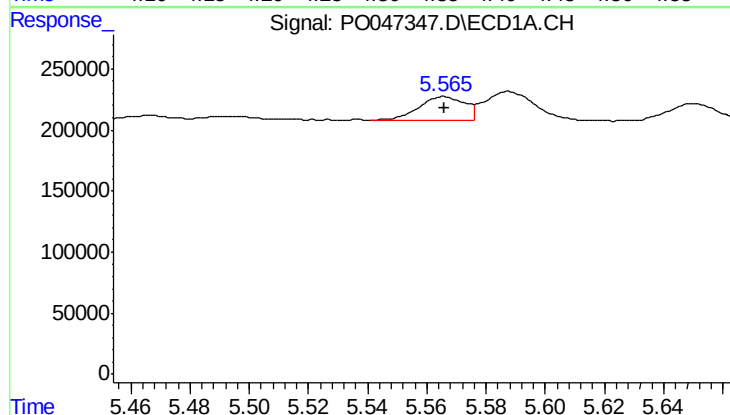


#12 AR-1232-2

R.T.: 5.566 min
Delta R.T.: 0.000 min
Response: 215501
Conc: 73.24 ng/ml

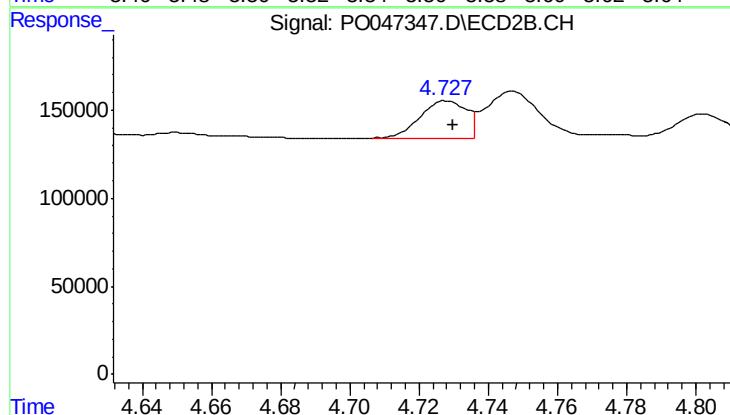

#12 AR-1232-2


R.T.: 4.728 min
Delta R.T.: -0.002 min
Response: 198935
Conc: 65.10 ng/ml

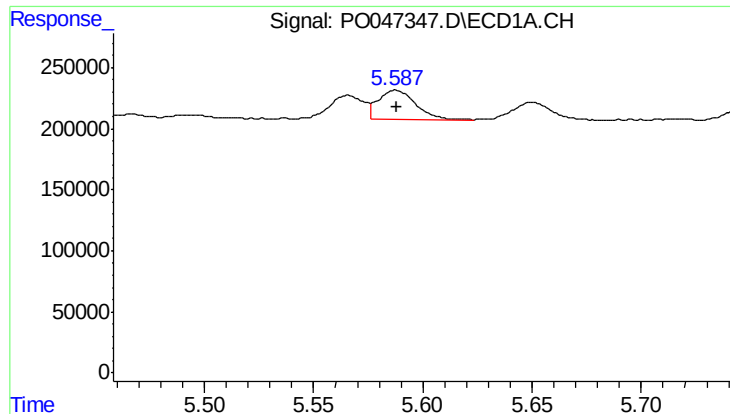

#13 AR-1232-3


R.T.: 5.588 min
Delta R.T.: 0.000 min
Response: 292155
Conc: 68.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2018

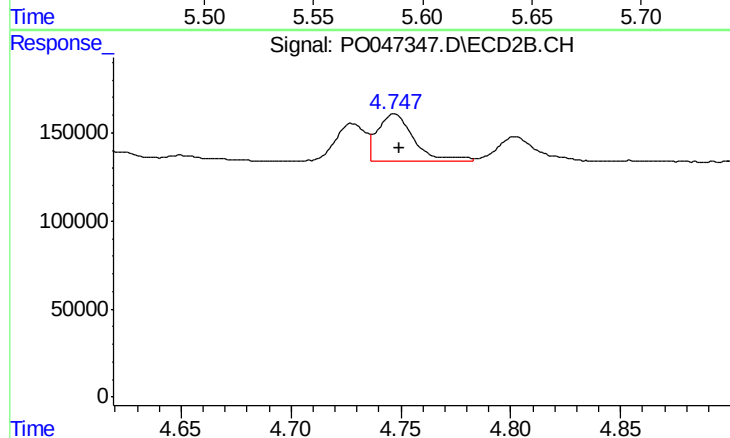


#13 AR-1232-3

R.T.: 4.747 min
Delta R.T.: -0.003 min
Response: 309250
Conc: 66.97 ng/ml

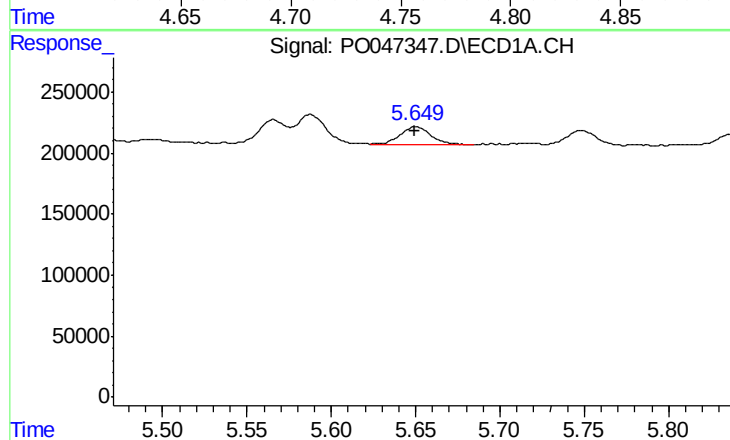


#14 AR-1232-4

R.T.: 5.650 min
Delta R.T.: 0.000 min
Response: 188524
Conc: 68.11 ng/ml

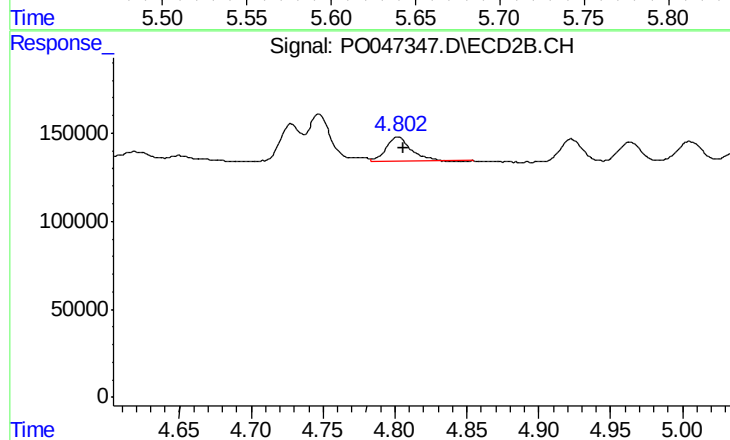

#14 AR-1232-4


R.T.: 4.802 min
Delta R.T.: -0.003 min
Response: 158624
Conc: 51.31 ng/ml

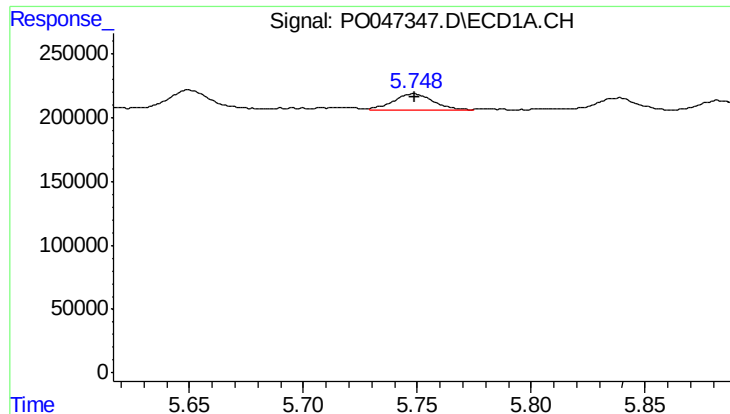

#15 AR-1232-5


R.T.: 5.749 min
Delta R.T.: 0.000 min
Response: 150439
Conc: 67.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2018

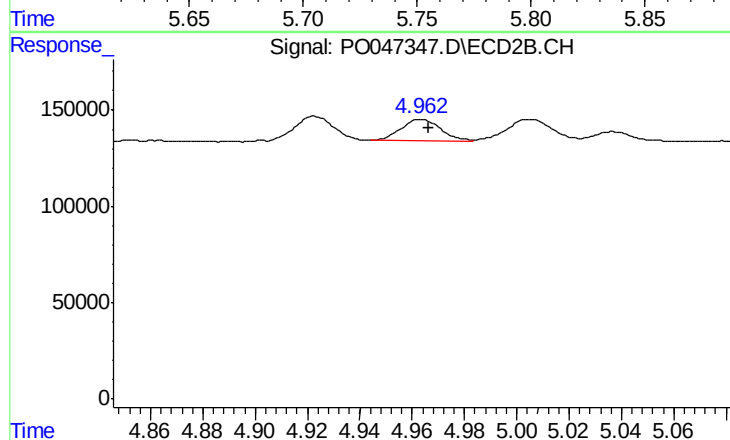


#15 AR-1232-5

R.T.: 4.963 min
Delta R.T.: -0.003 min
Response: 117436
Conc: 65.62 ng/ml

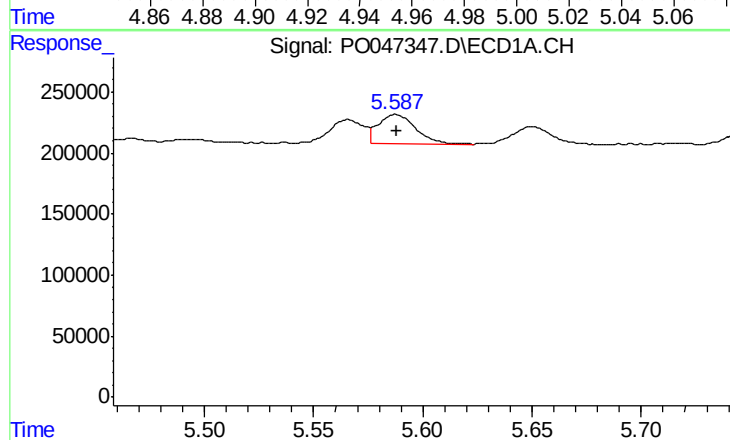


#16 AR-1242-1

R.T.: 5.588 min
Delta R.T.: 0.000 min
Response: 292155
Conc: 39.75 ng/ml

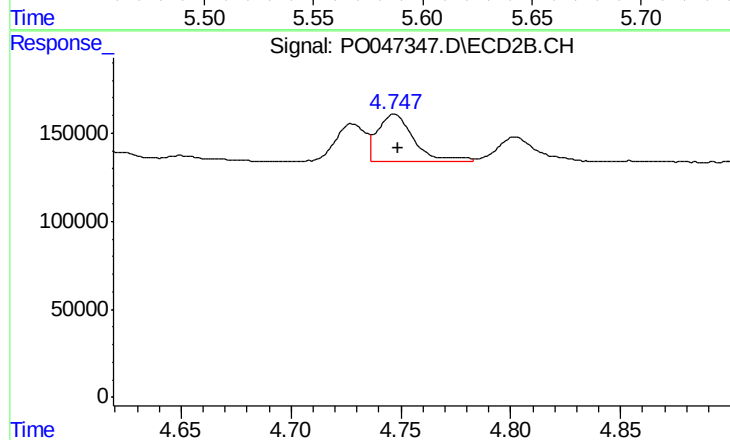

#16 AR-1242-1


R.T.: 4.747 min
Delta R.T.: -0.002 min
Response: 309250
Conc: 38.62 ng/ml

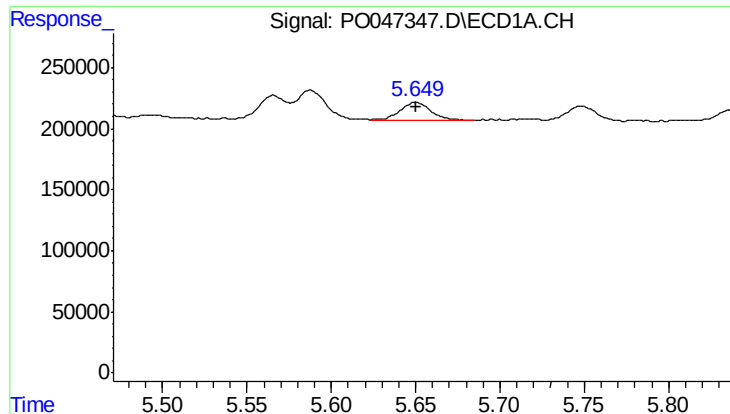

#17 AR-1242-2


R.T.: 5.650 min
Delta R.T.: 0.000 min
Response: 188524
Conc: 40.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2018

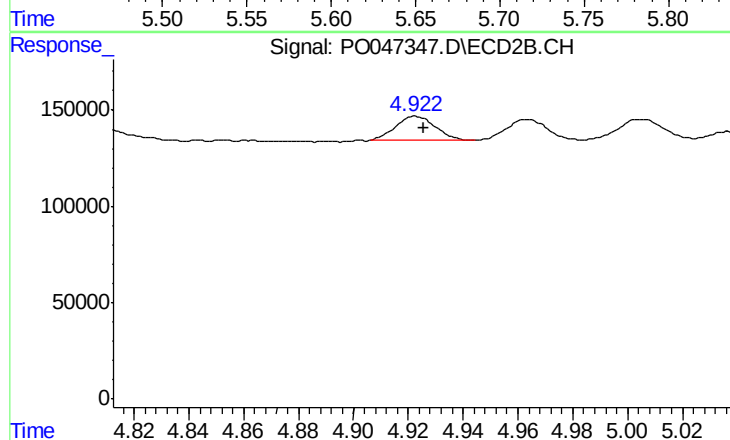


#17 AR-1242-2

R.T.: 4.923 min
Delta R.T.: -0.003 min
Response: 130581
Conc: 31.70 ng/ml

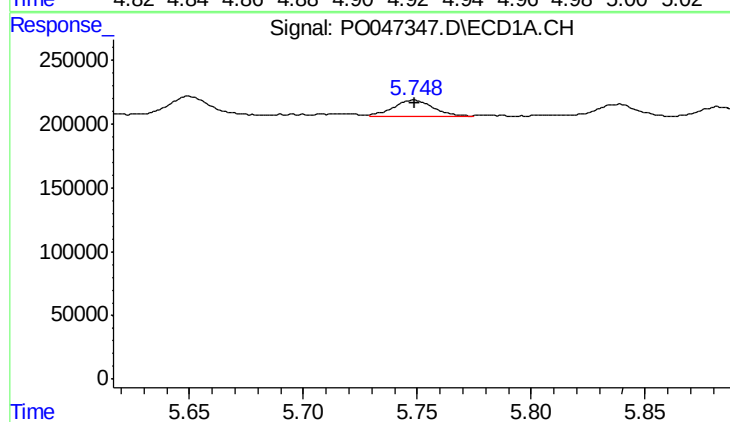


#18 AR-1242-3

R.T.: 5.749 min
Delta R.T.: 0.000 min
Response: 150439
Conc: 39.16 ng/ml

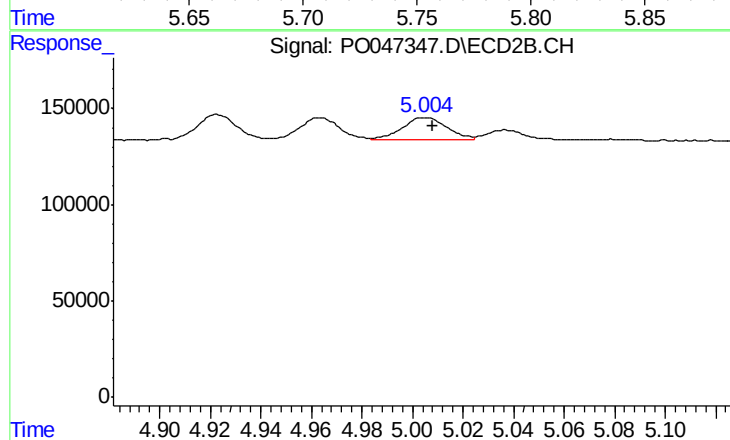

#18 AR-1242-3


R.T.: 5.005 min
Delta R.T.: -0.003 min
Response: 135469
Conc: 32.30 ng/ml

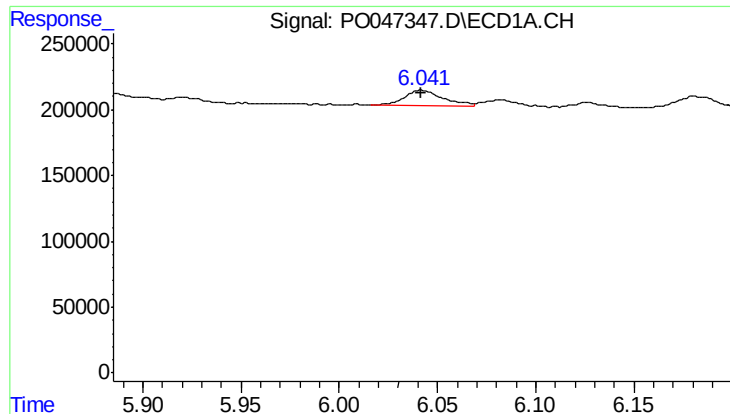

#19 AR-1242-4


R.T.: 6.042 min
Delta R.T.: 0.000 min
Response: 165644
Conc: 43.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2018

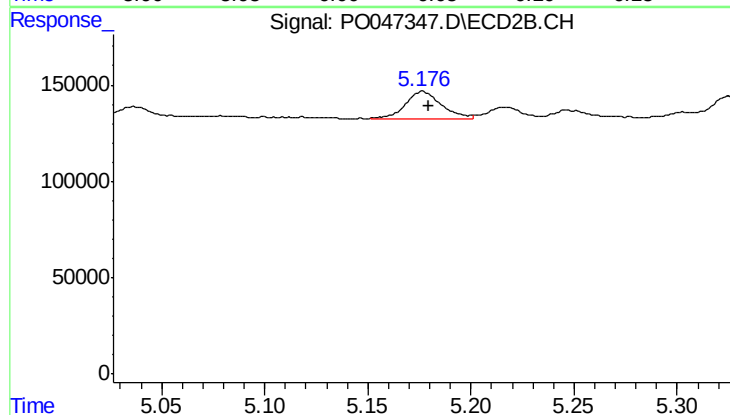


#19 AR-1242-4

R.T.: 5.177 min
Delta R.T.: -0.003 min
Response: 170467
Conc: 36.10 ng/ml

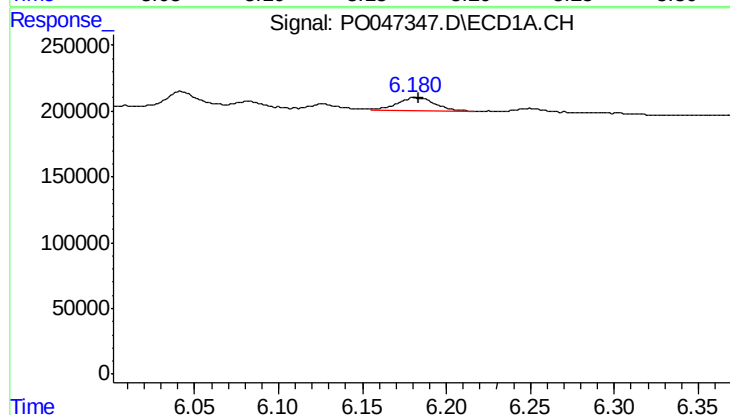


#20 AR-1242-5

R.T.: 6.181 min
Delta R.T.: -0.002 min
Response: 154395
Conc: 36.07 ng/ml

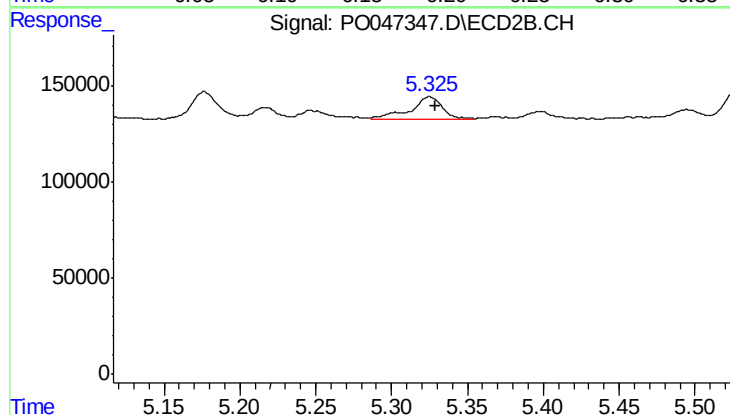

#20 AR-1242-5


R.T.: 5.325 min
Delta R.T.: -0.003 min
Response: 163314
Conc: 42.18 ng/ml

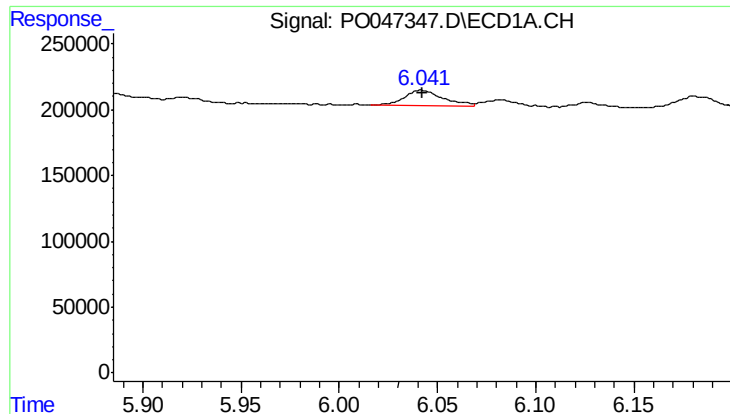

#21 AR-1248-1


R.T.: 6.042 min
Delta R.T.: 0.000 min
Response: 165644
Conc: 26.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2018

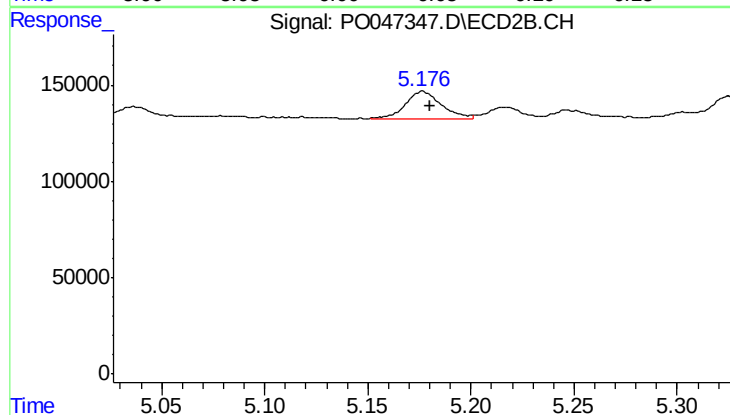


#21 AR-1248-1

R.T.: 5.177 min
Delta R.T.: -0.004 min
Response: 170467
Conc: 22.85 ng/ml

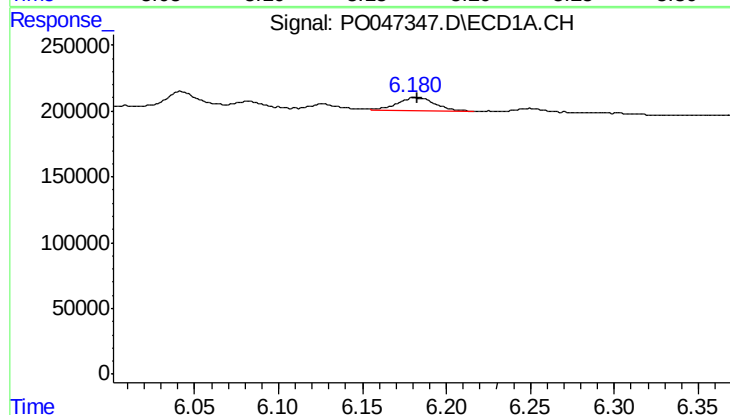


#22 AR-1248-2

R.T.: 6.181 min
Delta R.T.: -0.002 min
Response: 154395
Conc: 28.34 ng/ml

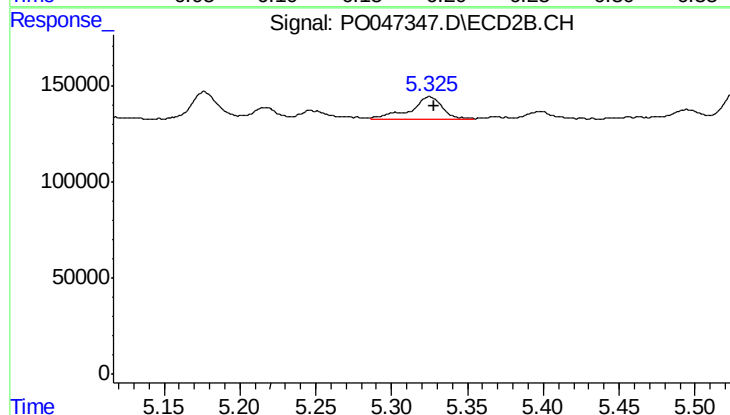

#22 AR-1248-2


R.T.: 5.325 min
Delta R.T.: -0.003 min
Response: 163314
Conc: 30.53 ng/ml

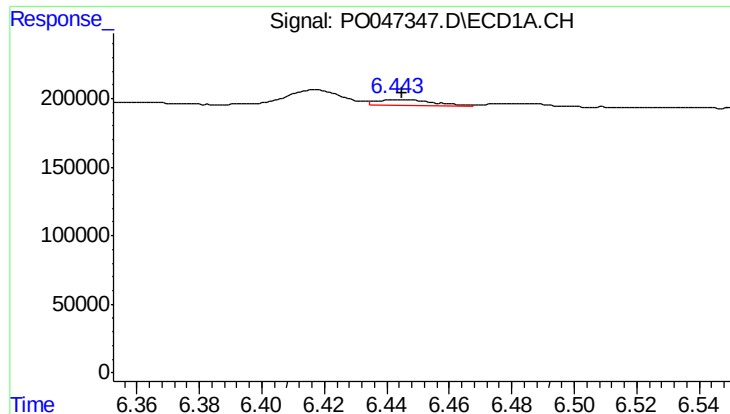

#23 AR-1248-3


R.T.: 6.444 min
Delta R.T.: -0.001 min
Response: 57550
Conc: 8.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2018

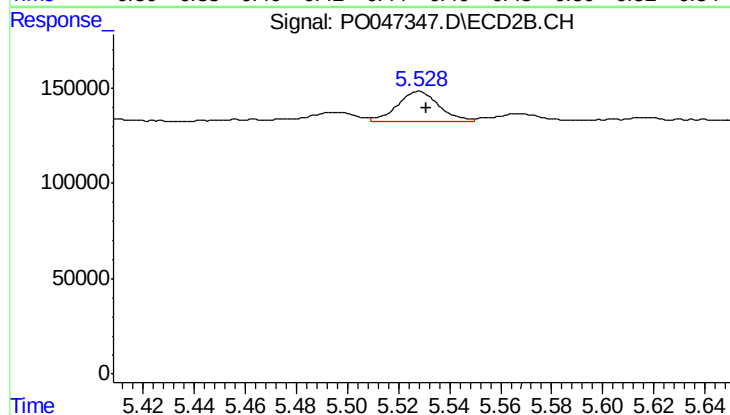


#23 AR-1248-3

R.T.: 5.528 min
Delta R.T.: -0.003 min
Response: 175128
Conc: 17.60 ng/ml

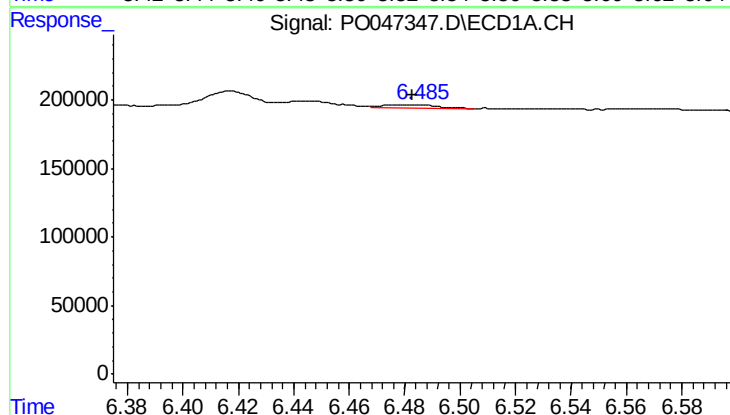


#24 AR-1248-4

R.T.: 6.486 min
Delta R.T.: 0.003 min
Response: 33742
Conc: 5.03 ng/ml

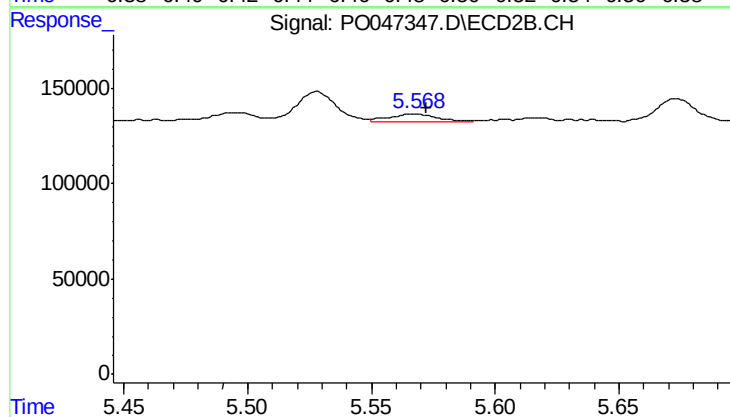

#24 AR-1248-4


R.T.: 5.567 min
Delta R.T.: -0.005 min
Response: 51797
Conc: 7.39 ng/ml

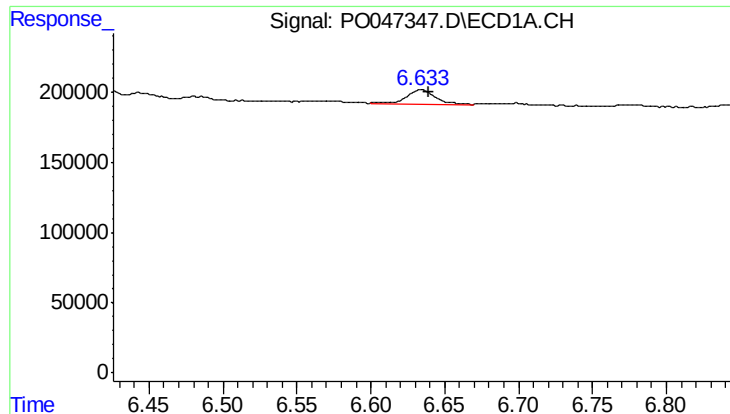

#25 AR-1248-5


R.T.: 6.634 min
Delta R.T.: -0.006 min
Response: 128636
Conc: 18.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2018

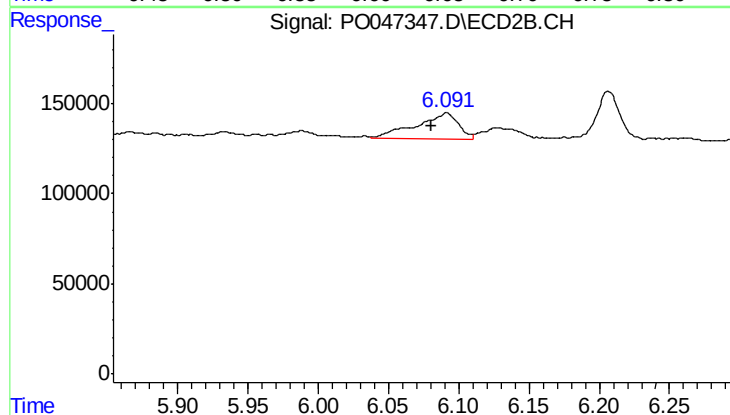


#25 AR-1248-5

R.T.: 6.091 min
Delta R.T.: 0.010 min
Response: 314624
Conc: 66.02 ng/ml

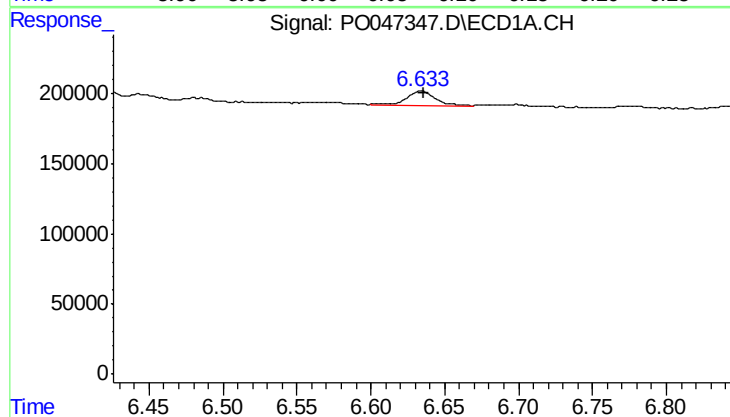


#26 AR-1254-1

R.T.: 6.634 min
Delta R.T.: -0.002 min
Response: 128636
Conc: 10.52 ng/ml

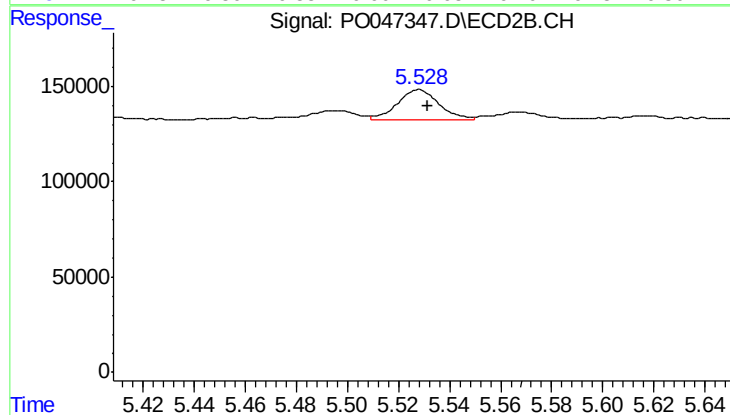

#26 AR-1254-1


R.T.: 5.528 min
Delta R.T.: -0.003 min
Response: 175128
Conc: 14.23 ng/ml

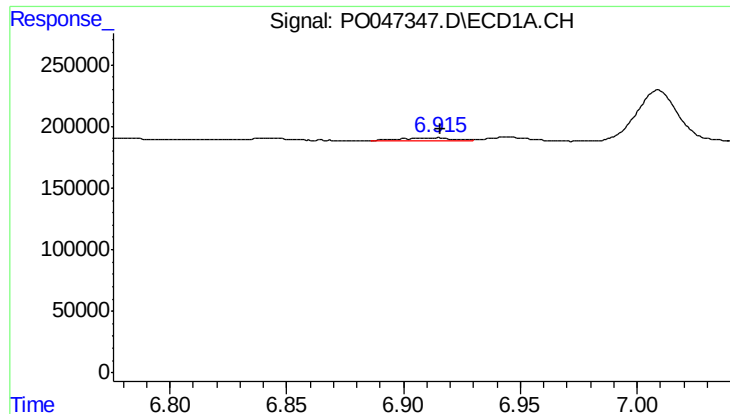

#27 AR-1254-2


R.T.: 6.915 min
Delta R.T.: -0.001 min
Response: 40623
Conc: 5.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2018

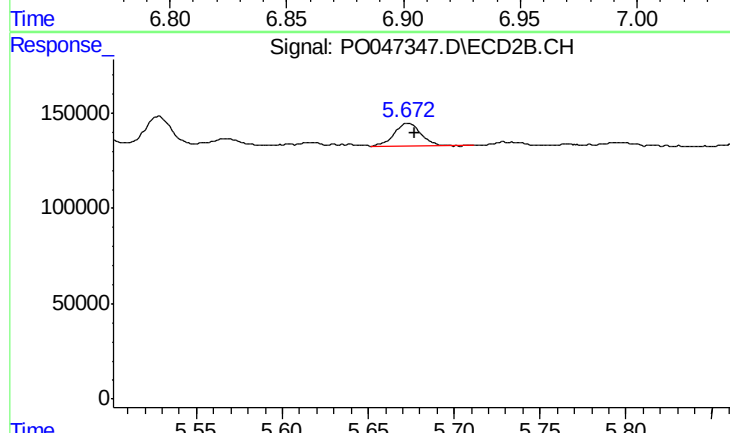


#27 AR-1254-2

R.T.: 5.673 min
Delta R.T.: -0.004 min
Response: 127164
Conc: 12.22 ng/ml

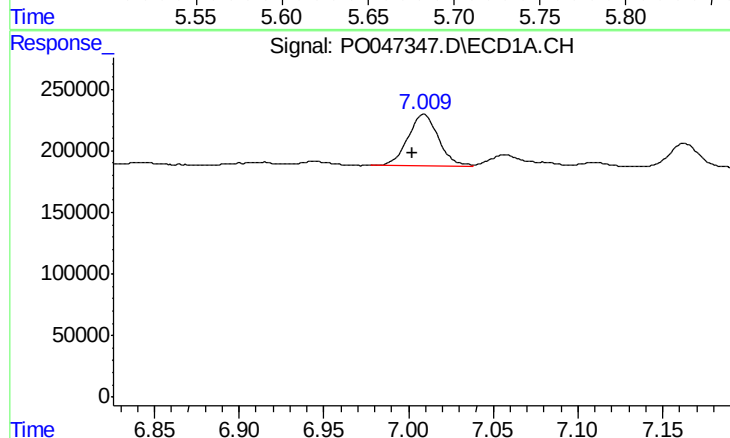


#28 AR-1254-3

R.T.: 7.009 min
Delta R.T.: 0.007 min
Response: 529126
Conc: 40.57 ng/ml

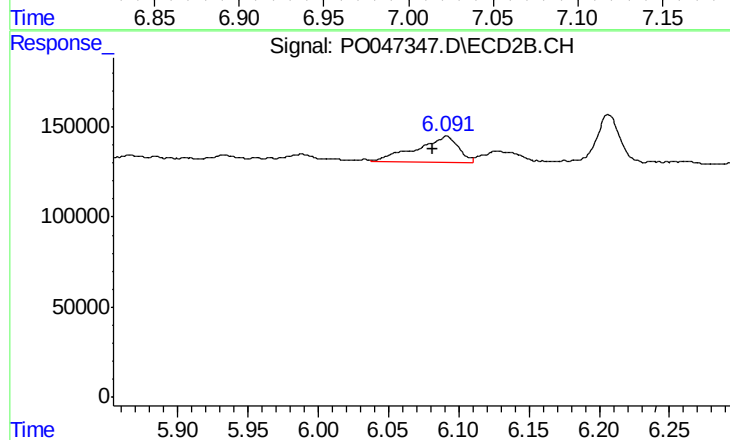

#28 AR-1254-3


R.T.: 6.091 min
Delta R.T.: 0.009 min
Response: 314624
Conc: 18.13 ng/ml

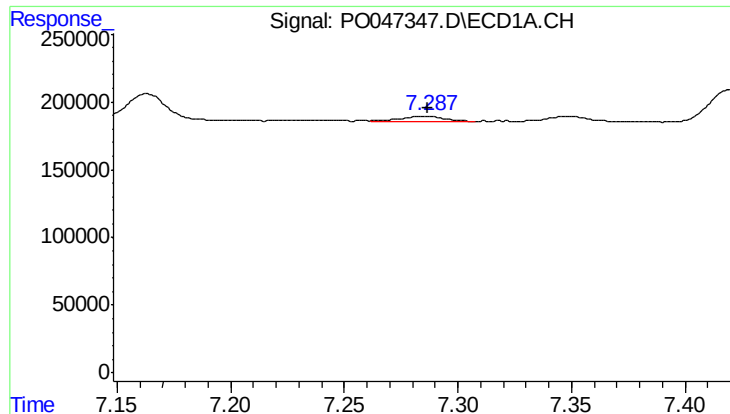

#29 AR-1254-4


R.T.: 7.287 min
Delta R.T.: 0.000 min
Response: 45812
Conc: 4.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2018

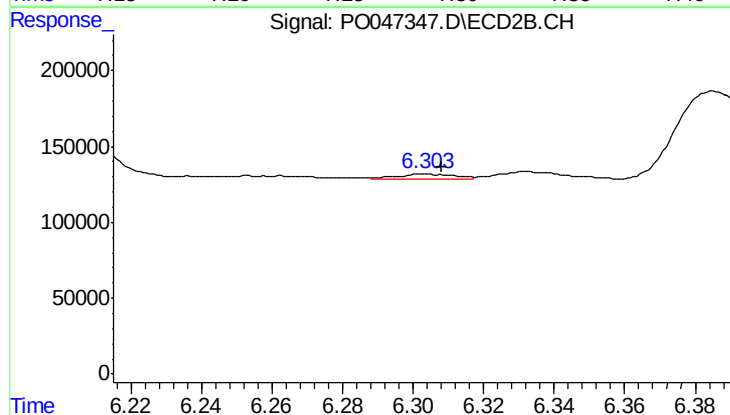


#29 AR-1254-4

R.T.: 6.304 min
Delta R.T.: -0.004 min
Response: 41143
Conc: 3.80 ng/ml

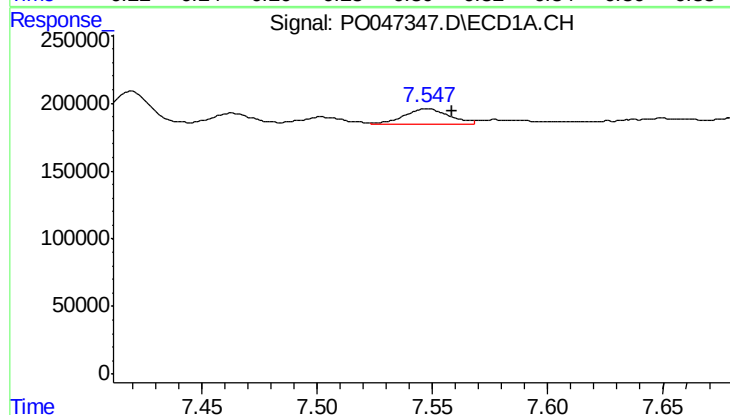


#30 AR-1254-5

R.T.: 7.548 min
Delta R.T.: -0.011 min
Response: 147744
Conc: 20.00 ng/ml

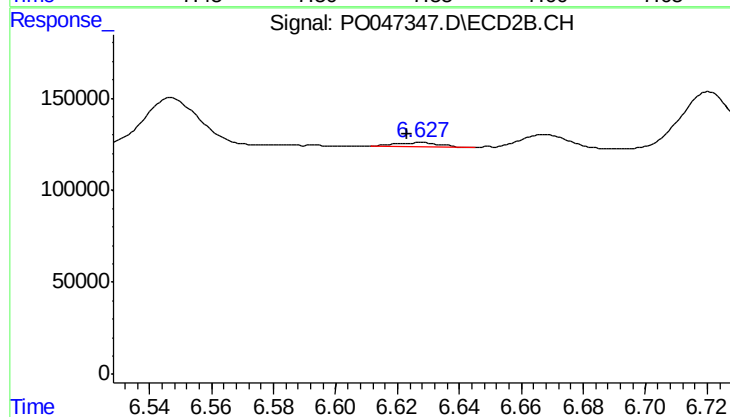

#30 AR-1254-5


R.T.: 6.627 min
Delta R.T.: 0.003 min
Response: 26163
Conc: 3.42 ng/ml

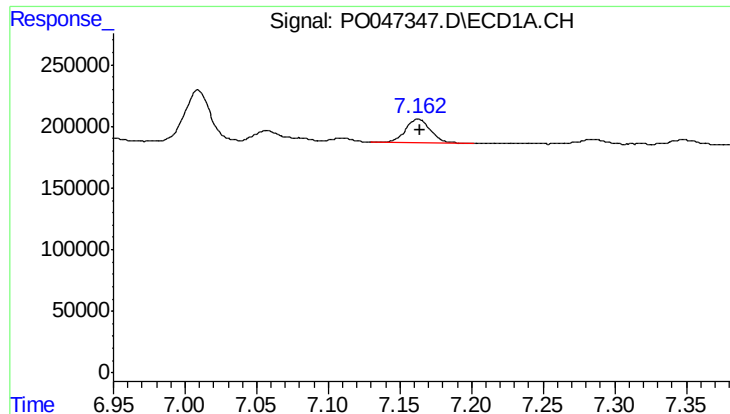

#31 AR-1260-1


R.T.: 7.163 min
Delta R.T.: -0.002 min
Response: 226963
Conc: 24.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2018

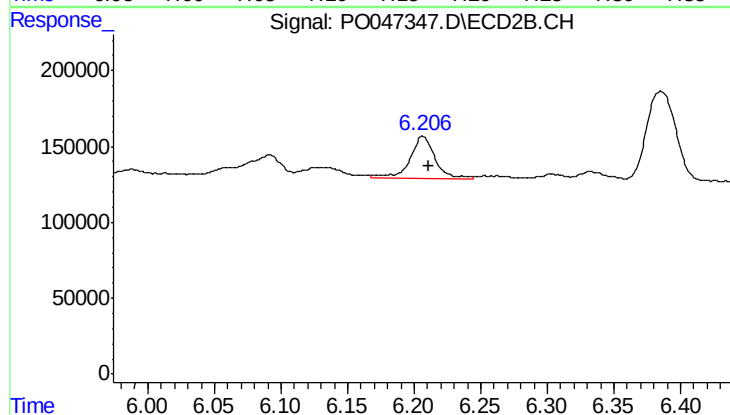


#31 AR-1260-1

R.T.: 6.207 min
Delta R.T.: -0.004 min
Response: 359272
Conc: 32.51 ng/ml

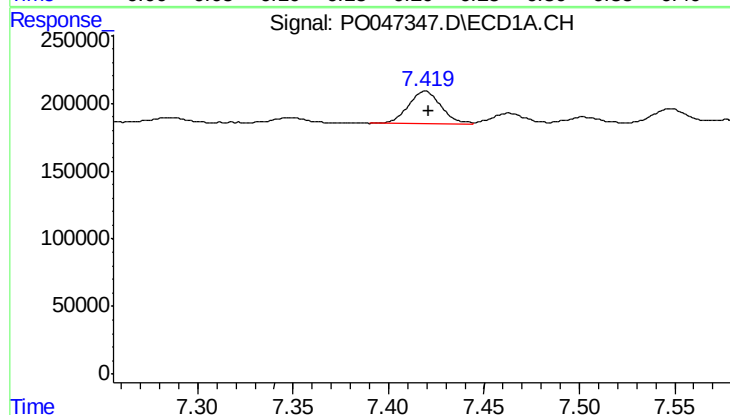


#32 AR-1260-2

R.T.: 7.419 min
Delta R.T.: -0.002 min
Response: 283347
Conc: 25.41 ng/ml

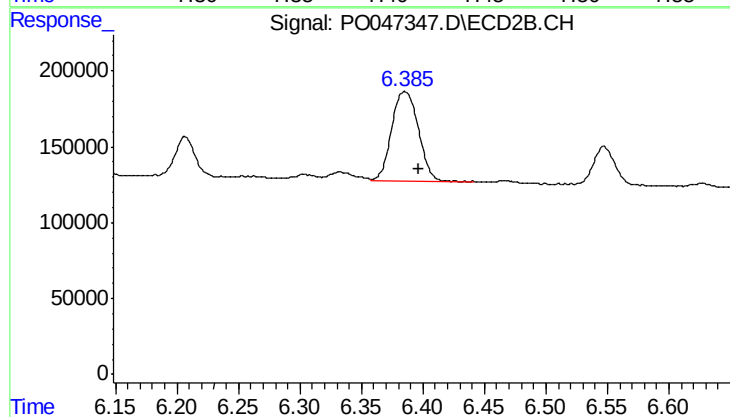

#32 AR-1260-2


R.T.: 6.385 min
Delta R.T.: -0.012 min
Response: 880967
Conc: 65.70 ng/ml

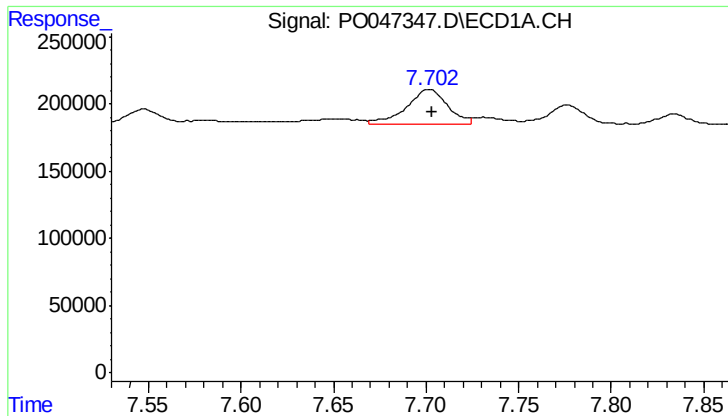

#33 AR-1260-3


R.T.: 7.702 min
Delta R.T.: -0.002 min
Response: 408173
Conc: 31.72 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2018

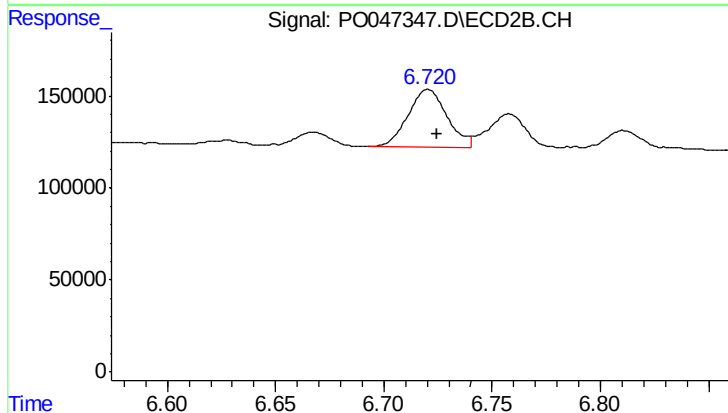


#33 AR-1260-3

R.T.: 6.720 min
Delta R.T.: -0.004 min
Response: 397180
Conc: 27.32 ng/ml

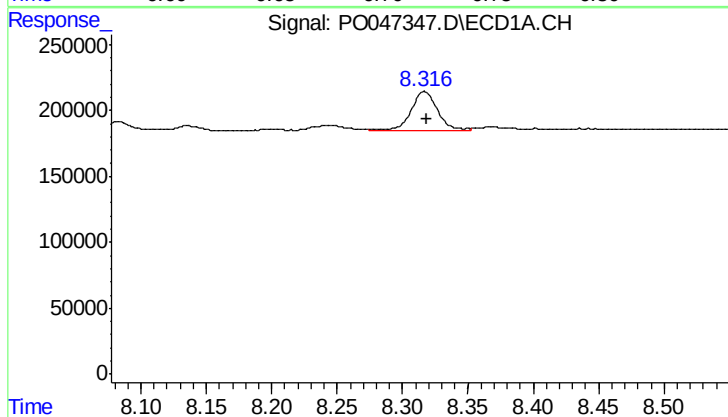


#34 AR-1260-4

R.T.: 8.317 min
Delta R.T.: -0.002 min
Response: 428766
Conc: 24.10 ng/ml

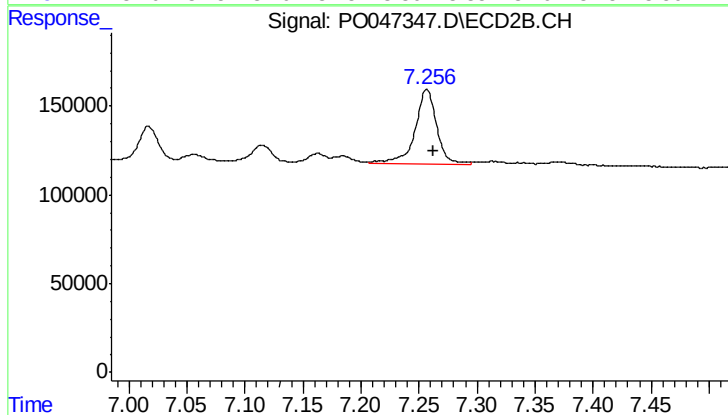

#34 AR-1260-4


R.T.: 7.257 min
Delta R.T.: -0.005 min
Response: 536356
Conc: 24.38 ng/ml

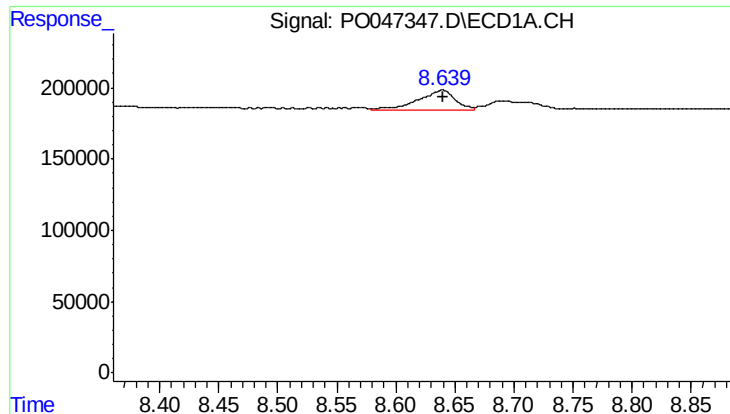

#35 AR-1260-5


R.T.: 8.639 min
Delta R.T.: 0.000 min
Response: 287179
Conc: 25.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2018

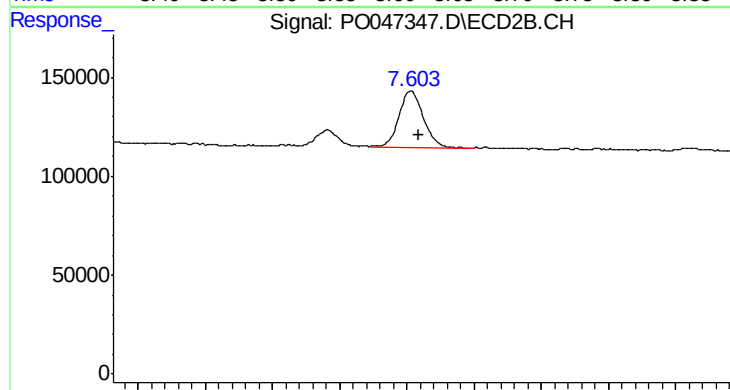


#35 AR-1260-5

R.T.: 7.603 min
Delta R.T.: -0.006 min
Response: 364195
Conc: 23.35 ng/ml

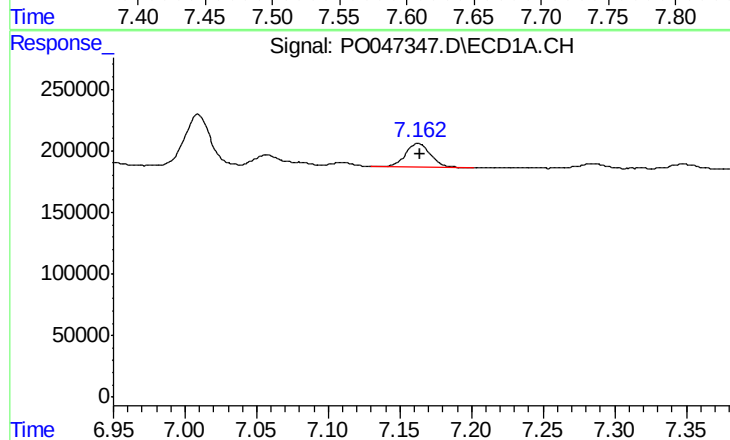


#36 AR-1262-1

R.T.: 7.163 min
Delta R.T.: 0.000 min
Response: 226963
Conc: 27.40 ng/ml

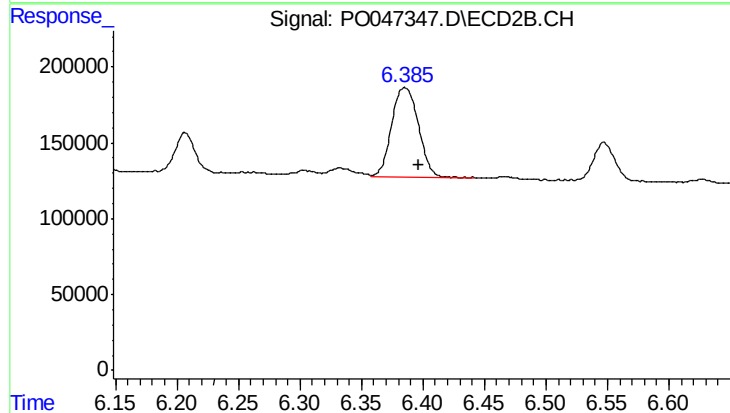

#36 AR-1262-1


R.T.: 6.385 min
Delta R.T.: -0.011 min
Response: 880967
Conc: 77.70 ng/ml

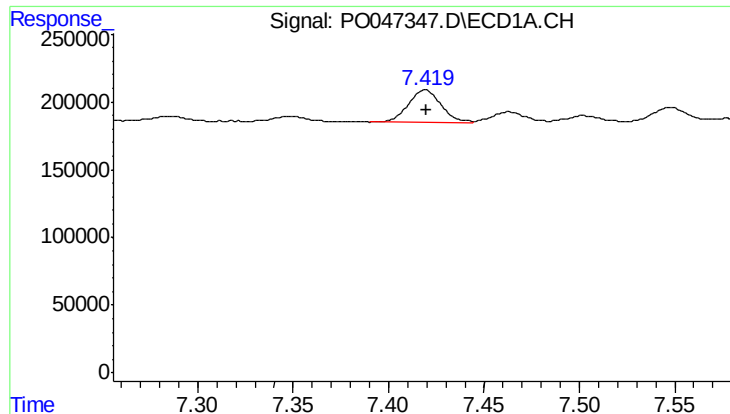

#37 AR-1262-2


R.T.: 7.419 min
Delta R.T.: 0.000 min
Response: 283347
Conc: 29.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2018

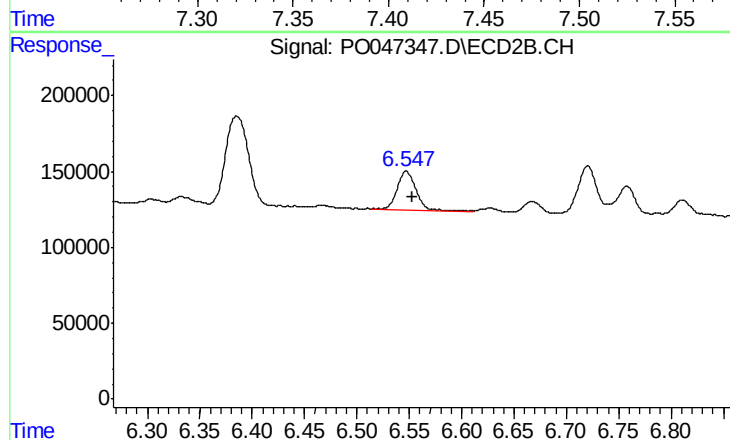


#37 AR-1262-2

R.T.: 6.547 min
Delta R.T.: -0.006 min
Response: 318681
Conc: 28.24 ng/ml

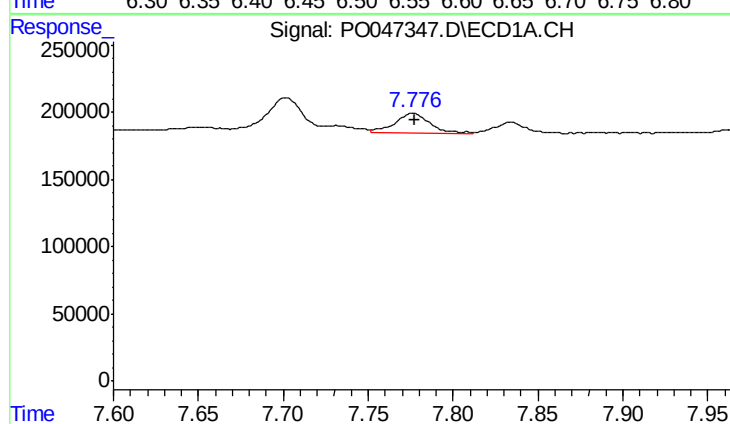


#38 AR-1262-3

R.T.: 7.776 min
Delta R.T.: -0.001 min
Response: 211108
Conc: 17.20 ng/ml

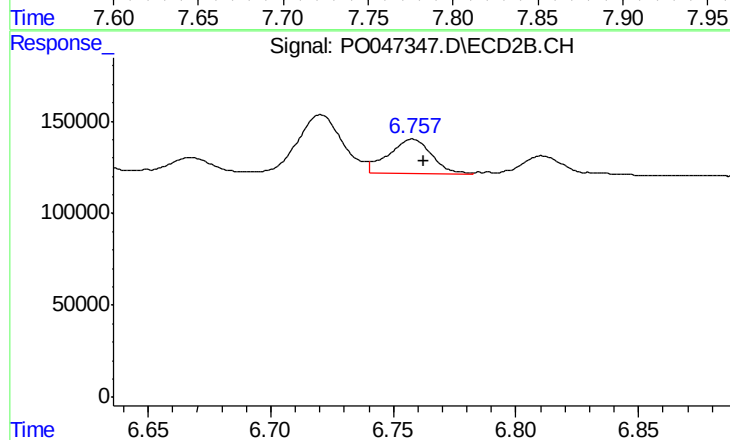

#38 AR-1262-3


R.T.: 6.758 min
Delta R.T.: -0.005 min
Response: 226420
Conc: 15.00 ng/ml

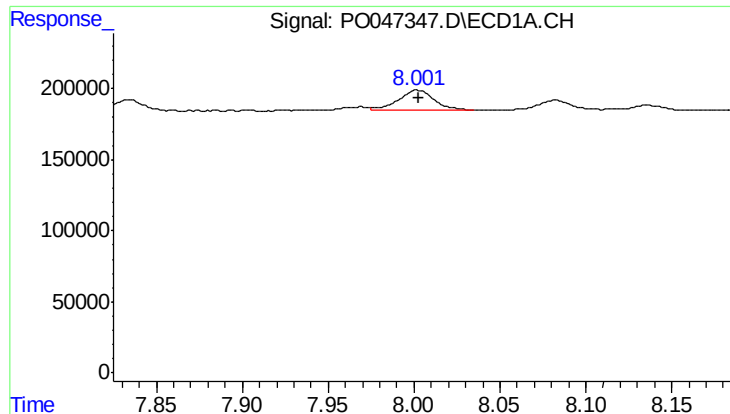

#39 AR-1262-4


R.T.: 8.002 min
Delta R.T.: -0.001 min
Response: 218145
Conc: 18.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2018

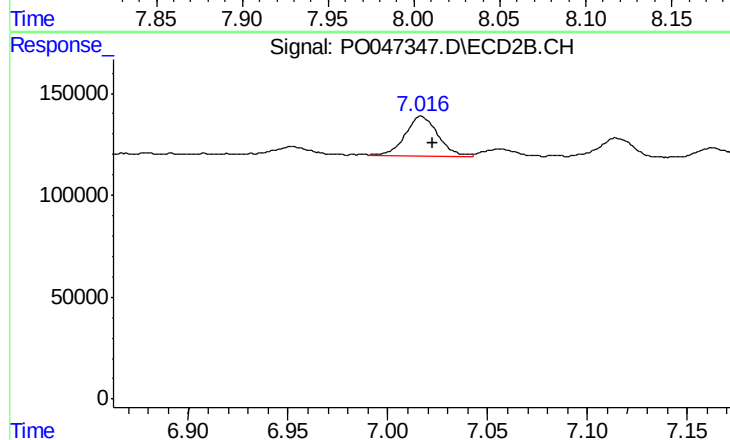


#39 AR-1262-4

R.T.: 7.017 min
Delta R.T.: -0.005 min
Response: 222734
Conc: 16.91 ng/ml

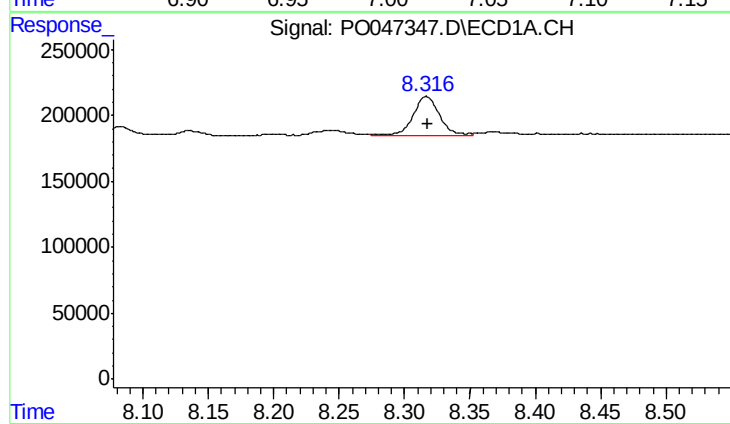


#40 AR-1262-5

R.T.: 8.317 min
Delta R.T.: -0.001 min
Response: 428766
Conc: 19.96 ng/ml

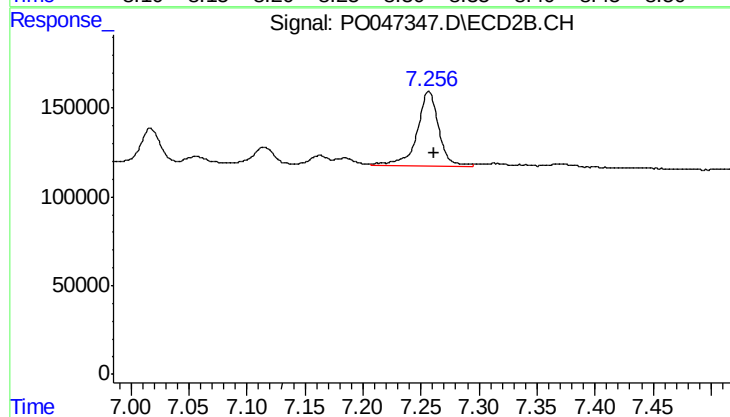

#40 AR-1262-5


R.T.: 7.257 min
Delta R.T.: -0.004 min
Response: 536356
Conc: 20.77 ng/ml

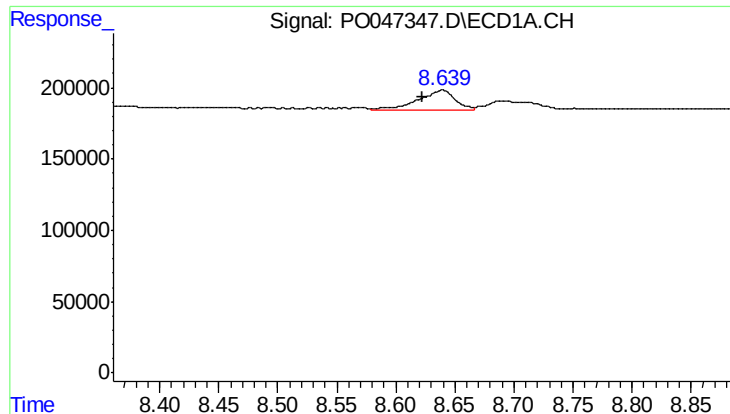

#41 AR-1268-1


R.T.: 8.639 min
Delta R.T.: 0.017 min
Response: 287179
Conc: 12.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2018

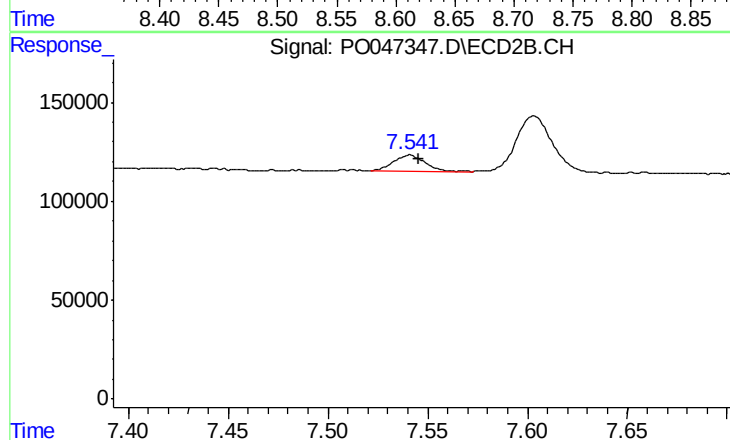


#41 AR-1268-1

R.T.: 7.541 min
Delta R.T.: -0.005 min
Response: 95027
Conc: 3.65 ng/ml

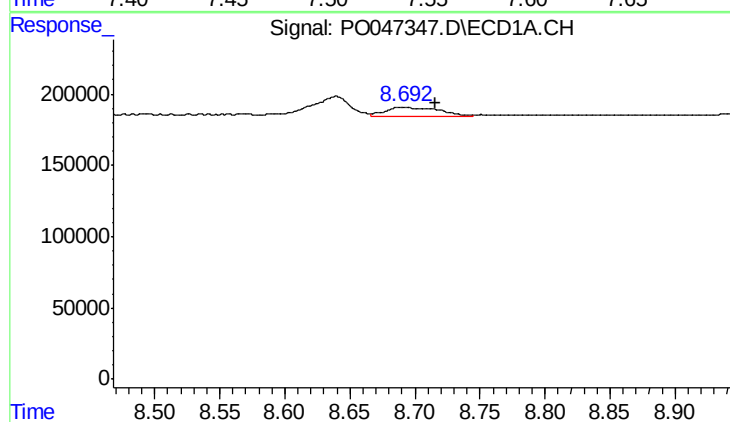


#42 AR-1268-2

R.T.: 8.692 min
Delta R.T.: -0.024 min
Response: 167351
Conc: 7.81 ng/ml

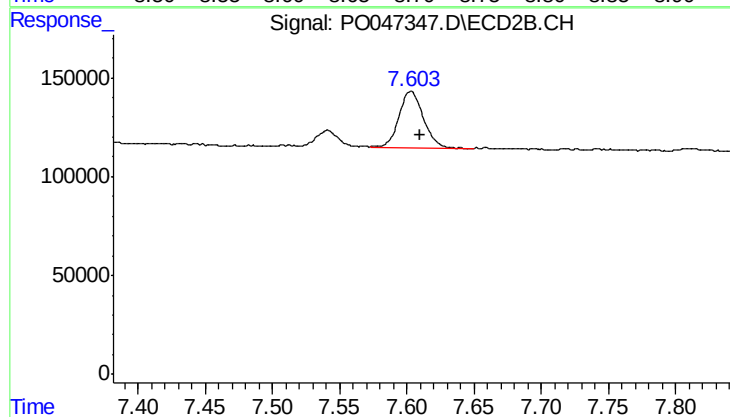

#42 AR-1268-2


R.T.: 7.603 min
Delta R.T.: -0.006 min
Response: 364195
Conc: 14.62 ng/ml

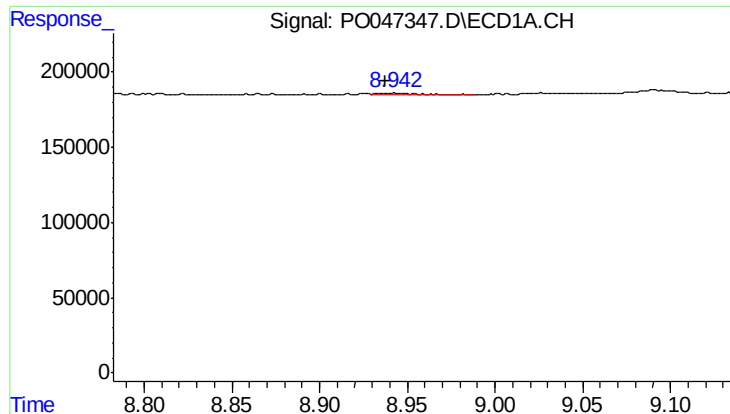

#43 AR-1268-3


R.T.: 8.943 min
Delta R.T.: 0.005 min
Response: 13066
Conc: 0.72 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2018

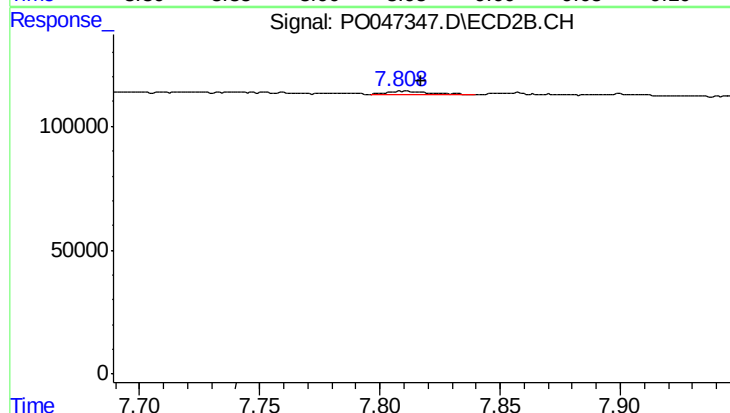


#43 AR-1268-3

R.T.: 7.810 min
Delta R.T.: -0.007 min
Response: 15557
Conc: 0.79 ng/ml

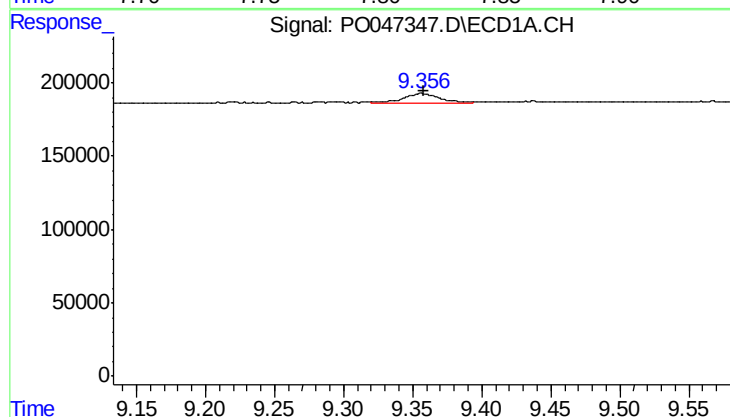


#44 AR-1268-4

R.T.: 9.357 min
Delta R.T.: 0.000 min
Response: 137564
Conc: 17.25 ng/ml

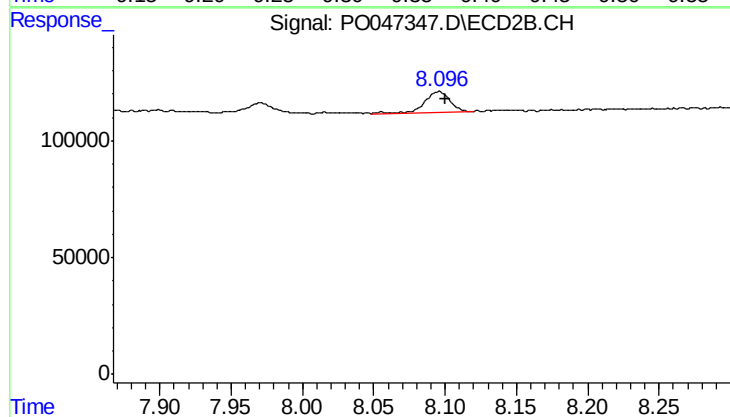

#44 AR-1268-4


R.T.: 8.096 min
Delta R.T.: -0.005 min
Response: 111647
Conc: 13.31 ng/ml

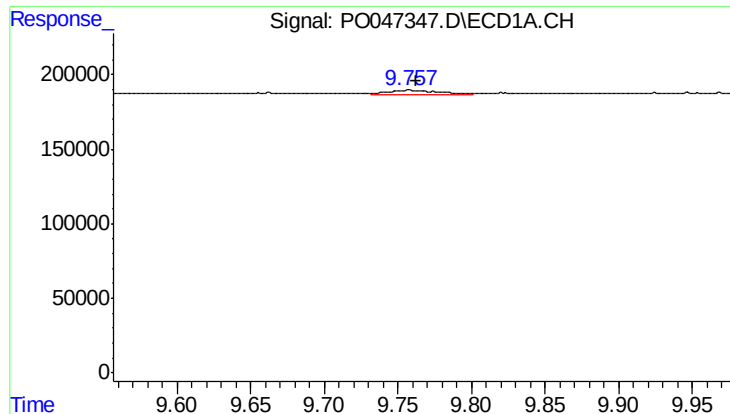

#45 AR-1268-5

R.T.: 9.757 min
Delta R.T.: -0.005 min
Response: 63681
Conc: 1.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2018

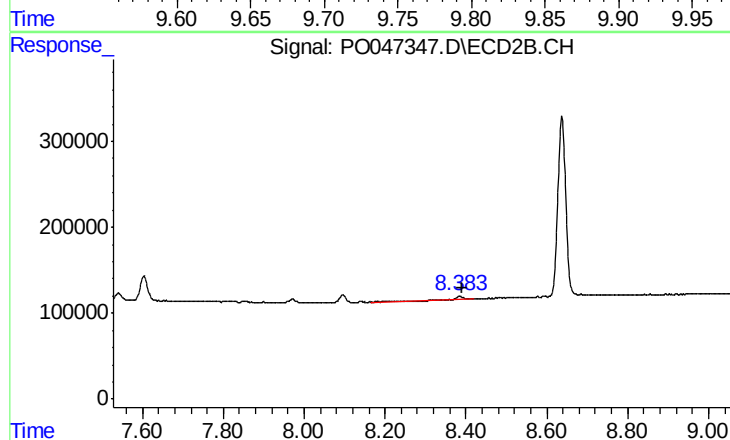

#45 AR-1268-5

R.T.: 8.384 min
Delta R.T.: -0.006 min
Response: 48996
Conc: 0.90 ng/ml