

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0073018\
 Data File : P0047349.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Jul 2018 11:06
 Operator : SM/SJ
 Sample : J3762-09
 Misc : AR1660 MDL WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 MDL-WATER-03-QT3-2018

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 31 03:49:51 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jul 27 02:33:29 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.397	3.645	3651831	3917949	18.088	15.945
2) SA Decachlor...	10.086	8.637	2842145	2903752	17.426	18.473
Target Compounds						
3) L1 AR-1016-1	5.298	4.508	153056	187546	32.044	32.805
4) L1 AR-1016-2	5.649	4.923	189633	131463	32.212	25.038
5) L1 AR-1016-3	5.747	4.964	146243	122736	29.489	27.953
6) L1 AR-1016-4	6.041	5.005	159509	136786	34.293	26.379
7) L1 AR-1016-5	6.181	5.177	145227	176648	27.859	30.116
8) L2 AR-1221-1	4.596	3.856	25835	28758	11.682	12.187
9) L2 AR-1221-2	4.702	3.945	71969	90778	44.012	50.041
10) L2 AR-1221-3	4.768	4.020	100465	120076	19.459	20.772
11) L3 AR-1232-1	5.104	4.317	145442	251679	67.631	107.019 #
12) L3 AR-1232-2	5.564	4.747	211447	531678	71.861	173.985 #
13) L3 AR-1232-3	5.587	4.747	296970	531678	69.123	115.137 #
14) L3 AR-1232-4	5.649	4.802	189633	165049	68.512	53.390
15) L3 AR-1232-5	5.747	4.964	146243	122736	65.488	68.578
16) L4 AR-1242-1	5.587	4.747	296970	531678	40.404	66.391 #
17) L4 AR-1242-2	5.649	4.923	189633	131463	40.972	31.911
18) L4 AR-1242-3	5.747	5.005	146243	136786	38.064	32.616
19) L4 AR-1242-4	6.041	5.177	159509	176648	41.493	37.408
20) L4 AR-1242-5	6.181	5.325	145227	173676	33.927	44.858 #
21) L5 AR-1248-1	6.041	5.177	159509	176648	25.509	23.679
22) L5 AR-1248-2	6.181	5.325	145227	173676	26.659	32.463
23) L5 AR-1248-3	6.444	5.528	59001	173365	8.384	17.423 #
24) L5 AR-1248-4	6.482	5.567	36503	49241	5.437	7.026 #
25) L5 AR-1248-5	6.632	6.091	123209	289929	17.408	60.836 #
26) L6 AR-1254-1	6.632	5.528	123209	173365	10.075	14.089 #
27) L6 AR-1254-2	6.913	5.673	39900	128935	5.350	12.386 #
28) L6 AR-1254-3	7.007	6.091	340454	289929	26.106	16.705 #
29) L6 AR-1254-4	7.283	6.304	57407	41526	5.890	3.832 #
30) L6 AR-1254-5	7.546	6.625	127855	35220	17.306	4.605 #
31) L7 AR-1260-1	7.162	6.206	228955	330792	24.417	29.936
32) L7 AR-1260-2	7.418	6.388	295560	703544	26.505	52.472 #
33) L7 AR-1260-3	7.701	6.720	337203	411860	26.209	28.330
34) L7 AR-1260-4	8.315	7.257	368542	573541	20.719	26.066 #
35) L7 AR-1260-5	8.637	7.603	301619	404370	26.413	25.922
36) L8 AR-1262-1	7.162	6.388	228955	703544	27.637	62.052 #
37) L8 AR-1262-2	7.418	6.546	295560	347287	30.496	30.775
38) L8 AR-1262-3	7.775	6.758	194376	231465	15.839	15.337

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0073018\
 Data File : P0047349.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Jul 2018 11:06
 Operator : SM/SJ
 Sample : J3762-09
 Misc : AR1660 MDL WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT3-2018

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 31 03:49:51 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jul 27 02:33:29 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
39)	L8 AR-1262-4	8.000	7.017	205525	235200	17.453	17.861
40)	L8 AR-1262-5	8.315	7.257	368542	573541	17.153	22.206 #
41)	L9 AR-1268-1	8.637	7.540	301619	110480	12.996	4.249 #
42)	L9 AR-1268-2	8.690	7.603	179119	404370	8.360	16.231 #
43)	L9 AR-1268-3	8.941	7.812	7029	15628	0.389	0.792 #
44)	L9 AR-1268-4	9.353	8.095	106850	109461	13.400	13.049
45)	L9 AR-1268-5	9.756	8.385	56761	24187	1.042	0.443 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0073018\
Data File : P0047349.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Jul 2018 11:06
Operator : SM/SJ
Sample : J3762-09
Misc : AR1660 MDL WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2018

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 31 03:49:51 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072718.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 27 02:33:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

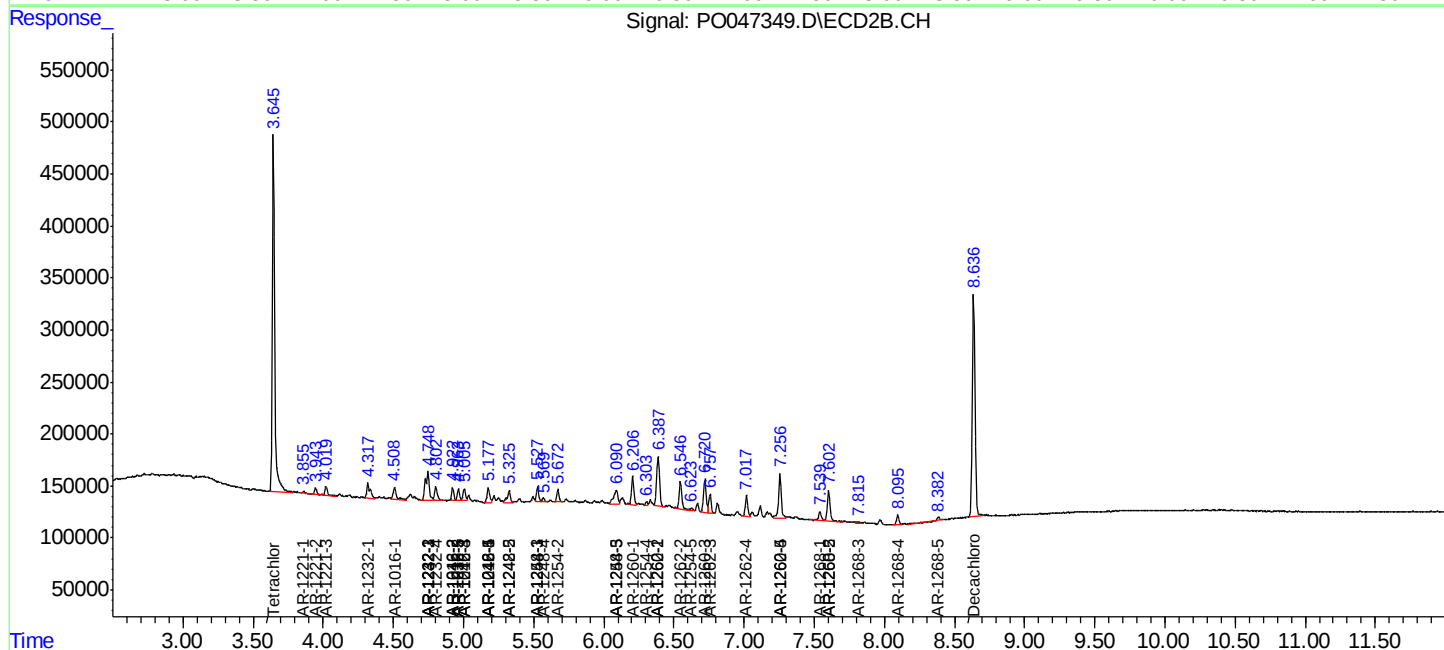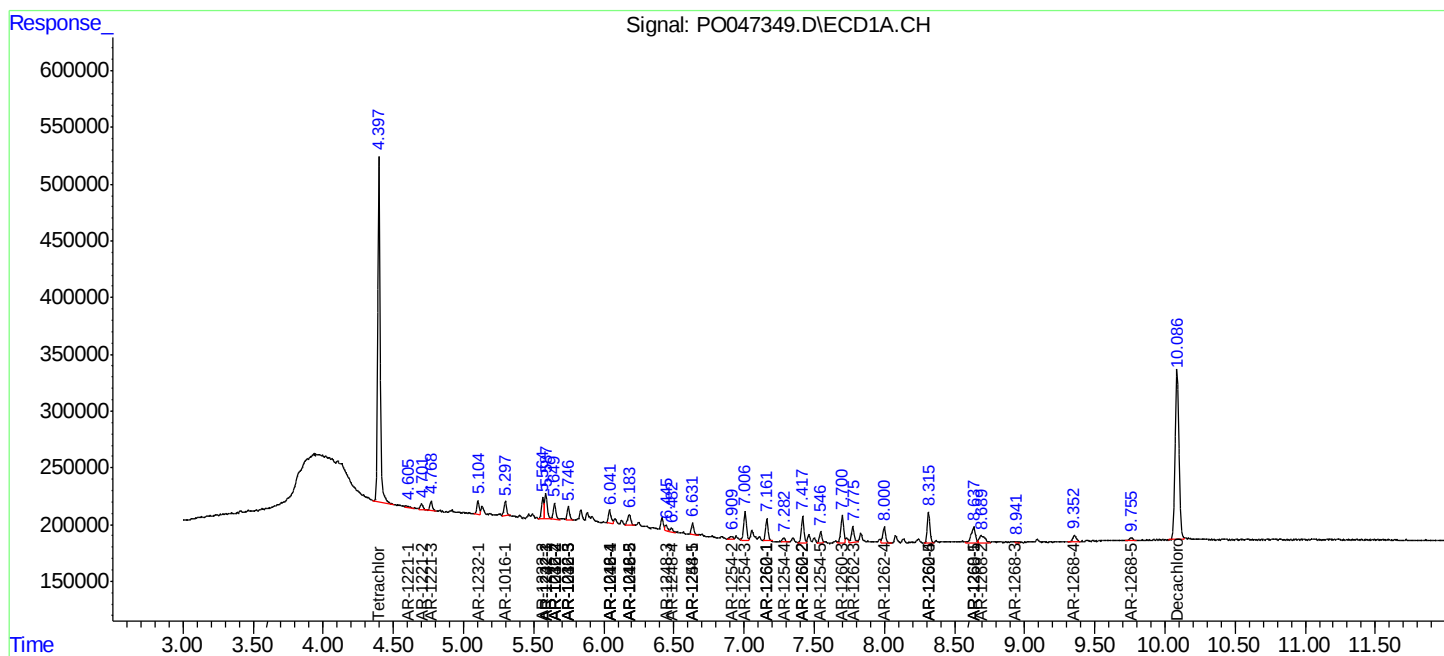


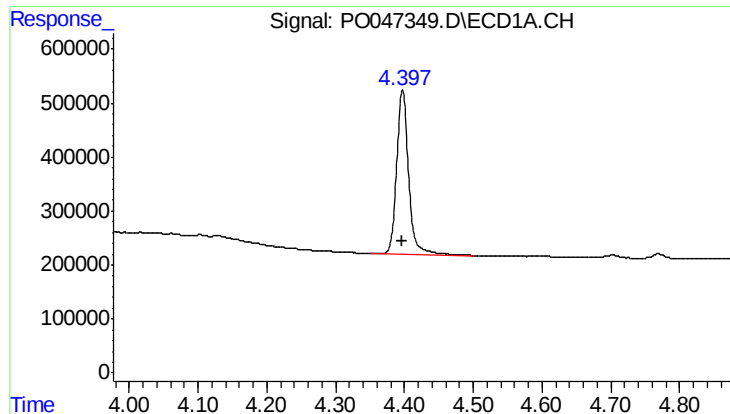

#1 Tetrachloro-m-xylene


R.T.: 4.397 min
Delta R.T.: 0.000 min
Response: 3651831
Conc: 18.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2018

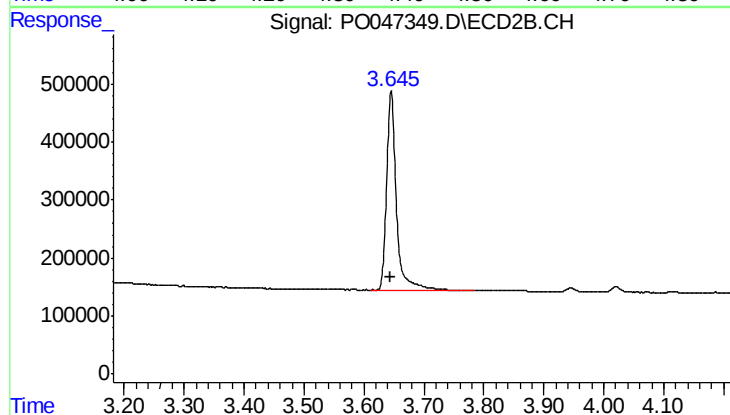


#1 Tetrachloro-m-xylene

R.T.: 3.645 min
Delta R.T.: 0.000 min
Response: 3917949
Conc: 15.95 ng/ml

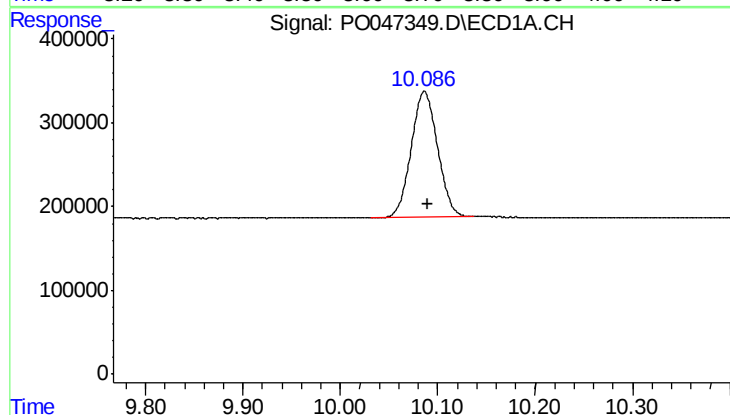


#2 Decachlorobiphenyl

R.T.: 10.086 min
Delta R.T.: -0.004 min
Response: 2842145
Conc: 17.43 ng/ml

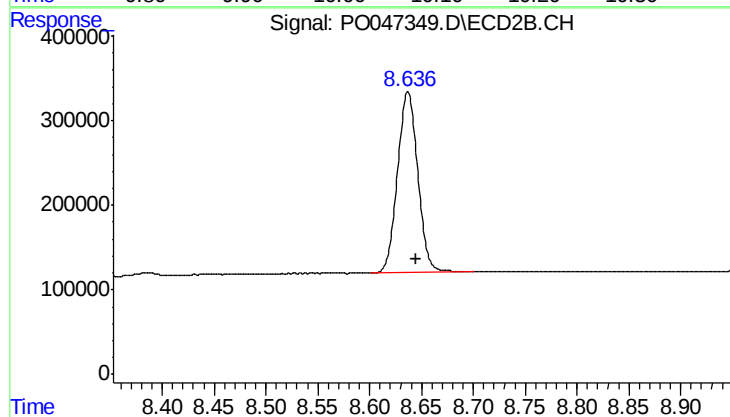

#2 Decachlorobiphenyl


R.T.: 8.637 min
Delta R.T.: -0.008 min
Response: 2903752
Conc: 18.47 ng/ml

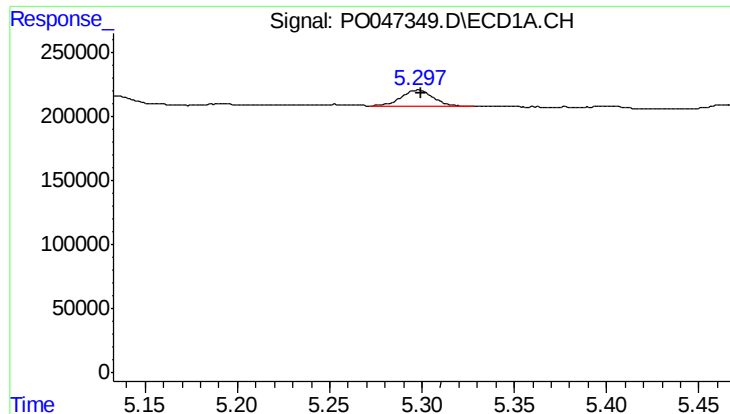

#3 AR-1016-1


R.T.: 5.298 min
Delta R.T.: -0.002 min
Response: 153056
Conc: 32.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2018

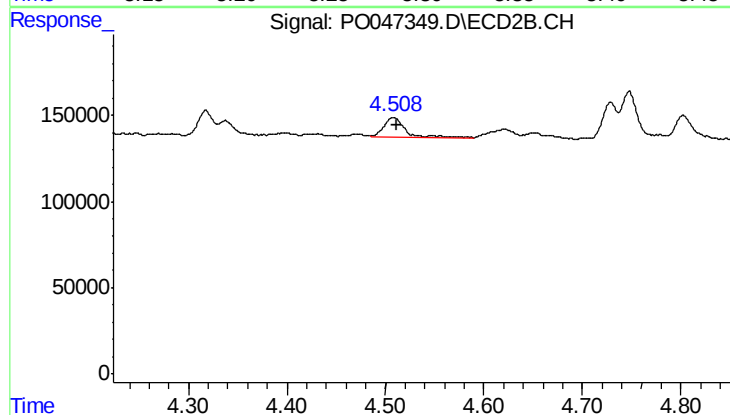


#3 AR-1016-1

R.T.: 4.508 min
Delta R.T.: -0.003 min
Response: 187546
Conc: 32.80 ng/ml

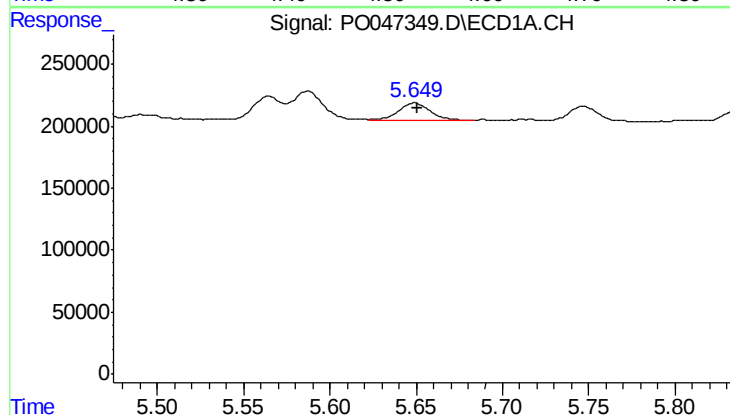


#4 AR-1016-2

R.T.: 5.649 min
Delta R.T.: -0.001 min
Response: 189633
Conc: 32.21 ng/ml

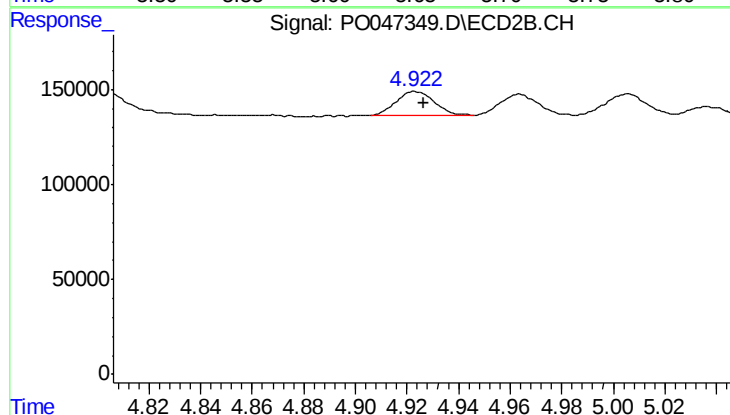

#4 AR-1016-2


R.T.: 4.923 min
Delta R.T.: -0.003 min
Response: 131463
Conc: 25.04 ng/ml

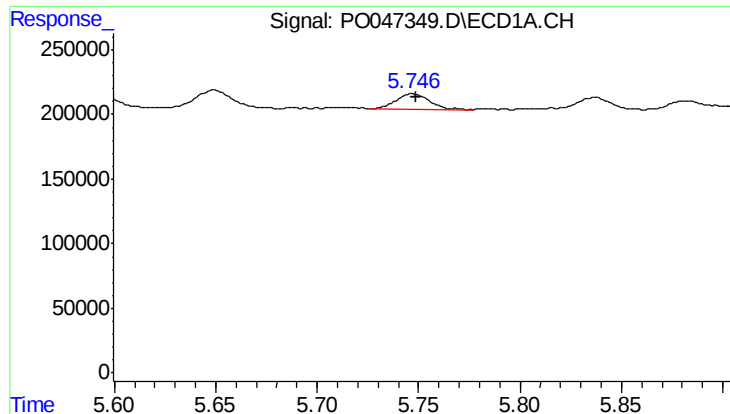

#5 AR-1016-3


R.T.: 5.747 min
Delta R.T.: -0.002 min
Response: 146243
Conc: 29.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2018

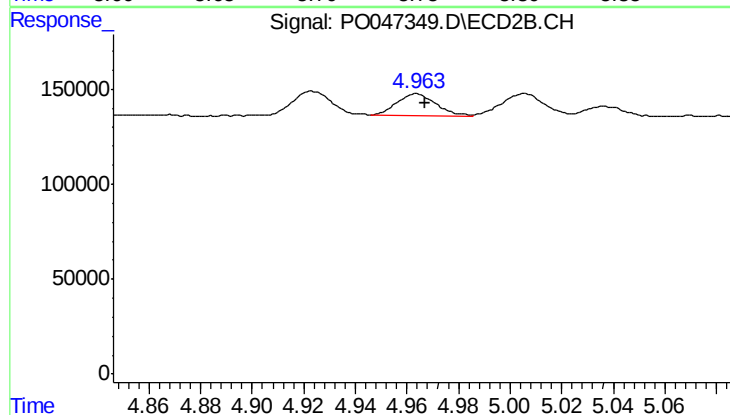


#5 AR-1016-3

R.T.: 4.964 min
Delta R.T.: -0.003 min
Response: 122736
Conc: 27.95 ng/ml

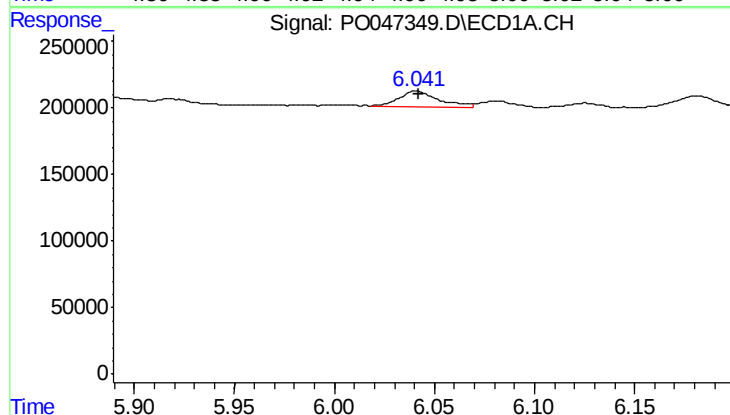


#6 AR-1016-4

R.T.: 6.041 min
Delta R.T.: -0.001 min
Response: 159509
Conc: 34.29 ng/ml

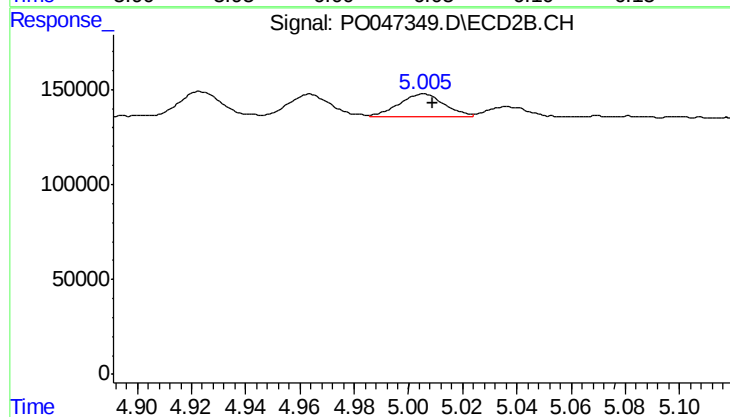

#6 AR-1016-4


R.T.: 5.005 min
Delta R.T.: -0.004 min
Response: 136786
Conc: 26.38 ng/ml

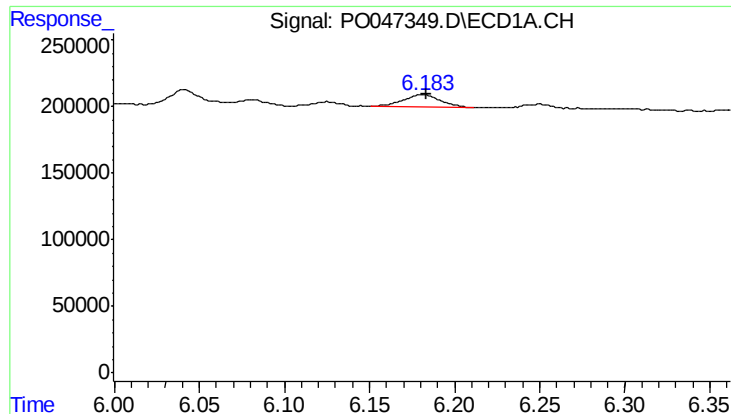

#7 AR-1016-5


R.T.: 6.181 min
Delta R.T.: -0.002 min
Response: 145227
Conc: 27.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2018

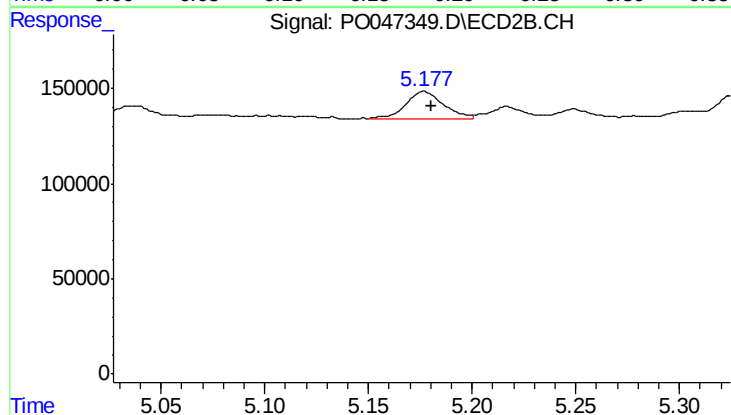


#7 AR-1016-5

R.T.: 5.177 min
Delta R.T.: -0.003 min
Response: 176648
Conc: 30.12 ng/ml

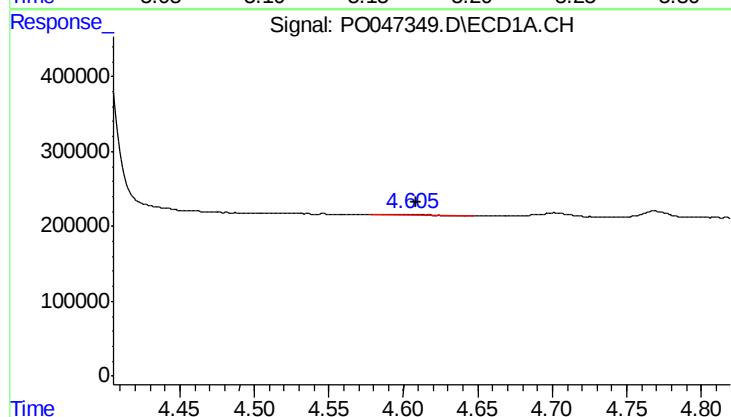


#8 AR-1221-1

R.T.: 4.596 min
Delta R.T.: -0.013 min
Response: 25835
Conc: 11.68 ng/ml

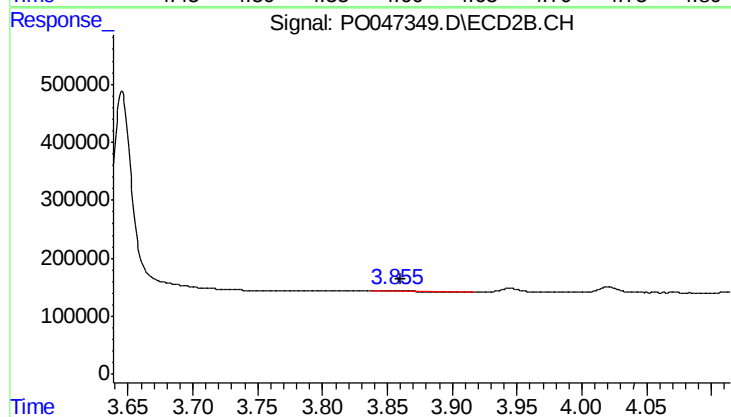

#8 AR-1221-1


R.T.: 3.856 min
Delta R.T.: -0.005 min
Response: 28758
Conc: 12.19 ng/ml

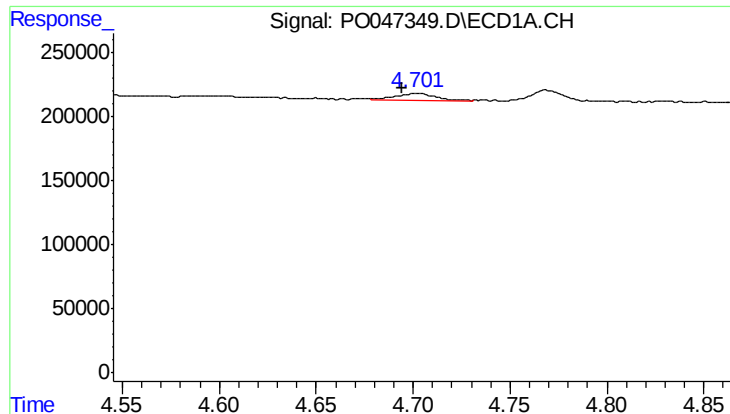

#9 AR-1221-2


R.T.: 4.702 min
Delta R.T.: 0.008 min
Response: 71969
Conc: 44.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2018

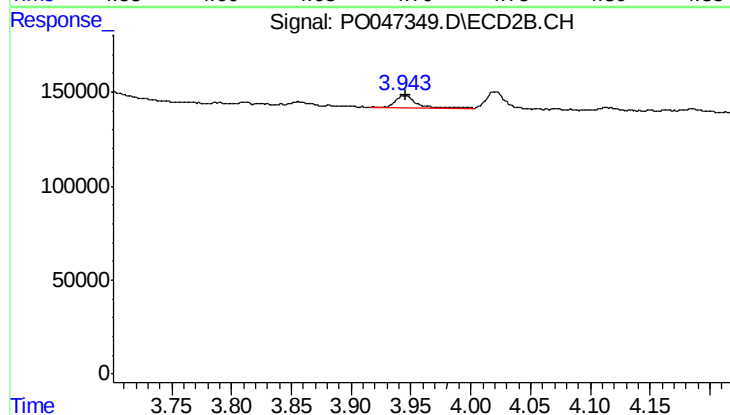


#9 AR-1221-2

R.T.: 3.945 min
Delta R.T.: -0.001 min
Response: 90778
Conc: 50.04 ng/ml

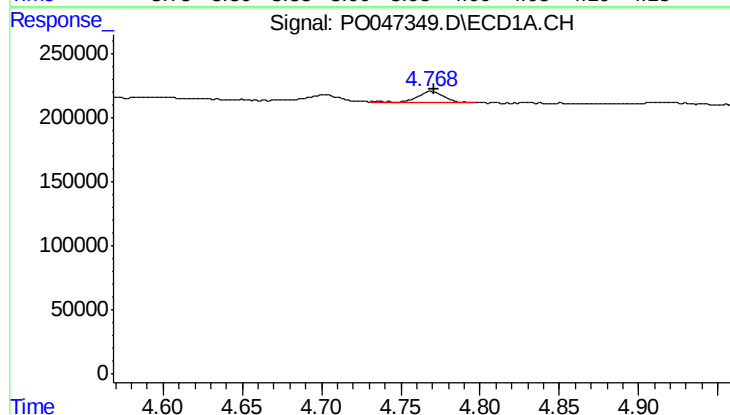


#10 AR-1221-3

R.T.: 4.768 min
Delta R.T.: -0.003 min
Response: 100465
Conc: 19.46 ng/ml

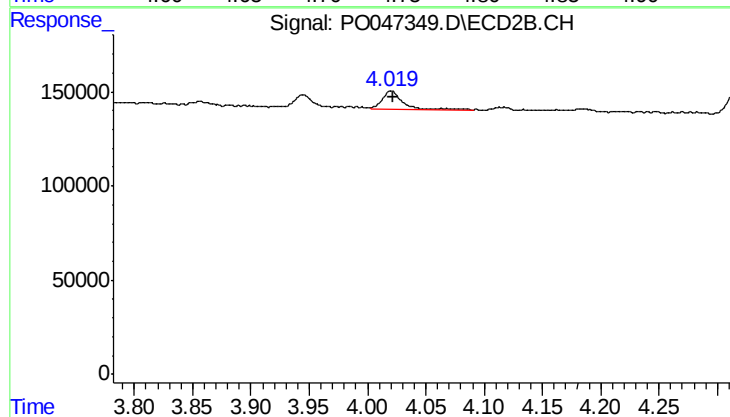

#10 AR-1221-3


R.T.: 4.020 min
Delta R.T.: -0.002 min
Response: 120076
Conc: 20.77 ng/ml

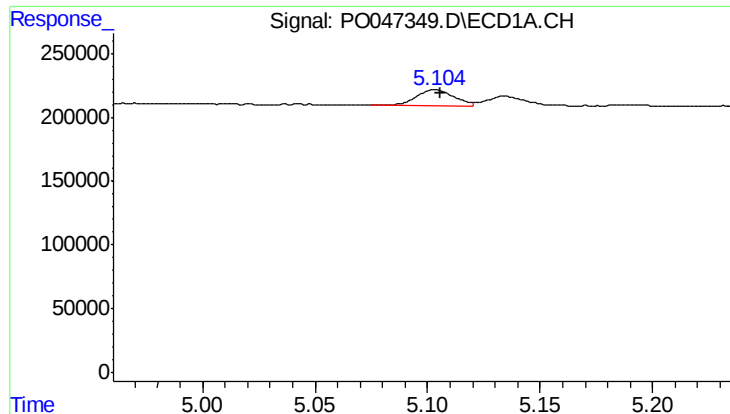

#11 AR-1232-1


R.T.: 5.104 min
Delta R.T.: -0.002 min
Response: 145442
Conc: 67.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2018

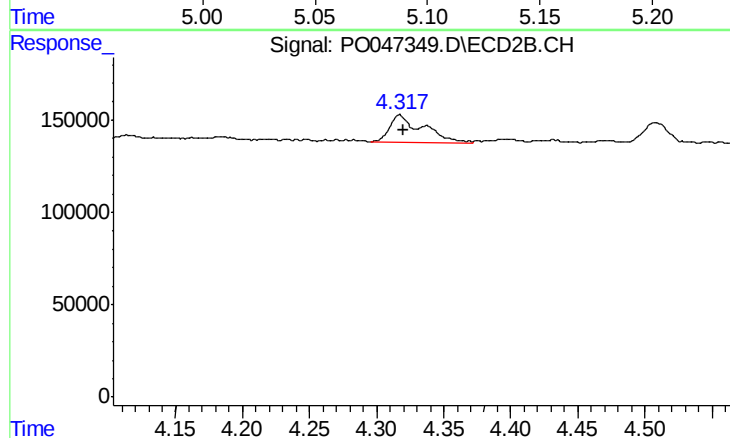


#11 AR-1232-1

R.T.: 4.317 min
Delta R.T.: -0.003 min
Response: 251679
Conc: 107.02 ng/ml

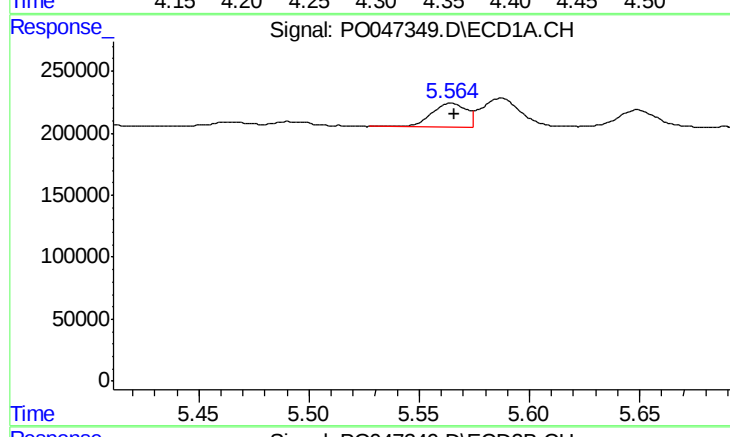


#12 AR-1232-2

R.T.: 5.564 min
Delta R.T.: -0.001 min
Response: 211447
Conc: 71.86 ng/ml

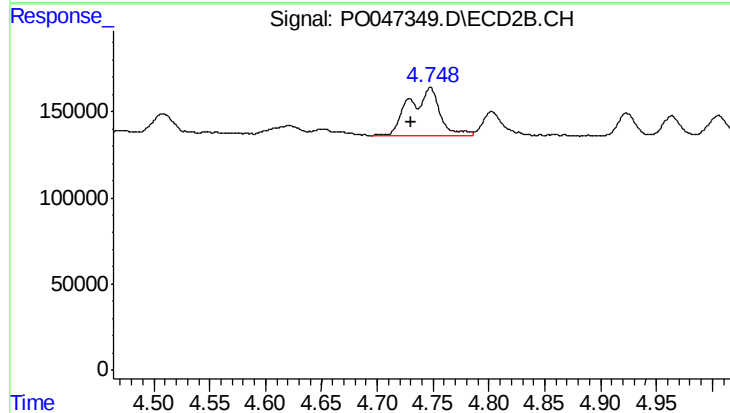

#12 AR-1232-2


R.T.: 4.747 min
Delta R.T.: 0.017 min
Response: 531678
Conc: 173.98 ng/ml

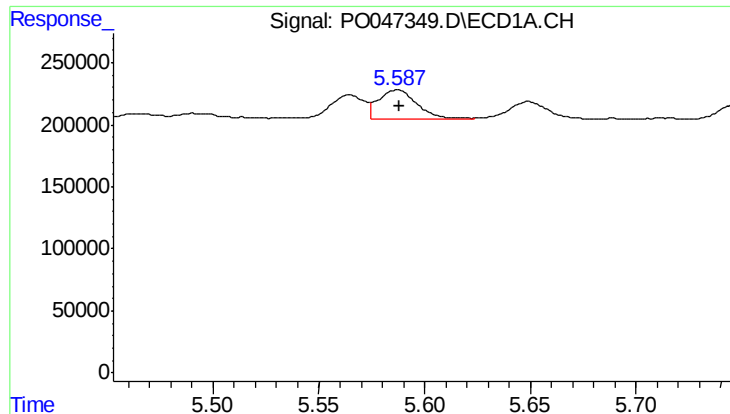

#13 AR-1232-3


R.T.: 5.587 min
Delta R.T.: -0.001 min
Response: 296970
Conc: 69.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2018

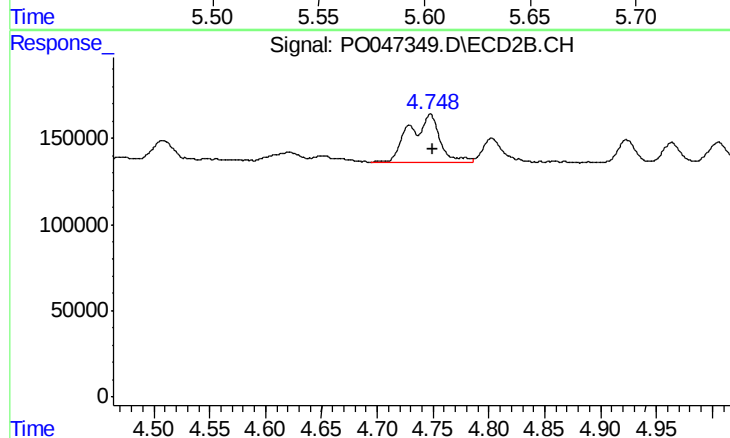


#13 AR-1232-3

R.T.: 4.747 min
Delta R.T.: -0.002 min
Response: 531678
Conc: 115.14 ng/ml

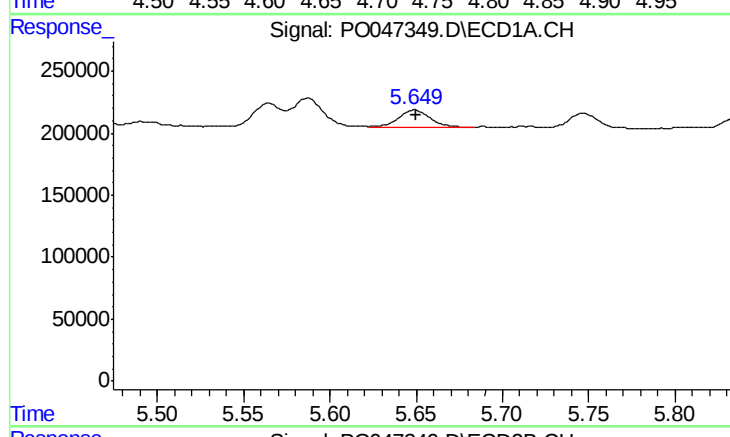


#14 AR-1232-4

R.T.: 5.649 min
Delta R.T.: 0.000 min
Response: 189633
Conc: 68.51 ng/ml

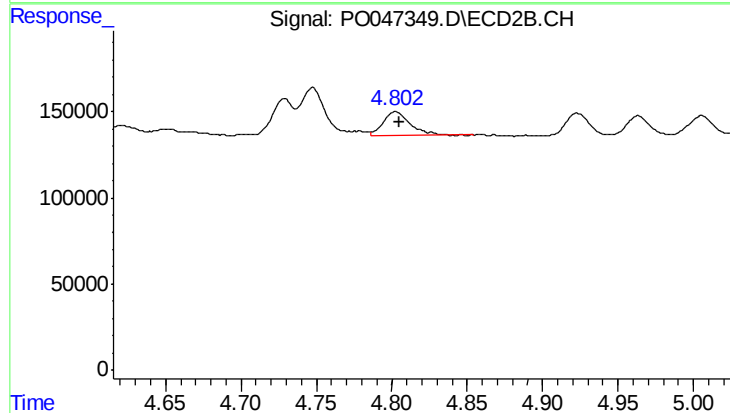

#14 AR-1232-4


R.T.: 4.802 min
Delta R.T.: -0.003 min
Response: 165049
Conc: 53.39 ng/ml

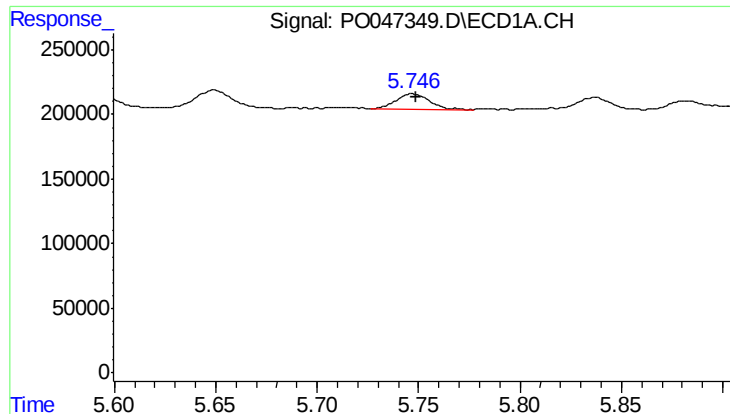

#15 AR-1232-5


R.T.: 5.747 min
Delta R.T.: -0.002 min
Response: 146243
Conc: 65.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2018

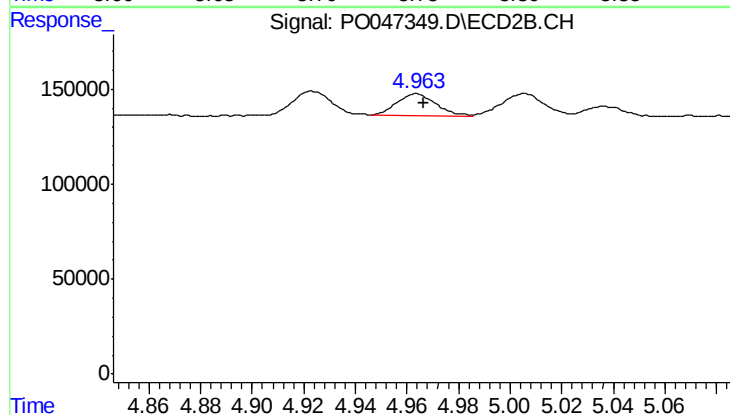


#15 AR-1232-5

R.T.: 4.964 min
Delta R.T.: -0.003 min
Response: 122736
Conc: 68.58 ng/ml

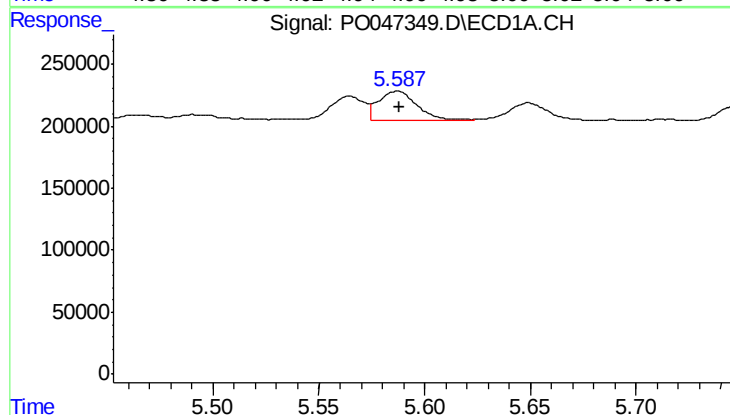


#16 AR-1242-1

R.T.: 5.587 min
Delta R.T.: 0.000 min
Response: 296970
Conc: 40.40 ng/ml

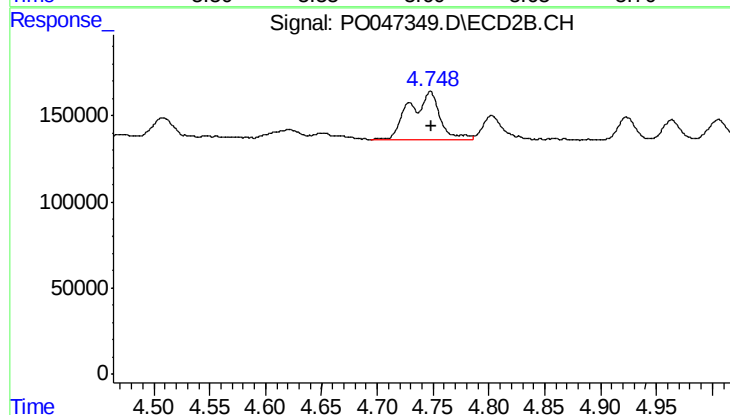

#16 AR-1242-1


R.T.: 4.747 min
Delta R.T.: -0.001 min
Response: 531678
Conc: 66.39 ng/ml

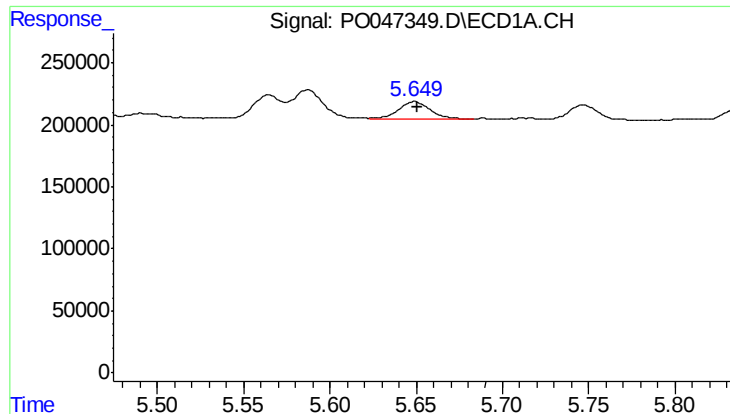

#17 AR-1242-2


R.T.: 5.649 min
Delta R.T.: -0.001 min
Response: 189633
Conc: 40.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2018

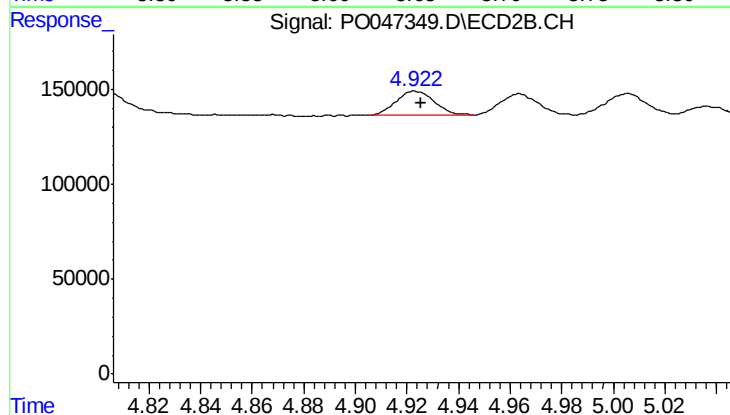


#17 AR-1242-2

R.T.: 4.923 min
Delta R.T.: -0.002 min
Response: 131463
Conc: 31.91 ng/ml

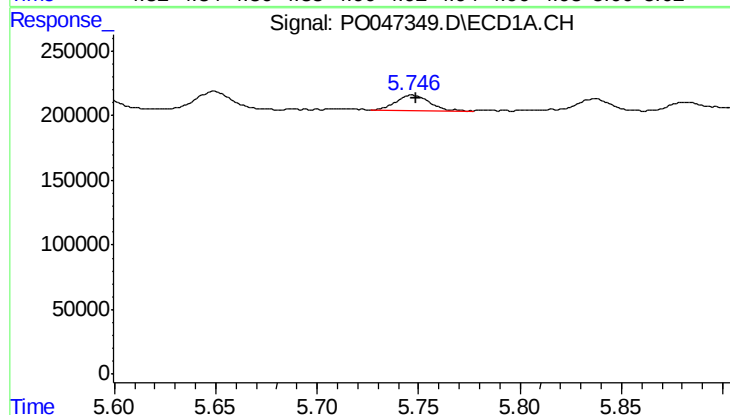


#18 AR-1242-3

R.T.: 5.747 min
Delta R.T.: -0.002 min
Response: 146243
Conc: 38.06 ng/ml

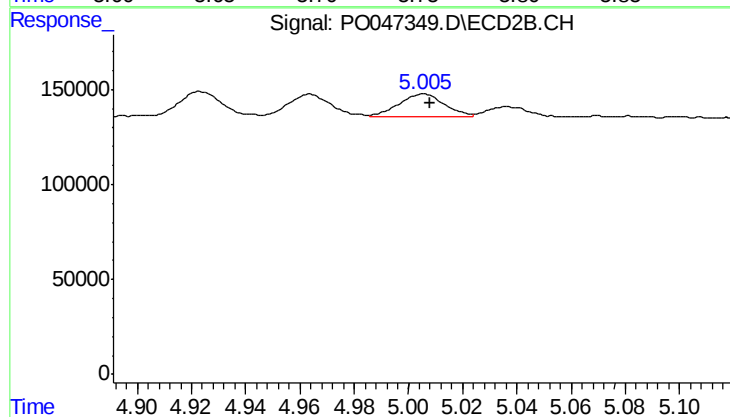

#18 AR-1242-3


R.T.: 5.005 min
Delta R.T.: -0.003 min
Response: 136786
Conc: 32.62 ng/ml

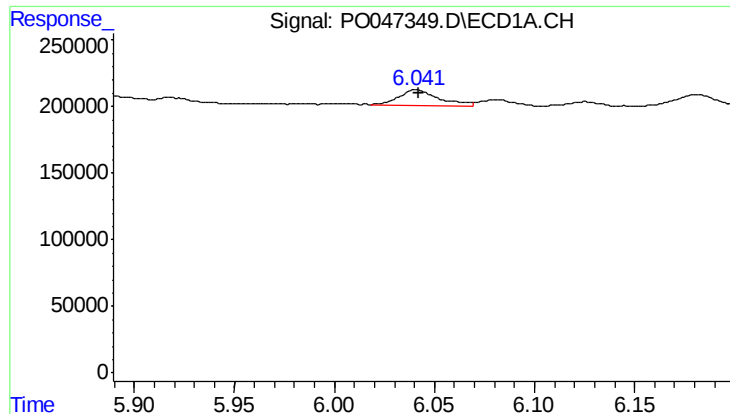

#19 AR-1242-4


R.T.: 6.041 min
Delta R.T.: -0.001 min
Response: 159509
Conc: 41.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2018

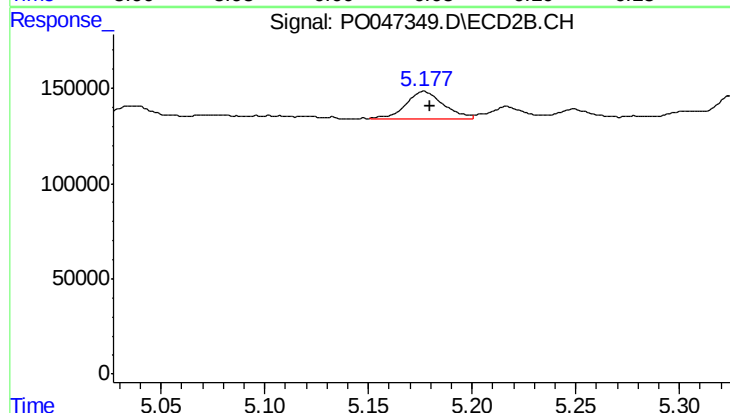


#19 AR-1242-4

R.T.: 5.177 min
Delta R.T.: -0.003 min
Response: 176648
Conc: 37.41 ng/ml

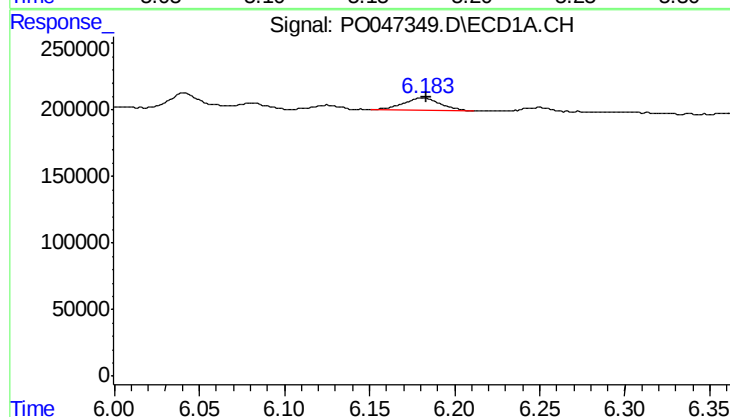


#20 AR-1242-5

R.T.: 6.181 min
Delta R.T.: -0.002 min
Response: 145227
Conc: 33.93 ng/ml

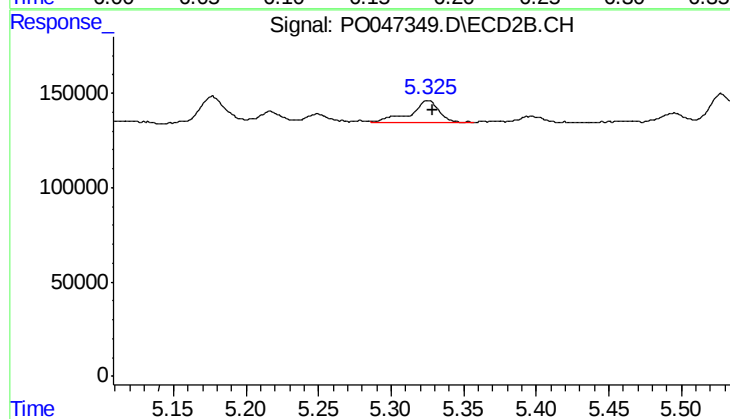

#20 AR-1242-5


R.T.: 5.325 min
Delta R.T.: -0.003 min
Response: 173676
Conc: 44.86 ng/ml

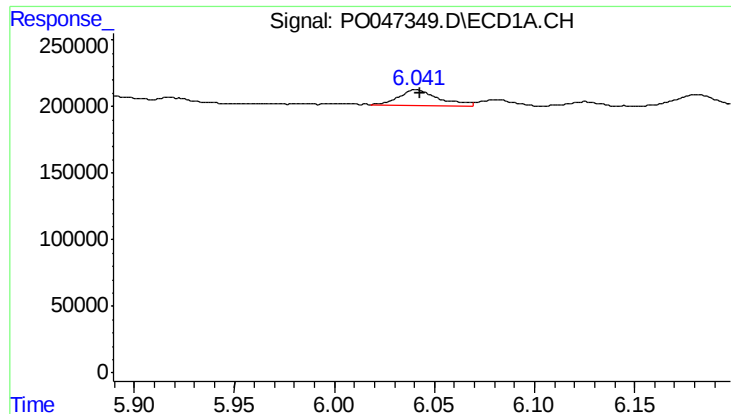

#21 AR-1248-1


R.T.: 6.041 min
Delta R.T.: -0.002 min
Response: 159509
Conc: 25.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2018

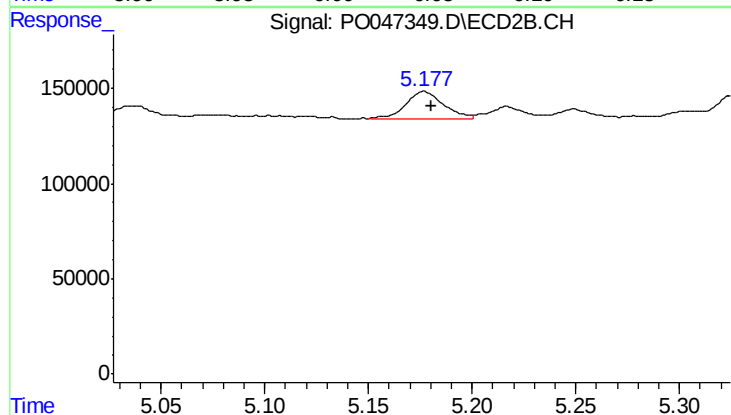


#21 AR-1248-1

R.T.: 5.177 min
Delta R.T.: -0.003 min
Response: 176648
Conc: 23.68 ng/ml

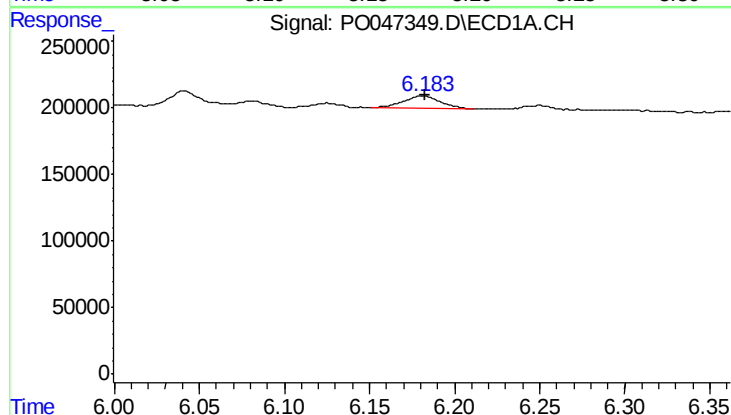


#22 AR-1248-2

R.T.: 6.181 min
Delta R.T.: 0.000 min
Response: 145227
Conc: 26.66 ng/ml

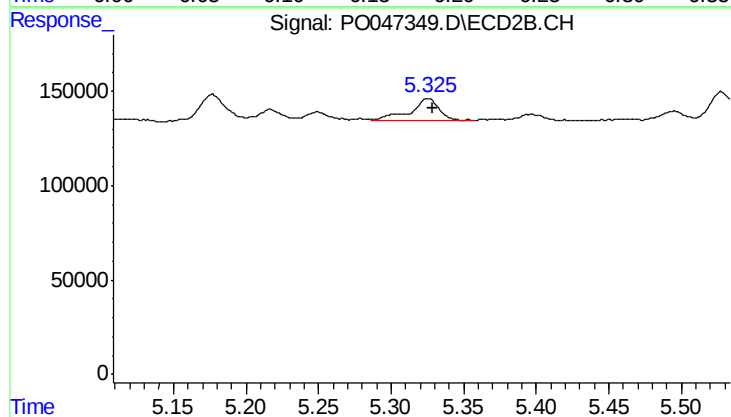

#22 AR-1248-2


R.T.: 5.325 min
Delta R.T.: -0.003 min
Response: 173676
Conc: 32.46 ng/ml

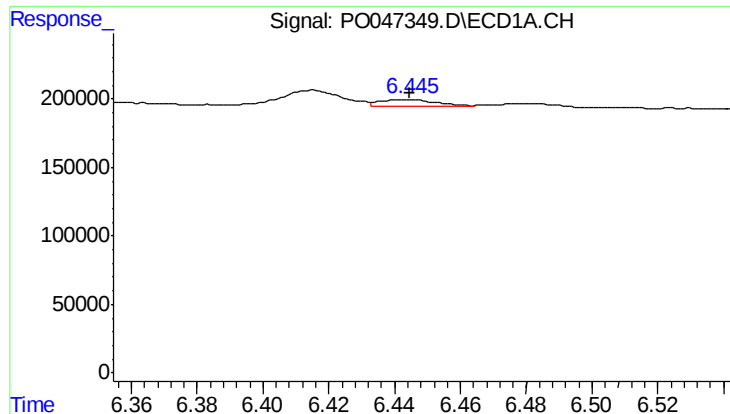

#23 AR-1248-3


R.T.: 6.444 min
Delta R.T.: 0.000 min
Response: 59001
Conc: 8.38 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2018

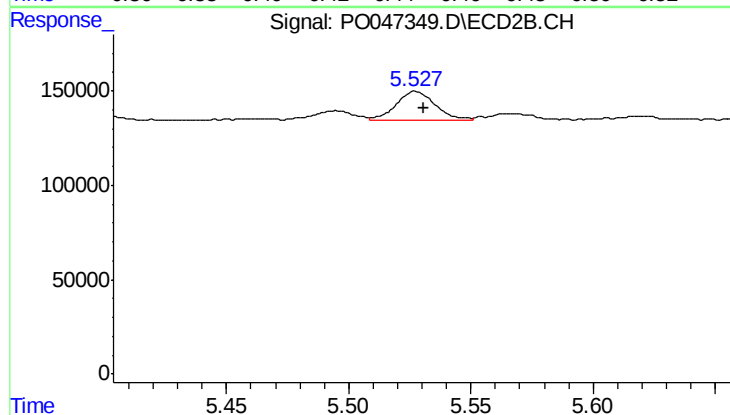


#23 AR-1248-3

R.T.: 5.528 min
Delta R.T.: -0.003 min
Response: 173365
Conc: 17.42 ng/ml

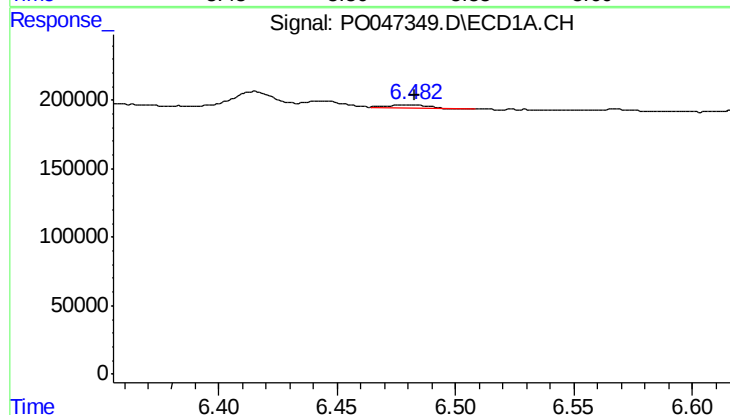


#24 AR-1248-4

R.T.: 6.482 min
Delta R.T.: 0.000 min
Response: 36503
Conc: 5.44 ng/ml

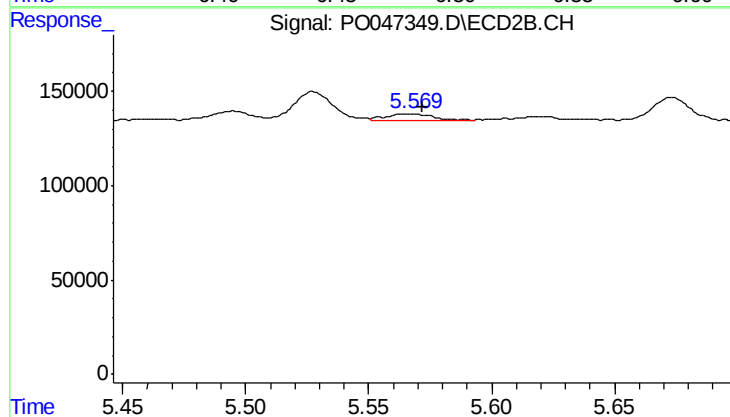

#24 AR-1248-4


R.T.: 5.567 min
Delta R.T.: -0.005 min
Response: 49241
Conc: 7.03 ng/ml

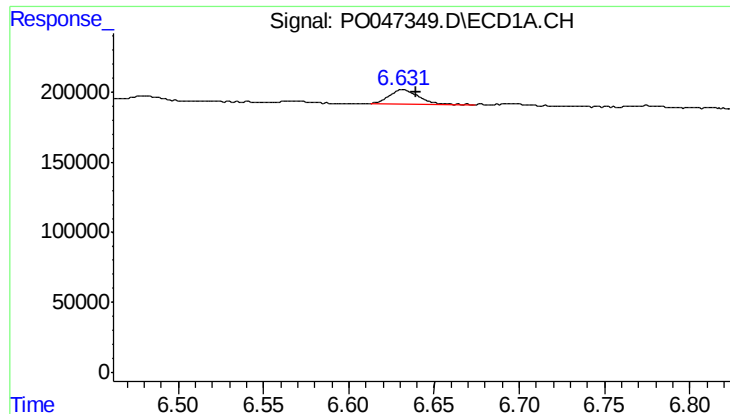

#25 AR-1248-5


R.T.: 6.632 min
Delta R.T.: -0.008 min
Response: 123209
Conc: 17.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2018

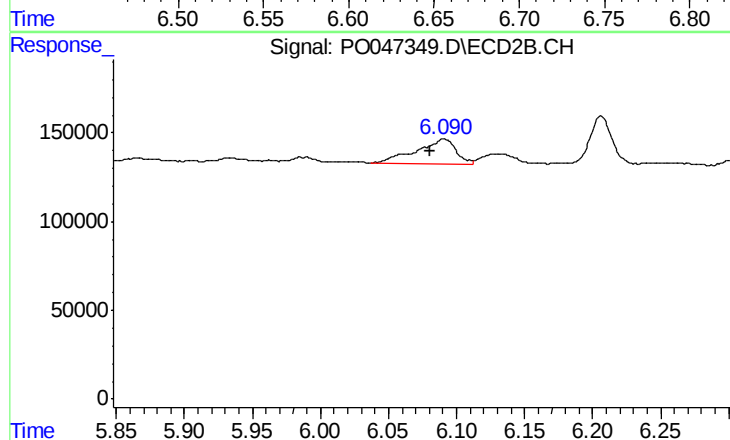


#25 AR-1248-5

R.T.: 6.091 min
Delta R.T.: 0.010 min
Response: 289929
Conc: 60.84 ng/ml

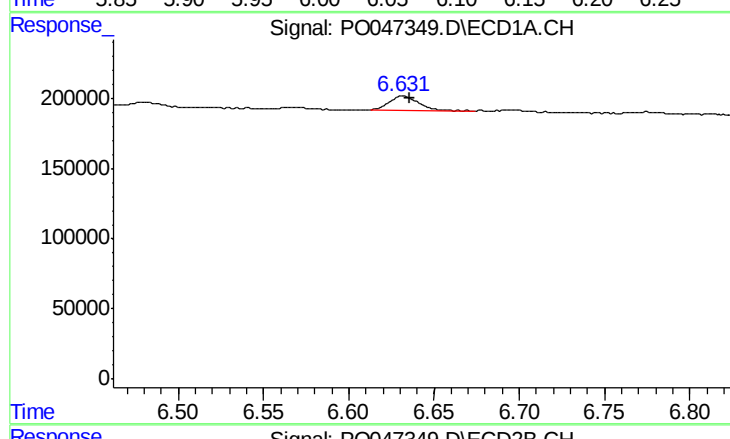


#26 AR-1254-1

R.T.: 6.632 min
Delta R.T.: -0.004 min
Response: 123209
Conc: 10.08 ng/ml

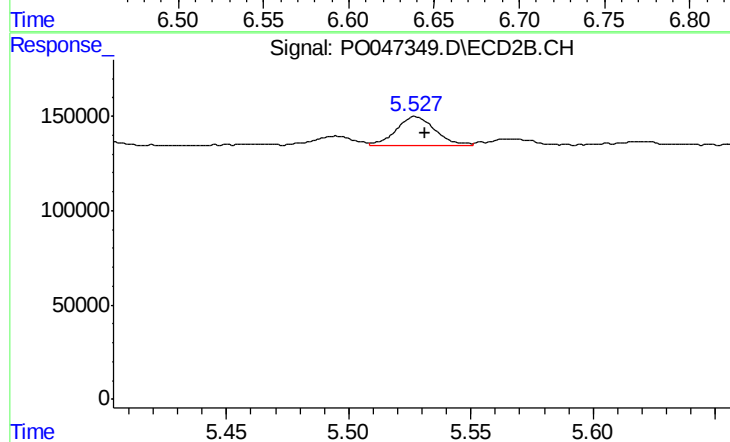

#26 AR-1254-1


R.T.: 5.528 min
Delta R.T.: -0.004 min
Response: 173365
Conc: 14.09 ng/ml

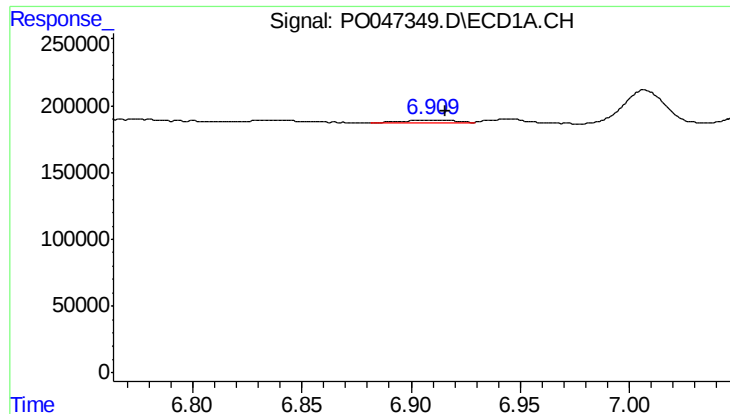

#27 AR-1254-2


R.T.: 6.913 min
Delta R.T.: -0.003 min
Response: 39900
Conc: 5.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2018

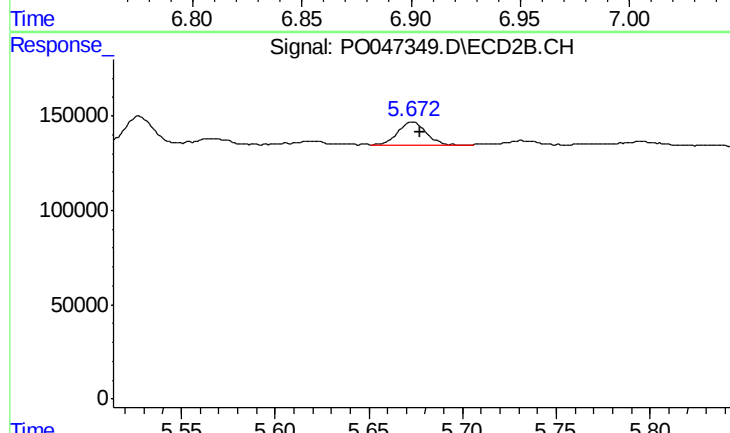


#27 AR-1254-2

R.T.: 5.673 min
Delta R.T.: -0.004 min
Response: 128935
Conc: 12.39 ng/ml

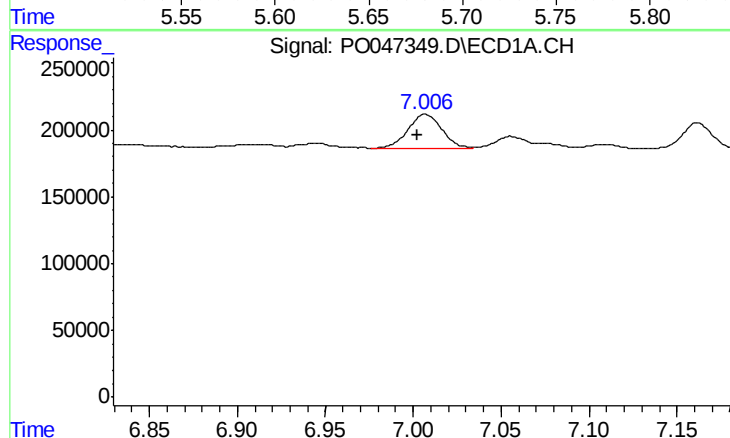


#28 AR-1254-3

R.T.: 7.007 min
Delta R.T.: 0.005 min
Response: 340454
Conc: 26.11 ng/ml

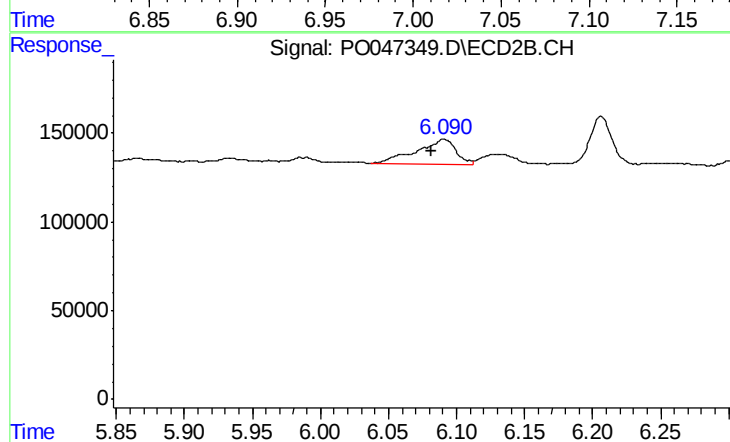

#28 AR-1254-3


R.T.: 6.091 min
Delta R.T.: 0.009 min
Response: 289929
Conc: 16.71 ng/ml

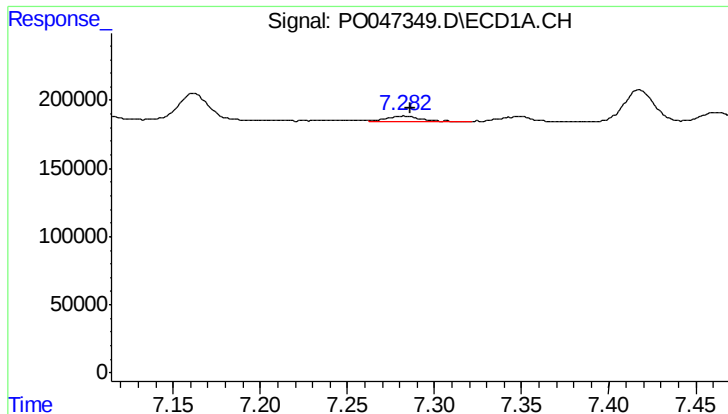

#29 AR-1254-4


R.T.: 7.283 min
Delta R.T.: -0.004 min
Response: 57407
Conc: 5.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2018

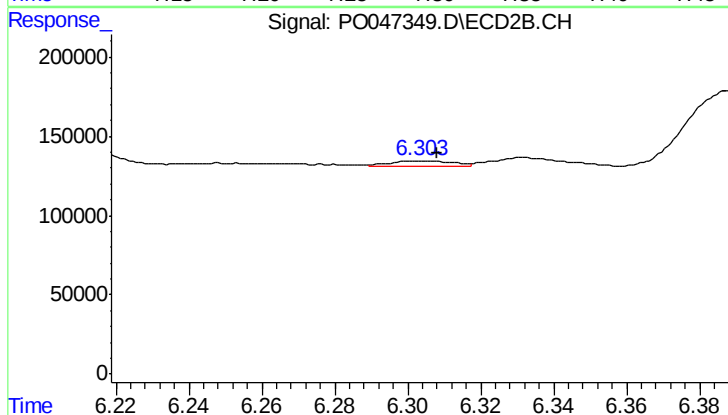


#29 AR-1254-4

R.T.: 6.304 min
Delta R.T.: -0.005 min
Response: 41526
Conc: 3.83 ng/ml

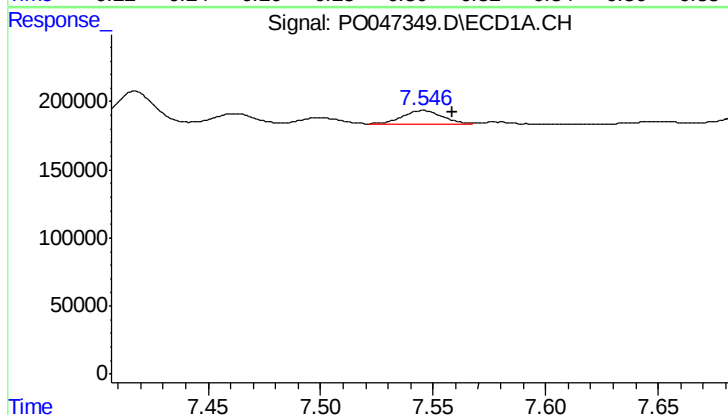


#30 AR-1254-5

R.T.: 7.546 min
Delta R.T.: -0.013 min
Response: 127855
Conc: 17.31 ng/ml

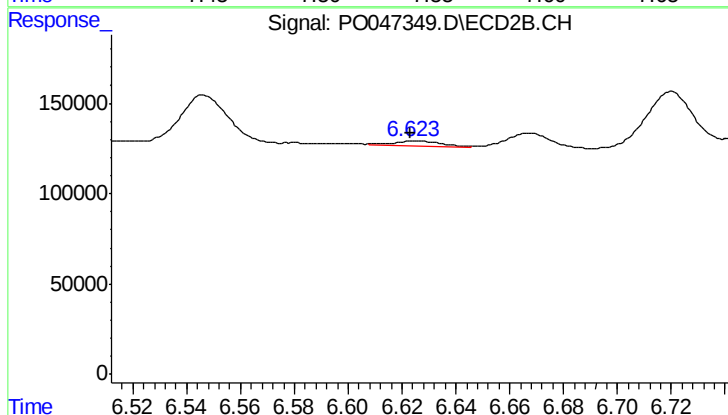

#30 AR-1254-5


R.T.: 6.625 min
Delta R.T.: 0.001 min
Response: 35220
Conc: 4.61 ng/ml

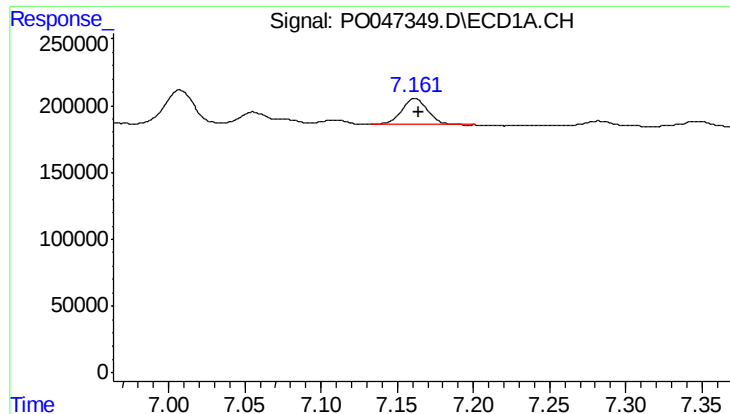

#31 AR-1260-1


R.T.: 7.162 min
Delta R.T.: -0.003 min
Response: 228955
Conc: 24.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2018

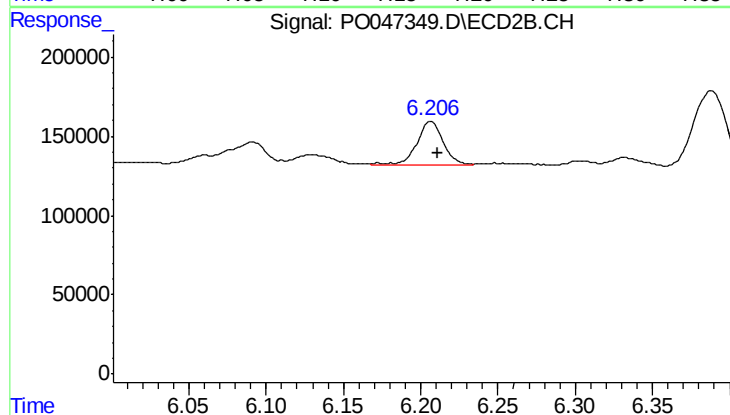


#31 AR-1260-1

R.T.: 6.206 min
Delta R.T.: -0.005 min
Response: 330792
Conc: 29.94 ng/ml

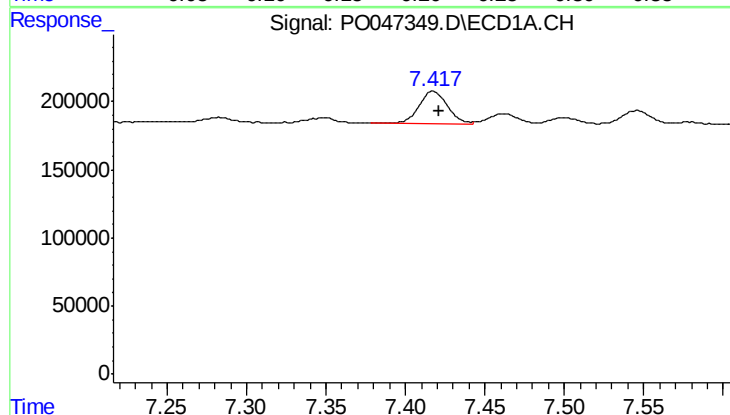


#32 AR-1260-2

R.T.: 7.418 min
Delta R.T.: -0.003 min
Response: 295560
Conc: 26.50 ng/ml

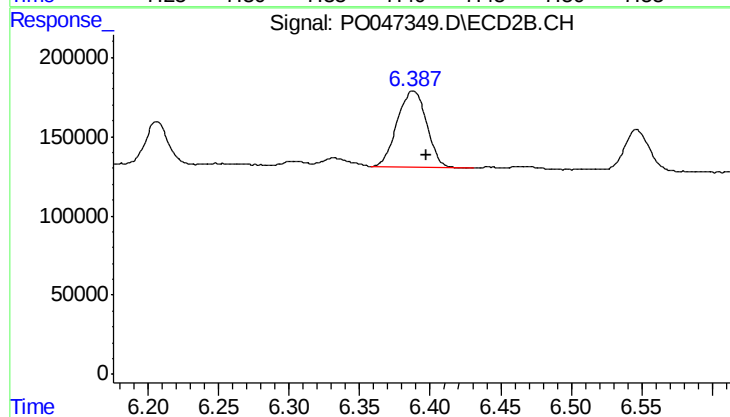

#32 AR-1260-2


R.T.: 6.388 min
Delta R.T.: -0.009 min
Response: 703544
Conc: 52.47 ng/ml

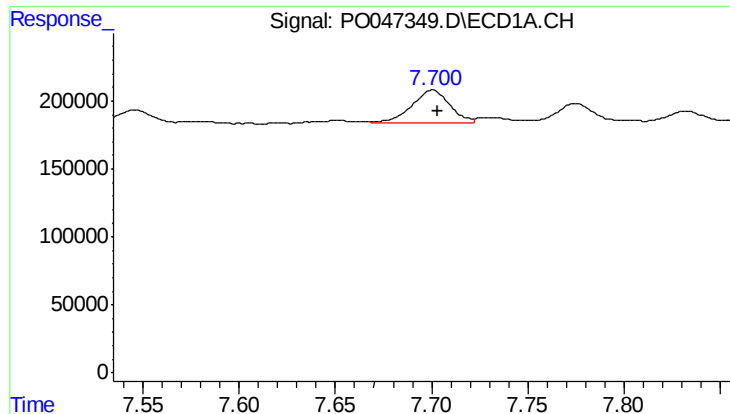

#33 AR-1260-3


R.T.: 7.701 min
Delta R.T.: -0.003 min
Response: 337203
Conc: 26.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2018

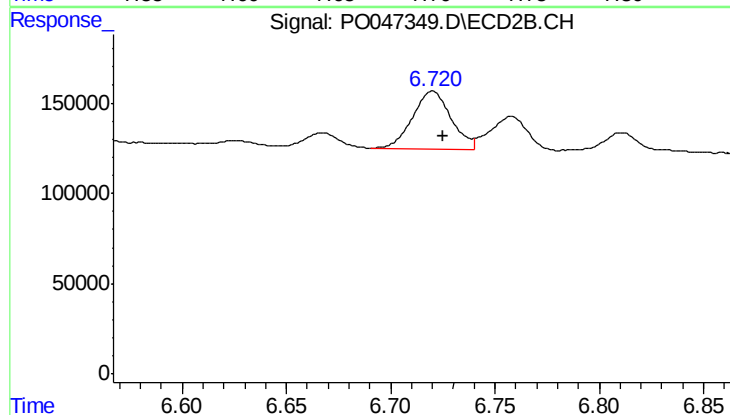


#33 AR-1260-3

R.T.: 6.720 min
Delta R.T.: -0.005 min
Response: 411860
Conc: 28.33 ng/ml

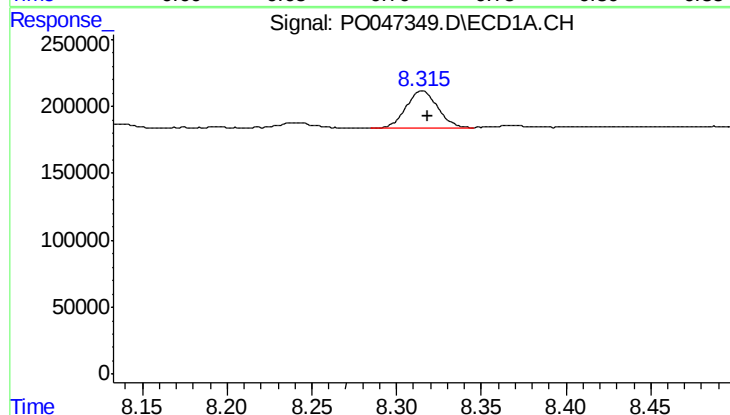


#34 AR-1260-4

R.T.: 8.315 min
Delta R.T.: -0.003 min
Response: 368542
Conc: 20.72 ng/ml

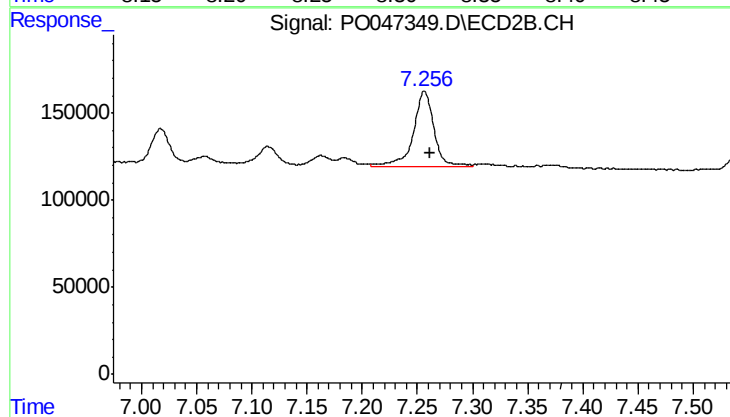

#34 AR-1260-4


R.T.: 7.257 min
Delta R.T.: -0.005 min
Response: 573541
Conc: 26.07 ng/ml

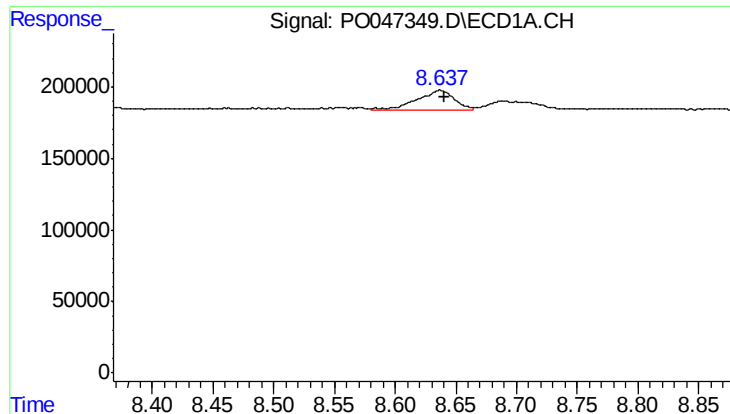

#35 AR-1260-5


R.T.: 8.637 min
Delta R.T.: -0.003 min
Response: 301619
Conc: 26.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2018

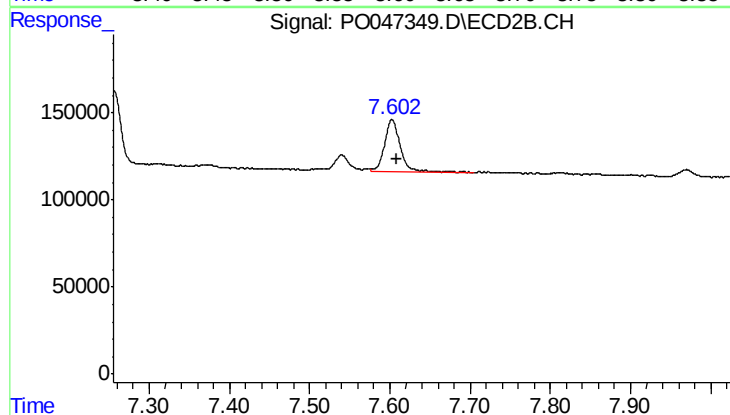


#35 AR-1260-5

R.T.: 7.603 min
Delta R.T.: -0.006 min
Response: 404370
Conc: 25.92 ng/ml

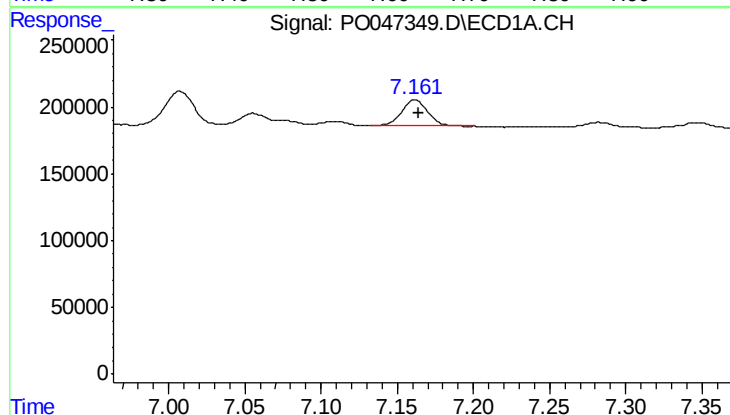


#36 AR-1262-1

R.T.: 7.162 min
Delta R.T.: -0.002 min
Response: 228955
Conc: 27.64 ng/ml

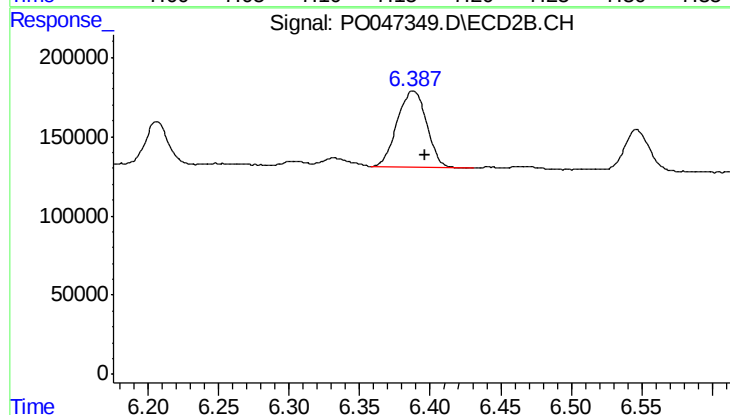

#36 AR-1262-1


R.T.: 6.388 min
Delta R.T.: -0.009 min
Response: 703544
Conc: 62.05 ng/ml

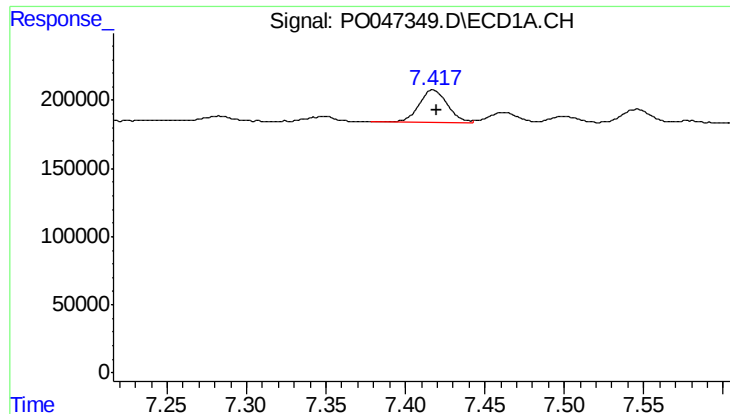

#37 AR-1262-2


R.T.: 7.418 min
Delta R.T.: -0.002 min
Response: 295560
Conc: 30.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2018

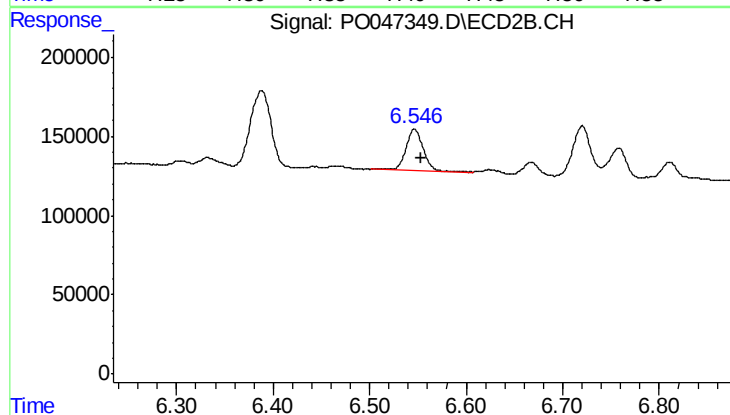


#37 AR-1262-2

R.T.: 6.546 min
Delta R.T.: -0.007 min
Response: 347287
Conc: 30.78 ng/ml

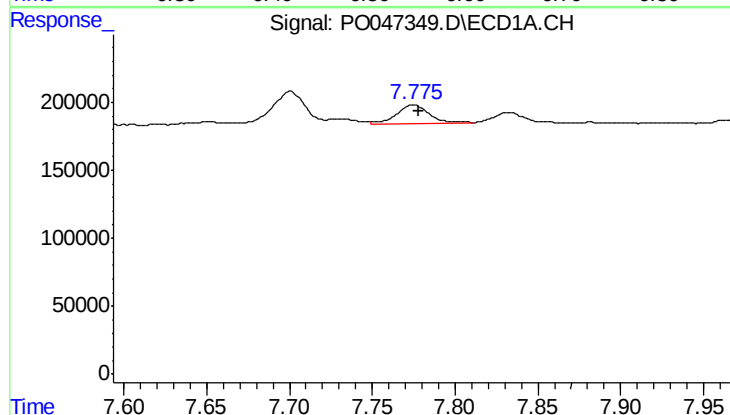


#38 AR-1262-3

R.T.: 7.775 min
Delta R.T.: -0.002 min
Response: 194376
Conc: 15.84 ng/ml

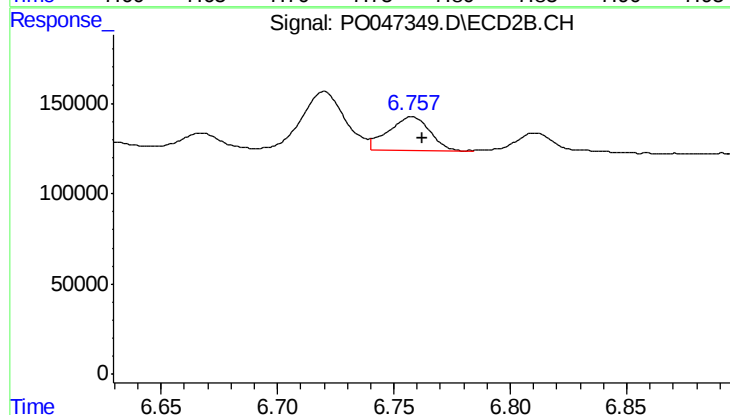

#38 AR-1262-3


R.T.: 6.758 min
Delta R.T.: -0.005 min
Response: 231465
Conc: 15.34 ng/ml

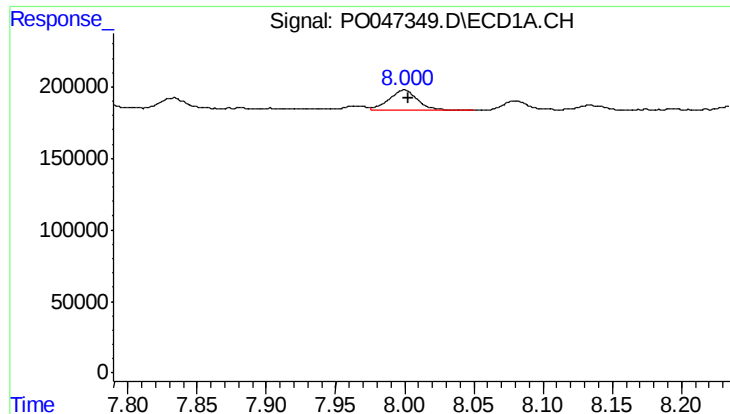

#39 AR-1262-4


R.T.: 8.000 min
Delta R.T.: -0.003 min
Response: 205525
Conc: 17.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2018

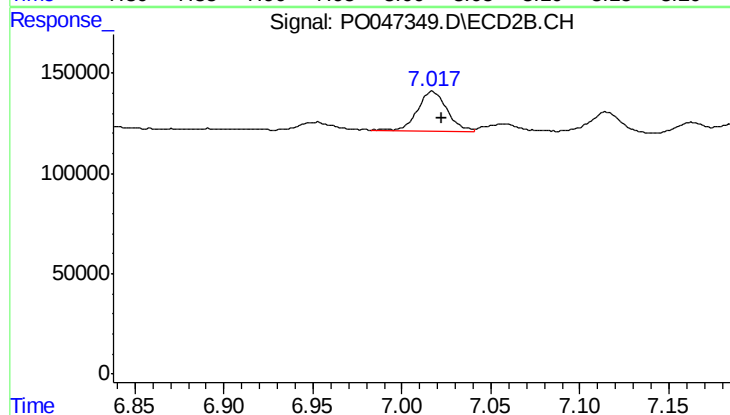


#39 AR-1262-4

R.T.: 7.017 min
Delta R.T.: -0.005 min
Response: 235200
Conc: 17.86 ng/ml

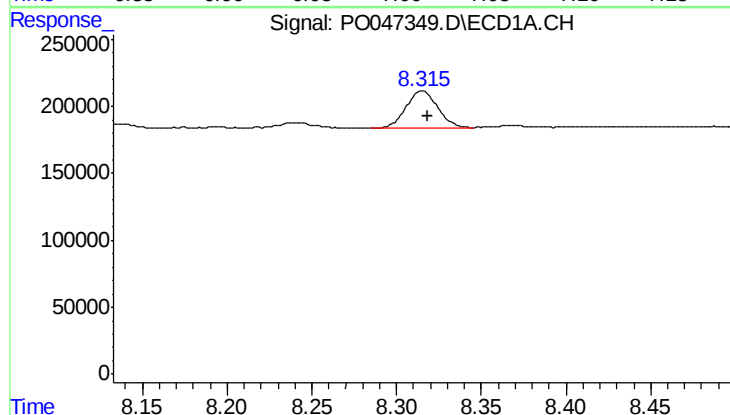


#40 AR-1262-5

R.T.: 8.315 min
Delta R.T.: -0.003 min
Response: 368542
Conc: 17.15 ng/ml

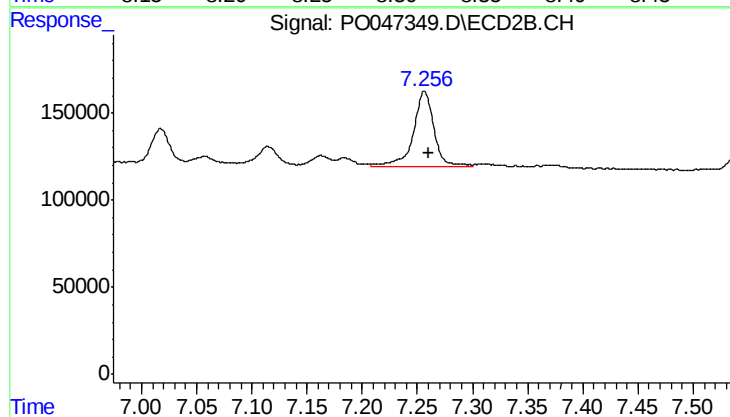

#40 AR-1262-5


R.T.: 7.257 min
Delta R.T.: -0.004 min
Response: 573541
Conc: 22.21 ng/ml

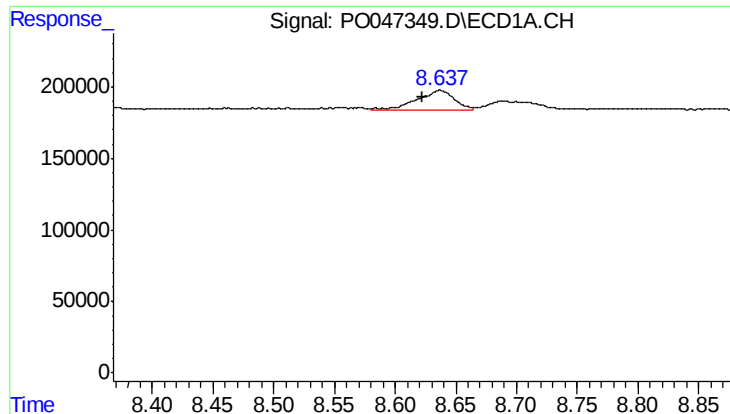

#41 AR-1268-1


R.T.: 8.637 min
Delta R.T.: 0.014 min
Response: 301619
Conc: 13.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2018

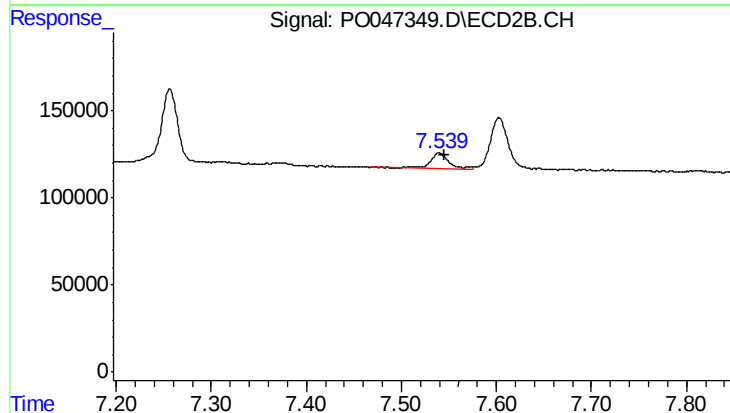


#41 AR-1268-1

R.T.: 7.540 min
Delta R.T.: -0.006 min
Response: 110480
Conc: 4.25 ng/ml

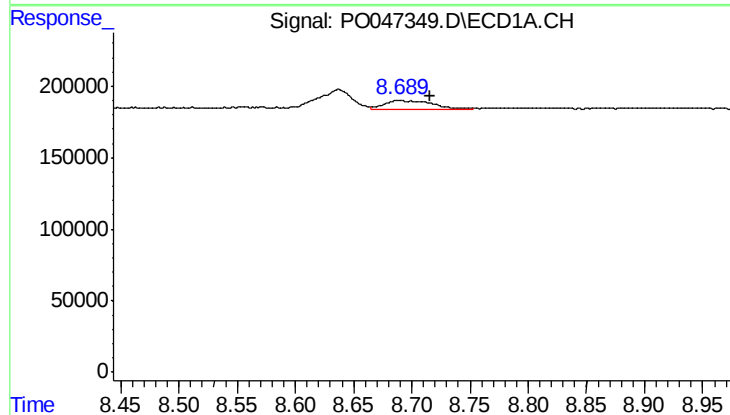


#42 AR-1268-2

R.T.: 8.690 min
Delta R.T.: -0.026 min
Response: 179119
Conc: 8.36 ng/ml

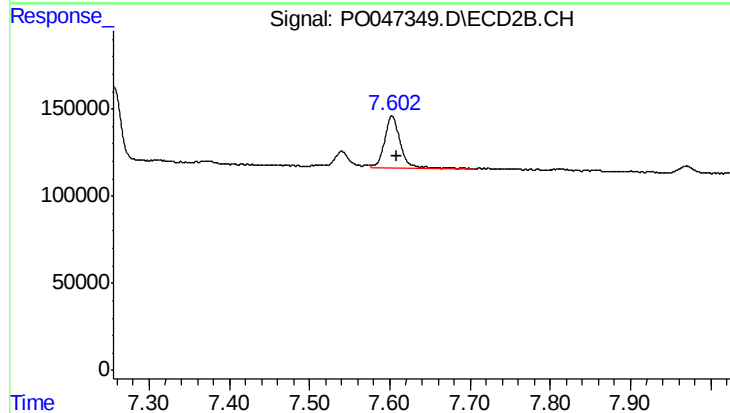

#42 AR-1268-2


R.T.: 7.603 min
Delta R.T.: -0.007 min
Response: 404370
Conc: 16.23 ng/ml

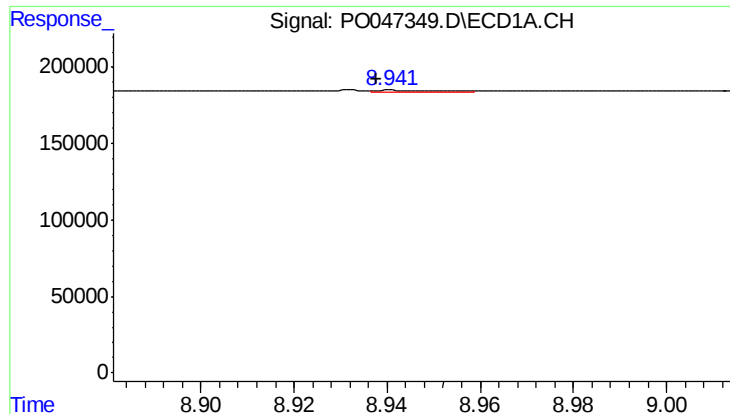

#43 AR-1268-3


R.T.: 8.941 min
Delta R.T.: 0.003 min
Response: 7029
Conc: 0.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2018

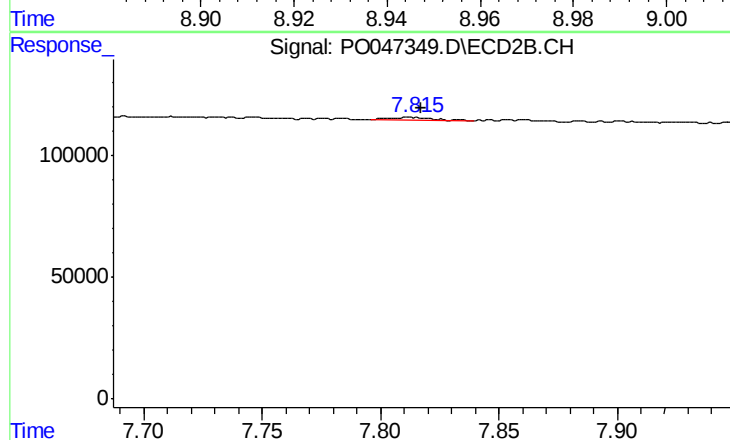


#43 AR-1268-3

R.T.: 7.812 min
Delta R.T.: -0.005 min
Response: 15628
Conc: 0.79 ng/ml

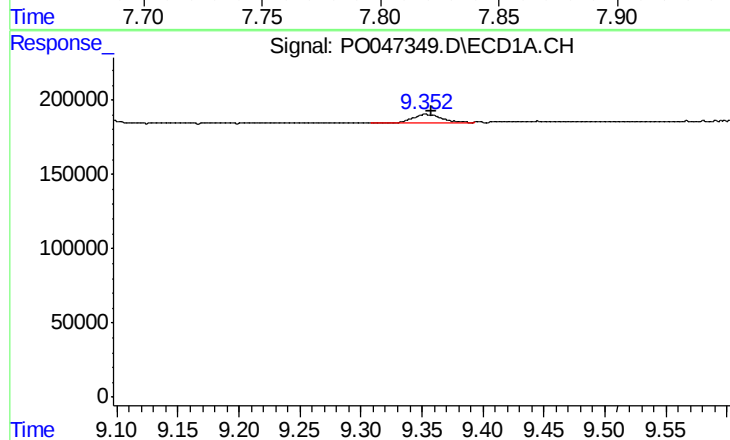


#44 AR-1268-4

R.T.: 9.353 min
Delta R.T.: -0.005 min
Response: 106850
Conc: 13.40 ng/ml

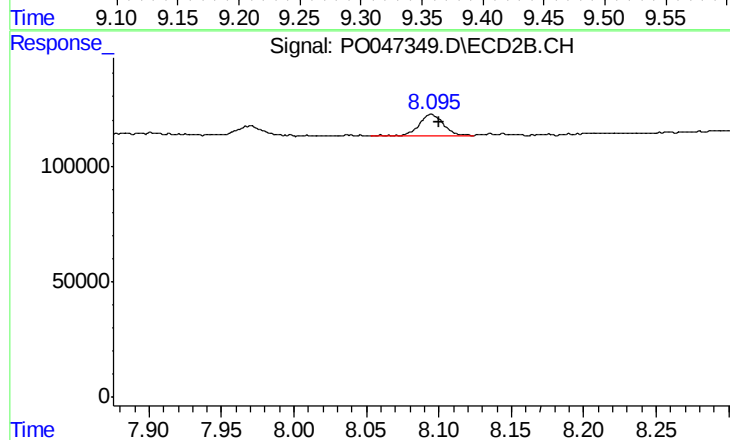

#44 AR-1268-4


R.T.: 8.095 min
Delta R.T.: -0.006 min
Response: 109461
Conc: 13.05 ng/ml

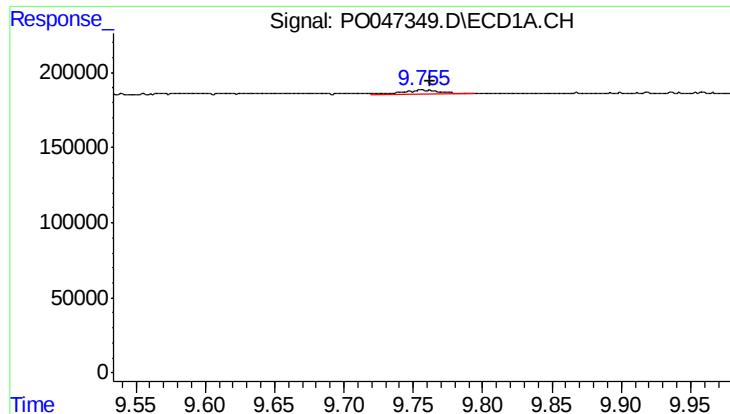

#45 AR-1268-5

R.T.: 9.756 min
Delta R.T.: -0.006 min
Response: 56761
Conc: 1.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2018

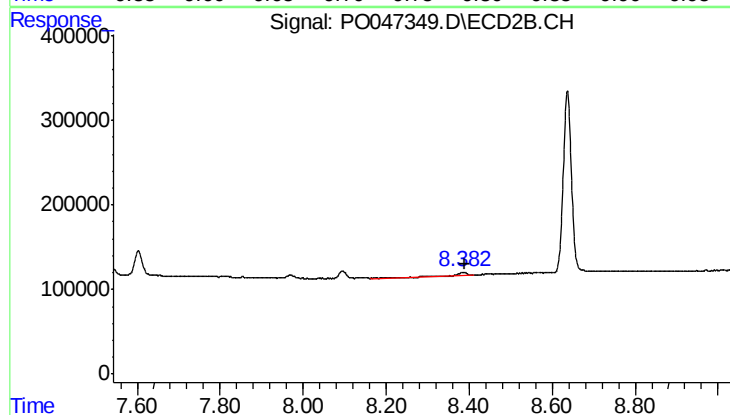

#45 AR-1268-5

R.T.: 8.385 min
Delta R.T.: -0.005 min
Response: 24187
Conc: 0.44 ng/ml