

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0073020\
 Data File : P0070212.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Jul 2020 14:11
 Operator : DD\AJ
 Sample : L3478-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ROLLOFF-VNJ-213

Manual Integrations
 APPROVED

Ankita
 7/31/2020 1:31:23 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 31 06:36:37 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0073020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 30 06:42:22 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.388	3.580f	920795	1062787	19.949m	25.435m#
2) SA Decachlor...	10.010	8.752	1501308	3047408	23.220	49.212m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0073020\
Data File : P0070212.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Jul 2020 14:11
Operator : DD\AJ
Sample : L3478-01
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
ROLLOFF-VNJ-213


Manual Integrations
APPROVED

Ankita
7/31/2020 1:31:23 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 31 06:36:37 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0073020.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 30 06:42:22 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

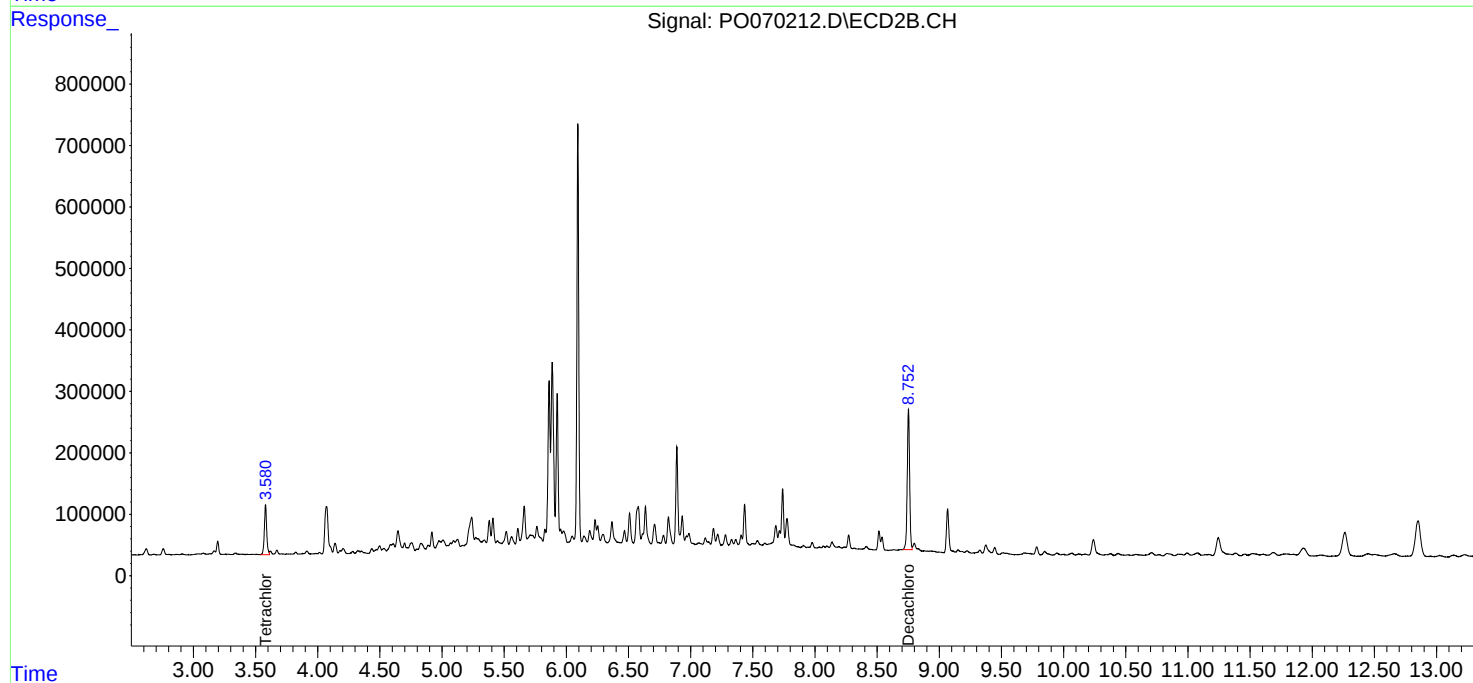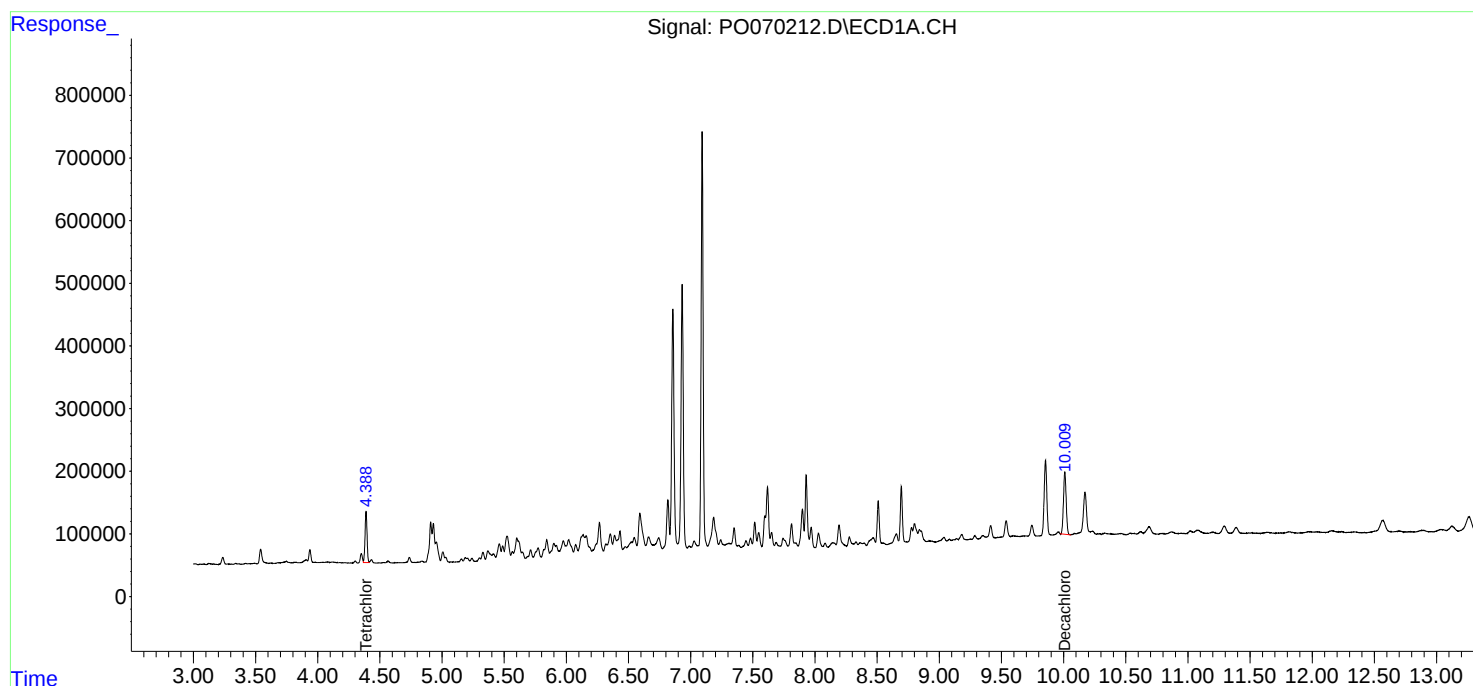

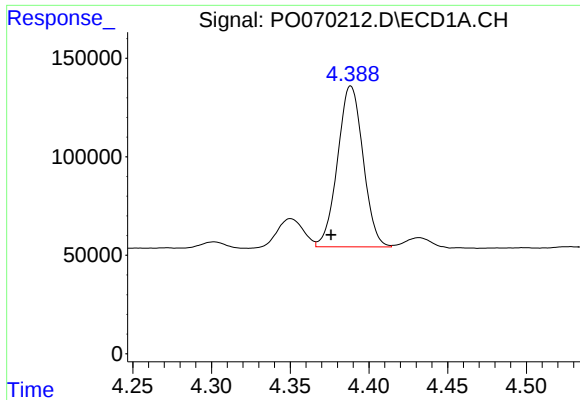

#1 Tetrachloro-m-xylene

R.T.: 4.388 min

Delta R.T.: 0.012 min


Response: 920795

Conc: 19.95 ng/ml m

Instrument :
ECD_O
ClientSampleId :
ROLLOFF-VNJ-213

Manual Integrations
APPROVED

Ankita
7/31/2020 1:31:23 PM

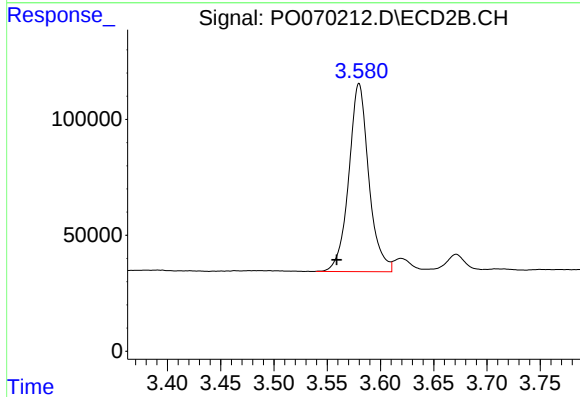


#1 Tetrachloro-m-xylene

R.T.: 3.580 min

Delta R.T.: 0.021 min

Response: 1062787

Conc: 25.43 ng/ml m

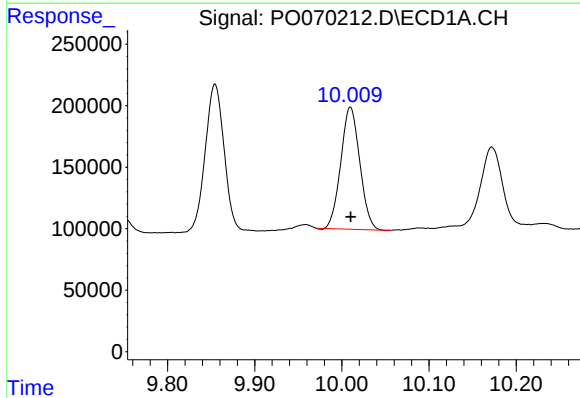


#2 Decachlorobiphenyl

R.T.: 10.010 min

Delta R.T.: 0.000 min

Response: 1501308

Conc: 23.22 ng/ml

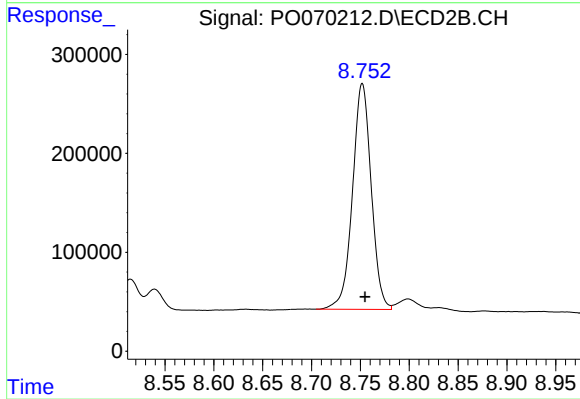

#2 Decachlorobiphenyl

R.T.: 8.752 min

Delta R.T.: -0.003 min

Response: 3047408

Conc: 49.21 ng/ml m