

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0073021\
 Data File : P0080030.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Jul 2021 20:38
 Operator : DD\AJ
 Sample : M3235-03
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MH-462-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 01:59:59 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 28 18:45:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.002	4.120	1326482	541493	22.013	23.645
2) SA Decachlor...	11.115	9.533	929986	419221	19.825	20.173
Target Compounds						
8) L2 AR-1221-1	5.254	0.000	43694	0	67.809	N.D. #
28) L6 AR-1254-3	7.878f	0.000	59367	0	17.242	N.D. #
31) L7 AR-1260-1	8.037	0.000	66057	0	26.924	N.D. #
32) L7 AR-1260-2	8.292	7.188f	126845	23636	41.275	15.451 #
38) L8 AR-1262-3	0.000	8.396	0	245824	N.D.	221.326 #
41) L9 AR-1268-1	0.000	8.396	0	245824	N.D.	80.904 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0073021\
Data File : P0080030.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Jul 2021 20:38
Operator : DD\AJ
Sample : M3235-03
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MH-462-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 01:59:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072821.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 28 18:45:36 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

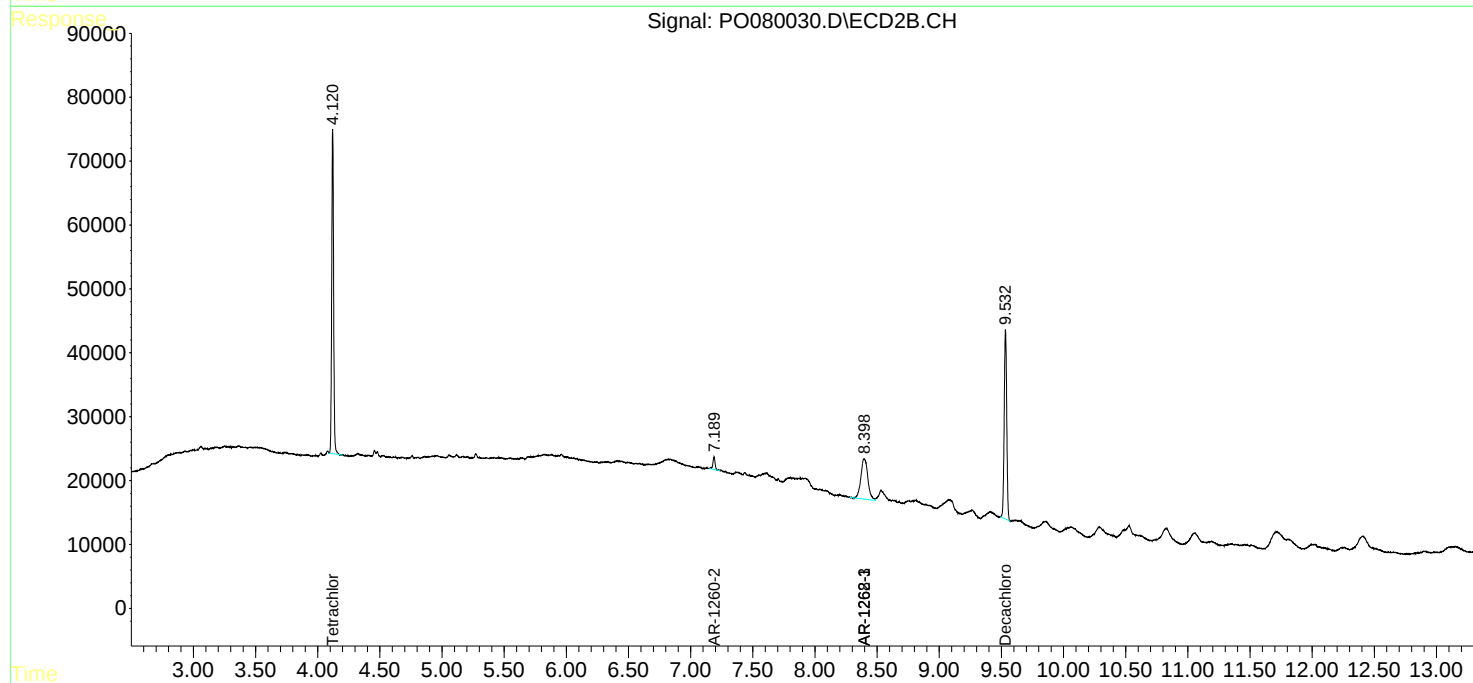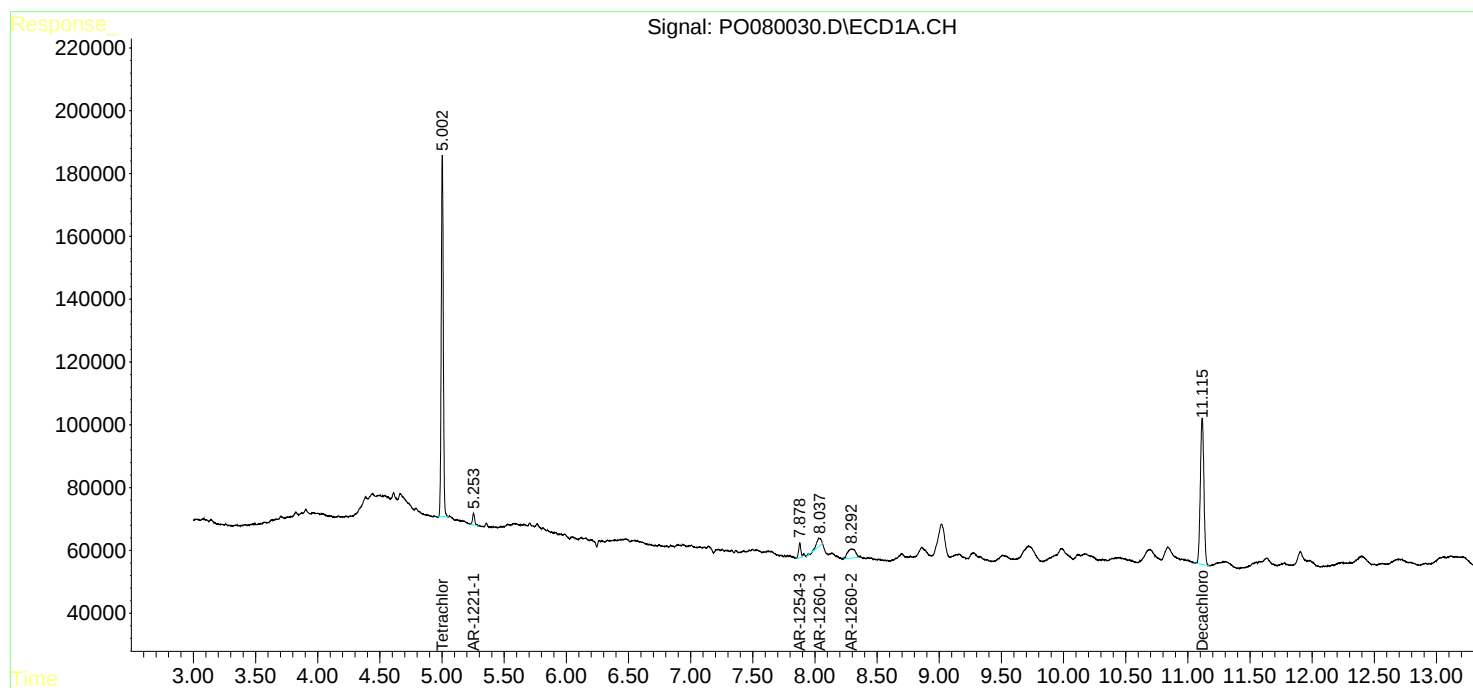


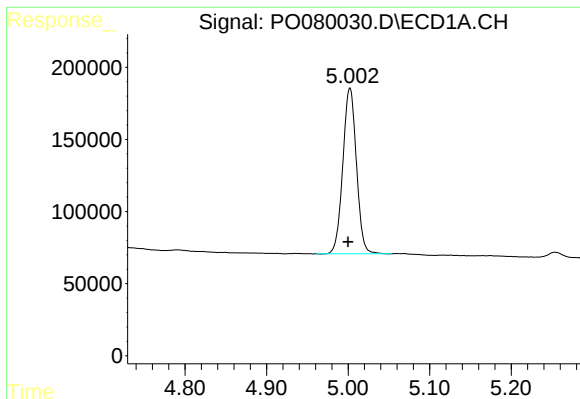

#1 Tetrachloro-m-xylene


R.T.: 5.002 min
Delta R.T.: 0.002 min
Response: 1326482
Conc: 22.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
MH-462-COMP

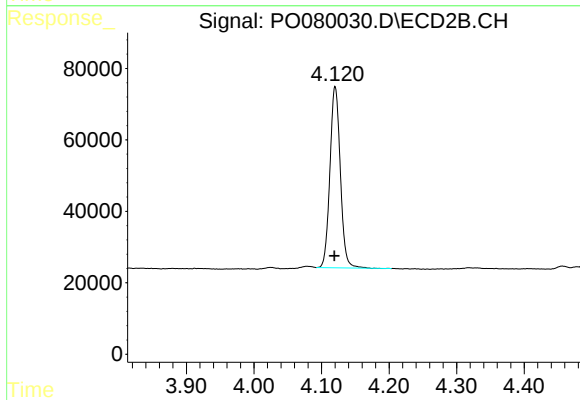


#1 Tetrachloro-m-xylene

R.T.: 4.120 min
Delta R.T.: 0.001 min
Response: 541493
Conc: 23.64 ng/ml

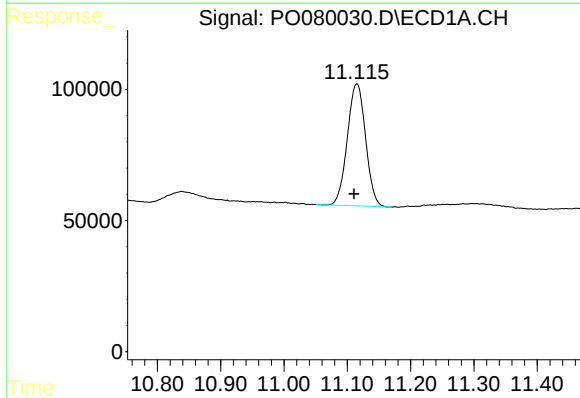


#2 Decachlorobiphenyl

R.T.: 11.115 min
Delta R.T.: 0.004 min
Response: 929986
Conc: 19.82 ng/ml

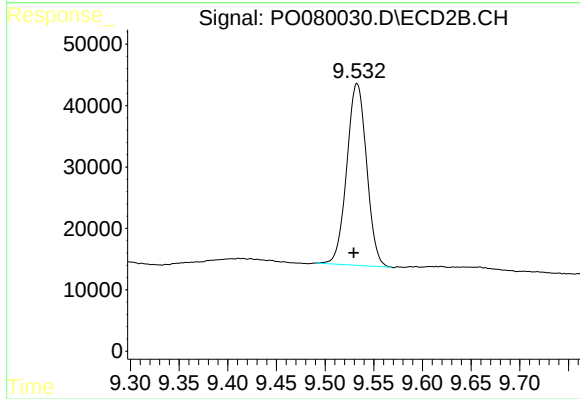

#2 Decachlorobiphenyl


R.T.: 9.533 min
Delta R.T.: 0.003 min
Response: 419221
Conc: 20.17 ng/ml

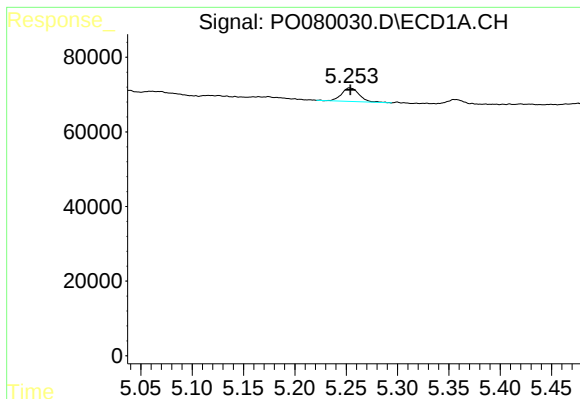

#8 AR-1221-1


R.T.: 5.254 min
Delta R.T.: 0.000 min
Response: 43694
Conc: 67.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
MH-462-COMP

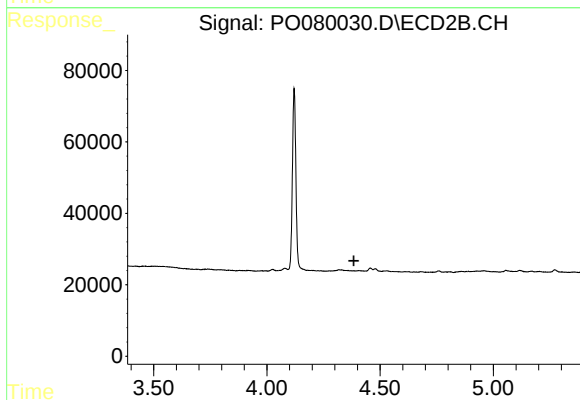


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.384 min
Response: 0
Conc: N.D.

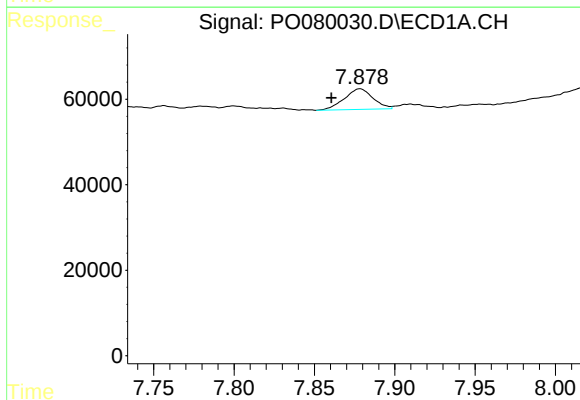


#28 AR-1254-3

R.T.: 7.878 min
Delta R.T.: 0.018 min
Response: 59367
Conc: 17.24 ng/ml

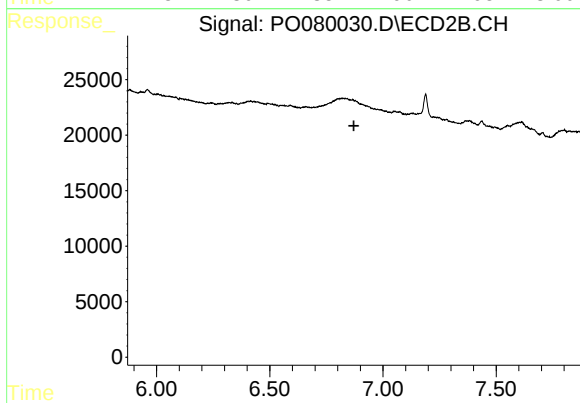

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.872 min
Response: 0
Conc: N.D.

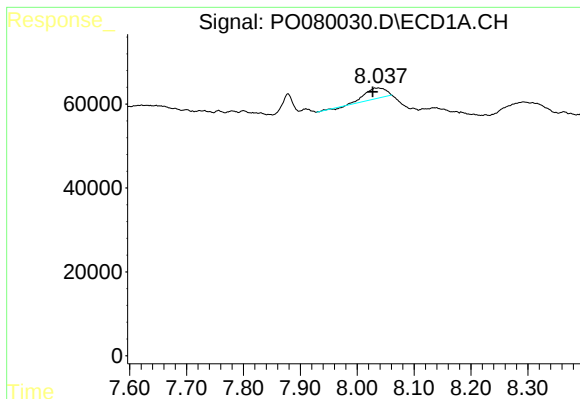

#31 AR-1260-1


R.T.: 8.037 min
Delta R.T.: 0.010 min
Response: 66057
Conc: 26.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
MH-462-COMP

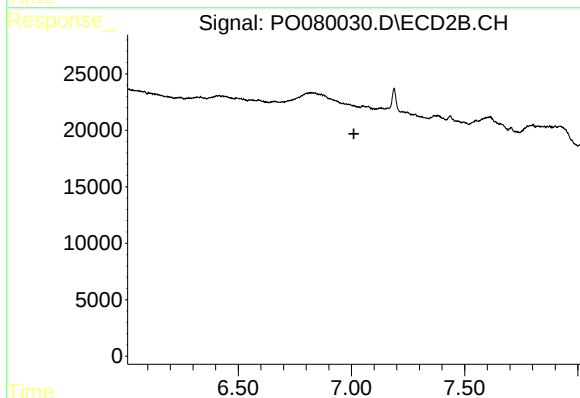


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T. : 7.011 min
Response: 0
Conc: N.D.

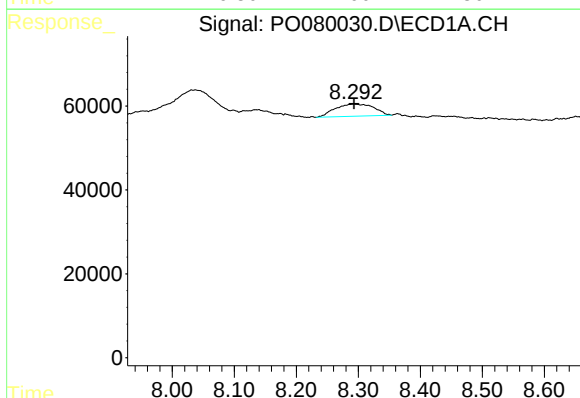


#32 AR-1260-2

R.T.: 8.292 min
Delta R.T.: -0.001 min
Response: 126845
Conc: 41.28 ng/ml

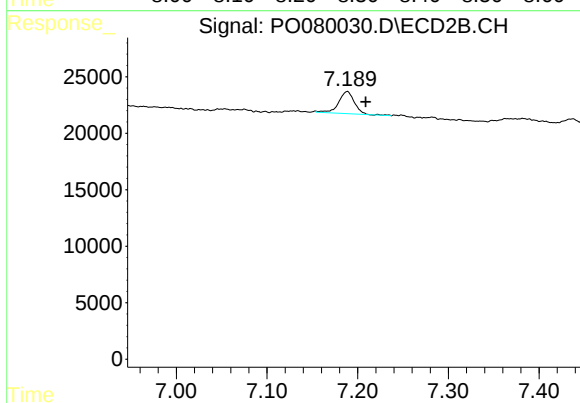

#32 AR-1260-2


R.T.: 7.188 min
Delta R.T.: -0.021 min
Response: 23636
Conc: 15.45 ng/ml

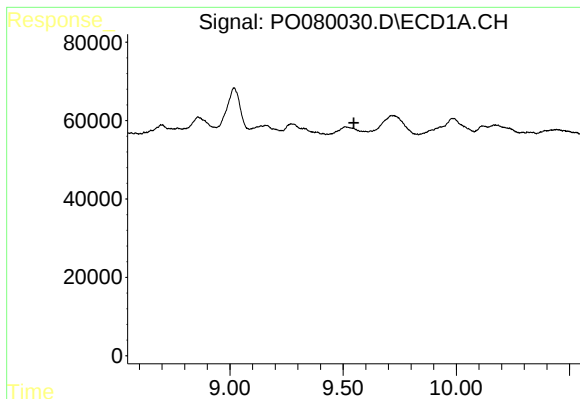

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T.: 9.547 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
MH-462-COMP

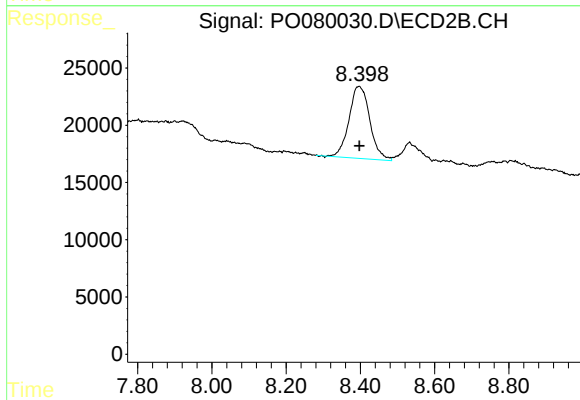


#38 AR-1262-3

R.T.: 8.396 min
Delta R.T.: -0.001 min
Response: 245824
Conc: 221.33 ng/ml

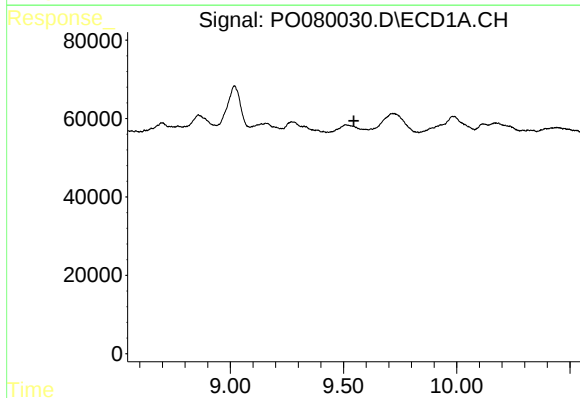

#41 AR-1268-1

R.T.: 0.000 min
Exp R.T.: 9.546 min
Response: 0
Conc: N.D.

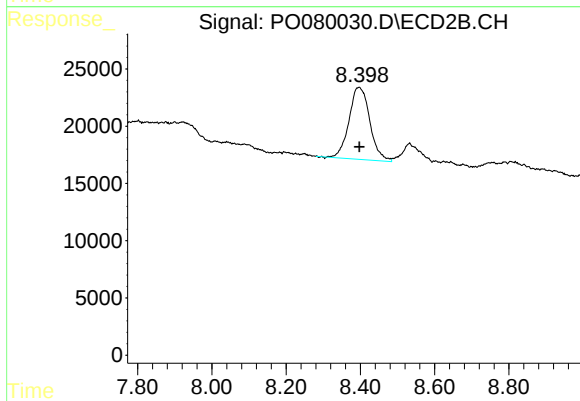

#41 AR-1268-1

R.T.: 8.396 min
Delta R.T.: -0.002 min
Response: 245824
Conc: 80.90 ng/ml