

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0073025\
 Data File : P0112622.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jul 2025 19:40
 Operator : YP/AJ
 Sample : Q2722-03 10X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LAW-25-0108

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/31/2025
 Supervised By :mohammad ahmed 08/01/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 31 04:10:21 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 24 04:54:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.669	3.661	6143599	4179537	0.756m	0.841m
2) SA Decachlor...	8.715	8.658	67033412	9810411	9.168m	5.552m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO073025\
Data File : PO112622.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jul 2025 19:40
Operator : YP/AJ
Sample : Q2722-03 10X
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
LAW-25-0108


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/31/2025
Supervised By :mohammad ahmed 08/01/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 31 04:10:21 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072325.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 24 04:54:06 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

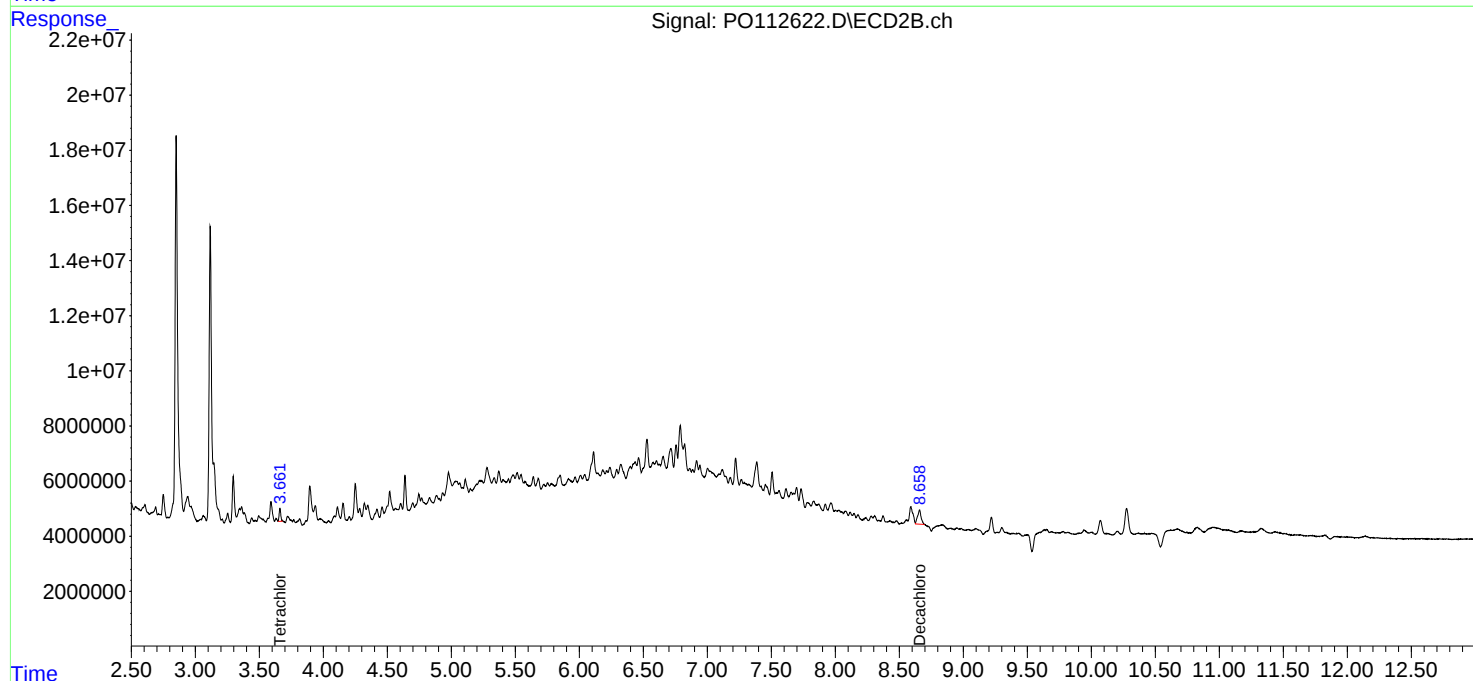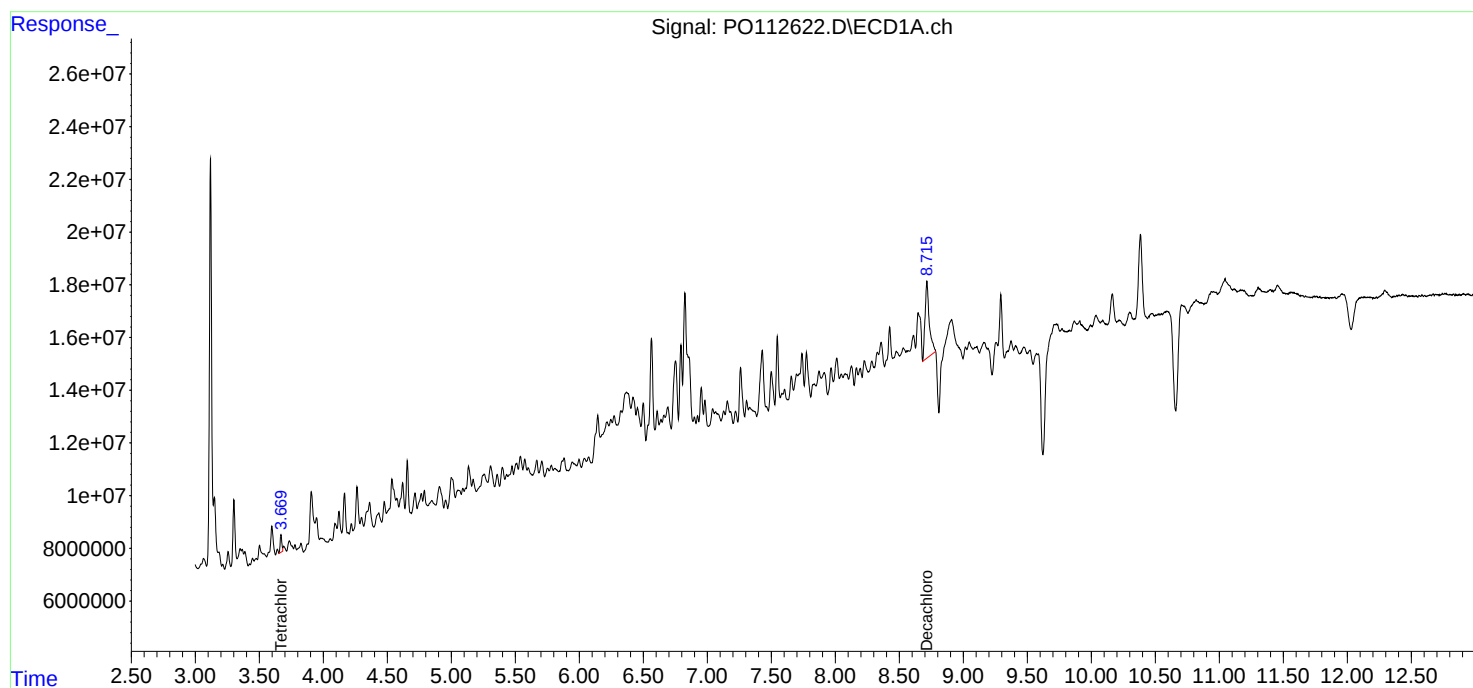

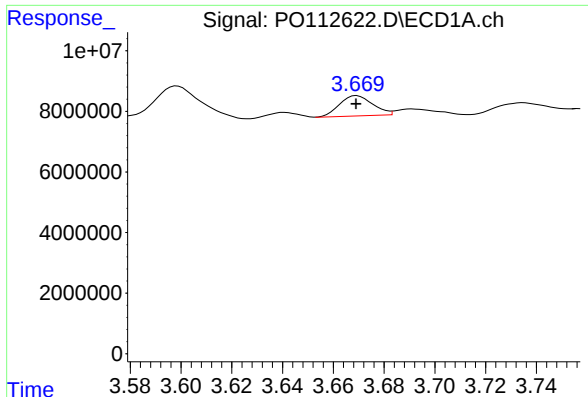


#1 Tetrachloro-m-xylene

R.T.: 3.669 min
Delta R.T.: 0.000 min
Response: 6143599
Conc: 0.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
LAW-25-0108


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/31/2025
Supervised By :mohammad ahmed 08/01/2025

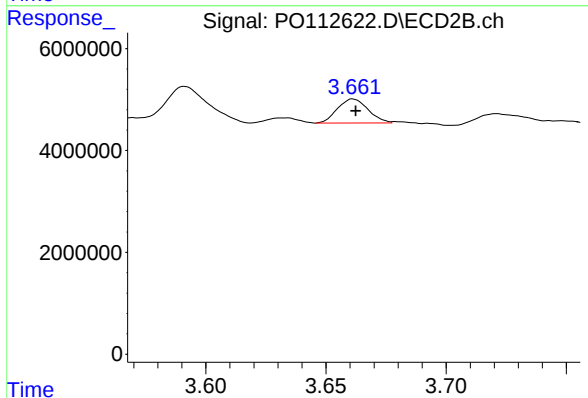


#1 Tetrachloro-m-xylene

R.T.: 3.661 min
Delta R.T.: -0.002 min
Response: 4179537
Conc: 0.84 ng/ml m

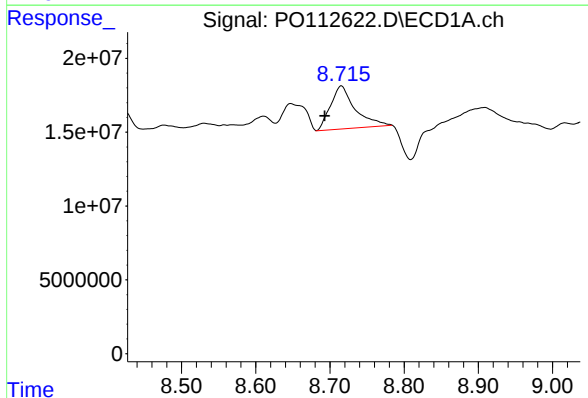

#2 Decachlorobiphenyl

R.T.: 8.715 min
Delta R.T.: 0.022 min
Response: 67033412
Conc: 9.17 ng/ml m

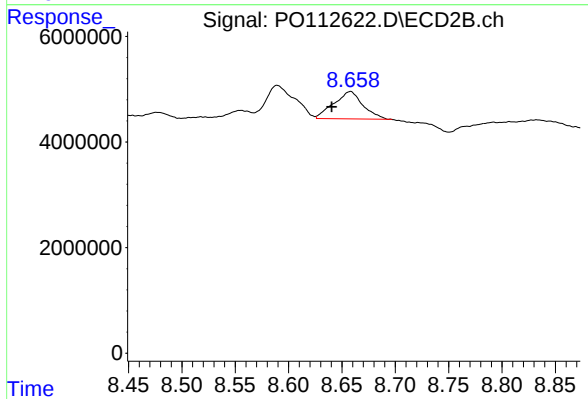

#2 Decachlorobiphenyl

R.T.: 8.658 min
Delta R.T.: 0.017 min
Response: 9810411
Conc: 5.55 ng/ml m