

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0073119\
 Data File : P0058596.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Jul 2019 9:50
 Operator : SM/AJ
 Sample : K4046-05RE
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S2-01-SRE

Manual Integrations
 APPROVED

Ankita
 7/31/2019 3:36:12 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 30 12:15:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jul 27 06:49:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.174	3.522	873131	763161	20.689	19.103
2)	SA Decachlor...	9.658	8.411	568983	452581	10.506m	11.466
Target Compounds							
26)	L6 AR-1254-1	6.166	5.364	327803	303547	138.824m	117.175
27)	L6 AR-1254-2	6.382	5.510	626572	374752	162.579	163.688
28)	L6 AR-1254-3	6.746	5.907	837378	764801	206.778	207.862
29)	L6 AR-1254-4	7.028	6.134	711593	461567	197.629	198.505
30)	L6 AR-1254-5	7.442	6.544	908014	808464	250.503	234.368

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0073119\
Data File : P0058596.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Jul 2019 9:50
Operator : SM/AJ
Sample : K4046-05RE
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
S2-01-SRE


Manual Integrations
APPROVED

Ankita
7/31/2019 3:36:12 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 30 12:15:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 27 06:49:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

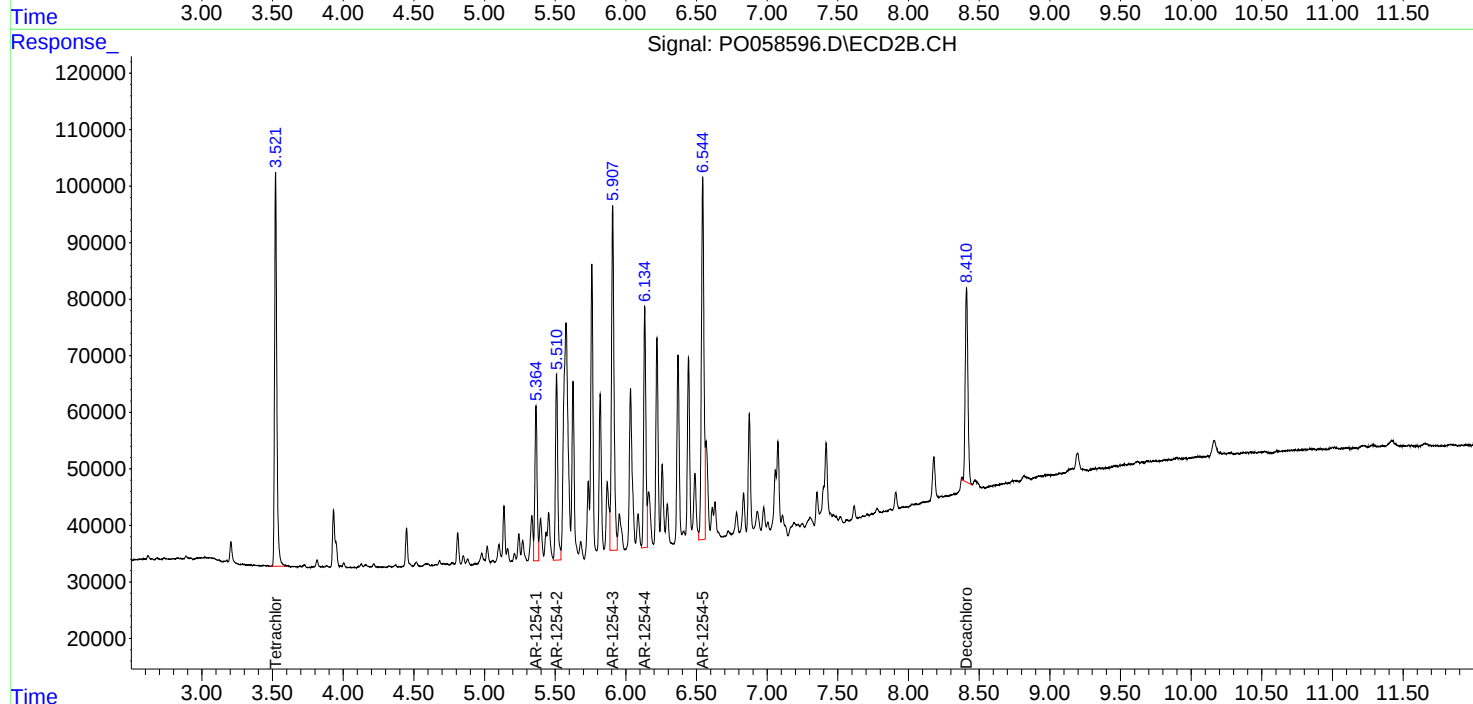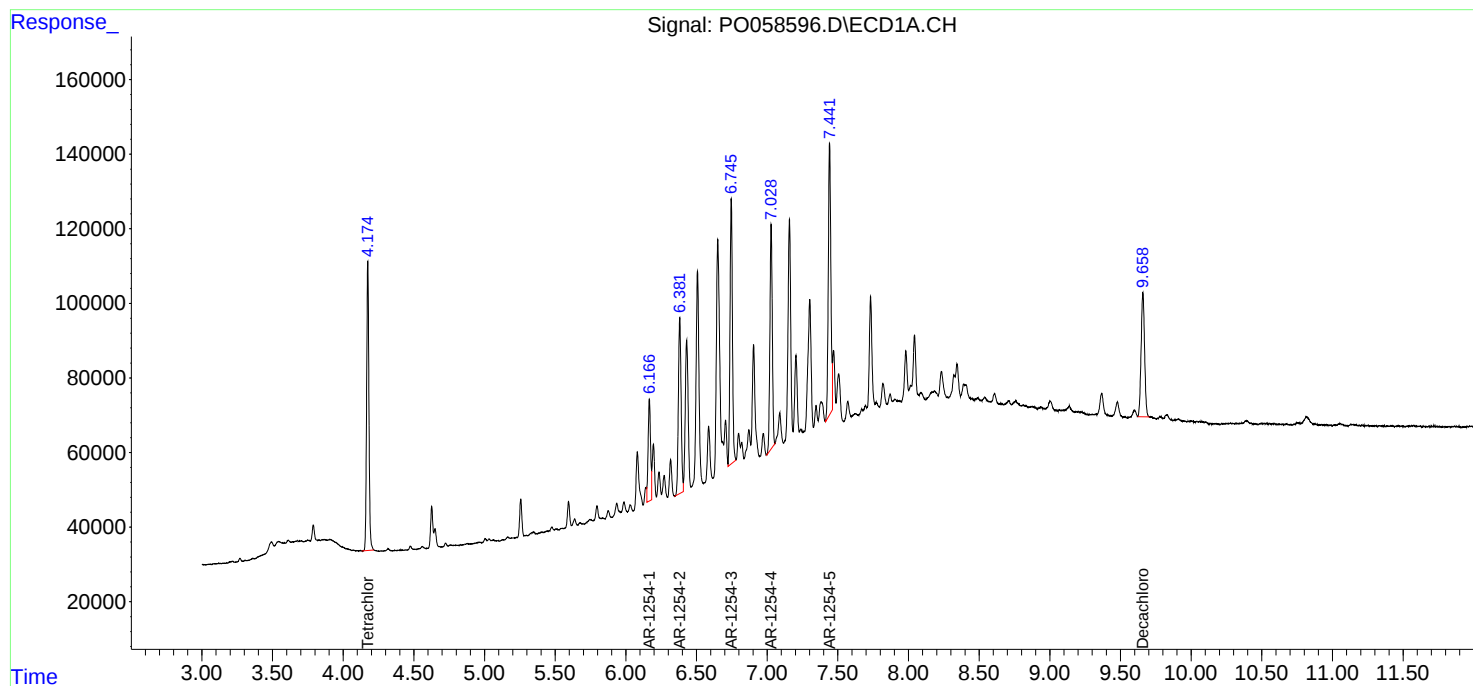

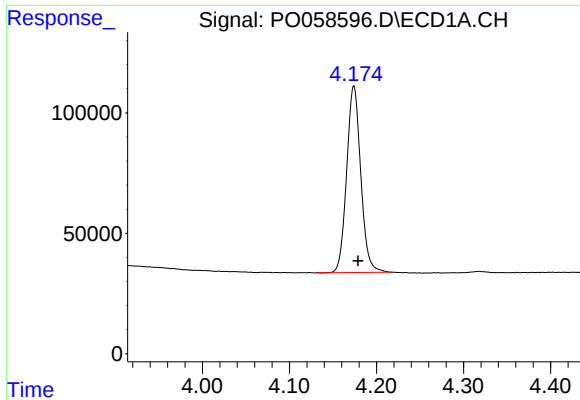


#1 Tetrachloro-m-xylene

R.T.: 4.174 min
Delta R.T.: -0.005 min
Response: 873131
Conc: 20.69 ng/ml

Instrument :
ECD_O
ClientSampleId :
S2-01-SRE


Manual Integrations
APPROVED

Ankita
7/31/2019 3:36:12 PM

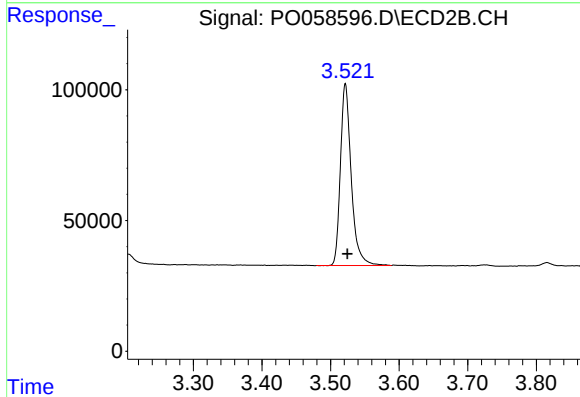


#1 Tetrachloro-m-xylene

R.T.: 3.522 min
Delta R.T.: -0.003 min
Response: 763161
Conc: 19.10 ng/ml

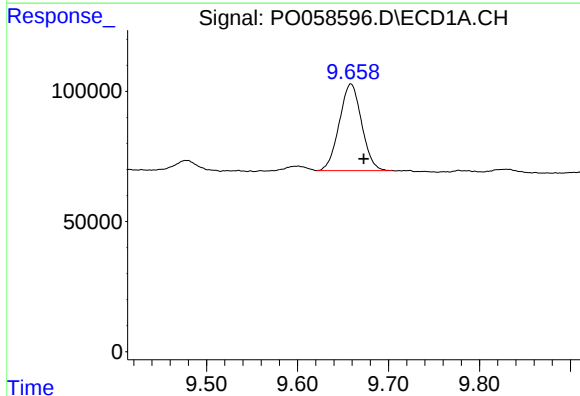


#2 Decachlorobiphenyl

R.T.: 9.658 min
Delta R.T.: -0.015 min
Response: 568983
Conc: 10.51 ng/ml m

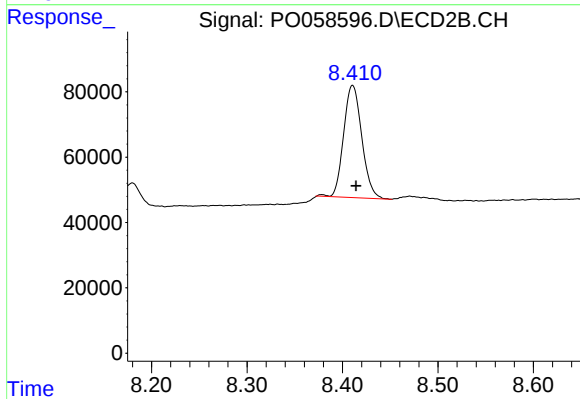

#2 Decachlorobiphenyl

R.T.: 8.411 min
Delta R.T.: -0.003 min
Response: 452581
Conc: 11.47 ng/ml

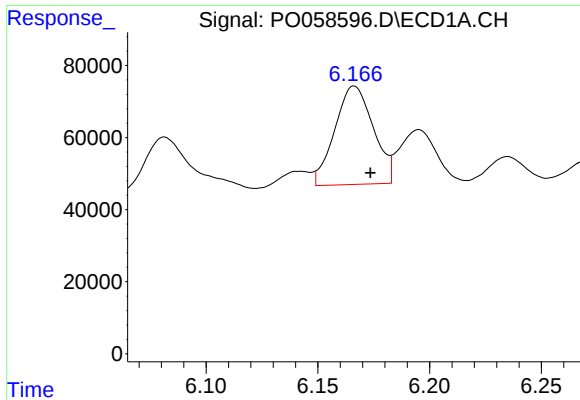


#26 AR-1254-1

R.T.: 6.166 min
Delta R.T.: -0.008 min
Response: 327803
Conc: 138.82 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S2-01-SRE


Manual Integrations
APPROVED

Ankita
7/31/2019 3:36:12 PM

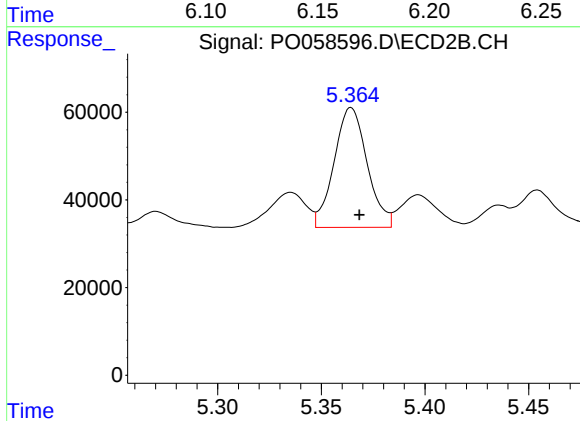


#26 AR-1254-1

R.T.: 5.364 min
Delta R.T.: -0.004 min
Response: 303547
Conc: 117.18 ng/ml

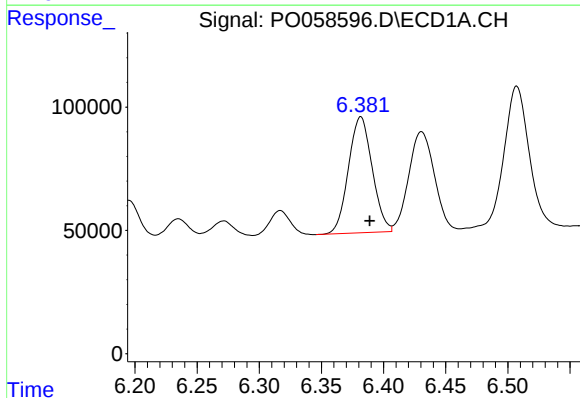


#27 AR-1254-2

R.T.: 6.382 min
Delta R.T.: -0.007 min
Response: 626572
Conc: 162.58 ng/ml

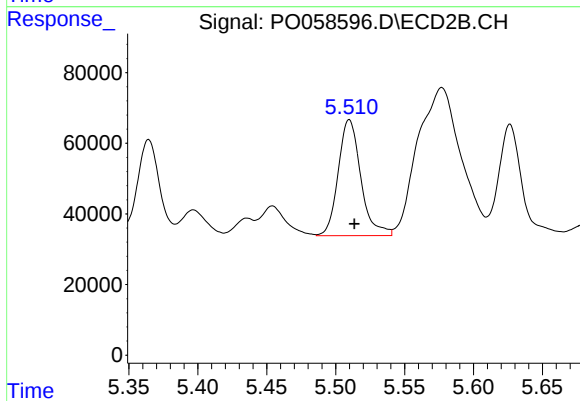

#27 AR-1254-2

R.T.: 5.510 min
Delta R.T.: -0.004 min
Response: 374752
Conc: 163.69 ng/ml

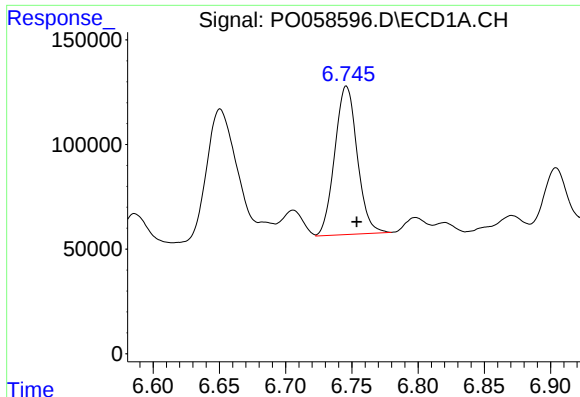


#28 AR-1254-3

R.T.: 6.746 min
Delta R.T.: -0.008 min
Response: 837378
Conc: 206.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
S2-01-SRE


Manual Integrations
APPROVED

Ankita
7/31/2019 3:36:12 PM

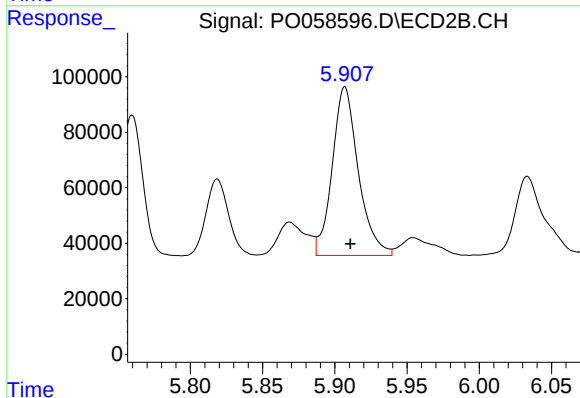


#28 AR-1254-3

R.T.: 5.907 min
Delta R.T.: -0.004 min
Response: 764801
Conc: 207.86 ng/ml

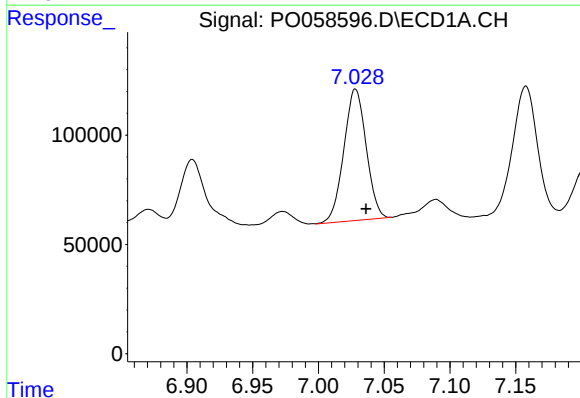


#29 AR-1254-4

R.T.: 7.028 min
Delta R.T.: -0.008 min
Response: 711593
Conc: 197.63 ng/ml

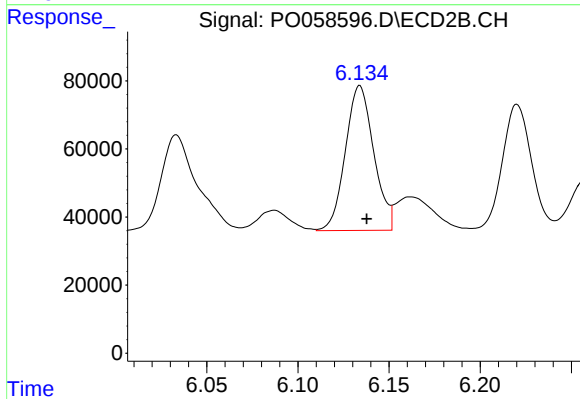

#29 AR-1254-4

R.T.: 6.134 min
Delta R.T.: -0.004 min
Response: 461567
Conc: 198.51 ng/ml

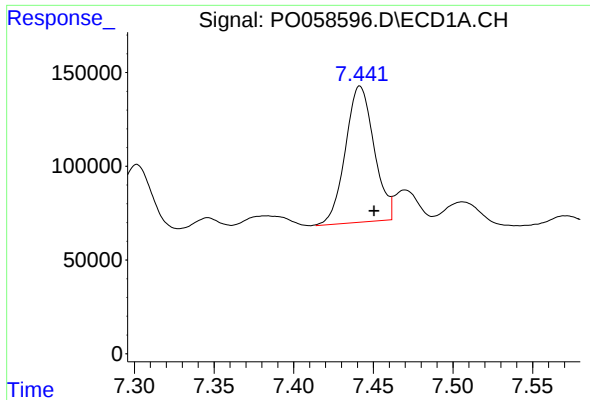


#30 AR-1254-5

R.T.: 7.442 min
Delta R.T.: -0.009 min
Response: 908014
Conc: 250.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
S2-01-SRE

Manual Integrations
APPROVED

Ankita
7/31/2019 3:36:12 PM

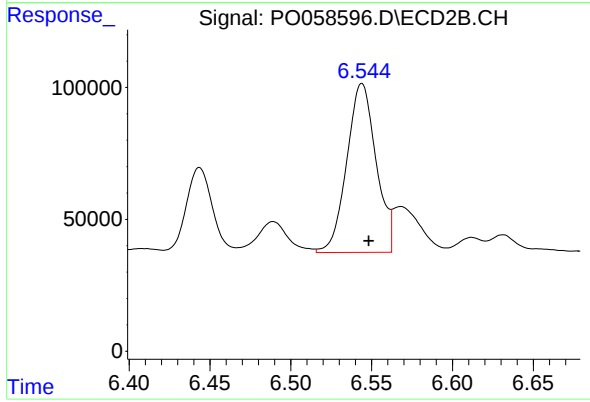

#30 AR-1254-5

R.T.: 6.544 min
Delta R.T.: -0.004 min
Response: 808464
Conc: 234.37 ng/ml