

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0073119\
 Data File : P0058601.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Jul 2019 11:15
 Operator : SM/AJ
 Sample : K3969-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TANK-1

Manual Integrations
 APPROVED

mohammad
 8/1/2019 1:27:35 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 30 13:53:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jul 27 06:49:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.172	3.522	1061440	1084813	25.151m	27.154m
2) SA Decachlor...	9.657	8.412	831120	613924	15.347	15.553m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0073119\
Data File : P0058601.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Jul 2019 11:15
Operator : SM/AJ
Sample : K3969-01
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TANK-1


Manual Integrations
APPROVED

mohammad
8/1/2019 1:27:35 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 30 13:53:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 27 06:49:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

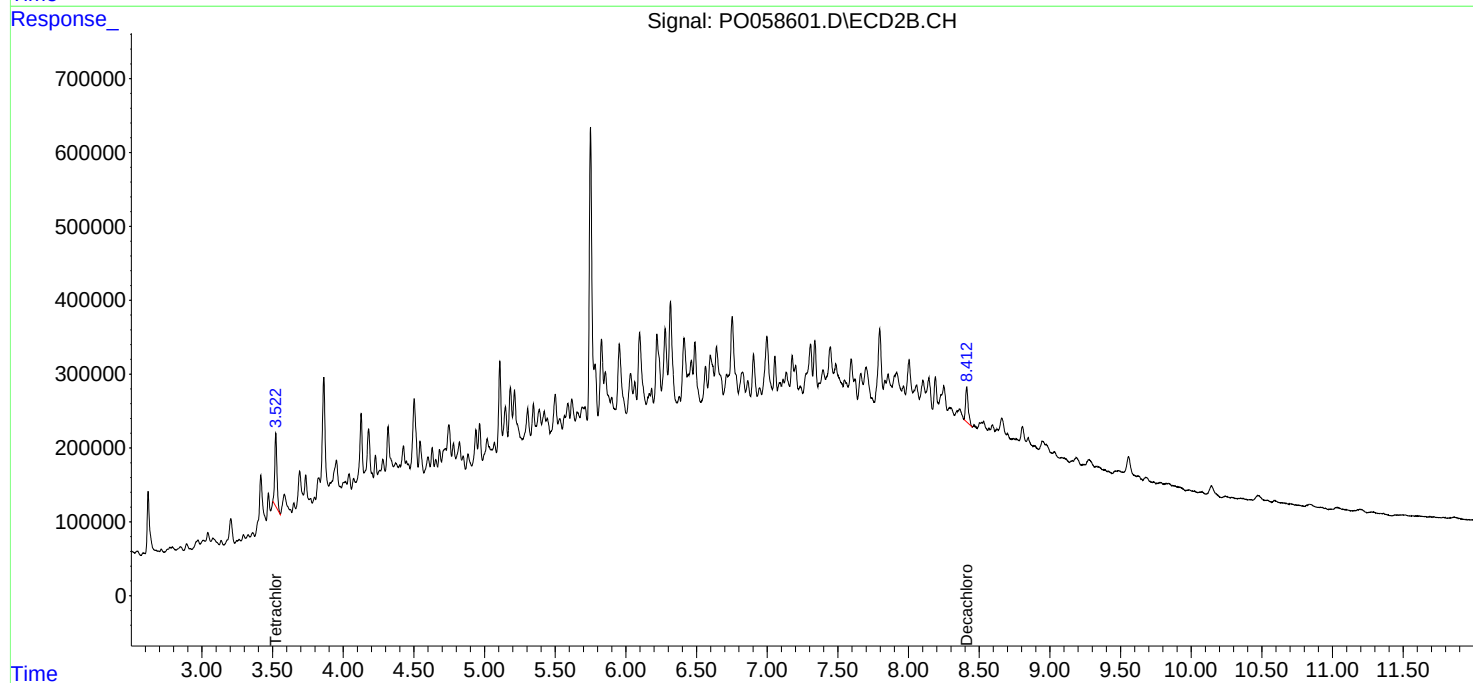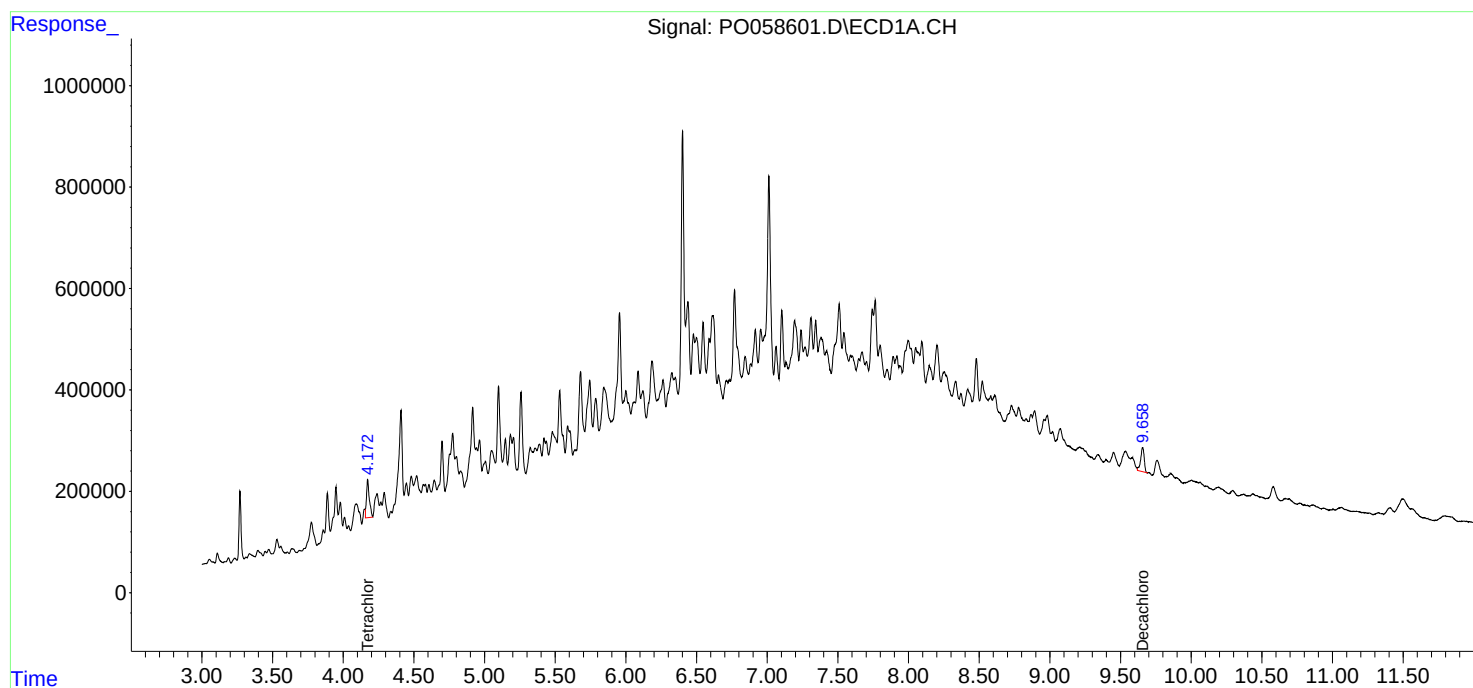

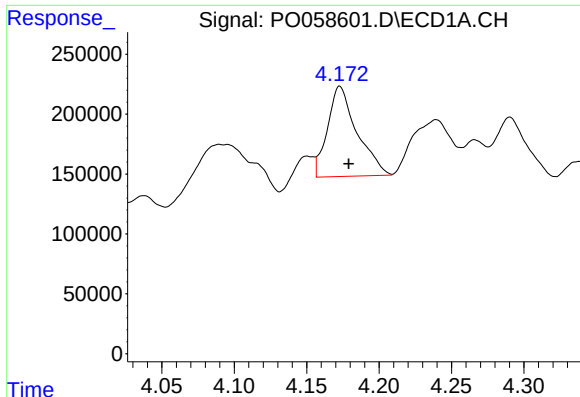


#1 Tetrachloro-m-xylene

R.T.: 4.172 min
Delta R.T.: -0.007 min
Response: 1061440
Conc: 25.15 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TANK-1


Manual Integrations
APPROVED

mohammad
8/1/2019 1:27:35 PM

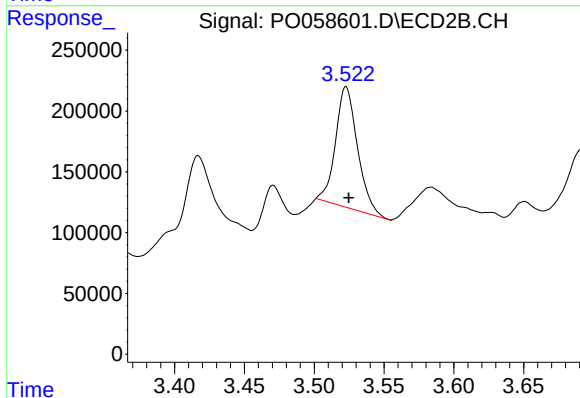


#1 Tetrachloro-m-xylene

R.T.: 3.522 min
Delta R.T.: -0.002 min
Response: 1084813
Conc: 27.15 ng/ml m

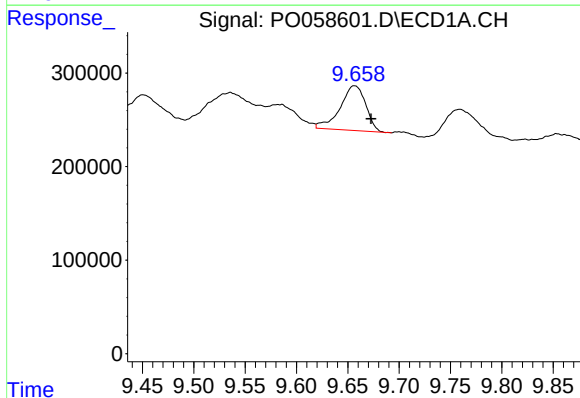

#2 Decachlorobiphenyl

R.T.: 9.657 min
Delta R.T.: -0.016 min
Response: 831120
Conc: 15.35 ng/ml

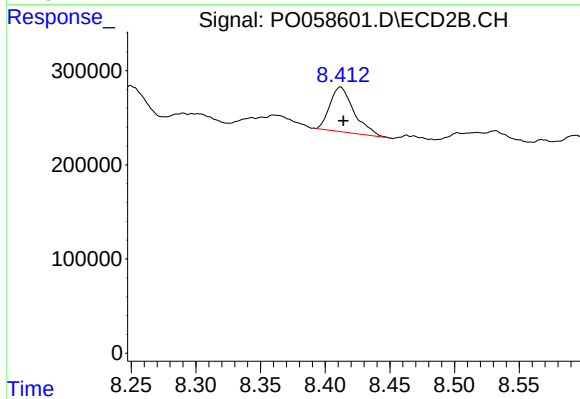

#2 Decachlorobiphenyl

R.T.: 8.412 min
Delta R.T.: -0.002 min
Response: 613924
Conc: 15.55 ng/ml m