

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0073119\
 Data File : P0058638.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Jul 2019 23:45
 Operator : SM/AJ
 Sample : K3622-13
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OR-03-072919-A

Manual Integrations
 APPROVED

Ankita
 7/31/2019 3:36:58 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 31 05:27:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jul 27 06:49:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.171	3.521	1122188	1034124	26.590m	25.885
2) SA Decachlor...	9.655	8.409	1190468	824942	21.982	20.899

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0073119\
Data File : P0058638.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Jul 2019 23:45
Operator : SM/AJ
Sample : K3622-13
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OR-03-072919-A


Manual Integrations
APPROVED

Ankita
7/31/2019 3:36:58 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 31 05:27:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 27 06:49:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

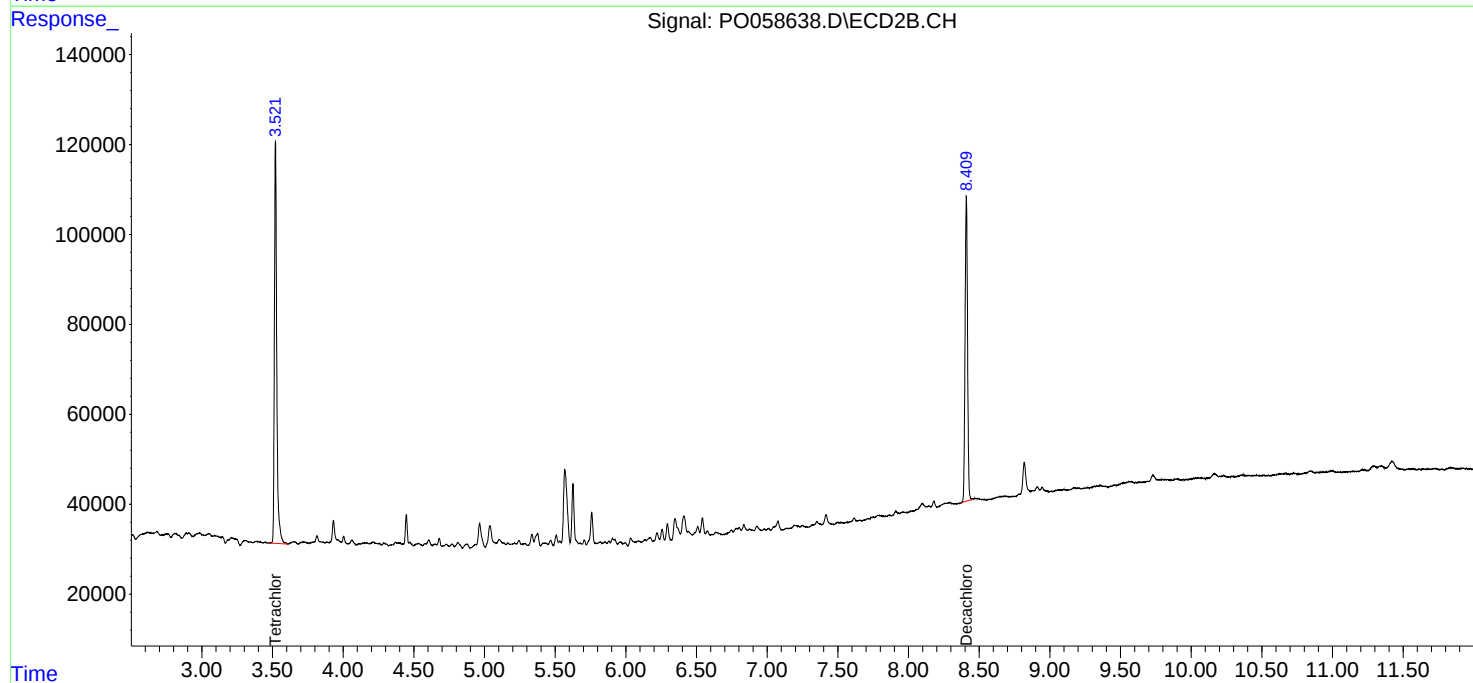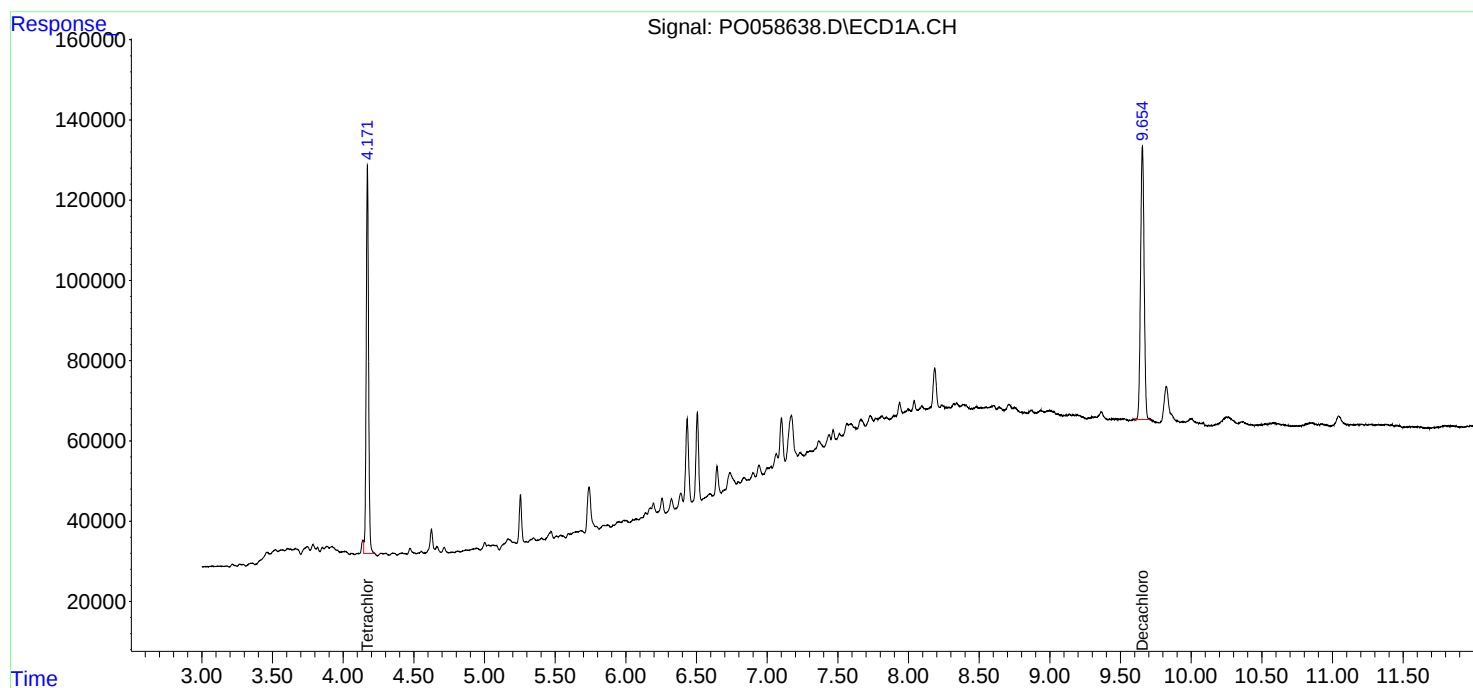

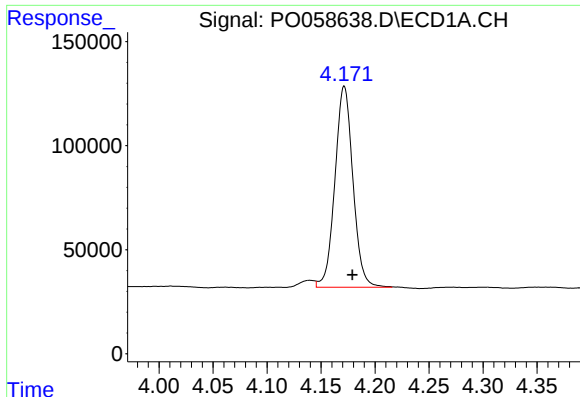


#1 Tetrachloro-m-xylene

R.T.: 4.171 min
Delta R.T.: -0.008 min
Response: 1122188
Conc: 26.59 ng/ml m

Instrument :
ECD_O
ClientSampleId :
OR-03-072919-A


Manual Integrations
APPROVED

Ankita
7/31/2019 3:36:58 PM

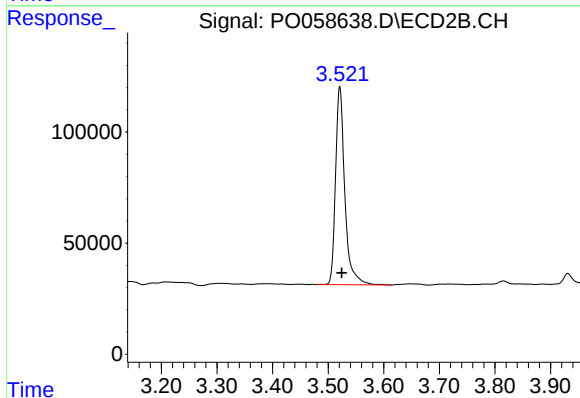


#1 Tetrachloro-m-xylene

R.T.: 3.521 min
Delta R.T.: -0.004 min
Response: 1034124
Conc: 25.89 ng/ml

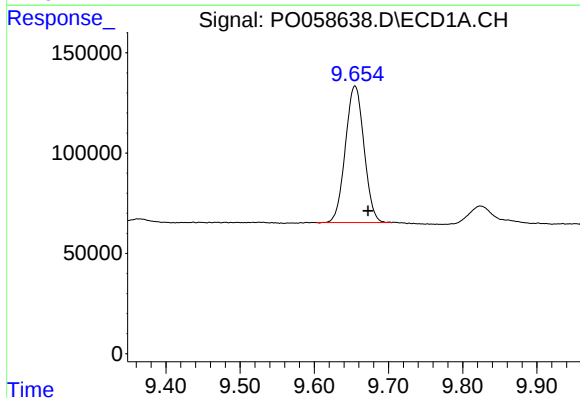

#2 Decachlorobiphenyl

R.T.: 9.655 min
Delta R.T.: -0.018 min
Response: 1190468
Conc: 21.98 ng/ml

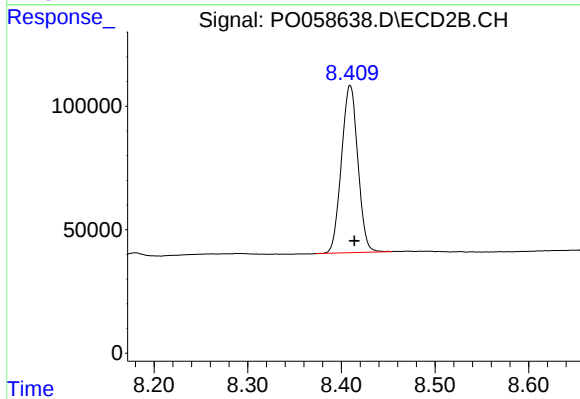

#2 Decachlorobiphenyl

R.T.: 8.409 min
Delta R.T.: -0.005 min
Response: 824942
Conc: 20.90 ng/ml