

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0073120\
 Data File : P0070230.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Jul 2020 10:09
 Operator : DD\AJ
 Sample : L3478-01RE
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ROLLOFF-VNJ-213RE

Manual Integrations
 APPROVED

Ankita
 8/3/2020 12:12:03 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 31 14:01:13 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0073020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 30 06:42:22 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.390	3.580f	945526	1045256	20.485m	25.015m
2) SA Decachlor...	10.009	8.751	1800028	3300099	27.840	53.293m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO073120\
Data File : PO070230.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Jul 2020 10:09
Operator : DD\AJ
Sample : L3478-01RE
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
ROLLOFF-VNJ-213RE


Manual Integrations
APPROVED

Ankita
8/3/2020 12:12:03 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 31 14:01:13 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO073020.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 30 06:42:22 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

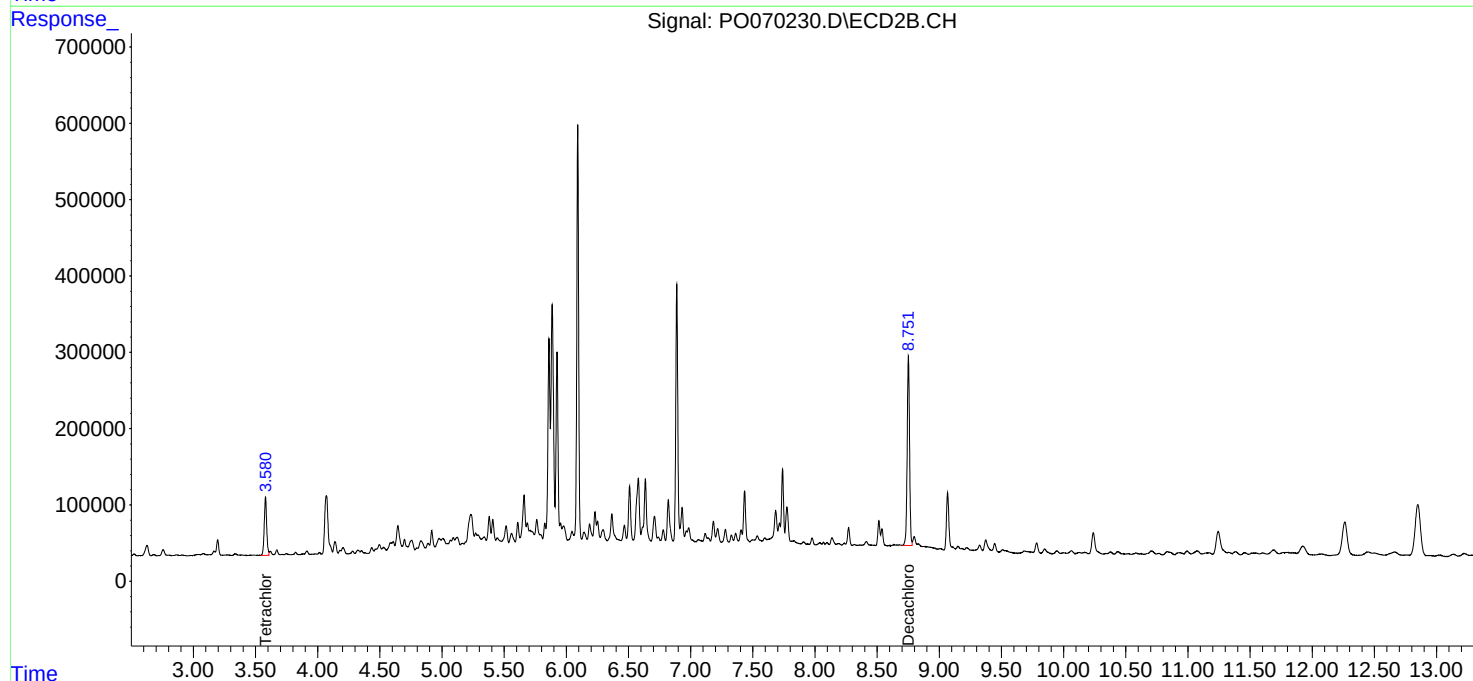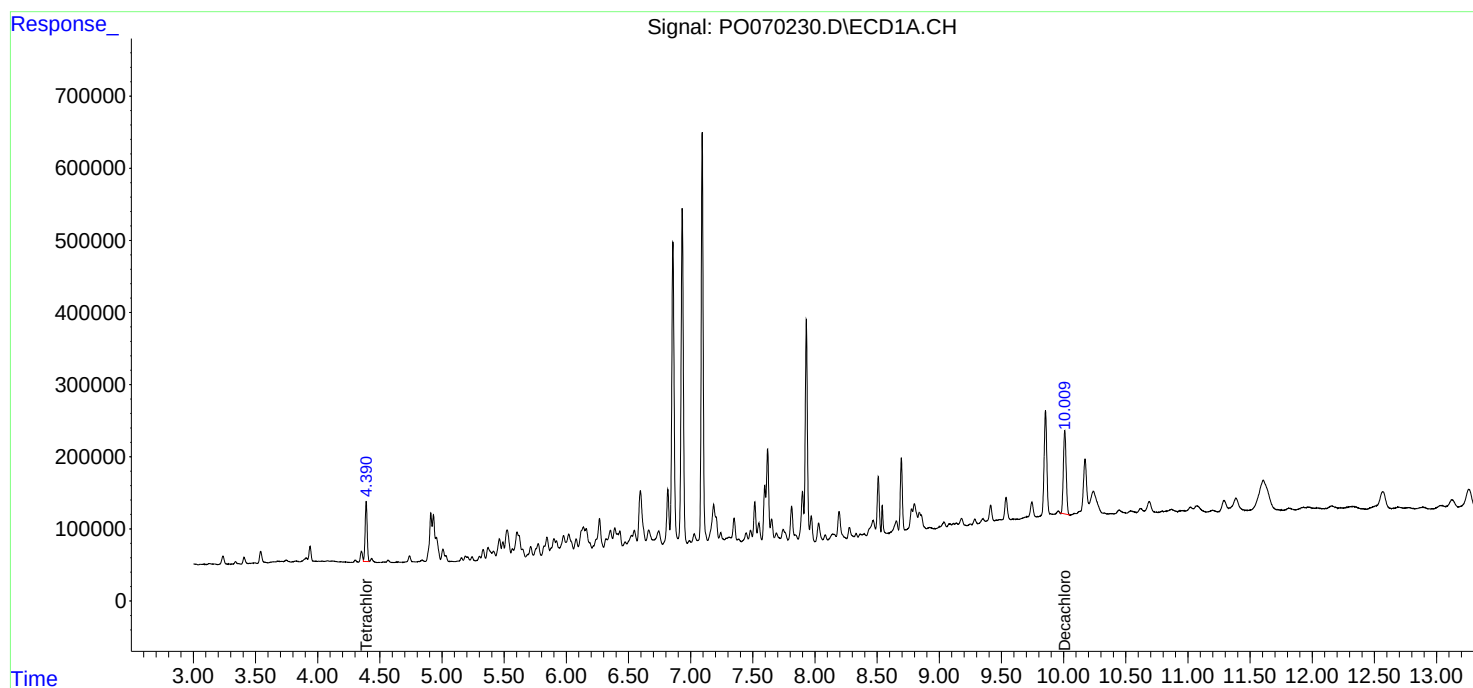

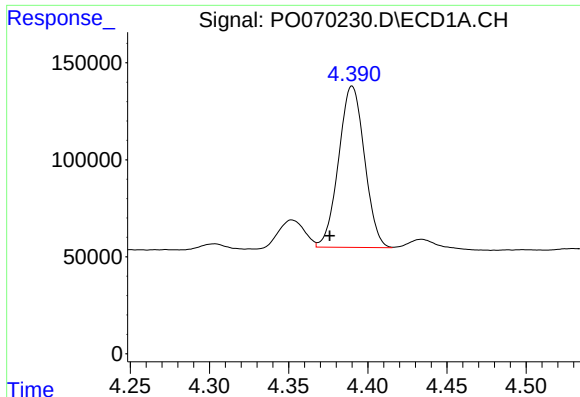


#1 Tetrachloro-m-xylene

R.T.: 4.390 min
Delta R.T.: 0.014 min
Response: 945526
Conc: 20.49 ng/ml m

Instrument :
ECD_O
ClientSampleId :
ROLLOFF-VNJ-213RE


Manual Integrations
APPROVED

Ankita
8/3/2020 12:12:03 PM

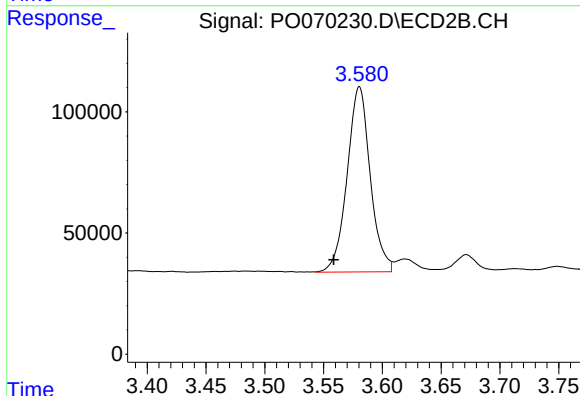


#1 Tetrachloro-m-xylene

R.T.: 3.580 min
Delta R.T.: 0.021 min
Response: 1045256
Conc: 25.02 ng/ml m

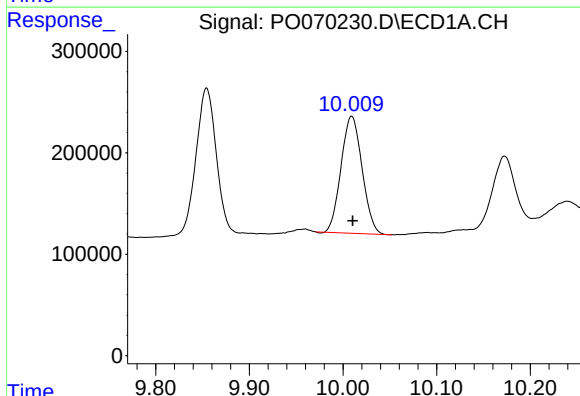

#2 Decachlorobiphenyl

R.T.: 10.009 min
Delta R.T.: 0.000 min
Response: 1800028
Conc: 27.84 ng/ml

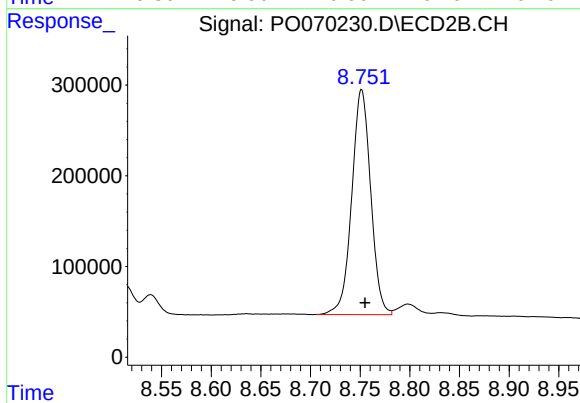

#2 Decachlorobiphenyl

R.T.: 8.751 min
Delta R.T.: -0.004 min
Response: 3300099
Conc: 53.29 ng/ml m