

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0073120\
 Data File : P0070240.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Jul 2020 13:46
 Operator : DD\AJ
 Sample : L3511-17
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SP

Manual Integrations
 APPROVED

Ankita
 8/3/2020 12:12:08 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 31 14:31:30 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0073020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 30 06:42:22 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.374	3.557	1041042	976515	22.555	23.370
2) SA Decachlor...	10.009	8.753	1389373	1249772	21.488	20.182
Target Compounds						
31) L7 AR-1260-1	7.338	6.352	344916	364249	108.823	115.760
32) L7 AR-1260-2	7.606	6.552	498145	431653	111.275m	103.909
33) L7 AR-1260-3	7.963	6.699	250340	371689	66.946	105.379 #
34) L7 AR-1260-4	8.189	7.177	298076	242518	84.497	79.642
35) L7 AR-1260-5	8.505	7.428	501856	480859	60.002	59.253

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0073120\
Data File : P0070240.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Jul 2020 13:46
Operator : DD\AJ
Sample : L3511-17
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
SP


Manual Integrations
APPROVED

Ankita
8/3/2020 12:12:08 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 31 14:31:30 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0073020.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 30 06:42:22 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

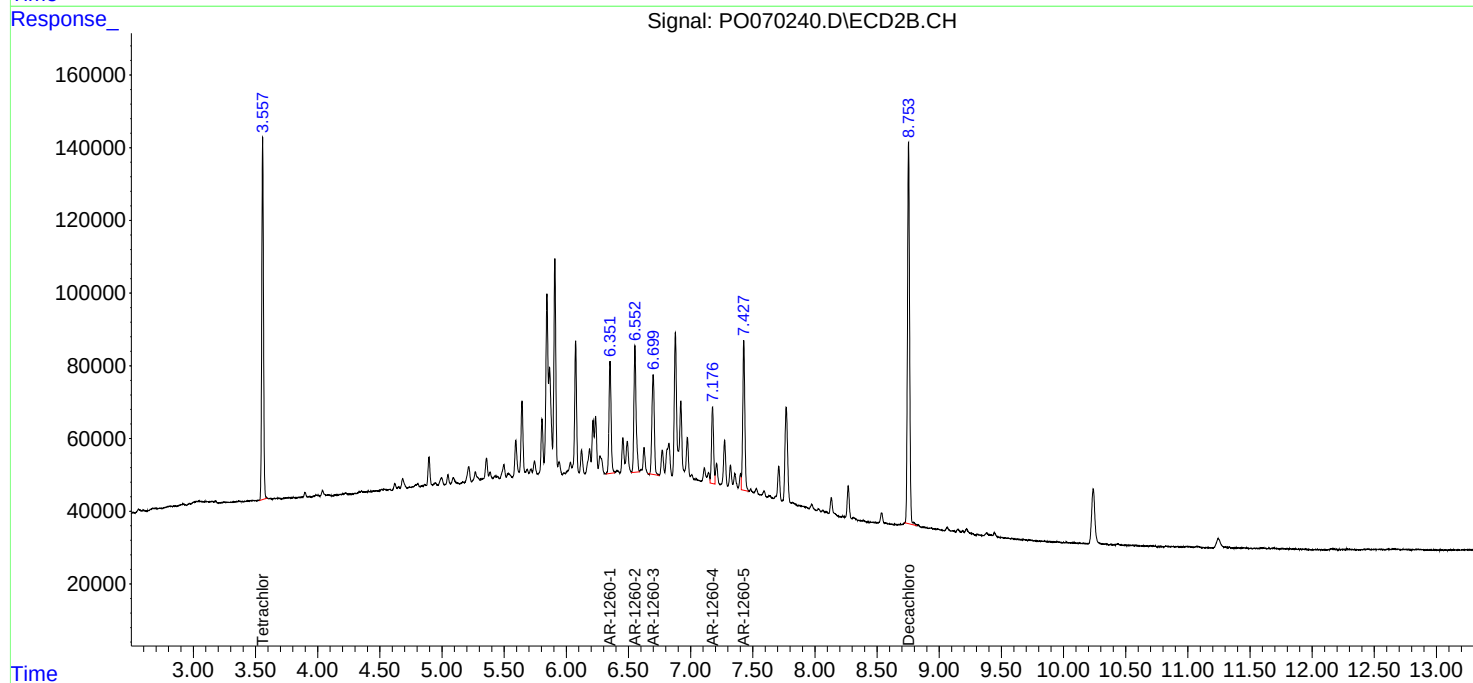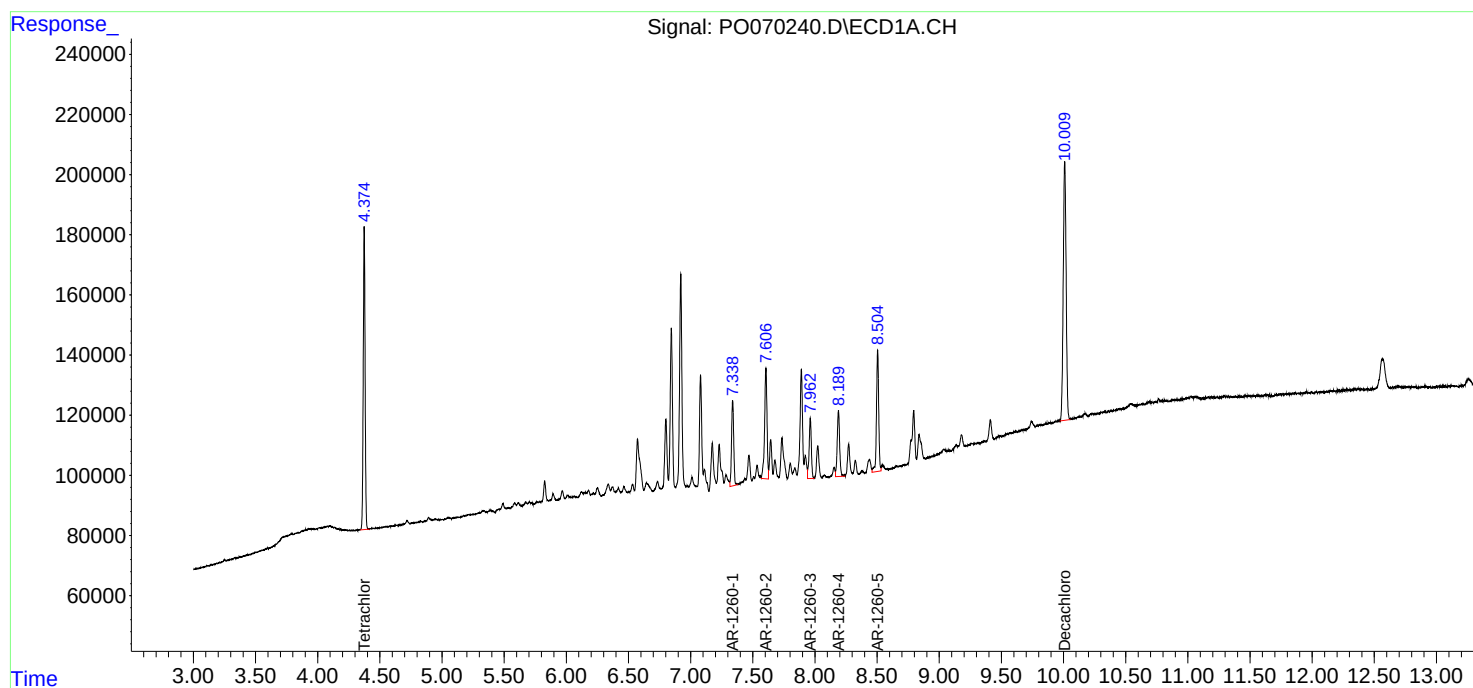

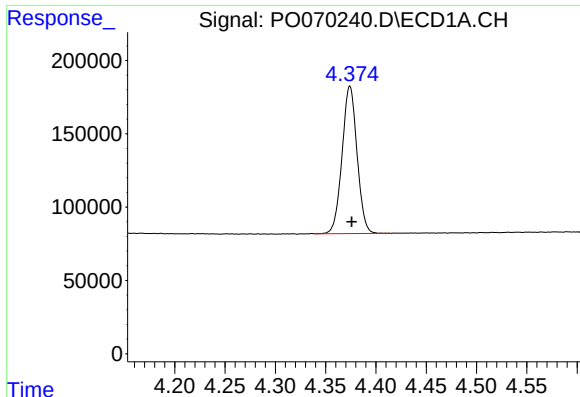


#1 Tetrachloro-m-xylene

R.T.: 4.374 min
Delta R.T.: -0.002 min
Response: 1041042
Conc: 22.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
SP


Manual Integrations
APPROVED

Ankita
8/3/2020 12:12:08 PM

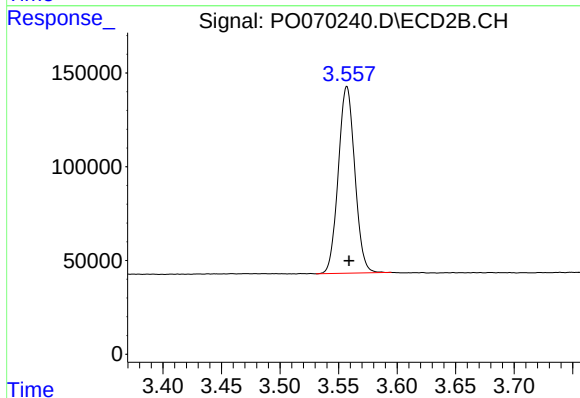


#1 Tetrachloro-m-xylene

R.T.: 3.557 min
Delta R.T.: -0.002 min
Response: 976515
Conc: 23.37 ng/ml

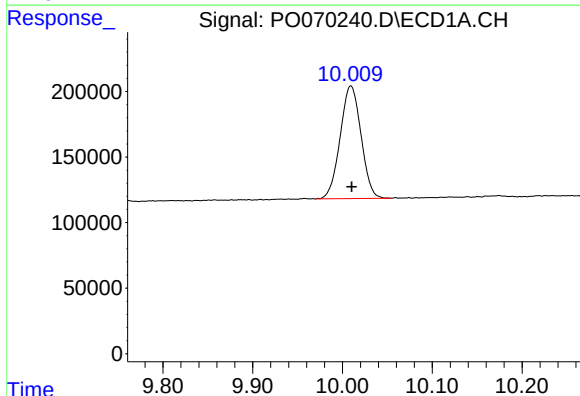


#2 Decachlorobiphenyl

R.T.: 10.009 min
Delta R.T.: 0.000 min
Response: 1389373
Conc: 21.49 ng/ml

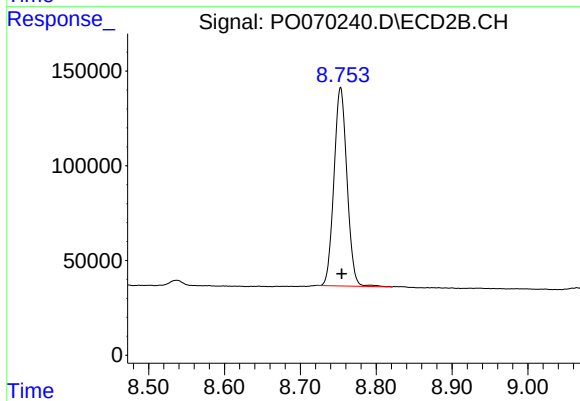

#2 Decachlorobiphenyl

R.T.: 8.753 min
Delta R.T.: -0.002 min
Response: 1249772
Conc: 20.18 ng/ml

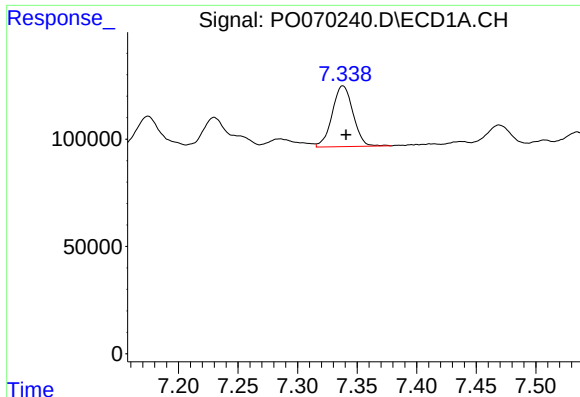


#31 AR-1260-1

R.T.: 7.338 min
Delta R.T.: -0.003 min
Response: 344916
Conc: 108.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
SP


Manual Integrations
APPROVED

Ankita
8/3/2020 12:12:08 PM

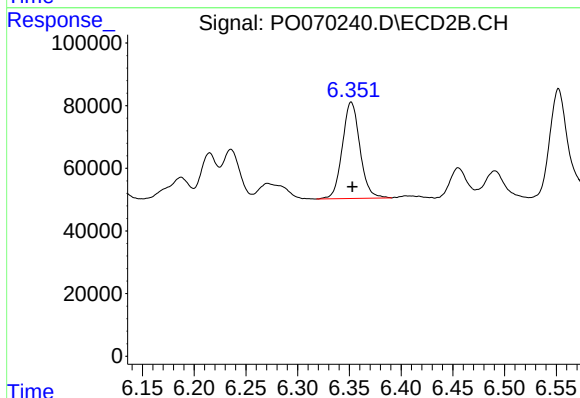


#31 AR-1260-1

R.T.: 6.352 min
Delta R.T.: -0.001 min
Response: 364249
Conc: 115.76 ng/ml

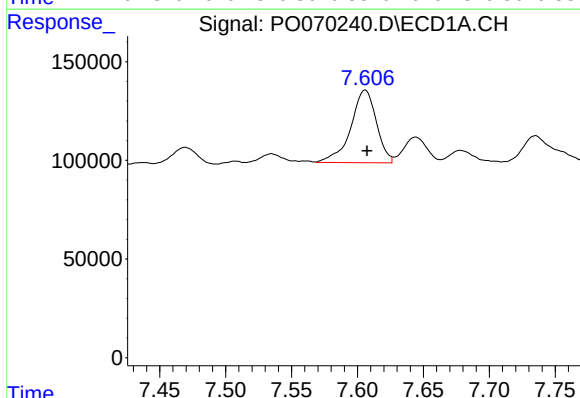


#32 AR-1260-2

R.T.: 7.606 min
Delta R.T.: -0.002 min
Response: 498145
Conc: 111.28 ng/ml m

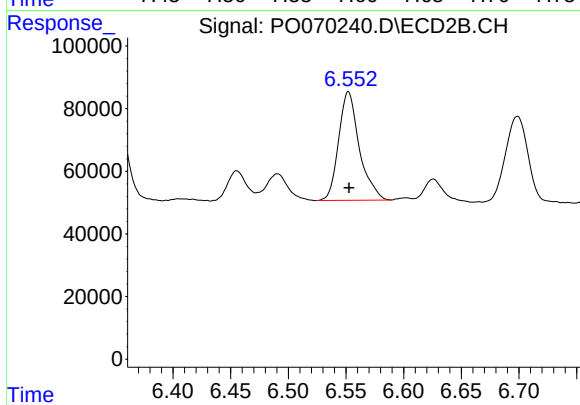

#32 AR-1260-2

R.T.: 6.552 min
Delta R.T.: 0.000 min
Response: 431653
Conc: 103.91 ng/ml

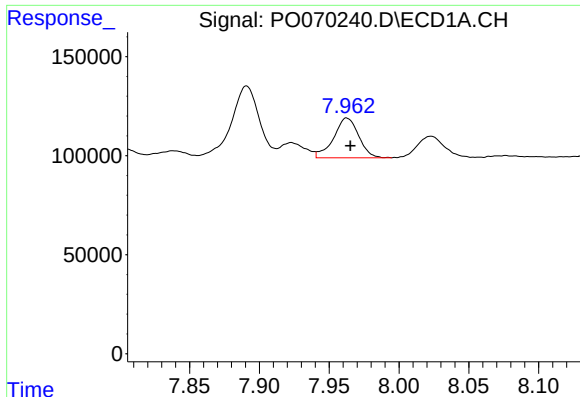


#33 AR-1260-3

R.T.: 7.963 min
Delta R.T.: -0.003 min
Response: 250340
Conc: 66.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
SP


Manual Integrations
APPROVED

Ankita
8/3/2020 12:12:08 PM

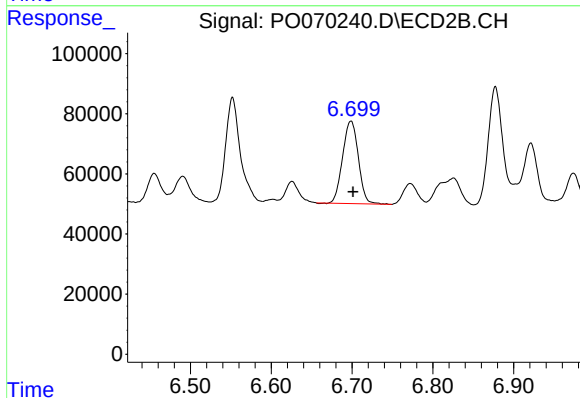


#33 AR-1260-3

R.T.: 6.699 min
Delta R.T.: -0.002 min
Response: 371689
Conc: 105.38 ng/ml

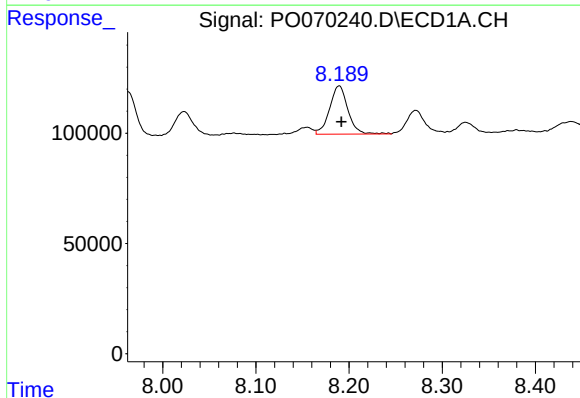


#34 AR-1260-4

R.T.: 8.189 min
Delta R.T.: -0.003 min
Response: 298076
Conc: 84.50 ng/ml

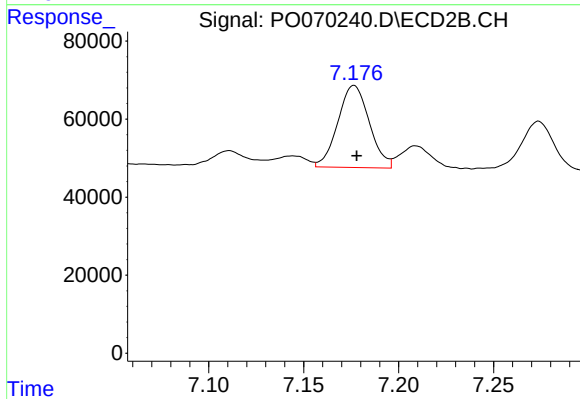

#34 AR-1260-4

R.T.: 7.177 min
Delta R.T.: -0.001 min
Response: 242518
Conc: 79.64 ng/ml

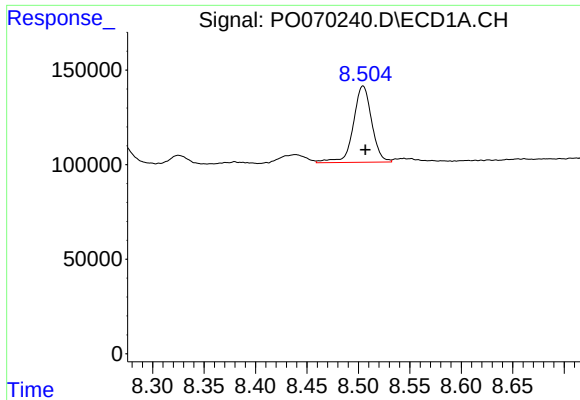


#35 AR-1260-5

R.T.: 8.505 min
Delta R.T.: -0.002 min
Response: 501856
Conc: 60.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
SP

Manual Integrations
APPROVED

Ankita
8/3/2020 12:12:08 PM

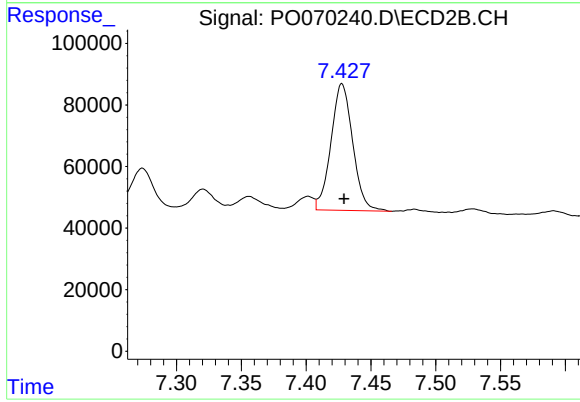

#35 AR-1260-5

R.T.: 7.428 min
Delta R.T.: -0.002 min
Response: 480859
Conc: 59.25 ng/ml