

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0073120\
 Data File : P0070249.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Jul 2020 17:45
 Operator : DD\AJ
 Sample : L3482-07 5X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 JEB403X-END-1

Manual Integrations
 APPROVED

Ankita
 8/3/2020 12:12:14 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 01:54:23 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0073020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 30 06:42:22 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.374	3.557	124472	145344	2.697m	3.478m#
2) SA Decachlor...	10.010	8.754	186368	177902	2.882	2.873

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0073120\
Data File : P0070249.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Jul 2020 17:45
Operator : DD\AJ
Sample : L3482-07 5X
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
JEB403X-END-1


Manual Integrations
APPROVED

Ankita
8/3/2020 12:12:14 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 01:54:23 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0073020.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 30 06:42:22 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

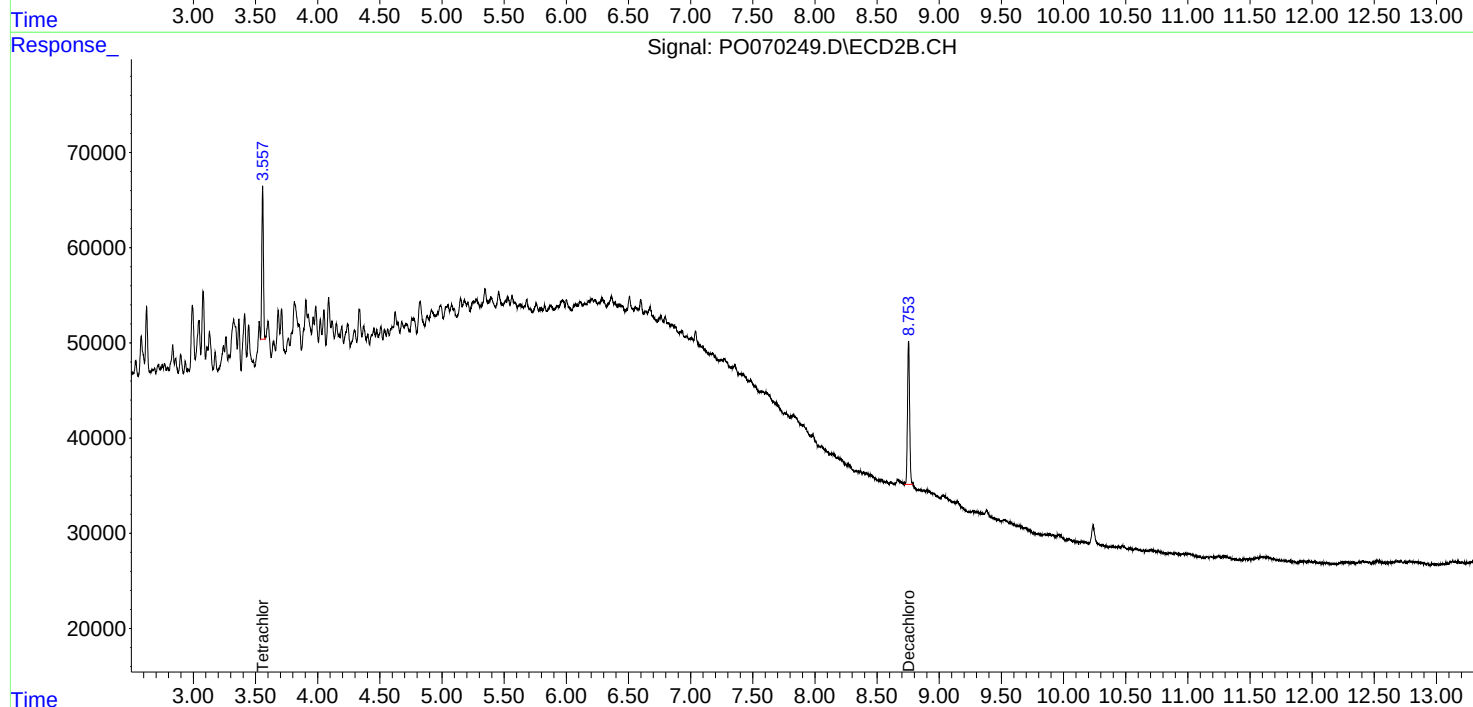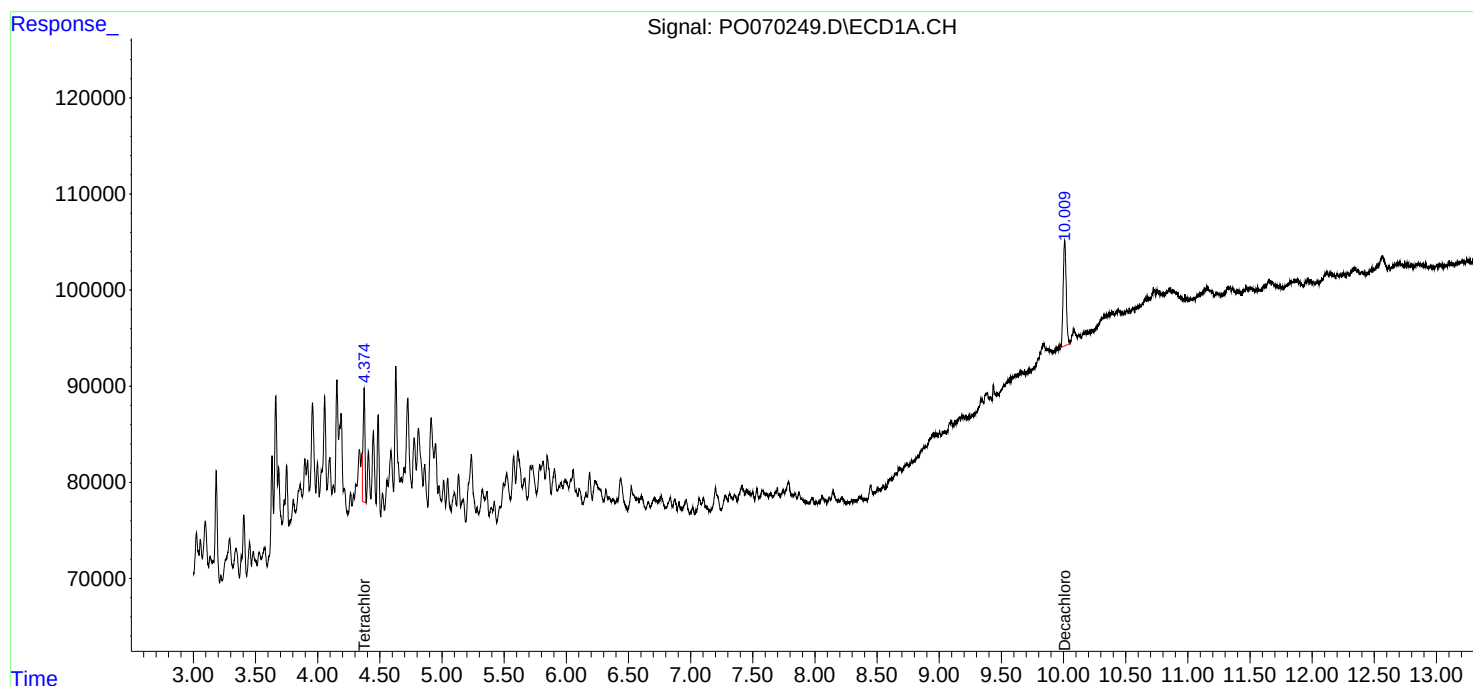

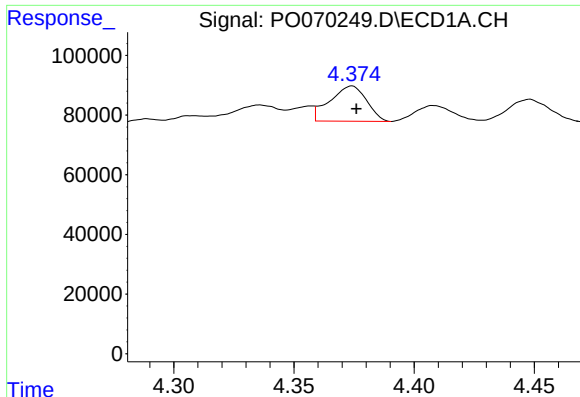


#1 Tetrachloro-m-xylene

R.T.: 4.374 min
Delta R.T.: -0.002 min
Response: 124472
Conc: 2.70 ng/ml m

Instrument :
ECD_O
ClientSampleId :
JEB403X-END-1


Manual Integrations
APPROVED

Ankita
8/3/2020 12:12:14 PM

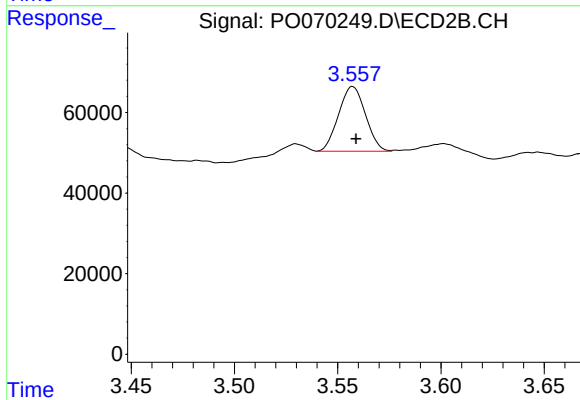


#1 Tetrachloro-m-xylene

R.T.: 3.557 min
Delta R.T.: -0.002 min
Response: 145344
Conc: 3.48 ng/ml m

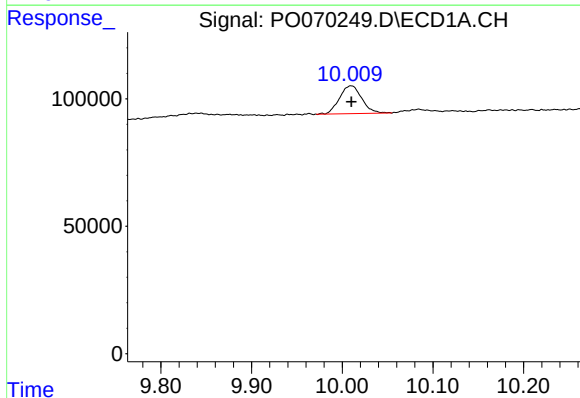

#2 Decachlorobiphenyl

R.T.: 10.010 min
Delta R.T.: 0.000 min
Response: 186368
Conc: 2.88 ng/ml

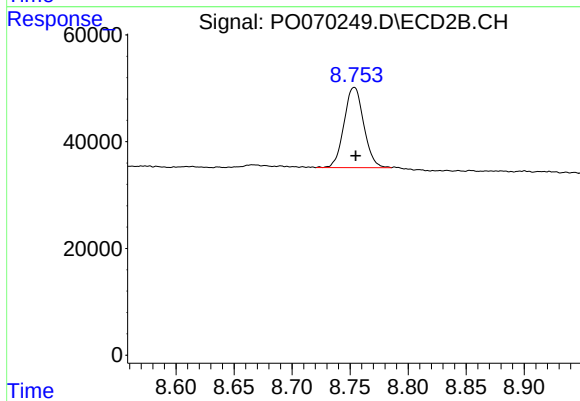

#2 Decachlorobiphenyl

R.T.: 8.754 min
Delta R.T.: -0.001 min
Response: 177902
Conc: 2.87 ng/ml