

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0073123\
 Data File : P0096515.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jul 2023 18:06
 Operator : YP/AJ
 Sample : 03800-06
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 295B-LEAD-PAINT-CHIPS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 04:04:07 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jul 28 01:38:03 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.416	3.625	62857056	25579562	18.813	18.058
2) SA Decachlor...	10.245	8.651	45611949	24465001	20.615	20.798

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0073123\
Data File : P0096515.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jul 2023 18:06
Operator : YP/AJ
Sample : 03800-06
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
295B-LEAD-PAINT-CHIPS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 04:04:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072723.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 28 01:38:03 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

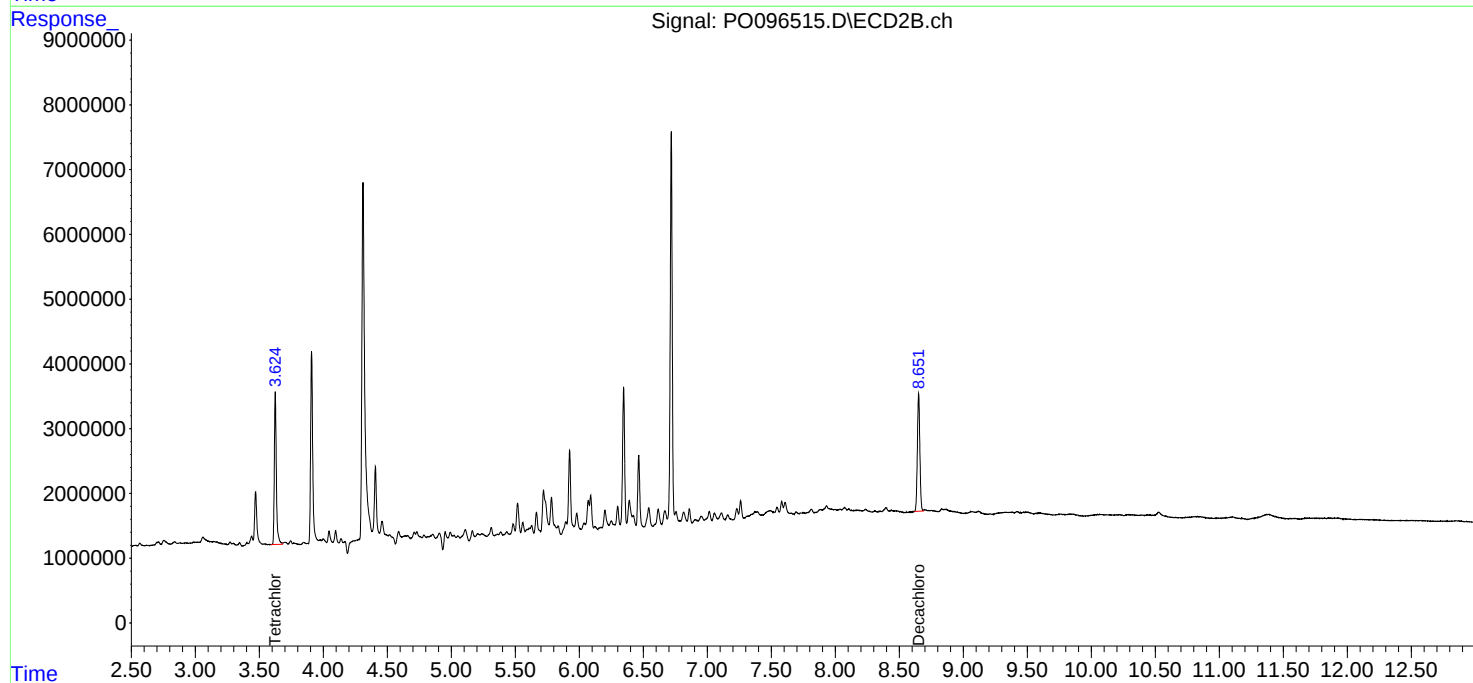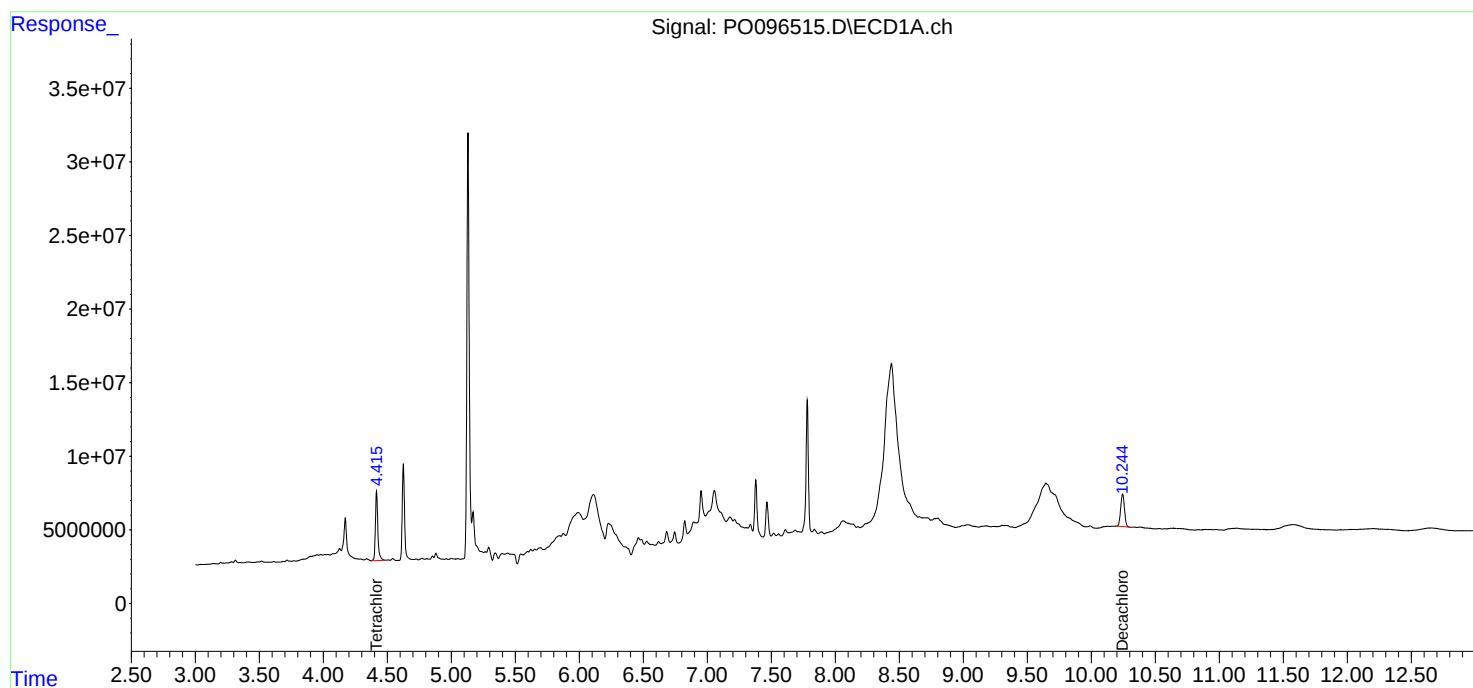


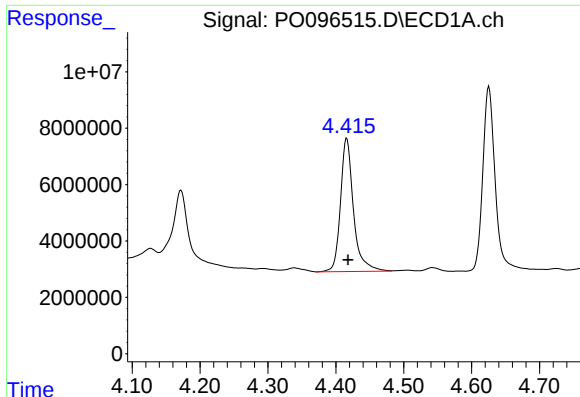

#1 Tetrachloro-m-xylene


R.T.: 4.416 min
Delta R.T.: -0.002 min
Response: 62857056
Conc: 18.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
295B-LEAD-PAINT-CHIPS

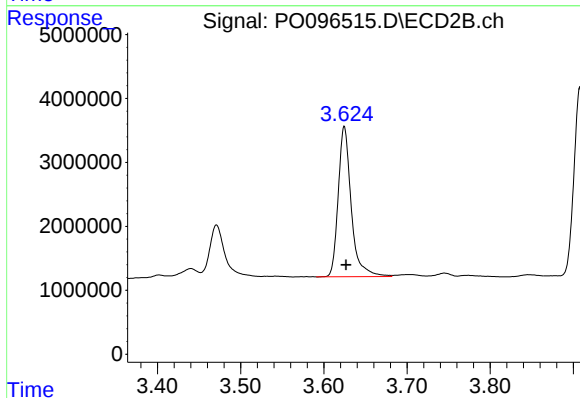


#1 Tetrachloro-m-xylene

R.T.: 3.625 min
Delta R.T.: -0.002 min
Response: 25579562
Conc: 18.06 ng/ml

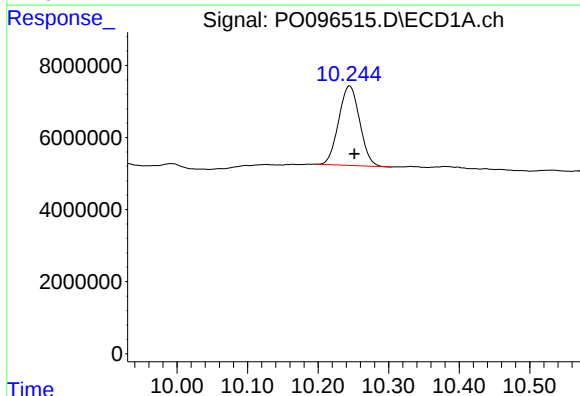

#2 Decachlorobiphenyl

R.T.: 10.245 min
Delta R.T.: -0.007 min
Response: 45611949
Conc: 20.62 ng/ml

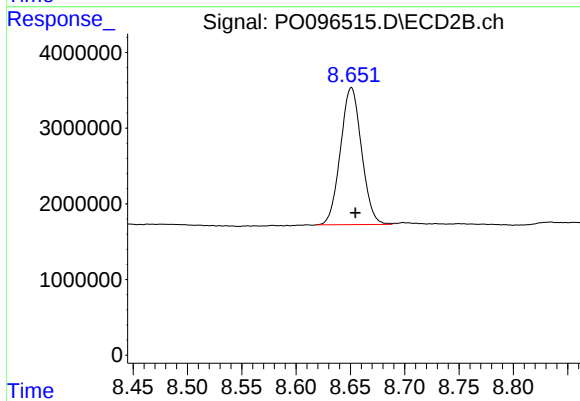

#2 Decachlorobiphenyl

R.T.: 8.651 min
Delta R.T.: -0.004 min
Response: 24465001
Conc: 20.80 ng/ml