

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0073123\
 Data File : P0096528.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jul 2023 23:12
 Operator : YP/AJ
 Sample : PB154551BL
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB154551BL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/08/2023
 Supervised By :Ankita Jodhani 08/08/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 05:48:40 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jul 28 01:38:03 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.416	3.624	58519668	24797356	17.515	17.505
2) SA Decachlor...	10.243	8.648	45502377	20537309	20.566	17.459m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0073123\
Data File : P0096528.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jul 2023 23:12
Operator : YP/AJ
Sample : PB154551BL
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PB154551BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/08/2023
Supervised By :Ankita Jodhani 08/08/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 05:48:40 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072723.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 28 01:38:03 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

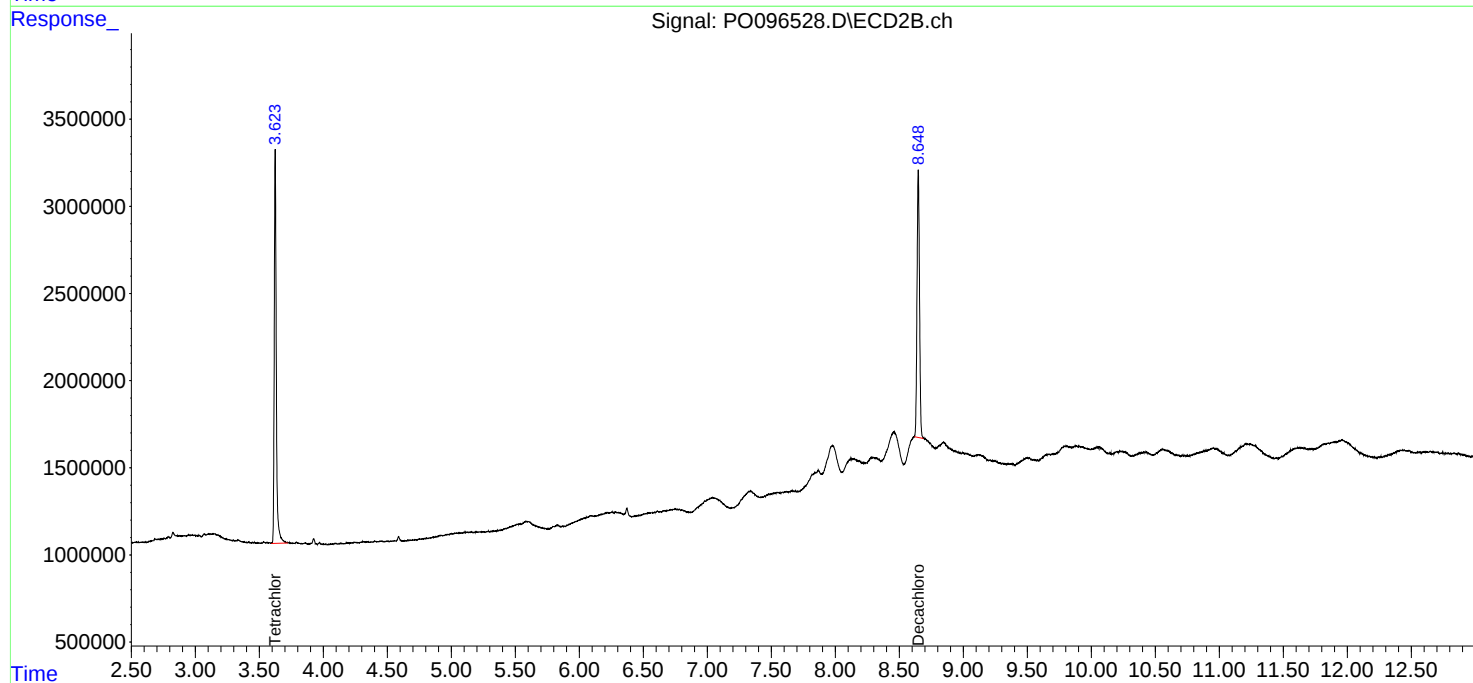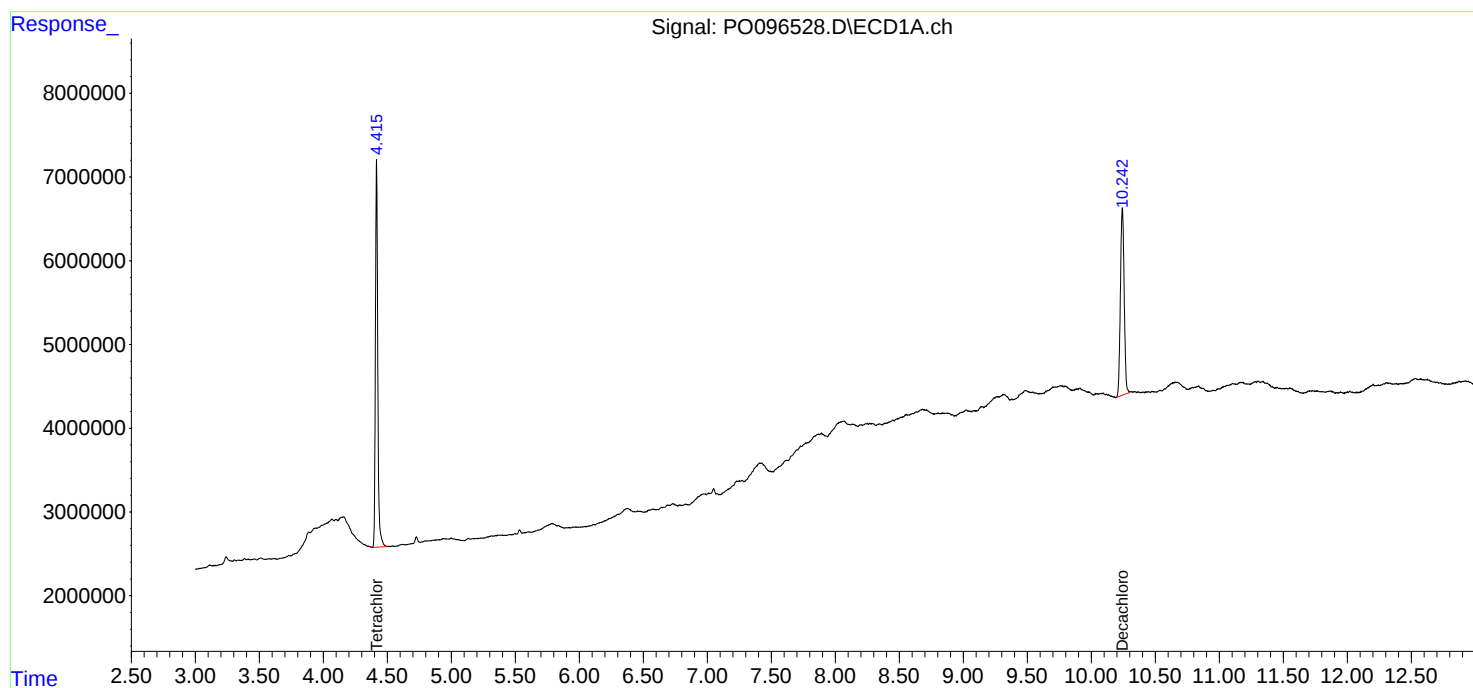

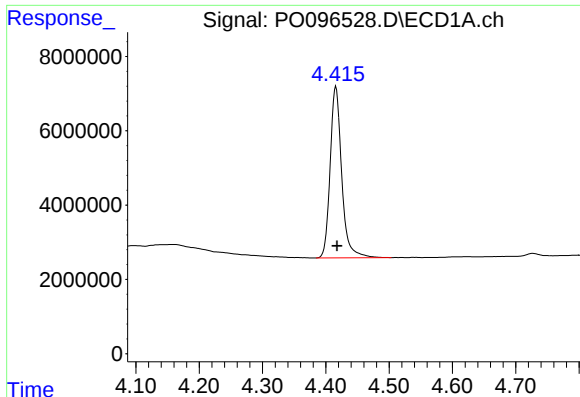


#1 Tetrachloro-m-xylene

R.T.: 4.416 min
Delta R.T.: -0.002 min
Response: 58519668
Conc: 17.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB154551BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/08/2023
Supervised By :Ankita Jodhani 08/08/2023

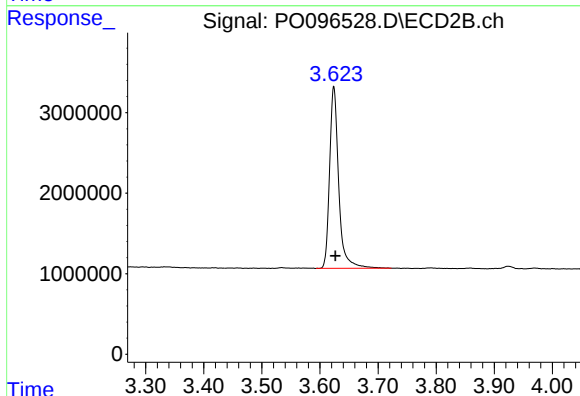


#1 Tetrachloro-m-xylene

R.T.: 3.624 min
Delta R.T.: -0.003 min
Response: 24797356
Conc: 17.51 ng/ml

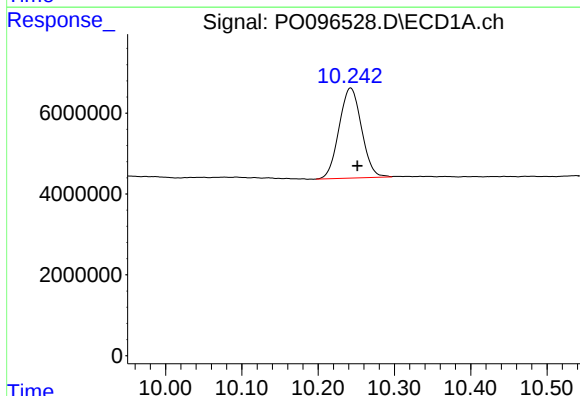

#2 Decachlorobiphenyl

R.T.: 10.243 min
Delta R.T.: -0.009 min
Response: 45502377
Conc: 20.57 ng/ml

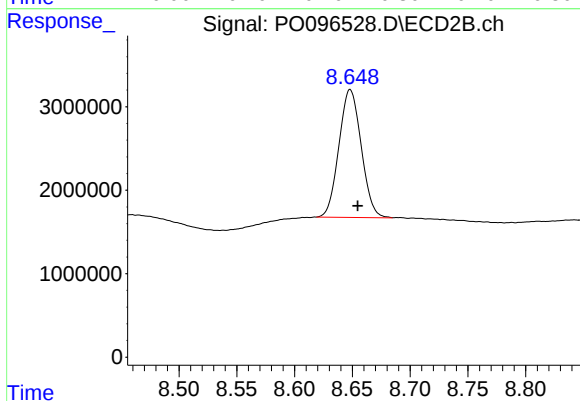

#2 Decachlorobiphenyl

R.T.: 8.648 min
Delta R.T.: -0.007 min
Response: 20537309
Conc: 17.46 ng/ml m