

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0073123\
 Data File : P0096531.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2023 00:03
 Operator : YP/AJ
 Sample : 03846-01
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SER-59AL4852

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/01/2023
 Supervised By :Ankita Jodhani 08/01/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 05:49:33 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jul 28 01:38:03 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.420	3.636	43591757	17409973	13.047m	12.290
2) SA Decachlor...	10.240	8.649	56964392	19482094	25.746	16.562 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0073123\
Data File : P0096531.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Aug 2023 00:03
Operator : YP/AJ
Sample : 03846-01
Misc :
ALS Vial : 34 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SER-59AL4852


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/01/2023
Supervised By :Ankita Jodhani 08/01/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 05:49:33 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072723.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 28 01:38:03 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

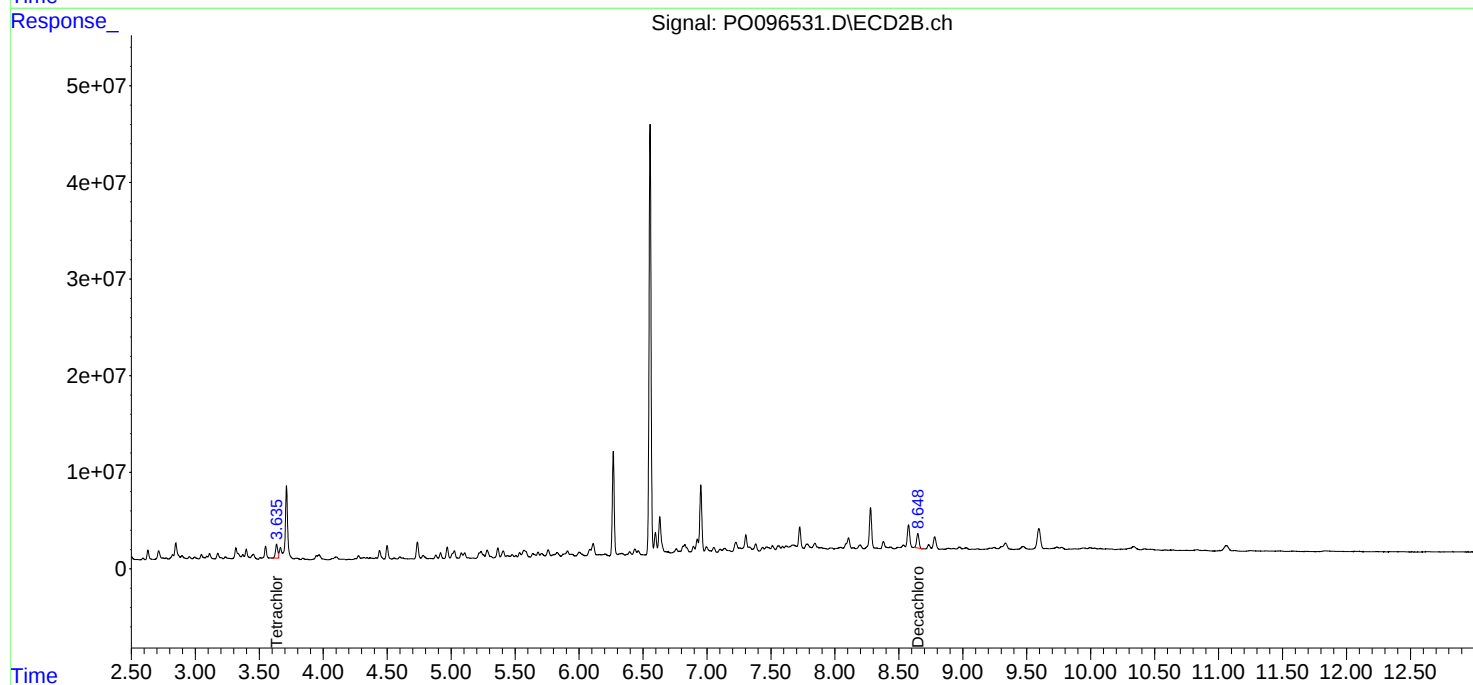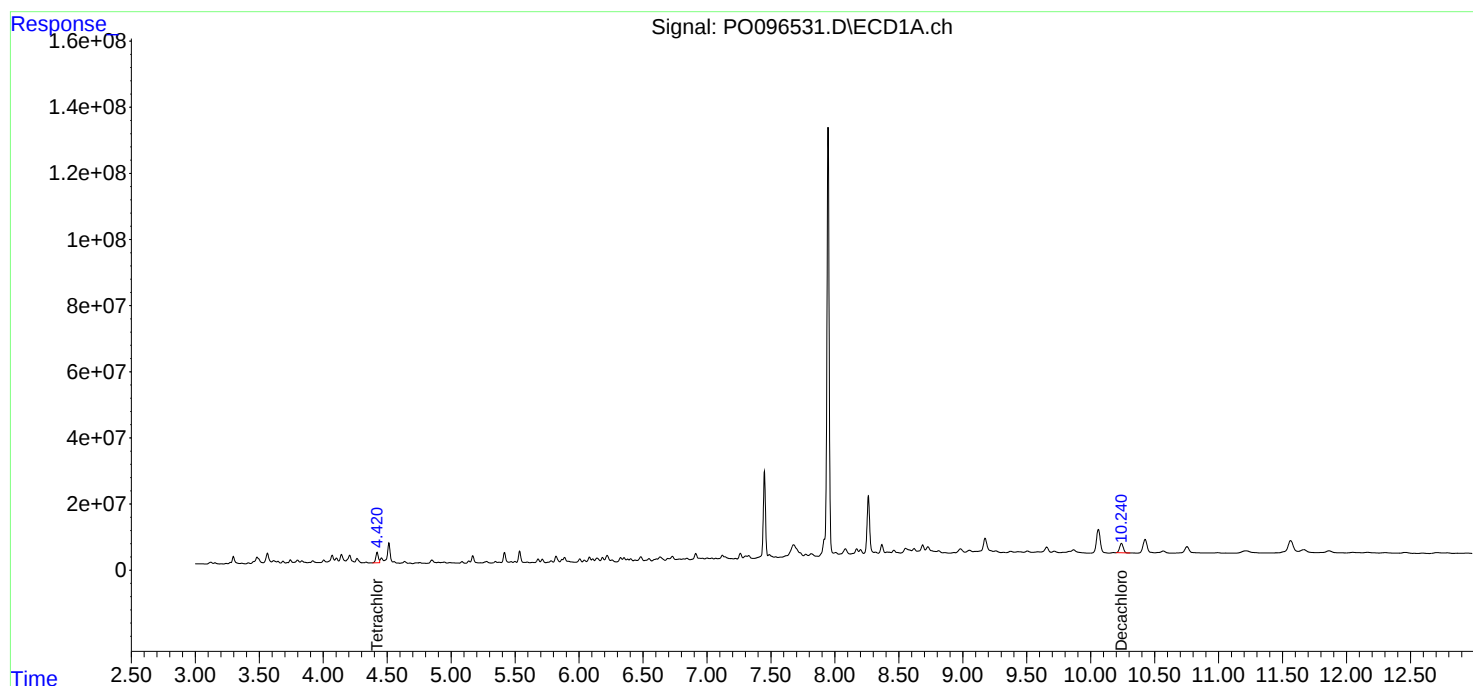

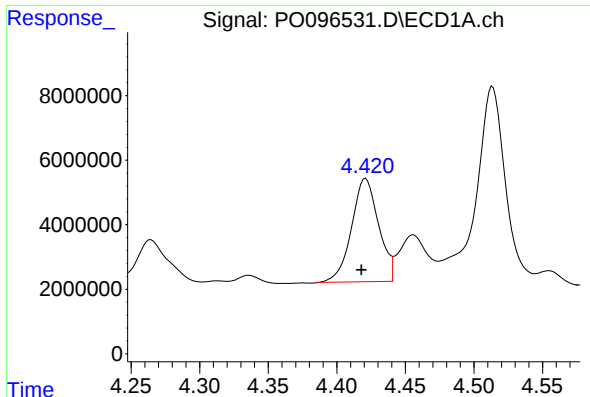

#1 Tetrachloro-m-xylene

R.T.: 4.420 min
Delta R.T.: 0.002 min
Response: 43591757
Conc: 13.05 ng/ml

Instrument :

ECD_O


ClientSampleId :

SER-59AL4852

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 08/01/2023
Supervised By :Ankita Jodhani 08/01/2023

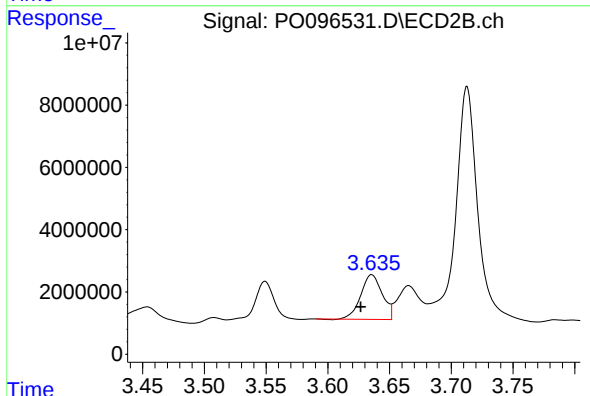


#1 Tetrachloro-m-xylene

R.T.: 3.636 min
Delta R.T.: 0.009 min
Response: 17409973
Conc: 12.29 ng/ml

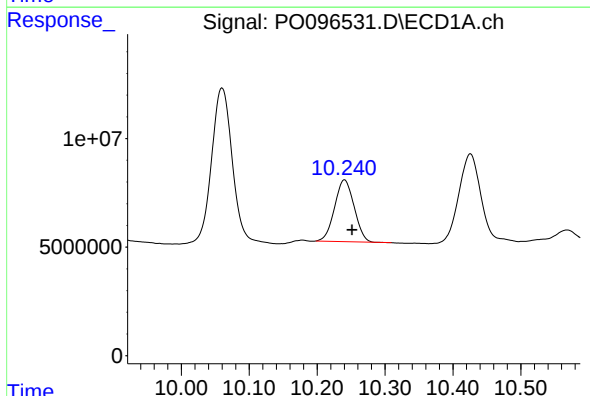

#2 Decachlorobiphenyl

R.T.: 10.240 min
Delta R.T.: -0.011 min
Response: 56964392
Conc: 25.75 ng/ml

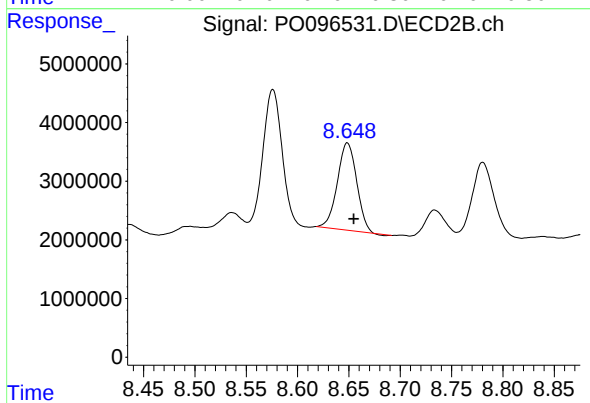

#2 Decachlorobiphenyl

R.T.: 8.649 min
Delta R.T.: -0.006 min
Response: 19482094
Conc: 16.56 ng/ml