

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0073124\
 Data File : P0105050.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jul 2024 13:41
 Operator : YP/AJ
 Sample : P3405-01 10X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 KZZ258D-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/01/2024
 Supervised By :Ankita Jodhani 08/01/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 02:02:27 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072924.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 30 07:11:20 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.429	3.541	11856363	4013485	1.722m	1.575
2) SA Decachlor...	10.226	8.437	8780402	1983619	1.710	1.249m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO073124\
Data File : PO105050.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jul 2024 13:41
Operator : YP/AJ
Sample : P3405-01 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
KZZ258D-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/01/2024
Supervised By :Ankita Jodhani 08/01/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 02:02:27 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072924.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 30 07:11:20 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

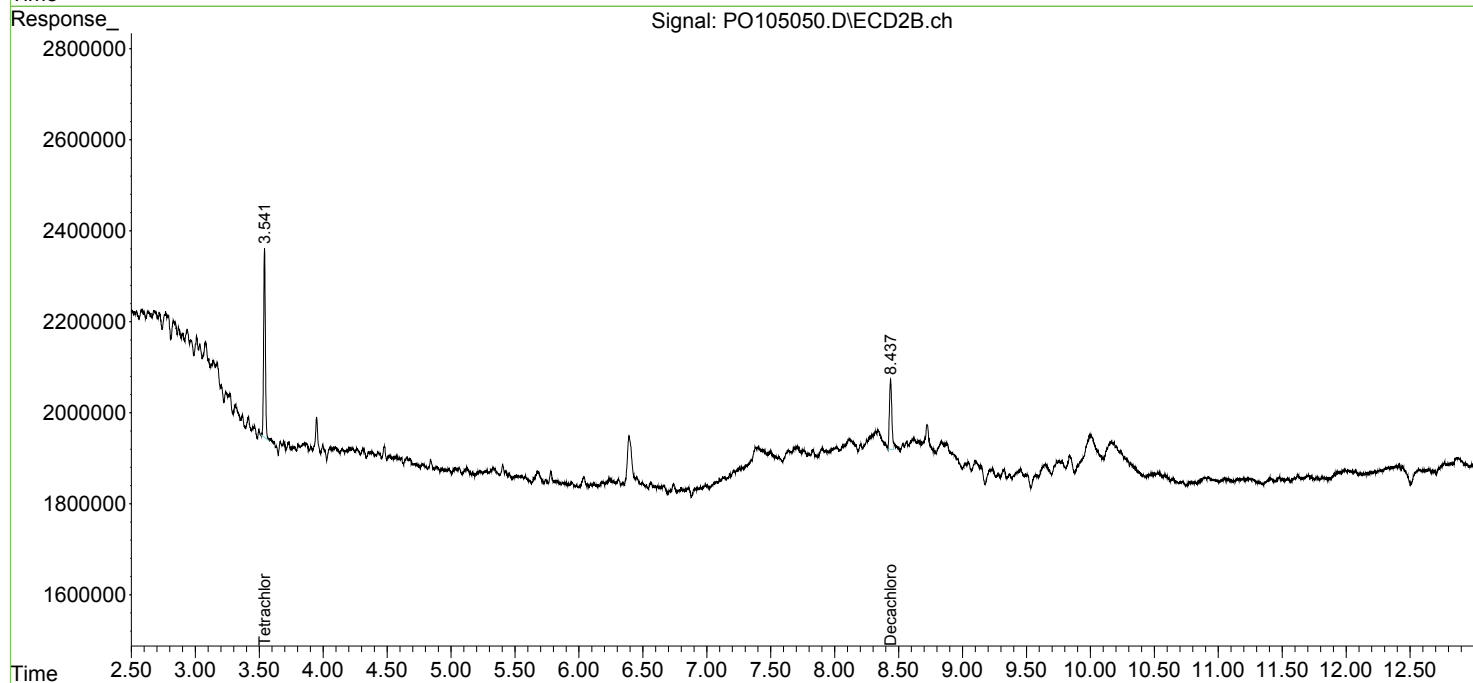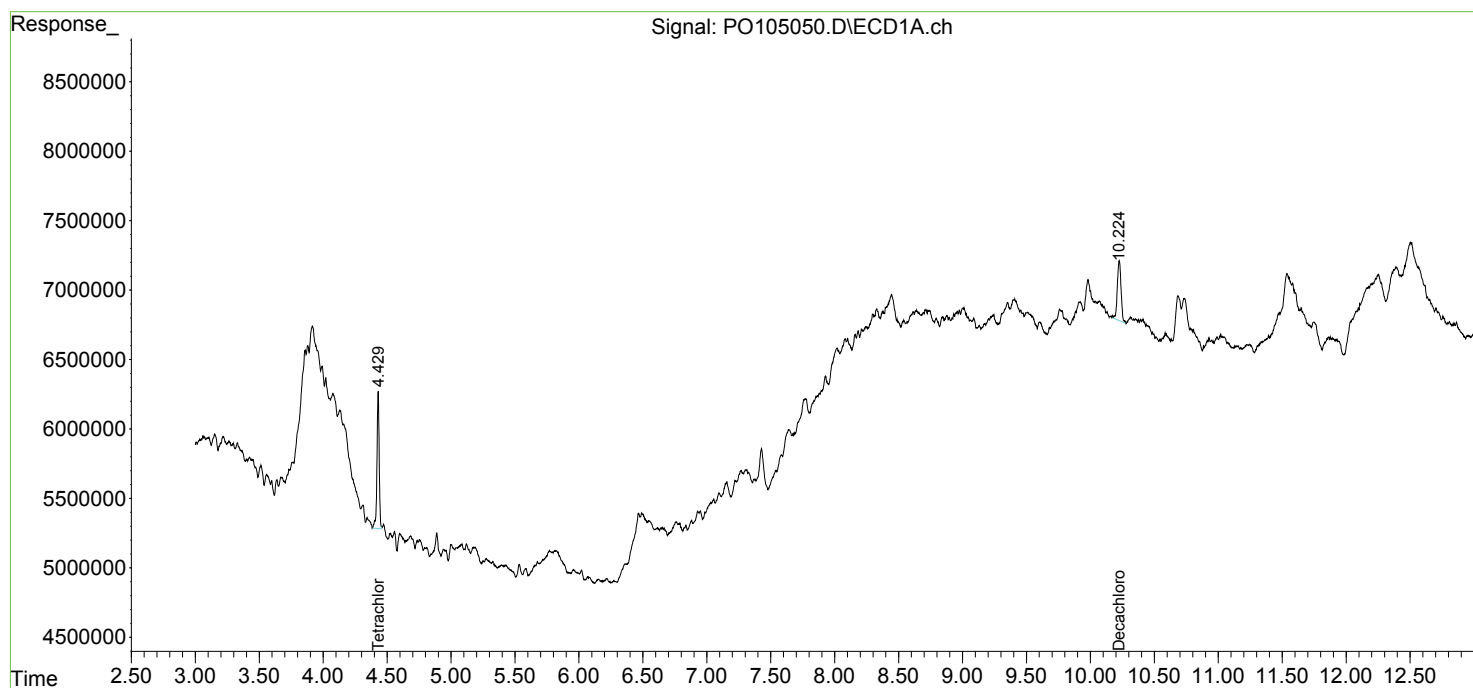

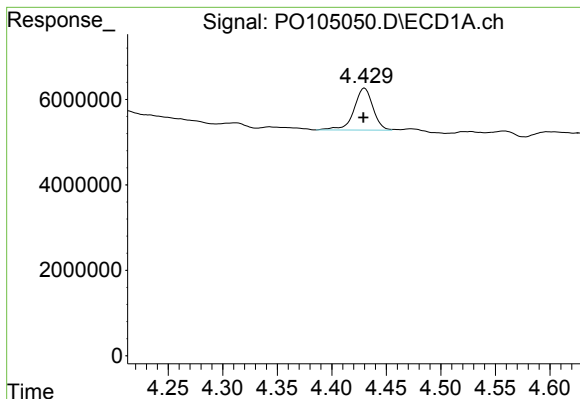


#1 Tetrachloro-m-xylene

R.T.: 4.429 min
Delta R.T.: 0.000 min
Response: 11856363
Conc: 1.72 ng/ml

Instrument :
ECD_O
ClientSampleId :
KZZ258D-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/01/2024
Supervised By :Ankita Jodhani 08/01/2024

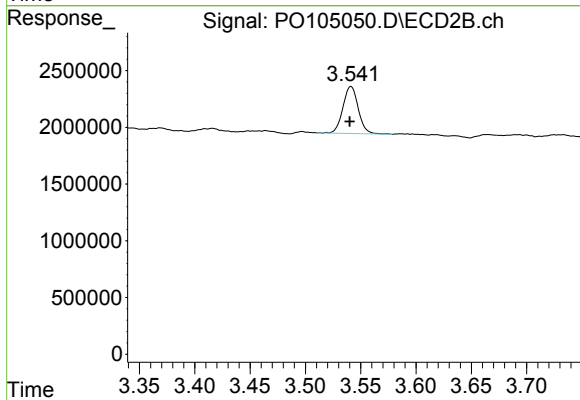


#1 Tetrachloro-m-xylene

R.T.: 3.541 min
Delta R.T.: 0.001 min
Response: 4013485
Conc: 1.58 ng/ml

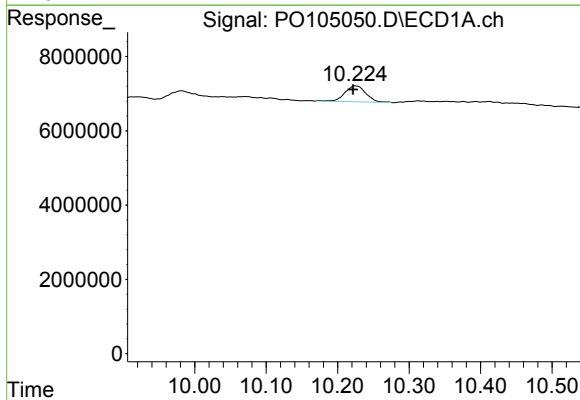

#2 Decachlorobiphenyl

R.T.: 10.226 min
Delta R.T.: 0.004 min
Response: 8780402
Conc: 1.71 ng/ml

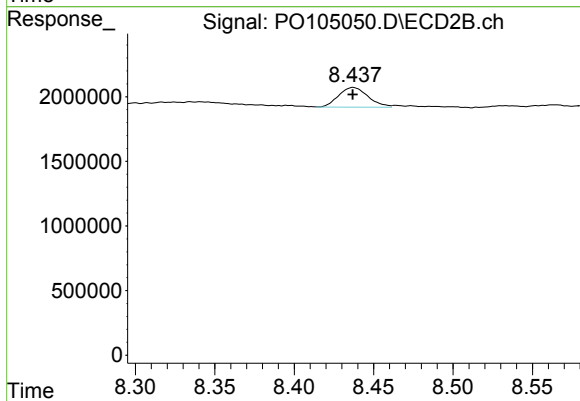

#2 Decachlorobiphenyl

R.T.: 8.437 min
Delta R.T.: 0.000 min
Response: 1983619
Conc: 1.25 ng/ml m