

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0073124\
Data File : P0105051.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jul 2024 13:59
Operator : YP/AJ
Sample : P3405-02 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
KZZ258D-1-2

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/01/2024
Supervised By :Ankita Jodhani 08/01/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 02:04:37 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072924.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 30 07:11:20 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.430	3.540	8925741	3437136	1.297	1.349
2) SA Decachlor...	10.224	8.436	6450628	2023836	1.256m	1.274

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO073124\
Data File : PO105051.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jul 2024 13:59
Operator : YP/AJ
Sample : P3405-02 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
KZZ258D-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/01/2024
Supervised By :Ankita Jodhani 08/01/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 02:04:37 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072924.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 30 07:11:20 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

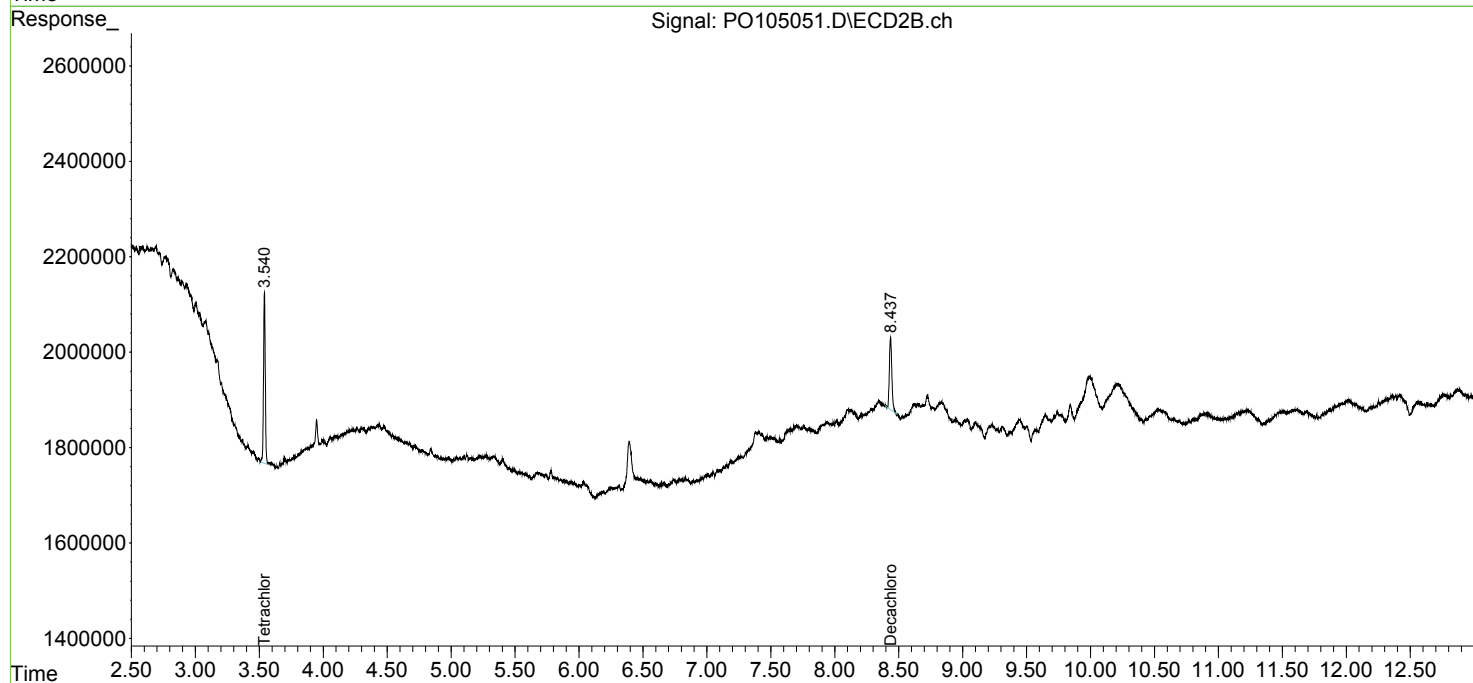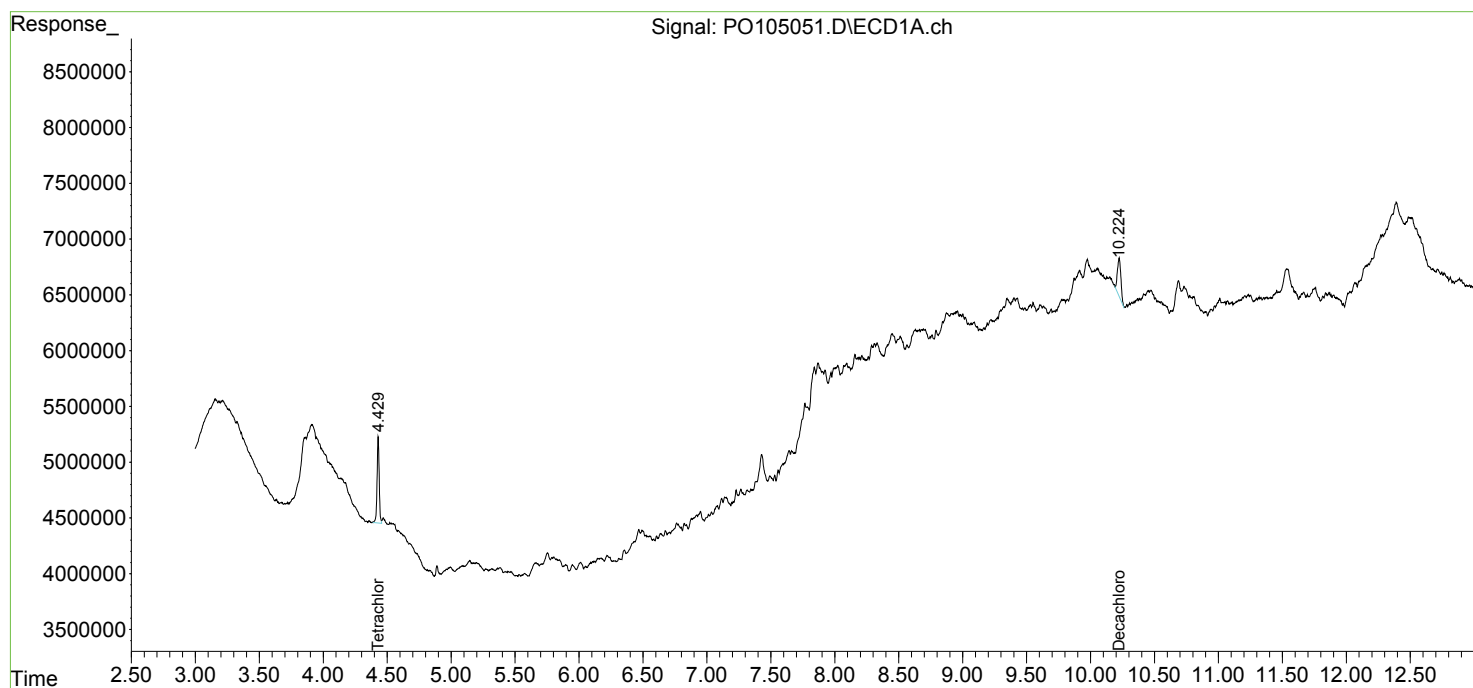

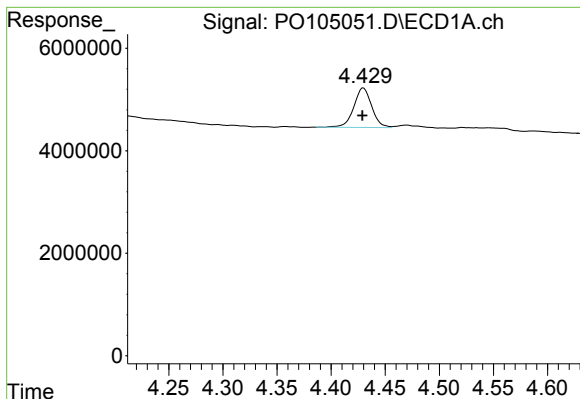


#1 Tetrachloro-m-xylene

R.T.: 4.430 min
Delta R.T.: 0.000 min
Response: 8925741
Conc: 1.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
KZZ258D-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/01/2024
Supervised By :Ankita Jodhani 08/01/2024

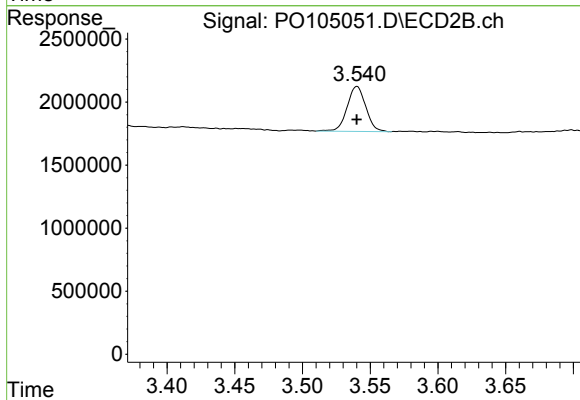


#1 Tetrachloro-m-xylene

R.T.: 3.540 min
Delta R.T.: 0.000 min
Response: 3437136
Conc: 1.35 ng/ml

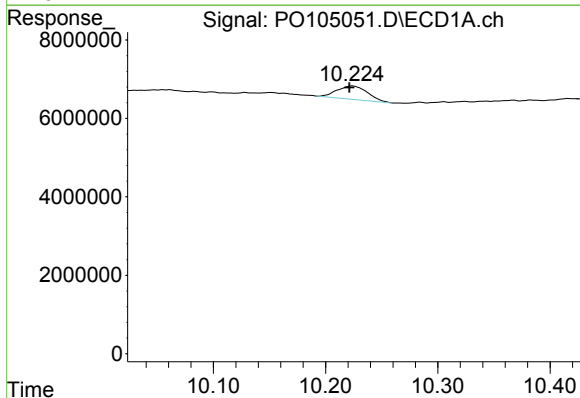

#2 Decachlorobiphenyl

R.T.: 10.224 min
Delta R.T.: 0.002 min
Response: 6450628
Conc: 1.26 ng/ml m

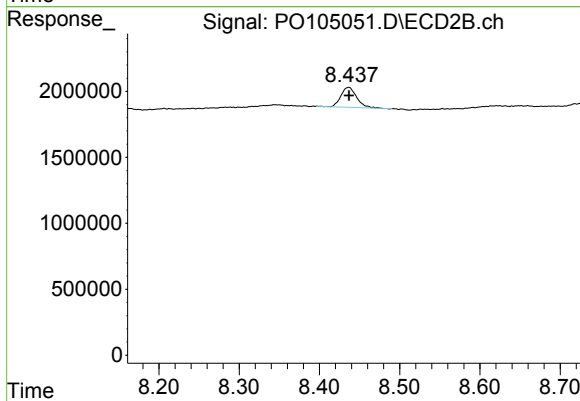

#2 Decachlorobiphenyl

R.T.: 8.436 min
Delta R.T.: 0.000 min
Response: 2023836
Conc: 1.27 ng/ml