

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0080118\
 Data File : P0047528.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Aug 2018 18:36
 Operator : SM/SJ
 Sample : J4231-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 2018-NYSEG-CLARK-AREA-14-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 01:50:13 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jul 27 02:33:29 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.399	3.644	4856789	4962146	24.056	20.195
2) SA Decachlor...	10.089	8.633	3431905	3563510	21.042	22.670
Target Compounds						
3) L1 AR-1016-1	5.299	4.531	568881	1539233	119.101	269.236 #
4) L1 AR-1016-2	5.653	4.919	30050	27257	5.104	5.191
5) L1 AR-1016-3	5.748	4.971	91953	112370	18.542	25.592 #
6) L1 AR-1016-4	6.042	5.026	40712	104841	8.753	20.218 #
7) L1 AR-1016-5	6.171	5.165	13557	120512	2.601	20.546 #
8) L2 AR-1221-1	4.609	0.000	6358	0	2.875	N.D. #
9) L2 AR-1221-2	4.704	3.947	150982	337954	92.332	186.297 #
10) L2 AR-1221-3	4.778	4.058	95759	211231	18.548	36.541 #
11) L3 AR-1232-1	5.099	4.324	277844	572750	129.198	243.544 #
12) L3 AR-1232-2	5.573	4.733	62002	445616	21.071	145.822 #
13) L3 AR-1232-3	5.585	4.733	20591	445616	4.793	96.500 #
14) L3 AR-1232-4	5.653	4.800	30050	126054	10.857	40.776 #
15) L3 AR-1232-5	5.748	4.971	91953	112370	41.177	62.786 #
16) L4 AR-1242-1	5.585	4.733	20591	445616	2.801	55.645 #
17) L4 AR-1242-2	5.653	4.919	30050	27257	6.492	6.616
18) L4 AR-1242-3	5.748	5.026	91953	104841	23.934	24.999
19) L4 AR-1242-4	6.042	5.165	40712	120512	10.590	25.520 #
20) L4 AR-1242-5	6.171	5.313	13557	237370	3.167	61.309 #
21) L5 AR-1248-1	6.042	5.165	40712	120512	6.511	16.154 #
22) L5 AR-1248-2	6.171	5.313	13557	237370	2.489	44.369 #
23) L5 AR-1248-3	6.451	5.524	51995	55281	7.388	5.556
24) L5 AR-1248-4	6.489	5.576	14029	45208	2.090	6.451 #
25) L5 AR-1248-5	6.640	6.090	323332	267609	45.683	56.152
26) L6 AR-1254-1	6.640	5.524	323332	55281	26.440	4.493 #
27) L6 AR-1254-2	6.898	5.674	199893	14321	26.803	1.376 #
28) L6 AR-1254-3	7.011	6.090	725667	267609	55.643	15.419 #
29) L6 AR-1254-4	7.287	6.247	11668	685402	1.197	63.256 #
30) L6 AR-1254-5	7.561	6.602	32808	102136	4.441	13.355 #
31) L7 AR-1260-1	7.170	6.215	42044	395356	4.484	35.779 #
32) L7 AR-1260-2	7.413	6.381	51069	784630	4.580	58.519 #
33) L7 AR-1260-3	7.709	6.716	23715	110795	1.843	7.621 #
34) L7 AR-1260-4	8.311	7.253	28000	32740	1.574	1.488
35) L7 AR-1260-5	8.643	7.606	12563	63829	1.100	4.092 #
36) L8 AR-1262-1	7.170	6.381	42044	784630	5.075	69.203 #
37) L8 AR-1262-2	7.413	6.545	51069	55019	5.269	4.876
38) L8 AR-1262-3	7.804	6.788	165186	10350	13.460	0.686 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0080118\
 Data File : P0047528.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Aug 2018 18:36
 Operator : SM/SJ
 Sample : J4231-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 2018-NYSEG-CLARK-AREA-14-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 01:50:13 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jul 27 02:33:29 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
39) L8	AR-1262-4	7.997	7.011	11541	29886	0.980	2.270 #
40) L8	AR-1262-5	8.311	7.253	28000	32740	1.303	1.268
41) L9	AR-1268-1	8.632	7.535	15779	50249	0.680	1.933 #
42) L9	AR-1268-2	8.710	7.606	6257	63829	0.292	2.562 #
43) L9	AR-1268-3	8.933	7.809	9598	100906	0.532	5.113 #
44) L9	AR-1268-4	9.359	8.097	8337	31143	1.046	3.713 #
45) L9	AR-1268-5	9.764	8.381	60819	37829	1.116	0.693 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080118\
Data File : P0047528.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Aug 2018 18:36
Operator : SM/SJ
Sample : J4231-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
2018-NYSEG-CLARK-AREA-14-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 01:50:13 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072718.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 27 02:33:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

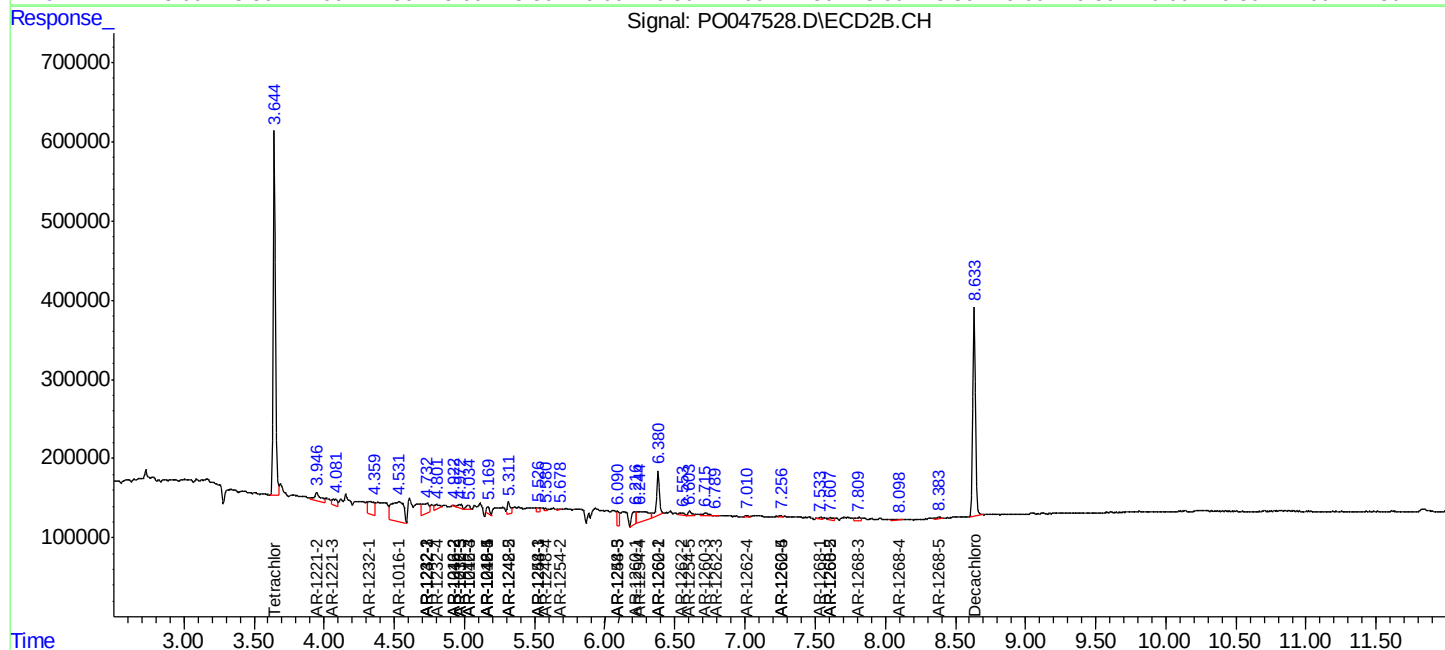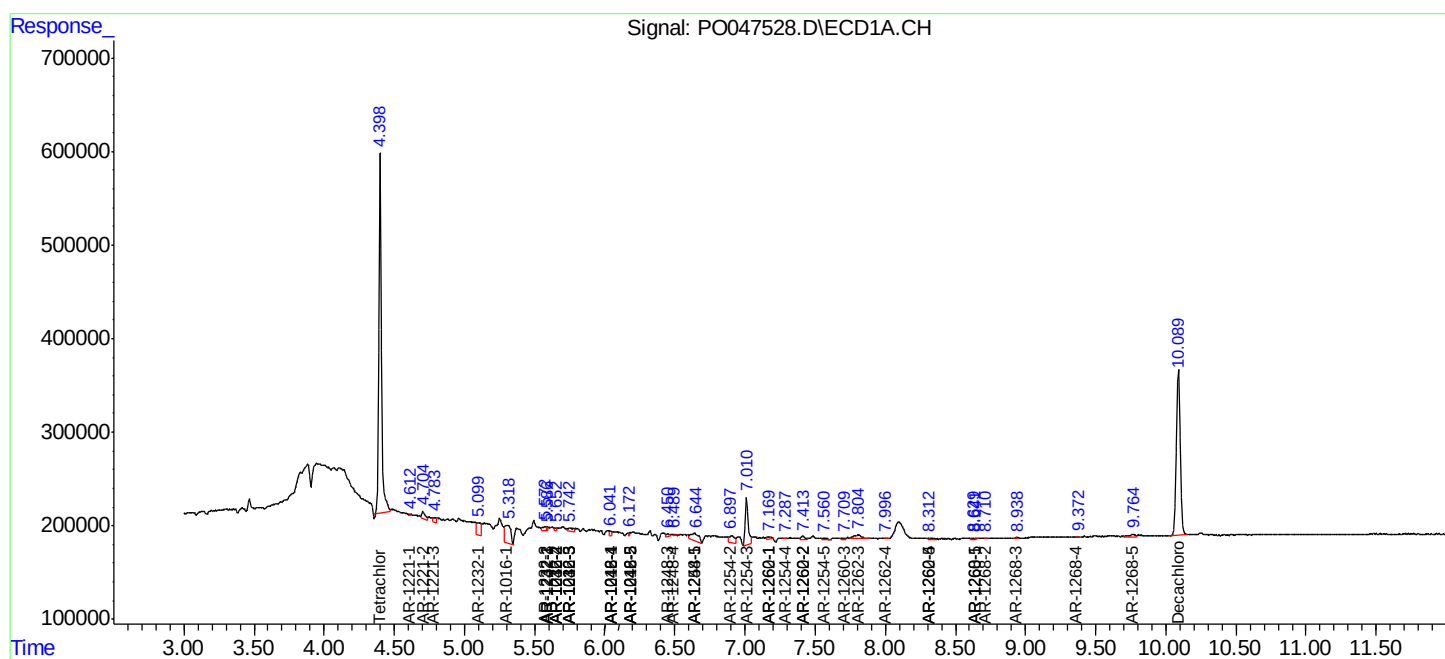


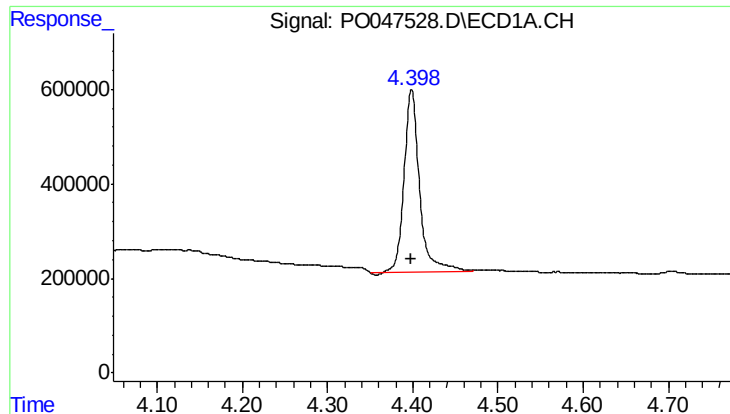

#1 Tetrachloro-m-xylene


R.T.: 4.399 min
Delta R.T.: 0.001 min
Response: 4856789
Conc: 24.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
2018-NYSEG-CLARK-AREA-14-2

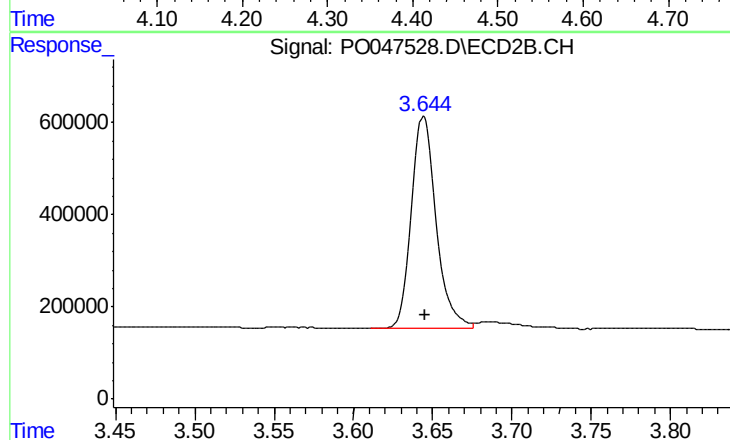


#1 Tetrachloro-m-xylene

R.T.: 3.644 min
Delta R.T.: -0.001 min
Response: 4962146
Conc: 20.19 ng/ml

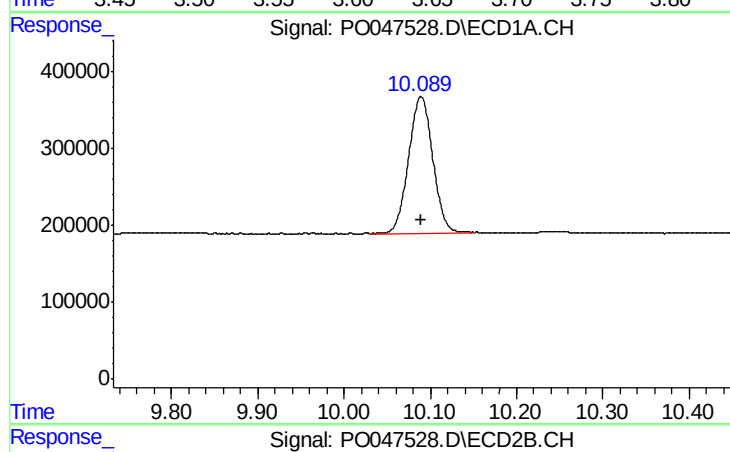


#2 Decachlorobiphenyl

R.T.: 10.089 min
Delta R.T.: 0.000 min
Response: 3431905
Conc: 21.04 ng/ml

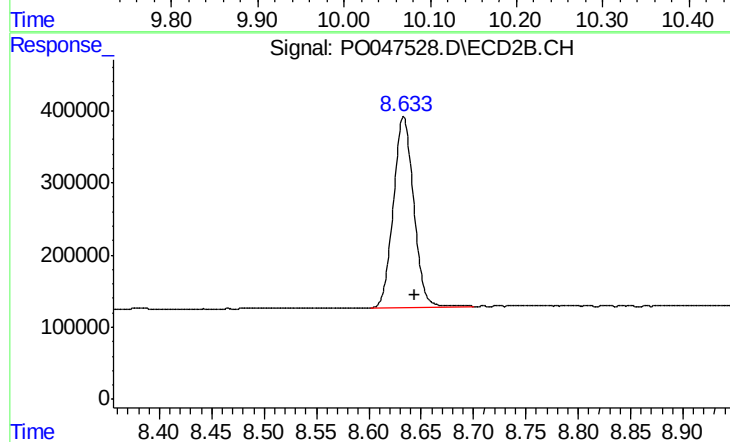

#2 Decachlorobiphenyl


R.T.: 8.633 min
Delta R.T.: -0.011 min
Response: 3563510
Conc: 22.67 ng/ml

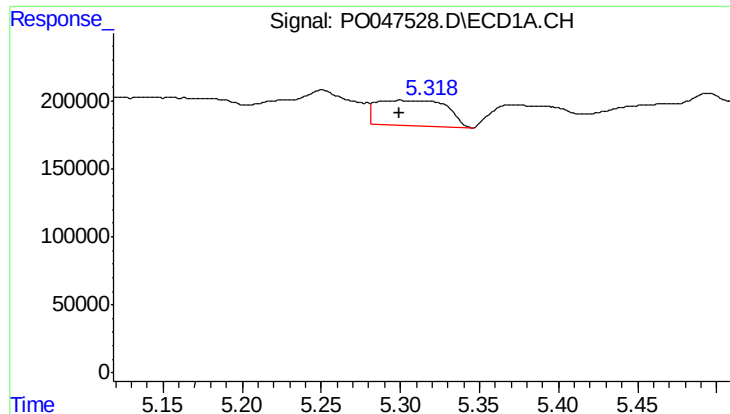

#3 AR-1016-1


R.T.: 5.299 min
Delta R.T.: 0.000 min
Response: 568881
Conc: 119.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
2018-NYSEG-CLARK-AREA-14-2

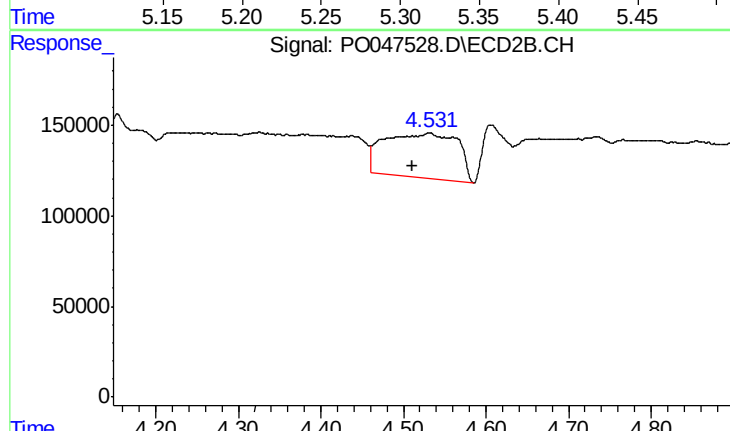


#3 AR-1016-1

R.T.: 4.531 min
Delta R.T.: 0.020 min
Response: 1539233
Conc: 269.24 ng/ml

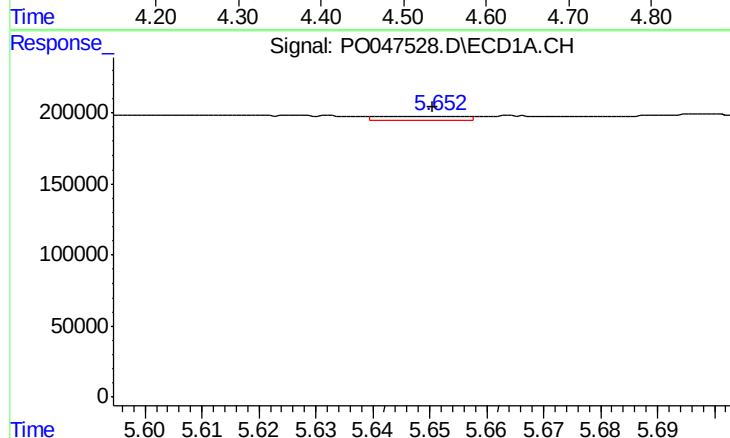


#4 AR-1016-2

R.T.: 5.653 min
Delta R.T.: 0.002 min
Response: 30050
Conc: 5.10 ng/ml

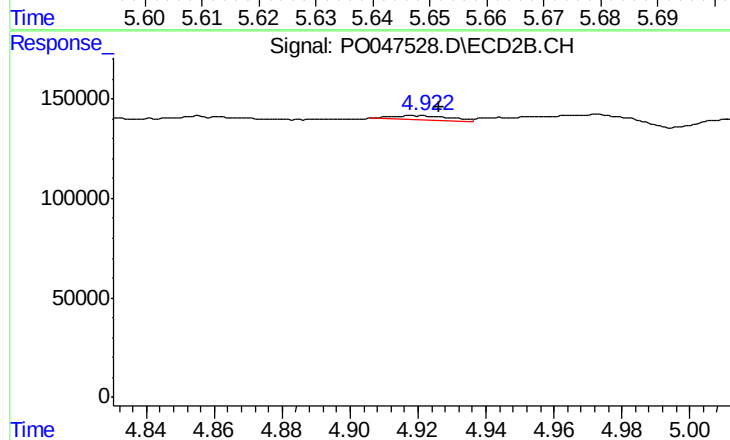

#4 AR-1016-2


R.T.: 4.919 min
Delta R.T.: -0.007 min
Response: 27257
Conc: 5.19 ng/ml

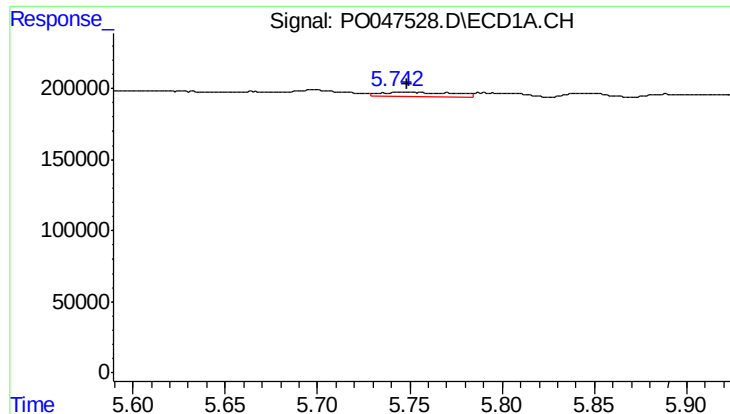

#5 AR-1016-3


R.T.: 5.748 min
Delta R.T.: -0.001 min
Response: 91953
Conc: 18.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
2018-NYSEG-CLARK-AREA-14-2

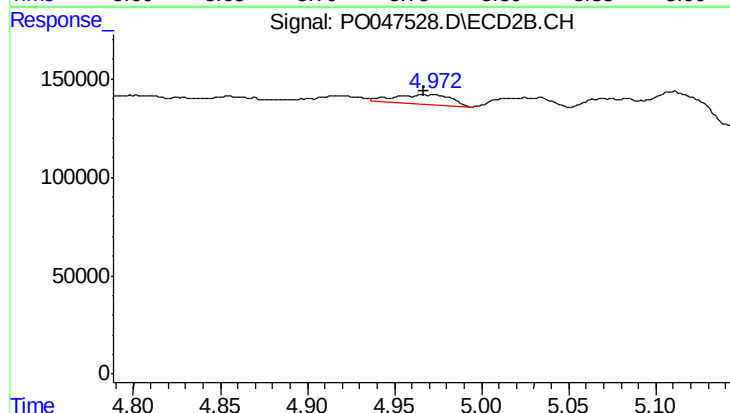


#5 AR-1016-3

R.T.: 4.971 min
Delta R.T.: 0.004 min
Response: 112370
Conc: 25.59 ng/ml

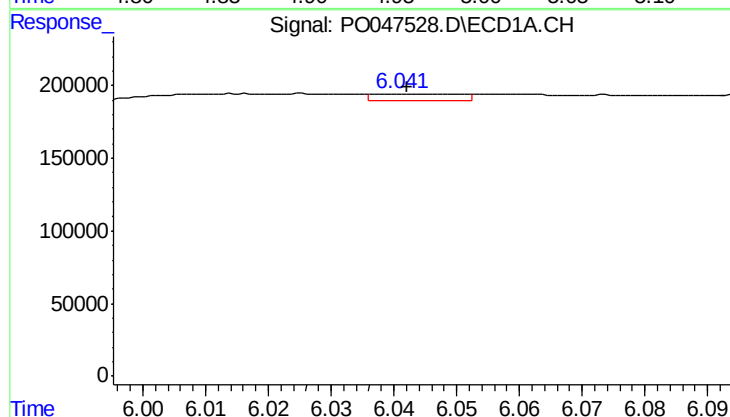


#6 AR-1016-4

R.T.: 6.042 min
Delta R.T.: 0.000 min
Response: 40712
Conc: 8.75 ng/ml

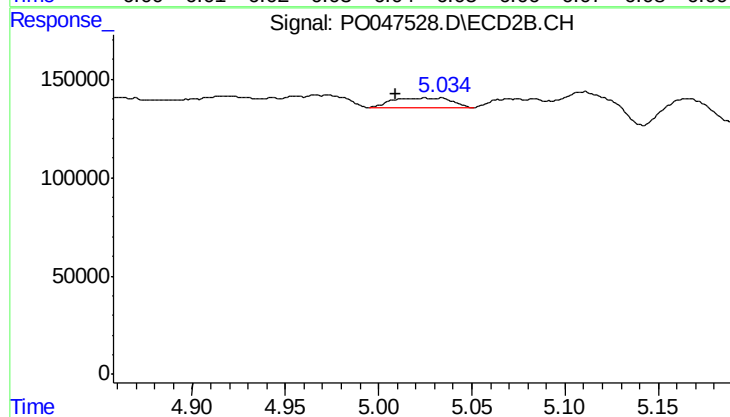

#6 AR-1016-4


R.T.: 5.026 min
Delta R.T.: 0.017 min
Response: 104841
Conc: 20.22 ng/ml

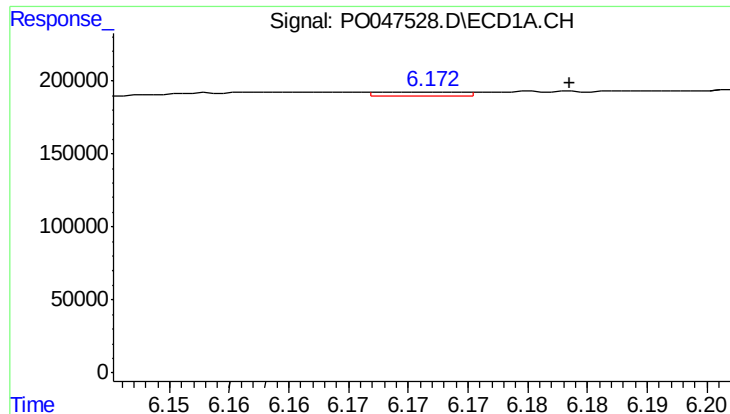

#7 AR-1016-5


R.T.: 6.171 min
Delta R.T.: -0.012 min
Response: 13557
Conc: 2.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
2018-NYSEG-CLARK-AREA-14-2

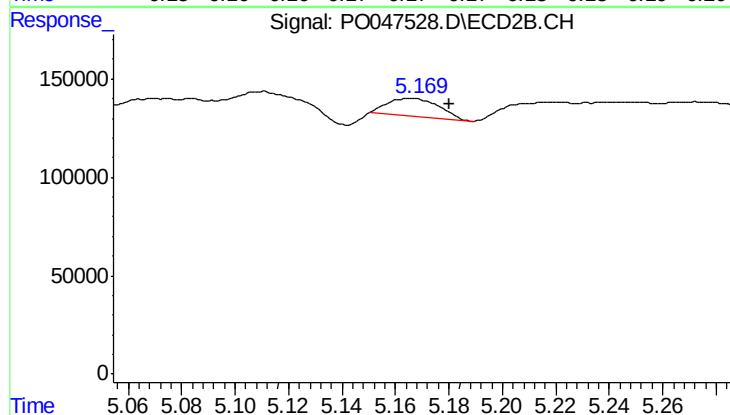


#7 AR-1016-5

R.T.: 5.165 min
Delta R.T.: -0.015 min
Response: 120512
Conc: 20.55 ng/ml

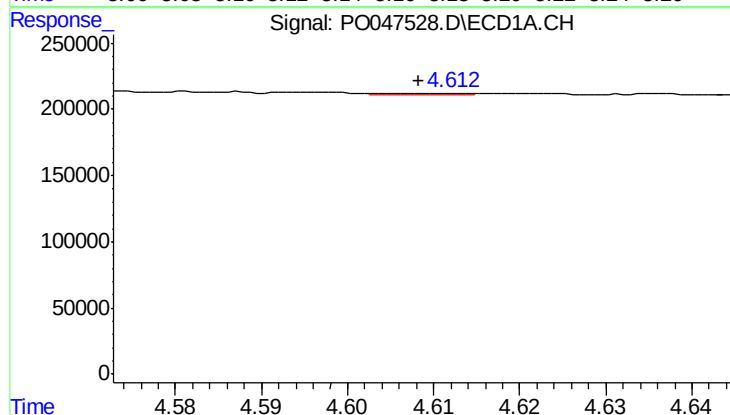


#8 AR-1221-1

R.T.: 4.609 min
Delta R.T.: 0.000 min
Response: 6358
Conc: 2.88 ng/ml

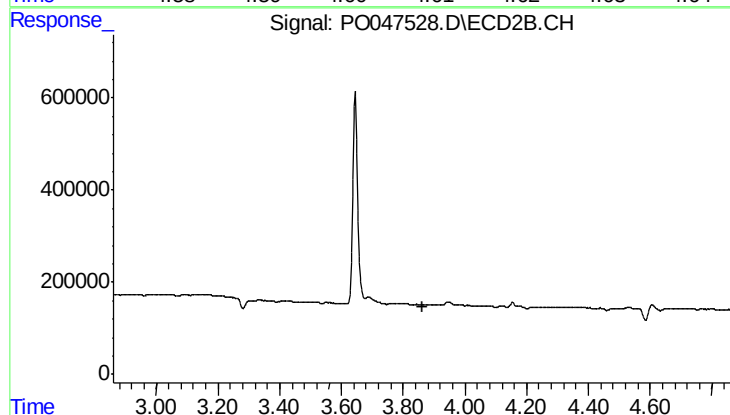

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T.: 3.861 min
Response: 0
Conc: N.D.

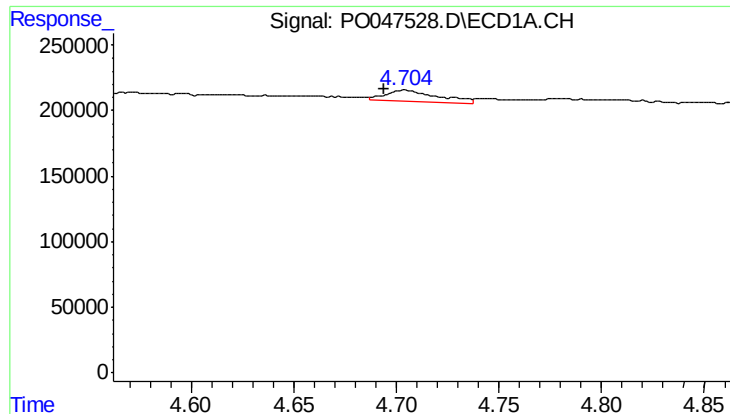

#9 AR-1221-2


R.T.: 4.704 min
Delta R.T.: 0.010 min
Response: 150982
Conc: 92.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
2018-NYSEG-CLARK-AREA-14-2

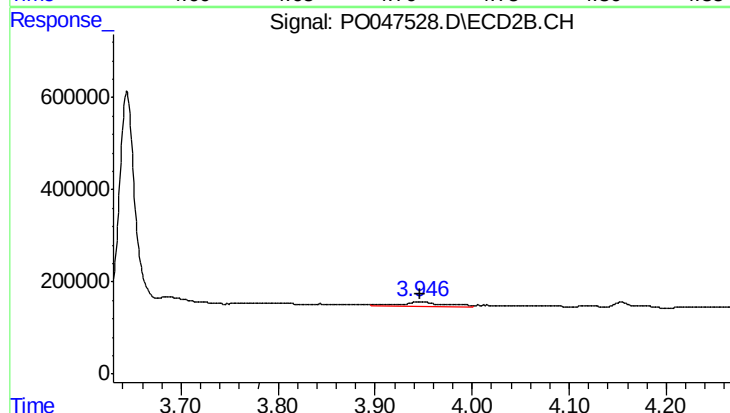


#9 AR-1221-2

R.T.: 3.947 min
Delta R.T.: 0.000 min
Response: 337954
Conc: 186.30 ng/ml

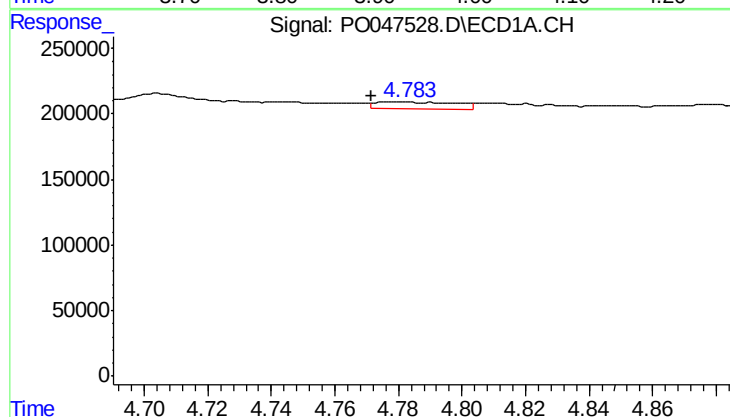


#10 AR-1221-3

R.T.: 4.778 min
Delta R.T.: 0.007 min
Response: 95759
Conc: 18.55 ng/ml

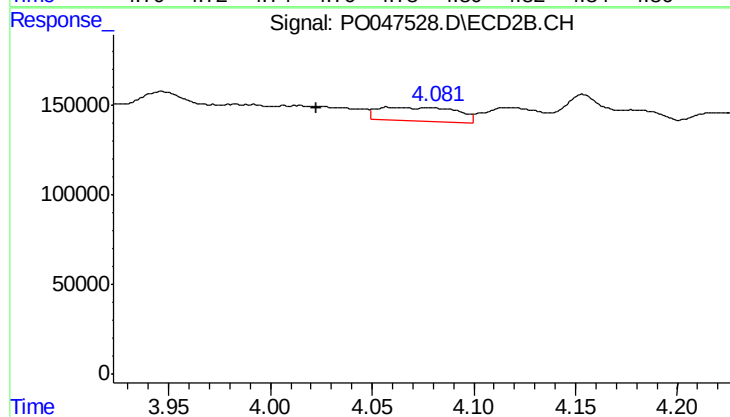

#10 AR-1221-3


R.T.: 4.058 min
Delta R.T.: 0.036 min
Response: 211231
Conc: 36.54 ng/ml

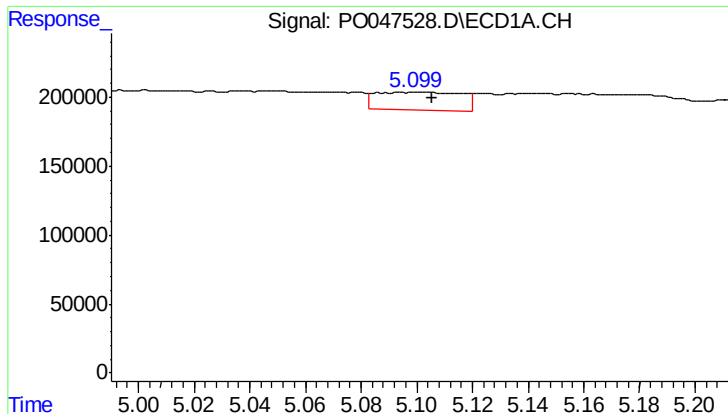

#11 AR-1232-1


R.T.: 5.099 min
Delta R.T.: -0.006 min
Response: 277844
Conc: 129.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
2018-NYSEG-CLARK-AREA-14-2

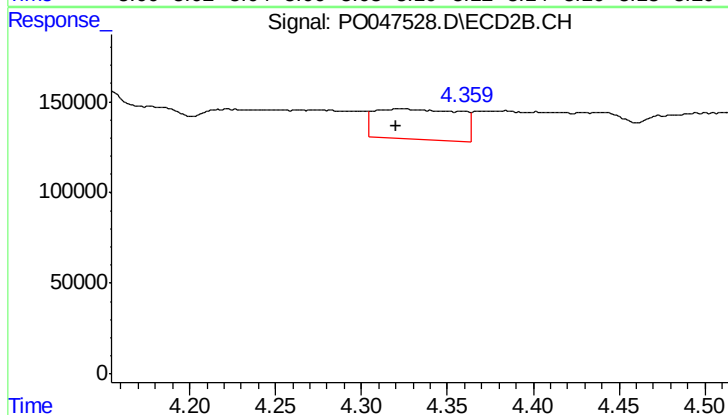


#11 AR-1232-1

R.T.: 4.324 min
Delta R.T.: 0.004 min
Response: 572750
Conc: 243.54 ng/ml

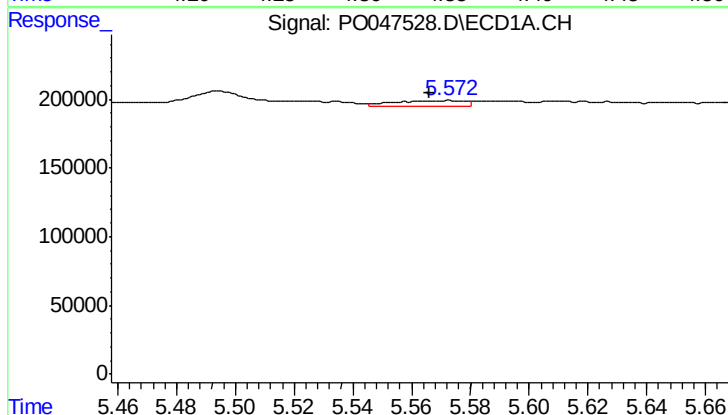


#12 AR-1232-2

R.T.: 5.573 min
Delta R.T.: 0.007 min
Response: 62002
Conc: 21.07 ng/ml

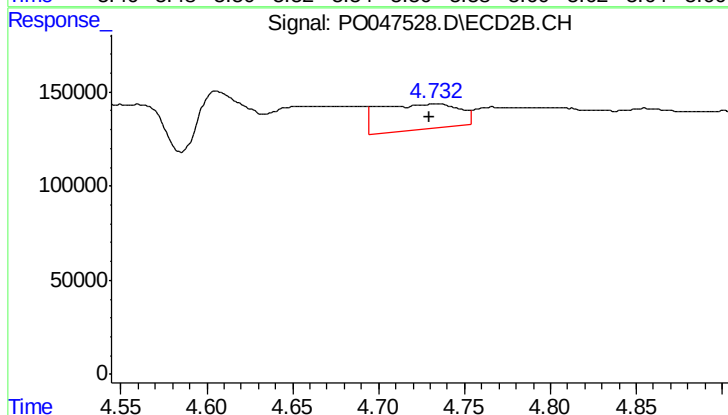

#12 AR-1232-2


R.T.: 4.733 min
Delta R.T.: 0.003 min
Response: 445616
Conc: 145.82 ng/ml

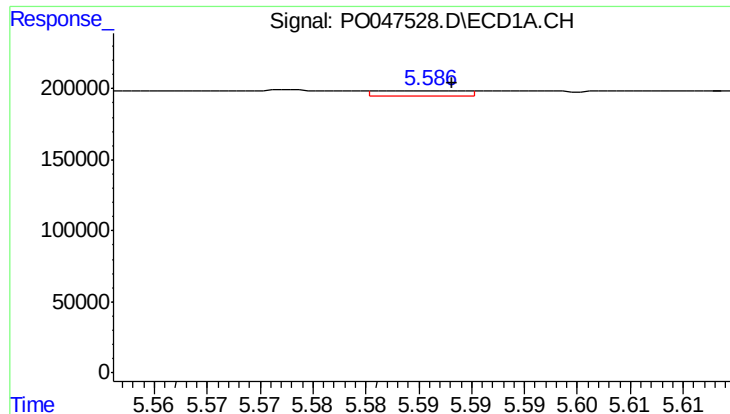

#13 AR-1232-3


R.T.: 5.585 min
Delta R.T.: -0.003 min
Response: 20591
Conc: 4.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
2018-NYSEG-CLARK-AREA-14-2

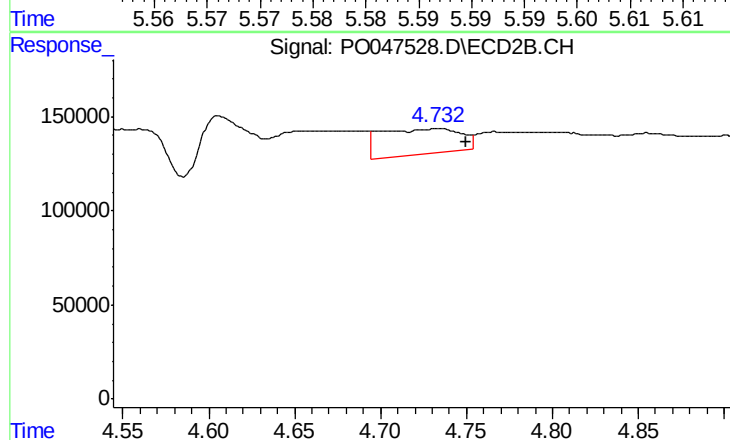


#13 AR-1232-3

R.T.: 4.733 min
Delta R.T.: -0.016 min
Response: 445616
Conc: 96.50 ng/ml

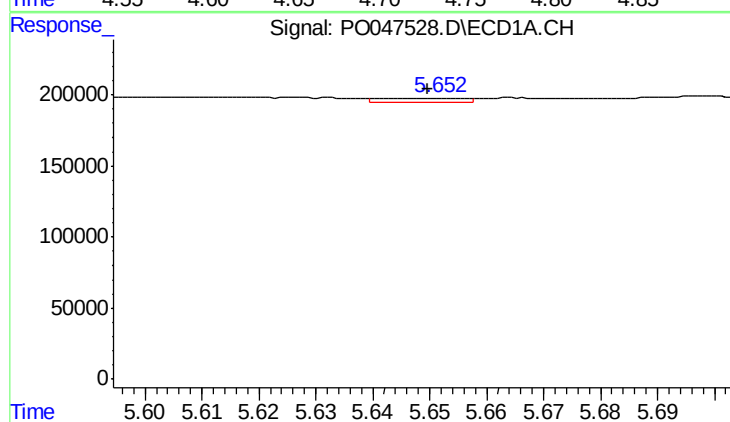


#14 AR-1232-4

R.T.: 5.653 min
Delta R.T.: 0.003 min
Response: 30050
Conc: 10.86 ng/ml

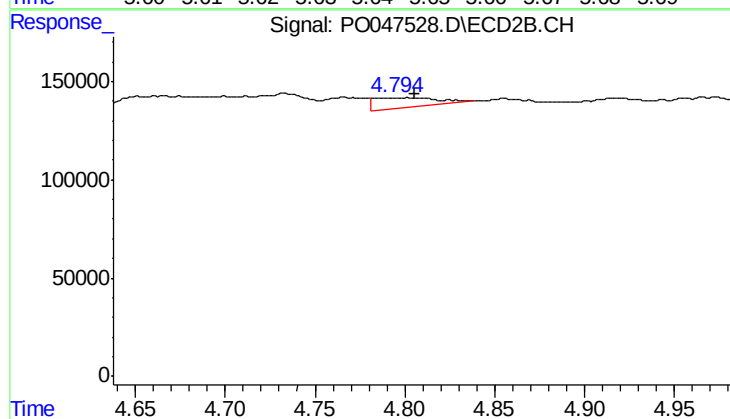

#14 AR-1232-4


R.T.: 4.800 min
Delta R.T.: -0.005 min
Response: 126054
Conc: 40.78 ng/ml

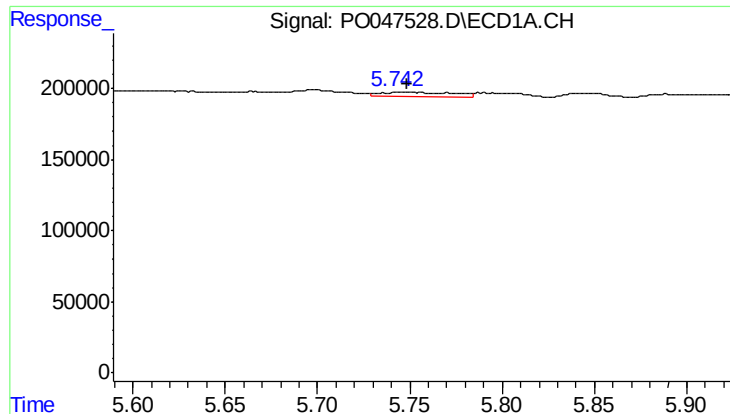

#15 AR-1232-5


R.T.: 5.748 min
Delta R.T.: -0.001 min
Response: 91953
Conc: 41.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
2018-NYSEG-CLARK-AREA-14-2

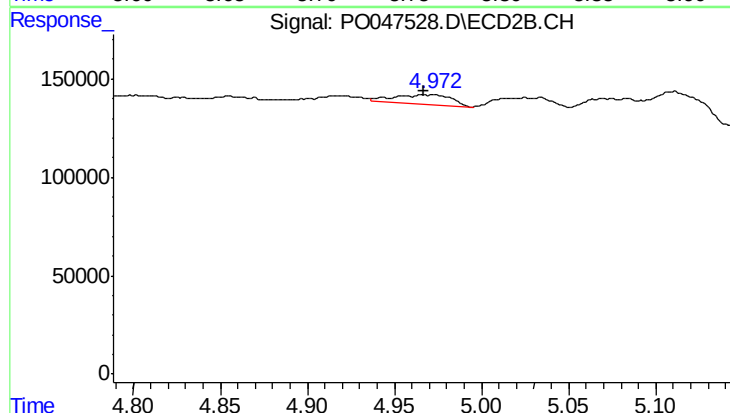


#15 AR-1232-5

R.T.: 4.971 min
Delta R.T.: 0.005 min
Response: 112370
Conc: 62.79 ng/ml

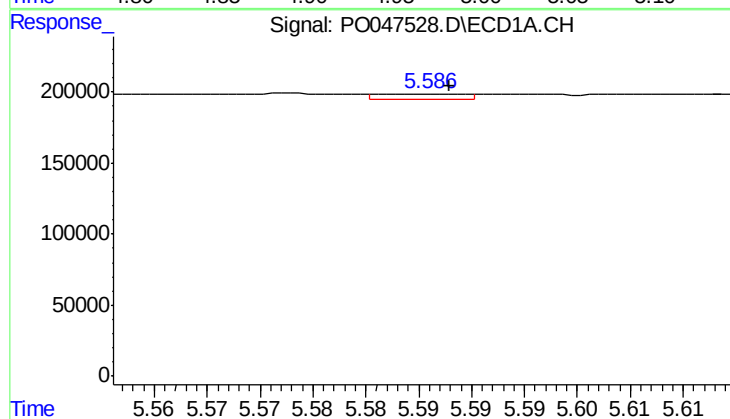


#16 AR-1242-1

R.T.: 5.585 min
Delta R.T.: -0.003 min
Response: 20591
Conc: 2.80 ng/ml

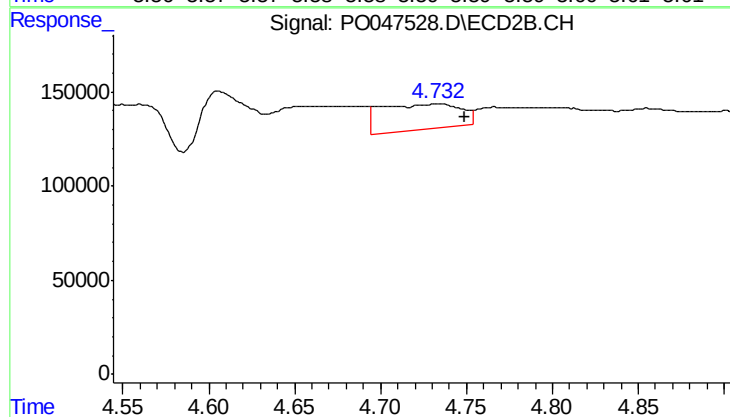

#16 AR-1242-1


R.T.: 4.733 min
Delta R.T.: -0.015 min
Response: 445616
Conc: 55.64 ng/ml

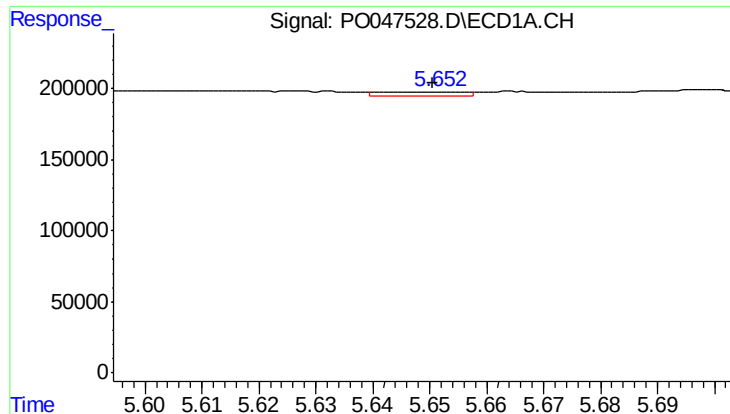

#17 AR-1242-2


R.T.: 5.653 min
Delta R.T.: 0.002 min
Response: 30050
Conc: 6.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
2018-NYSEG-CLARK-AREA-14-2

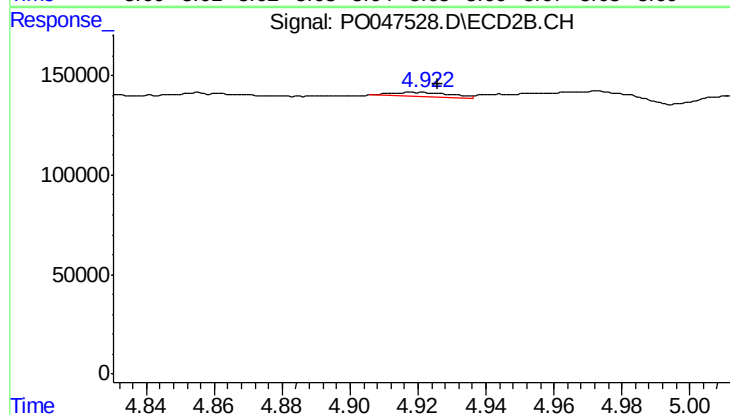


#17 AR-1242-2

R.T.: 4.919 min
Delta R.T.: -0.007 min
Response: 27257
Conc: 6.62 ng/ml

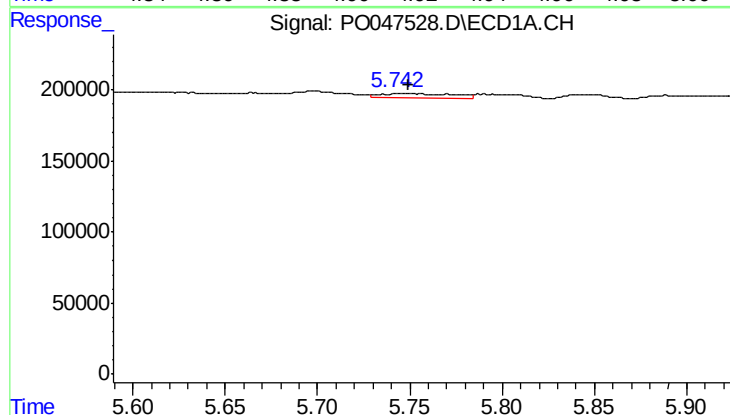


#18 AR-1242-3

R.T.: 5.748 min
Delta R.T.: -0.001 min
Response: 91953
Conc: 23.93 ng/ml

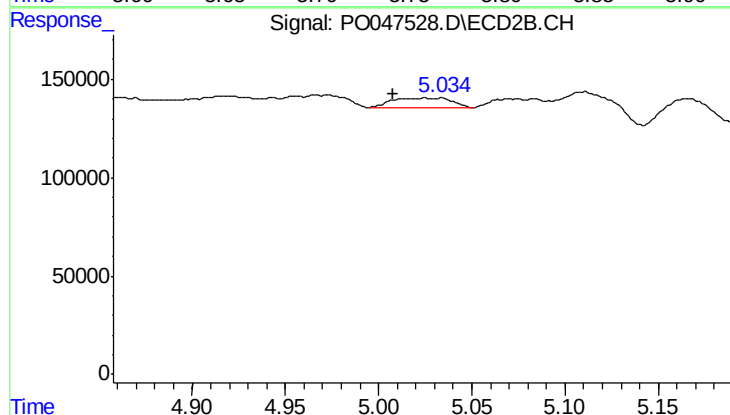

#18 AR-1242-3


R.T.: 5.026 min
Delta R.T.: 0.018 min
Response: 104841
Conc: 25.00 ng/ml

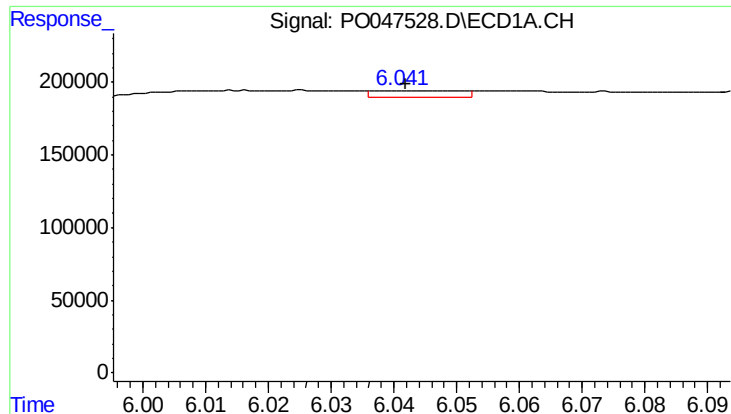

#19 AR-1242-4


R.T.: 6.042 min
Delta R.T.: 0.000 min
Response: 40712
Conc: 10.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
2018-NYSEG-CLARK-AREA-14-2

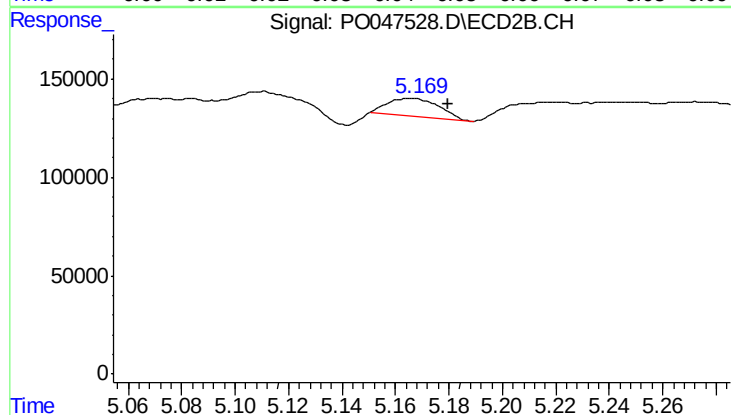


#19 AR-1242-4

R.T.: 5.165 min
Delta R.T.: -0.015 min
Response: 120512
Conc: 25.52 ng/ml

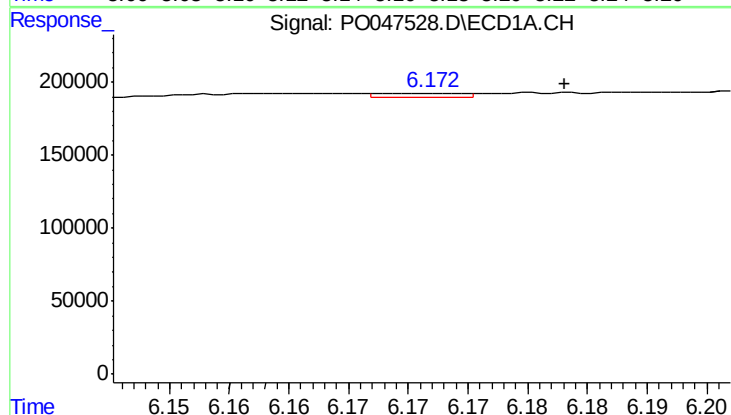


#20 AR-1242-5

R.T.: 6.171 min
Delta R.T.: -0.012 min
Response: 13557
Conc: 3.17 ng/ml

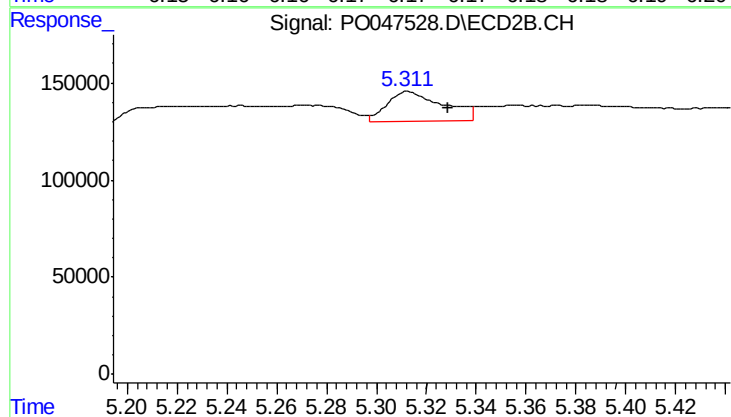

#20 AR-1242-5


R.T.: 5.313 min
Delta R.T.: -0.016 min
Response: 237370
Conc: 61.31 ng/ml

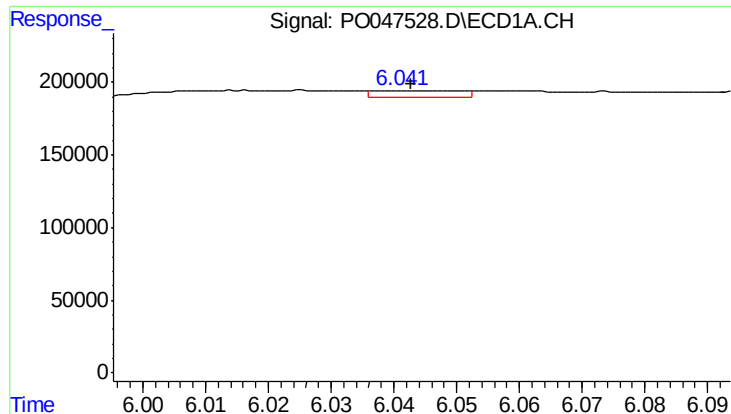

#21 AR-1248-1


R.T.: 6.042 min
Delta R.T.: 0.000 min
Response: 40712
Conc: 6.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
2018-NYSEG-CLARK-AREA-14-2

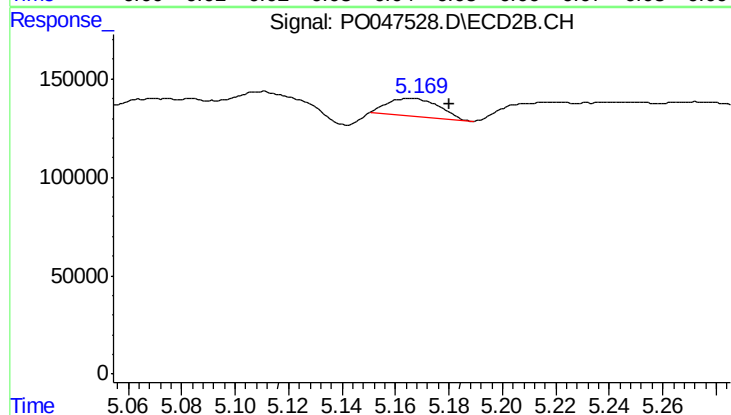


#21 AR-1248-1

R.T.: 5.165 min
Delta R.T.: -0.015 min
Response: 120512
Conc: 16.15 ng/ml

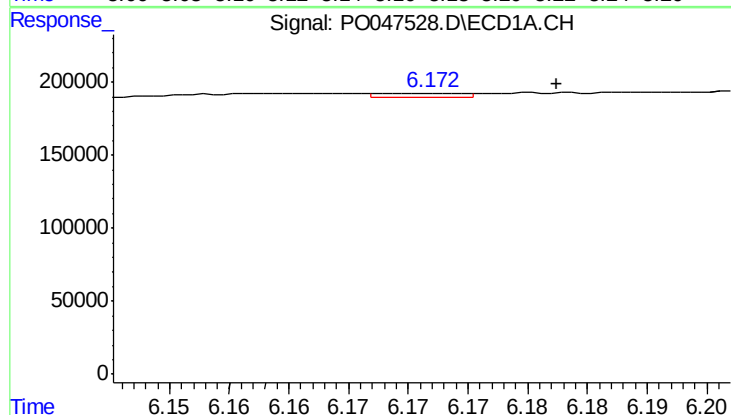


#22 AR-1248-2

R.T.: 6.171 min
Delta R.T.: -0.011 min
Response: 13557
Conc: 2.49 ng/ml

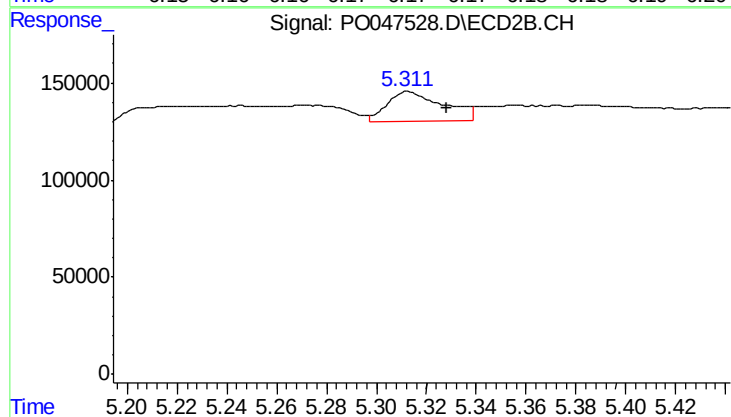

#22 AR-1248-2


R.T.: 5.313 min
Delta R.T.: -0.015 min
Response: 237370
Conc: 44.37 ng/ml

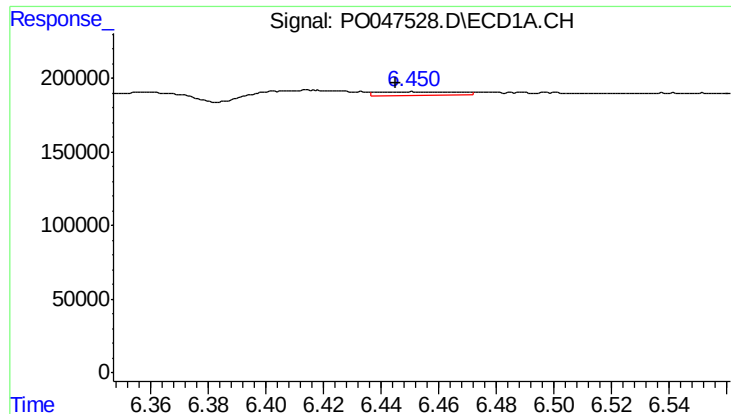

#23 AR-1248-3


R.T.: 6.451 min
Delta R.T.: 0.006 min
Response: 51995
Conc: 7.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
2018-NYSEG-CLARK-AREA-14-2

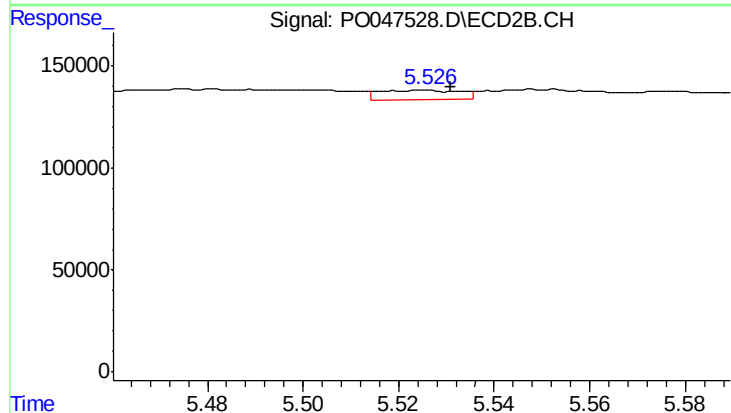


#23 AR-1248-3

R.T.: 5.524 min
Delta R.T.: -0.007 min
Response: 55281
Conc: 5.56 ng/ml

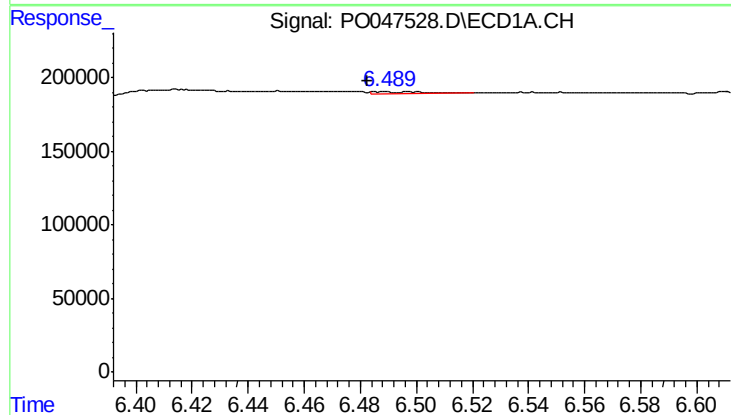


#24 AR-1248-4

R.T.: 6.489 min
Delta R.T.: 0.007 min
Response: 14029
Conc: 2.09 ng/ml

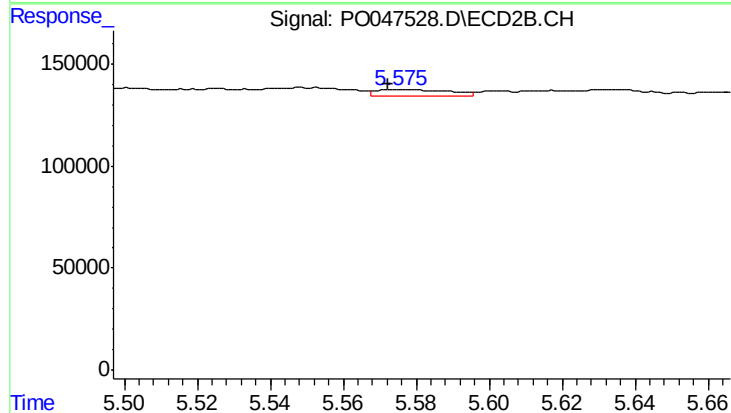

#24 AR-1248-4


R.T.: 5.576 min
Delta R.T.: 0.004 min
Response: 45208
Conc: 6.45 ng/ml

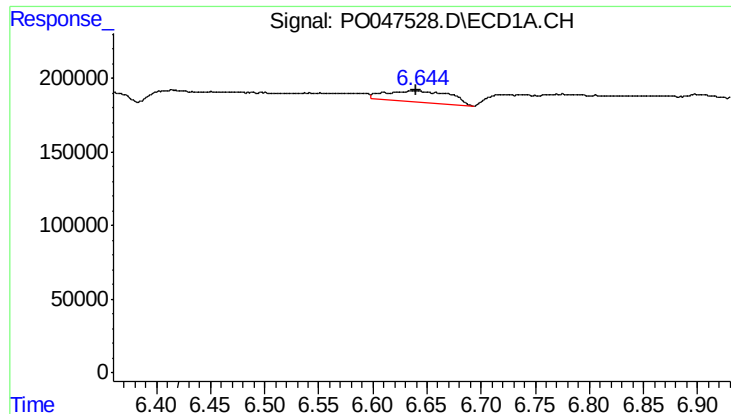

#25 AR-1248-5


R.T.: 6.640 min
Delta R.T.: 0.000 min
Response: 323332
Conc: 45.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
2018-NYSEG-CLARK-AREA-14-2

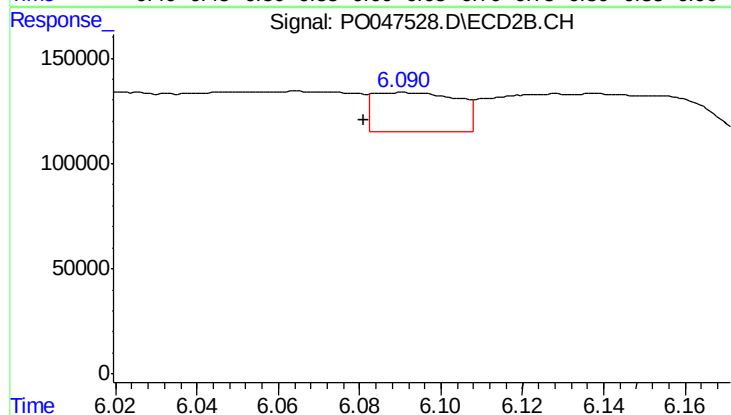


#25 AR-1248-5

R.T.: 6.090 min
Delta R.T.: 0.009 min
Response: 267609
Conc: 56.15 ng/ml

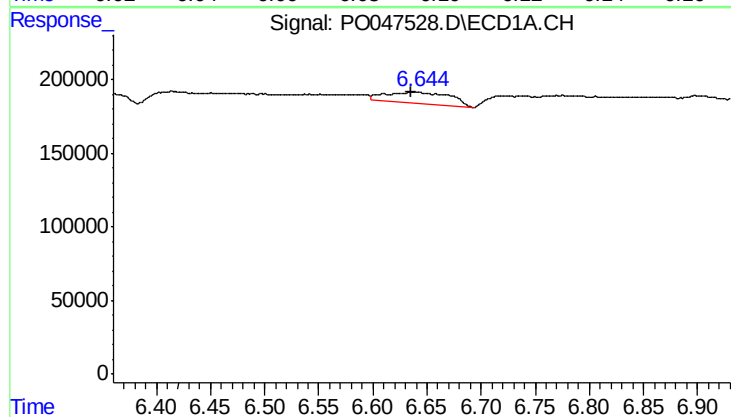


#26 AR-1254-1

R.T.: 6.640 min
Delta R.T.: 0.005 min
Response: 323332
Conc: 26.44 ng/ml

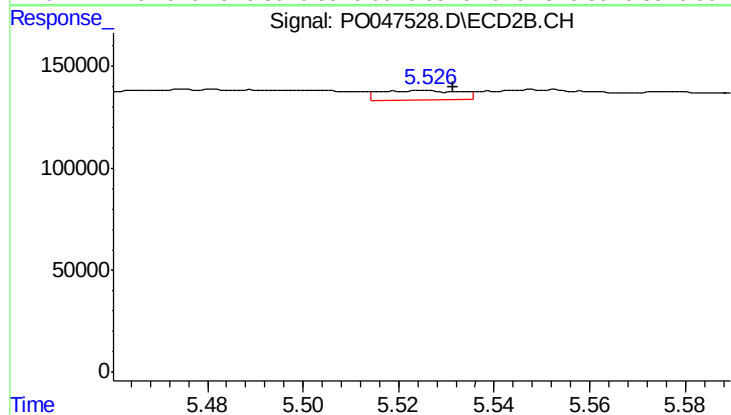

#26 AR-1254-1


R.T.: 5.524 min
Delta R.T.: -0.007 min
Response: 55281
Conc: 4.49 ng/ml

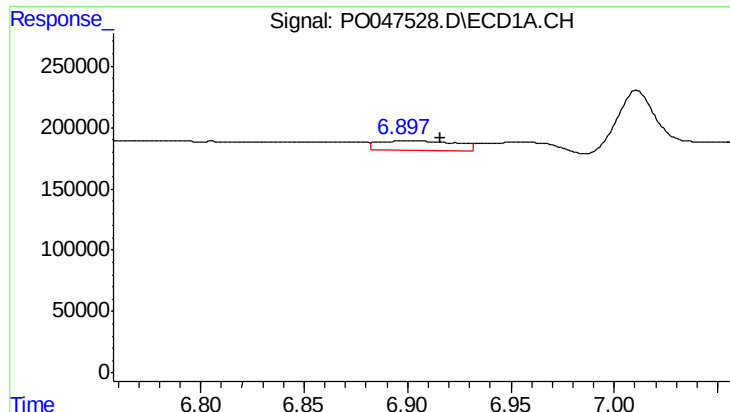

#27 AR-1254-2


R.T.: 6.898 min
Delta R.T.: -0.018 min
Response: 199893
Conc: 26.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
2018-NYSEG-CLARK-AREA-14-2

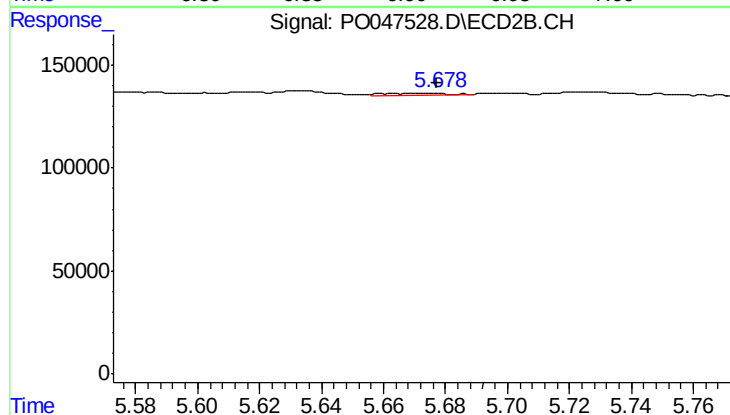


#27 AR-1254-2

R.T.: 5.674 min
Delta R.T.: -0.003 min
Response: 14321
Conc: 1.38 ng/ml

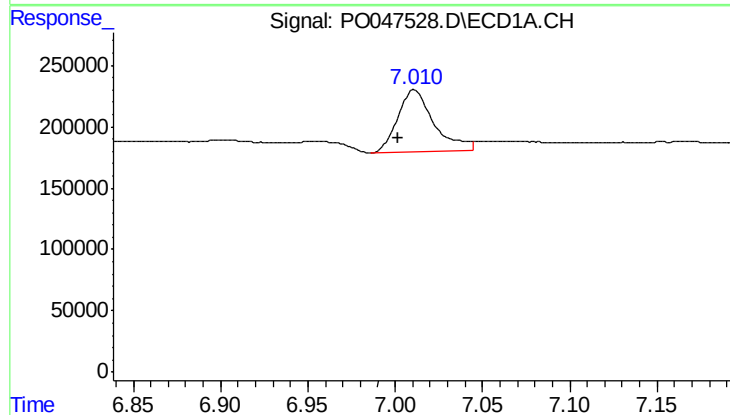


#28 AR-1254-3

R.T.: 7.011 min
Delta R.T.: 0.009 min
Response: 725667
Conc: 55.64 ng/ml

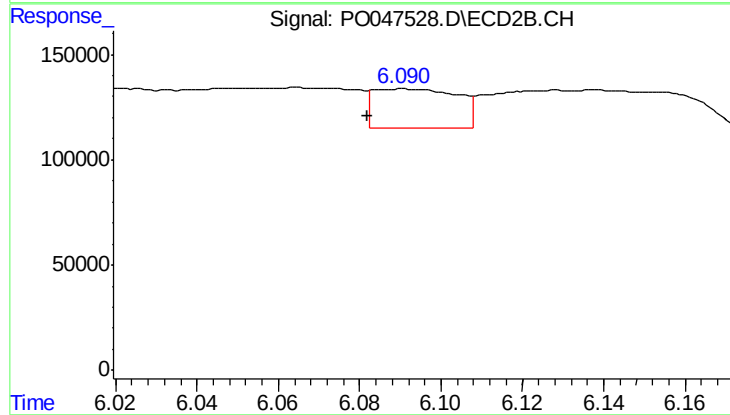

#28 AR-1254-3


R.T.: 6.090 min
Delta R.T.: 0.009 min
Response: 267609
Conc: 15.42 ng/ml

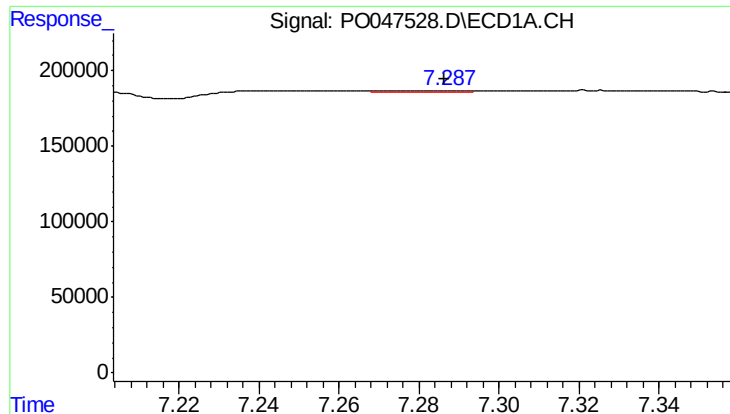

#29 AR-1254-4


R.T.: 7.287 min
Delta R.T.: 0.000 min
Response: 11668
Conc: 1.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
2018-NYSEG-CLARK-AREA-14-2

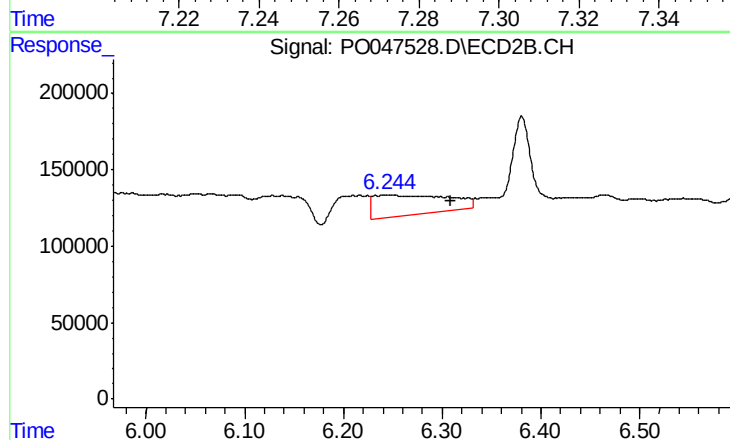


#29 AR-1254-4

R.T.: 6.247 min
Delta R.T.: -0.061 min
Response: 685402
Conc: 63.26 ng/ml

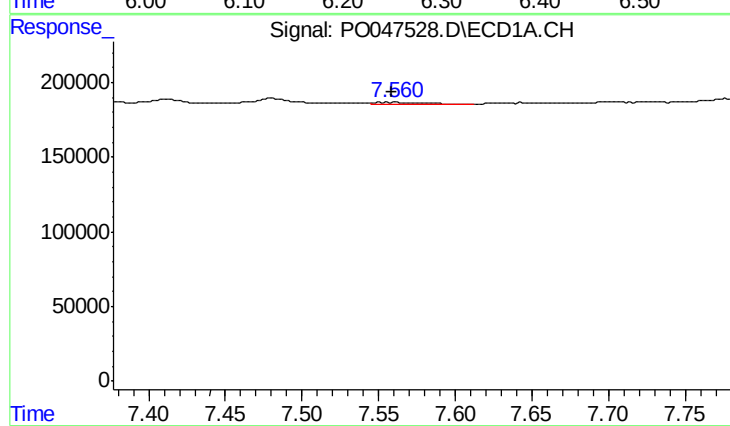


#30 AR-1254-5

R.T.: 7.561 min
Delta R.T.: 0.002 min
Response: 32808
Conc: 4.44 ng/ml

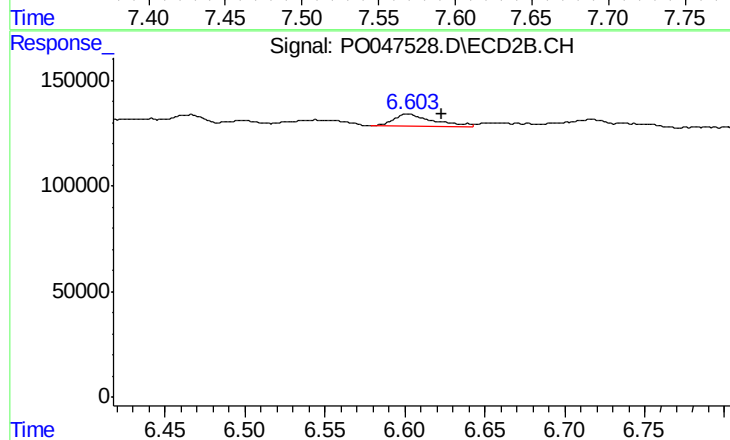

#30 AR-1254-5


R.T.: 6.602 min
Delta R.T.: -0.021 min
Response: 102136
Conc: 13.36 ng/ml

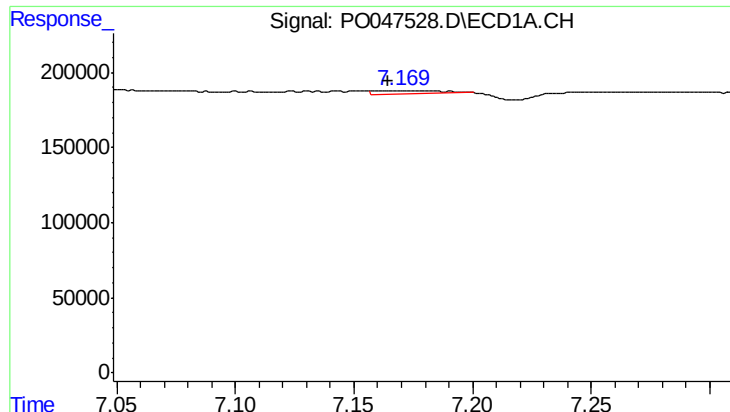

#31 AR-1260-1


R.T.: 7.170 min
Delta R.T.: 0.006 min
Response: 42044
Conc: 4.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
2018-NYSEG-CLARK-AREA-14-2

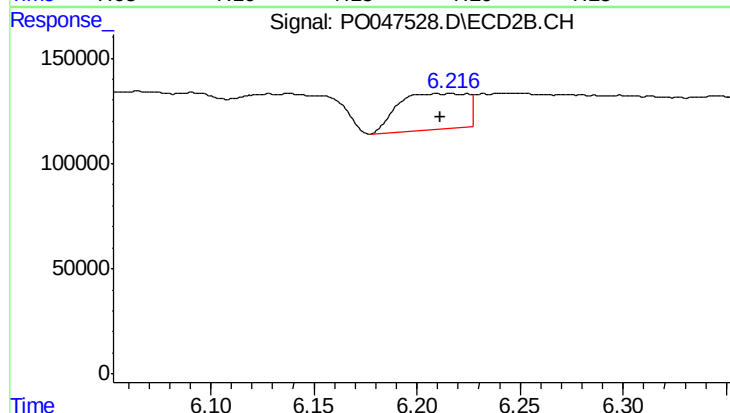


#31 AR-1260-1

R.T.: 6.215 min
Delta R.T.: 0.004 min
Response: 395356
Conc: 35.78 ng/ml

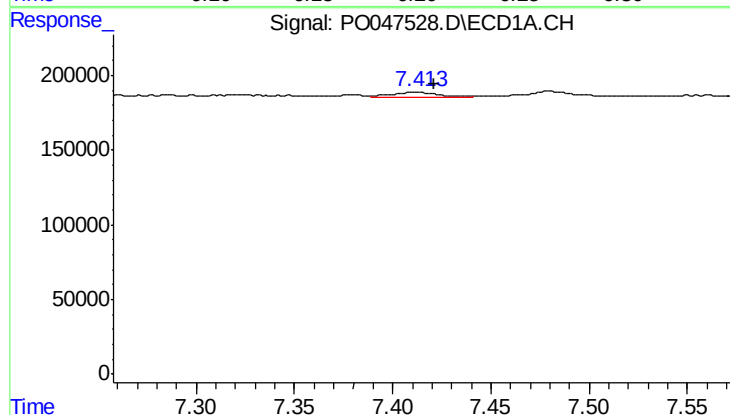


#32 AR-1260-2

R.T.: 7.413 min
Delta R.T.: -0.008 min
Response: 51069
Conc: 4.58 ng/ml

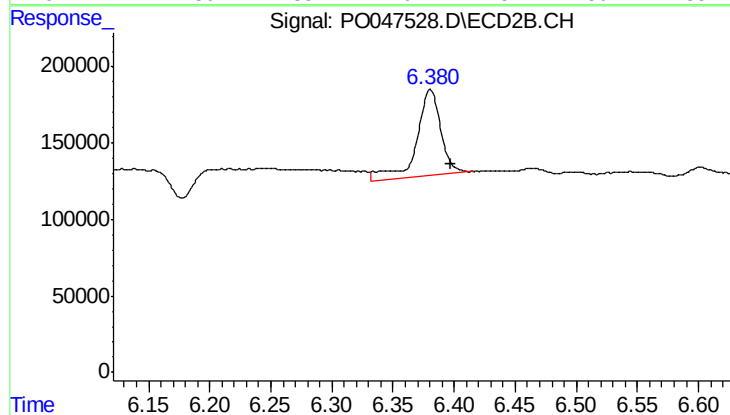

#32 AR-1260-2


R.T.: 6.381 min
Delta R.T.: -0.016 min
Response: 784630
Conc: 58.52 ng/ml

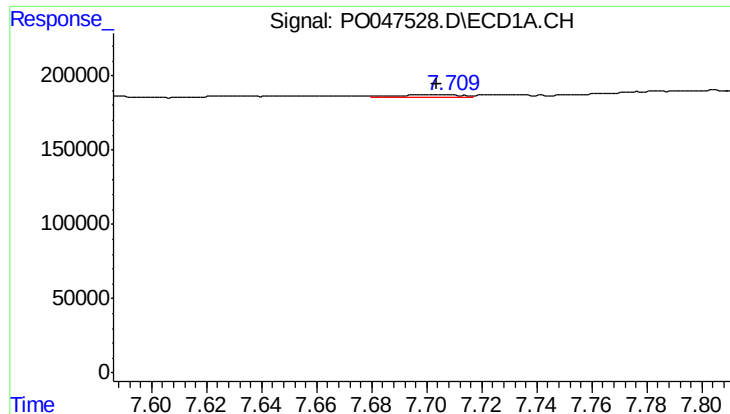

#33 AR-1260-3


R.T.: 7.709 min
Delta R.T.: 0.005 min
Response: 23715
Conc: 1.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
2018-NYSEG-CLARK-AREA-14-2

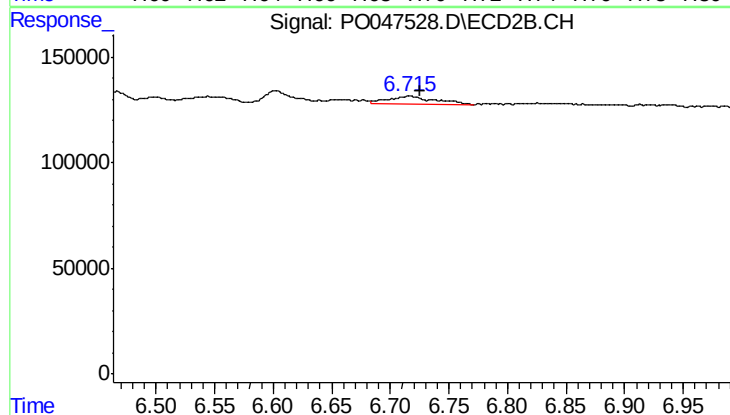


#33 AR-1260-3

R.T.: 6.716 min
Delta R.T.: -0.009 min
Response: 110795
Conc: 7.62 ng/ml

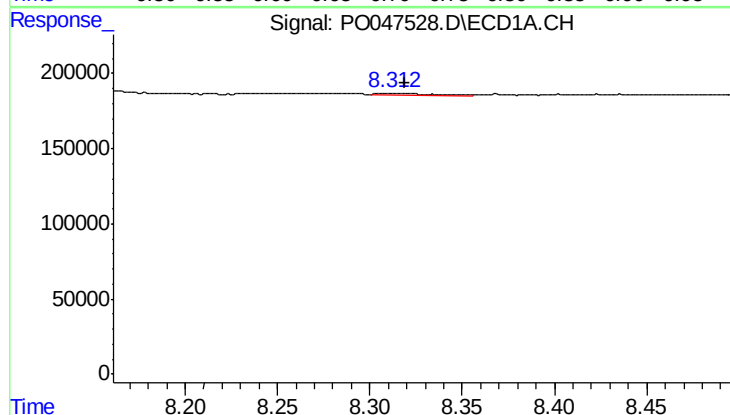


#34 AR-1260-4

R.T.: 8.311 min
Delta R.T.: -0.007 min
Response: 28000
Conc: 1.57 ng/ml

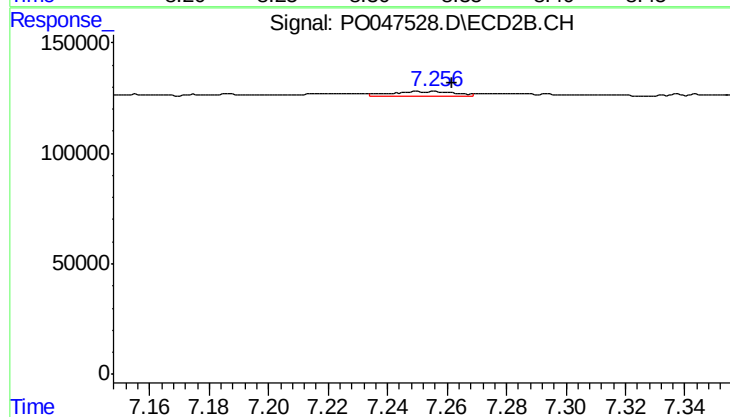

#34 AR-1260-4


R.T.: 7.253 min
Delta R.T.: -0.009 min
Response: 32740
Conc: 1.49 ng/ml

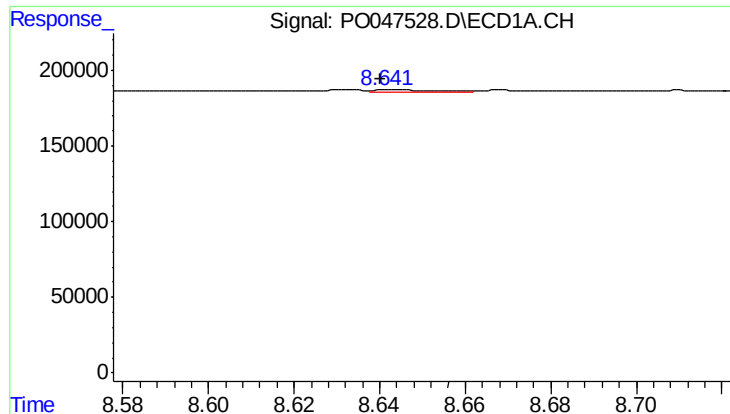

#35 AR-1260-5


R.T.: 8.643 min
Delta R.T.: 0.003 min
Response: 12563
Conc: 1.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
2018-NYSEG-CLARK-AREA-14-2

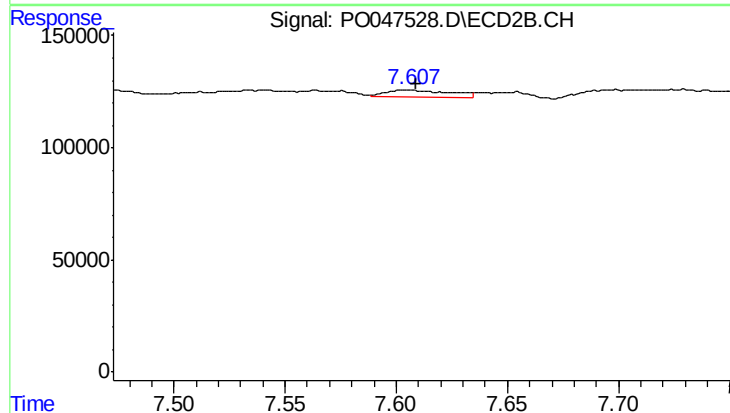


#35 AR-1260-5

R.T.: 7.606 min
Delta R.T.: -0.003 min
Response: 63829
Conc: 4.09 ng/ml

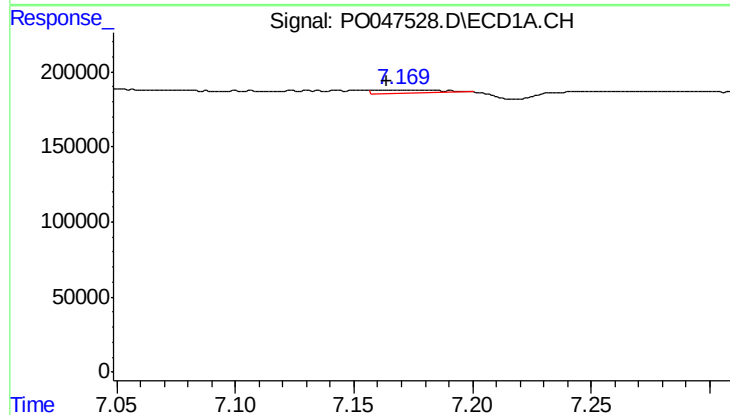


#36 AR-1262-1

R.T.: 7.170 min
Delta R.T.: 0.007 min
Response: 42044
Conc: 5.07 ng/ml

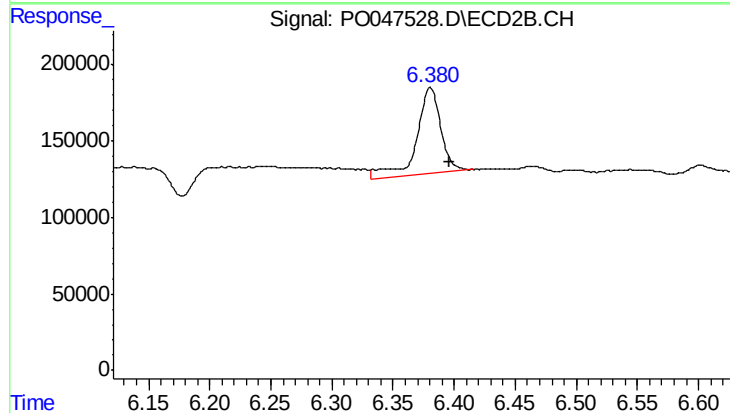

#36 AR-1262-1


R.T.: 6.381 min
Delta R.T.: -0.016 min
Response: 784630
Conc: 69.20 ng/ml

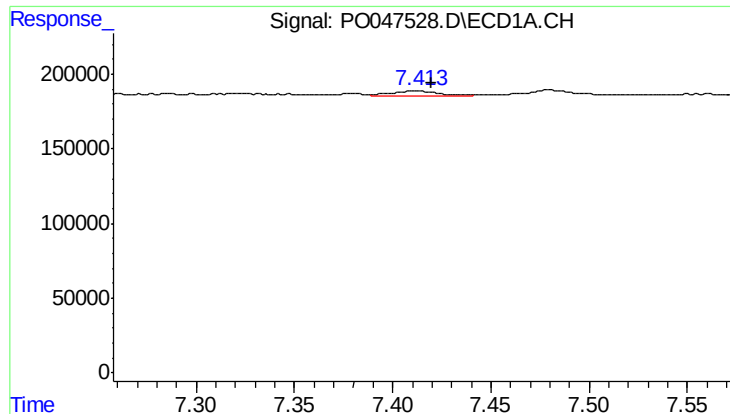

#37 AR-1262-2


R.T.: 7.413 min
Delta R.T.: -0.007 min
Response: 51069
Conc: 5.27 ng/ml

Instrument :
ECD_O
ClientSampleId :
2018-NYSEG-CLARK-AREA-14-2

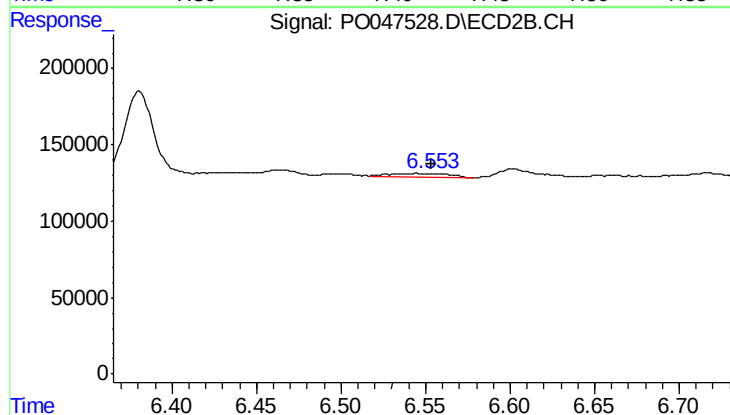


#37 AR-1262-2

R.T.: 6.545 min
Delta R.T.: -0.008 min
Response: 55019
Conc: 4.88 ng/ml

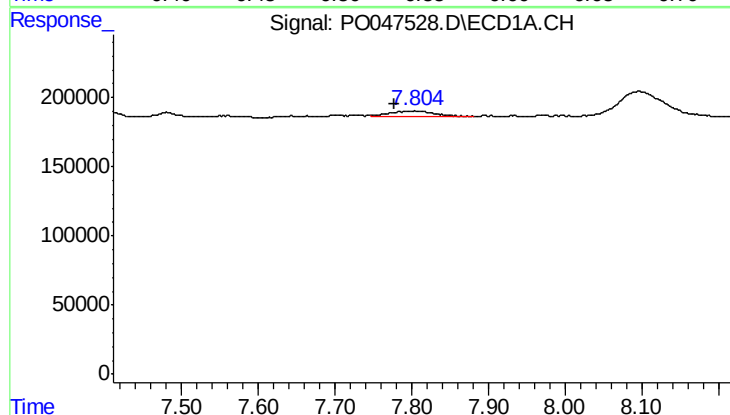


#38 AR-1262-3

R.T.: 7.804 min
Delta R.T.: 0.027 min
Response: 165186
Conc: 13.46 ng/ml

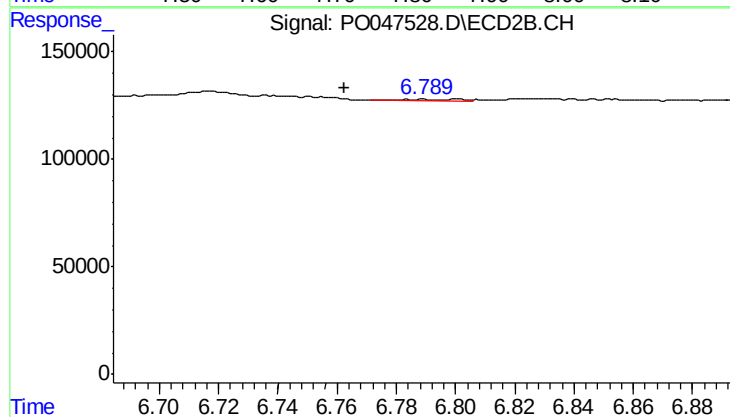

#38 AR-1262-3


R.T.: 6.788 min
Delta R.T.: 0.025 min
Response: 10350
Conc: 0.69 ng/ml

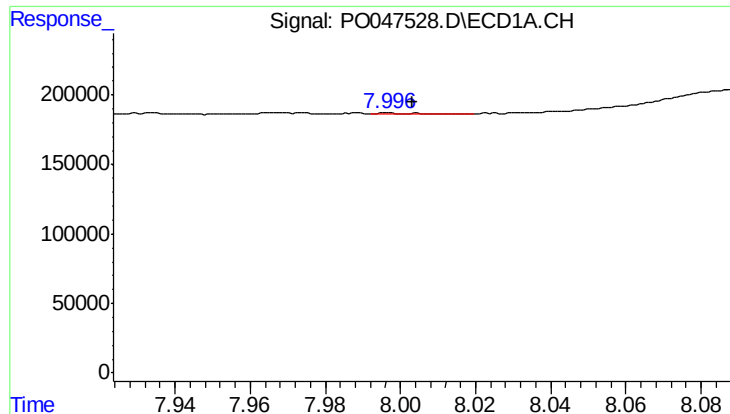

#39 AR-1262-4


R.T.: 7.997 min
Delta R.T.: -0.006 min
Response: 11541
Conc: 0.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
2018-NYSEG-CLARK-AREA-14-2

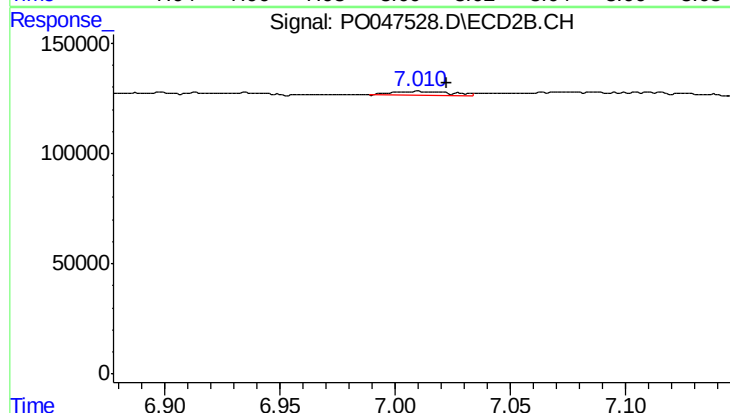


#39 AR-1262-4

R.T.: 7.011 min
Delta R.T.: -0.011 min
Response: 29886
Conc: 2.27 ng/ml

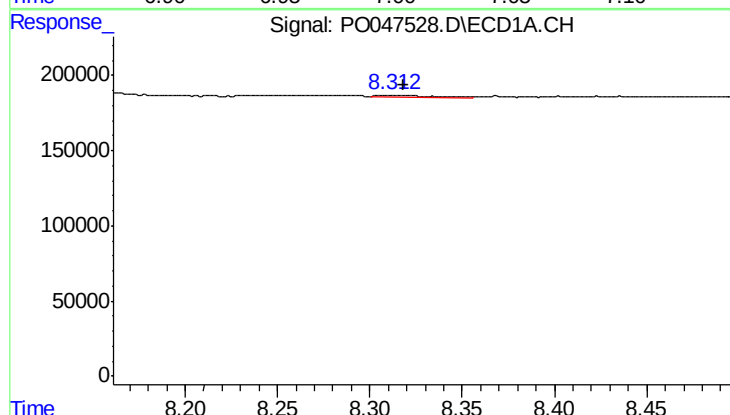


#40 AR-1262-5

R.T.: 8.311 min
Delta R.T.: -0.007 min
Response: 28000
Conc: 1.30 ng/ml

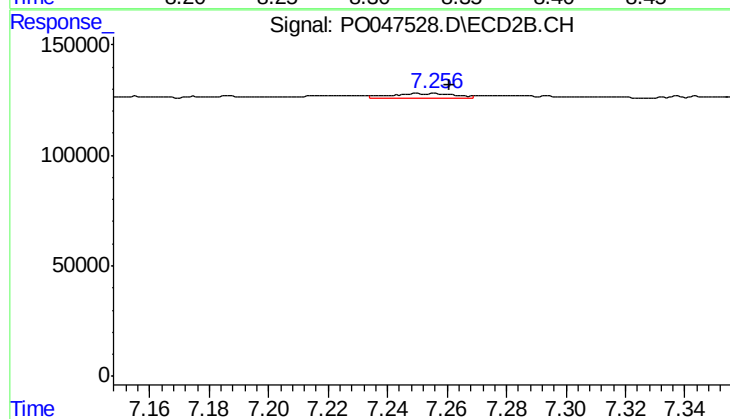

#40 AR-1262-5


R.T.: 7.253 min
Delta R.T.: -0.008 min
Response: 32740
Conc: 1.27 ng/ml

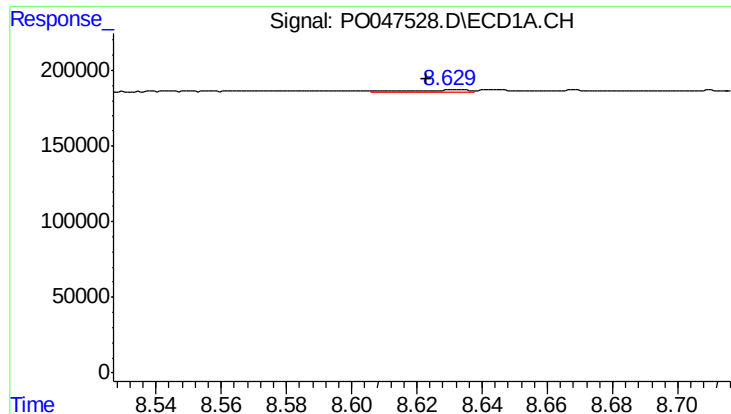

#41 AR-1268-1


R.T.: 8.632 min
Delta R.T.: 0.009 min
Response: 15779
Conc: 0.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
2018-NYSEG-CLARK-AREA-14-2

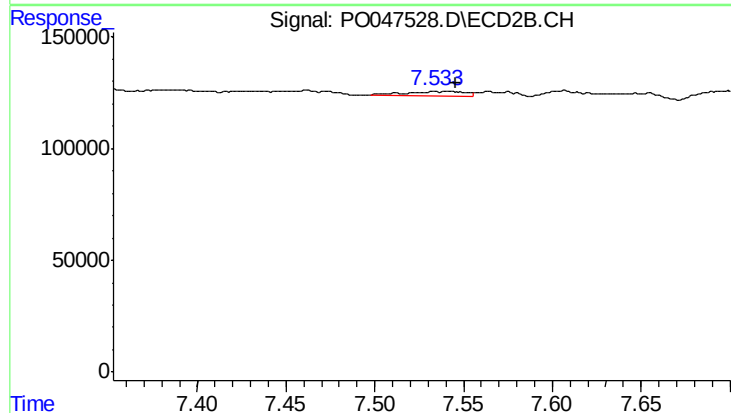


#41 AR-1268-1

R.T.: 7.535 min
Delta R.T.: -0.011 min
Response: 50249
Conc: 1.93 ng/ml

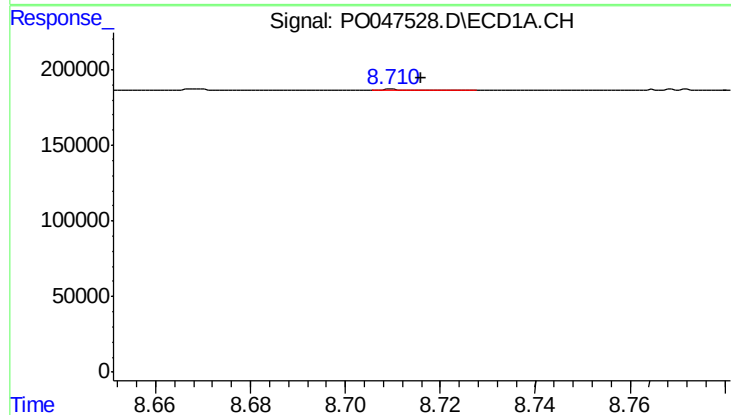


#42 AR-1268-2

R.T.: 8.710 min
Delta R.T.: -0.005 min
Response: 6257
Conc: 0.29 ng/ml

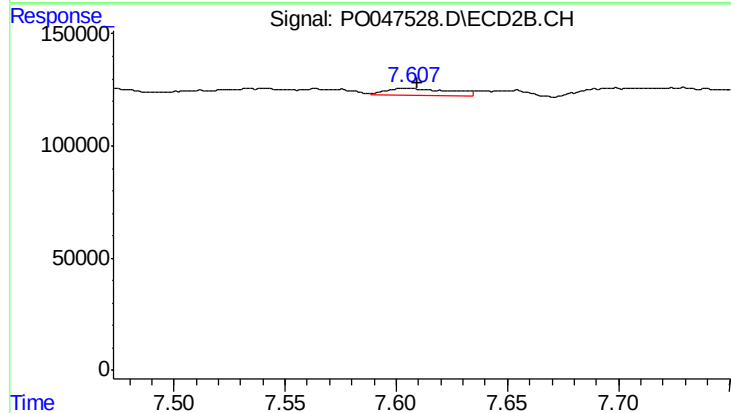

#42 AR-1268-2


R.T.: 7.606 min
Delta R.T.: -0.003 min
Response: 63829
Conc: 2.56 ng/ml

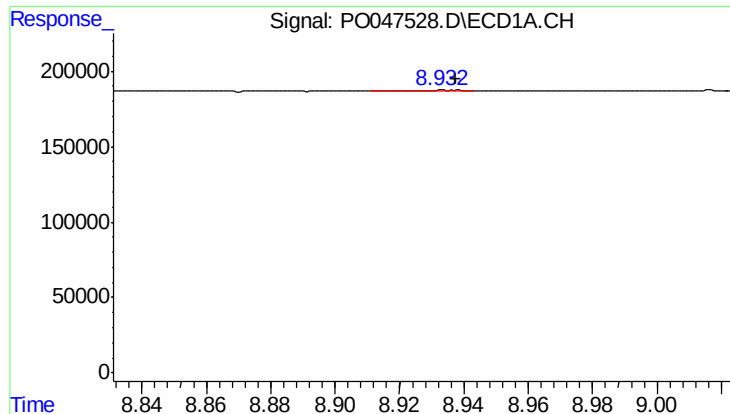

#43 AR-1268-3


R.T.: 8.933 min
Delta R.T.: -0.004 min
Response: 9598
Conc: 0.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
2018-NYSEG-CLARK-AREA-14-2

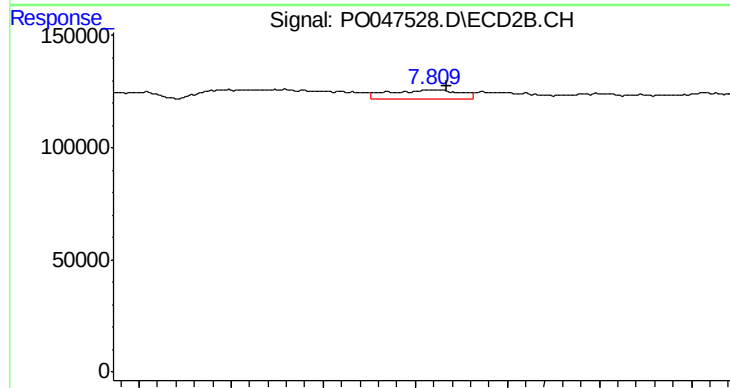


#43 AR-1268-3

R.T.: 7.809 min
Delta R.T.: -0.008 min
Response: 100906
Conc: 5.11 ng/ml

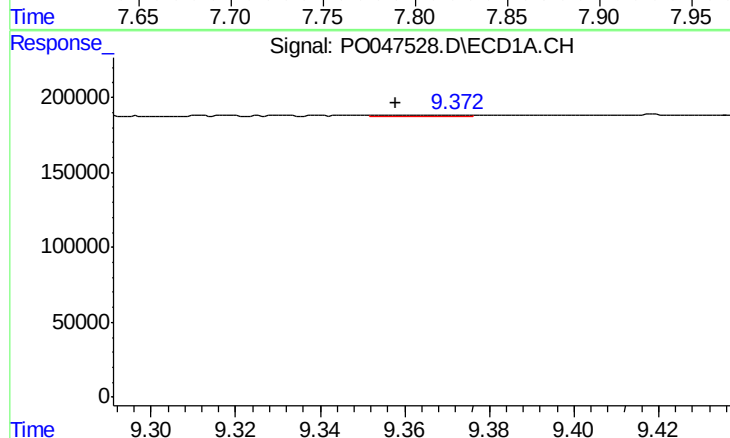


#44 AR-1268-4

R.T.: 9.359 min
Delta R.T.: 0.001 min
Response: 8337
Conc: 1.05 ng/ml

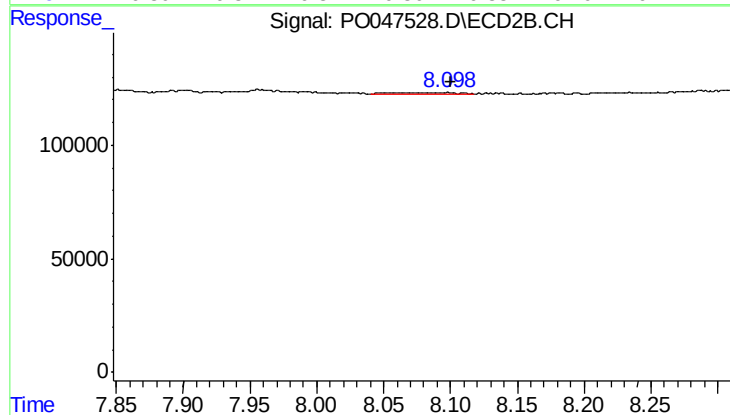

#44 AR-1268-4


R.T.: 8.097 min
Delta R.T.: -0.004 min
Response: 31143
Conc: 3.71 ng/ml

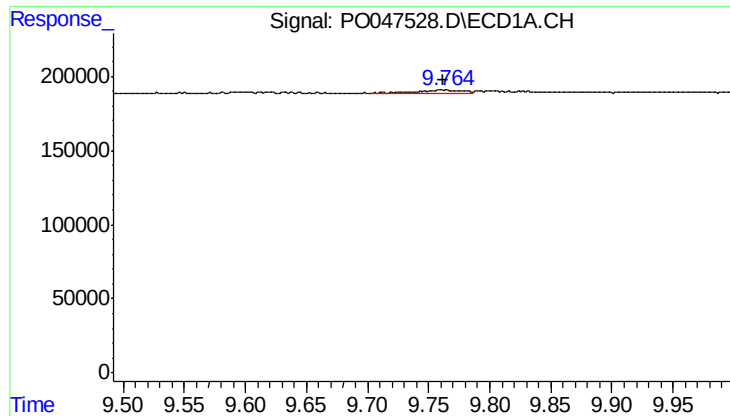

#45 AR-1268-5

R.T.: 9.764 min
Delta R.T.: 0.002 min
Response: 60819
Conc: 1.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
2018-NYSEG-CLARK-AREA-14-2

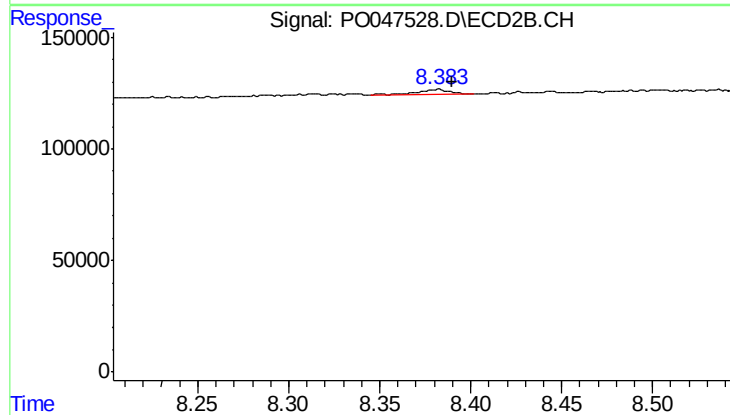

#45 AR-1268-5

R.T.: 8.381 min
Delta R.T.: -0.008 min
Response: 37829
Conc: 0.69 ng/ml