

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0080118\
Data File : P0047502.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Aug 2018 10:07
Operator : SM/SJ
Sample : J4176-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SV26835

Manual Integrations
APPROVED

Sohil
8/2/2018 9:43:06 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 11:58:17 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 27 02:33:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.405	3.646	1014813	1206787	5.026	4.911m
2) SA Decachlor...	10.099	8.637	579222	581707	3.551	3.701

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0080118\
Data File : P0047502.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Aug 2018 10:07
Operator : SM/SJ
Sample : J4176-01
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SV26835


Manual Integrations
APPROVED

Sohil
8/2/2018 9:43:06 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 11:58:17 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 27 02:33:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

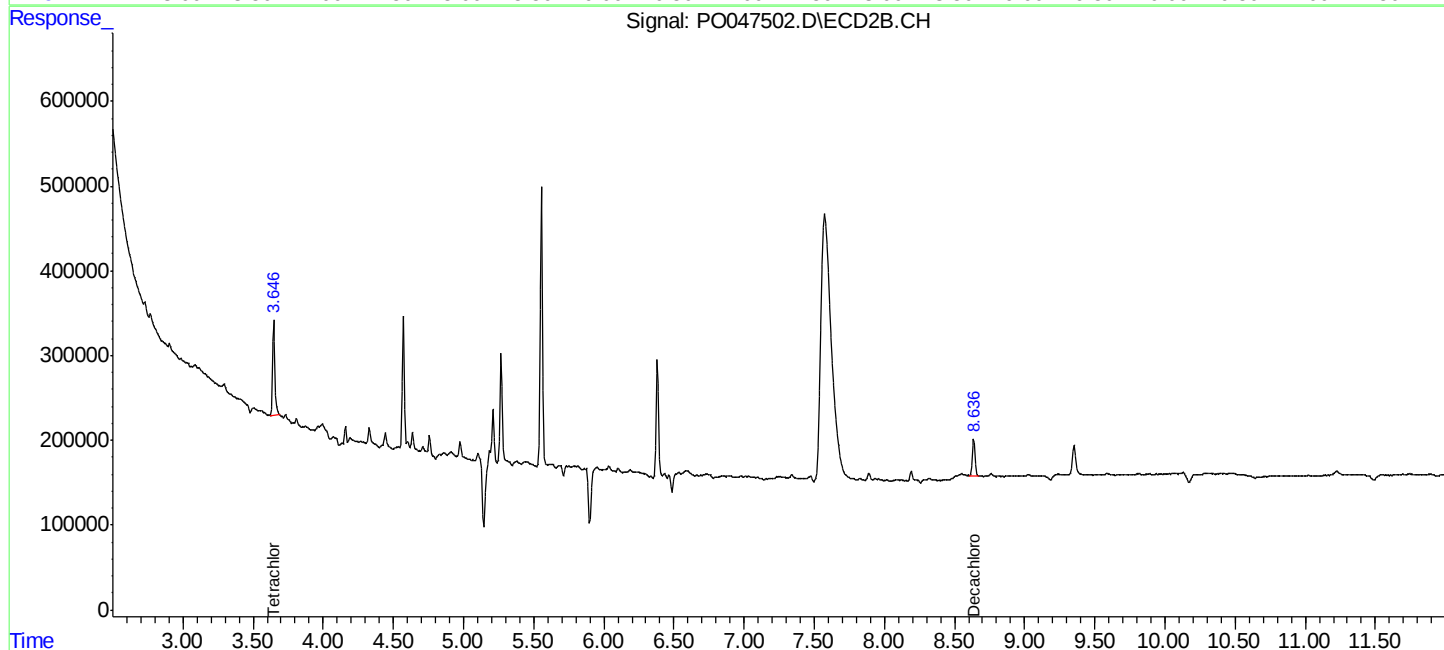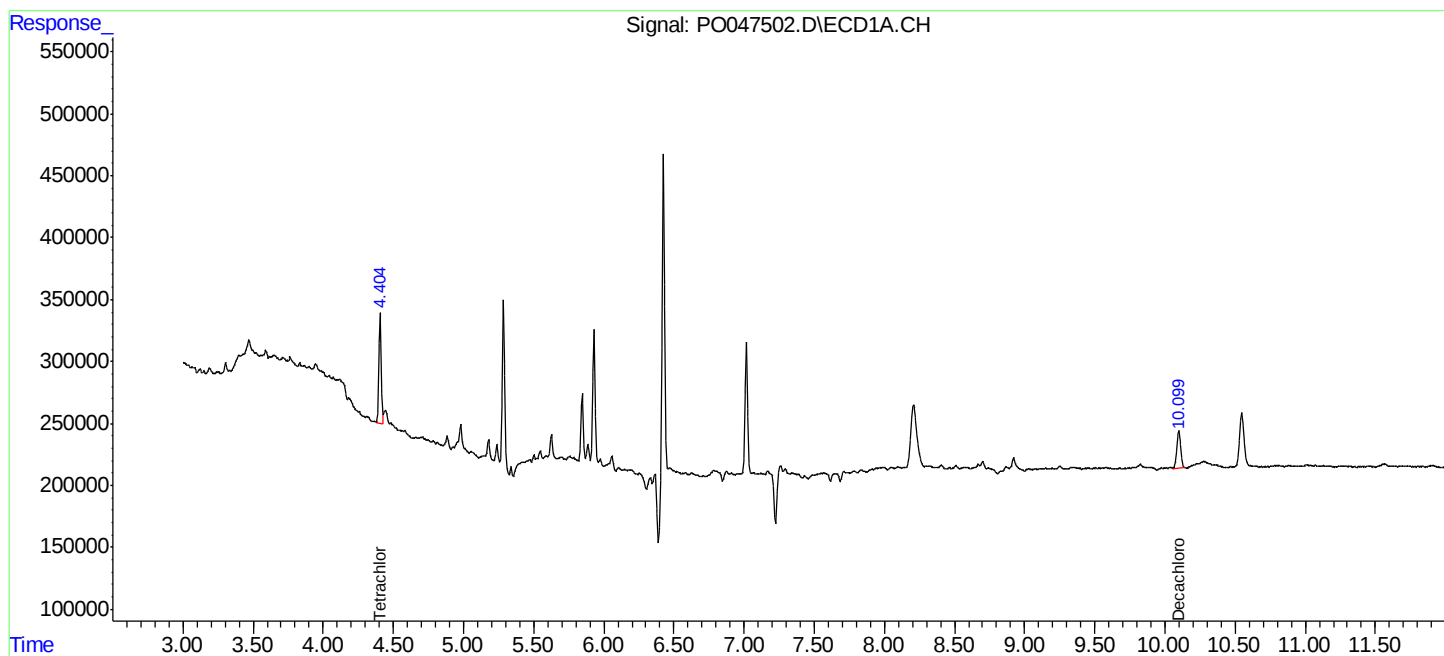

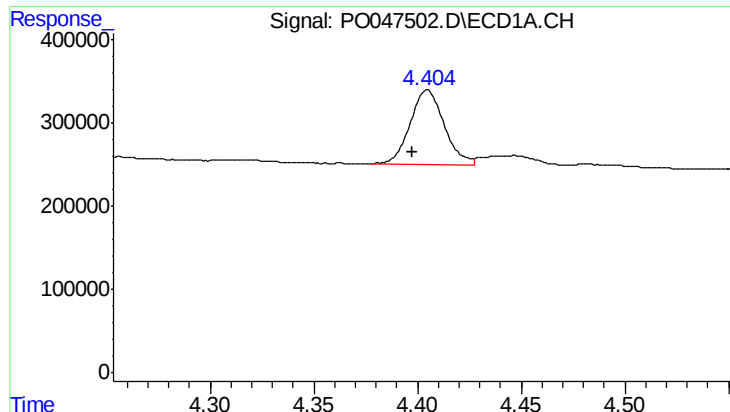


#1 Tetrachloro-m-xylene

R.T.: 4.405 min
Delta R.T.: 0.007 min
Response: 1014813
Conc: 5.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
SV26835


Manual Integrations
APPROVED

Sohil
8/2/2018 9:43:06 AM

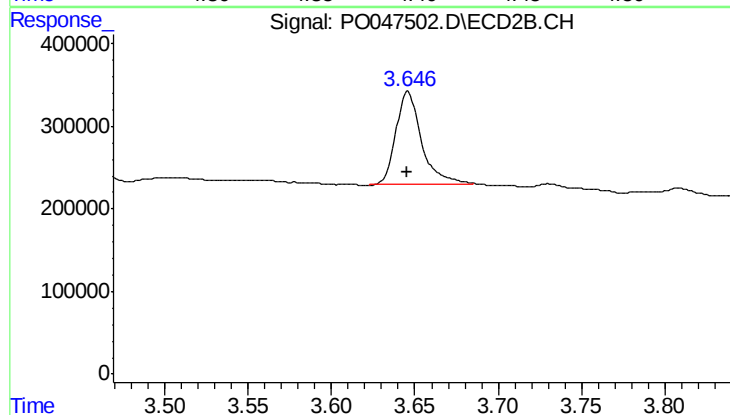


#1 Tetrachloro-m-xylene

R.T.: 3.646 min
Delta R.T.: 0.000 min
Response: 1206787
Conc: 4.91 ng/ml m

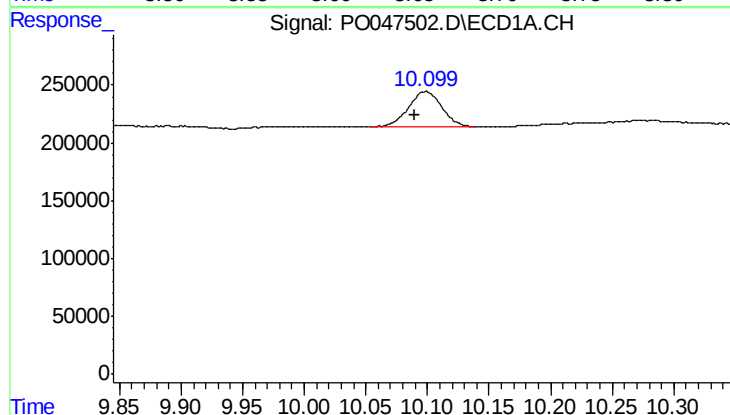

#2 Decachlorobiphenyl

R.T.: 10.099 min
Delta R.T.: 0.009 min
Response: 579222
Conc: 3.55 ng/ml

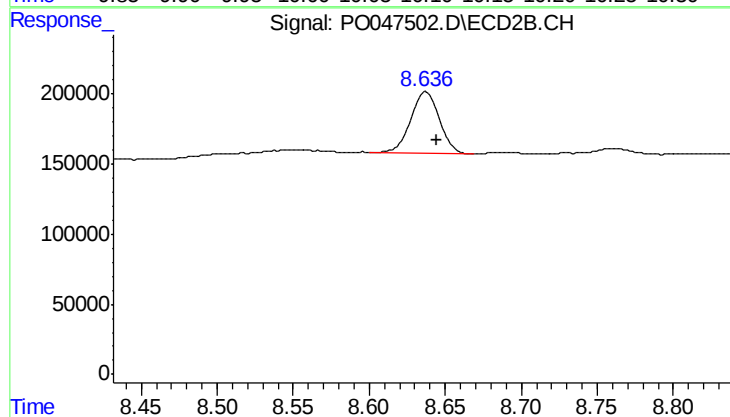

#2 Decachlorobiphenyl

R.T.: 8.637 min
Delta R.T.: -0.007 min
Response: 581707
Conc: 3.70 ng/ml