

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0080118\
 Data File : P0047503.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Aug 2018 10:23
 Operator : SM/SJ
 Sample : J4200-05
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CA-DRUM-2-BASELINEWATER

Manual Integrations
 APPROVED

Sohil
 8/2/2018 9:43:07 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 12:02:28 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jul 27 02:33:29 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.399	3.646	2892945	3275888	14.329m	13.332
2) SA Decachlor...	10.091	8.636	1228219	1170867	7.530	7.449m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0080118\
Data File : P0047503.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Aug 2018 10:23
Operator : SM/SJ
Sample : J4200-05
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CA-DRUM-2-BASELINEWATER


Manual Integrations
APPROVED

Sohil
8/2/2018 9:43:07 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 12:02:28 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 27 02:33:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

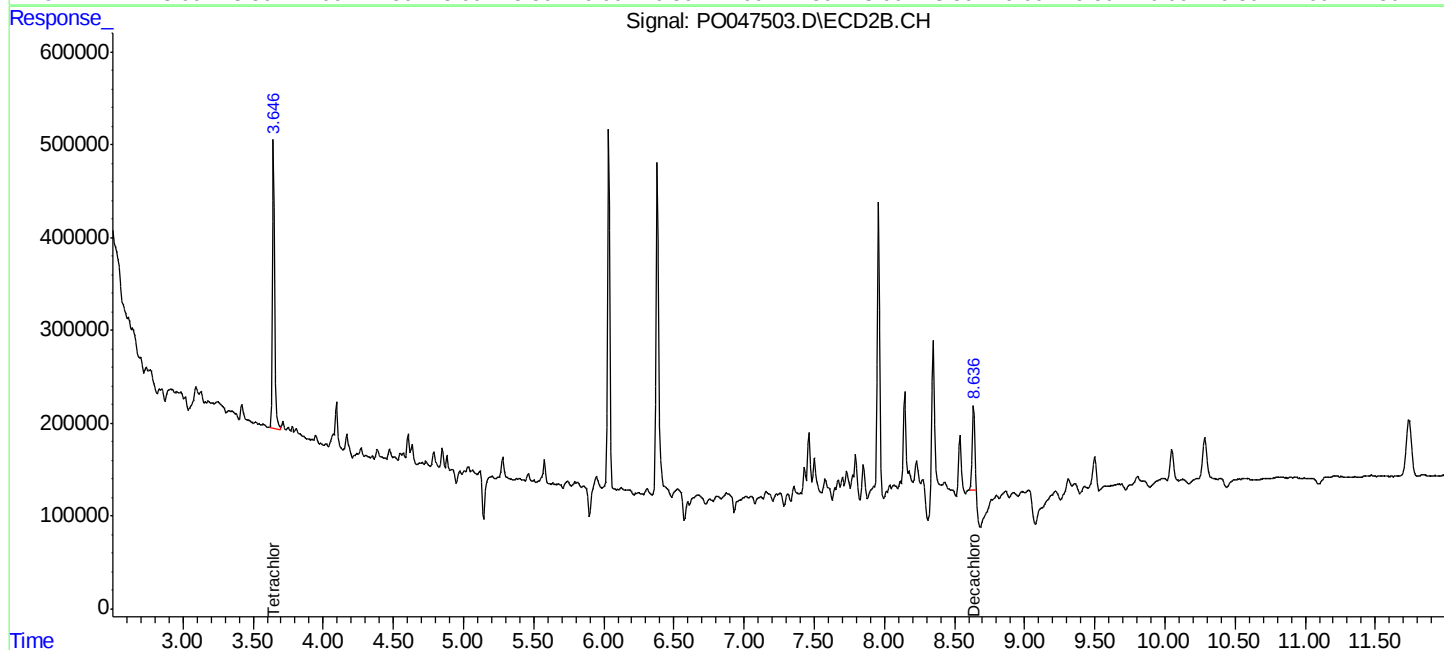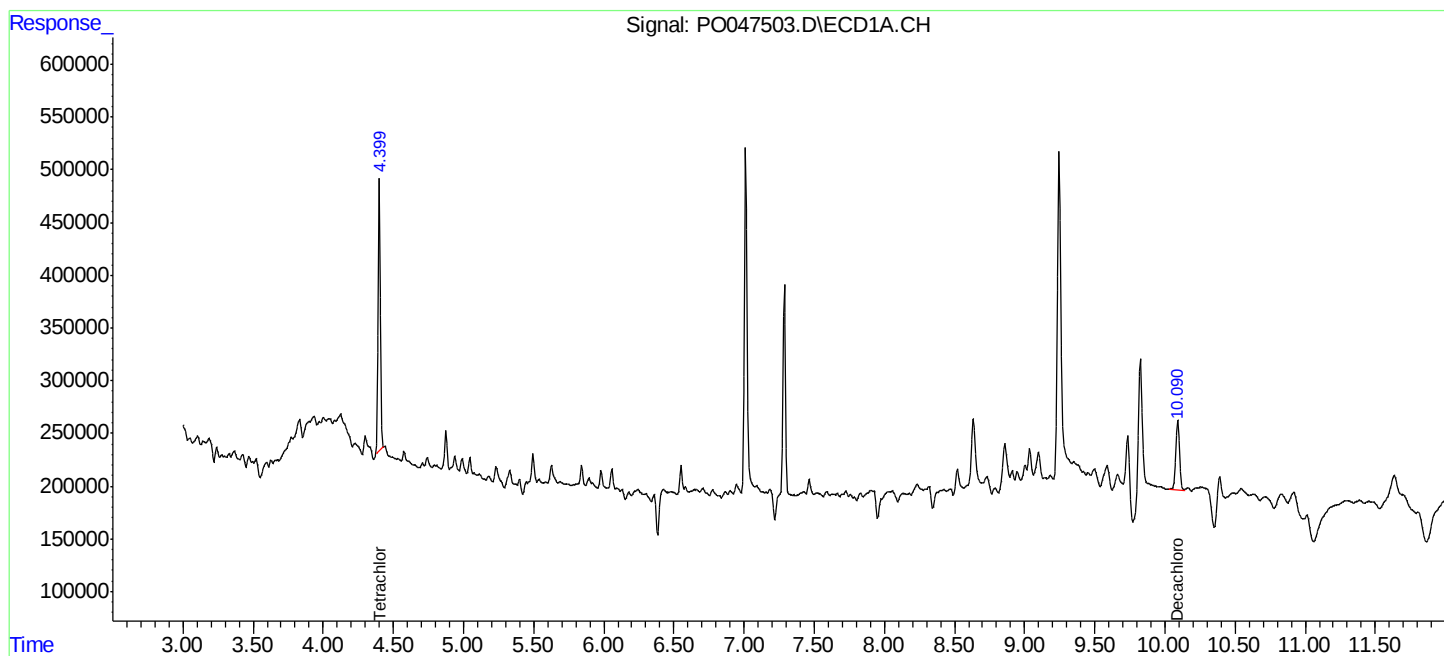

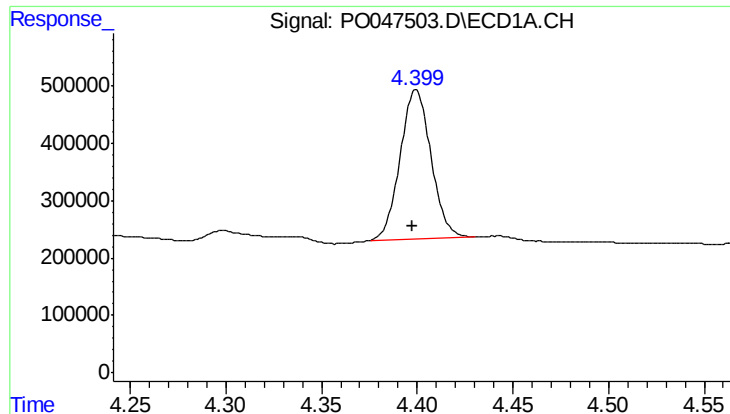


#1 Tetrachloro-m-xylene

R.T.: 4.399 min
Delta R.T.: 0.002 min
Response: 2892945
Conc: 14.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
CA-DRUM-2-BASELINEWATER


Manual Integrations
APPROVED

Sohil
8/2/2018 9:43:07 AM

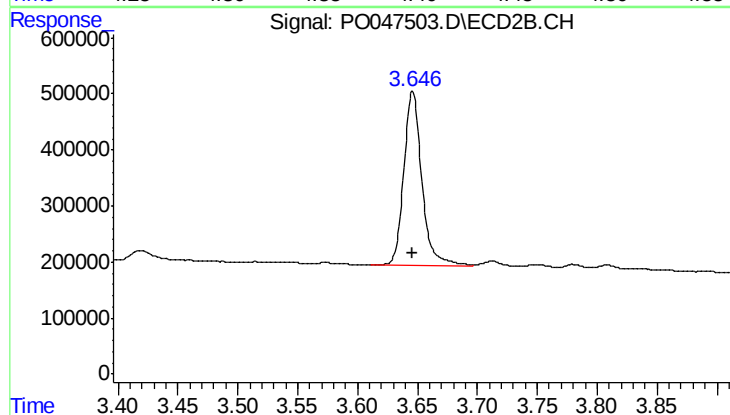


#1 Tetrachloro-m-xylene

R.T.: 3.646 min
Delta R.T.: 0.000 min
Response: 3275888
Conc: 13.33 ng/ml

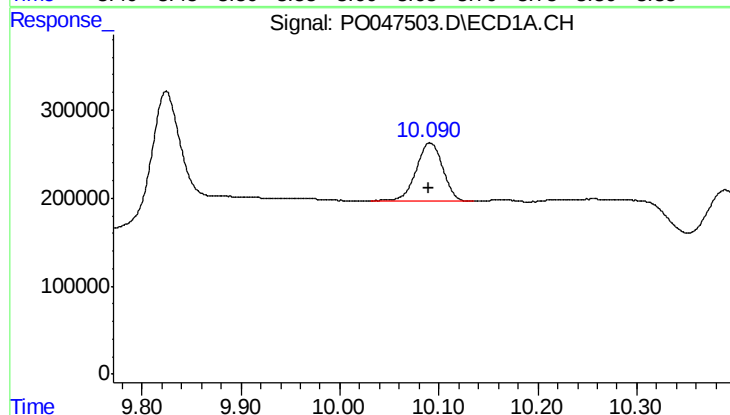

#2 Decachlorobiphenyl

R.T.: 10.091 min
Delta R.T.: 0.001 min
Response: 1228219
Conc: 7.53 ng/ml

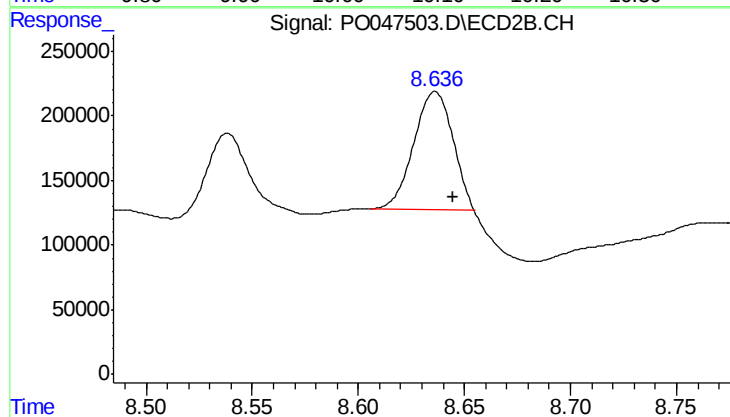

#2 Decachlorobiphenyl

R.T.: 8.636 min
Delta R.T.: -0.009 min
Response: 1170867
Conc: 7.45 ng/ml m