

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0080118\
Data File : P0047504.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Aug 2018 10:39
Operator : SM/SJ
Sample : J4255-01 10X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
A456930

Manual Integrations
APPROVED

Sohil
8/2/2018 9:43:08 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 12:04:08 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 27 02:33:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.396	3.646	386500	184424	1.914	0.751m#
2)	SA Decachlor...	10.091	8.636	293475	279526	1.799	1.778m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\PO080118\
Data File : PO047504.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Aug 2018 10:39
Operator : SM/SJ
Sample : J4255-01 10X
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
A456930


Manual Integrations
APPROVED

Sohil
8/2/2018 9:43:08 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 12:04:08 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO072718.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 27 02:33:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

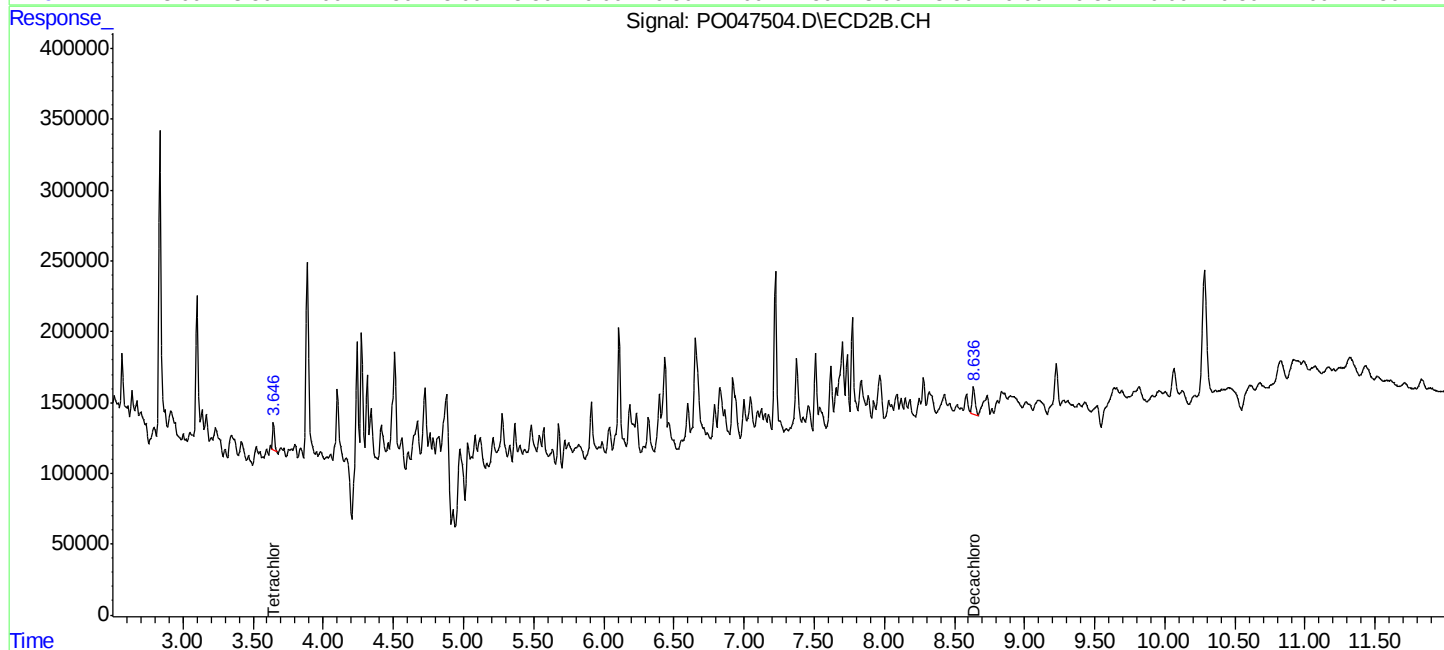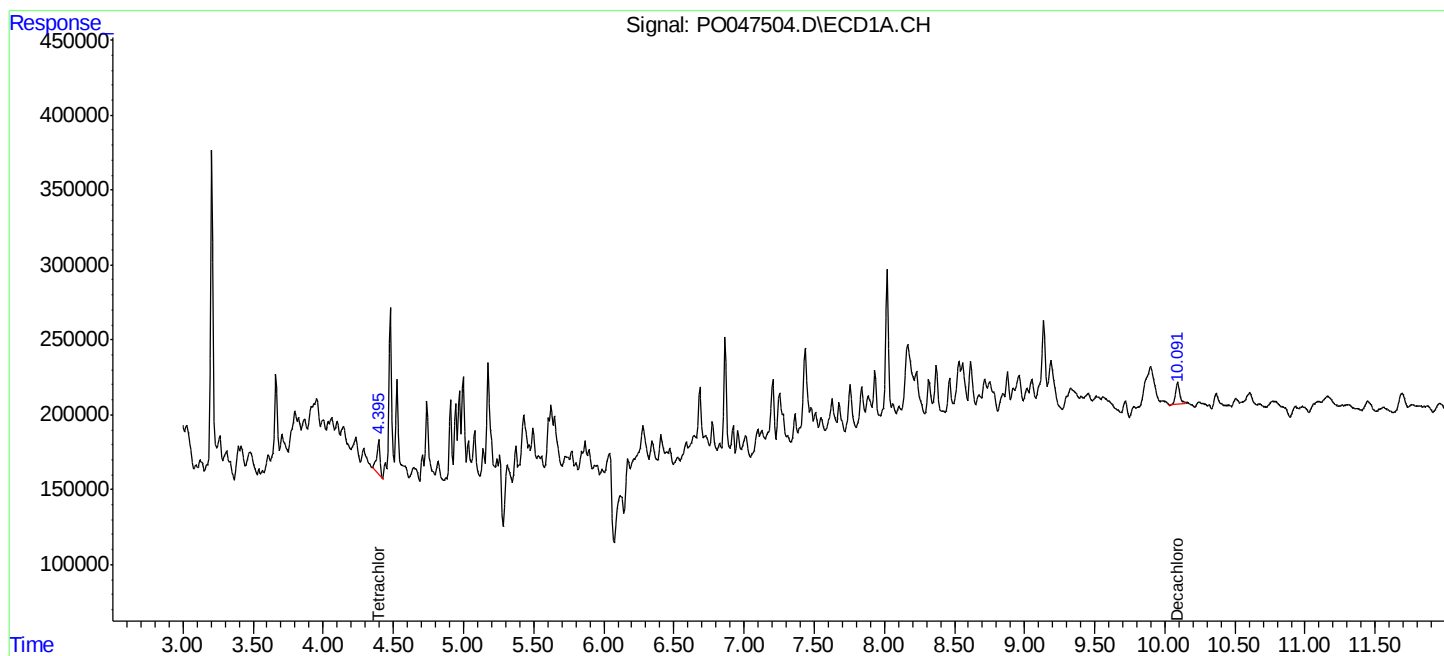

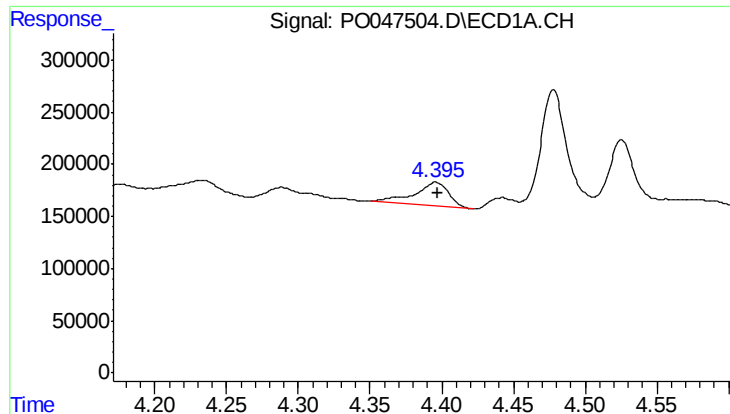


#1 Tetrachloro-m-xylene

R.T.: 4.396 min
Delta R.T.: -0.002 min
Response: 386500
Conc: 1.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
A456930


Manual Integrations
APPROVED

Sohil
8/2/2018 9:43:08 AM

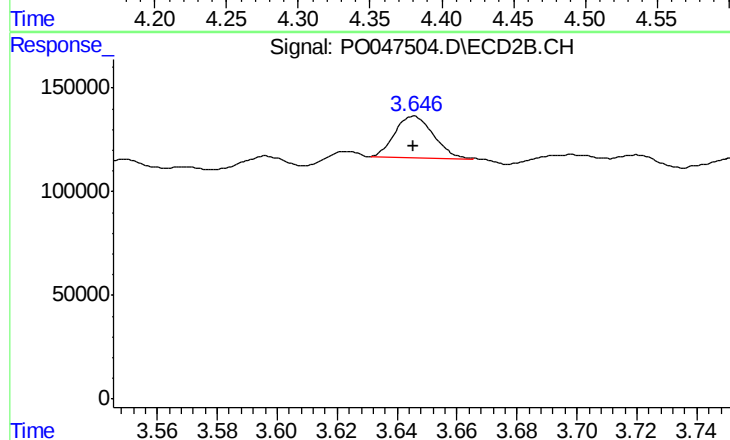


#1 Tetrachloro-m-xylene

R.T.: 3.646 min
Delta R.T.: 0.000 min
Response: 184424
Conc: 0.75 ng/ml m

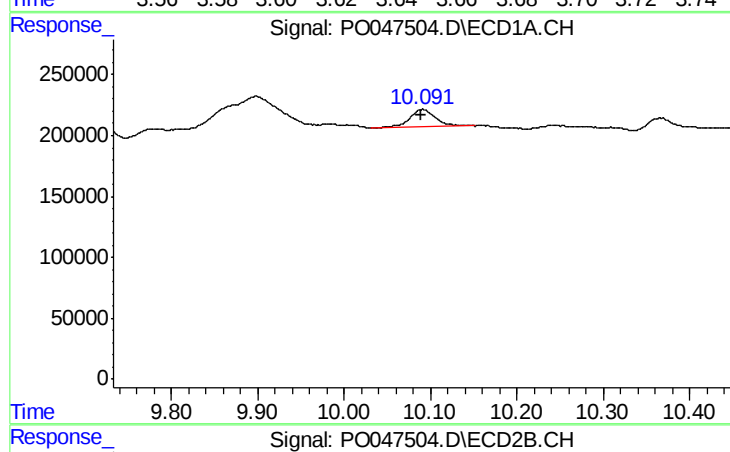

#2 Decachlorobiphenyl

R.T.: 10.091 min
Delta R.T.: 0.001 min
Response: 293475
Conc: 1.80 ng/ml

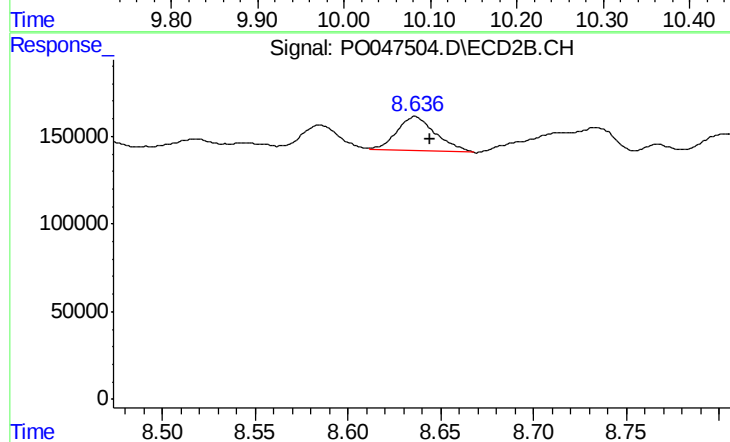

#2 Decachlorobiphenyl

R.T.: 8.636 min
Delta R.T.: -0.009 min
Response: 279526
Conc: 1.78 ng/ml m