

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0080118\
Data File : P0047513.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Aug 2018 13:07
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 14:23:09 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 27 02:33:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.400	3.647	3046478	3533572	15.089	14.381
2) SA Decachlor...	10.090	8.635	2822562	2811240	17.306	17.884

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0080118\
Data File : P0047513.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Aug 2018 13:07
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 14:23:09 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 27 02:33:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

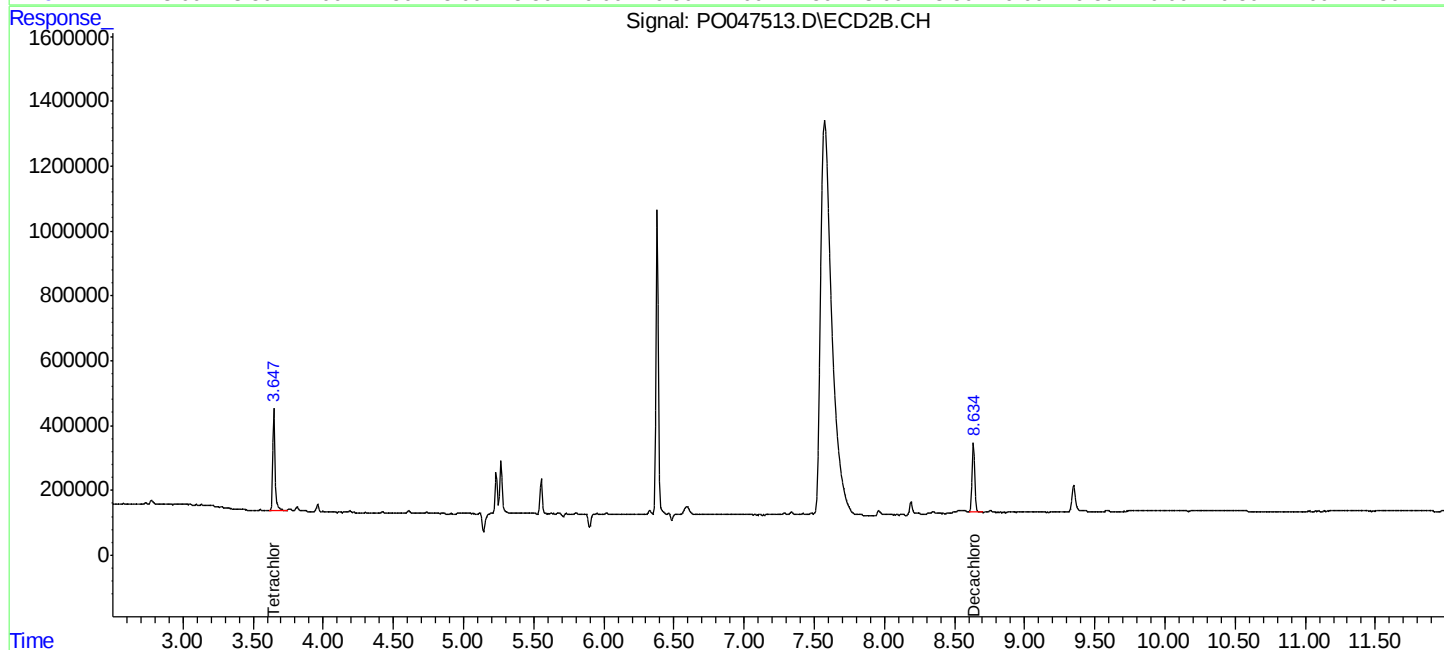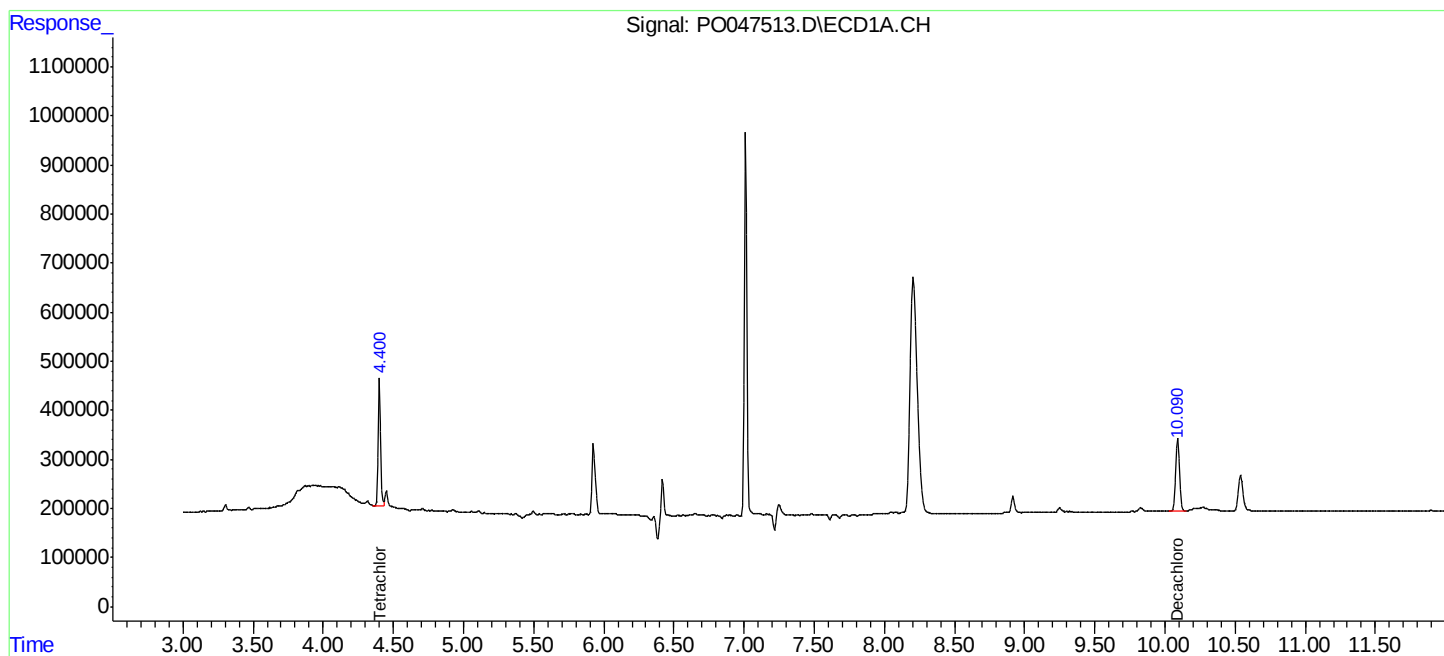


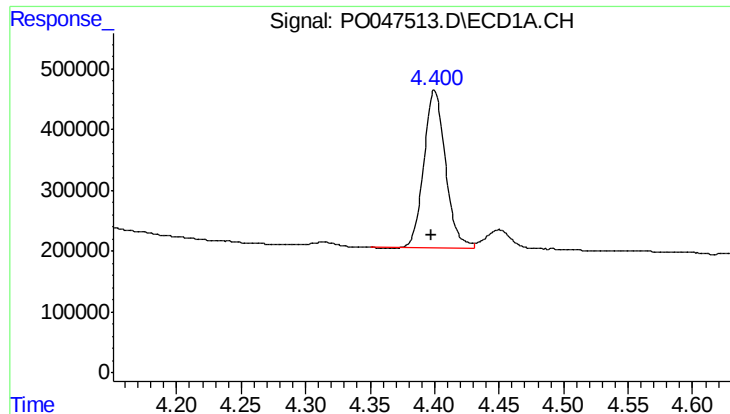

#1 Tetrachloro-m-xylene


R.T.: 4.400 min
Delta R.T.: 0.003 min
Response: 3046478
Conc: 15.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

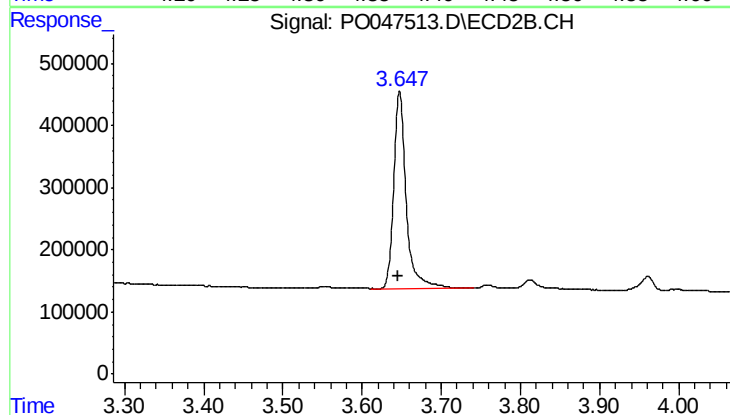


#1 Tetrachloro-m-xylene

R.T.: 3.647 min
Delta R.T.: 0.002 min
Response: 3533572
Conc: 14.38 ng/ml

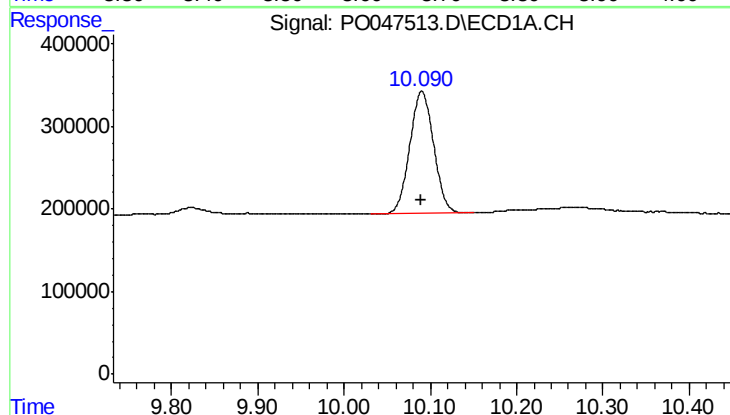

#2 Decachlorobiphenyl

R.T.: 10.090 min
Delta R.T.: 0.000 min
Response: 2822562
Conc: 17.31 ng/ml

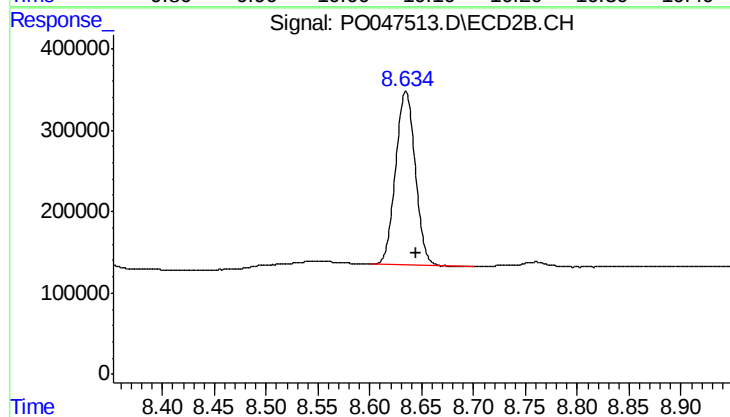

#2 Decachlorobiphenyl

R.T.: 8.635 min
Delta R.T.: -0.010 min
Response: 2811240
Conc: 17.88 ng/ml