

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0080118\
Data File : P0047534.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Aug 2018 20:12
Operator : SM/SJ
Sample : J4231-15
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
2018-NYSEG-CLARK-AREA-14-8

Manual Integrations
APPROVED

Sohil
8/2/2018 9:43:25 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 02:07:51 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 27 02:33:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.399	3.645	2951180	3768704	14.617m	15.338m
2)	SA Decachlor...	10.090	8.635	2009949	2113882	12.323	13.448

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0080118\
Data File : P0047534.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Aug 2018 20:12
Operator : SM/SJ
Sample : J4231-15
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
2018-NYSEG-CLARK-AREA-14-8


Manual Integrations
APPROVED

Sohil
8/2/2018 9:43:25 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 02:07:51 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 27 02:33:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

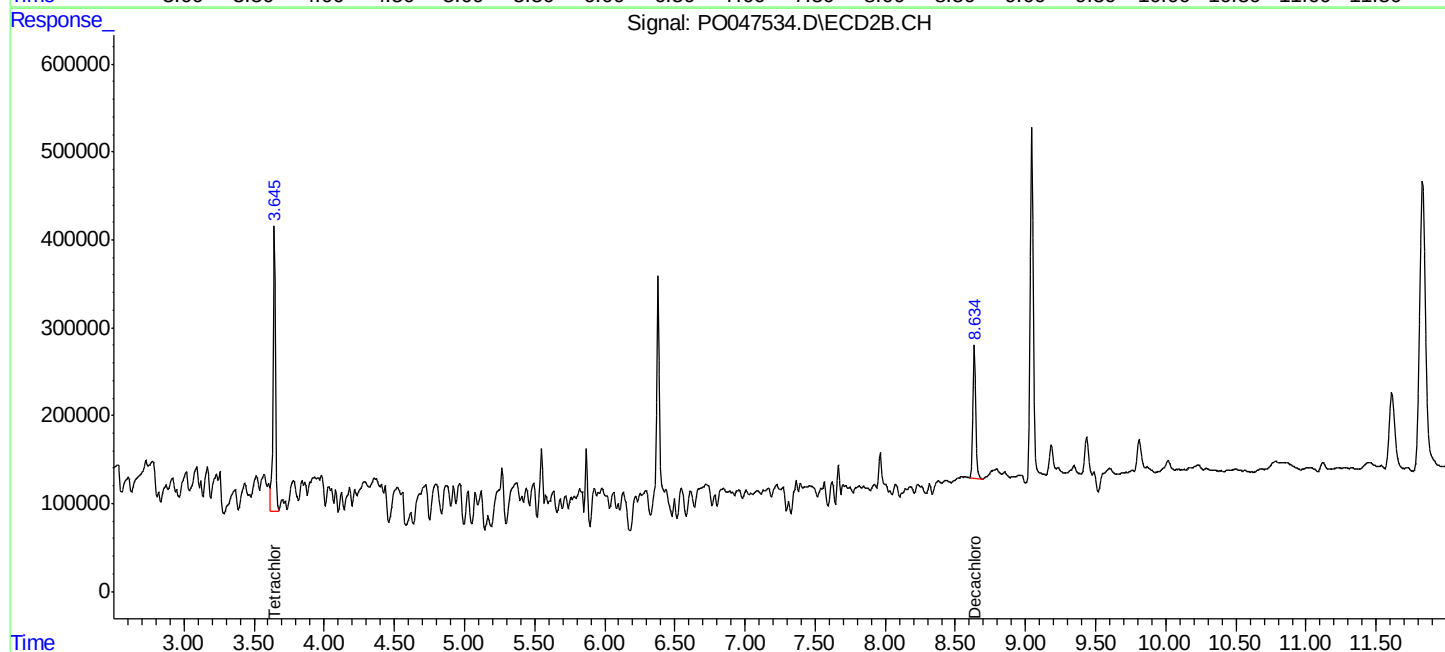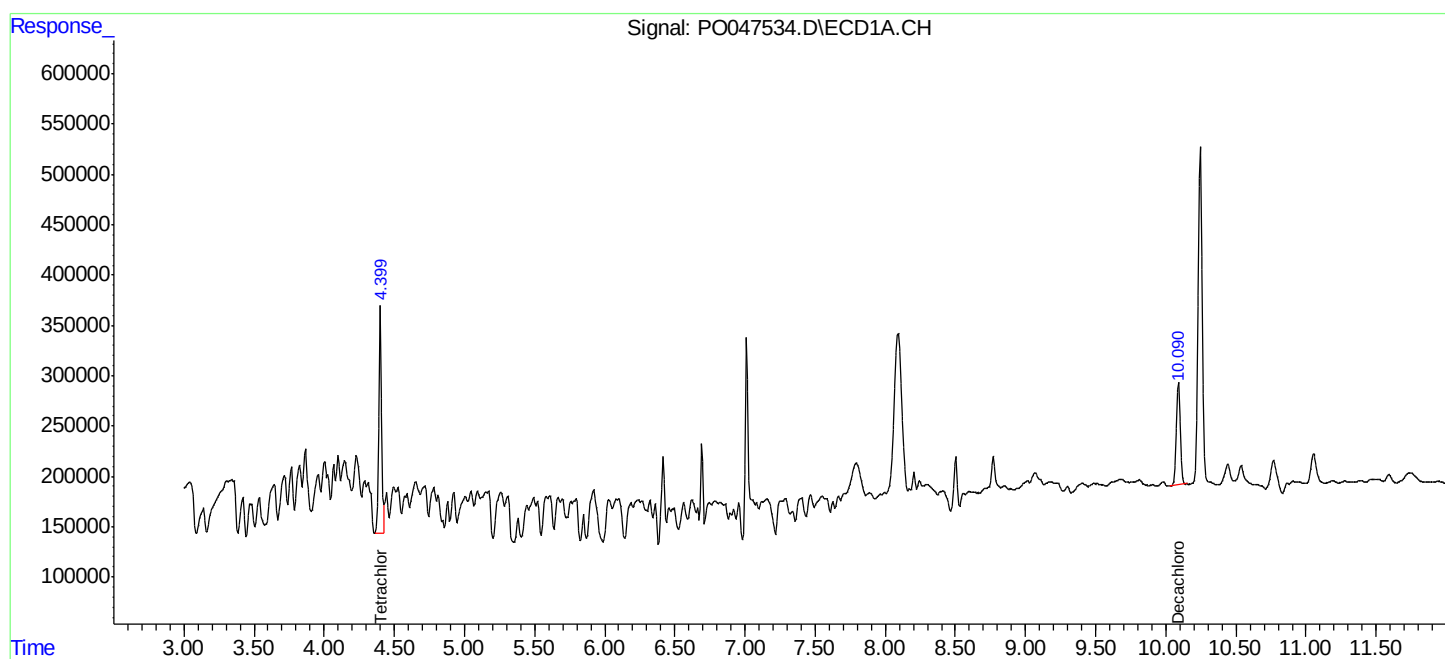

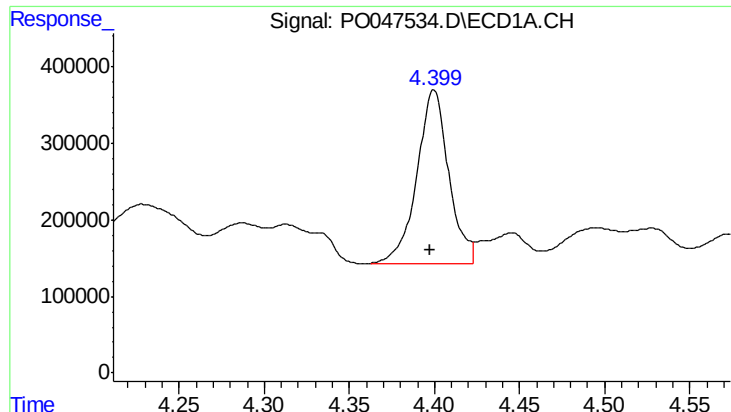


#1 Tetrachloro-m-xylene

R.T.: 4.399 min
 Delta R.T.: 0.002 min
 Response: 2951180
 Conc: 14.62 ng/ml

Instrument :
 ECD_O
 ClientSampleId :
 2018-NYSEG-CLARK-AREA-14-8


Manual Integrations
 APPROVED

Sohil
 8/2/2018 9:43:25 AM

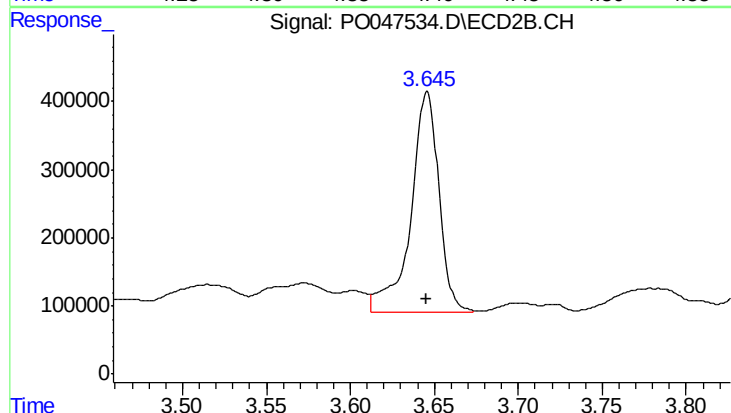


#1 Tetrachloro-m-xylene

R.T.: 3.645 min
 Delta R.T.: 0.000 min
 Response: 3768704
 Conc: 15.34 ng/ml m

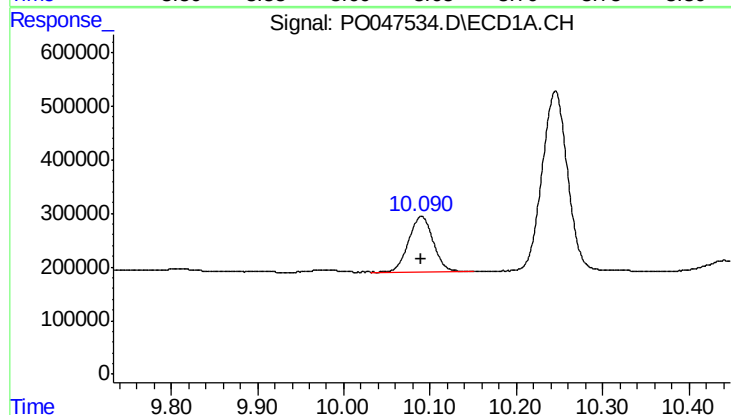

#2 Decachlorobiphenyl

R.T.: 10.090 min
 Delta R.T.: 0.000 min
 Response: 2009949
 Conc: 12.32 ng/ml

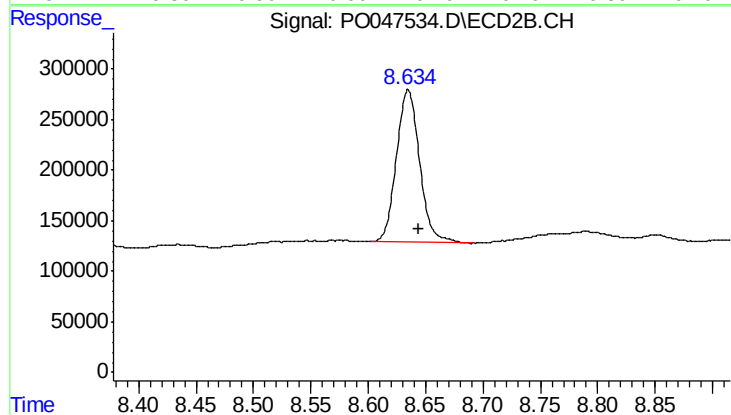

#2 Decachlorobiphenyl

R.T.: 8.635 min
 Delta R.T.: -0.010 min
 Response: 2113882
 Conc: 13.45 ng/ml