

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080119\
 Data File : P0058664.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Jul 2019 9:56
 Operator : SM/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 31 11:29:42 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jul 27 06:49:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.169	3.519	742352	664413	17.590	16.631
2)	SA Decachlor...	9.650	8.406	1191781	778905	22.007	19.733
Target Compounds							
32)	L7 AR-1260-2	0.000	6.218	0	16441	N.D.	5.427 #
35)	L7 AR-1260-5	0.000	7.076	0	242977	N.D.	45.118 #
37)	L8 AR-1262-2	0.000	7.076	0	242977	N.D.	43.035 #
38)	L8 AR-1262-3	0.000	7.353	0	168346	N.D.	68.210 #
39)	L8 AR-1262-4	0.000	7.415	0	145429	N.D.	34.249 #
41)	L9 AR-1268-1	0.000	7.353	0	168346	N.D.	20.669 #
42)	L9 AR-1268-2	0.000	7.415	0	145429	N.D.	19.193 #
43)	L9 AR-1268-3	0.000	7.663	0	144707	N.D.	22.639 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080119\
Data File : PO058664.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Jul 2019 9:56
Operator : SM/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 31 11:29:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072819.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 27 06:49:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

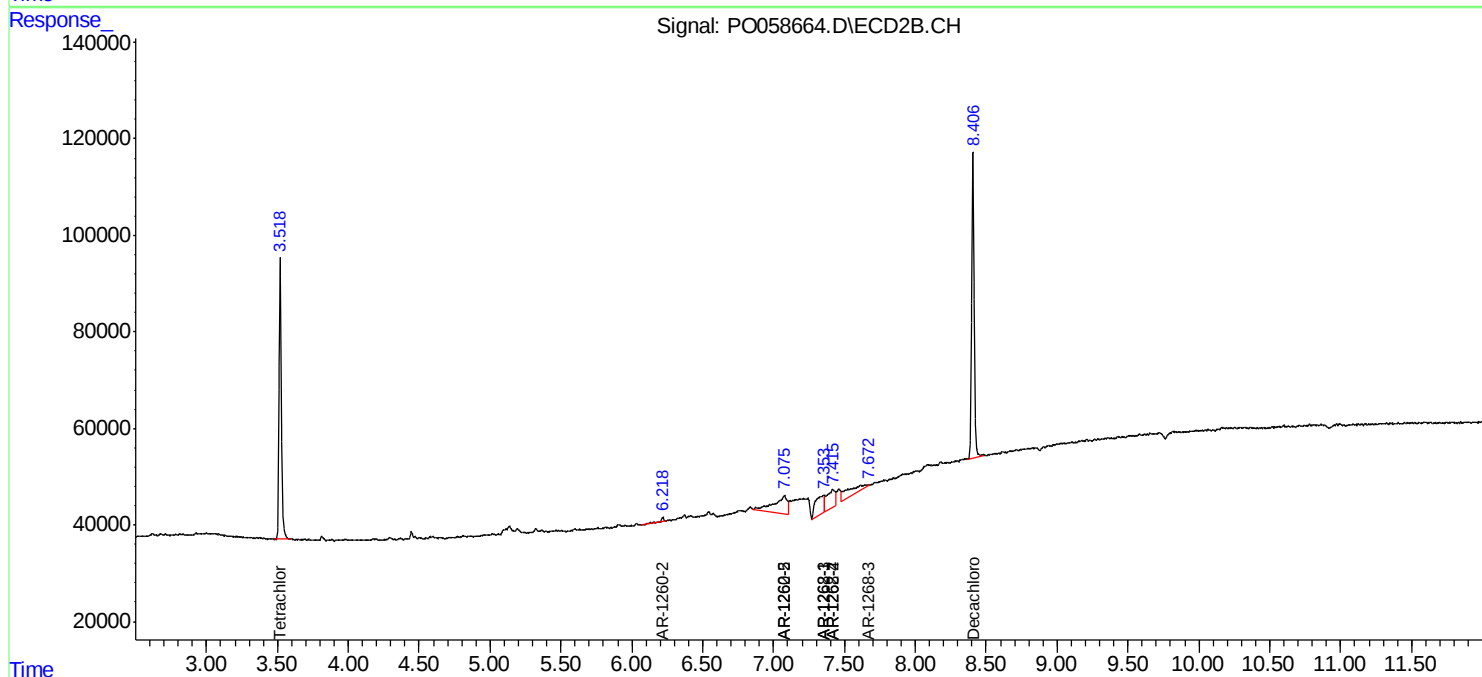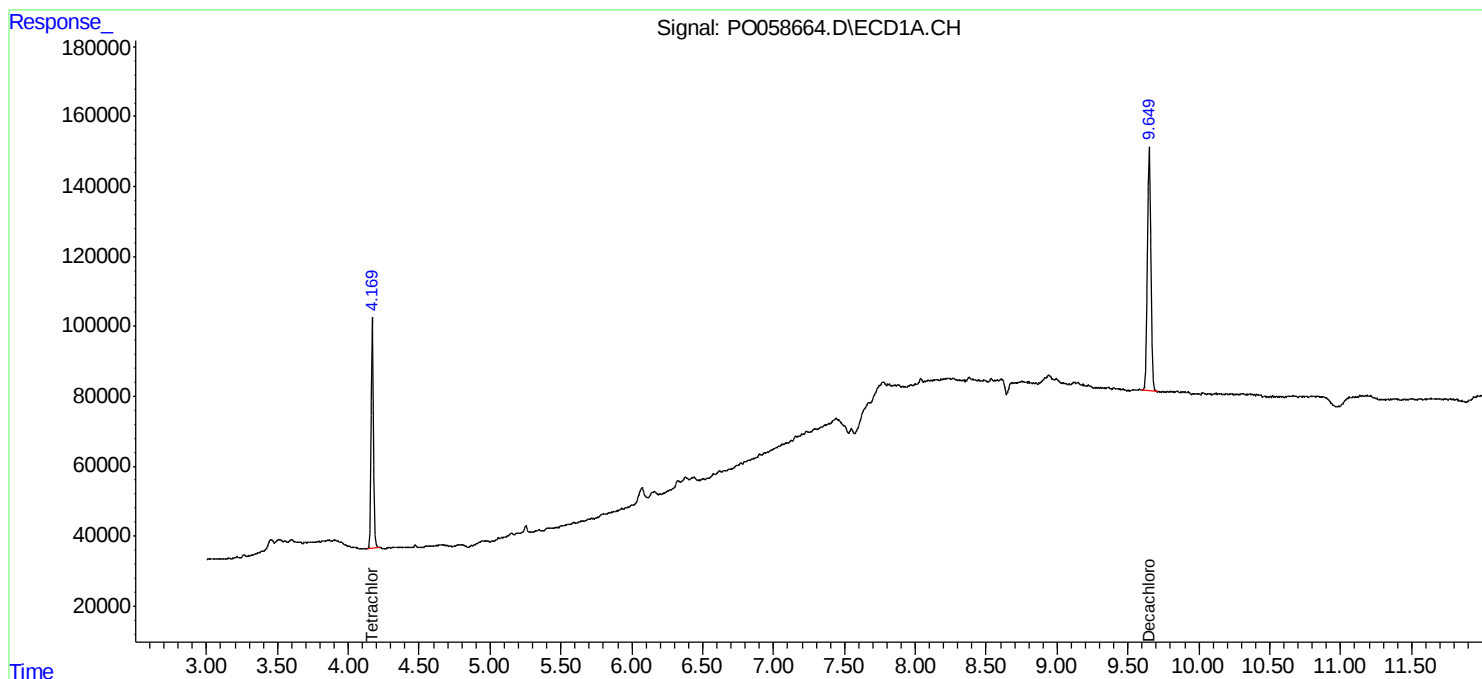


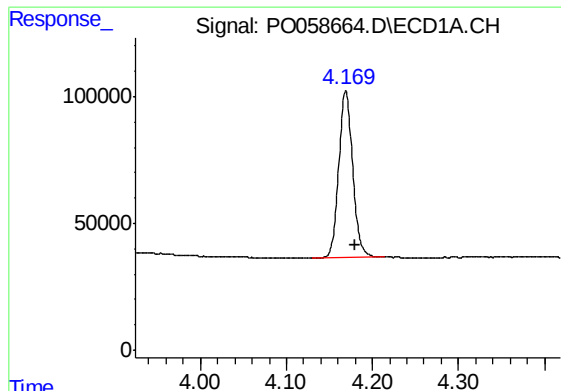

#1 Tetrachloro-m-xylene


R.T.: 4.169 min
Delta R.T.: -0.010 min
Response: 742352
Conc: 17.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

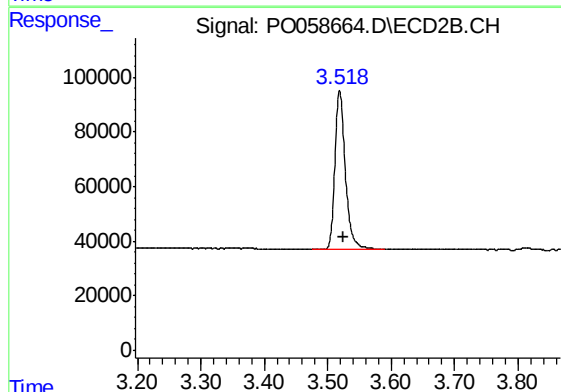


#1 Tetrachloro-m-xylene

R.T.: 3.519 min
Delta R.T.: -0.006 min
Response: 664413
Conc: 16.63 ng/ml

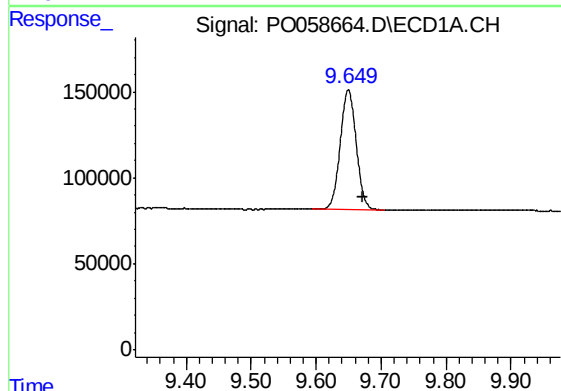


#2 Decachlorobiphenyl

R.T.: 9.650 min
Delta R.T.: -0.023 min
Response: 1191781
Conc: 22.01 ng/ml

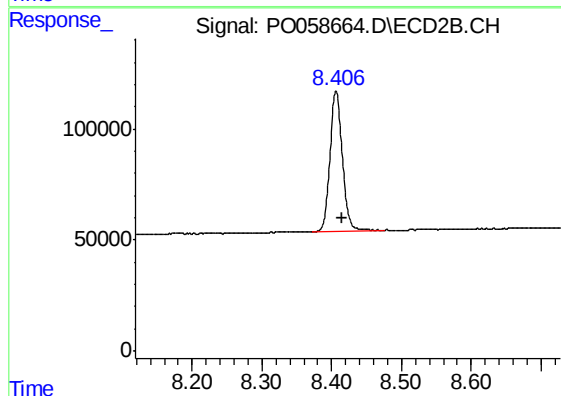

#2 Decachlorobiphenyl


R.T.: 8.406 min
Delta R.T.: -0.008 min
Response: 778905
Conc: 19.73 ng/ml

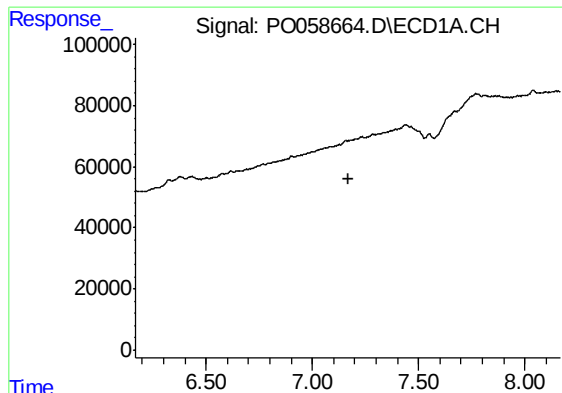

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T.: 7.167 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

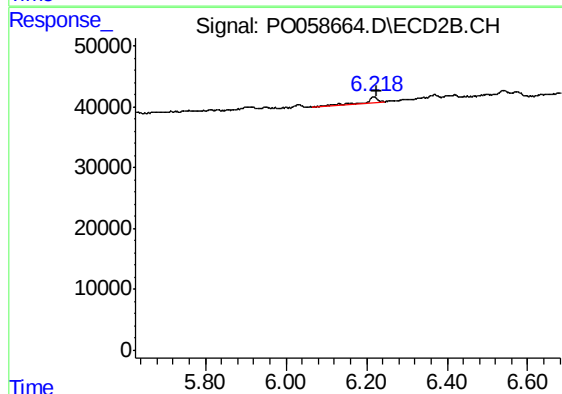


#32 AR-1260-2

R.T.: 6.218 min
Delta R.T.: -0.006 min
Response: 16441
Conc: 5.43 ng/ml

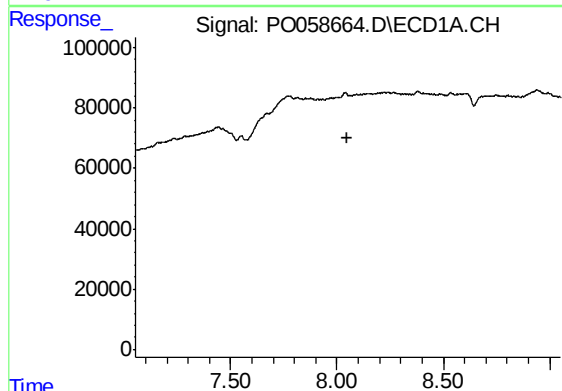


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T.: 8.051 min
Response: 0
Conc: N.D.

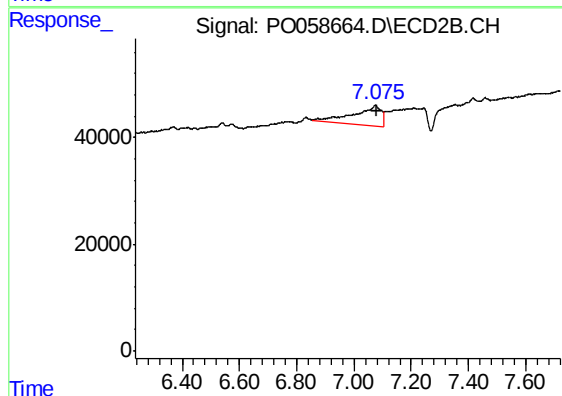

#35 AR-1260-5


R.T.: 7.076 min
Delta R.T.: -0.006 min
Response: 242977
Conc: 45.12 ng/ml

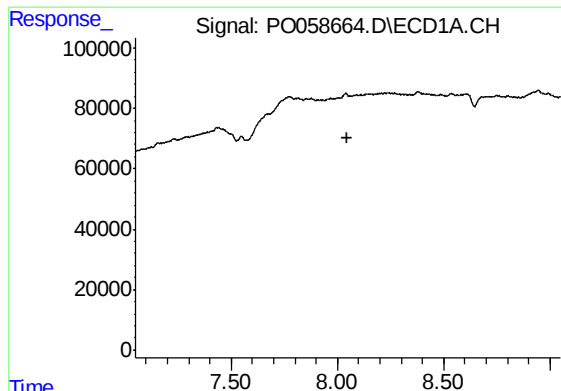

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T. : 8.050 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

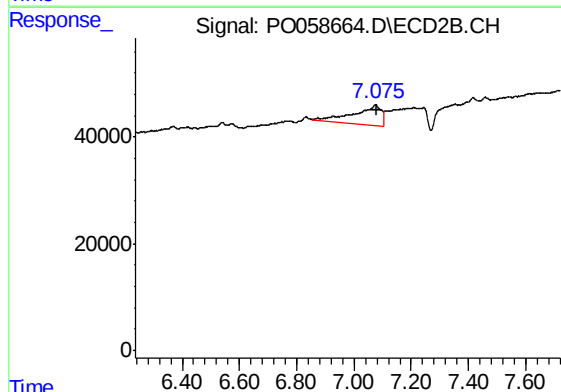


#37 AR-1262-2

R.T.: 7.076 min
Delta R.T.: -0.006 min
Response: 242977
Conc: 43.04 ng/ml

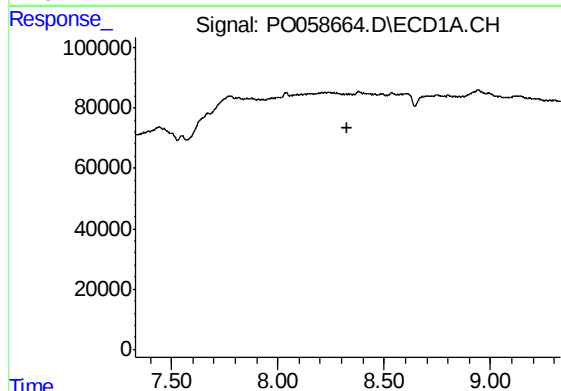


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 8.330 min
Response: 0
Conc: N.D.

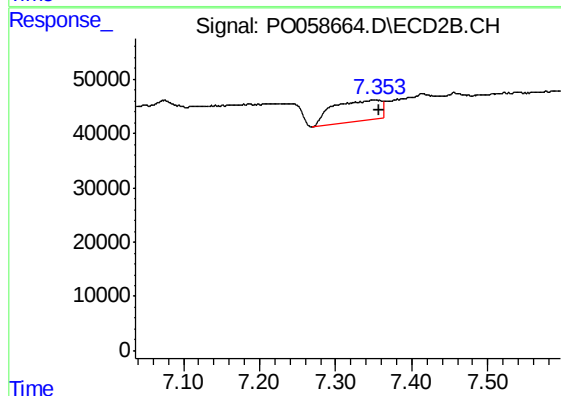

#38 AR-1262-3


R.T.: 7.353 min
Delta R.T.: -0.003 min
Response: 168346
Conc: 68.21 ng/ml

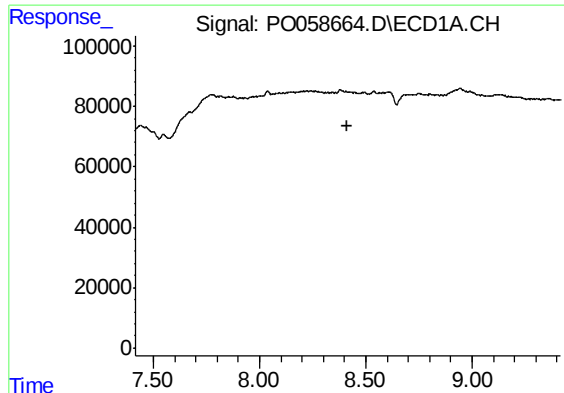

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 8.415 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

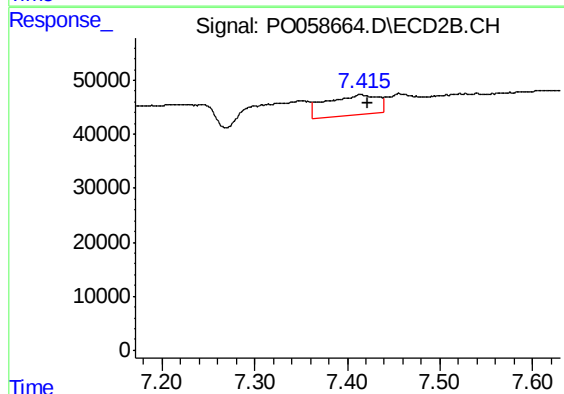


#39 AR-1262-4

R.T.: 7.415 min
Delta R.T.: -0.007 min
Response: 145429
Conc: 34.25 ng/ml

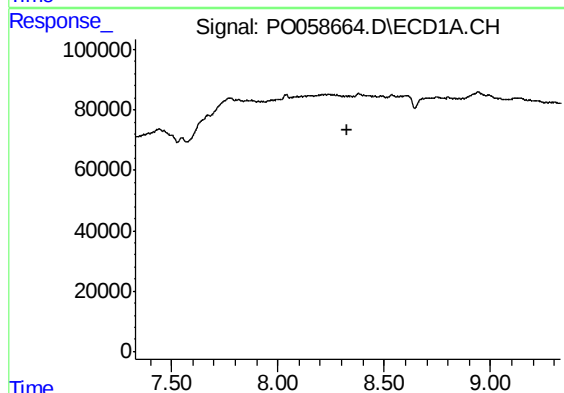


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T.: 8.330 min
Response: 0
Conc: N.D.

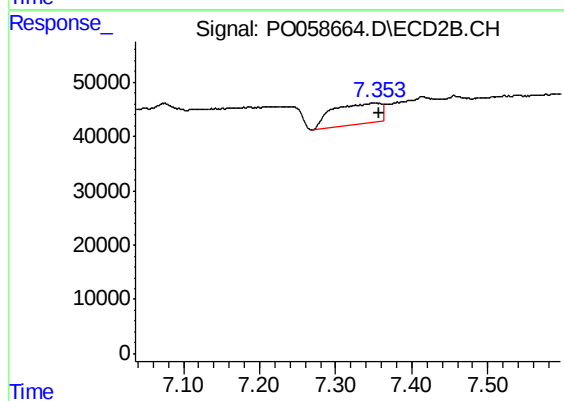

#41 AR-1268-1


R.T.: 7.353 min
Delta R.T.: -0.003 min
Response: 168346
Conc: 20.67 ng/ml

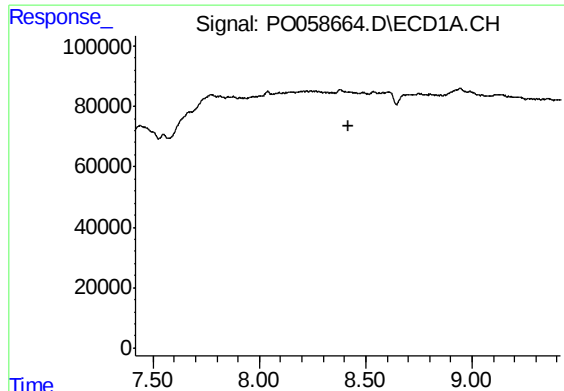

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T. : 8.417 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

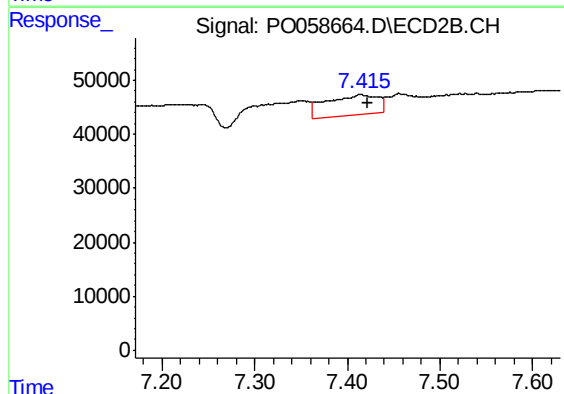


#42 AR-1268-2

R.T.: 7.415 min
Delta R.T.: -0.007 min
Response: 145429
Conc: 19.19 ng/ml

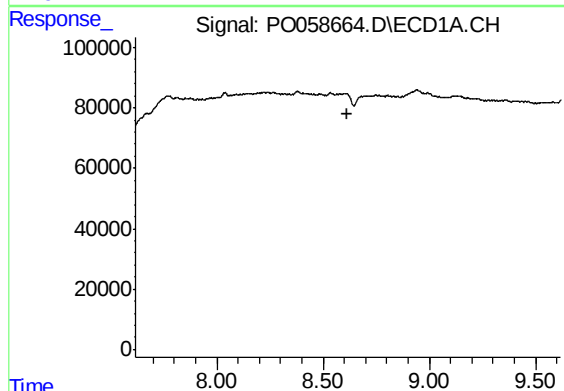

#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 8.617 min
Response: 0
Conc: N.D.

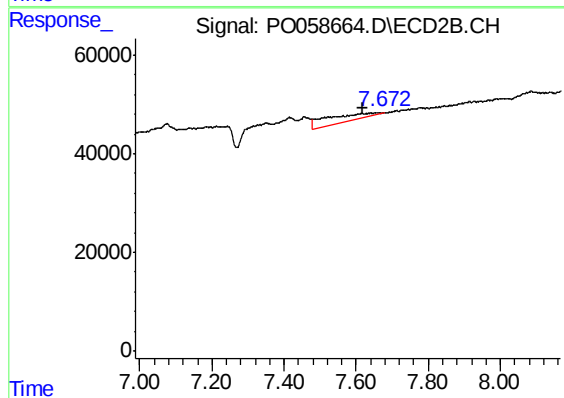

#43 AR-1268-3

R.T.: 7.663 min
Delta R.T.: 0.044 min
Response: 144707
Conc: 22.64 ng/ml