

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080119\
 Data File : P0058669.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Jul 2019 11:44
 Operator : SM/AJ
 Sample : K4053-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S12-01-A

Manual Integrations
 APPROVED

mohammad
 8/1/2019 2:40:46 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 31 12:16:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jul 27 06:49:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.168	3.519	848488	719271	20.105m	18.004
2) SA Decachlor...	9.648	8.407	1036826	772547	19.145m	19.572

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080119\
Data File : PO058669.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Jul 2019 11:44
Operator : SM/AJ
Sample : K4053-01
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
S12-01-A


Manual Integrations
APPROVED

mohammad
8/1/2019 2:40:46 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 31 12:16:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072819.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 27 06:49:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

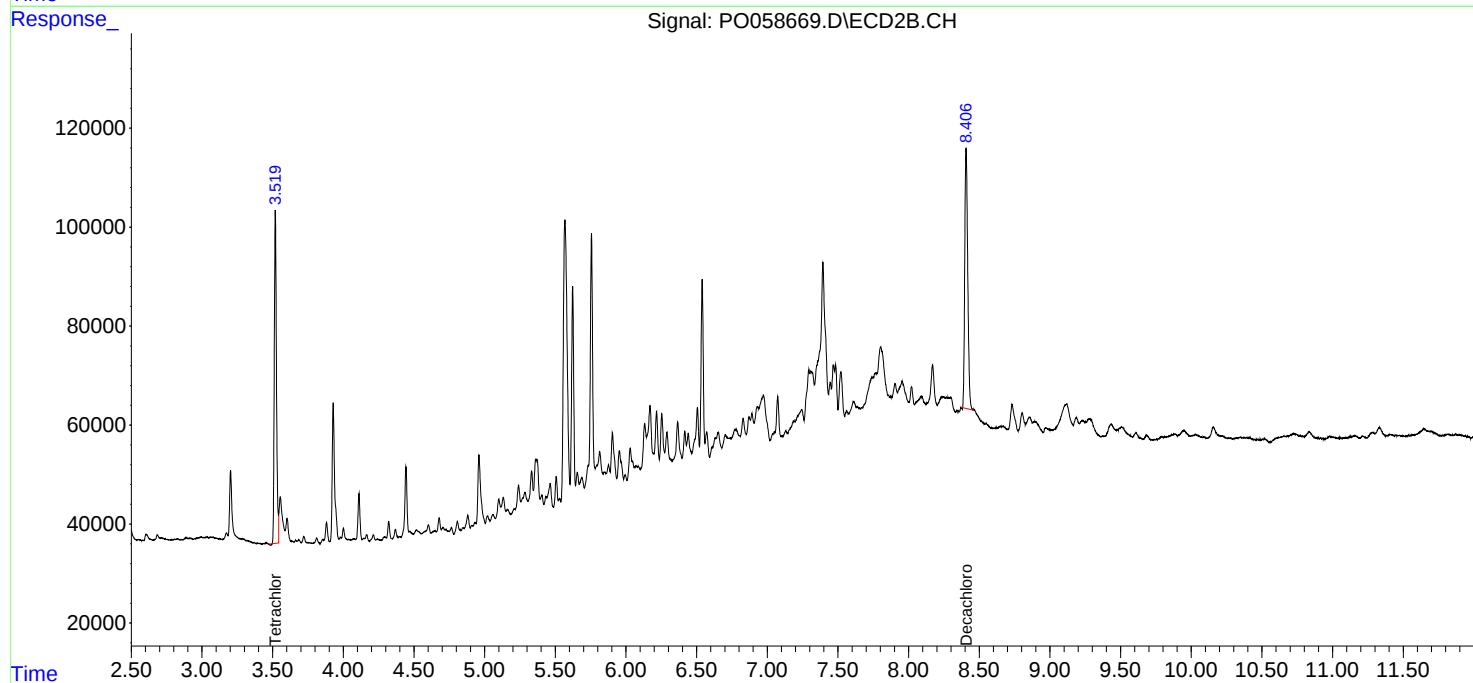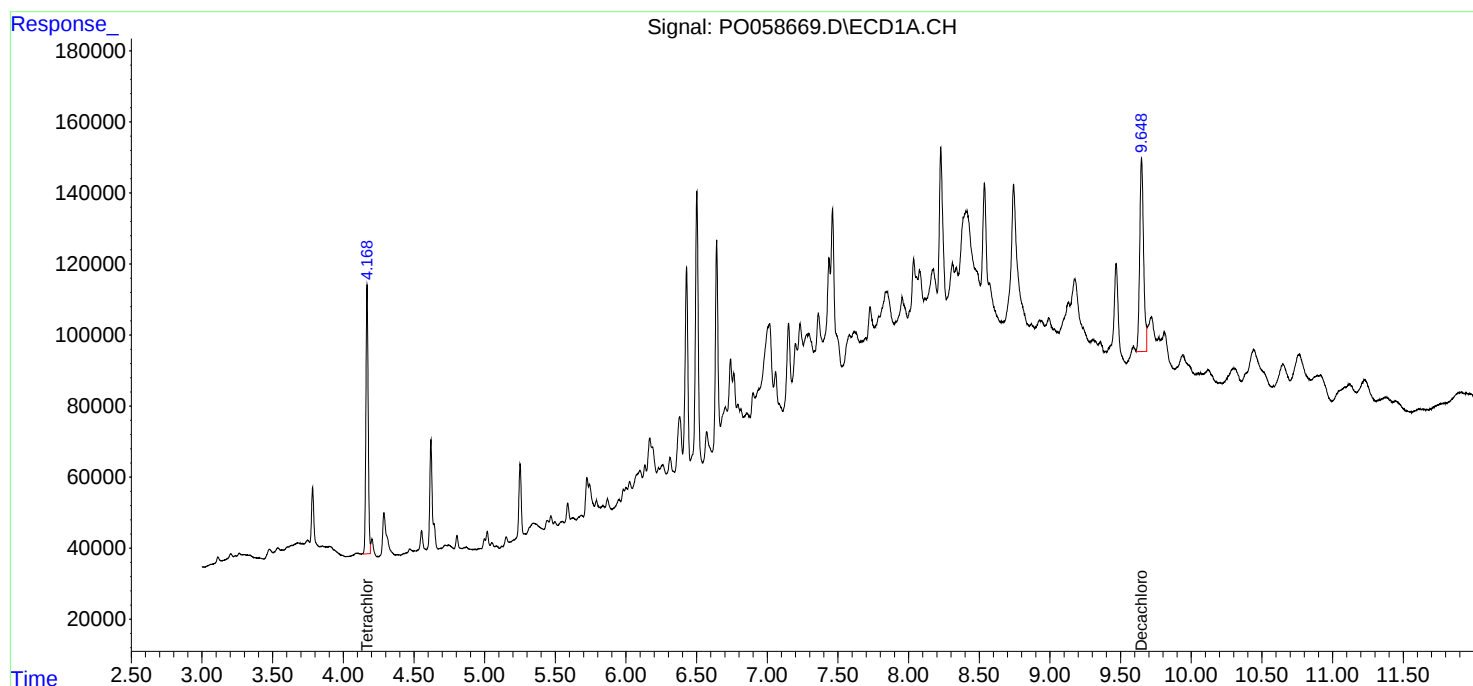

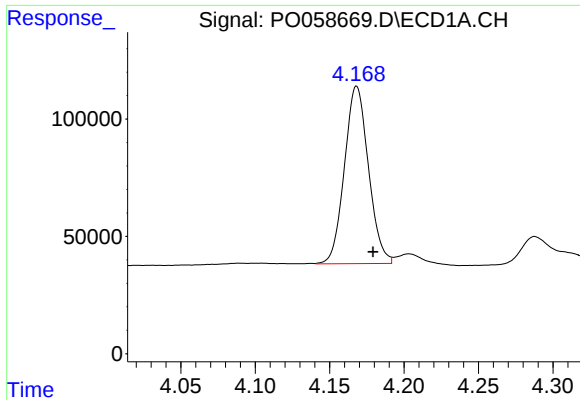


#1 Tetrachloro-m-xylene

R.T.: 4.168 min
Delta R.T.: -0.011 min
Response: 848488
Conc: 20.11 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S12-01-A


Manual Integrations
APPROVED

mohammad
8/1/2019 2:40:46 PM

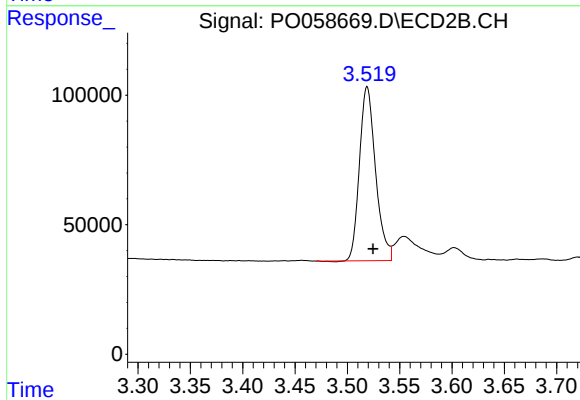


#1 Tetrachloro-m-xylene

R.T.: 3.519 min
Delta R.T.: -0.006 min
Response: 719271
Conc: 18.00 ng/ml

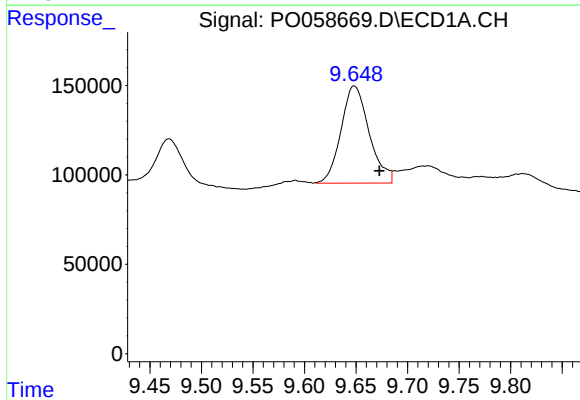

#2 Decachlorobiphenyl

R.T.: 9.648 min
Delta R.T.: -0.025 min
Response: 1036826
Conc: 19.15 ng/ml m

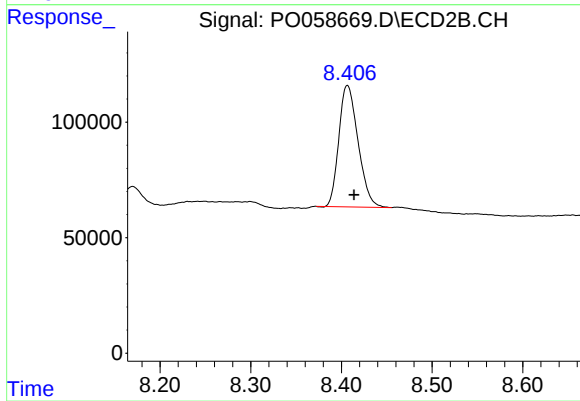

#2 Decachlorobiphenyl

R.T.: 8.407 min
Delta R.T.: -0.007 min
Response: 772547
Conc: 19.57 ng/ml