

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080119\
 Data File : P0058674.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Jul 2019 13:09
 Operator : SM/AJ
 Sample : K4056-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S7-01-A

Manual Integrations
 APPROVED

mohammad
 8/1/2019 2:40:55 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 31 16:28:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jul 27 06:49:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.169	3.519	750789	694988	17.790	17.396
2) SA Decachlor...	9.705	8.407	784563	538205	14.487	13.635m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080119\
Data File : P0058674.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Jul 2019 13:09
Operator : SM/AJ
Sample : K4056-01
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
S7-01-A


Manual Integrations
APPROVED

mohammad
8/1/2019 2:40:55 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 31 16:28:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 27 06:49:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

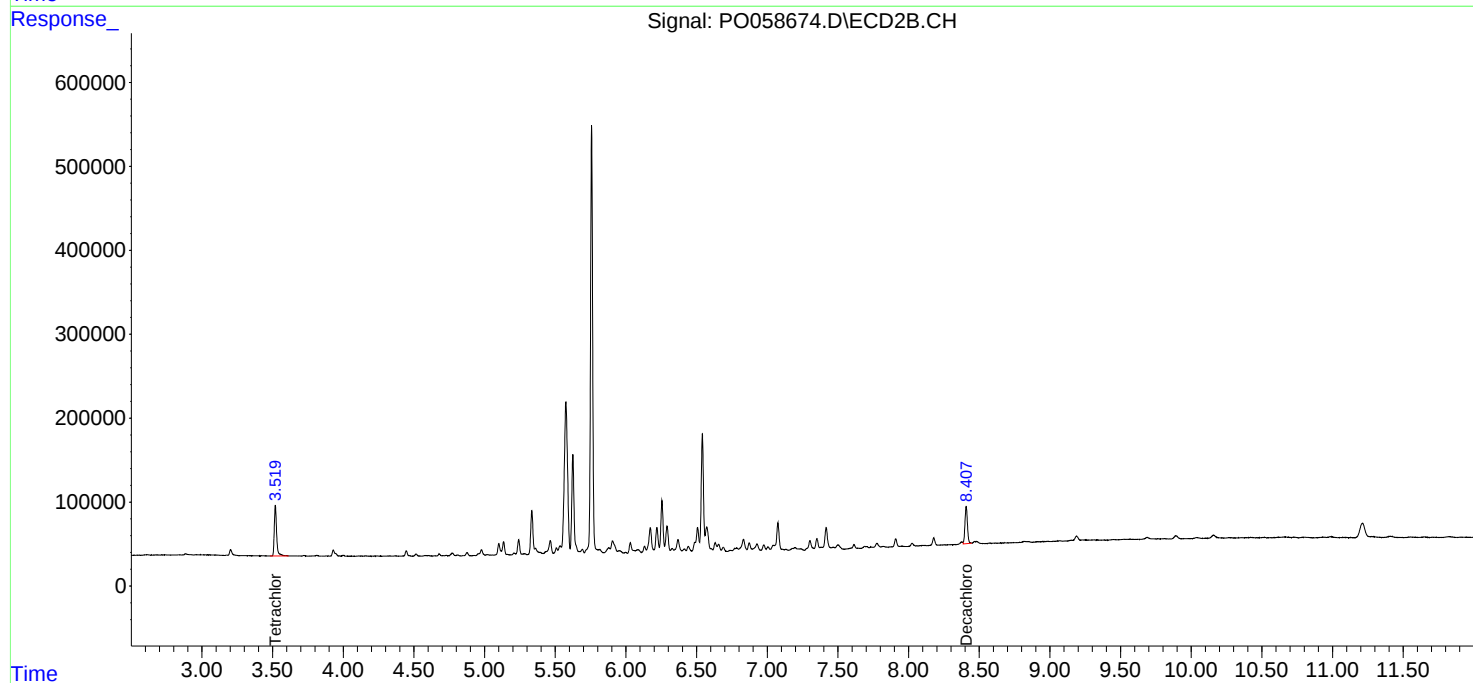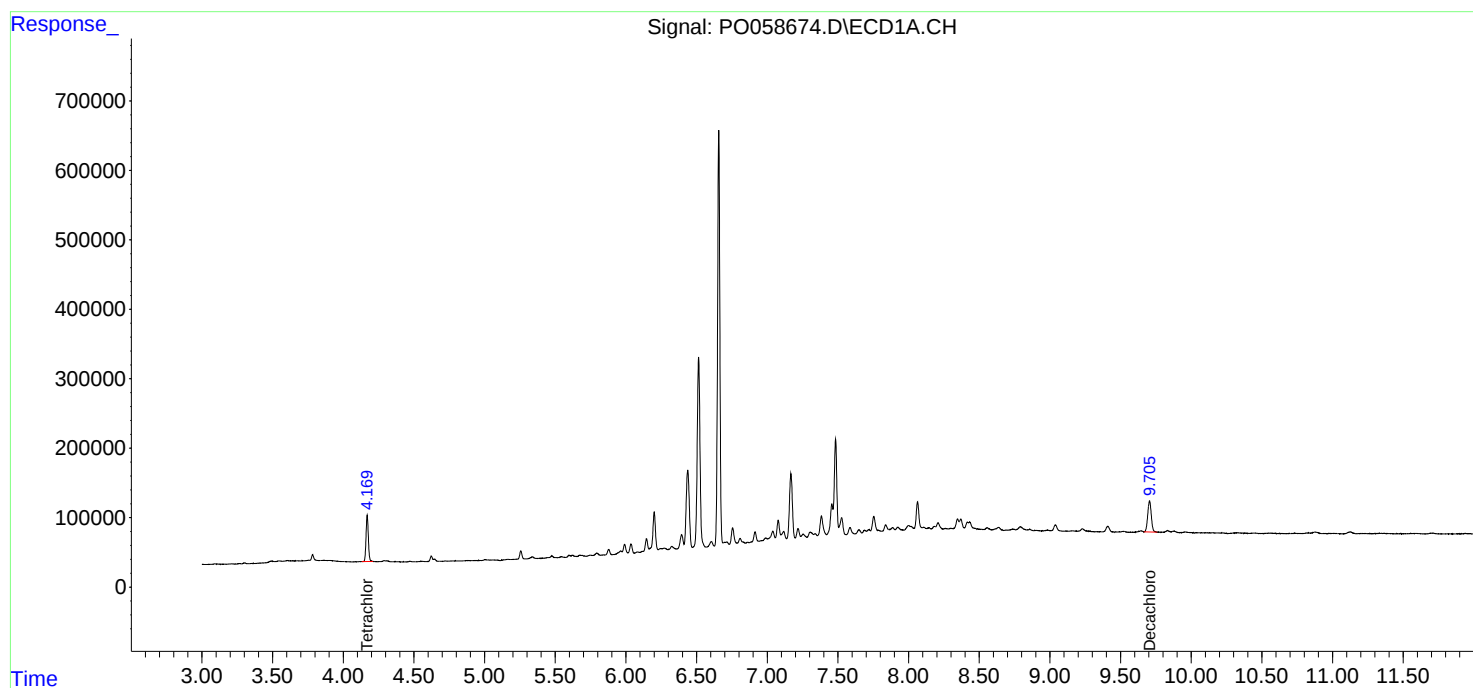

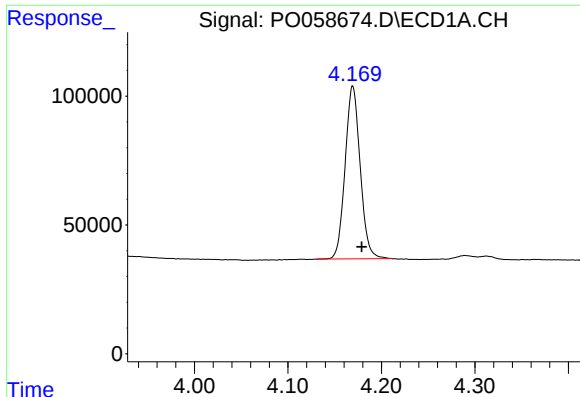


#1 Tetrachloro-m-xylene

R.T.: 4.169 min
Delta R.T.: -0.010 min
Response: 750789
Conc: 17.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
S7-01-A


Manual Integrations
APPROVED

mohammad
8/1/2019 2:40:55 PM

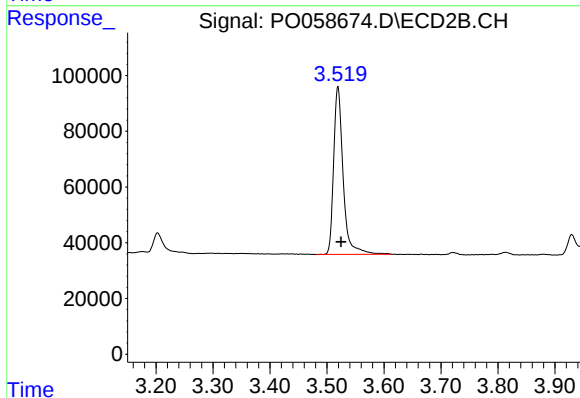


#1 Tetrachloro-m-xylene

R.T.: 3.519 min
Delta R.T.: -0.006 min
Response: 694988
Conc: 17.40 ng/ml

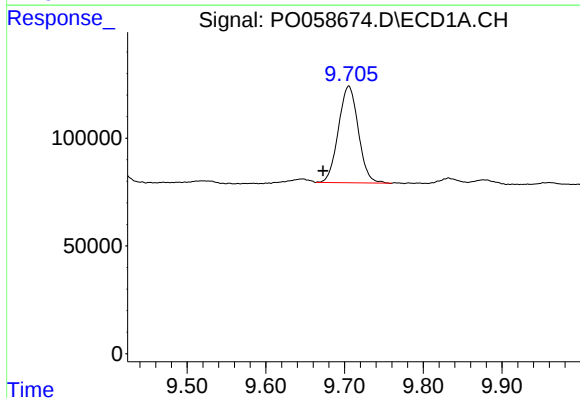

#2 Decachlorobiphenyl

R.T.: 9.705 min
Delta R.T.: 0.033 min
Response: 784563
Conc: 14.49 ng/ml

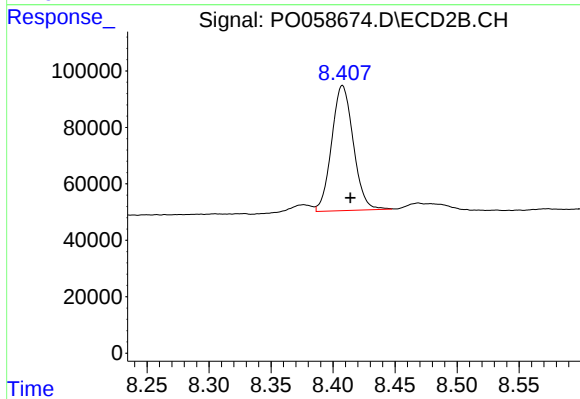

#2 Decachlorobiphenyl

R.T.: 8.407 min
Delta R.T.: -0.007 min
Response: 538205
Conc: 13.63 ng/ml m