

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080119\
 Data File : P0058713.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Aug 2019 1:00
 Operator : SM/AJ
 Sample : K4100-02
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S5-06-B

Manual Integrations
 APPROVED

Ankita
 8/2/2019 1:53:26 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 12:54:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jul 27 06:49:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.168	3.519	1110937	963333	26.324	24.113
2) SA Decachlor...	9.701	8.404	1166188	861918	21.534	21.836m
Target Compounds						
26) L6 AR-1254-1	6.170	5.361	123984	137806	52.507m	53.196
27) L6 AR-1254-2	6.389	5.507	266892	115039	69.251	50.248 #
28) L6 AR-1254-3	6.755	5.903	356613	334761	88.060	90.983
29) L6 AR-1254-4	7.038	6.130	181522	122726	50.414	52.780
30) L6 AR-1254-5	7.481	6.540	452257	646247	124.769m	187.342 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080119\
Data File : PO058713.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Aug 2019 1:00
Operator : SM/AJ
Sample : K4100-02
Misc :
ALS Vial : 34 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
S5-06-B


Manual Integrations
APPROVED

Ankita
8/2/2019 1:53:26 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 12:54:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072819.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 27 06:49:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

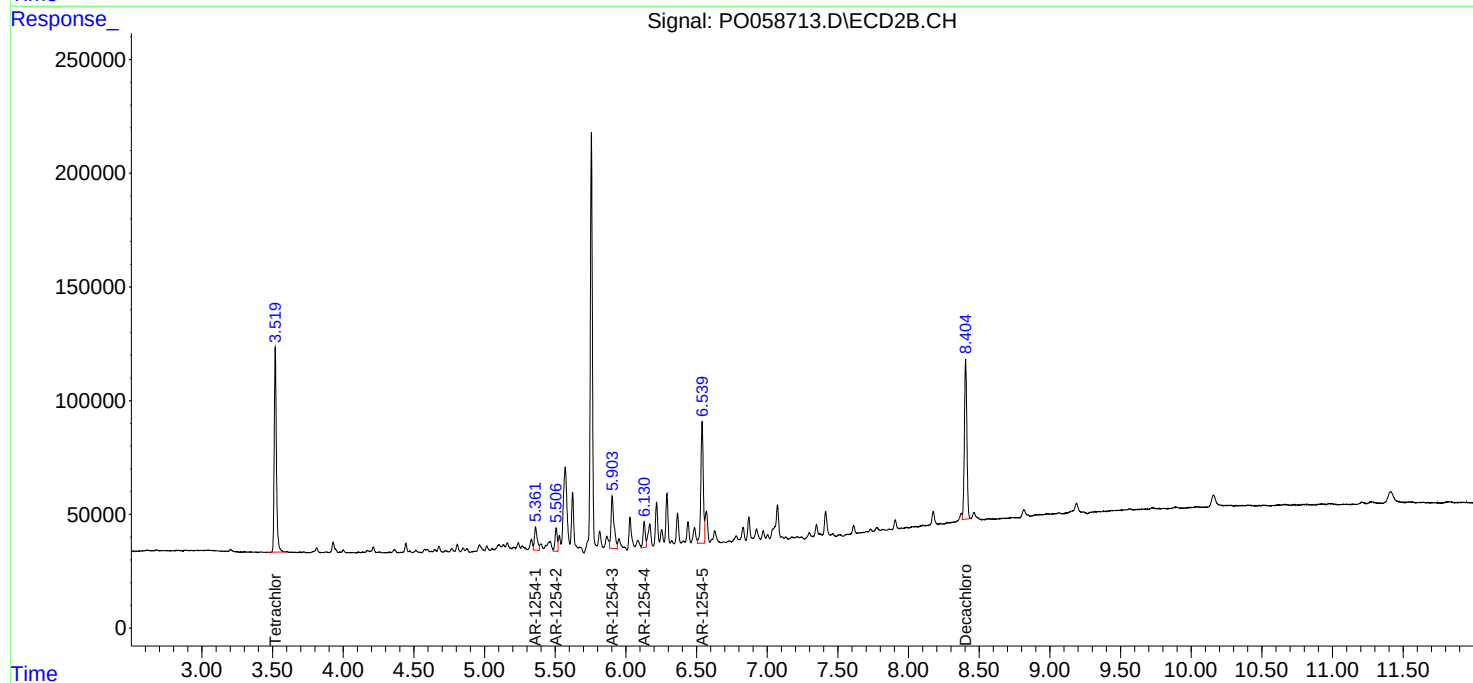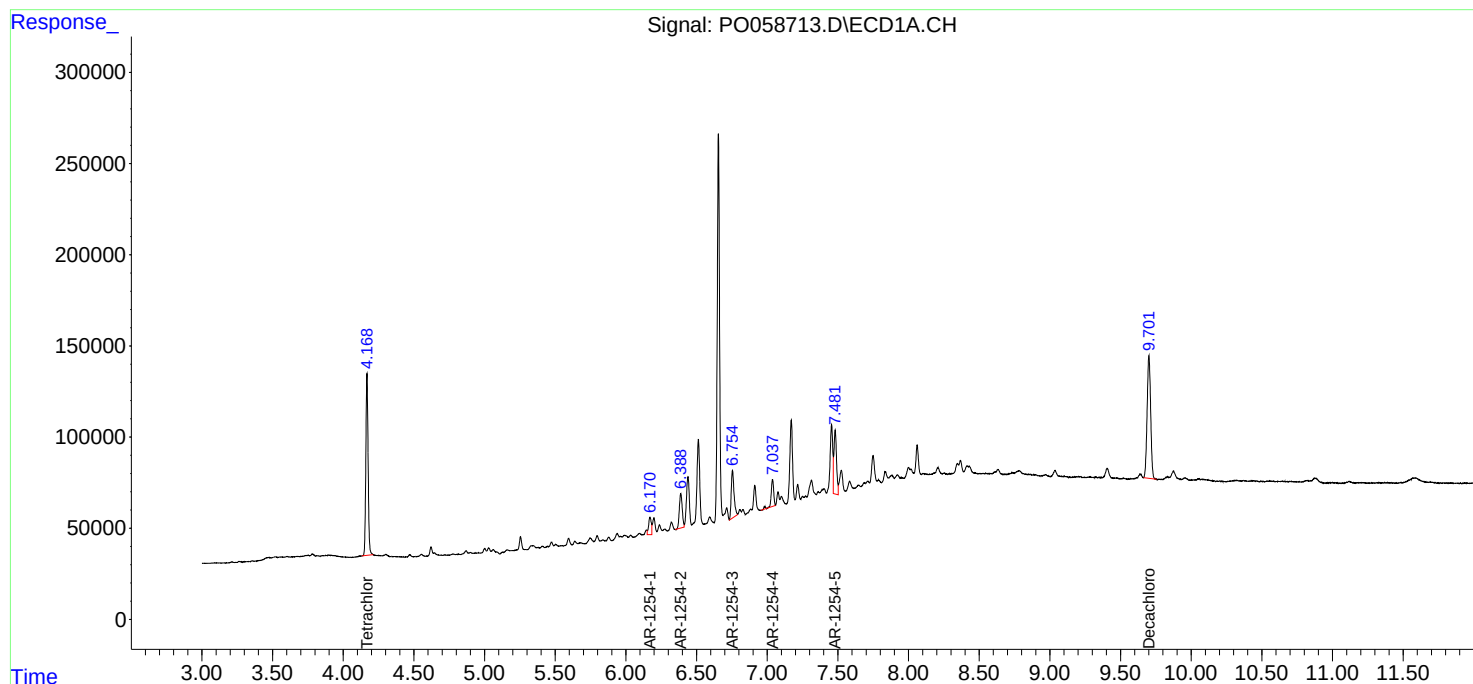

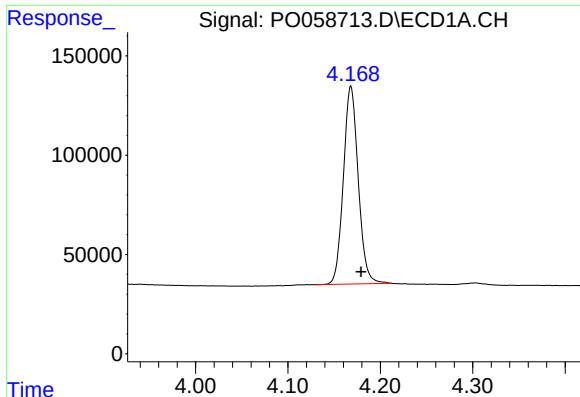


#1 Tetrachloro-m-xylene

R.T.: 4.168 min
Delta R.T.: -0.011 min
Response: 1110937
Conc: 26.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
S5-06-B


Manual Integrations
APPROVED

Ankita
8/2/2019 1:53:26 PM

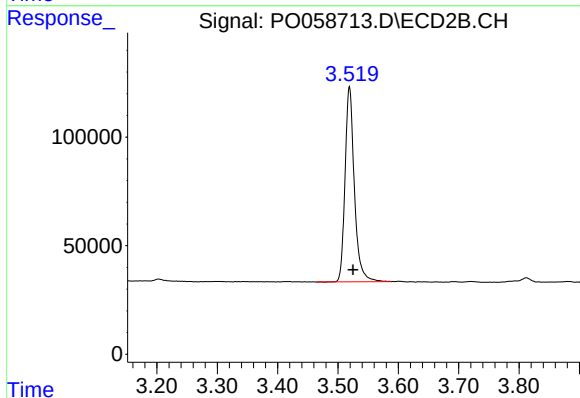


#1 Tetrachloro-m-xylene

R.T.: 3.519 min
Delta R.T.: -0.006 min
Response: 963333
Conc: 24.11 ng/ml

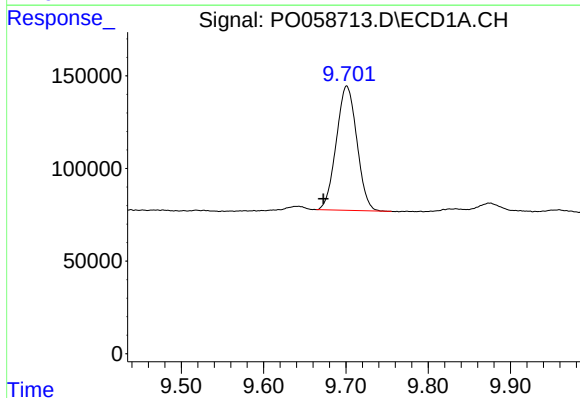


#2 Decachlorobiphenyl

R.T.: 9.701 min
Delta R.T.: 0.028 min
Response: 1166188
Conc: 21.53 ng/ml

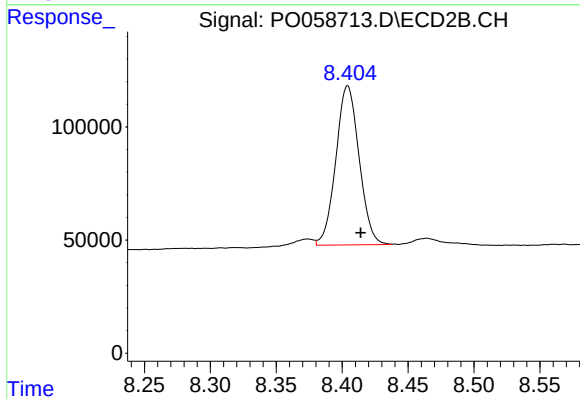

#2 Decachlorobiphenyl

R.T.: 8.404 min
Delta R.T.: -0.010 min
Response: 861918
Conc: 21.84 ng/ml m

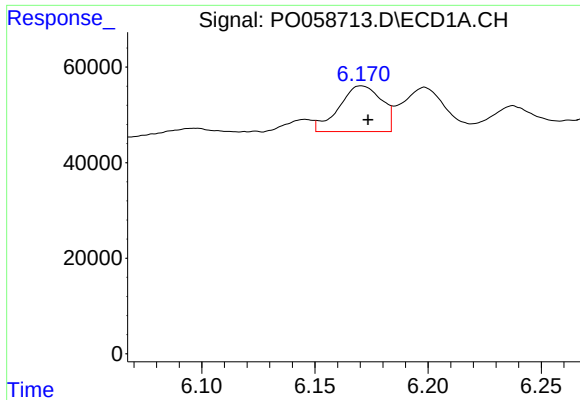


#26 AR-1254-1

R.T.: 6.170 min
Delta R.T.: -0.003 min
Response: 123984
Conc: 52.51 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S5-06-B


Manual Integrations
APPROVED

Ankita
8/2/2019 1:53:26 PM

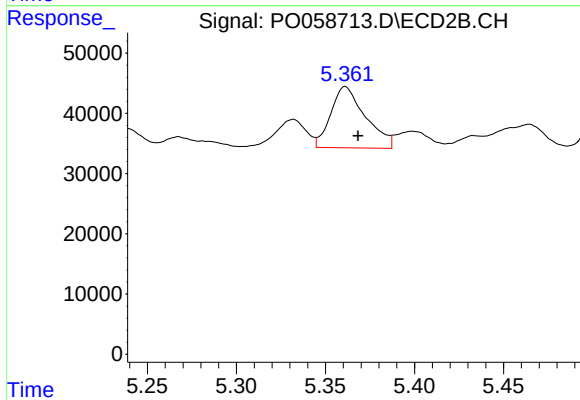


#26 AR-1254-1

R.T.: 5.361 min
Delta R.T.: -0.007 min
Response: 137806
Conc: 53.20 ng/ml

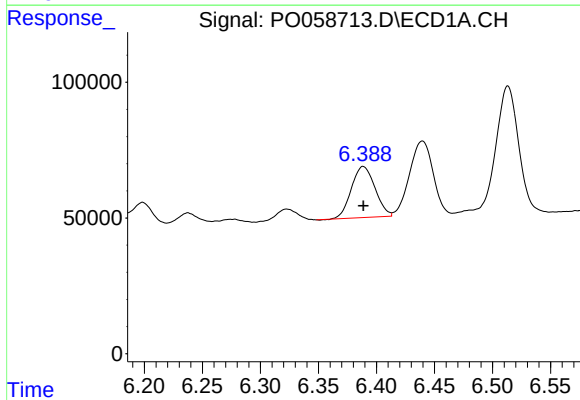


#27 AR-1254-2

R.T.: 6.389 min
Delta R.T.: 0.000 min
Response: 266892
Conc: 69.25 ng/ml

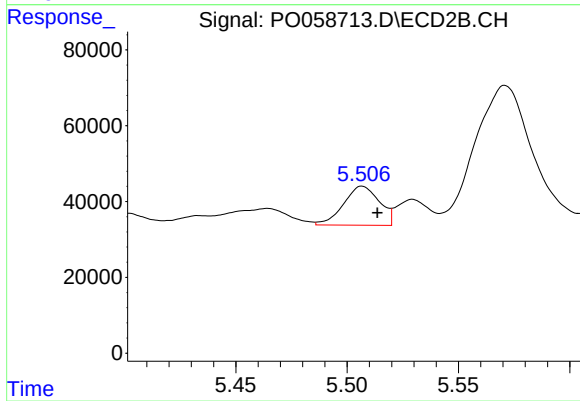

#27 AR-1254-2

R.T.: 5.507 min
Delta R.T.: -0.007 min
Response: 115039
Conc: 50.25 ng/ml

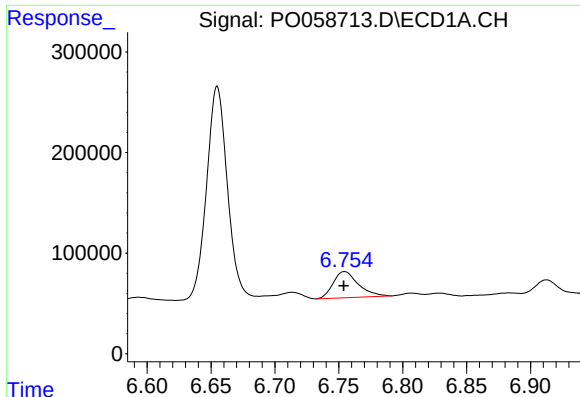


#28 AR-1254-3

R.T.: 6.755 min
Delta R.T.: 0.000 min
Response: 356613
Conc: 88.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
S5-06-B


Manual Integrations
APPROVED

Ankita
8/2/2019 1:53:26 PM

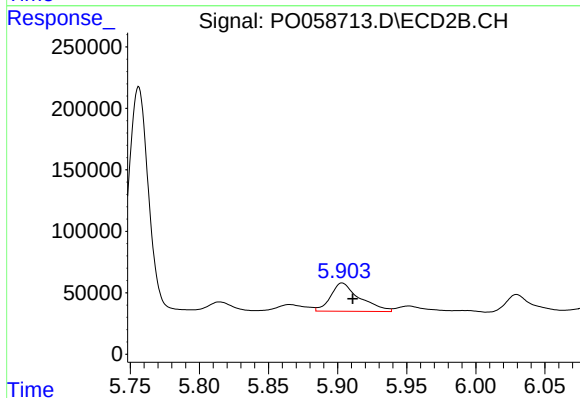


#28 AR-1254-3

R.T.: 5.903 min
Delta R.T.: -0.008 min
Response: 334761
Conc: 90.98 ng/ml

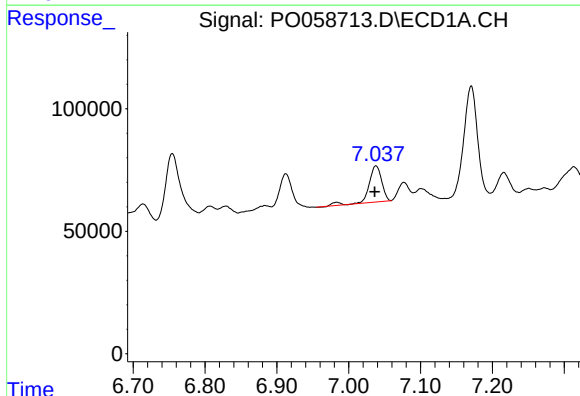


#29 AR-1254-4

R.T.: 7.038 min
Delta R.T.: 0.002 min
Response: 181522
Conc: 50.41 ng/ml

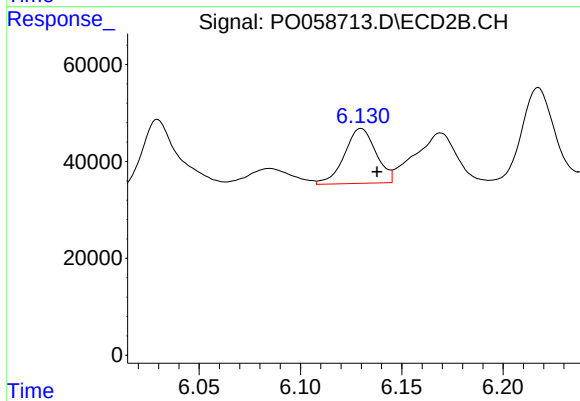

#29 AR-1254-4

R.T.: 6.130 min
Delta R.T.: -0.008 min
Response: 122726
Conc: 52.78 ng/ml

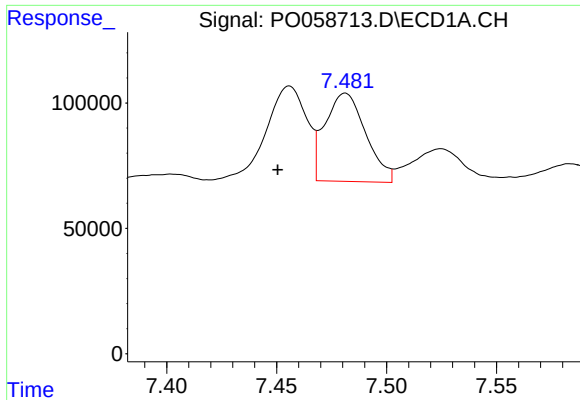


#30 AR-1254-5

R.T.: 7.481 min
Delta R.T.: 0.030 min
Response: 452257
Conc: 124.77 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S5-06-B

Manual Integrations
APPROVED

Ankita
8/2/2019 1:53:26 PM

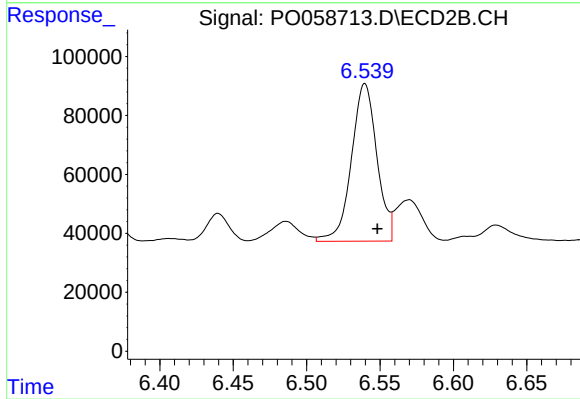

#30 AR-1254-5

R.T.: 6.540 min
Delta R.T.: -0.008 min
Response: 646247
Conc: 187.34 ng/ml