

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080119\
 Data File : P0058715.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Aug 2019 1:34
 Operator : SM/AJ
 Sample : K4100-04
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DUP-5

Manual Integrations
 APPROVED

Ankita
 8/2/2019 1:59:30 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 13:02:42 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jul 27 06:49:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.168	3.519	1032896	883794	24.475	22.122
2) SA Decachlor...	9.700	8.404	1105562	842078	20.415	21.333m
Target Compounds						
26) L6 AR-1254-1	6.171	5.361	101882	147687	43.147m	57.010 #
27) L6 AR-1254-2	6.389	5.506	281041	102876	72.923	44.935 #
28) L6 AR-1254-3	6.754	5.903	343143	290444	84.734	78.939
29) L6 AR-1254-4	7.037	6.129	283306	169485	78.682	72.890
30) L6 AR-1254-5	7.481	6.539	748296	849990	206.440m	246.406

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080119\
Data File : P0058715.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Aug 2019 1:34
Operator : SM/AJ
Sample : K4100-04
Misc :
ALS Vial : 36 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
DUP-5


Manual Integrations
APPROVED

Ankita
8/2/2019 1:59:30 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 13:02:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 27 06:49:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

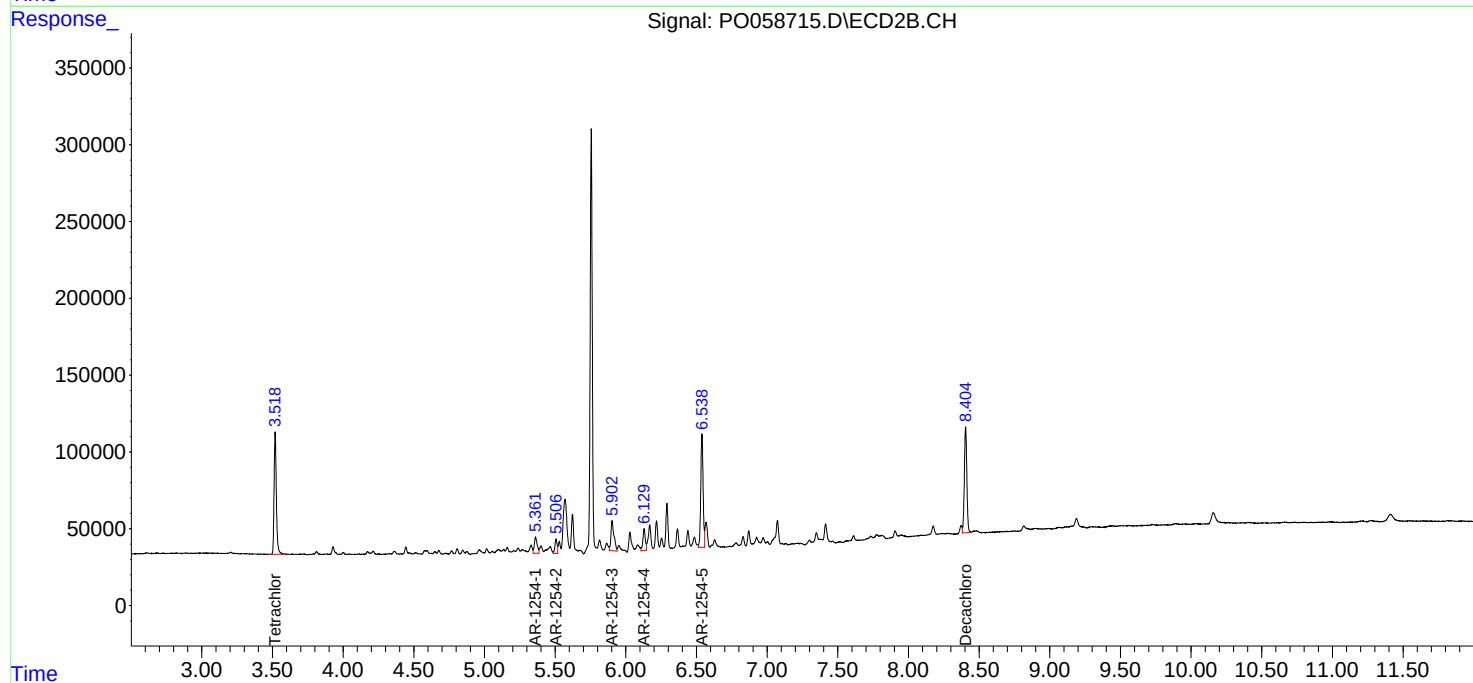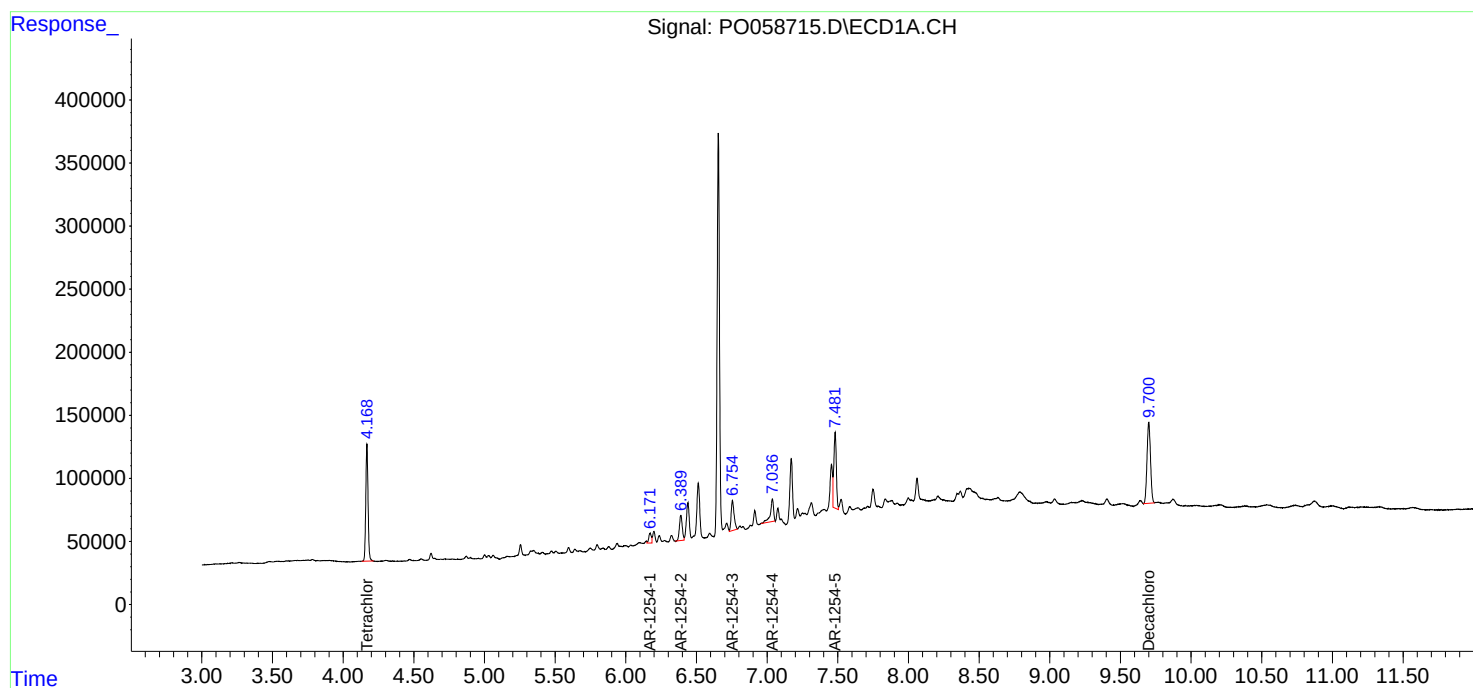

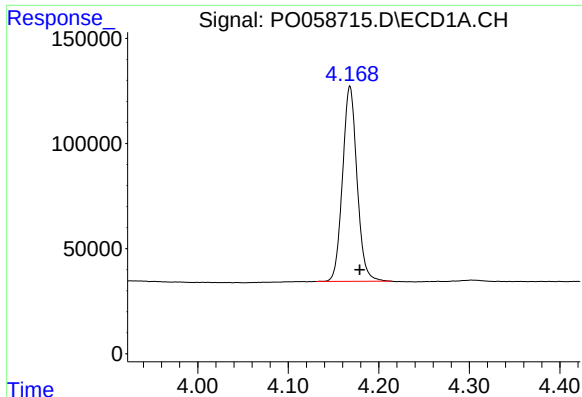


#1 Tetrachloro-m-xylene

R.T.: 4.168 min
Delta R.T.: -0.011 min
Response: 1032896
Conc: 24.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
DUP-5


Manual Integrations
APPROVED

Ankita
8/2/2019 1:59:30 PM

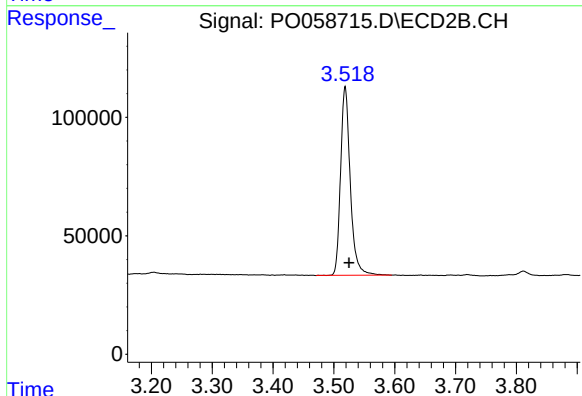


#1 Tetrachloro-m-xylene

R.T.: 3.519 min
Delta R.T.: -0.006 min
Response: 883794
Conc: 22.12 ng/ml

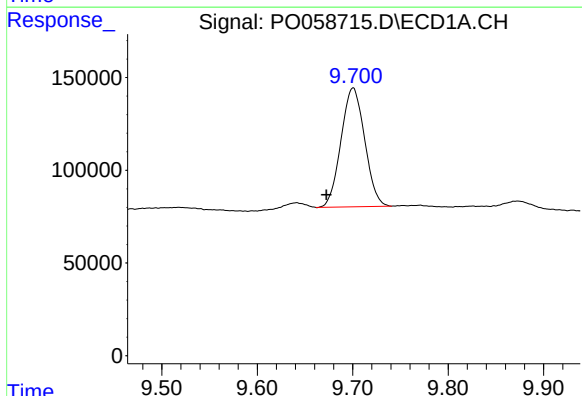


#2 Decachlorobiphenyl

R.T.: 9.700 min
Delta R.T.: 0.028 min
Response: 1105562
Conc: 20.41 ng/ml

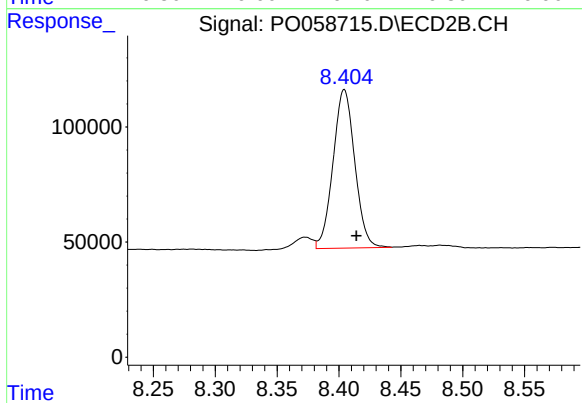

#2 Decachlorobiphenyl

R.T.: 8.404 min
Delta R.T.: -0.010 min
Response: 842078
Conc: 21.33 ng/ml m

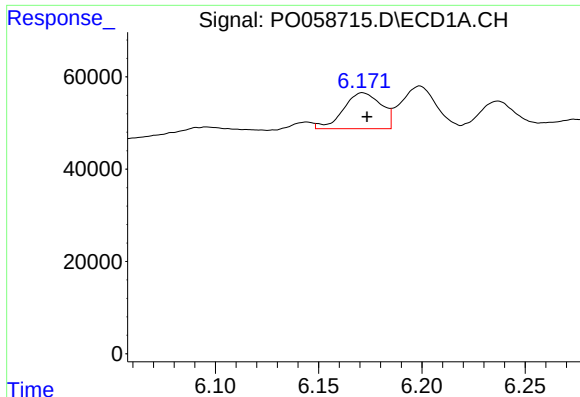


#26 AR-1254-1

R.T.: 6.171 min
Delta R.T.: -0.003 min
Response: 101882
Conc: 43.15 ng/ml m

Instrument :
ECD_O
ClientSampleId :
DUP-5


Manual Integrations
APPROVED

Ankita
8/2/2019 1:59:30 PM

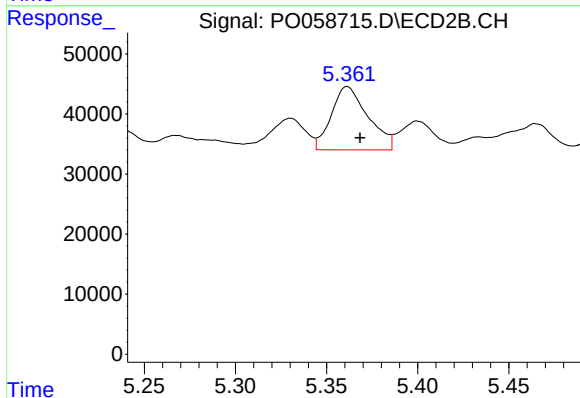


#26 AR-1254-1

R.T.: 5.361 min
Delta R.T.: -0.007 min
Response: 147687
Conc: 57.01 ng/ml

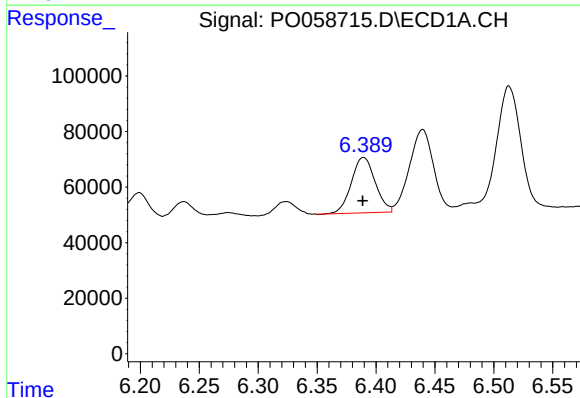


#27 AR-1254-2

R.T.: 6.389 min
Delta R.T.: 0.000 min
Response: 281041
Conc: 72.92 ng/ml

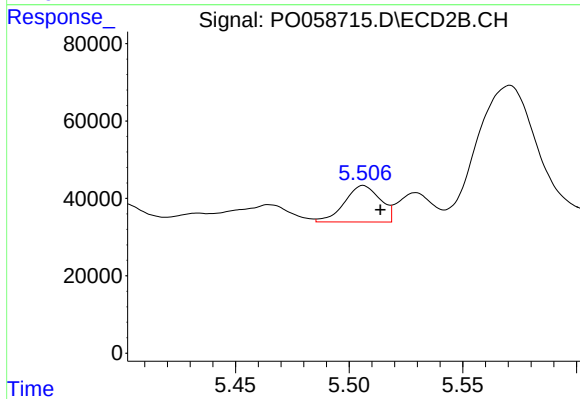

#27 AR-1254-2

R.T.: 5.506 min
Delta R.T.: -0.007 min
Response: 102876
Conc: 44.94 ng/ml

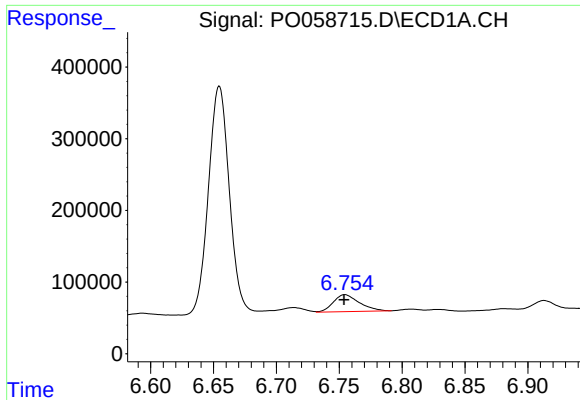


#28 AR-1254-3

R.T.: 6.754 min
Delta R.T.: 0.000 min
Response: 343143
Conc: 84.73 ng/ml

Instrument :
ECD_O
ClientSampled :
DUP-5


Manual Integrations
APPROVED

Ankita
8/2/2019 1:59:30 PM

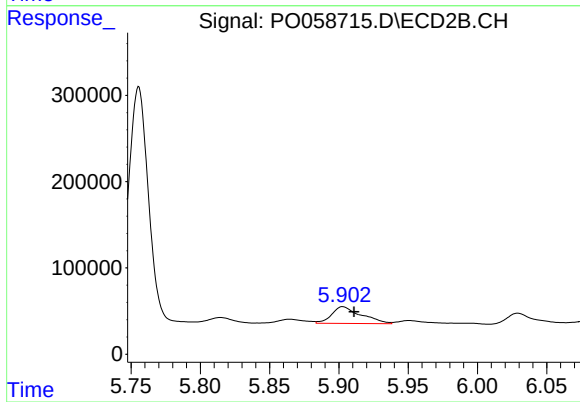


#28 AR-1254-3

R.T.: 5.903 min
Delta R.T.: -0.008 min
Response: 290444
Conc: 78.94 ng/ml

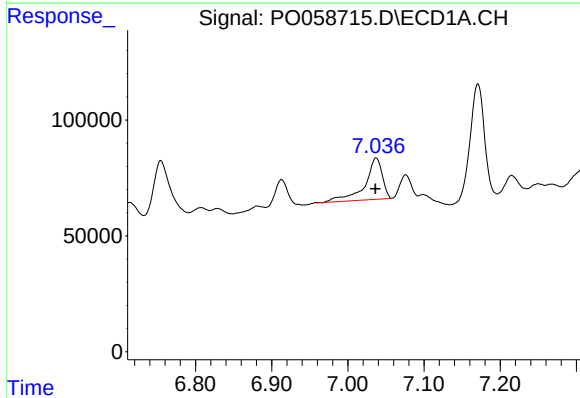


#29 AR-1254-4

R.T.: 7.037 min
Delta R.T.: 0.000 min
Response: 283306
Conc: 78.68 ng/ml

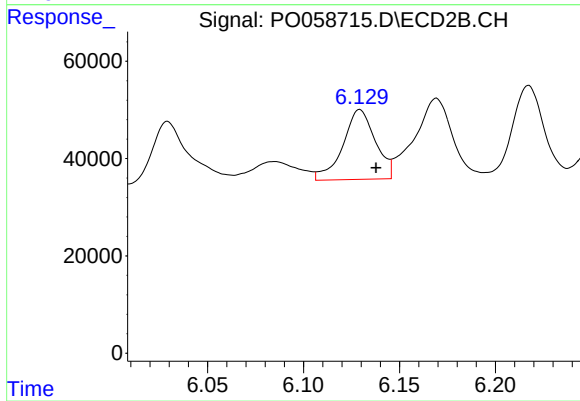

#29 AR-1254-4

R.T.: 6.129 min
Delta R.T.: -0.008 min
Response: 169485
Conc: 72.89 ng/ml

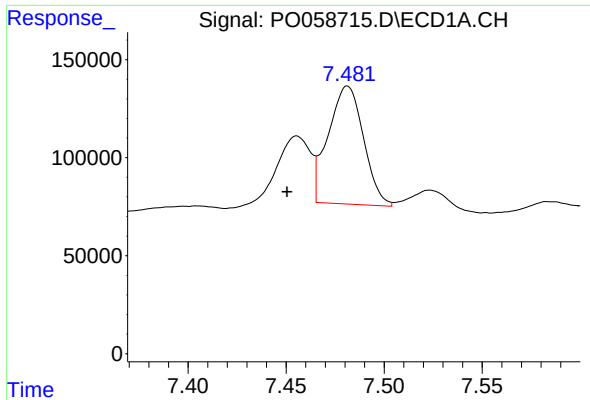


#30 AR-1254-5

R.T.: 7.481 min
Delta R.T.: 0.030 min
Response: 748296
Conc: 206.44 ng/ml m

Instrument :
ECD_O
ClientSampleId :
DUP-5

Manual Integrations
APPROVED

Ankita
8/2/2019 1:59:30 PM

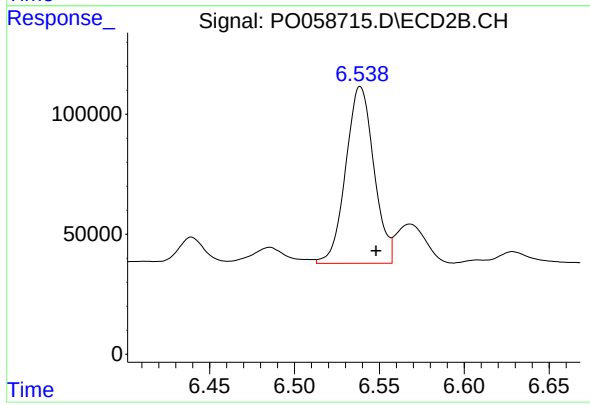

#30 AR-1254-5

R.T.: 6.539 min
Delta R.T.: -0.009 min
Response: 849990
Conc: 246.41 ng/ml