

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080119\
 Data File : P0058718.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Aug 2019 2:25
 Operator : SM/AJ
 Sample : K4102-02
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S6-03-S

Manual Integrations
 APPROVED

Ankita
 8/2/2019 1:53:33 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 13:05:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jul 27 06:49:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.167	3.519	1030499	893647	24.418	22.369
2) SA Decachlor...	9.644	8.404	1282473	945369	23.681	23.950
Target Compounds						
26) L6 AR-1254-1	6.157	5.359	130012	160395	55.060m	61.916m
27) L6 AR-1254-2	6.375	5.506	301256	136163	78.168	59.475
28) L6 AR-1254-3	6.739	5.903	383779	385822	94.769	104.861
29) L6 AR-1254-4	7.020	6.130	280308	176720	77.849	76.002
30) L6 AR-1254-5	7.461	6.539	1476676	1600570	407.386	463.993

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080119\
Data File : PO058718.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Aug 2019 2:25
Operator : SM/AJ
Sample : K4102-02
Misc :
ALS Vial : 39 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
S6-03-S


Manual Integrations
APPROVED

Ankita
8/2/2019 1:53:33 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 13:05:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072819.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 27 06:49:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

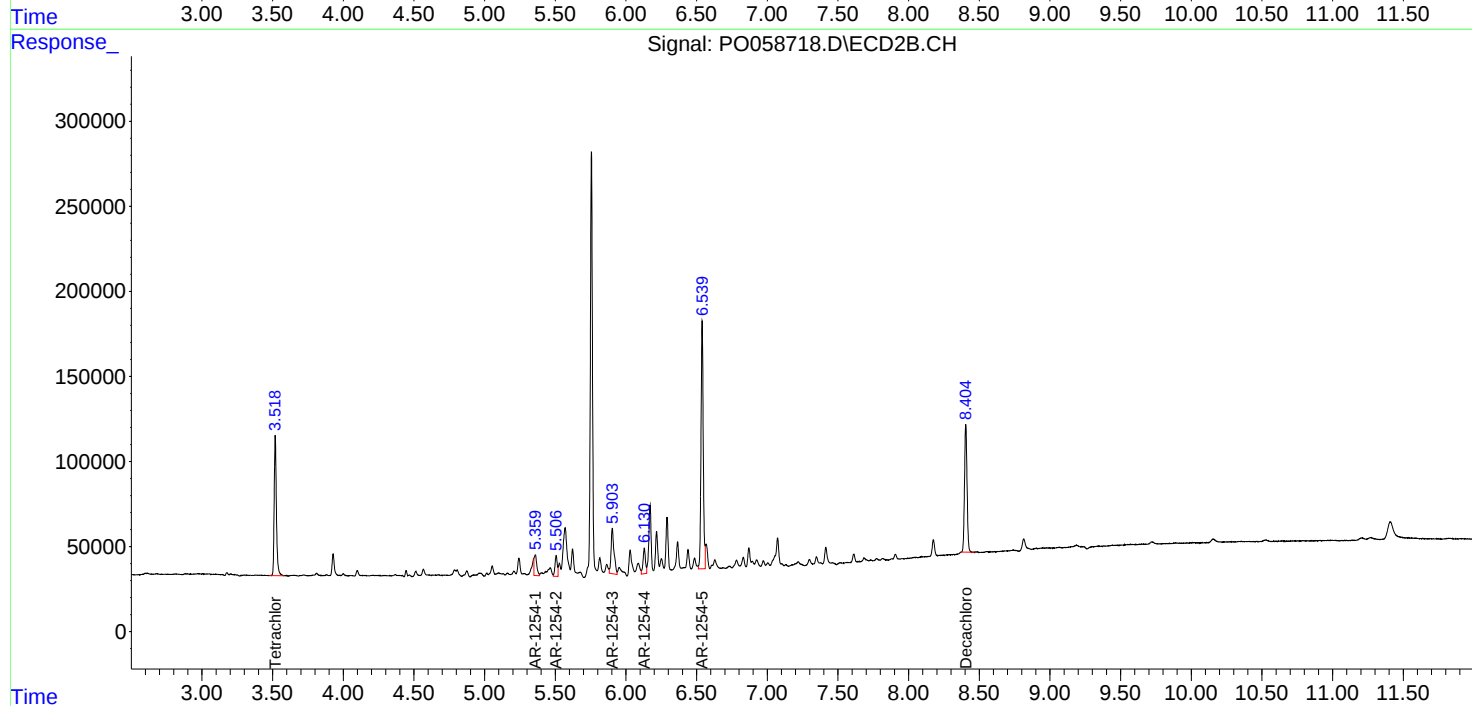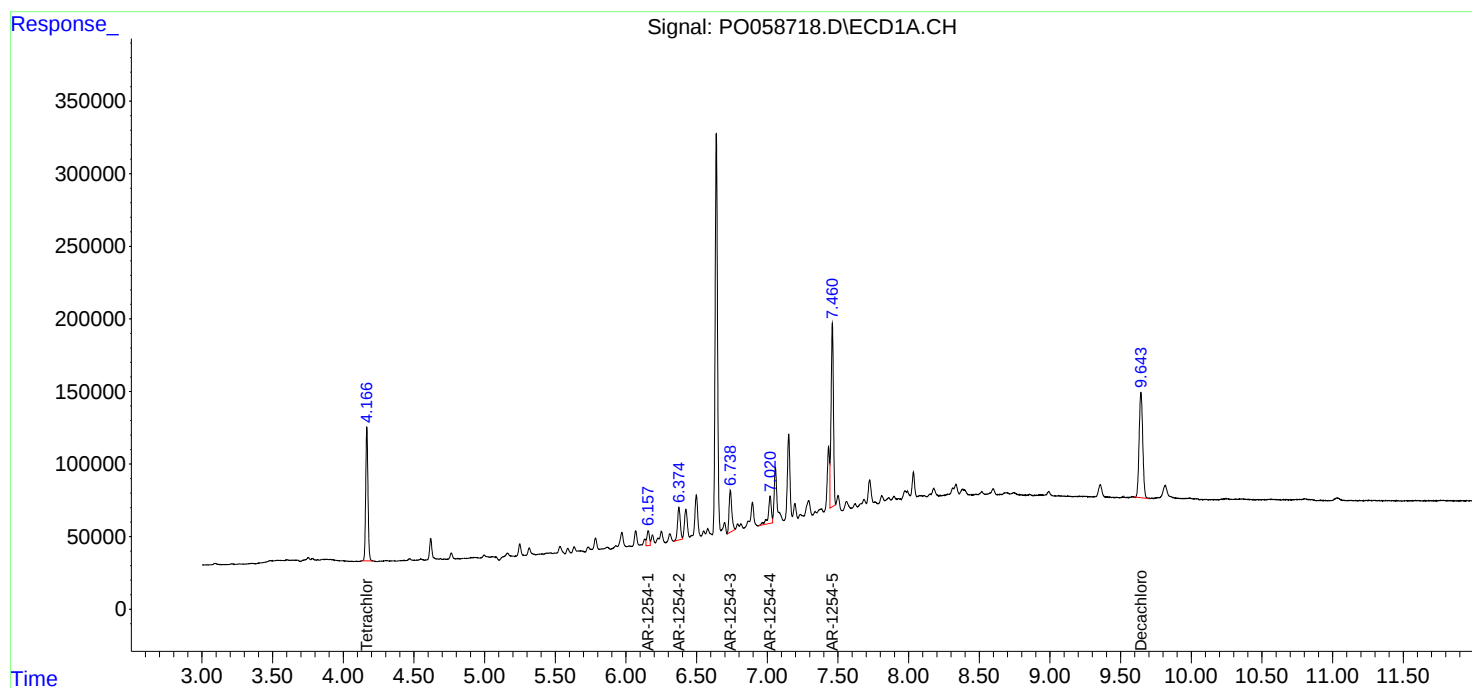

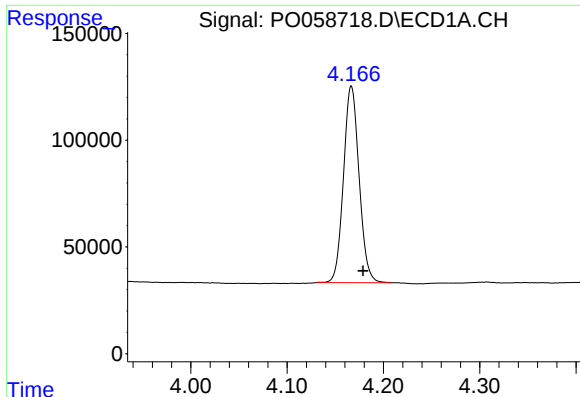


#1 Tetrachloro-m-xylene

R.T.: 4.167 min
Delta R.T.: -0.012 min
Response: 1030499
Conc: 24.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
S6-03-S


Manual Integrations
APPROVED

Ankita
8/2/2019 1:53:33 PM

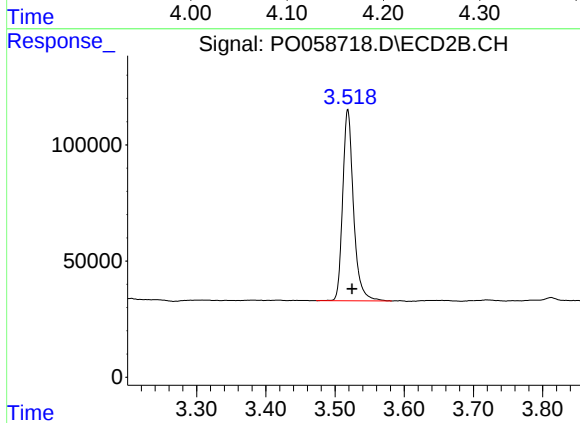


#1 Tetrachloro-m-xylene

R.T.: 3.519 min
Delta R.T.: -0.006 min
Response: 893647
Conc: 22.37 ng/ml

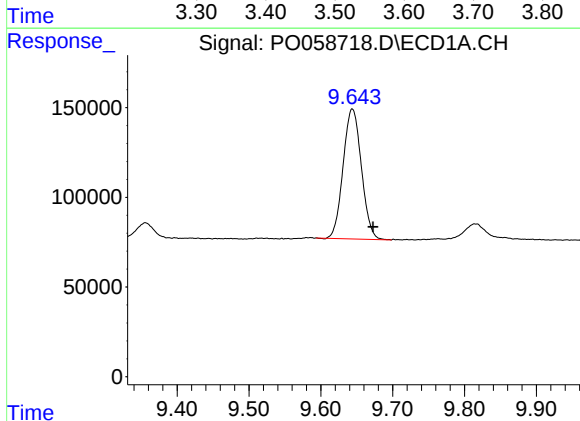


#2 Decachlorobiphenyl

R.T.: 9.644 min
Delta R.T.: -0.029 min
Response: 1282473
Conc: 23.68 ng/ml

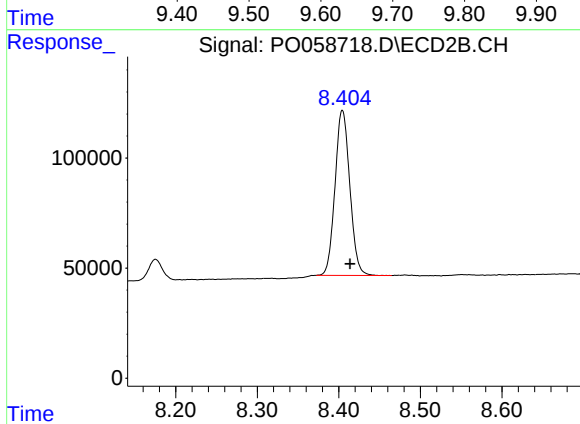

#2 Decachlorobiphenyl

R.T.: 8.404 min
Delta R.T.: -0.010 min
Response: 945369
Conc: 23.95 ng/ml

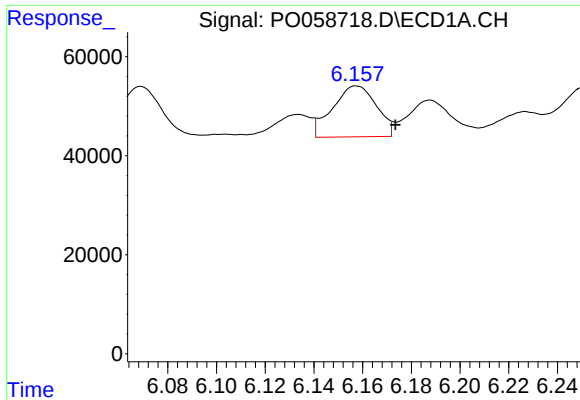


#26 AR-1254-1

R.T.: 6.157 min
Delta R.T.: -0.017 min
Response: 130012
Conc: 55.06 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S6-03-S


Manual Integrations
APPROVED

Ankita
8/2/2019 1:53:33 PM

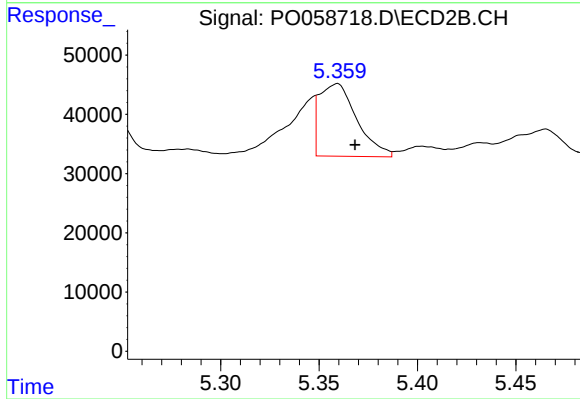


#26 AR-1254-1

R.T.: 5.359 min
Delta R.T.: -0.009 min
Response: 160395
Conc: 61.92 ng/ml m

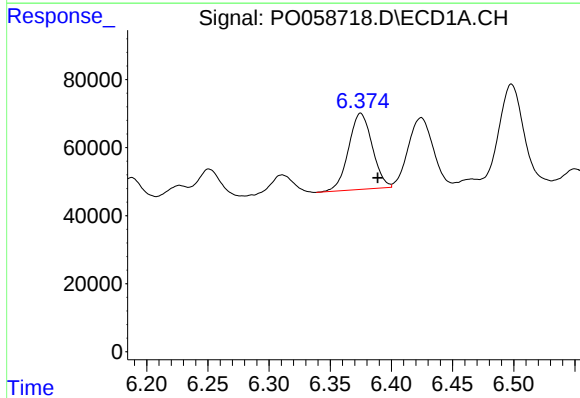


#27 AR-1254-2

R.T.: 6.375 min
Delta R.T.: -0.014 min
Response: 301256
Conc: 78.17 ng/ml

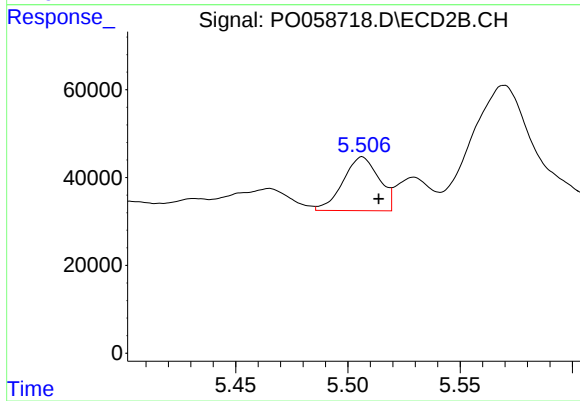

#27 AR-1254-2

R.T.: 5.506 min
Delta R.T.: -0.007 min
Response: 136163
Conc: 59.47 ng/ml

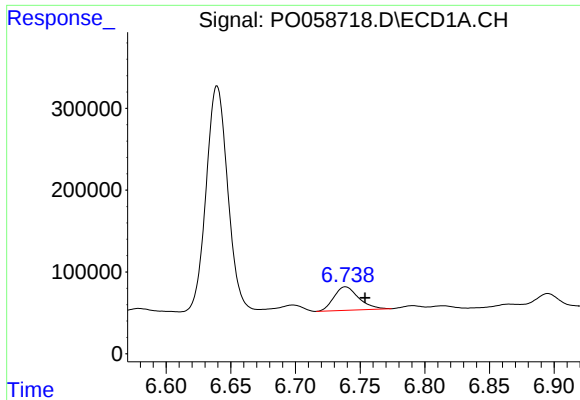


#28 AR-1254-3

R.T.: 6.739 min
Delta R.T.: -0.015 min
Response: 383779
Conc: 94.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
S6-03-S


Manual Integrations
APPROVED

Ankita
8/2/2019 1:53:33 PM

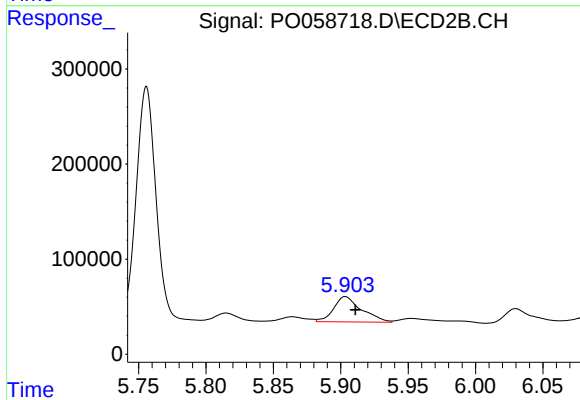


#28 AR-1254-3

R.T.: 5.903 min
Delta R.T.: -0.007 min
Response: 385822
Conc: 104.86 ng/ml

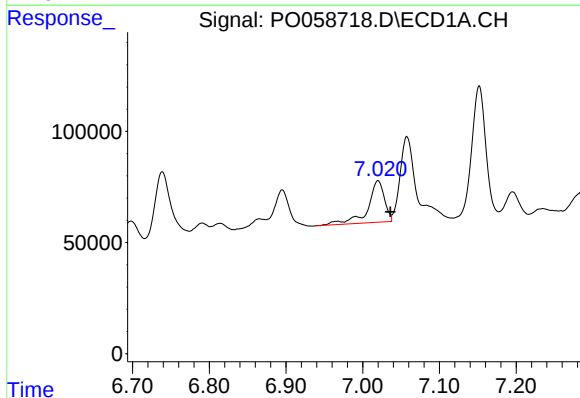


#29 AR-1254-4

R.T.: 7.020 min
Delta R.T.: -0.016 min
Response: 280308
Conc: 77.85 ng/ml

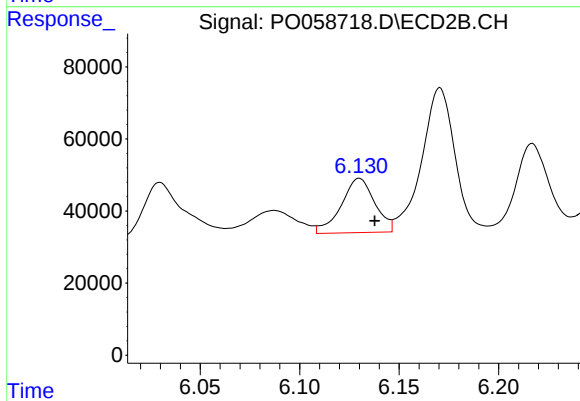

#29 AR-1254-4

R.T.: 6.130 min
Delta R.T.: -0.008 min
Response: 176720
Conc: 76.00 ng/ml

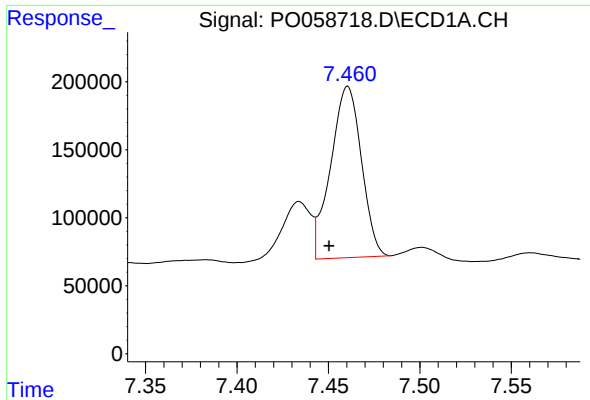


#30 AR-1254-5

R.T.: 7.461 min
Delta R.T.: 0.010 min
Response: 1476676
Conc: 407.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
S6-03-S

Manual Integrations
APPROVED

Ankita
8/2/2019 1:53:33 PM

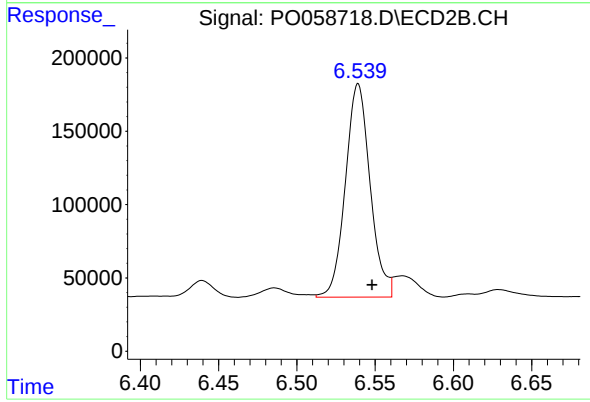

#30 AR-1254-5

R.T.: 6.539 min
Delta R.T.: -0.009 min
Response: 1600570
Conc: 463.99 ng/ml