

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080122\
 Data File : P0088467.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2022 12:15
 Operator : YP/AJ
 Sample : N3967-05DL 10X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S2-02-SDL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/02/2022
 Supervised By :Ankita Jodhani 08/02/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 12:42:43 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 26 11:20:17 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.443	3.603	6113638	2064096	2.396	2.188
2) SA Decachlor...	10.284	8.595	4237609	2858880	1.995	2.736 #
Target Compounds						
26) L6 AR-1254-1	6.478	5.478	8716687	5598622	91.935	97.106
27) L6 AR-1254-2	6.697	5.625	19988290	9619739	139.234	187.609 #
28) L6 AR-1254-3	7.067	6.029	33220697	20483626	226.799	252.418
29) L6 AR-1254-4	7.353	6.257	35827469	18249287	331.038	365.907
30) L6 AR-1254-5	7.774	6.674	64407771	71765325	535.156m	950.214 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080122\
Data File : PO088467.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Aug 2022 12:15
Operator : YP/AJ
Sample : N3967-05DL 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
S2-02-SDL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/02/2022
Supervised By :Ankita Jodhani 08/02/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 12:42:43 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO071422.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 26 11:20:17 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

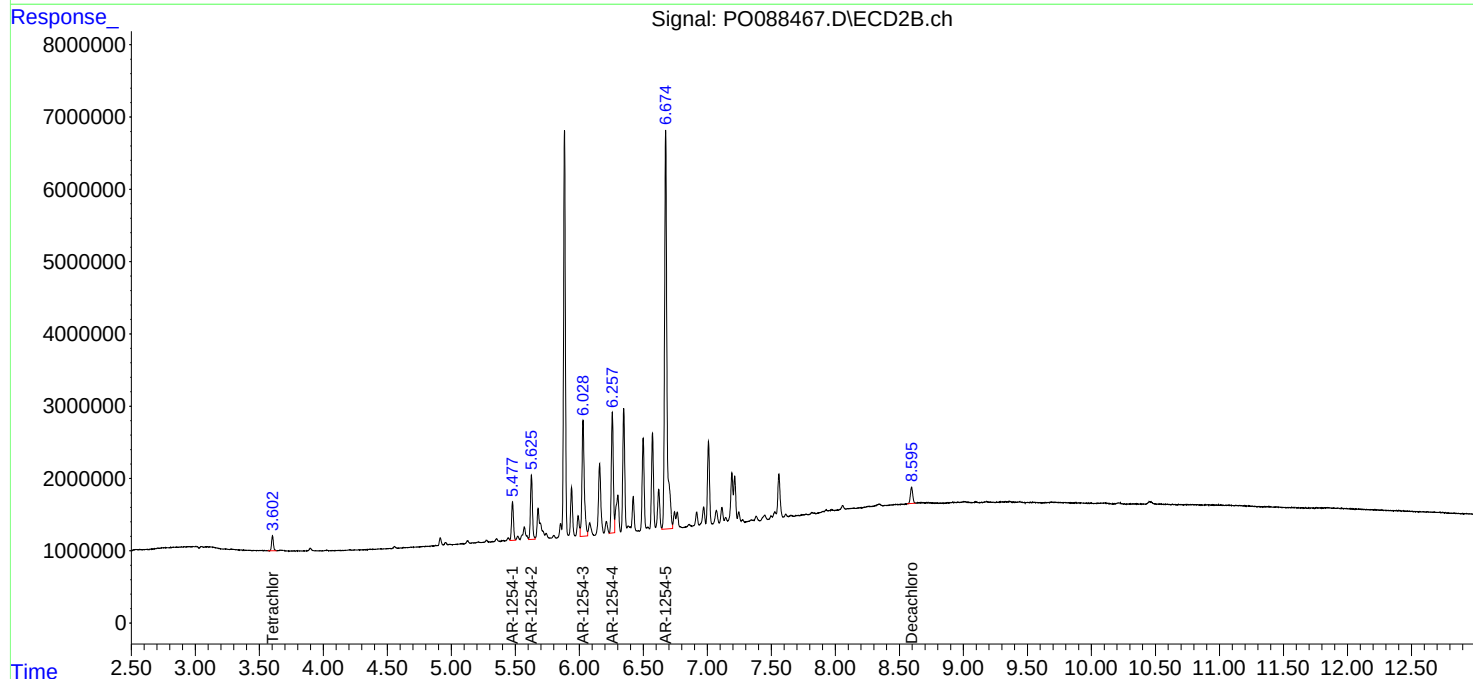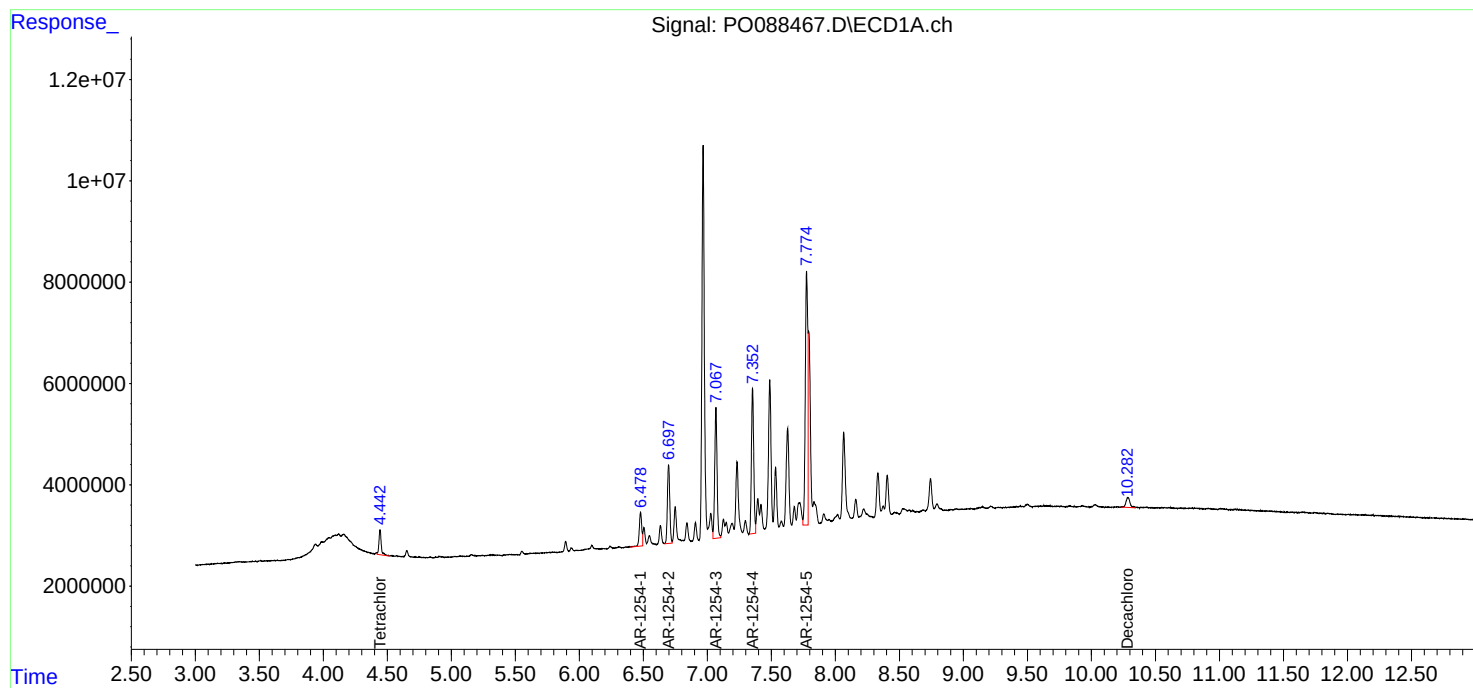

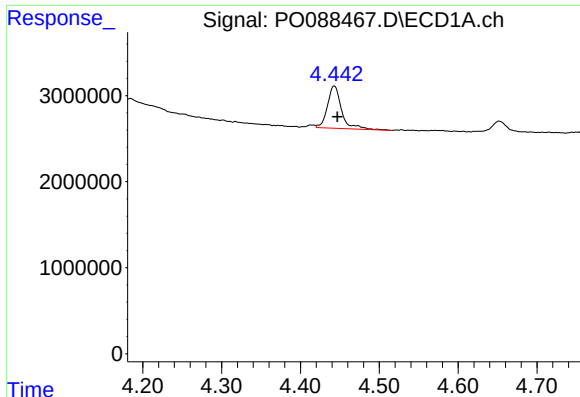


#1 Tetrachloro-m-xylene

R.T.: 4.443 min
Delta R.T.: -0.004 min
Response: 6113638
Conc: 2.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
S2-02-SDL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/02/2022
Supervised By :Ankita Jodhani 08/02/2022

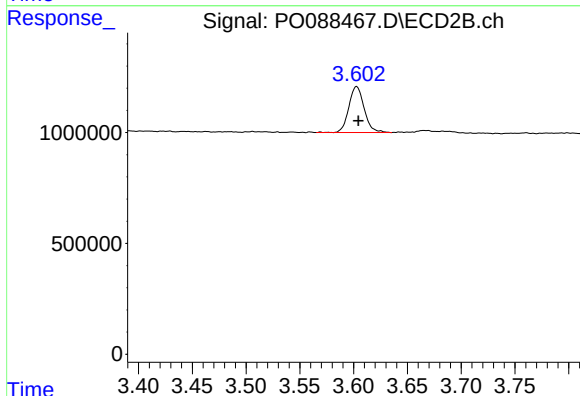


#1 Tetrachloro-m-xylene

R.T.: 3.603 min
Delta R.T.: -0.002 min
Response: 2064096
Conc: 2.19 ng/ml

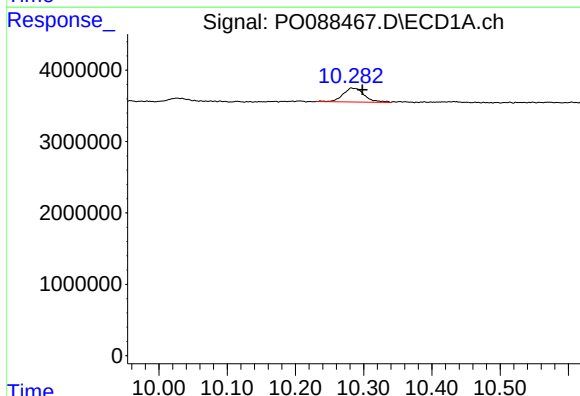


#2 Decachlorobiphenyl

R.T.: 10.284 min
Delta R.T.: -0.014 min
Response: 4237609
Conc: 2.00 ng/ml

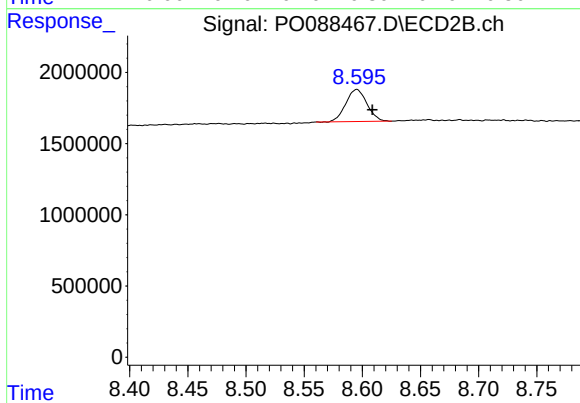

#2 Decachlorobiphenyl

R.T.: 8.595 min
Delta R.T.: -0.013 min
Response: 2858880
Conc: 2.74 ng/ml

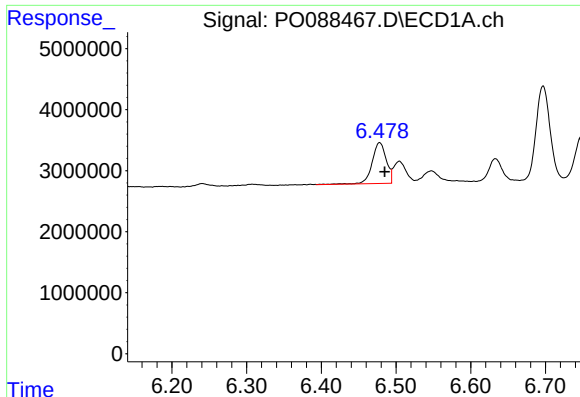


#26 AR-1254-1

R.T.: 6.478 min
Delta R.T.: -0.007 min
Response: 8716687
Conc: 91.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
S2-02-SDL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/02/2022
Supervised By :Ankita Jodhani 08/02/2022

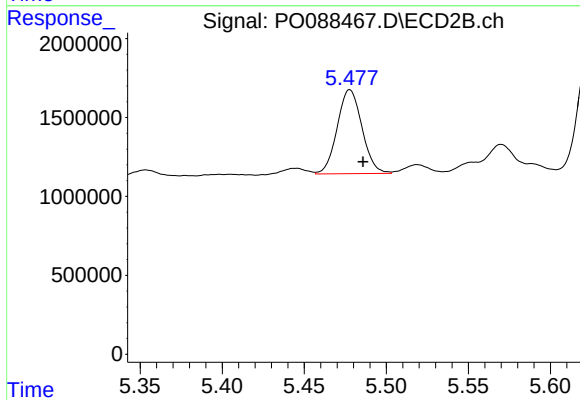


#26 AR-1254-1

R.T.: 5.478 min
Delta R.T.: -0.008 min
Response: 5598622
Conc: 97.11 ng/ml

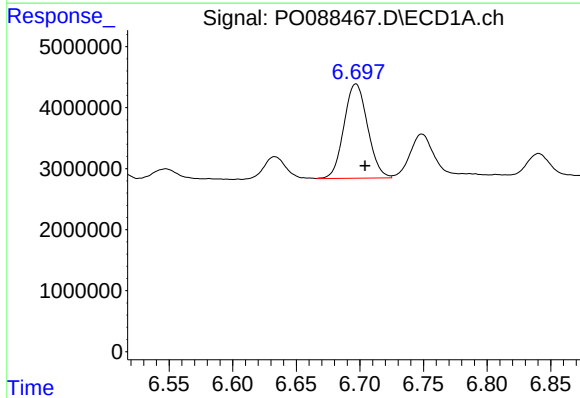


#27 AR-1254-2

R.T.: 6.697 min
Delta R.T.: -0.007 min
Response: 19988290
Conc: 139.23 ng/ml

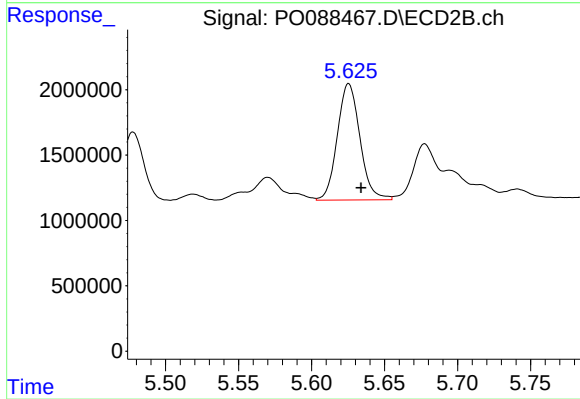

#27 AR-1254-2

R.T.: 5.625 min
Delta R.T.: -0.008 min
Response: 9619739
Conc: 187.61 ng/ml

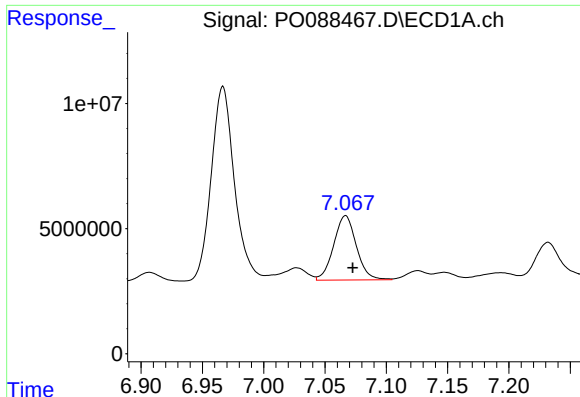


#28 AR-1254-3

R.T.: 7.067 min
Delta R.T.: -0.006 min
Response: 33220697
Conc: 226.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
S2-02-SDL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/02/2022
Supervised By :Ankita Jodhani 08/02/2022

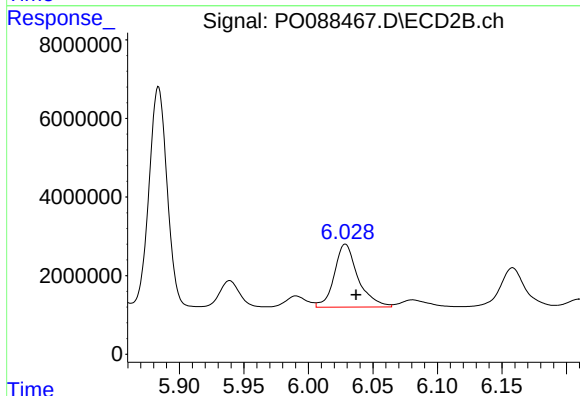


#28 AR-1254-3

R.T.: 6.029 min
Delta R.T.: -0.008 min
Response: 20483626
Conc: 252.42 ng/ml

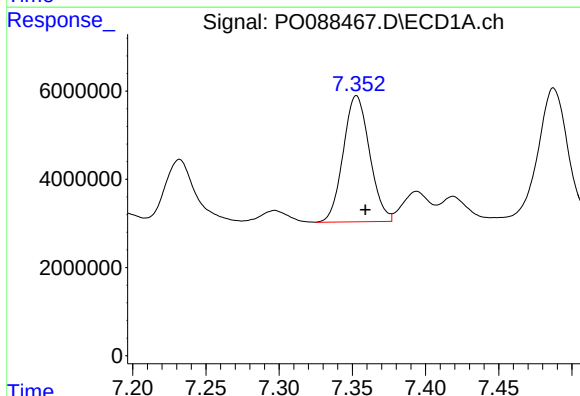


#29 AR-1254-4

R.T.: 7.353 min
Delta R.T.: -0.006 min
Response: 35827469
Conc: 331.04 ng/ml

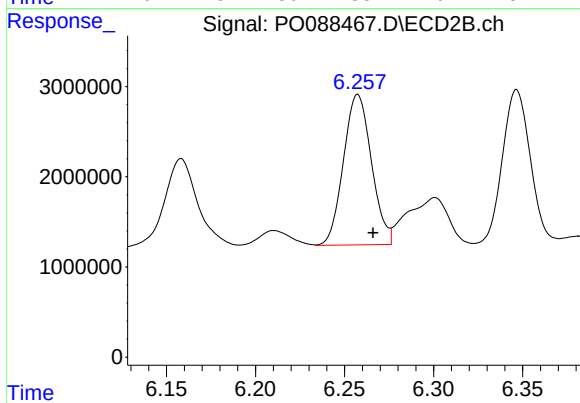

#29 AR-1254-4

R.T.: 6.257 min
Delta R.T.: -0.009 min
Response: 18249287
Conc: 365.91 ng/ml

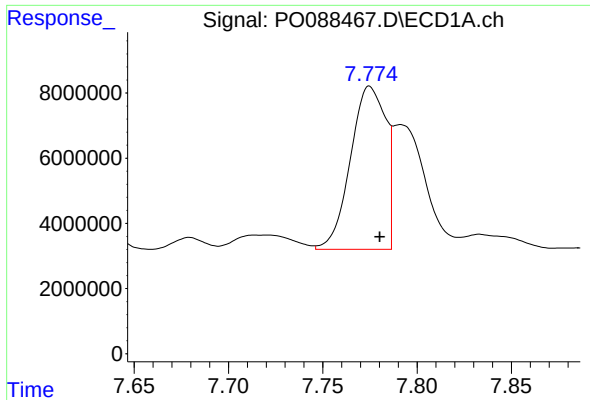


#30 AR-1254-5

R.T.: 7.774 min
Delta R.T.: -0.006 min
Response: 64407771
Conc: 535.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
S2-02-SDL

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/02/2022
Supervised By :Ankita Jodhani 08/02/2022

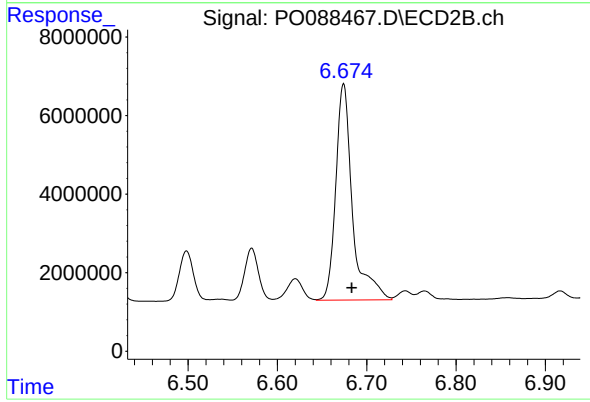

#30 AR-1254-5

R.T.: 6.674 min
Delta R.T.: -0.009 min
Response: 71765325
Conc: 950.21 ng/ml