

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080123\
 Data File : P0096564.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2023 19:23
 Operator : YP/AJ
 Sample : 03840-03
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BUILDING-B-19-(0-5)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 21:43:36 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jul 28 01:38:03 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.415	3.623	53525560	21554640	16.020	15.216
2) SA Decachlor...	10.242	8.647	30611281	16126296	13.835	13.709

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080123\
Data File : PO096564.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Aug 2023 19:23
Operator : YP/AJ
Sample : 03840-03
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
BUILDING-B-19-(0-5)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 21:43:36 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072723.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 28 01:38:03 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

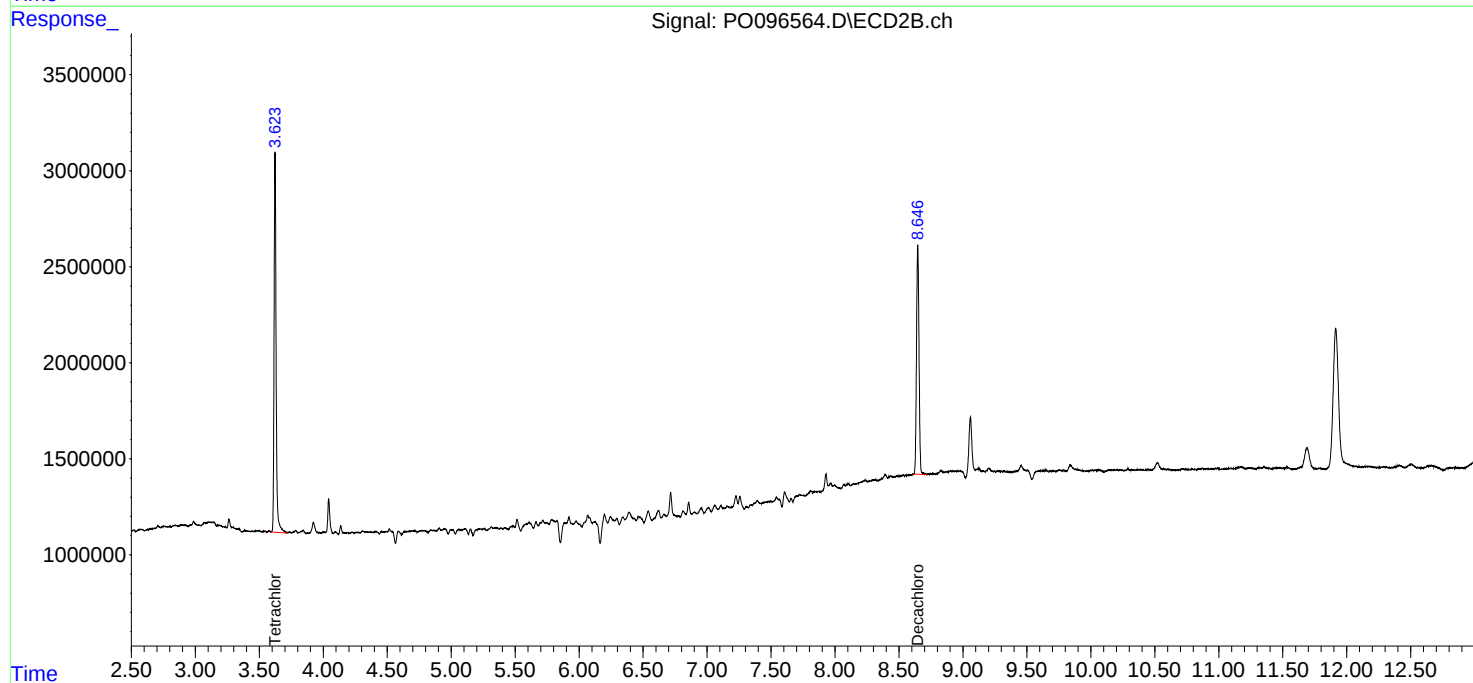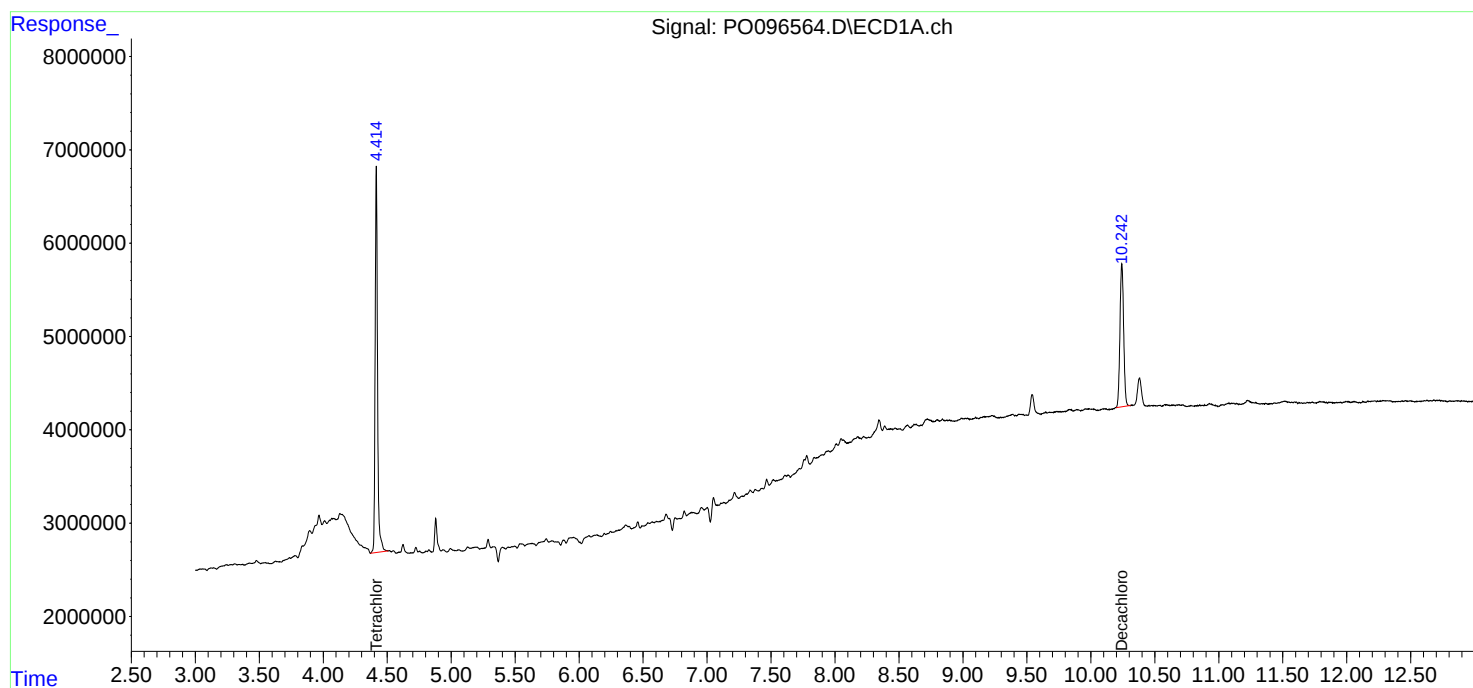


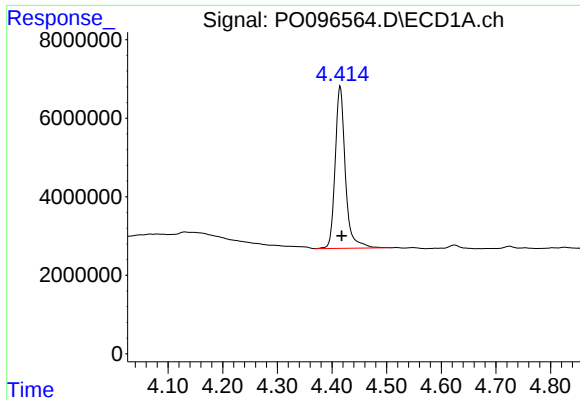

#1 Tetrachloro-m-xylene


R.T.: 4.415 min
Delta R.T.: -0.003 min
Response: 53525560
Conc: 16.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
BUILDING-B-19-(0-5)

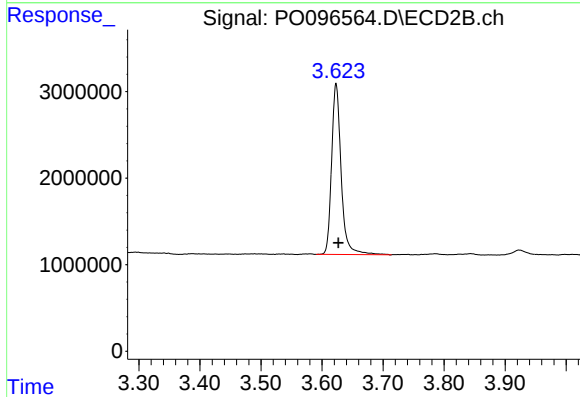


#1 Tetrachloro-m-xylene

R.T.: 3.623 min
Delta R.T.: -0.004 min
Response: 21554640
Conc: 15.22 ng/ml

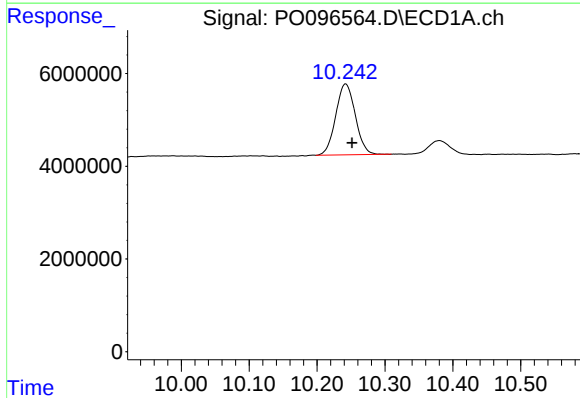

#2 Decachlorobiphenyl

R.T.: 10.242 min
Delta R.T.: -0.009 min
Response: 30611281
Conc: 13.84 ng/ml

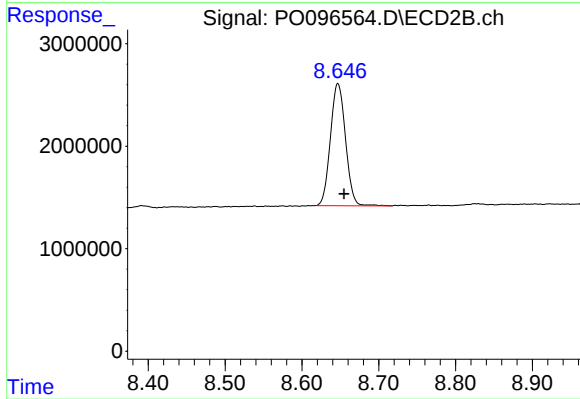

#2 Decachlorobiphenyl

R.T.: 8.647 min
Delta R.T.: -0.008 min
Response: 16126296
Conc: 13.71 ng/ml