

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080124\
 Data File : P0105096.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2024 14:38
 Operator : YP/AJ
 Sample : P3414-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PL-02-07312024-A

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/02/2024
 Supervised By :Ankita Jodhani 08/02/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 15:13:51 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072924.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 30 07:11:20 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.429	3.540	129.3E6	50765205	18.780m	19.923
2) SA Decachlor...	10.223	8.433	87699842	22752770	17.082	14.323

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080124\
Data File : PO105096.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Aug 2024 14:38
Operator : YP/AJ
Sample : P3414-01
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PL-02-07312024-A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/02/2024
Supervised By :Ankita Jodhani 08/02/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 15:13:51 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072924.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 30 07:11:20 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

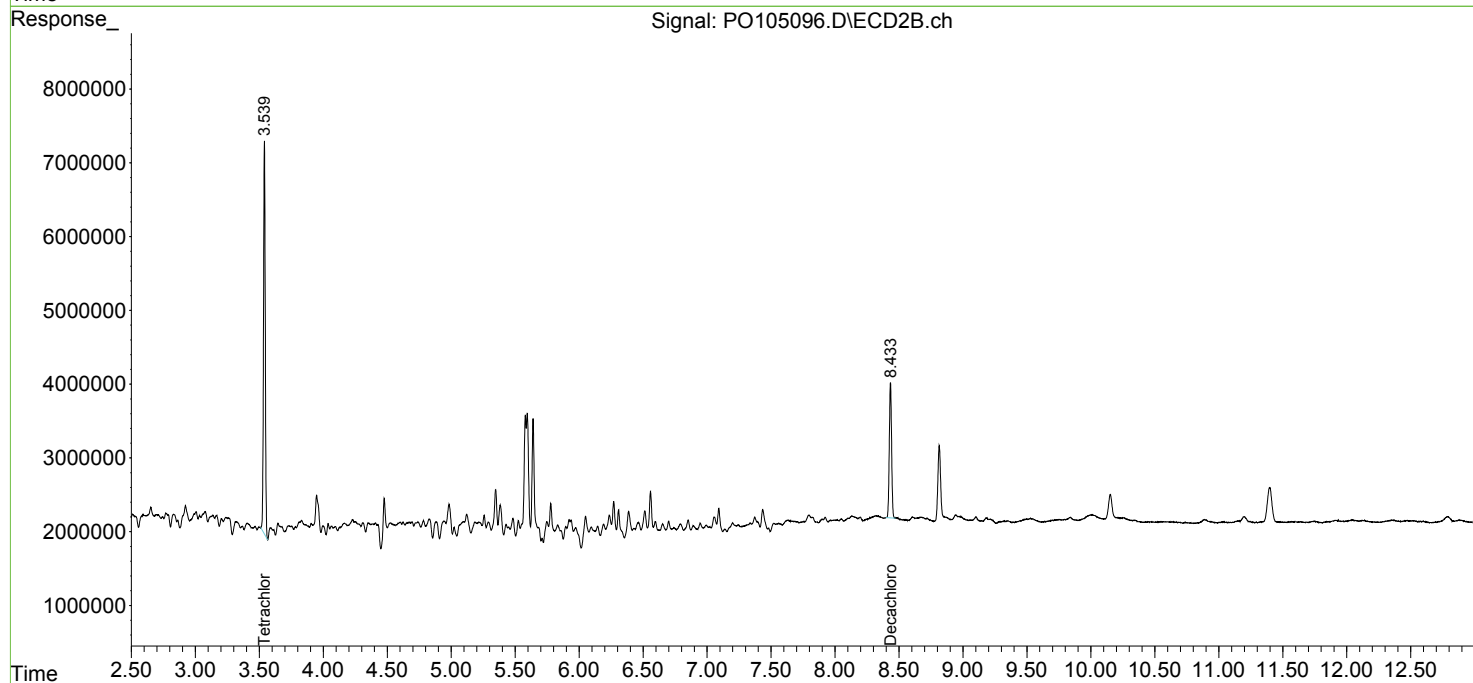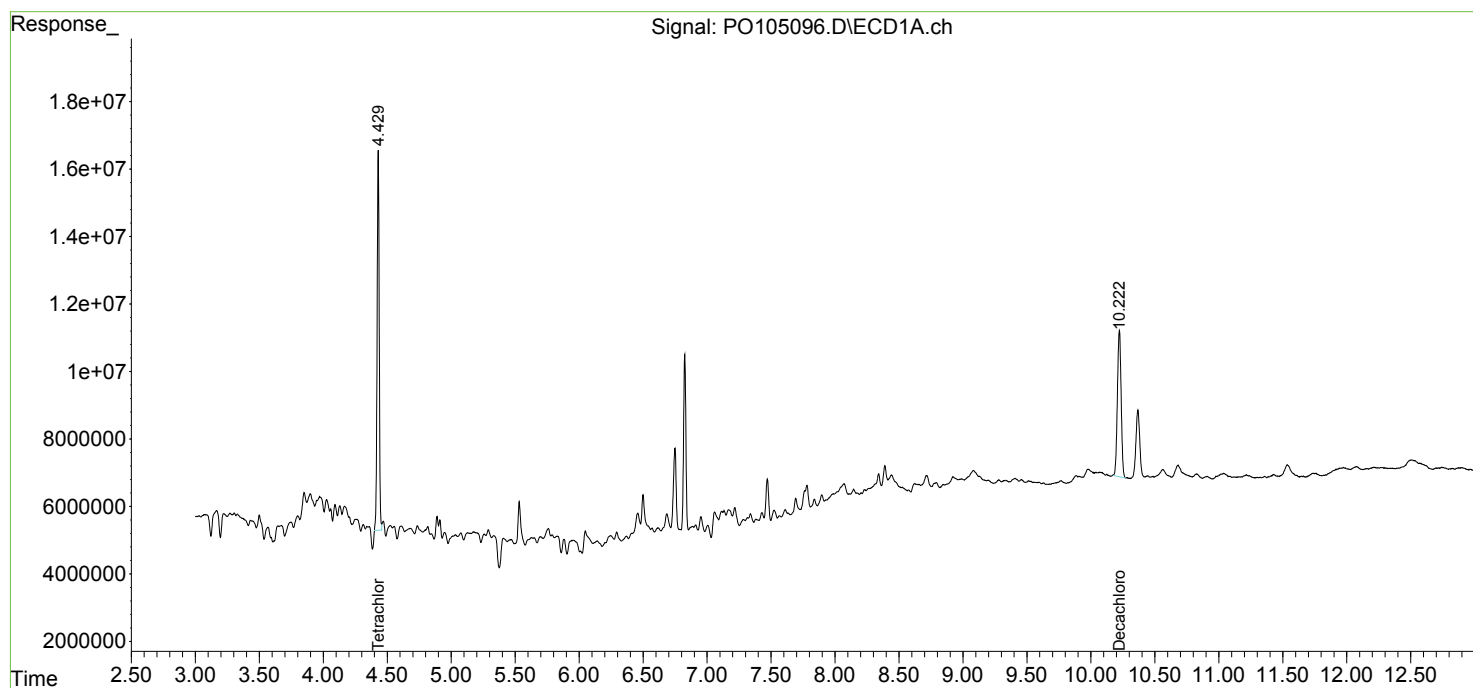

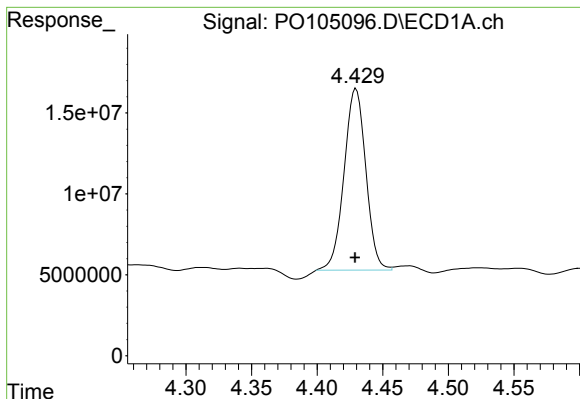

#1 Tetrachloro-m-xylene

R.T.: 4.429 min
Delta R.T.: 0.000 min
Response: 129287843
Conc: 18.78 ng/ml

Instrument :

ECD_O


ClientSampleId :

PL-02-07312024-A

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 08/02/2024
Supervised By :Ankita Jodhani 08/02/2024

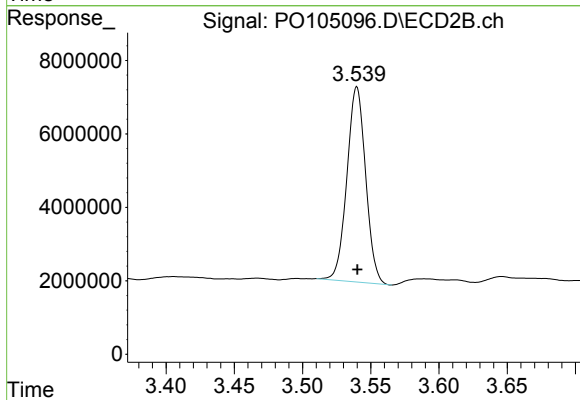


#1 Tetrachloro-m-xylene

R.T.: 3.540 min
Delta R.T.: 0.000 min
Response: 50765205
Conc: 19.92 ng/ml

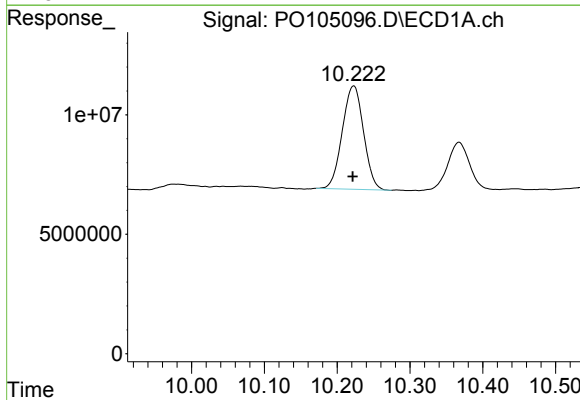

#2 Decachlorobiphenyl

R.T.: 10.223 min
Delta R.T.: 0.001 min
Response: 87699842
Conc: 17.08 ng/ml

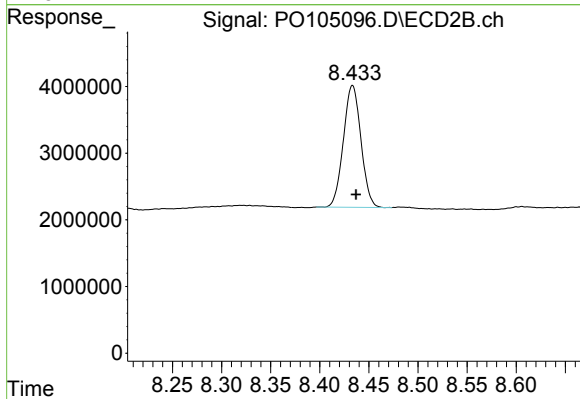

#2 Decachlorobiphenyl

R.T.: 8.433 min
Delta R.T.: -0.003 min
Response: 22752770
Conc: 14.32 ng/ml