

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080124\
 Data File : P0105097.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2024 14:55
 Operator : YP/AJ
 Sample : P3414-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PL-02-07312024-B

Manual Integrations
 APPROVED

Reviewed By :Yogesh
 Patel
 08/02/2024

Supervised By :Ankita
 Jodhani
 08/02/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 15:14:30 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072924.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 30 07:11:20 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.429	3.540	134.8E6	56375735	19.576m	22.125
2) SA Decachlor...	10.223	8.433	92104995	23943464	17.940	15.073

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080124\
Data File : PO105097.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Aug 2024 14:55
Operator : YP/AJ
Sample : P3414-03
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PL-02-07312024-B


Manual Integrations
APPROVED

Reviewed By :Yogesh
Patel
08/02/2024
Supervised By :Ankita
Jodhani
08/02/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 15:14:30 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072924.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 30 07:11:20 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

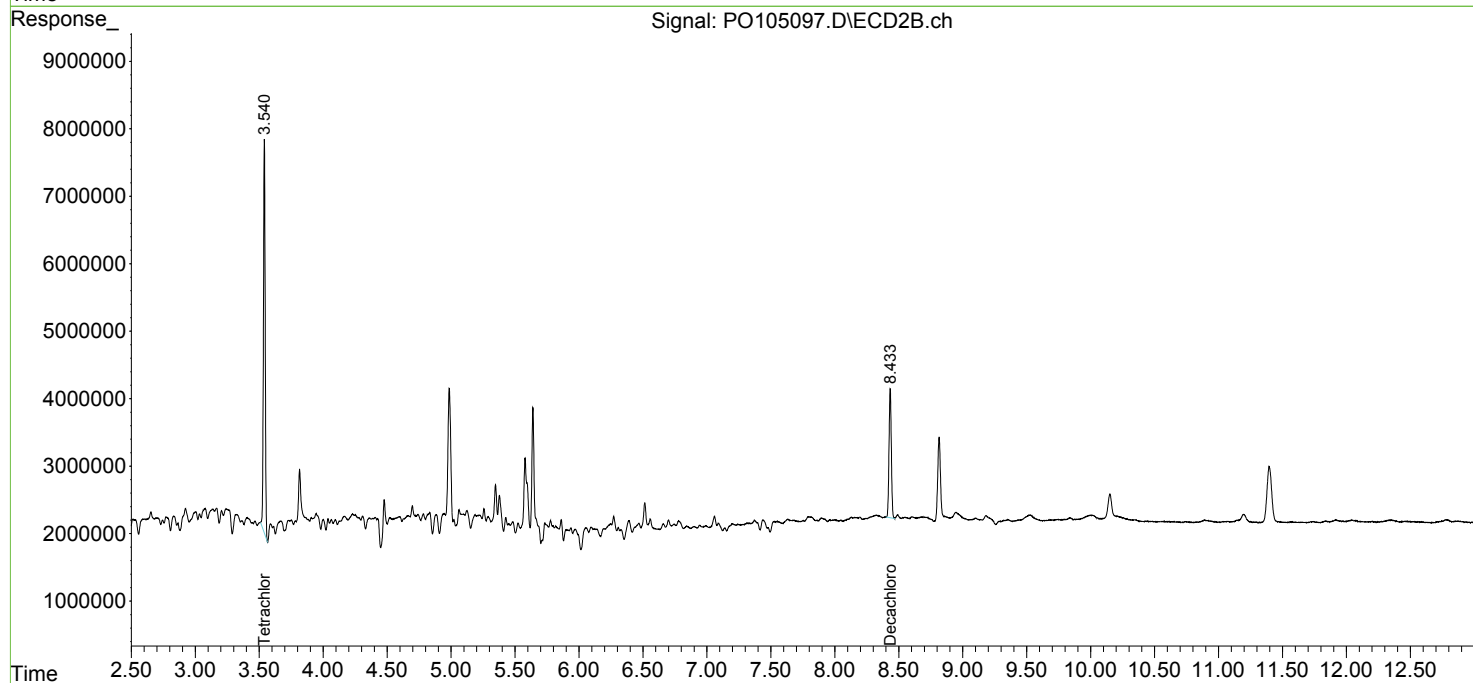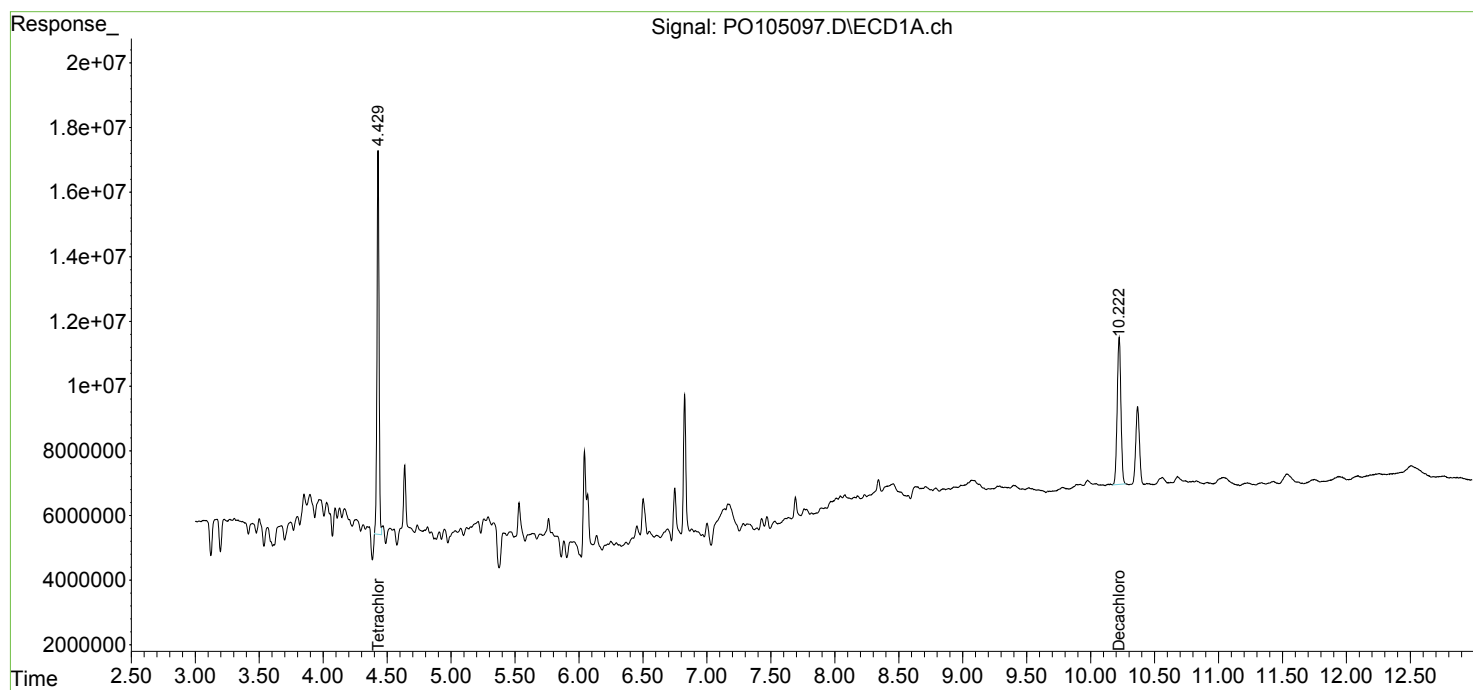

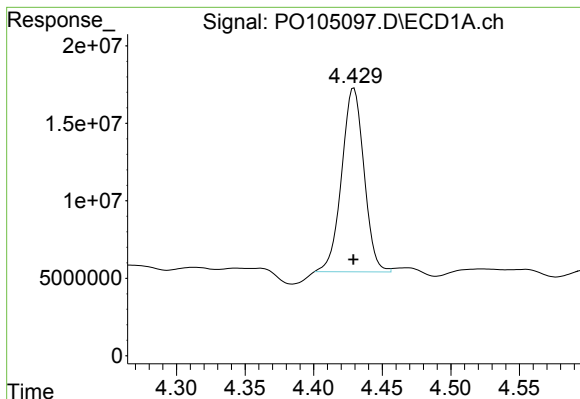

#1 Tetrachloro-m-xylene


R.T.: 4.429 min
Delta R.T.: 0.000 min
Response: 134765936
Conc: 19.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
PL-02-07312024-B

Manual Integrations
APPROVED


Reviewed By :Yogesh
Patel
08/02/2024

Supervised By :Ankita
Jodhani
08/02/2024

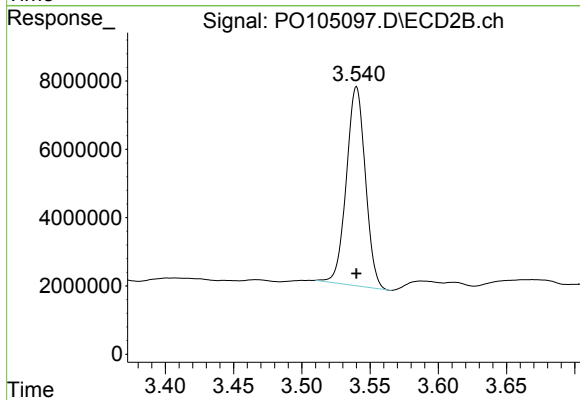


#1 Tetrachloro-m-xylene

R.T.: 3.540 min
Delta R.T.: 0.000 min
Response: 56375735
Conc: 22.12 ng/ml

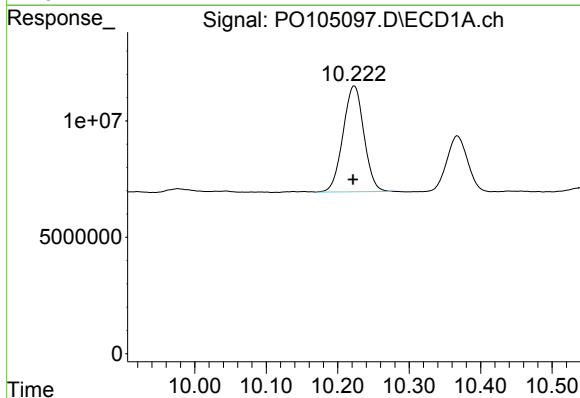

#2 Decachlorobiphenyl

R.T.: 10.223 min
Delta R.T.: 0.002 min
Response: 92104995
Conc: 17.94 ng/ml

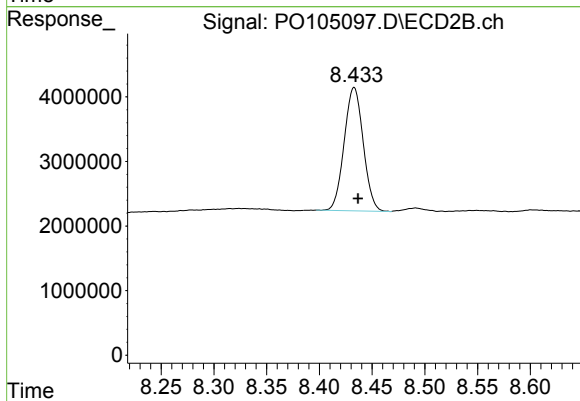

#2 Decachlorobiphenyl

R.T.: 8.433 min
Delta R.T.: -0.004 min
Response: 23943464
Conc: 15.07 ng/ml