

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080125\
 Data File : P0112662.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 10:32
 Operator : YP/AJ
 Sample : DDT ANALOG
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DDT ANALOG

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 02:30:26 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 24 04:54:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.670	3.662	132753	49442	0.016	0.010 #
2)	SA Decachlor...	8.692	8.623	43245	211793	0.006	0.120 #
Target Compounds							
3)	L1 AR-1016-1	4.758	4.733	1182326	358042	4.406	2.046 #
4)	L1 AR-1016-2	4.758	4.752	1182326	158396	2.911	0.608 #
5)	L1 AR-1016-3	4.825	4.936	1997111	3192959	7.632	23.483 #
6)	L1 AR-1016-4	4.945	4.982	7070888	4045754	33.378	36.420
7)	L1 AR-1016-5	5.220	5.190	67211667	13950460	306.245	97.349 #
8)	L2 AR-1221-1	3.892	3.869	277545	233124	2.871	3.466
9)	L2 AR-1221-2	3.982	3.966	544990	328631	7.584	6.478
10)	L2 AR-1221-3	3.982f	4.031	544990	147313	2.293	0.929 #
11)	L3 AR-1232-1	3.982f	4.031	544990	147313	2.915	1.164 #
12)	L3 AR-1232-2	4.554	4.752	2327124	158396	21.623	1.208 #
13)	L3 AR-1232-3	4.791	4.936	1866399	3192959	9.025	47.517 #
14)	L3 AR-1232-4	4.945	5.015	7070888	2779533	67.509	46.458 #
15)	L3 AR-1232-5	5.021	5.190	23396783	13950460	344.674	213.954 #
16)	L4 AR-1242-1	4.758	4.733	1182326	358042	4.775	2.260 #
17)	L4 AR-1242-2	4.758	4.752	1182326	158396	3.197	0.678 #
18)	L4 AR-1242-3	4.825	4.936	1997111	3192959	8.439	26.347 #
19)	L4 AR-1242-4	4.945	5.015	7070888	2779533	36.396	22.646 #
20)	L4 AR-1242-5	5.581	5.517	112.0E6	9980768	523.449	62.003 #
21)	L5 AR-1248-1	4.758	4.733	1182326	358042	6.316	2.947 #
22)	L5 AR-1248-2	5.021	4.982	23396783	4045754	91.712	23.900 #
23)	L5 AR-1248-3	5.220	5.015	67211667	2779533	195.553	15.646 #
24)	L5 AR-1248-4	5.546	5.190	40382019	13950460	79.480	66.955
25)	L5 AR-1248-5	5.581	5.587	112.0E6	3947174	320.299	18.379 #
26)	L6 AR-1254-1	5.546	5.517	40382019	9980768	73.561	30.372 #
27)	L6 AR-1254-2	5.728	5.700	88798000	26449525	182.742	91.366 #
28)	L6 AR-1254-3	6.128	6.097	13811100	32687070	18.556	76.468 #
29)	L6 AR-1254-4	6.343	6.309	973975	1369461	1.772	5.017 #
30)	L6 AR-1254-5	6.757	6.722	4100.3E6	1893.1E6	5792.825	5667.747
31)	L7 AR-1260-1	6.243	6.211	304408	3052326	0.693	12.282 #
32)	L7 AR-1260-2	6.434	6.400	10189274	5766025	14.812	17.500
33)	L7 AR-1260-3	6.825	6.596f	1421961	539588	2.418	2.100
34)	L7 AR-1260-4	7.055	7.016	5102607	760819	11.314	3.977 #
35)	L7 AR-1260-5	7.309	7.254	1673590	525500	1.351	1.275
36)	L8 AR-1262-1	6.825	6.722f	1421961	1893.1E6	1.530	4563.672 #
37)	L8 AR-1262-2	7.309	7.254	1673590	525500	1.125	1.019
38)	L8 AR-1262-3	7.598	7.553	58092347	26586960	98.419	142.538 #
39)	L8 AR-1262-4	7.598f	7.553f	58092347	26586960	58.433	92.283 #
40)	L8 AR-1262-5	8.156	0.000	545727	0	1.257	N.D. #
41)	L9 AR-1268-1	7.598	7.553	58092347	26586960	33.174	51.340 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080125\
 Data File : P0112662.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 10:32
 Operator : YP/AJ
 Sample : DDT ANALOG
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DDT ANALOG

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 02:30:26 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 24 04:54:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	7.704f	7.553f	661689	26586960	0.449	62.548 #
43) L9	AR-1268-3	7.845	7.870f	703916	89877	0.562	0.280 #
44) L9	AR-1268-4	8.156	0.000	545727	0	1.133	N.D. #
45) L9	AR-1268-5	8.434	8.380	697545	198753	0.208	0.272 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080125\
Data File : PO112662.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Aug 2025 10:32
Operator : YP/AJ
Sample : DDT ANALOG
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 02:30:26 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072325.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 24 04:54:06 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

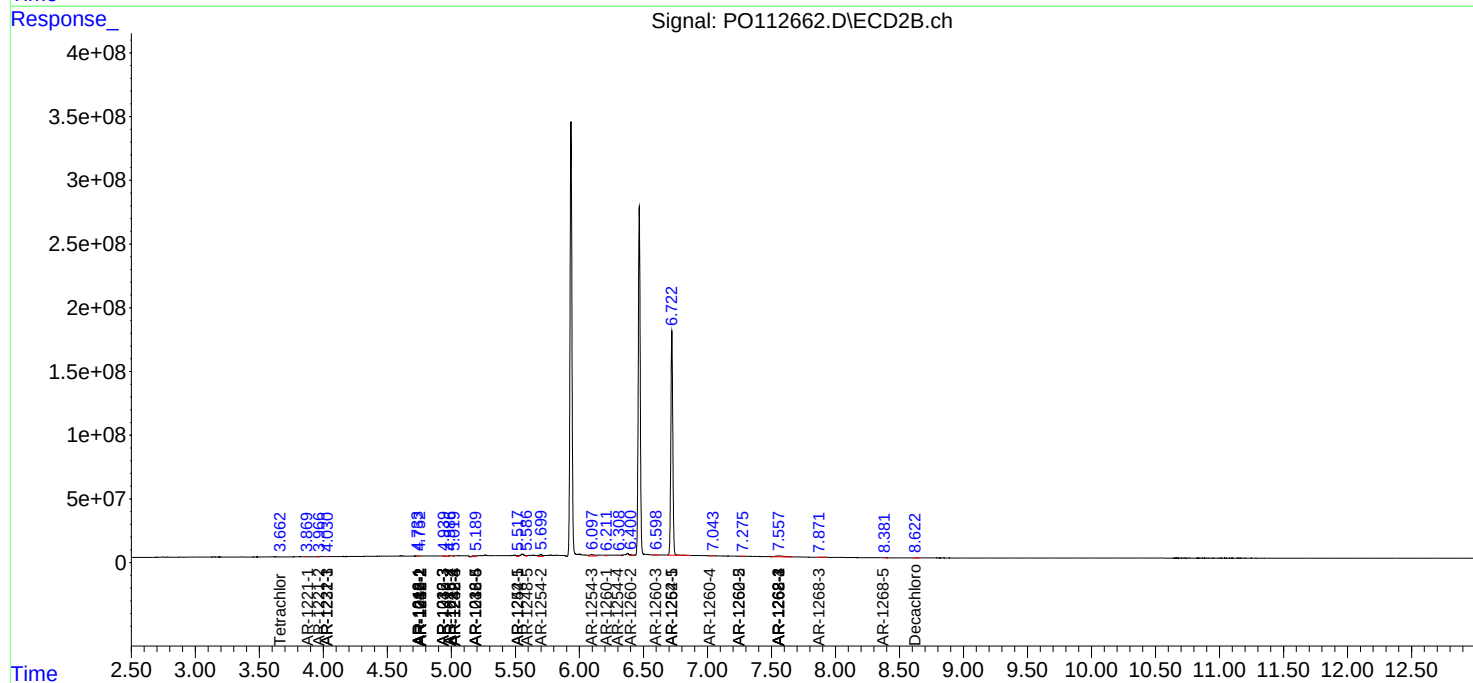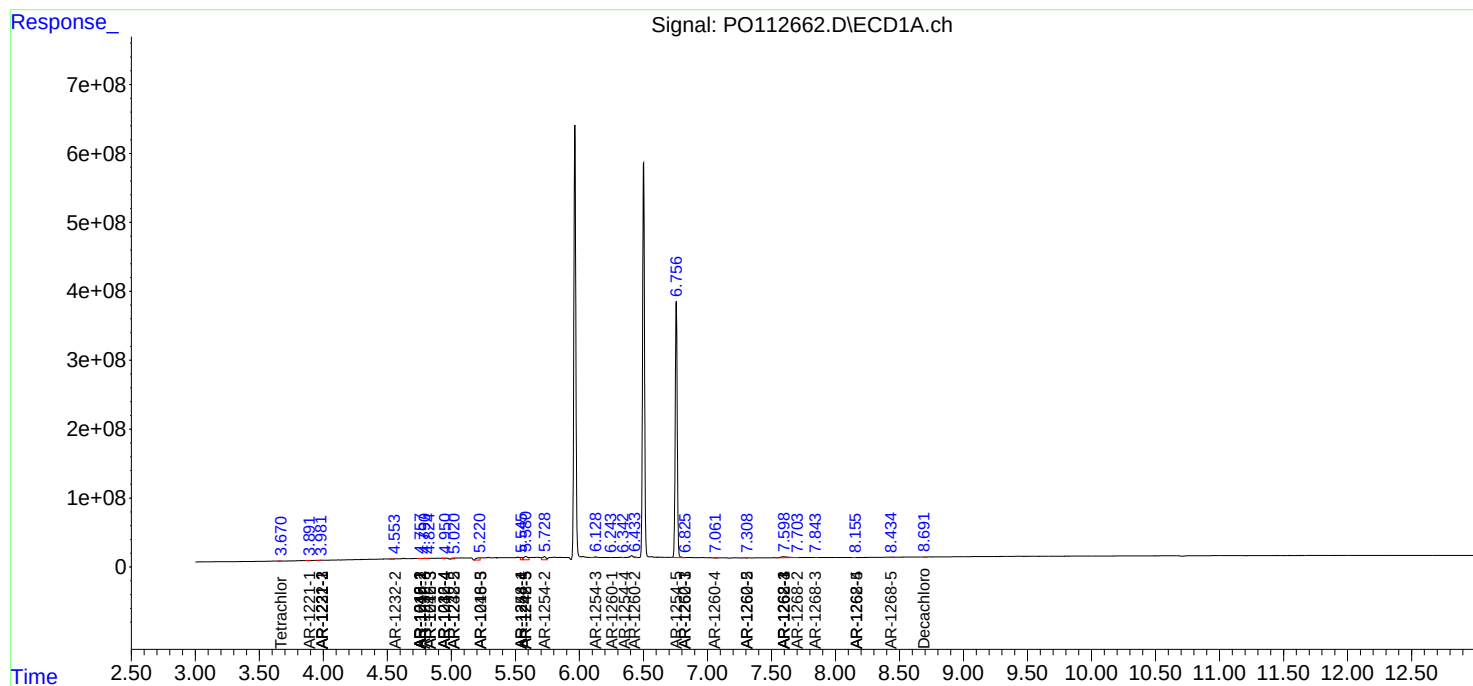


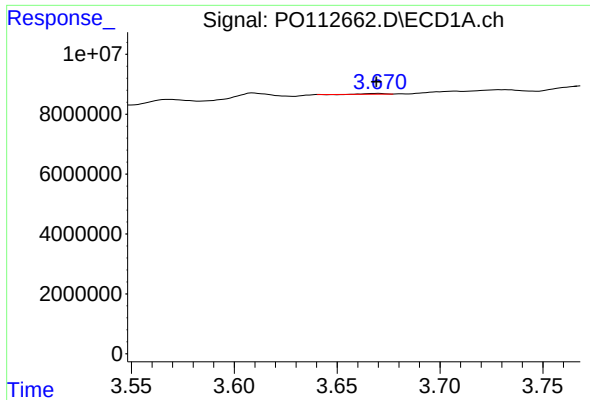

#1 Tetrachloro-m-xylene


R.T.: 3.670 min
Delta R.T.: 0.000 min
Response: 132753
Conc: 0.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

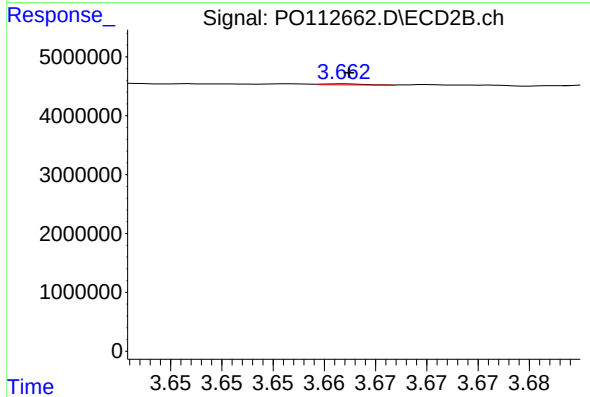


#1 Tetrachloro-m-xylene

R.T.: 3.662 min
Delta R.T.: 0.000 min
Response: 49442
Conc: 0.01 ng/ml

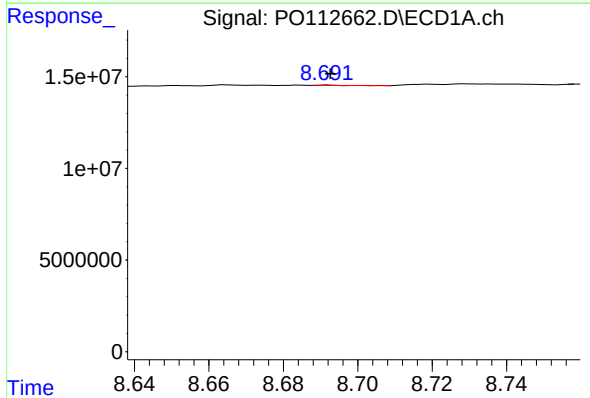


#2 Decachlorobiphenyl

R.T.: 8.692 min
Delta R.T.: 0.000 min
Response: 43245
Conc: 0.01 ng/ml

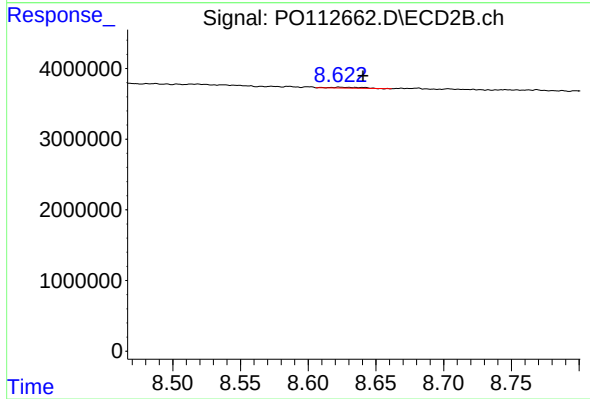

#2 Decachlorobiphenyl


R.T.: 8.623 min
Delta R.T.: -0.018 min
Response: 211793
Conc: 0.12 ng/ml

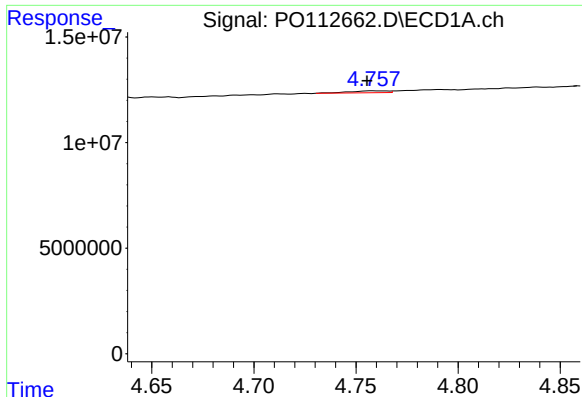

#3 AR-1016-1


R.T.: 4.758 min
Delta R.T.: 0.003 min
Response: 1182326
Conc: 4.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

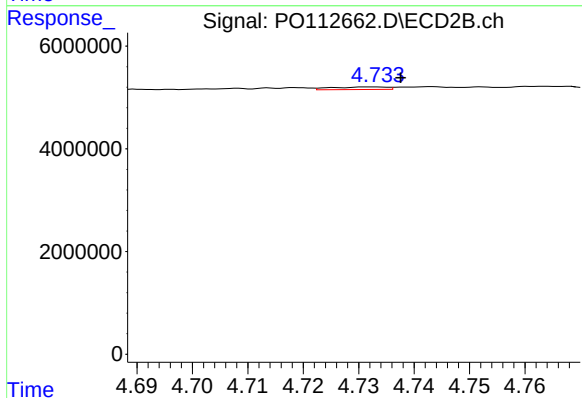


#3 AR-1016-1

R.T.: 4.733 min
Delta R.T.: -0.005 min
Response: 358042
Conc: 2.05 ng/ml

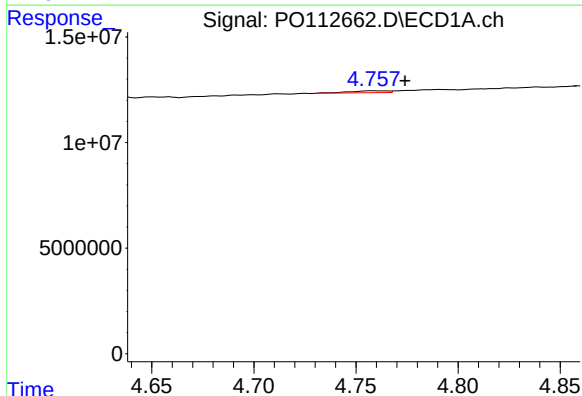


#4 AR-1016-2

R.T.: 4.758 min
Delta R.T.: -0.016 min
Response: 1182326
Conc: 2.91 ng/ml

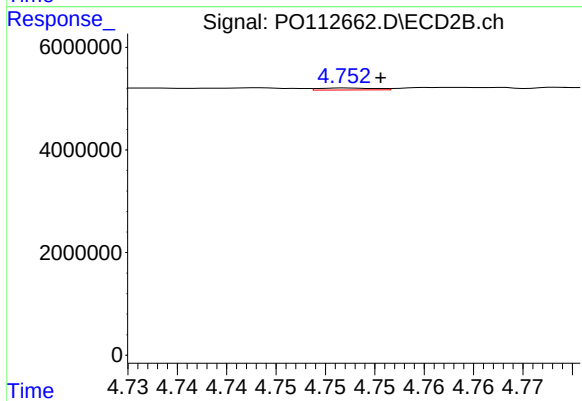

#4 AR-1016-2


R.T.: 4.752 min
Delta R.T.: -0.004 min
Response: 158396
Conc: 0.61 ng/ml

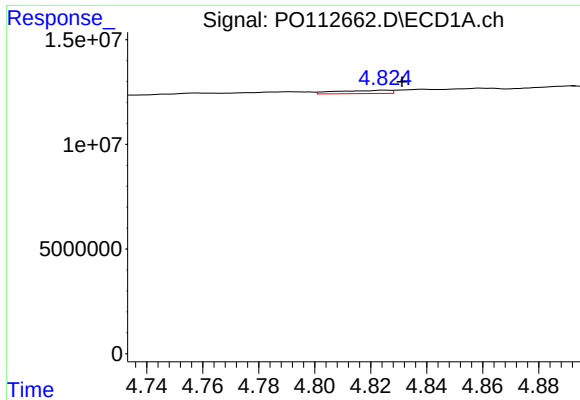

#5 AR-1016-3


R.T.: 4.825 min
Delta R.T.: -0.006 min
Response: 1997111
Conc: 7.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

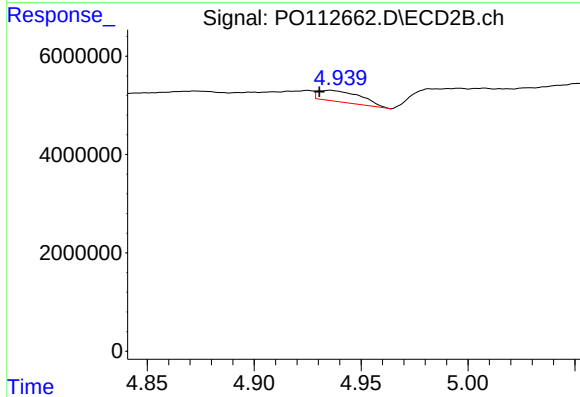


#5 AR-1016-3

R.T.: 4.936 min
Delta R.T.: 0.005 min
Response: 3192959
Conc: 23.48 ng/ml

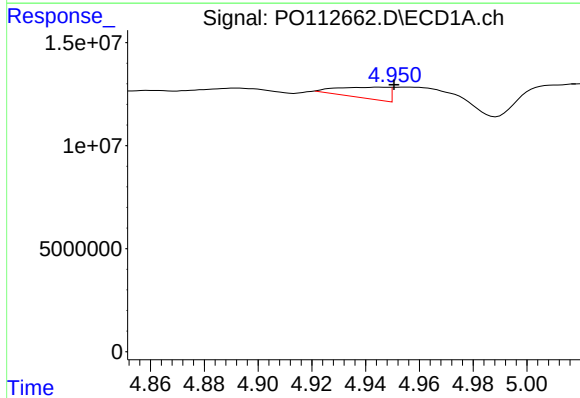


#6 AR-1016-4

R.T.: 4.945 min
Delta R.T.: -0.005 min
Response: 7070888
Conc: 33.38 ng/ml

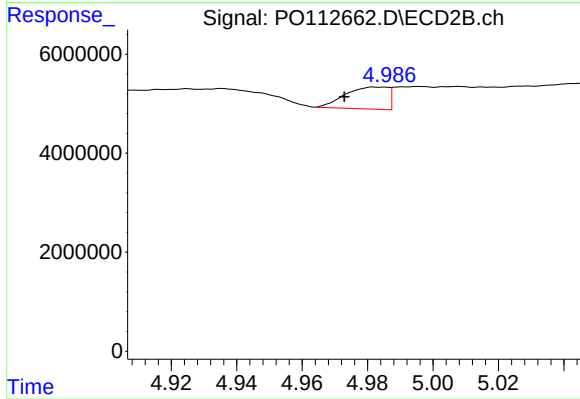

#6 AR-1016-4


R.T.: 4.982 min
Delta R.T.: 0.009 min
Response: 4045754
Conc: 36.42 ng/ml

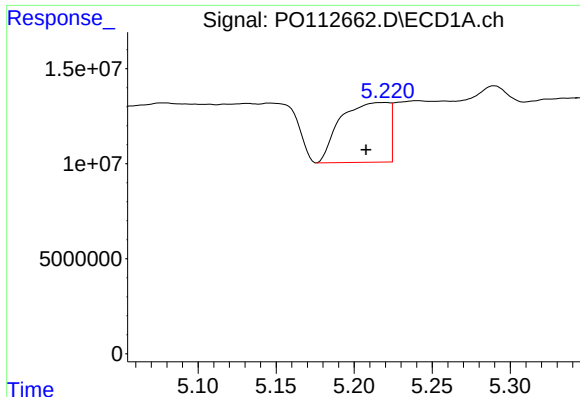

#7 AR-1016-5


R.T.: 5.220 min
Delta R.T.: 0.012 min
Response: 67211667
Conc: 306.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

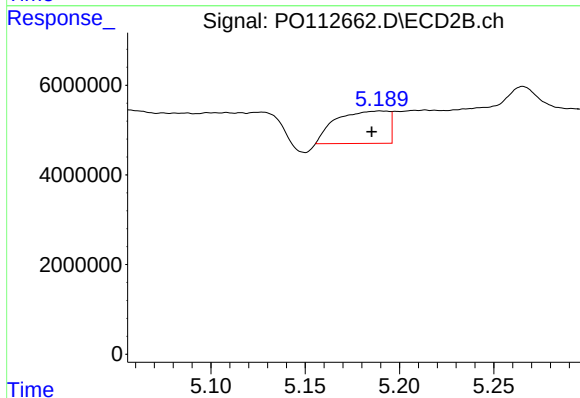


#7 AR-1016-5

R.T.: 5.190 min
Delta R.T.: 0.004 min
Response: 13950460
Conc: 97.35 ng/ml

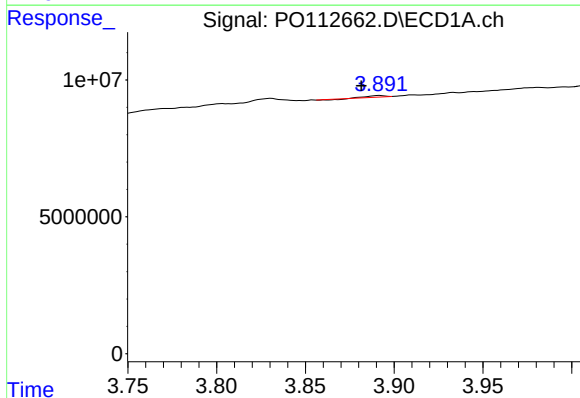


#8 AR-1221-1

R.T.: 3.892 min
Delta R.T.: 0.010 min
Response: 277545
Conc: 2.87 ng/ml

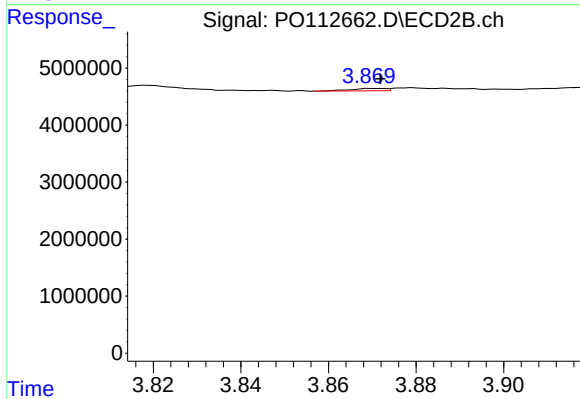

#8 AR-1221-1


R.T.: 3.869 min
Delta R.T.: -0.002 min
Response: 233124
Conc: 3.47 ng/ml

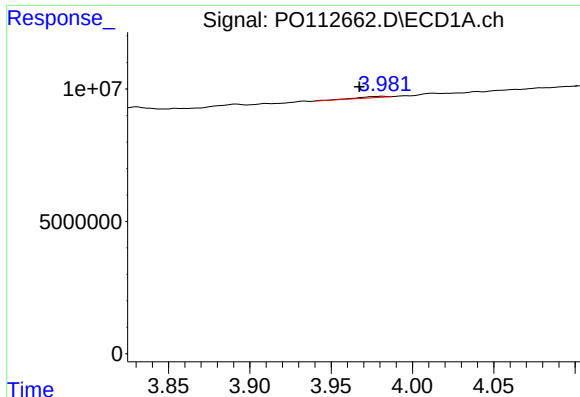

#9 AR-1221-2


R.T.: 3.982 min
Delta R.T.: 0.015 min
Response: 544990
Conc: 7.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

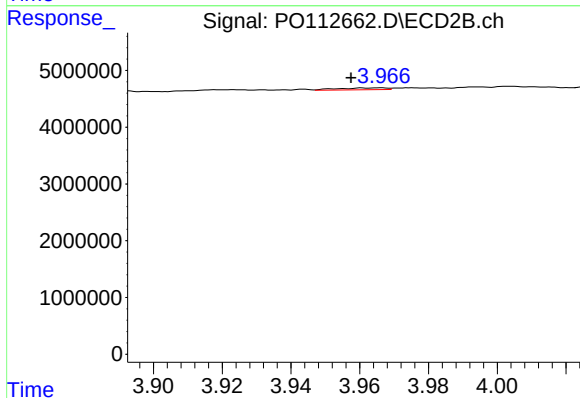


#9 AR-1221-2

R.T.: 3.966 min
Delta R.T.: 0.009 min
Response: 328631
Conc: 6.48 ng/ml

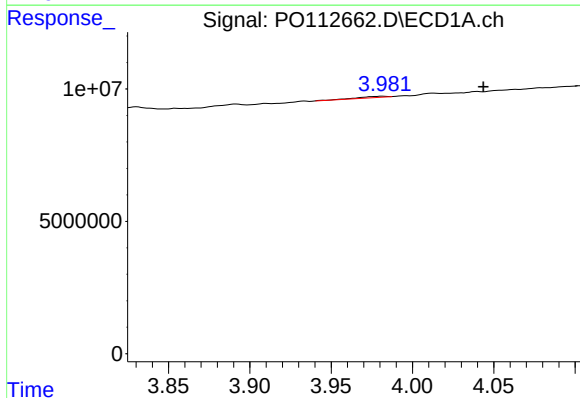


#10 AR-1221-3

R.T.: 3.982 min
Delta R.T.: -0.062 min
Response: 544990
Conc: 2.29 ng/ml

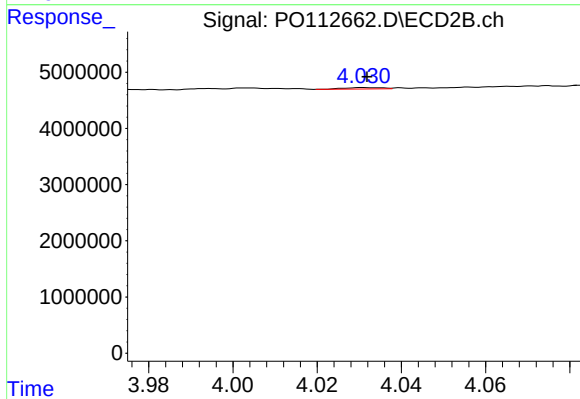

#10 AR-1221-3


R.T.: 4.031 min
Delta R.T.: 0.000 min
Response: 147313
Conc: 0.93 ng/ml

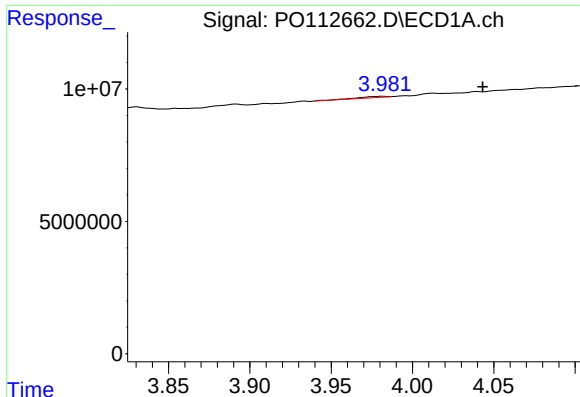

#11 AR-1232-1


R.T.: 3.982 min
Delta R.T.: -0.061 min
Response: 544990
Conc: 2.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

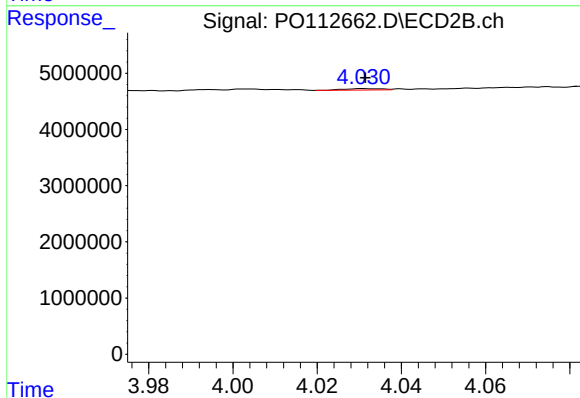


#11 AR-1232-1

R.T.: 4.031 min
Delta R.T.: 0.000 min
Response: 147313
Conc: 1.16 ng/ml

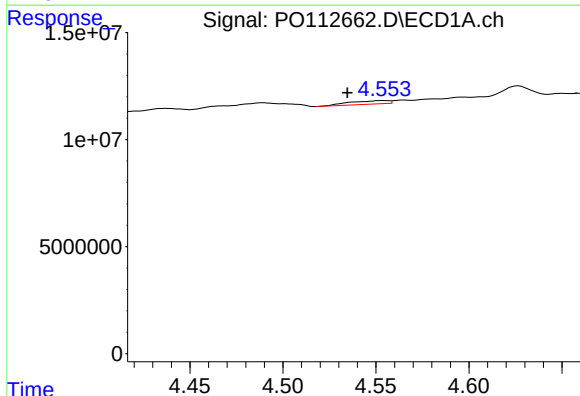


#12 AR-1232-2

R.T.: 4.554 min
Delta R.T.: 0.020 min
Response: 2327124
Conc: 21.62 ng/ml

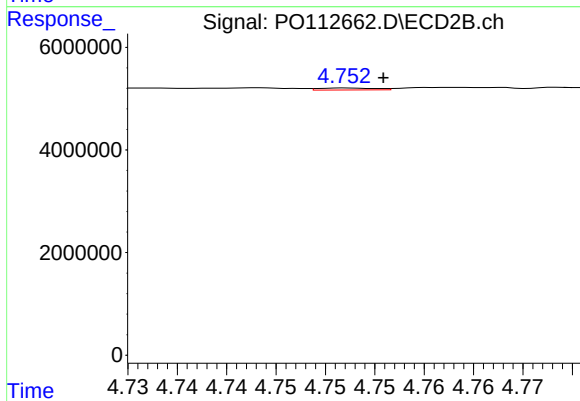

#12 AR-1232-2


R.T.: 4.752 min
Delta R.T.: -0.004 min
Response: 158396
Conc: 1.21 ng/ml

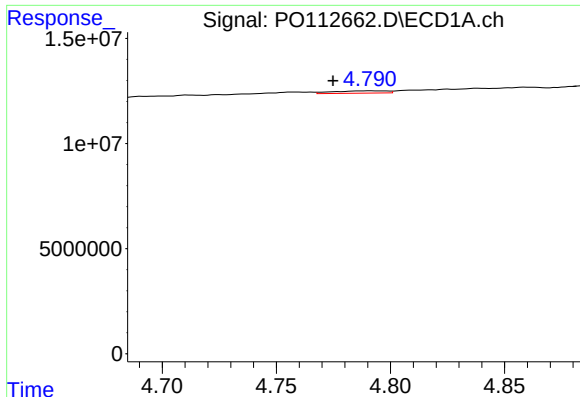

#13 AR-1232-3


R.T.: 4.791 min
Delta R.T.: 0.016 min
Response: 1866399
Conc: 9.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

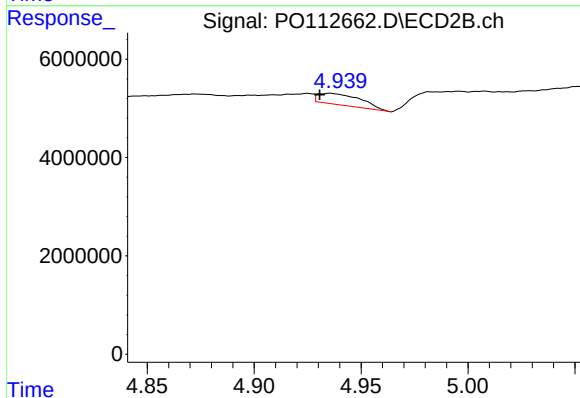


#13 AR-1232-3

R.T.: 4.936 min
Delta R.T.: 0.005 min
Response: 3192959
Conc: 47.52 ng/ml

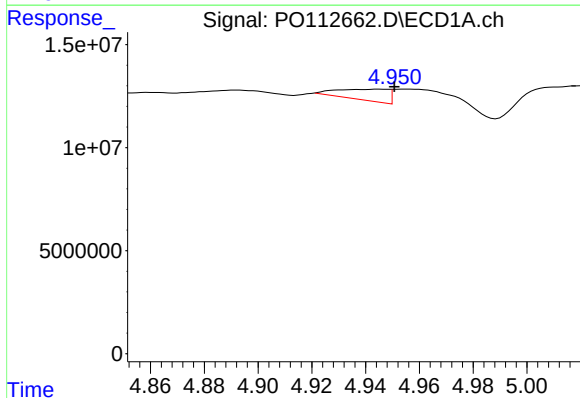


#14 AR-1232-4

R.T.: 4.945 min
Delta R.T.: -0.005 min
Response: 7070888
Conc: 67.51 ng/ml

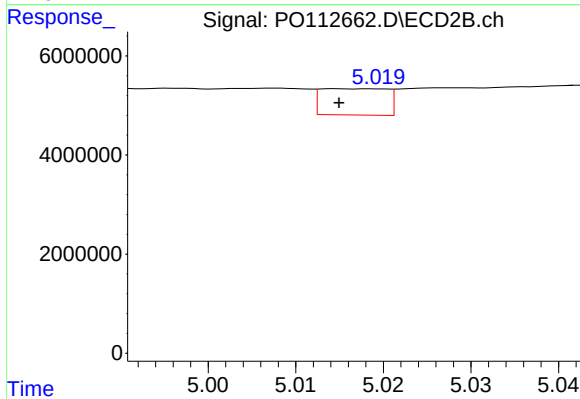

#14 AR-1232-4


R.T.: 5.015 min
Delta R.T.: 0.000 min
Response: 2779533
Conc: 46.46 ng/ml

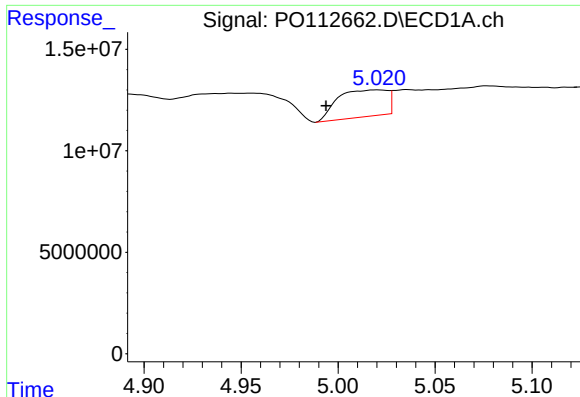

#15 AR-1232-5


R.T.: 5.021 min
Delta R.T.: 0.027 min
Response: 23396783
Conc: 344.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

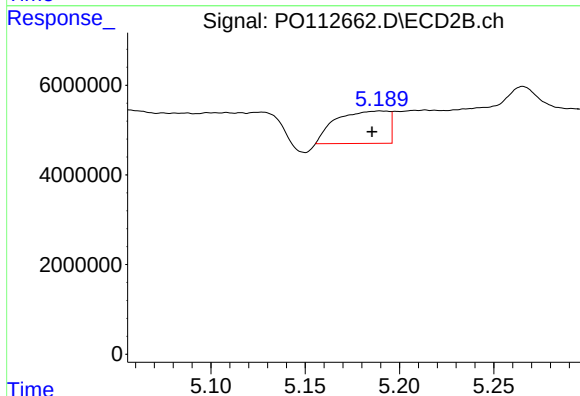


#15 AR-1232-5

R.T.: 5.190 min
Delta R.T.: 0.004 min
Response: 13950460
Conc: 213.95 ng/ml

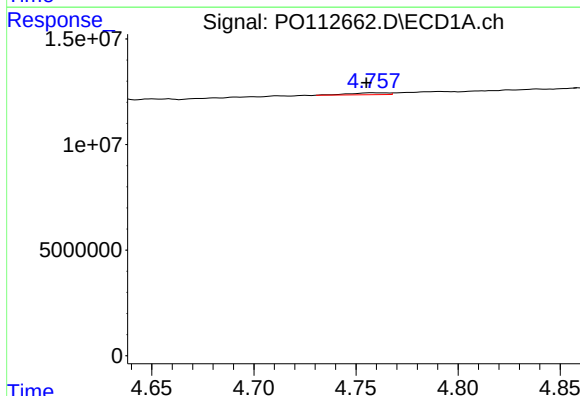


#16 AR-1242-1

R.T.: 4.758 min
Delta R.T.: 0.003 min
Response: 1182326
Conc: 4.78 ng/ml

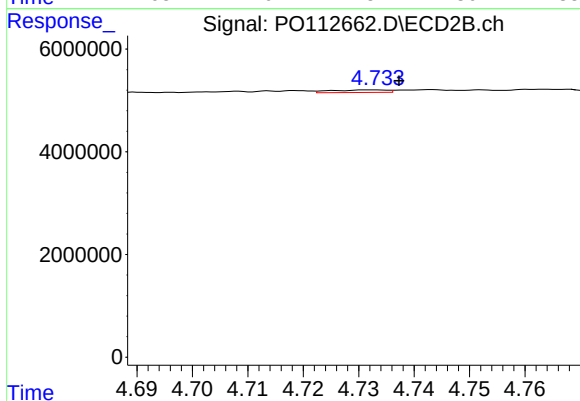

#16 AR-1242-1


R.T.: 4.733 min
Delta R.T.: -0.005 min
Response: 358042
Conc: 2.26 ng/ml

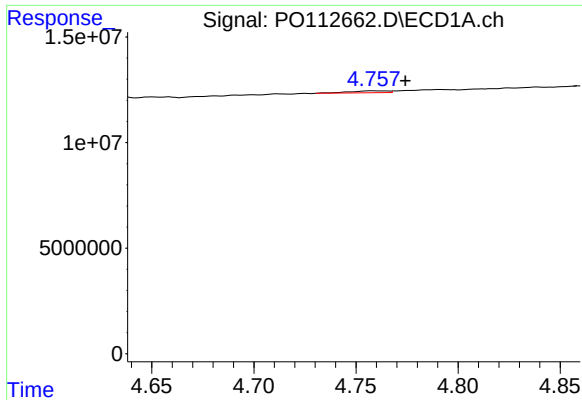

#17 AR-1242-2


R.T.: 4.758 min
Delta R.T.: -0.016 min
Response: 1182326
Conc: 3.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

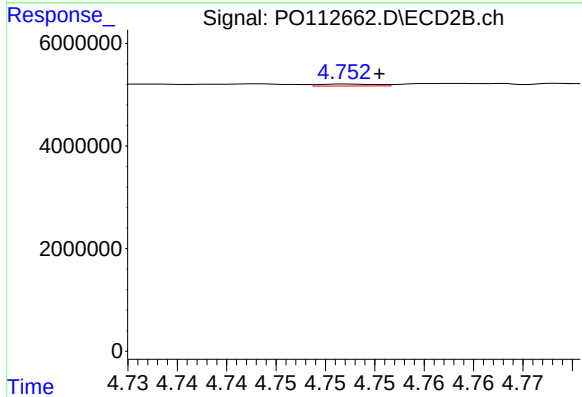


#17 AR-1242-2

R.T.: 4.752 min
Delta R.T.: -0.003 min
Response: 158396
Conc: 0.68 ng/ml

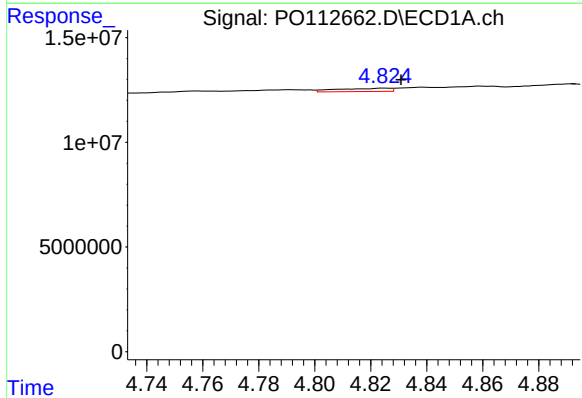


#18 AR-1242-3

R.T.: 4.825 min
Delta R.T.: -0.006 min
Response: 1997111
Conc: 8.44 ng/ml

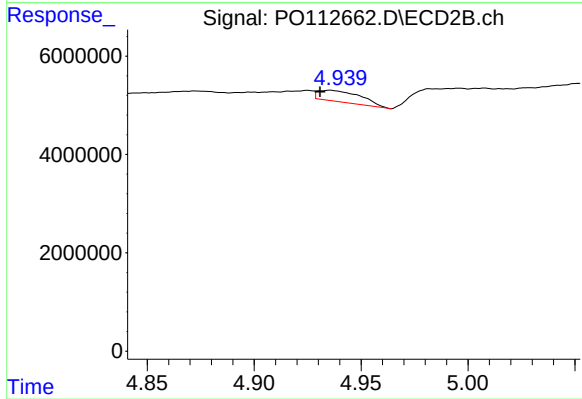

#18 AR-1242-3


R.T.: 4.936 min
Delta R.T.: 0.005 min
Response: 3192959
Conc: 26.35 ng/ml

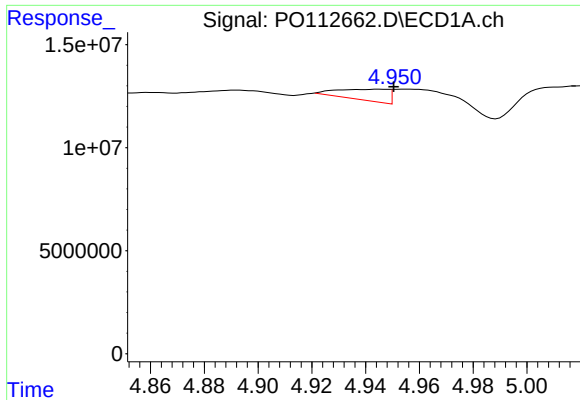

#19 AR-1242-4


R.T.: 4.945 min
Delta R.T.: -0.005 min
Response: 7070888
Conc: 36.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

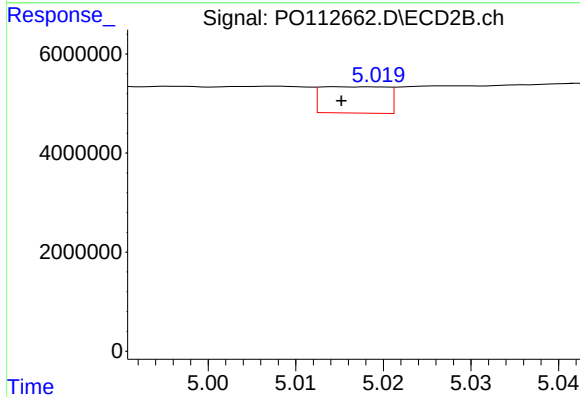


#19 AR-1242-4

R.T.: 5.015 min
Delta R.T.: 0.000 min
Response: 2779533
Conc: 22.65 ng/ml

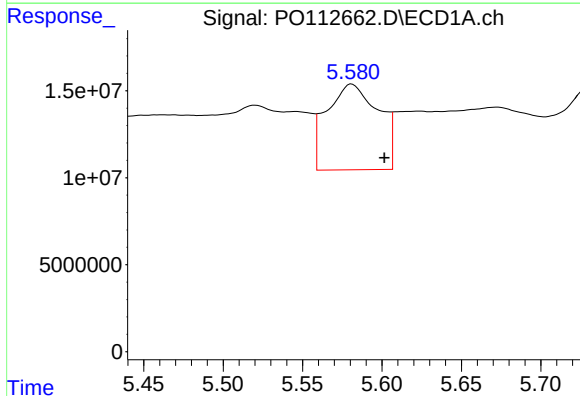


#20 AR-1242-5

R.T.: 5.581 min
Delta R.T.: -0.021 min
Response: 111973853
Conc: 523.45 ng/ml

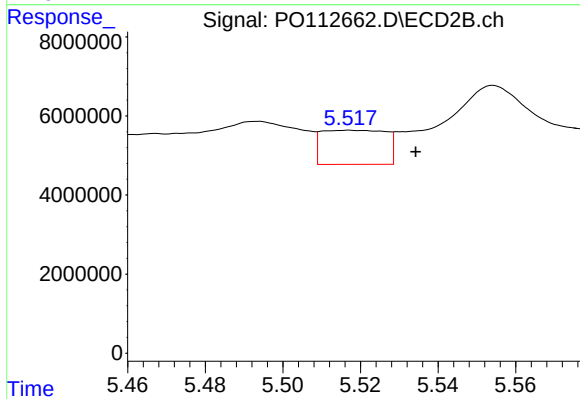

#20 AR-1242-5


R.T.: 5.517 min
Delta R.T.: -0.017 min
Response: 9980768
Conc: 62.00 ng/ml

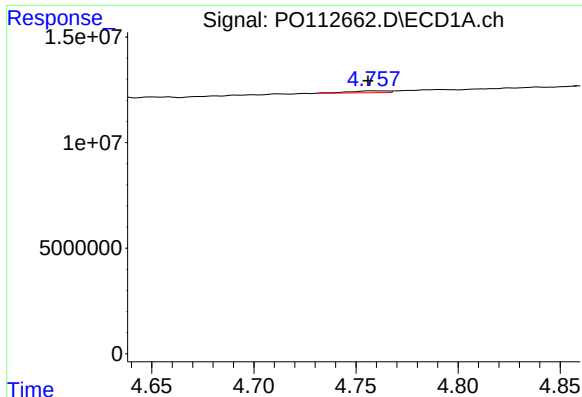

#21 AR-1248-1


R.T.: 4.758 min
Delta R.T.: 0.002 min
Response: 1182326
Conc: 6.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

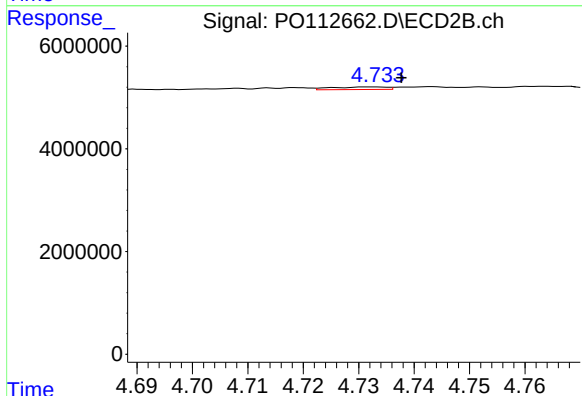


#21 AR-1248-1

R.T.: 4.733 min
Delta R.T.: -0.005 min
Response: 358042
Conc: 2.95 ng/ml

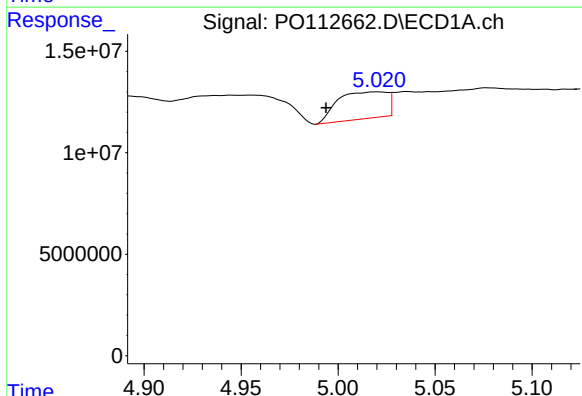


#22 AR-1248-2

R.T.: 5.021 min
Delta R.T.: 0.027 min
Response: 23396783
Conc: 91.71 ng/ml

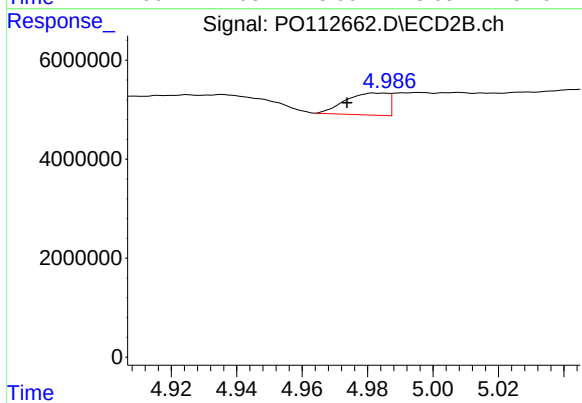

#22 AR-1248-2


R.T.: 4.982 min
Delta R.T.: 0.008 min
Response: 4045754
Conc: 23.90 ng/ml

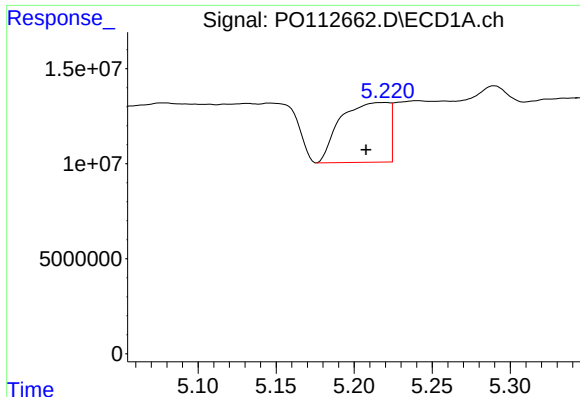

#23 AR-1248-3


R.T.: 5.220 min
Delta R.T.: 0.012 min
Response: 67211667
Conc: 195.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

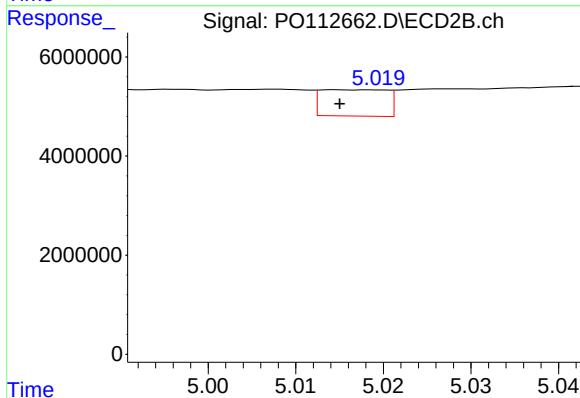


#23 AR-1248-3

R.T.: 5.015 min
Delta R.T.: 0.000 min
Response: 2779533
Conc: 15.65 ng/ml

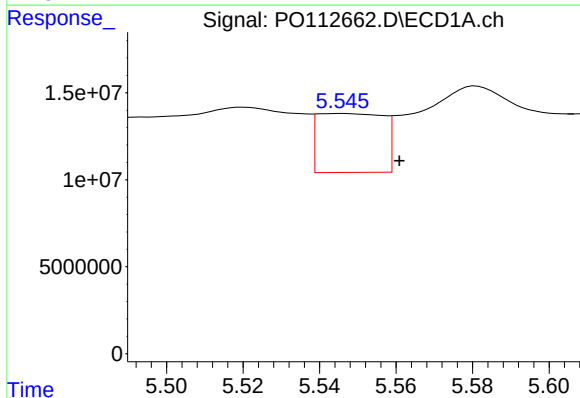


#24 AR-1248-4

R.T.: 5.546 min
Delta R.T.: -0.015 min
Response: 40382019
Conc: 79.48 ng/ml

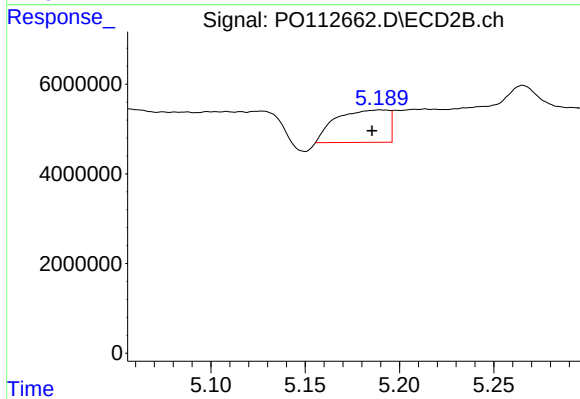

#24 AR-1248-4


R.T.: 5.190 min
Delta R.T.: 0.004 min
Response: 13950460
Conc: 66.96 ng/ml

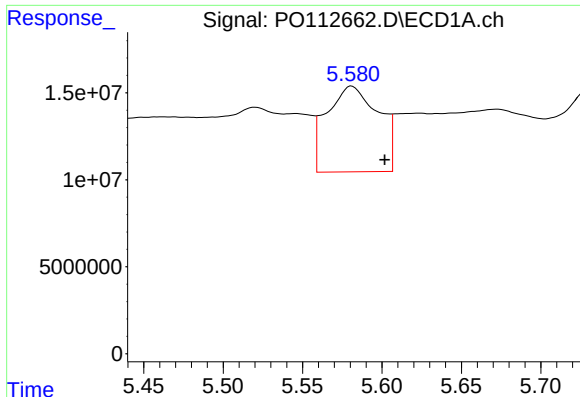

#25 AR-1248-5


R.T.: 5.581 min
Delta R.T.: -0.021 min
Response: 111973853
Conc: 320.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

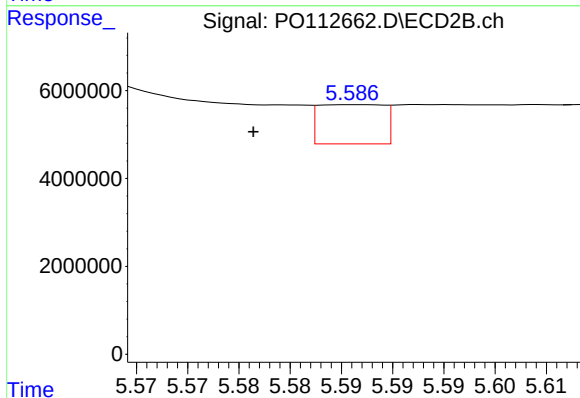


#25 AR-1248-5

R.T.: 5.587 min
Delta R.T.: 0.010 min
Response: 3947174
Conc: 18.38 ng/ml

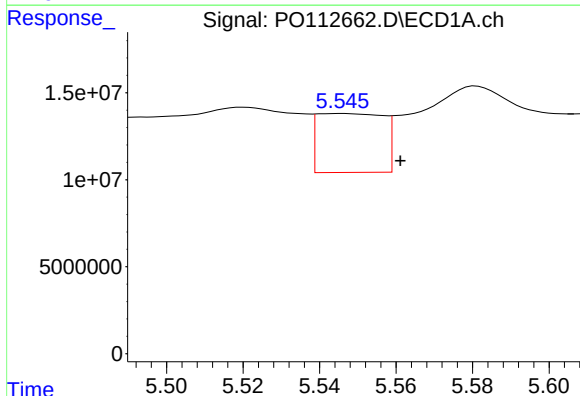


#26 AR-1254-1

R.T.: 5.546 min
Delta R.T.: -0.015 min
Response: 40382019
Conc: 73.56 ng/ml

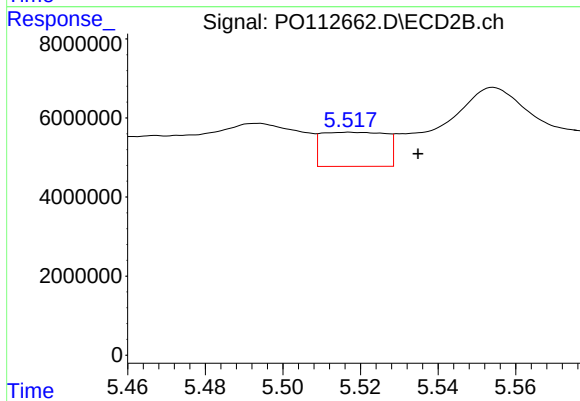

#26 AR-1254-1


R.T.: 5.517 min
Delta R.T.: -0.018 min
Response: 9980768
Conc: 30.37 ng/ml

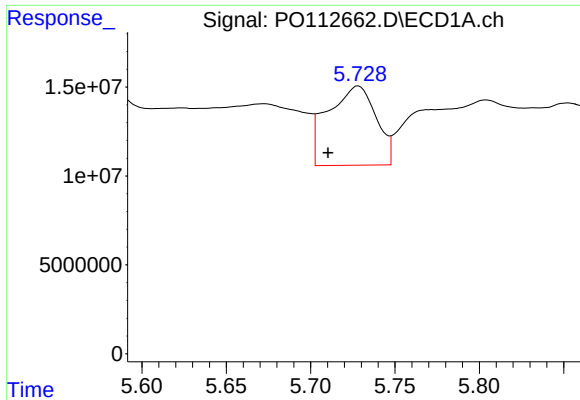

#27 AR-1254-2


R.T.: 5.728 min
Delta R.T.: 0.018 min
Response: 88798000
Conc: 182.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

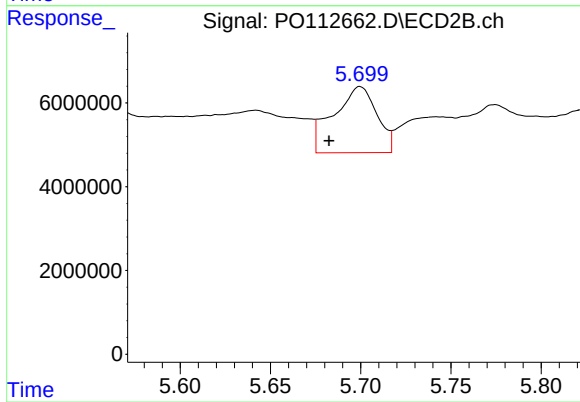


#27 AR-1254-2

R.T.: 5.700 min
Delta R.T.: 0.017 min
Response: 26449525
Conc: 91.37 ng/ml

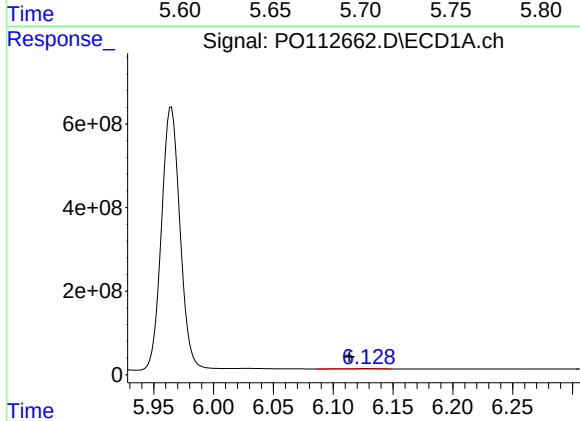


#28 AR-1254-3

R.T.: 6.128 min
Delta R.T.: 0.015 min
Response: 13811100
Conc: 18.56 ng/ml

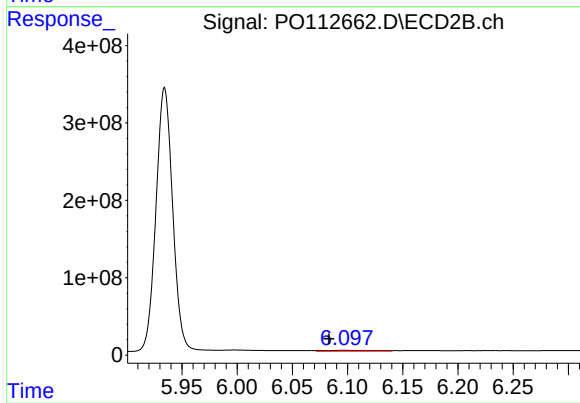

#28 AR-1254-3


R.T.: 6.097 min
Delta R.T.: 0.014 min
Response: 32687070
Conc: 76.47 ng/ml

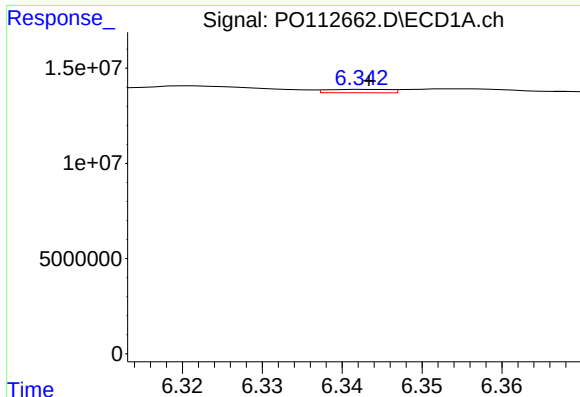

#29 AR-1254-4


R.T.: 6.343 min
Delta R.T.: 0.000 min
Response: 973975
Conc: 1.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

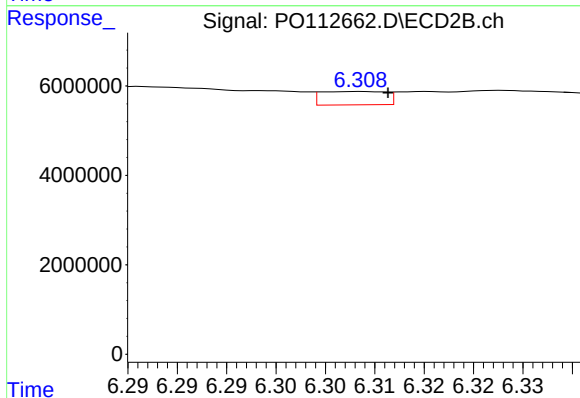


#29 AR-1254-4

R.T.: 6.309 min
Delta R.T.: -0.003 min
Response: 1369461
Conc: 5.02 ng/ml

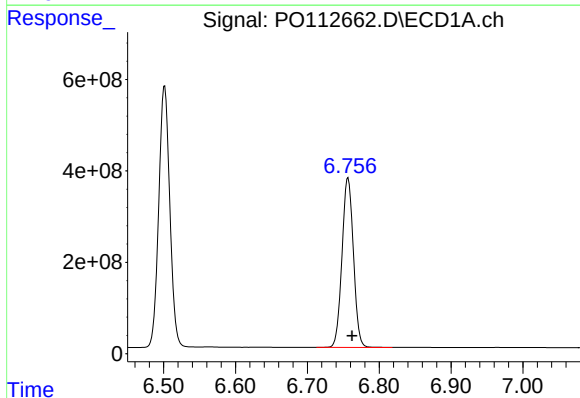


#30 AR-1254-5

R.T.: 6.757 min
Delta R.T.: -0.006 min
Response: 4100301801
Conc: 5792.82 ng/ml

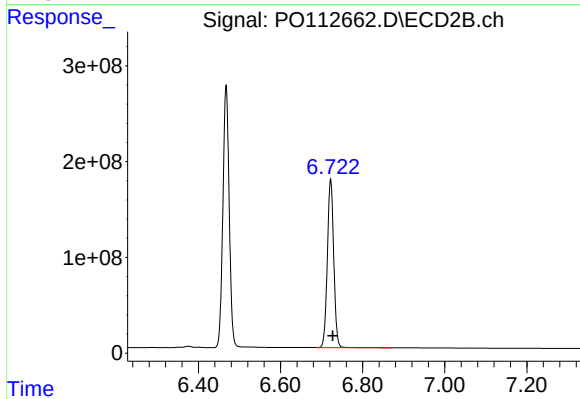

#30 AR-1254-5


R.T.: 6.722 min
Delta R.T.: -0.005 min
Response: 1893138773
Conc: 5667.75 ng/ml

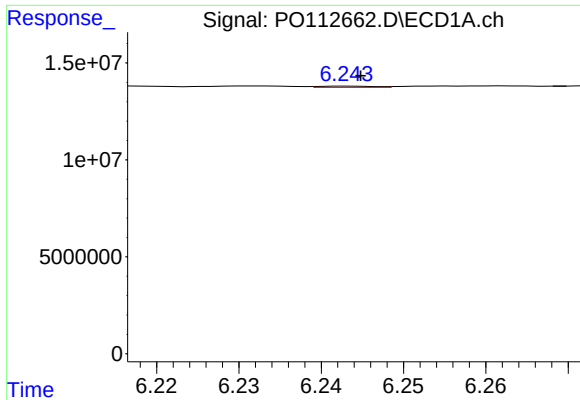

#31 AR-1260-1


R.T.: 6.243 min
Delta R.T.: -0.001 min
Response: 304408
Conc: 0.69 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

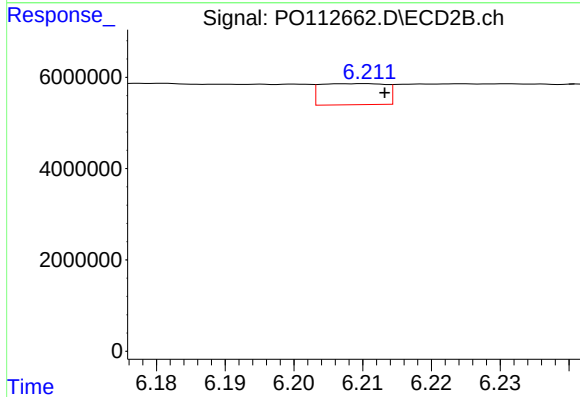


#31 AR-1260-1

R.T.: 6.211 min
Delta R.T.: -0.003 min
Response: 3052326
Conc: 12.28 ng/ml

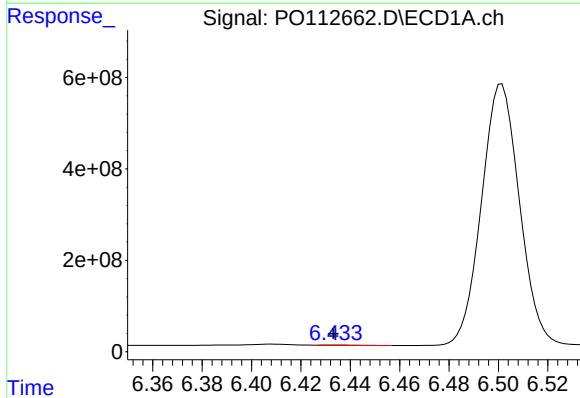


#32 AR-1260-2

R.T.: 6.434 min
Delta R.T.: 0.000 min
Response: 10189274
Conc: 14.81 ng/ml

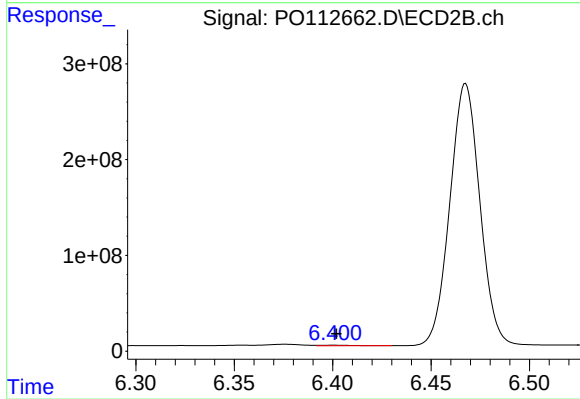

#32 AR-1260-2


R.T.: 6.400 min
Delta R.T.: -0.002 min
Response: 5766025
Conc: 17.50 ng/ml

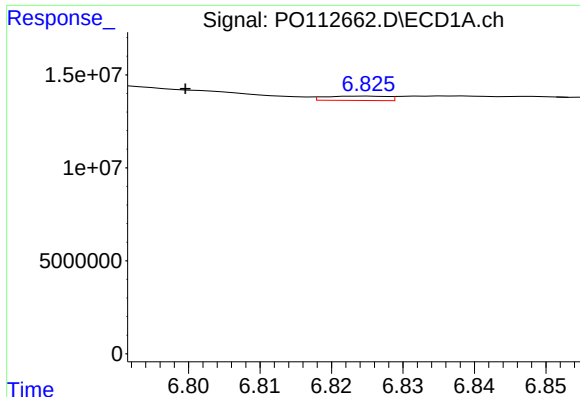

#33 AR-1260-3


R.T.: 6.825 min
Delta R.T.: 0.025 min
Response: 1421961
Conc: 2.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

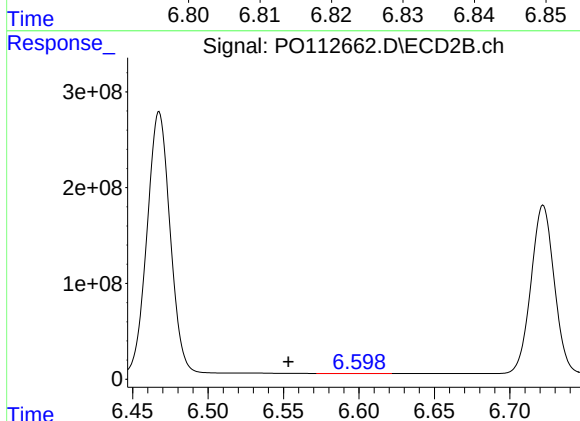


#33 AR-1260-3

R.T.: 6.596 min
Delta R.T.: 0.042 min
Response: 539588
Conc: 2.10 ng/ml

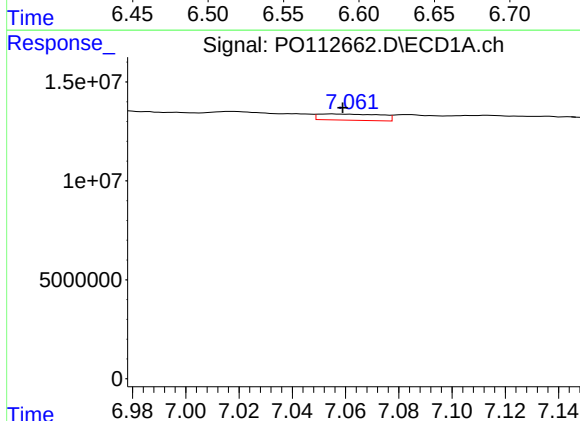


#34 AR-1260-4

R.T.: 7.055 min
Delta R.T.: -0.004 min
Response: 5102607
Conc: 11.31 ng/ml

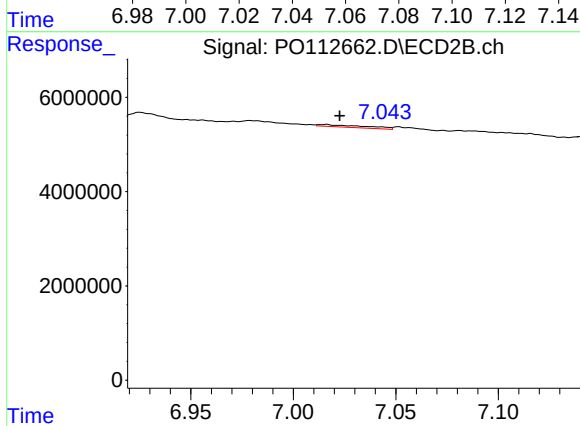

#34 AR-1260-4


R.T.: 7.016 min
Delta R.T.: -0.007 min
Response: 760819
Conc: 3.98 ng/ml

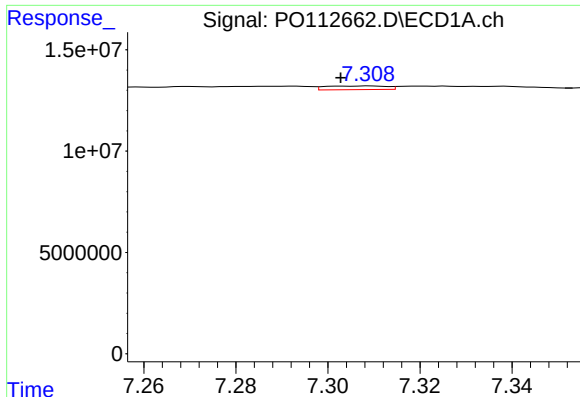

#35 AR-1260-5


R.T.: 7.309 min
Delta R.T.: 0.006 min
Response: 1673590
Conc: 1.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

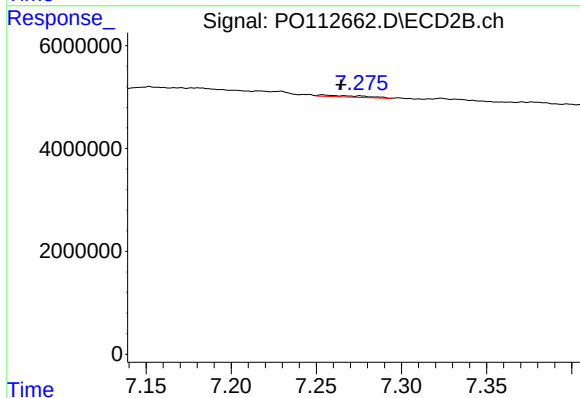


#35 AR-1260-5

R.T.: 7.254 min
Delta R.T.: -0.011 min
Response: 525500
Conc: 1.27 ng/ml

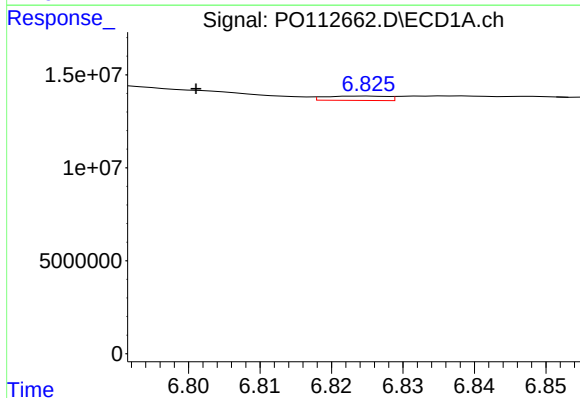


#36 AR-1262-1

R.T.: 6.825 min
Delta R.T.: 0.024 min
Response: 1421961
Conc: 1.53 ng/ml

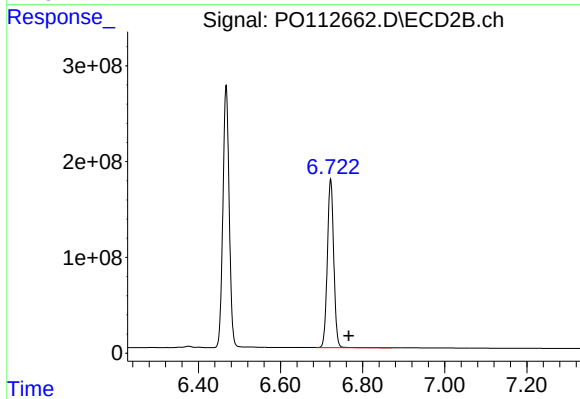

#36 AR-1262-1


R.T.: 6.722 min
Delta R.T.: -0.044 min
Response: 1893138773
Conc: 4563.67 ng/ml

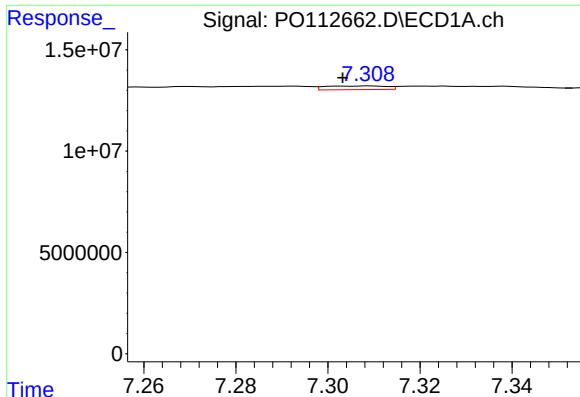

#37 AR-1262-2


R.T.: 7.309 min
Delta R.T.: 0.006 min
Response: 1673590
Conc: 1.13 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

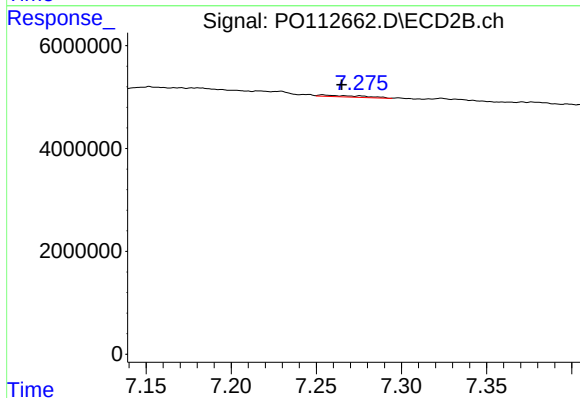


#37 AR-1262-2

R.T.: 7.254 min
Delta R.T.: -0.011 min
Response: 525500
Conc: 1.02 ng/ml

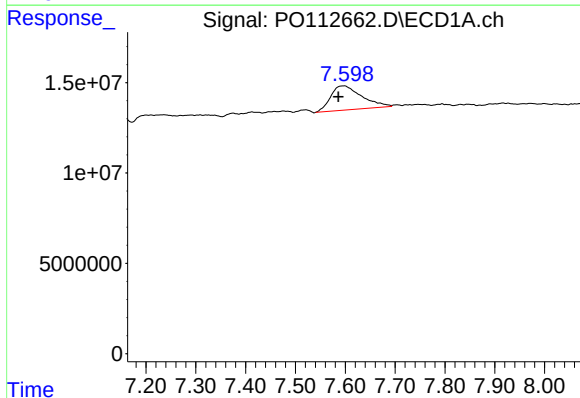


#38 AR-1262-3

R.T.: 7.598 min
Delta R.T.: 0.012 min
Response: 58092347
Conc: 98.42 ng/ml

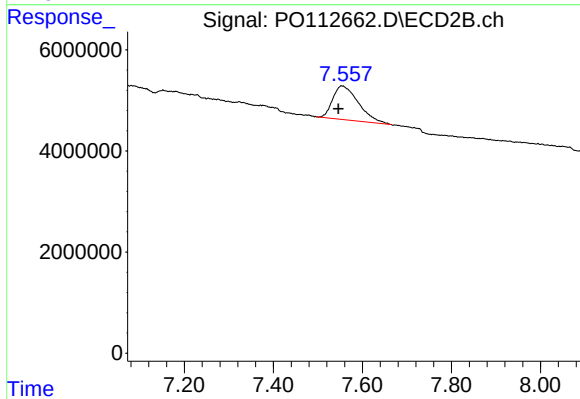

#38 AR-1262-3


R.T.: 7.553 min
Delta R.T.: 0.007 min
Response: 26586960
Conc: 142.54 ng/ml

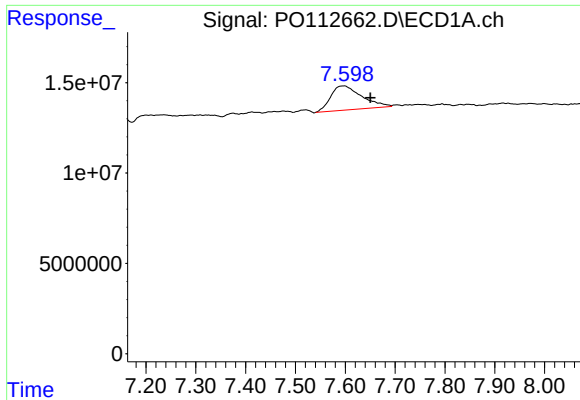

#39 AR-1262-4


R.T.: 7.598 min
Delta R.T.: -0.052 min
Response: 58092347
Conc: 58.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

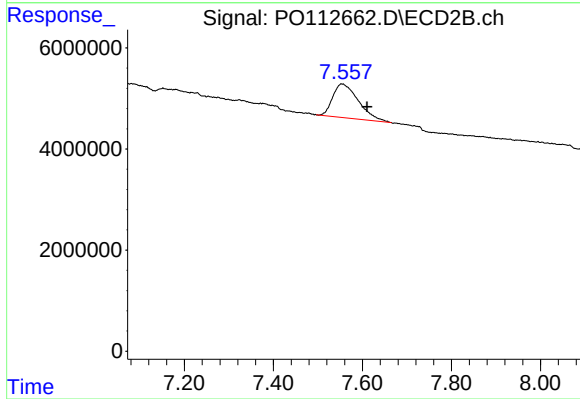


#39 AR-1262-4

R.T.: 7.553 min
Delta R.T.: -0.058 min
Response: 26586960
Conc: 92.28 ng/ml

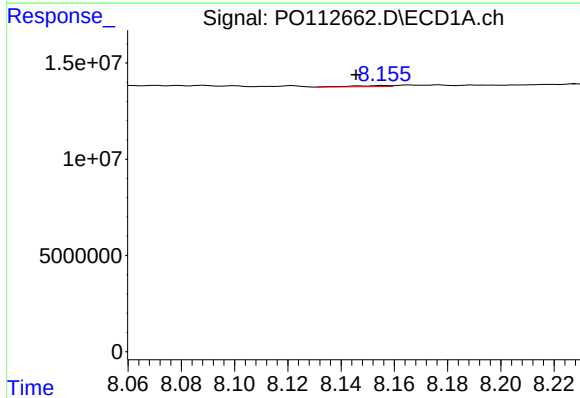


#40 AR-1262-5

R.T.: 8.156 min
Delta R.T.: 0.011 min
Response: 545727
Conc: 1.26 ng/ml

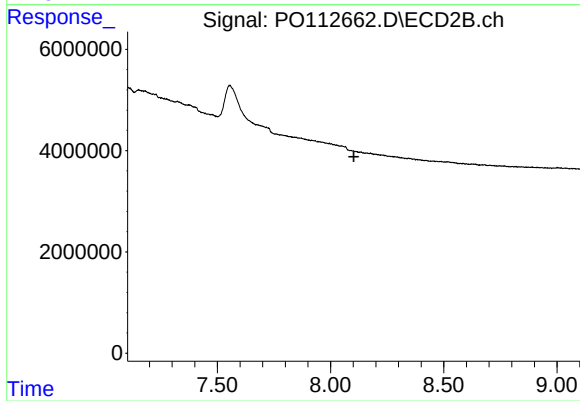

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T. : 8.103 min
Response: 0
Conc: N.D.

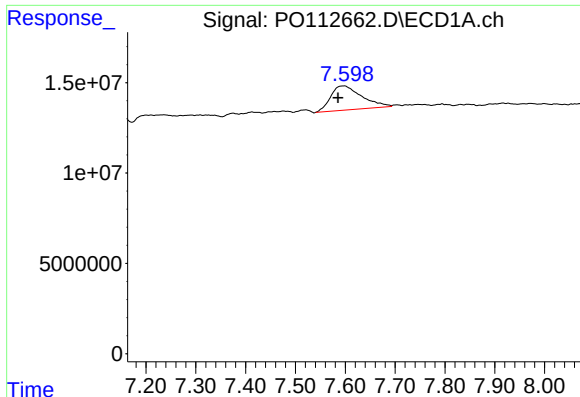

#41 AR-1268-1


R.T.: 7.598 min
Delta R.T.: 0.013 min
Response: 58092347
Conc: 33.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

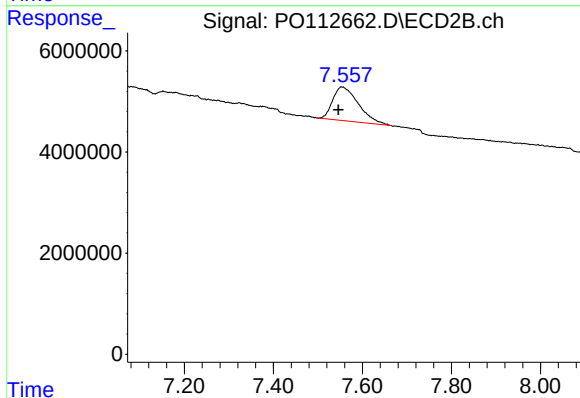


#41 AR-1268-1

R.T.: 7.553 min
Delta R.T.: 0.007 min
Response: 26586960
Conc: 51.34 ng/ml

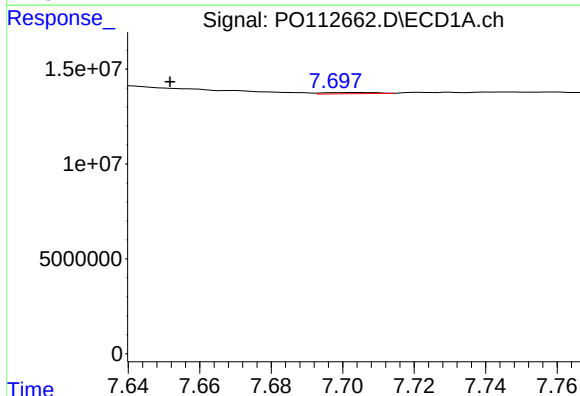


#42 AR-1268-2

R.T.: 7.704 min
Delta R.T.: 0.052 min
Response: 661689
Conc: 0.45 ng/ml

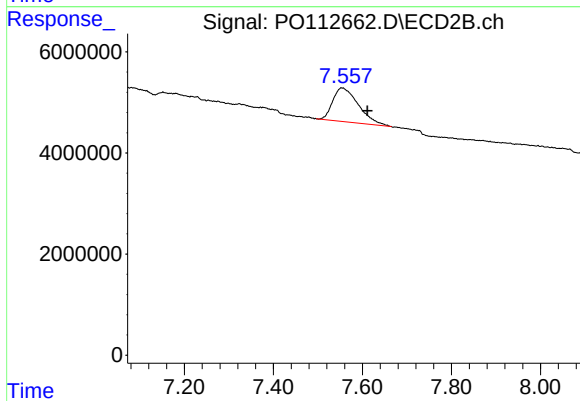

#42 AR-1268-2


R.T.: 7.553 min
Delta R.T.: -0.059 min
Response: 26586960
Conc: 62.55 ng/ml

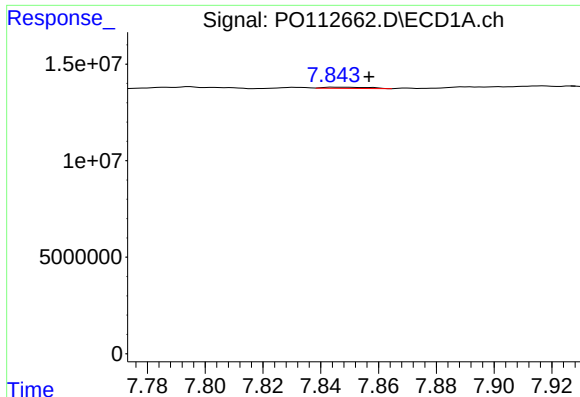

#43 AR-1268-3


R.T.: 7.845 min
Delta R.T.: -0.012 min
Response: 703916
Conc: 0.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

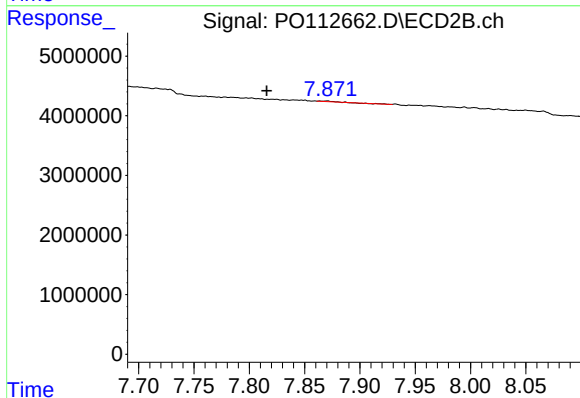


#43 AR-1268-3

R.T.: 7.870 min
Delta R.T.: 0.055 min
Response: 89877
Conc: 0.28 ng/ml

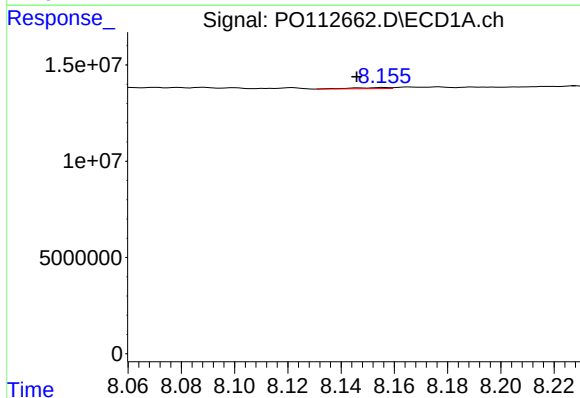


#44 AR-1268-4

R.T.: 8.156 min
Delta R.T.: 0.010 min
Response: 545727
Conc: 1.13 ng/ml

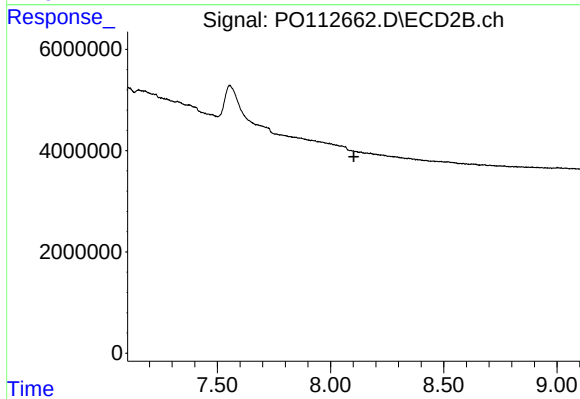

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T.: 8.103 min
Response: 0
Conc: N.D.

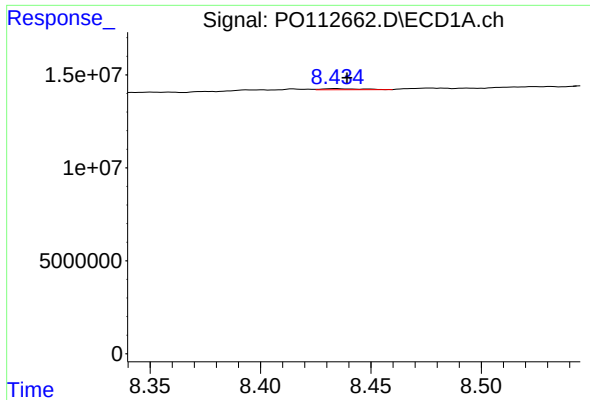

#45 AR-1268-5

R.T.: 8.434 min
Delta R.T.: -0.005 min
Response: 697545
Conc: 0.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

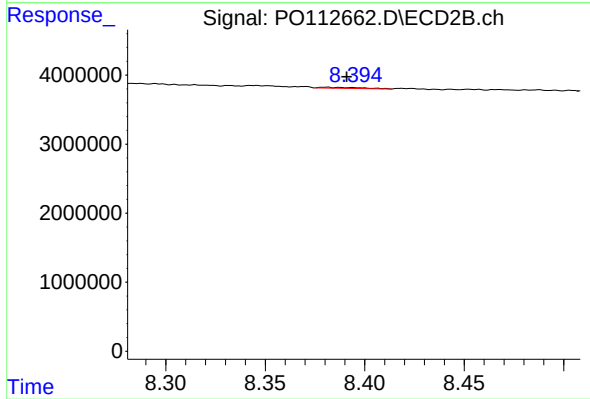

#45 AR-1268-5

R.T.: 8.380 min
Delta R.T.: -0.010 min
Response: 198753
Conc: 0.27 ng/ml