

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080219\
 Data File : P0058731.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Aug 2019 9:56
 Operator : SM/AJ
 Sample : K4057-07RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S13-04-CRE

Manual Integrations
 APPROVED

Ankita
 8/2/2019 2:03:46 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 14:01:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jul 27 06:49:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.167	3.517	612474	541612	14.513m	13.557
2) SA Decachlor...	9.697	8.402	442646	369111	8.174m	9.351m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080219\
Data File : PO058731.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Aug 2019 9:56
Operator : SM/AJ
Sample : K4057-07RE
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
S13-04-CRE


Manual Integrations
APPROVED

Ankita
8/2/2019 2:03:46 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 14:01:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072819.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 27 06:49:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

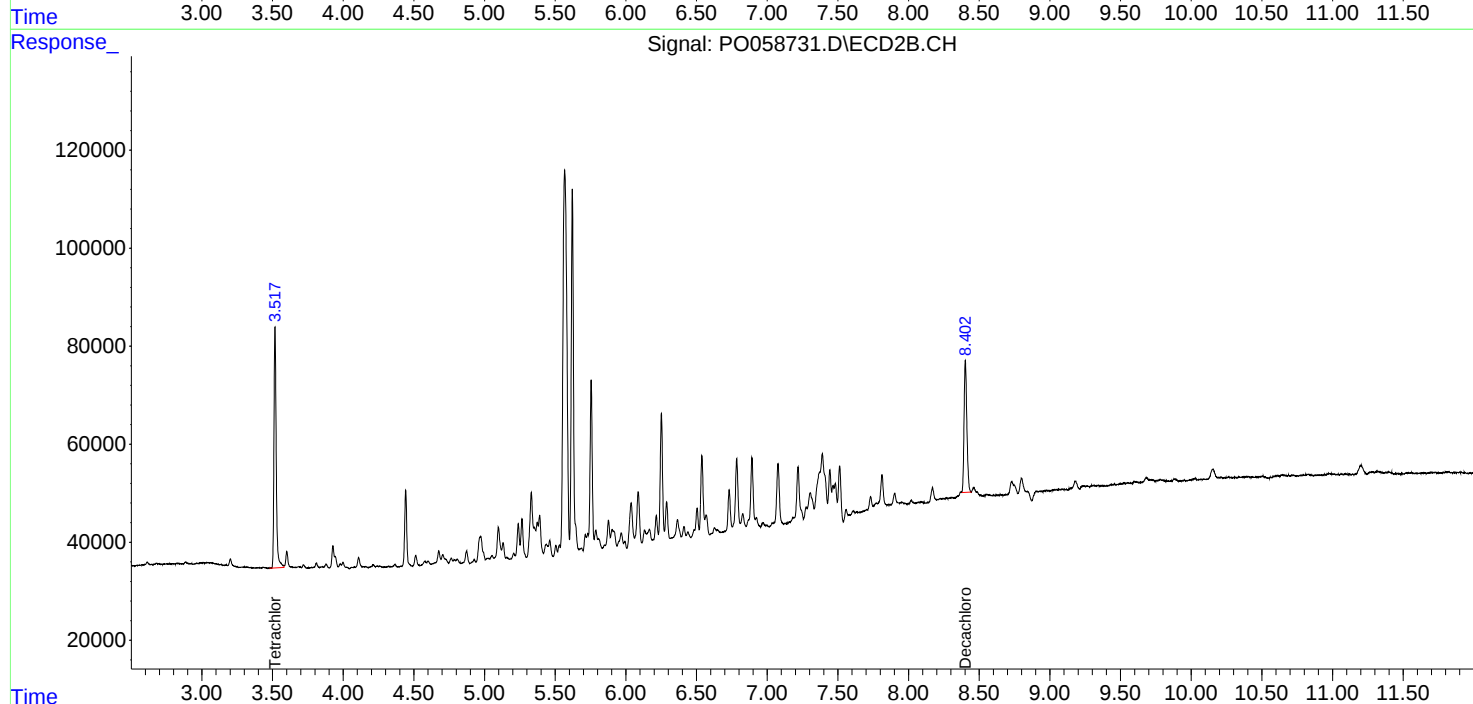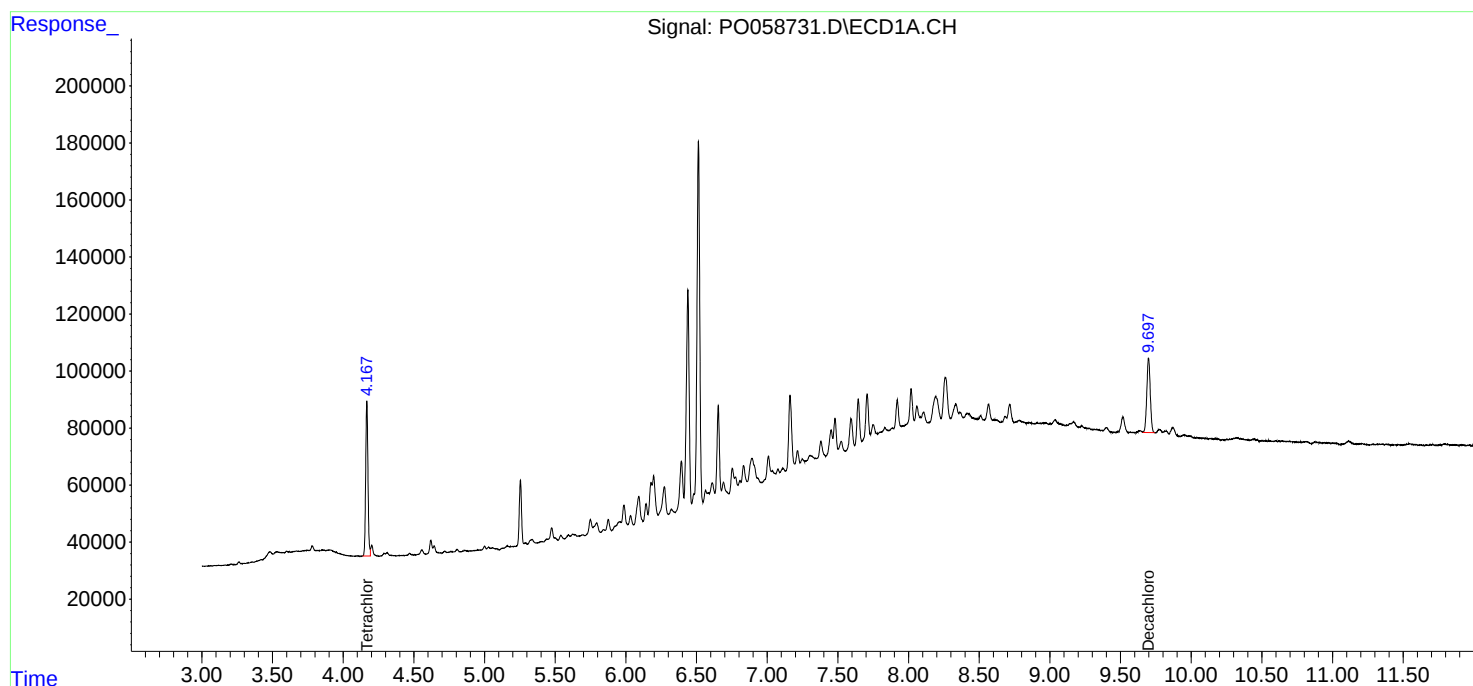

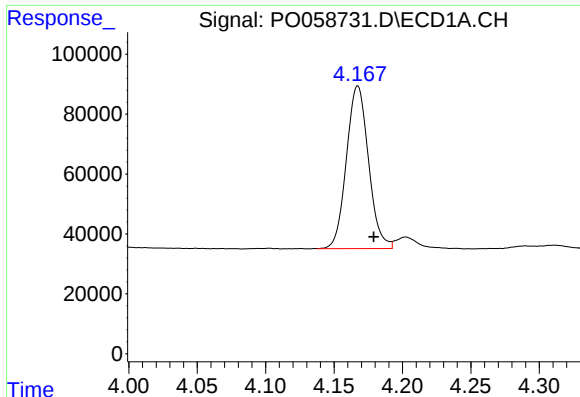


#1 Tetrachloro-m-xylene

R.T.: 4.167 min
Delta R.T.: -0.012 min
Response: 612474
Conc: 14.51 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S13-04-CRE


Manual Integrations
APPROVED

Ankita
8/2/2019 2:03:46 PM

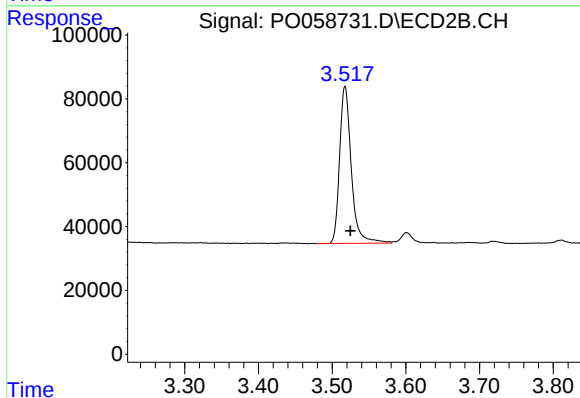


#1 Tetrachloro-m-xylene

R.T.: 3.517 min
Delta R.T.: -0.007 min
Response: 541612
Conc: 13.56 ng/ml

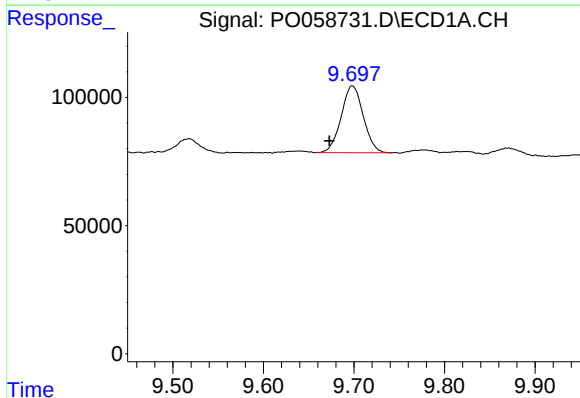

#2 Decachlorobiphenyl

R.T.: 9.697 min
Delta R.T.: 0.025 min
Response: 442646
Conc: 8.17 ng/ml m

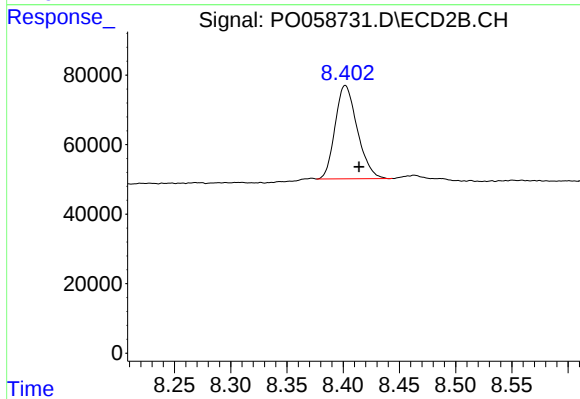

#2 Decachlorobiphenyl

R.T.: 8.402 min
Delta R.T.: -0.013 min
Response: 369111
Conc: 9.35 ng/ml m