

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080219\
 Data File : P0058733.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Aug 2019 10:31
 Operator : SM/AJ
 Sample : K4053-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S12-01-A

Manual Integrations
 APPROVED

Ankita
 8/2/2019 2:03:50 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 14:02:26 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jul 27 06:49:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.166	3.518	919683	772596	21.792m	19.339
2) SA Decachlor...	9.642	8.405	819681	692163	15.136m	17.535
Target Compounds						
26) L6 AR-1254-1	6.166	5.360	182941	90446	77.475m	34.914m#
27) L6 AR-1254-2	6.378	5.505	282674	64470	73.347	28.160 #
28) L6 AR-1254-3	6.736	5.900	218866	109108	54.046m	29.654m#
29) L6 AR-1254-4	7.018	6.129	105537	64211	29.311m	27.615m
30) L6 AR-1254-5	7.458	6.537	499602	454351	137.830m	131.713

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080219\
Data File : PO058733.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Aug 2019 10:31
Operator : SM/AJ
Sample : K4053-01
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
S12-01-A


Manual Integrations
APPROVED

Ankita
8/2/2019 2:03:50 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 14:02:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072819.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 27 06:49:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

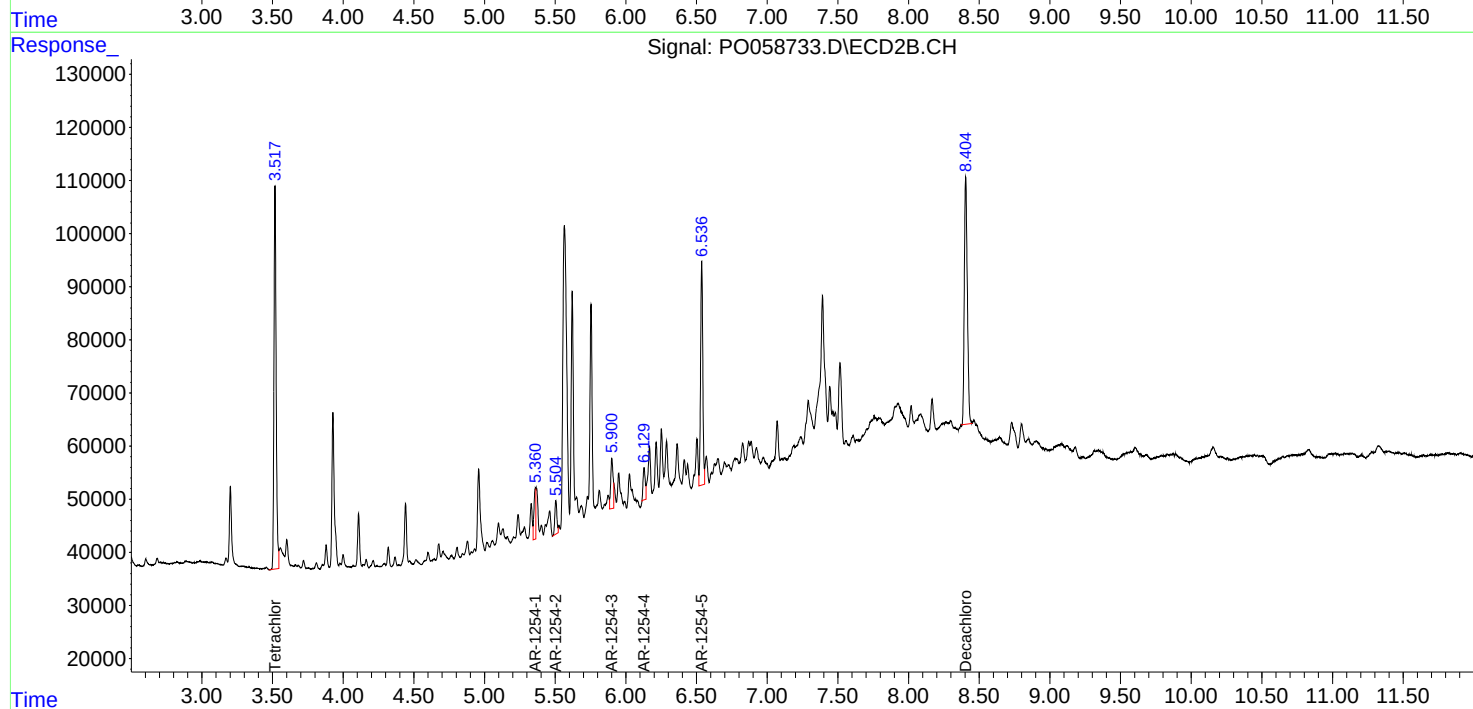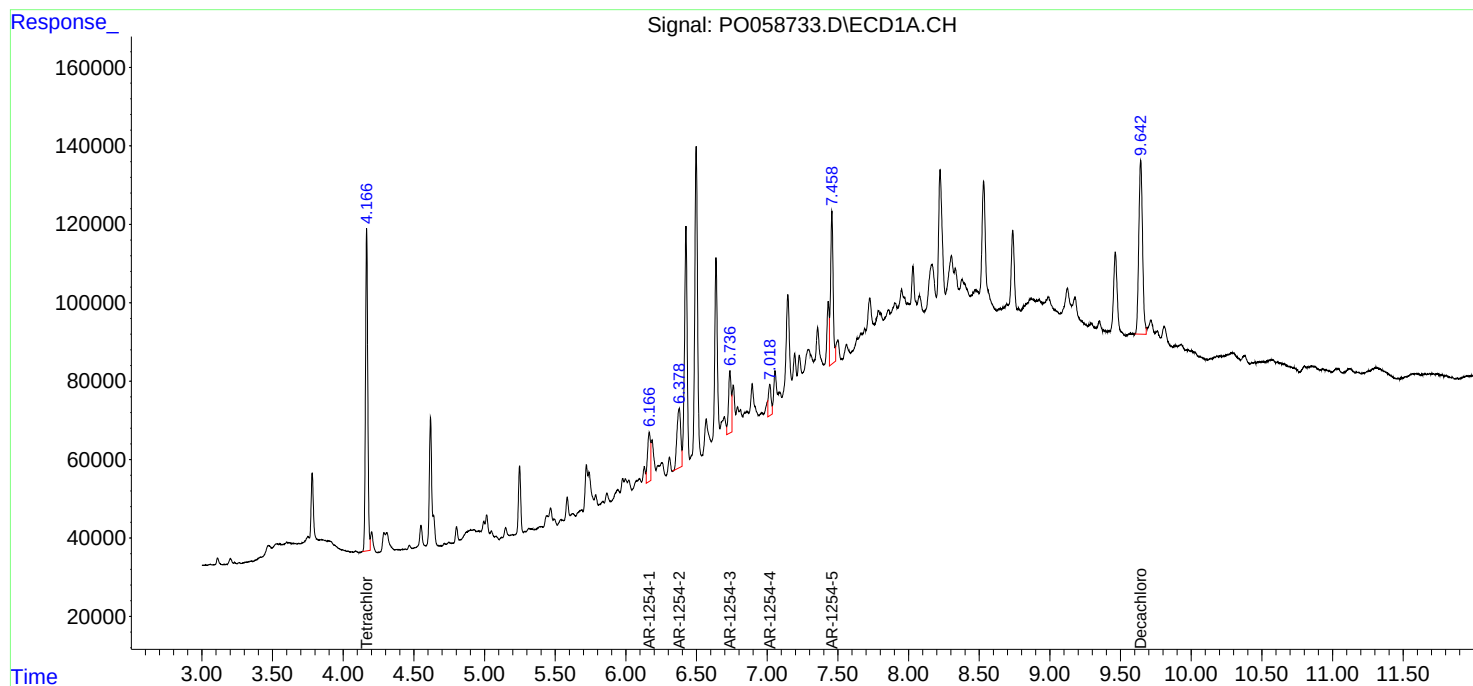

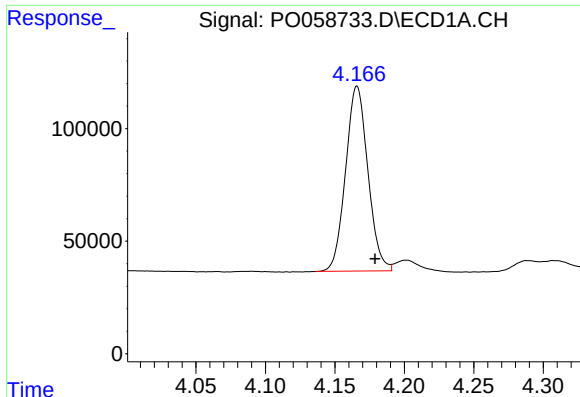


#1 Tetrachloro-m-xylene

R.T.: 4.166 min
Delta R.T.: -0.013 min
Response: 919683
Conc: 21.79 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S12-01-A


Manual Integrations
APPROVED

Ankita
8/2/2019 2:03:50 PM

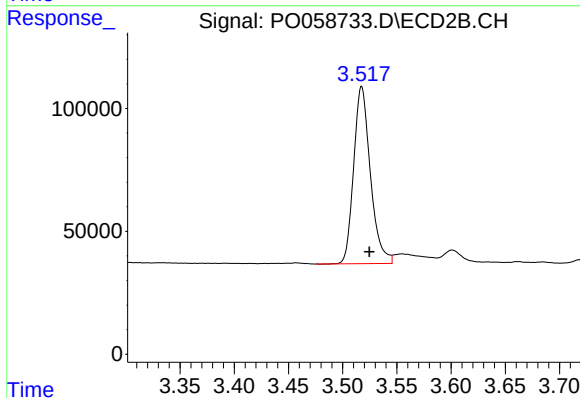


#1 Tetrachloro-m-xylene

R.T.: 3.518 min
Delta R.T.: -0.007 min
Response: 772596
Conc: 19.34 ng/ml

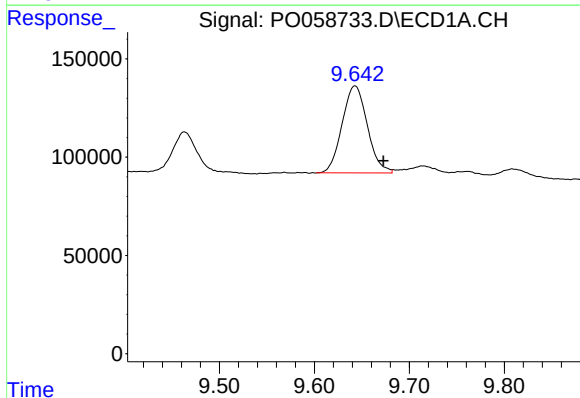


#2 Decachlorobiphenyl

R.T.: 9.642 min
Delta R.T.: -0.030 min
Response: 819681
Conc: 15.14 ng/ml m

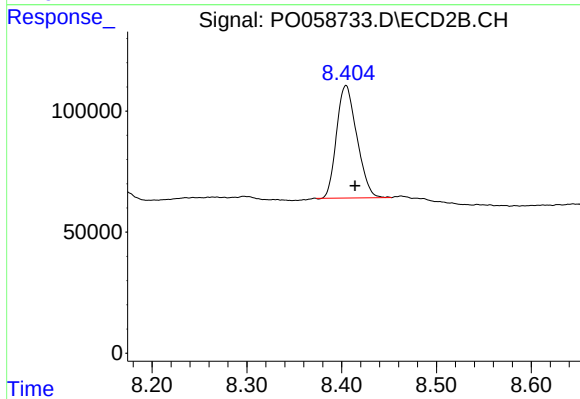

#2 Decachlorobiphenyl

R.T.: 8.405 min
Delta R.T.: -0.010 min
Response: 692163
Conc: 17.54 ng/ml

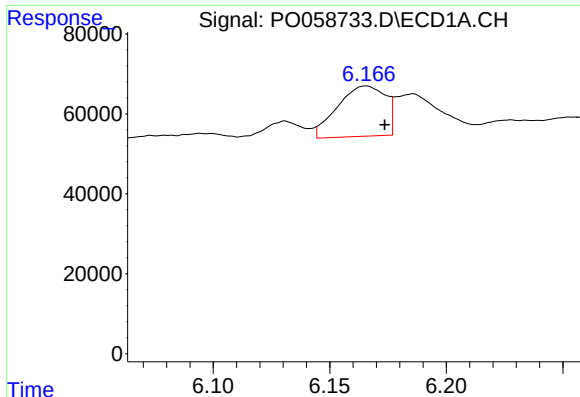


#26 AR-1254-1

R.T.: 6.166 min
Delta R.T.: -0.008 min
Response: 182941
Conc: 77.48 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S12-01-A


Manual Integrations
APPROVED

Ankita
8/2/2019 2:03:50 PM

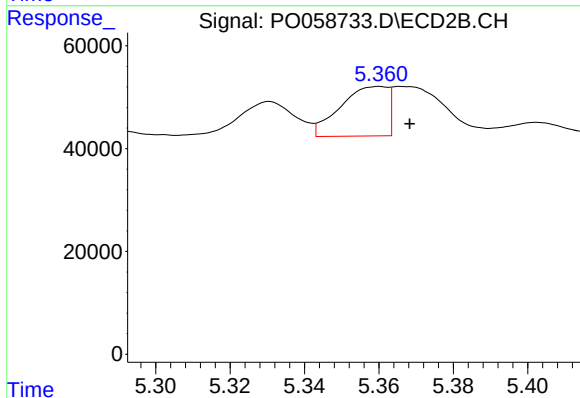


#26 AR-1254-1

R.T.: 5.360 min
Delta R.T.: -0.008 min
Response: 90446
Conc: 34.91 ng/ml m

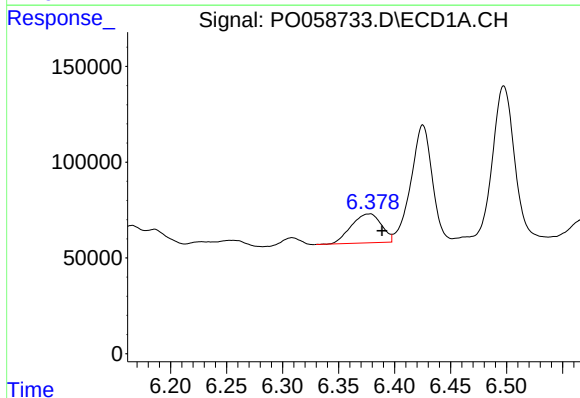


#27 AR-1254-2

R.T.: 6.378 min
Delta R.T.: -0.011 min
Response: 282674
Conc: 73.35 ng/ml

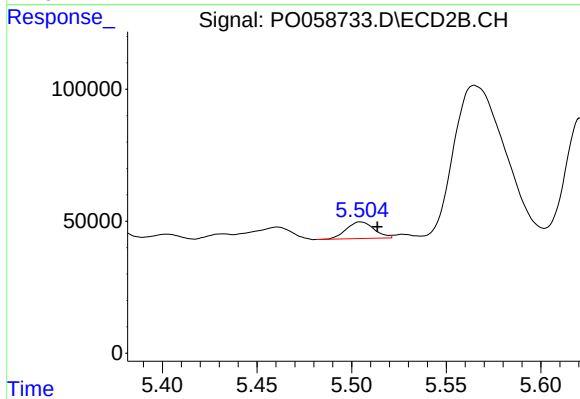

#27 AR-1254-2

R.T.: 5.505 min
Delta R.T.: -0.009 min
Response: 64470
Conc: 28.16 ng/ml

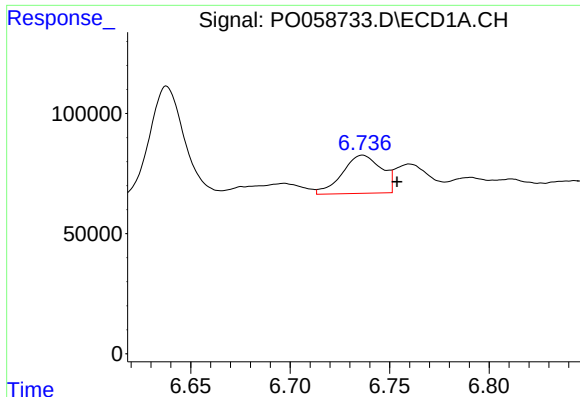


#28 AR-1254-3

R.T.: 6.736 min
Delta R.T.: -0.018 min
Response: 218866
Conc: 54.05 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S12-01-A


Manual Integrations
APPROVED

Ankita
8/2/2019 2:03:50 PM

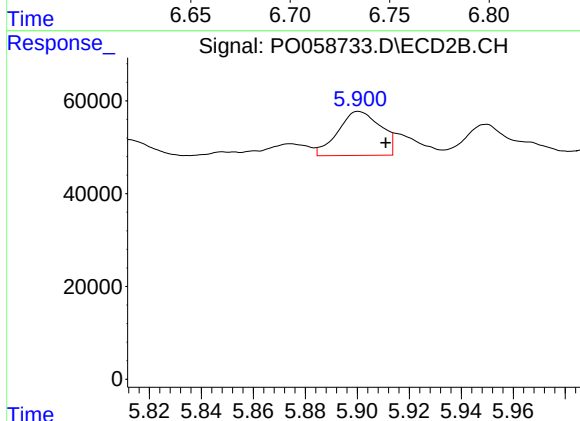


#28 AR-1254-3

R.T.: 5.900 min
Delta R.T.: -0.011 min
Response: 109108
Conc: 29.65 ng/ml m

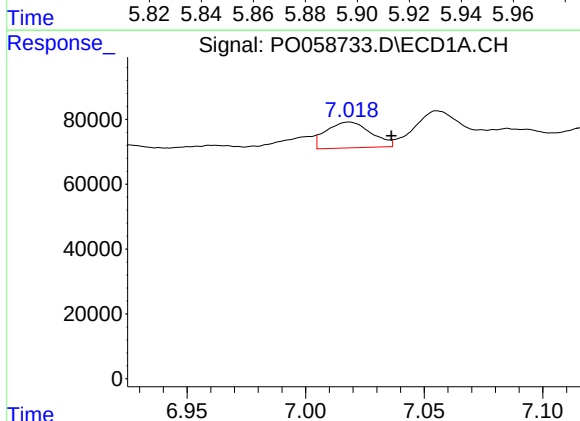


#29 AR-1254-4

R.T.: 7.018 min
Delta R.T.: -0.018 min
Response: 105537
Conc: 29.31 ng/ml m

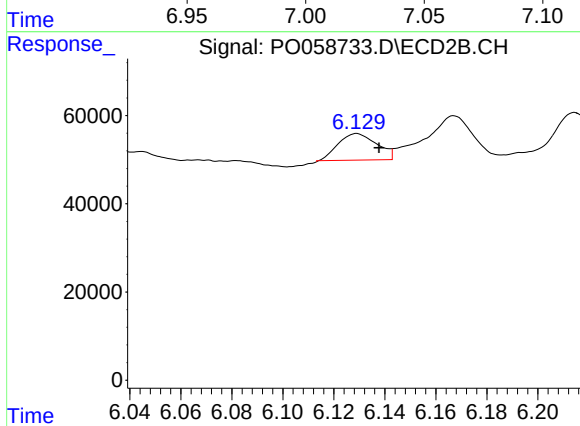

#29 AR-1254-4

R.T.: 6.129 min
Delta R.T.: -0.009 min
Response: 64211
Conc: 27.62 ng/ml m

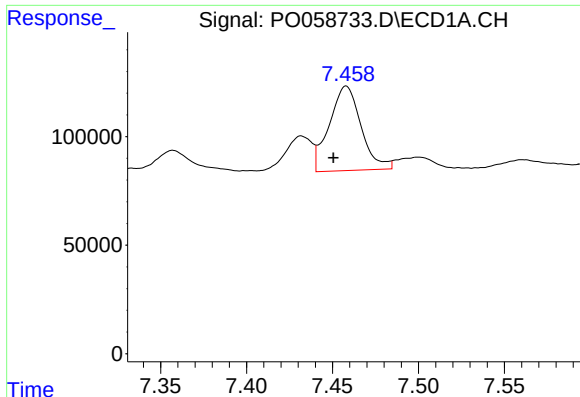


#30 AR-1254-5

R.T.: 7.458 min
Delta R.T.: 0.007 min
Response: 499602
Conc: 137.83 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S12-01-A

Manual Integrations
APPROVED

Ankita
8/2/2019 2:03:50 PM

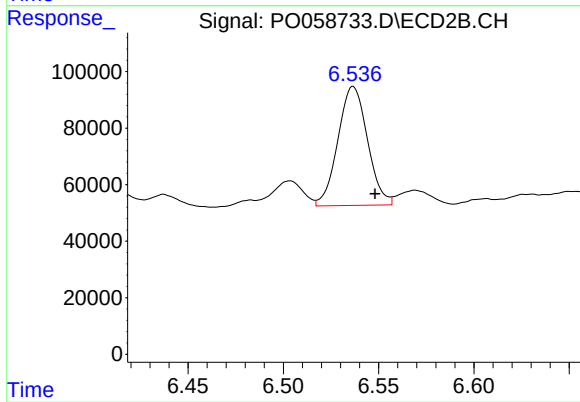

#30 AR-1254-5

R.T.: 6.537 min
Delta R.T.: -0.011 min
Response: 454351
Conc: 131.71 ng/ml