

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080219\
 Data File : P0058770.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Aug 2019 21:34
 Operator : SM/AJ
 Sample : K4049-03RE
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SP-3RE

Manual Integrations
 APPROVED

Ankita
 8/2/2019 2:04:33 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 01:54:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jul 27 06:49:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.164	3.518	708806	647429	16.795	16.206
2) SA Decachlor...	9.640	8.403	579052	414208	10.692	10.493
Target Compounds						
26) L6 AR-1254-1	6.155	5.359	843768	689823	357.334m	266.285 #
27) L6 AR-1254-2	6.371	5.505	1126151	508651	292.207	222.174
28) L6 AR-1254-3	6.734	5.901	1341202	1188708	331.191	323.074
29) L6 AR-1254-4	7.017	6.128	710637	443838	197.364m	190.880
30) L6 AR-1254-5	7.430	6.537	1185286	1330440	326.997m	385.684m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080219\
Data File : PO058770.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Aug 2019 21:34
Operator : SM/AJ
Sample : K4049-03RE
Misc :
ALS Vial : 42 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
SP-3RE


Manual Integrations
APPROVED

Ankita
8/2/2019 2:04:33 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 01:54:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072819.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 27 06:49:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

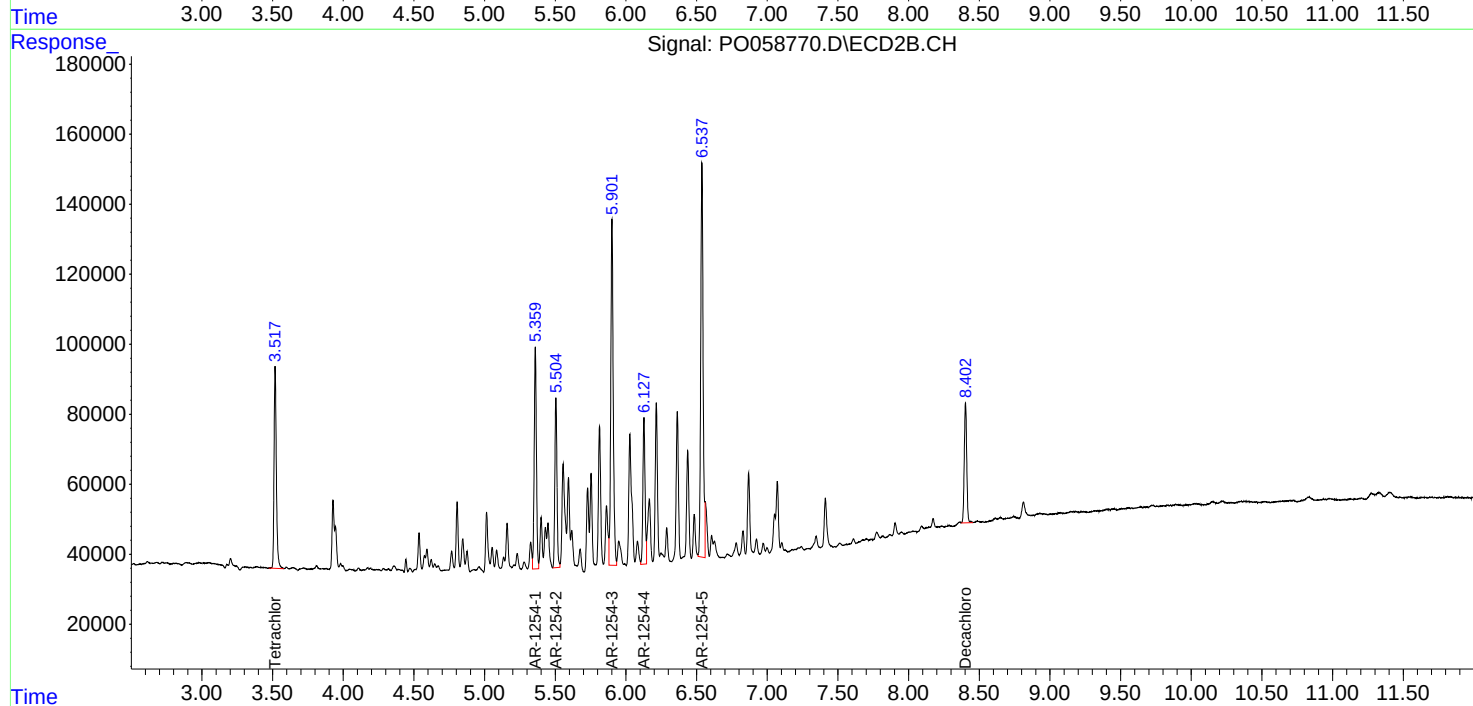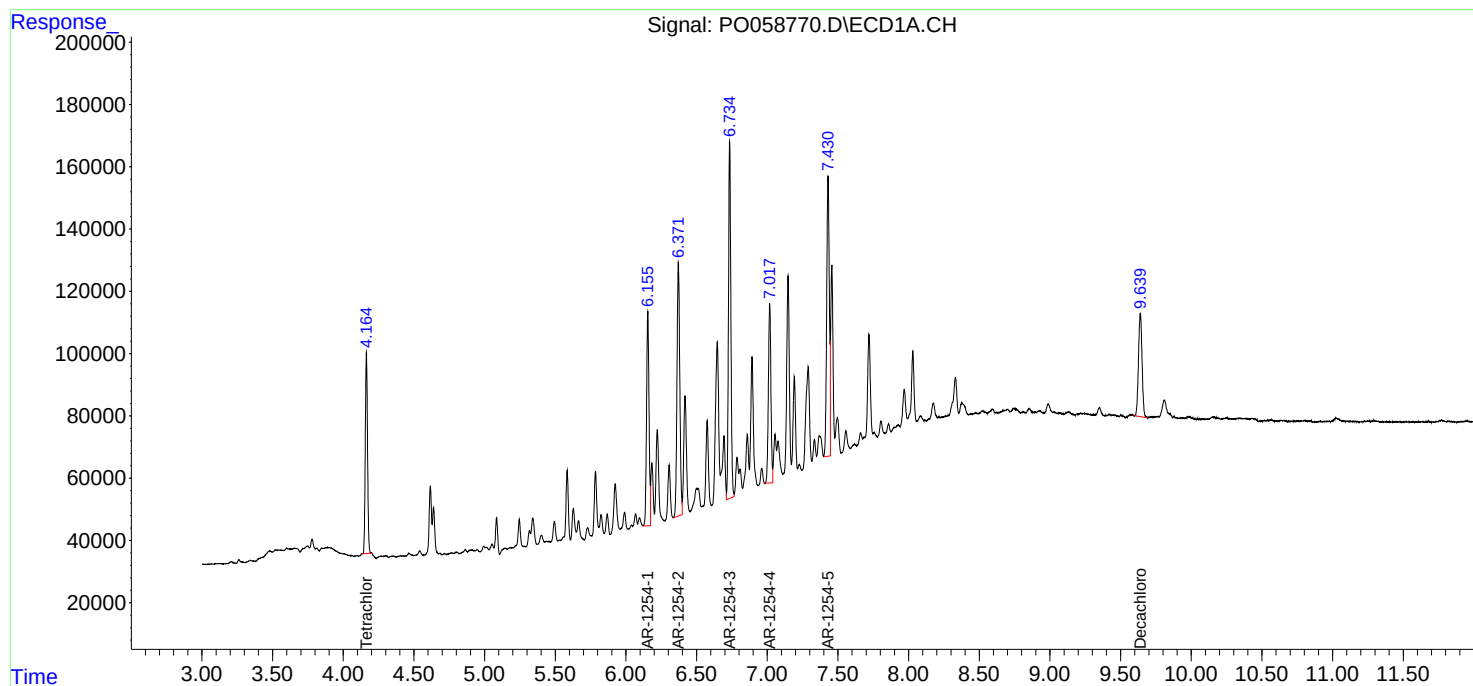

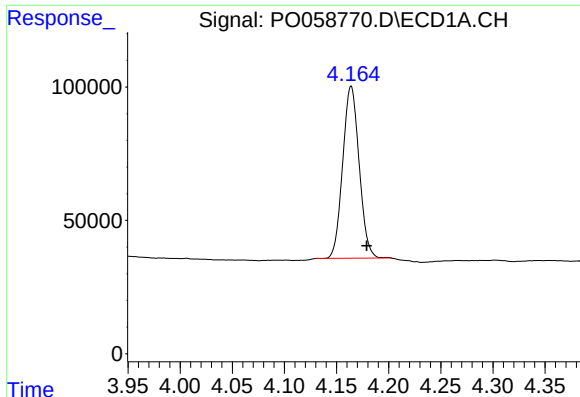


#1 Tetrachloro-m-xylene

R.T.: 4.164 min
Delta R.T.: -0.015 min
Response: 708806
Conc: 16.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
SP-3RE


Manual Integrations
APPROVED

Ankita
8/2/2019 2:04:33 PM

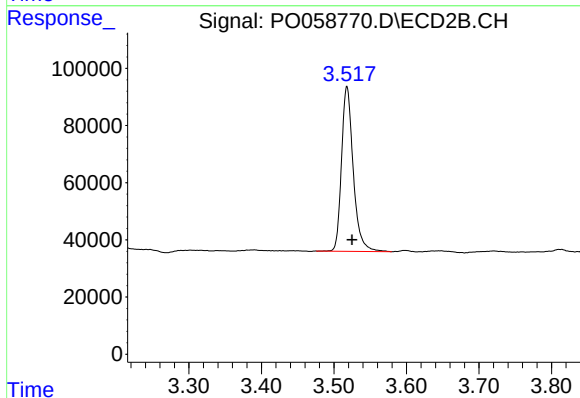


#1 Tetrachloro-m-xylene

R.T.: 3.518 min
Delta R.T.: -0.007 min
Response: 647429
Conc: 16.21 ng/ml

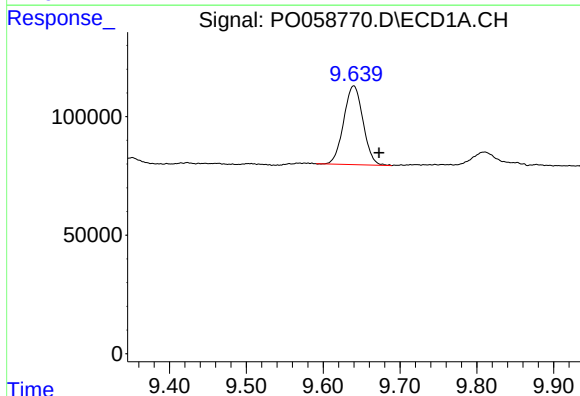


#2 Decachlorobiphenyl

R.T.: 9.640 min
Delta R.T.: -0.033 min
Response: 579052
Conc: 10.69 ng/ml

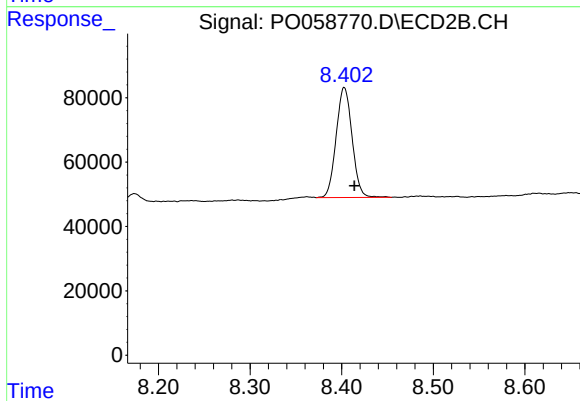

#2 Decachlorobiphenyl

R.T.: 8.403 min
Delta R.T.: -0.011 min
Response: 414208
Conc: 10.49 ng/ml

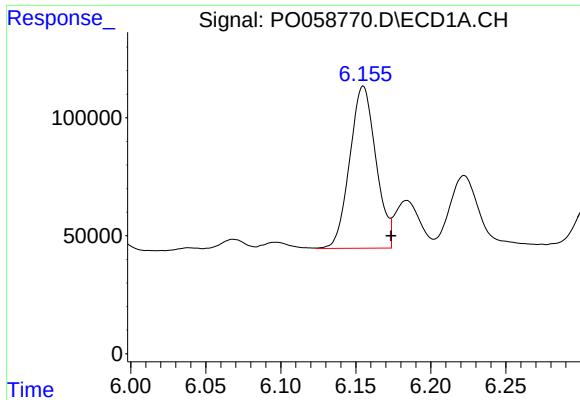


#26 AR-1254-1

R.T.: 6.155 min
Delta R.T.: -0.019 min
Response: 843768
Conc: 357.33 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SP-3RE


Manual Integrations
APPROVED

Ankita
8/2/2019 2:04:33 PM

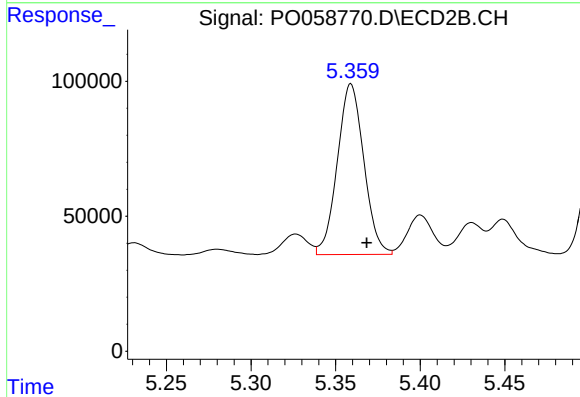


#26 AR-1254-1

R.T.: 5.359 min
Delta R.T.: -0.009 min
Response: 689823
Conc: 266.29 ng/ml

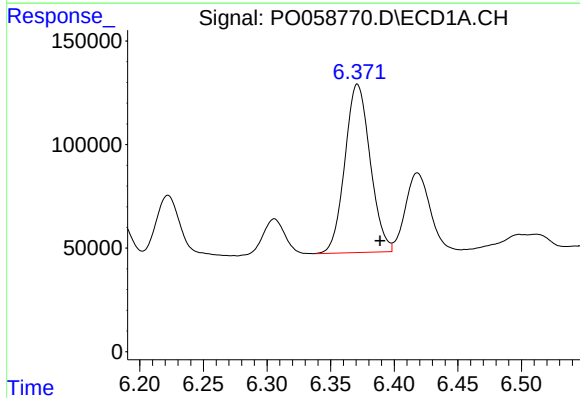


#27 AR-1254-2

R.T.: 6.371 min
Delta R.T.: -0.018 min
Response: 1126151
Conc: 292.21 ng/ml

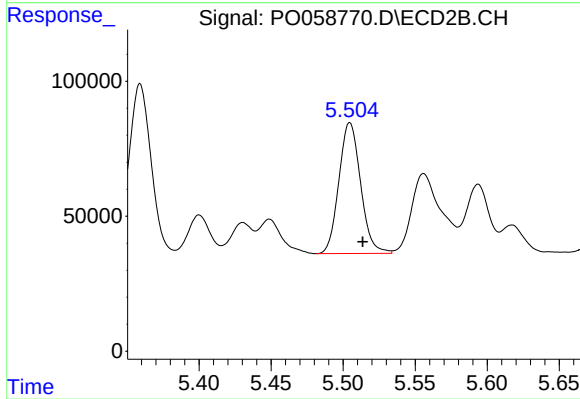

#27 AR-1254-2

R.T.: 5.505 min
Delta R.T.: -0.009 min
Response: 508651
Conc: 222.17 ng/ml

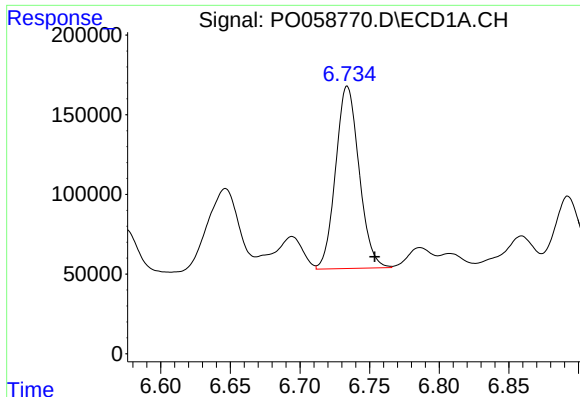


#28 AR-1254-3

R.T.: 6.734 min
Delta R.T.: -0.020 min
Response: 1341202
Conc: 331.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
SP-3RE


Manual Integrations
APPROVED

Ankita
8/2/2019 2:04:33 PM

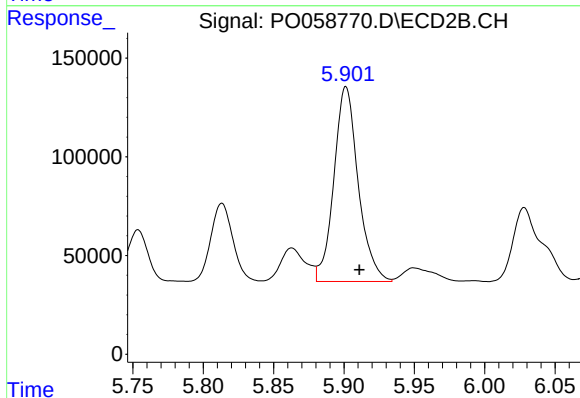


#28 AR-1254-3

R.T.: 5.901 min
Delta R.T.: -0.009 min
Response: 1188708
Conc: 323.07 ng/ml

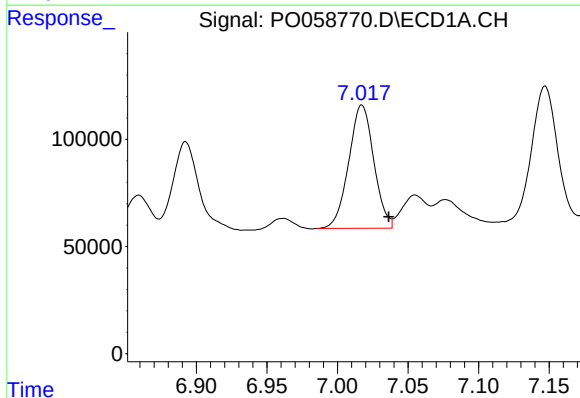


#29 AR-1254-4

R.T.: 7.017 min
Delta R.T.: -0.019 min
Response: 710637
Conc: 197.36 ng/ml m

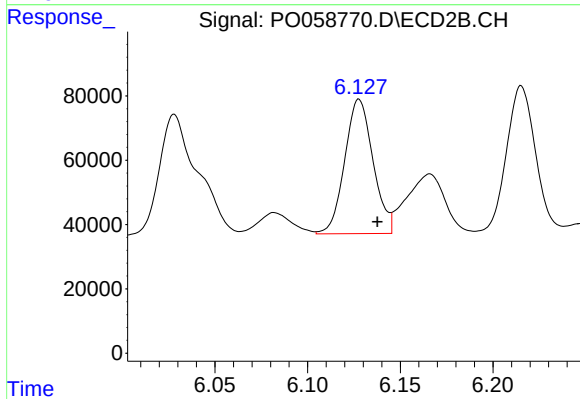

#29 AR-1254-4

R.T.: 6.128 min
Delta R.T.: -0.010 min
Response: 443838
Conc: 190.88 ng/ml

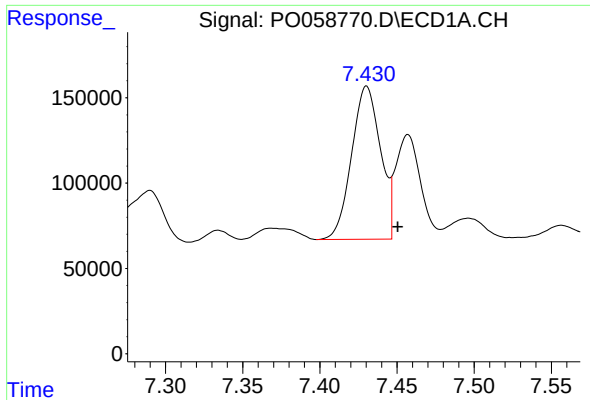


#30 AR-1254-5

R.T.: 7.430 min
Delta R.T.: -0.021 min
Response: 1185286
Conc: 327.00 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SP-3RE

Manual Integrations
APPROVED

Ankita
8/2/2019 2:04:33 PM

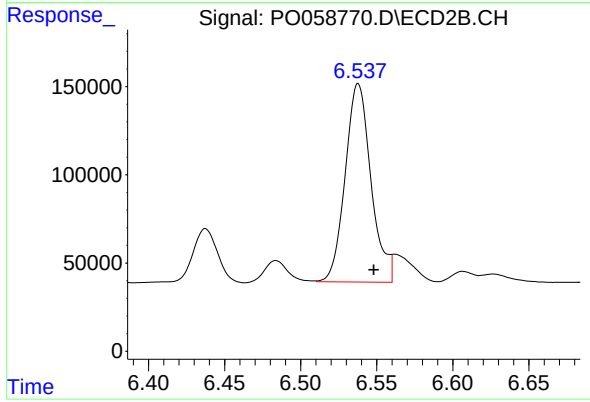

#30 AR-1254-5

R.T.: 6.537 min
Delta R.T.: -0.011 min
Response: 1330440
Conc: 385.68 ng/ml m