

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080221\
 Data File : P0080088.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Aug 2021 2:06
 Operator : DD\AJ
 Sample : M3247-16
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HEF3176(1-1)

Manual Integrations
 APPROVED

mohammad
 8/3/2021 3:10:27 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 03 05:37:00 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 28 18:45:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.999	4.118	1011539	424201	16.787	18.523
2) SA Decachlor...	11.116	9.542	755998	356550	16.116	17.157m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080221\
Data File : PO080088.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Aug 2021 2:06
Operator : DD\AJ
Sample : M3247-16
Misc :
ALS Vial : 35 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
HEF3176(1-1)


Manual Integrations
APPROVED

mohammad
8/3/2021 3:10:27 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 03 05:37:00 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072821.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 28 18:45:36 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

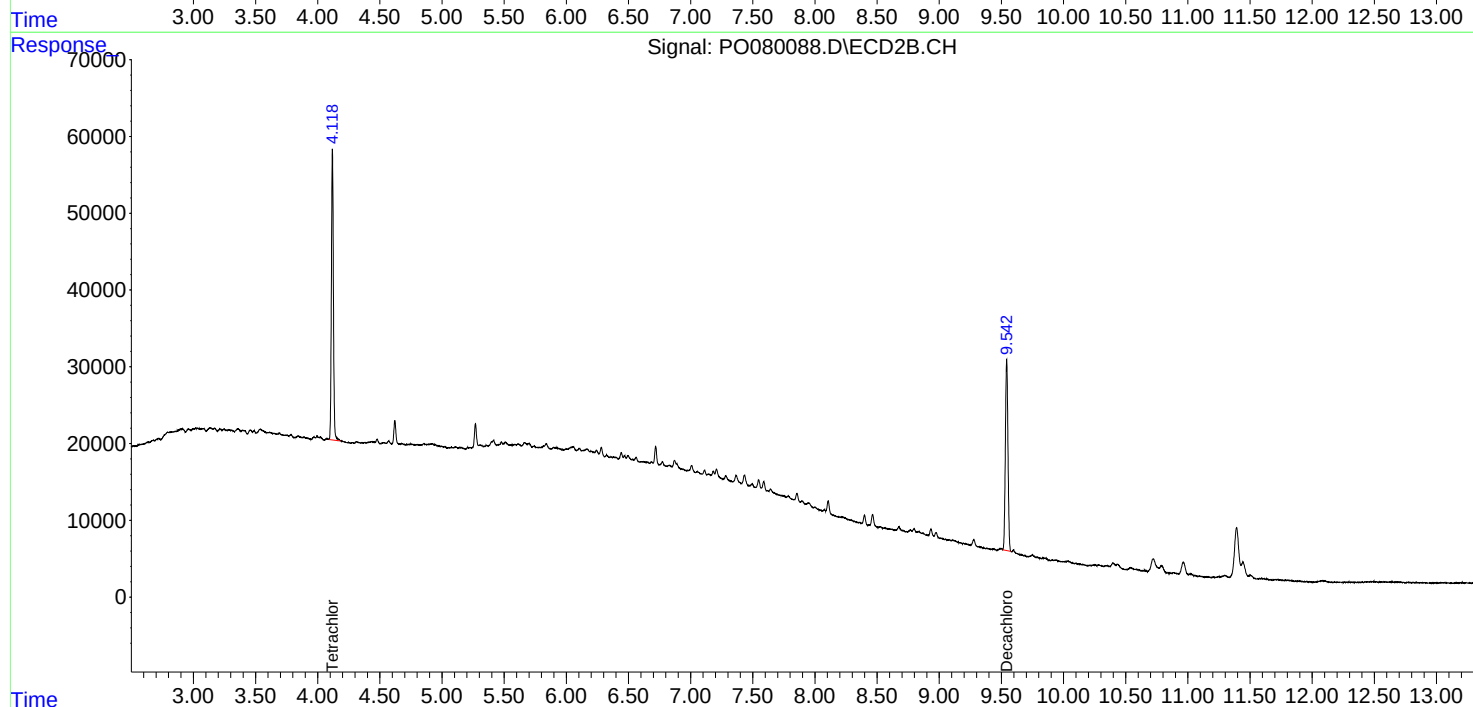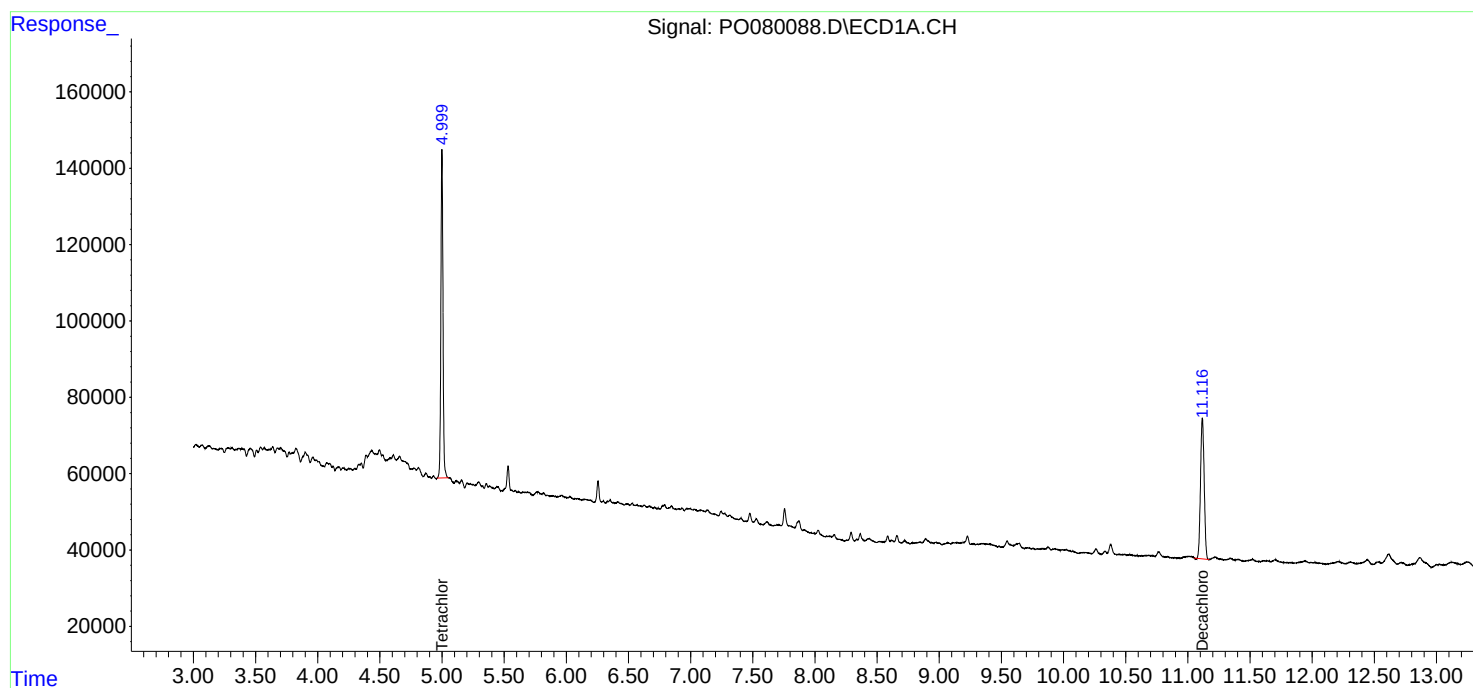

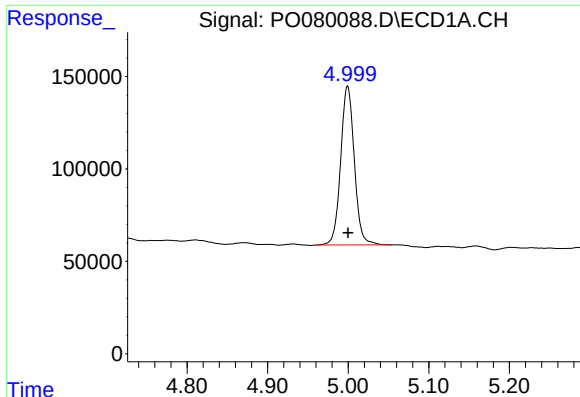


#1 Tetrachloro-m-xylene

R.T.: 4.999 min
Delta R.T.: 0.000 min
Response: 1011539
Conc: 16.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
HEF3176(1-1)


Manual Integrations
APPROVED

mohammad
8/3/2021 3:10:27 PM

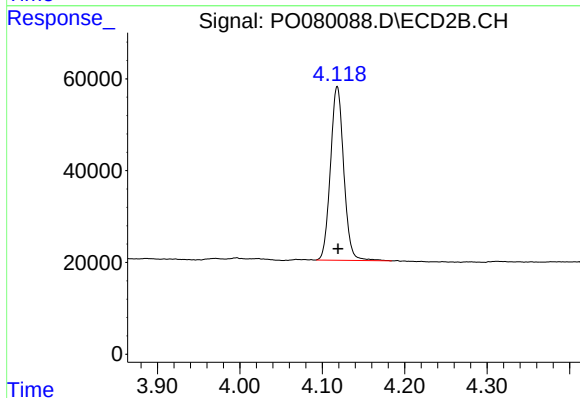


#1 Tetrachloro-m-xylene

R.T.: 4.118 min
Delta R.T.: -0.001 min
Response: 424201
Conc: 18.52 ng/ml

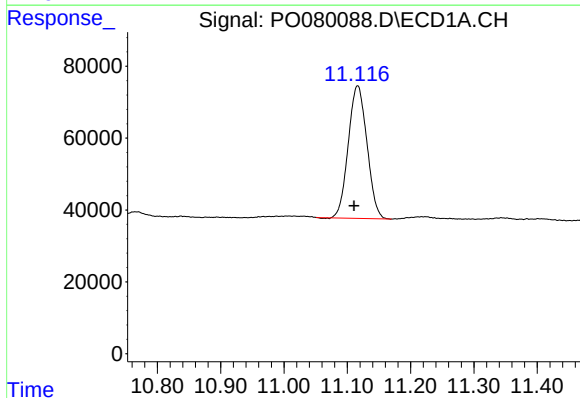

#2 Decachlorobiphenyl

R.T.: 11.116 min
Delta R.T.: 0.006 min
Response: 755998
Conc: 16.12 ng/ml

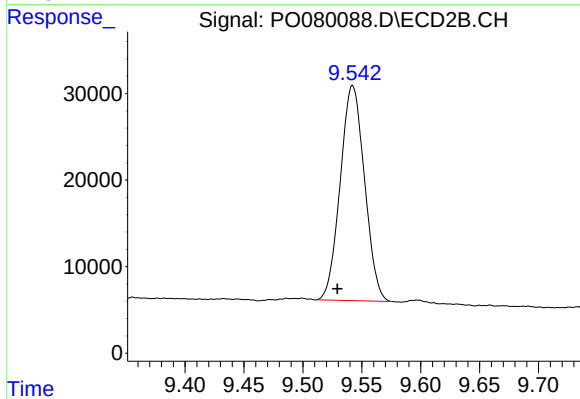

#2 Decachlorobiphenyl

R.T.: 9.542 min
Delta R.T.: 0.012 min
Response: 356550
Conc: 17.16 ng/ml m