

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080222\
 Data File : P0088539.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Aug 2022 17:27
 Operator : YP/AJ
 Sample : N3966-07DL 5X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S3-03-SDL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/03/2022
 Supervised By :Ankita Jodhani 08/03/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 03 00:07:03 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 26 11:20:17 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.444	3.604	10840398	3914979	4.249	4.149
2) SA Decachlor...	10.285	8.595	6723405	4867845	3.166	4.658 #
Target Compounds						
26) L6 AR-1254-1	6.479	5.479	8960104	5319854	94.503	92.270
27) L6 AR-1254-2	6.698	5.626	16077683	8131273	111.994	158.581 #
28) L6 AR-1254-3	7.068	6.029	32004081	17357476	218.493	213.895m
29) L6 AR-1254-4	7.354	6.258	19413981	10234649	179.381	205.210
30) L6 AR-1254-5	7.781	6.674	33868089	95515008	281.405m	1264.674 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080222\
Data File : PO088539.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Aug 2022 17:27
Operator : YP/AJ
Sample : N3966-07DL 5X
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
S3-03-SDL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/03/2022
Supervised By :Ankita Jodhani 08/03/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 03 00:07:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO071422.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 26 11:20:17 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

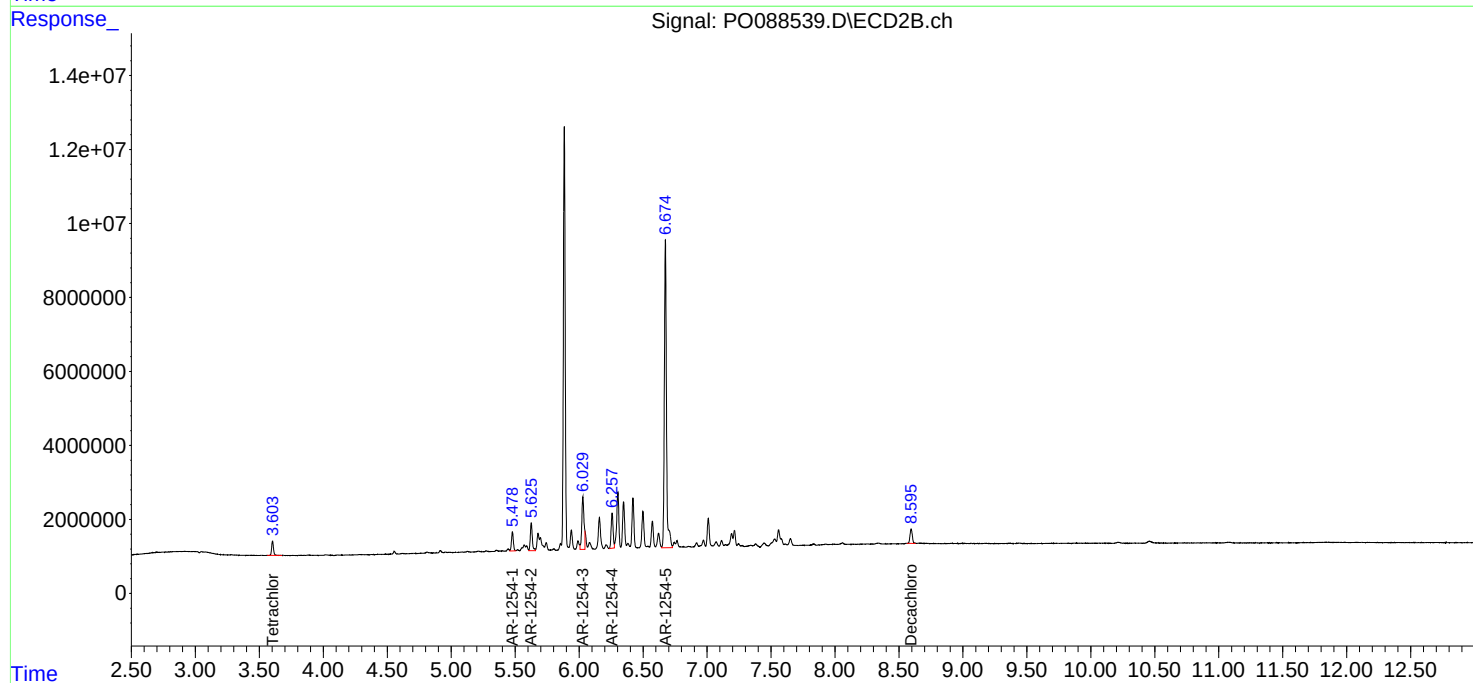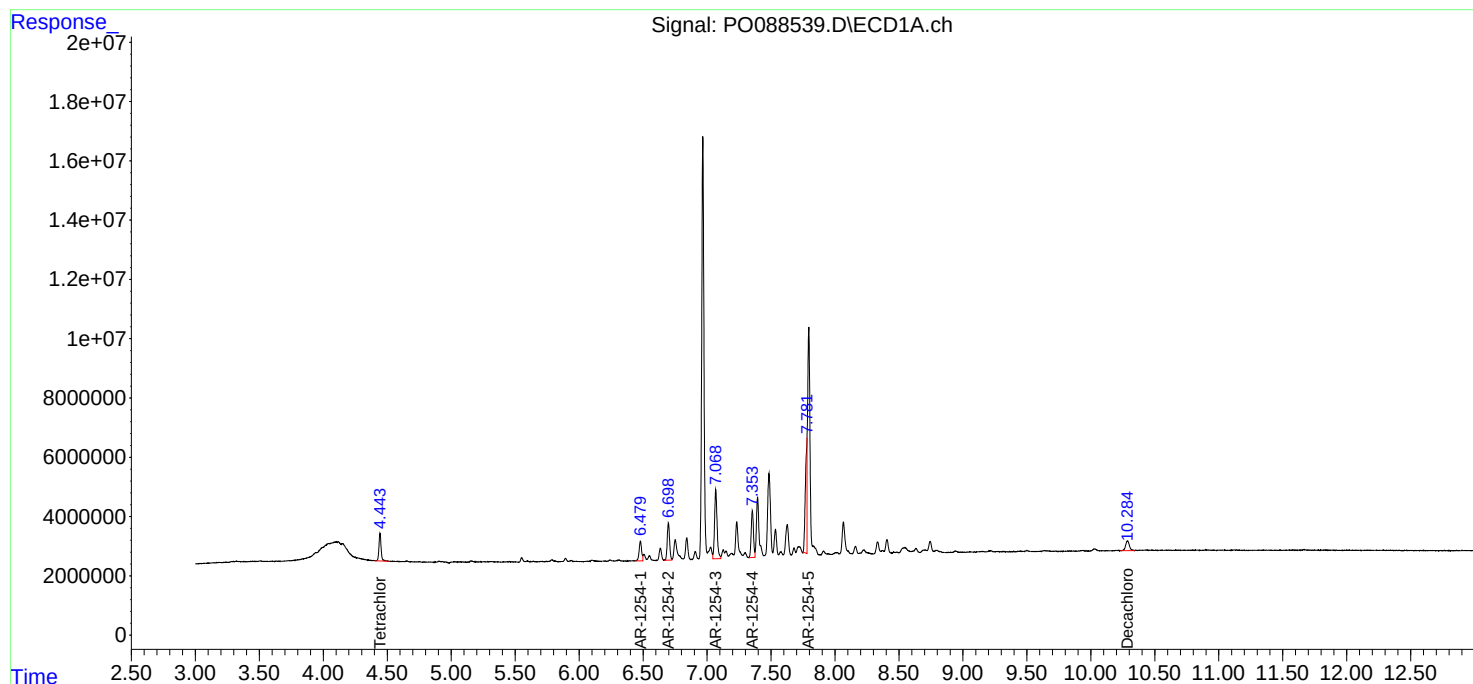

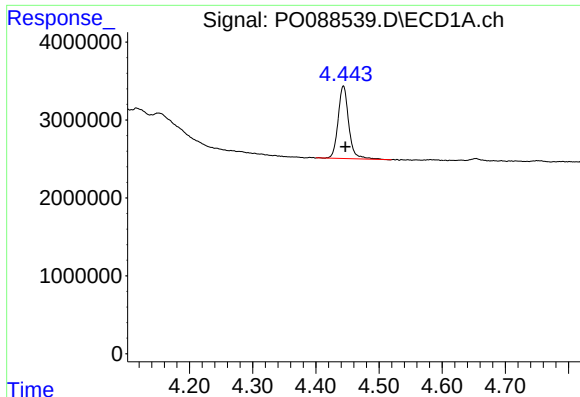


#1 Tetrachloro-m-xylene

R.T.: 4.444 min
Delta R.T.: -0.003 min
Response: 10840398
Conc: 4.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
S3-03-SDL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/03/2022
Supervised By :Ankita Jodhani 08/03/2022

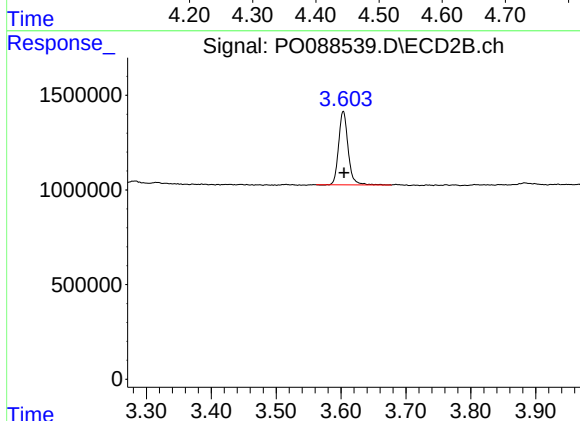


#1 Tetrachloro-m-xylene

R.T.: 3.604 min
Delta R.T.: -0.001 min
Response: 3914979
Conc: 4.15 ng/ml

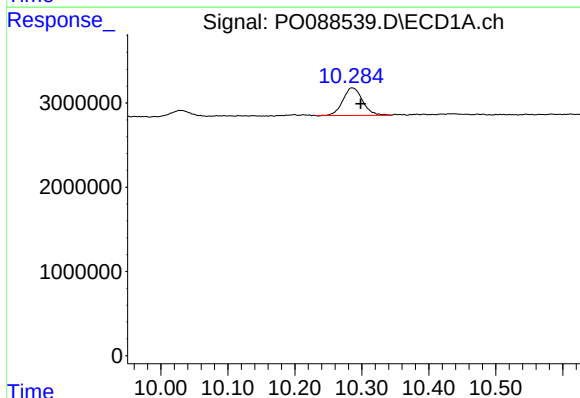


#2 Decachlorobiphenyl

R.T.: 10.285 min
Delta R.T.: -0.013 min
Response: 6723405
Conc: 3.17 ng/ml

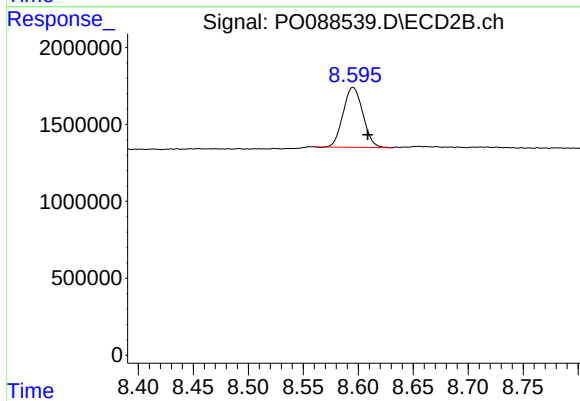

#2 Decachlorobiphenyl

R.T.: 8.595 min
Delta R.T.: -0.013 min
Response: 4867845
Conc: 4.66 ng/ml

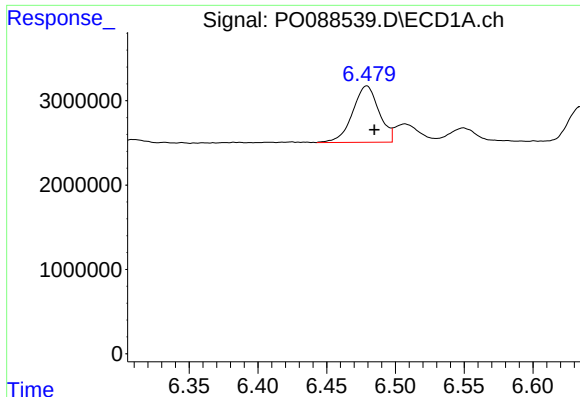


#26 AR-1254-1

R.T.: 6.479 min
Delta R.T.: -0.006 min
Response: 8960104
Conc: 94.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
S3-03-SDL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/03/2022
Supervised By :Ankita Jodhani 08/03/2022

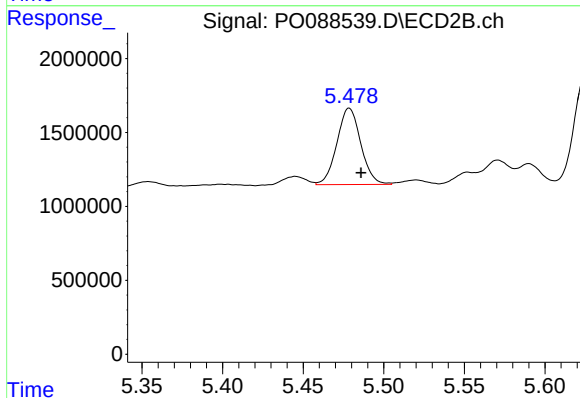


#26 AR-1254-1

R.T.: 5.479 min
Delta R.T.: -0.007 min
Response: 5319854
Conc: 92.27 ng/ml

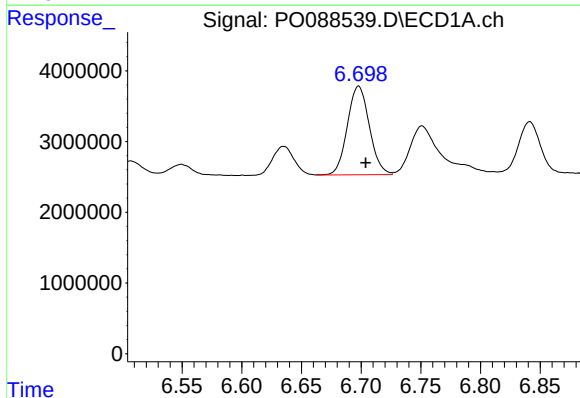


#27 AR-1254-2

R.T.: 6.698 min
Delta R.T.: -0.006 min
Response: 16077683
Conc: 111.99 ng/ml

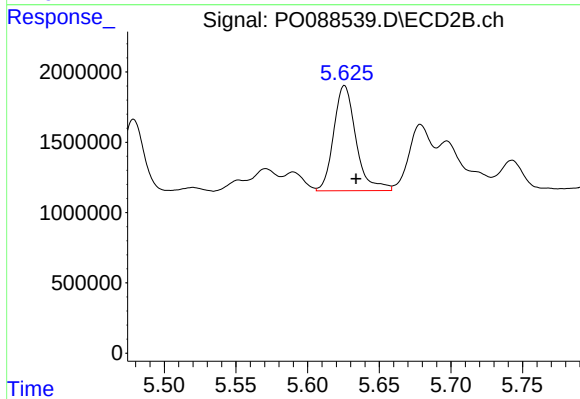

#27 AR-1254-2

R.T.: 5.626 min
Delta R.T.: -0.008 min
Response: 8131273
Conc: 158.58 ng/ml

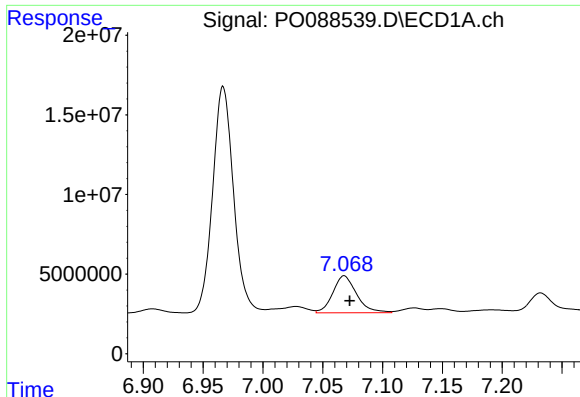


#28 AR-1254-3

R.T.: 7.068 min
Delta R.T.: -0.005 min
Response: 32004081
Conc: 218.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
S3-03-SDL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/03/2022
Supervised By :Ankita Jodhani 08/03/2022

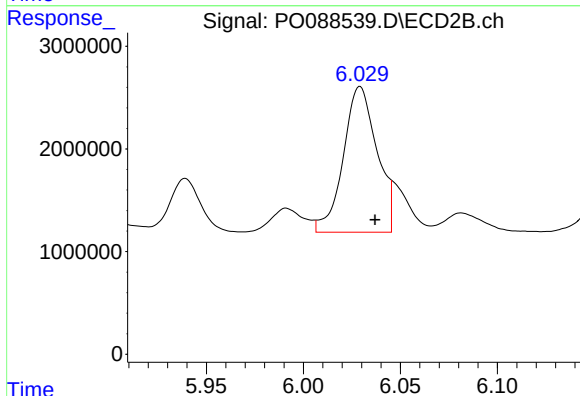


#28 AR-1254-3

R.T.: 6.029 min
Delta R.T.: -0.008 min
Response: 17357476
Conc: 213.89 ng/ml m

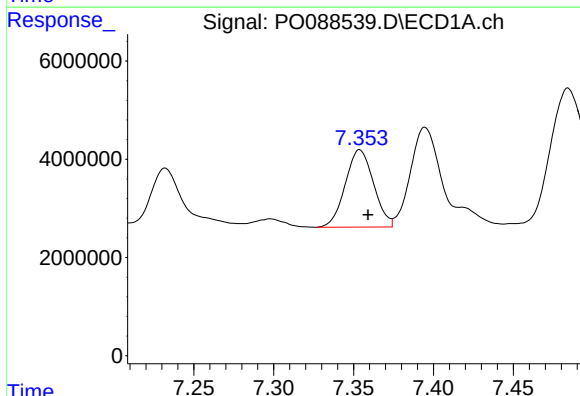


#29 AR-1254-4

R.T.: 7.354 min
Delta R.T.: -0.005 min
Response: 19413981
Conc: 179.38 ng/ml

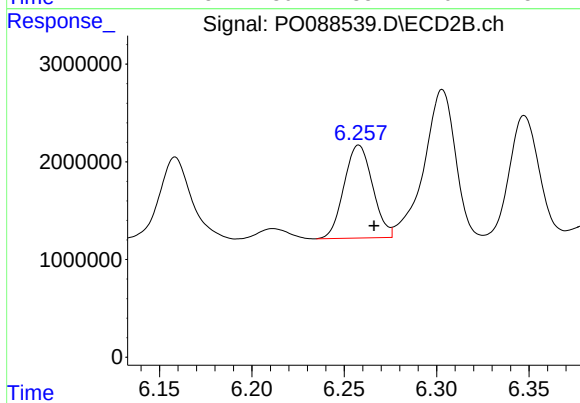

#29 AR-1254-4

R.T.: 6.258 min
Delta R.T.: -0.008 min
Response: 10234649
Conc: 205.21 ng/ml

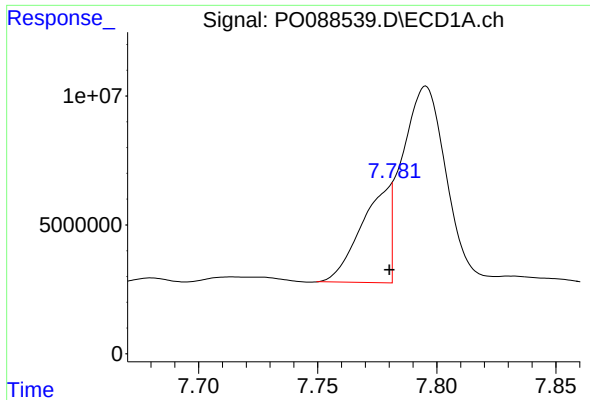


#30 AR-1254-5

R.T.: 7.781 min
Delta R.T.: 0.000 min
Response: 33868089
Conc: 281.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
S3-03-SDL

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/03/2022
Supervised By :Ankita Jodhani 08/03/2022

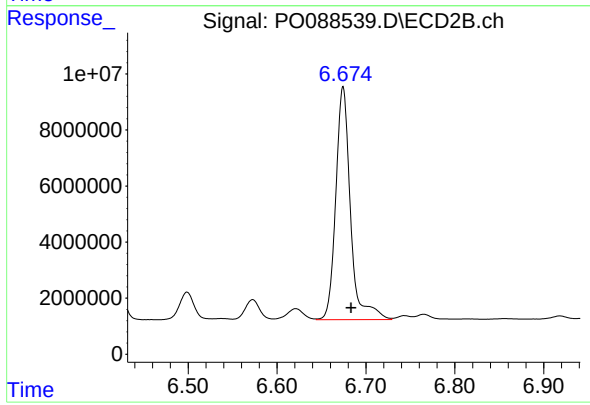

#30 AR-1254-5

R.T.: 6.674 min
Delta R.T.: -0.009 min
Response: 95515008
Conc: 1264.67 ng/ml