

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080223\
 Data File : P0096601.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Aug 2023 18:40
 Operator : YP/AJ
 Sample : 03862-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BUILDING-B-11-(10-15)

Manual Integrations
 APPROVED

Reviewed By :Yogesh
 Patel

08/14/2023
 Supervised By :Ankita
 Jodhani

08/14/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 03 02:06:22 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jul 28 01:38:03 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.412	3.622	71428032	29185168	21.378	20.603
2) SA Decachlor...	10.237	8.644	52995822	26804290	23.953	22.787m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080223\
Data File : PO096601.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Aug 2023 18:40
Operator : YP/AJ
Sample : 03862-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
BUILDING-B-11-(10-15)

Manual Integrations
APPROVED



Reviewed By :Yogesh
Patel


08/14/2023
Supervised By :Ankita
Jodhani

08/14/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 03 02:06:22 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072723.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 28 01:38:03 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

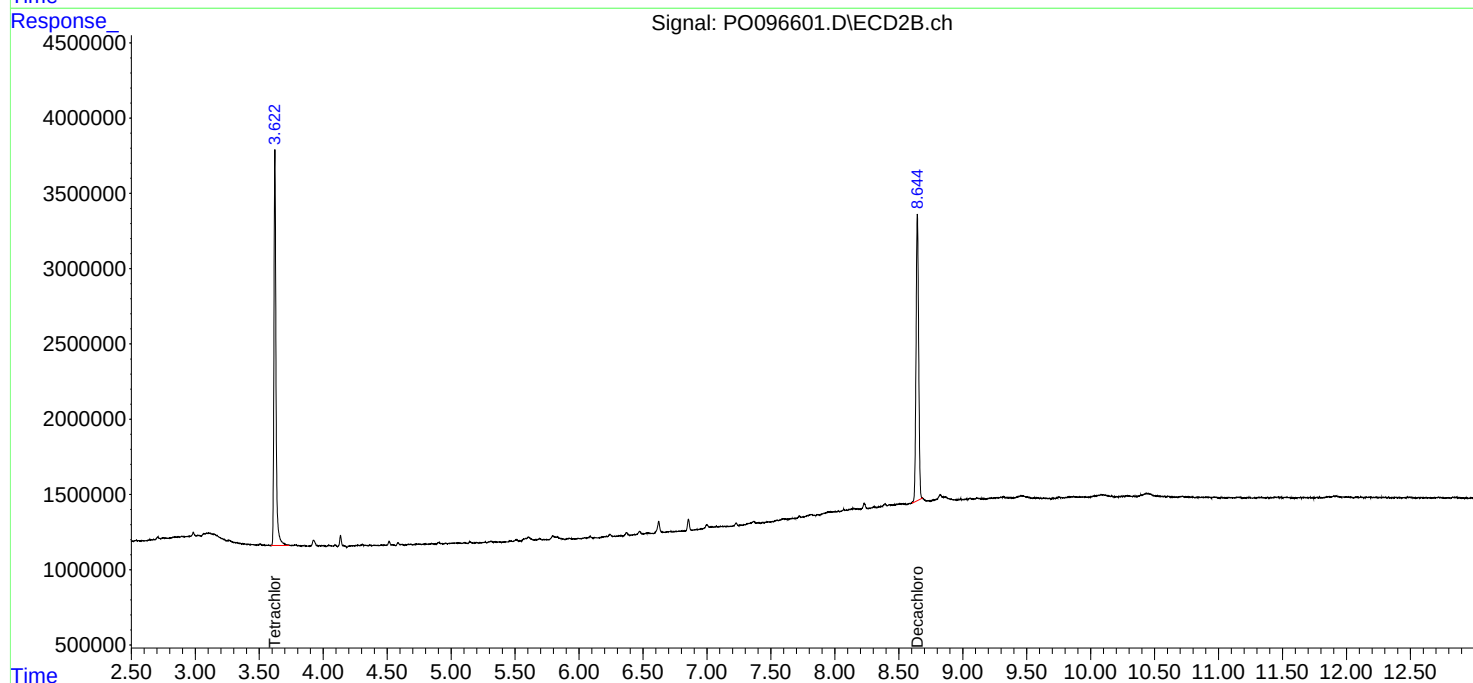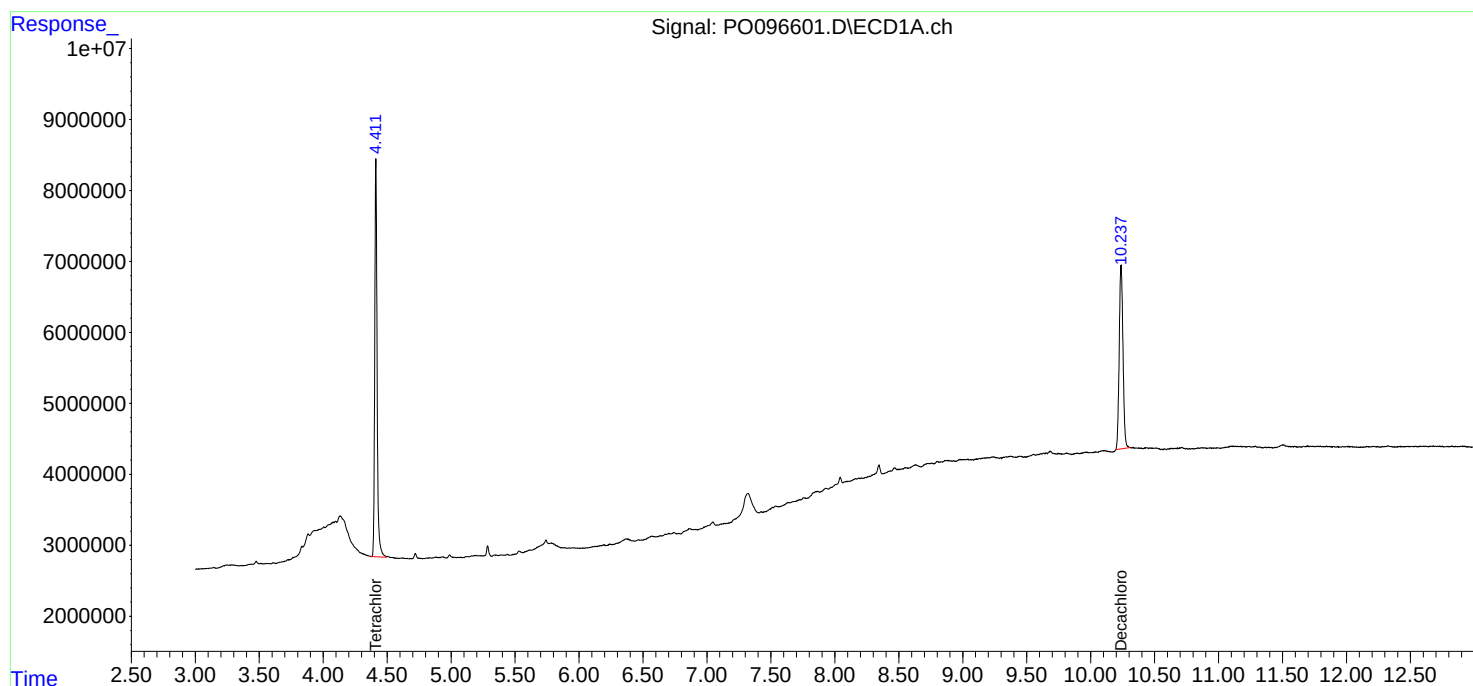

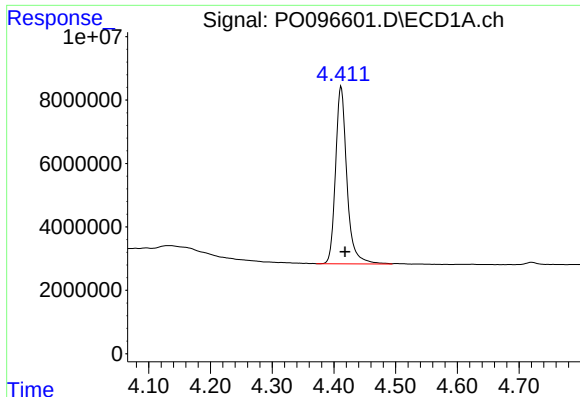

#1 Tetrachloro-m-xylene

R.T.: 4.412 min
Delta R.T.: -0.006 min
Response: 71428032
Conc: 21.38 ng/ml


Instrument :
ECD_O
ClientSampleId :
BUILDING-B-11-(10-15)

Manual Integrations
APPROVED

Reviewed By :Yogesh
Patel


08/14/2023
Supervised By :Ankita
Jodhani

08/14/2023

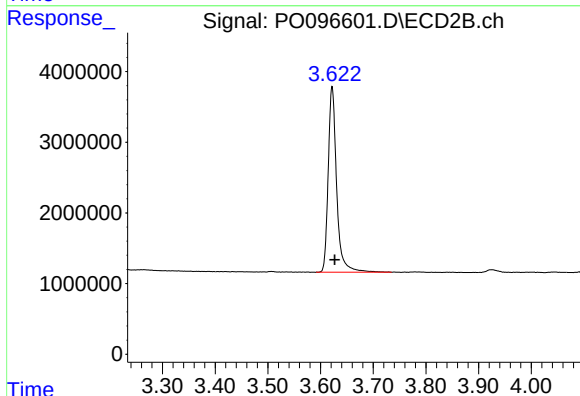


#1 Tetrachloro-m-xylene

R.T.: 3.622 min
Delta R.T.: -0.005 min
Response: 29185168
Conc: 20.60 ng/ml

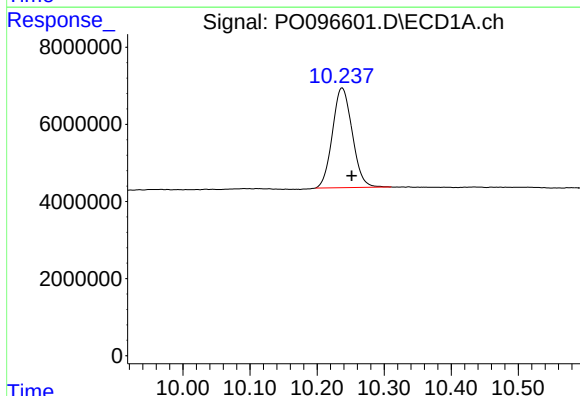

#2 Decachlorobiphenyl

R.T.: 10.237 min
Delta R.T.: -0.014 min
Response: 52995822
Conc: 23.95 ng/ml

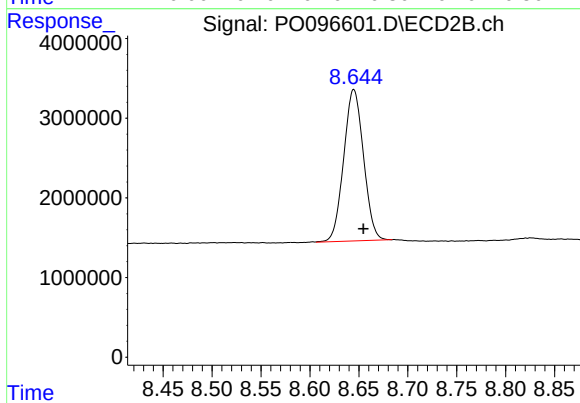

#2 Decachlorobiphenyl

R.T.: 8.644 min
Delta R.T.: -0.010 min
Response: 26804290
Conc: 22.79 ng/ml m