

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080223\
 Data File : P0096602.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Aug 2023 18:57
 Operator : YP/AJ
 Sample : 03862-02
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BUILDING-B-3-(5-10)

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/03/2023
 Supervised By :Ankita Jodhani 08/03/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 03 02:06:41 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jul 28 01:38:03 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.411	3.622	47847109	21839401	14.320m	15.417m
2) SA Decachlor...	10.236	8.645	51172337	23418274	23.128	19.908

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080223\
Data File : PO096602.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Aug 2023 18:57
Operator : YP/AJ
Sample : 03862-02
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BUILDING-B-3-(5-10)


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/03/2023
Supervised By :Ankita Jodhani 08/03/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 03 02:06:41 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072723.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 28 01:38:03 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

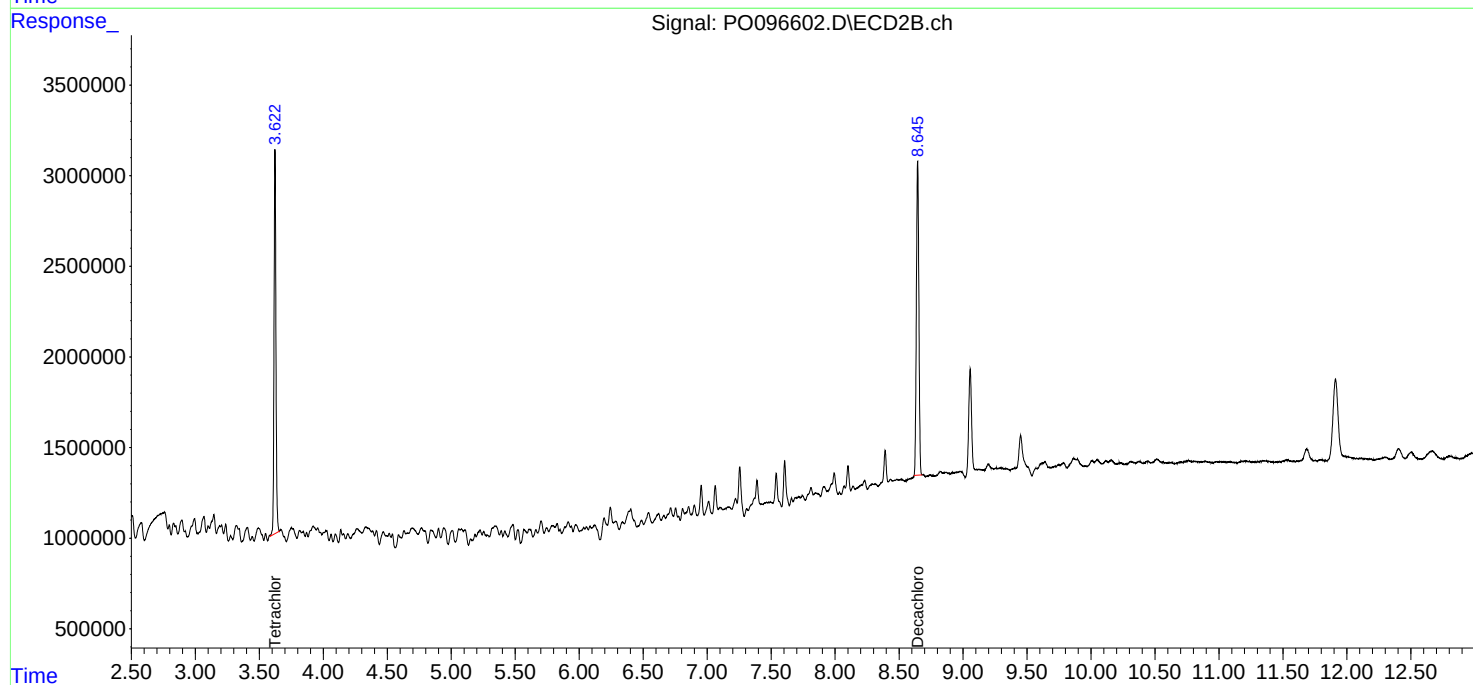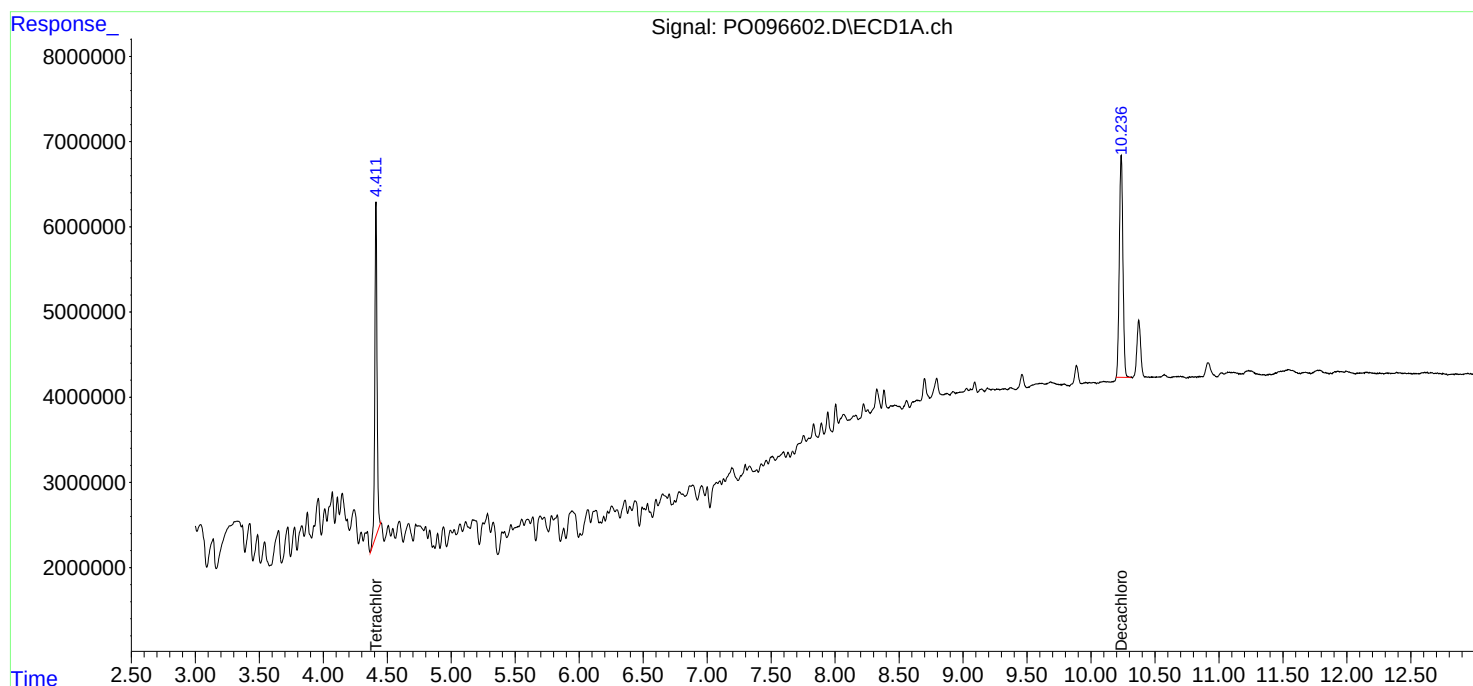

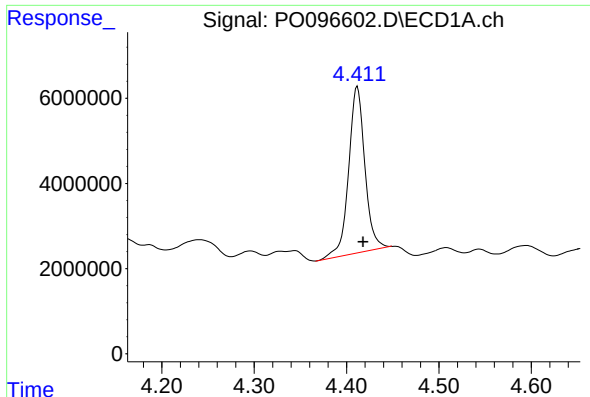


#1 Tetrachloro-m-xylene

R.T.: 4.411 min
Delta R.T.: -0.007 min
Response: 47847109
Conc: 14.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
BUILDING-B-3-(5-10)


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/03/2023
Supervised By :Ankita Jodhani 08/03/2023

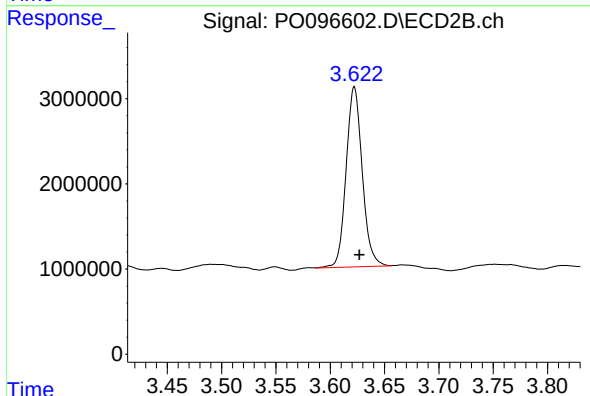


#1 Tetrachloro-m-xylene

R.T.: 3.622 min
Delta R.T.: -0.005 min
Response: 21839401
Conc: 15.42 ng/ml m

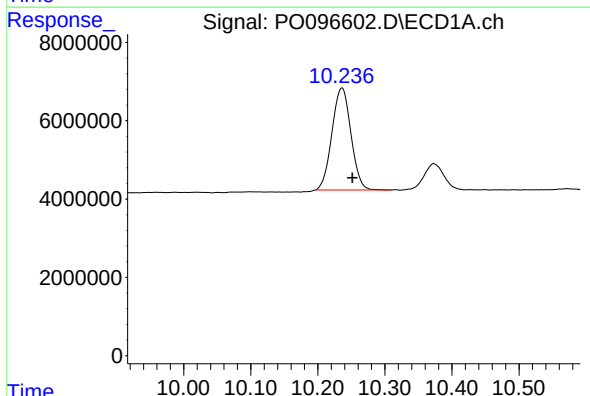

#2 Decachlorobiphenyl

R.T.: 10.236 min
Delta R.T.: -0.015 min
Response: 51172337
Conc: 23.13 ng/ml

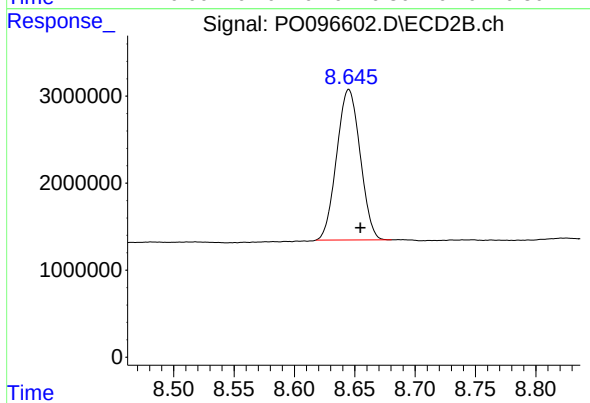

#2 Decachlorobiphenyl

R.T.: 8.645 min
Delta R.T.: -0.010 min
Response: 23418274
Conc: 19.91 ng/ml