

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0080318\
 Data File : P0047632.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Aug 2018 13:31
 Operator : SM/SJ
 Sample : J4257-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 FK-BPM-03-001-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 03 13:55:05 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jul 27 02:33:29 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.407	3.645	4663000	5245968	23.096	21.350
2) SA Decachlor...	10.100	8.635	2665158	2772687	16.341	17.639
Target Compounds						
3) L1 AR-1016-1	5.330	4.530	83634	115828	17.509	20.260
4) L1 AR-1016-2	5.644	0.000	13683	0	2.324	N.D. #
5) L1 AR-1016-3	5.749	5.006	6580	6757	1.327	1.539
6) L1 AR-1016-4	6.024	5.006	12447	6757	2.676	1.303 #
7) L1 AR-1016-5	6.206	5.164	150045	39147	28.783	6.674 #
8) L2 AR-1221-1	4.592	3.908	3086	6589	1.396	2.792 #
9) L2 AR-1221-2	4.713	3.947	65553	151600	40.089	83.570 #
10) L2 AR-1221-3	4.713	4.016	65553	32289	12.697	5.586 #
11) L3 AR-1232-1	5.101	4.320	144920	94074	67.388	40.002 #
12) L3 AR-1232-2	5.564	4.701	2287	74591	0.777	24.409 #
13) L3 AR-1232-3	5.595	4.701	12090	74591	2.814	16.153 #
14) L3 AR-1232-4	5.644	4.810	13683	14218	4.943	4.599
15) L3 AR-1232-5	5.749	5.006	6580	6757	2.947	3.776 #
16) L4 AR-1242-1	5.595	4.701	12090	74591	1.645	9.314 #
17) L4 AR-1242-2	5.644	0.000	13683	0	2.956	N.D. #
18) L4 AR-1242-3	5.749	5.006	6580	6757	1.713	1.611
19) L4 AR-1242-4	6.024	5.164	12447	39147	3.238	8.290 #
20) L4 AR-1242-5	6.206	5.279	150045	111389	35.053	28.770
21) L5 AR-1248-1	6.024	5.164	12447	39147	1.990	5.247 #
22) L5 AR-1248-2	6.206	5.279	150045	111389	27.543	20.821
23) L5 AR-1248-3	6.457	5.526	11328	67474	1.610	6.781 #
24) L5 AR-1248-4	6.485	5.609	4176	26422	0.622	3.770 #
25) L5 AR-1248-5	6.643	6.095	20235	89526	2.859	18.785 #
26) L6 AR-1254-1	6.643	5.526	20235	67474	1.655	5.483 #
27) L6 AR-1254-2	6.911	5.672	74681	6433	10.014	0.618 #
28) L6 AR-1254-3	7.017	6.095	211834	89526	16.243	5.158 #
29) L6 AR-1254-4	7.292	6.307	11793	34932	1.210	3.224 #
30) L6 AR-1254-5	7.557	6.609	3771	54020	0.510	7.064 #
31) L7 AR-1260-1	7.168	6.203	6603	32790	0.704	2.967 #
32) L7 AR-1260-2	7.418	6.380	78140	235713	7.007	17.580 #
33) L7 AR-1260-3	7.729	6.719	98395	169757	7.648	11.677 #
34) L7 AR-1260-4	8.317	7.231	46450	109882	2.611	4.994 #
35) L7 AR-1260-5	8.638	7.592	53948	81645	4.724	5.234
36) L8 AR-1262-1	7.168	6.380	6603	235713	0.797	20.790 #
37) L8 AR-1262-2	7.418	6.541	78140	21008	8.063	1.862 #
38) L8 AR-1262-3	7.780	6.719	6518	169757	0.531	11.248 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0080318\
 Data File : P0047632.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Aug 2018 13:31
 Operator : SM/SJ
 Sample : J4257-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-BPM-03-001-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 03 13:55:05 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jul 27 02:33:29 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
39)	L8 AR-1262-4	8.000	7.015	7100	22326	0.603	1.695 #
40)	L8 AR-1262-5	8.317	7.231	46450	109882	2.162	4.254 #
41)	L9 AR-1268-1	8.638	7.538	53948	38991	2.324	1.500 #
42)	L9 AR-1268-2	8.707	7.592	11183	81645	0.522	3.277 #
43)	L9 AR-1268-3	8.945	7.808	44555	36237	2.468	1.836 #
44)	L9 AR-1268-4	9.352	8.087	53461	21021	6.704	2.506 #
45)	L9 AR-1268-5	9.773	8.383	37287	23123	0.684	0.424 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080318\
Data File : P0047632.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Aug 2018 13:31
Operator : SM/SJ
Sample : J4257-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :
FK-BPM-03-001-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 03 13:55:05 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072718.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 27 02:33:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

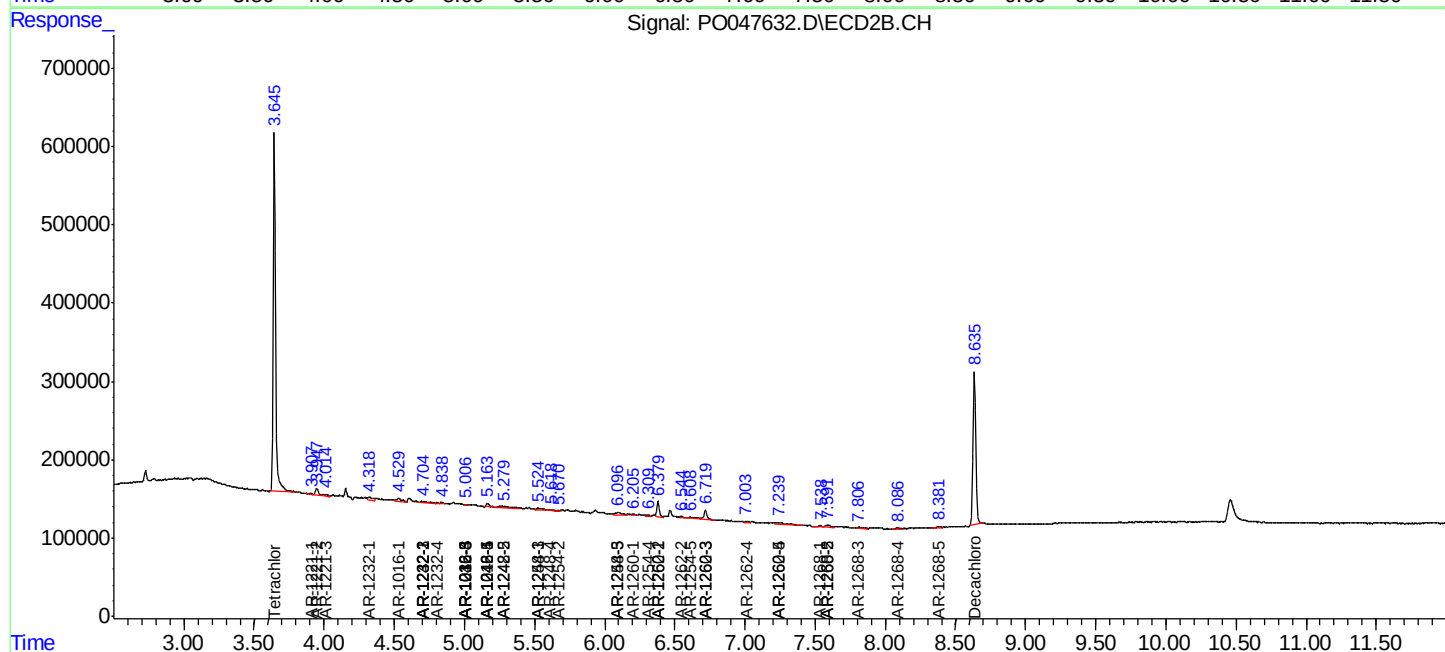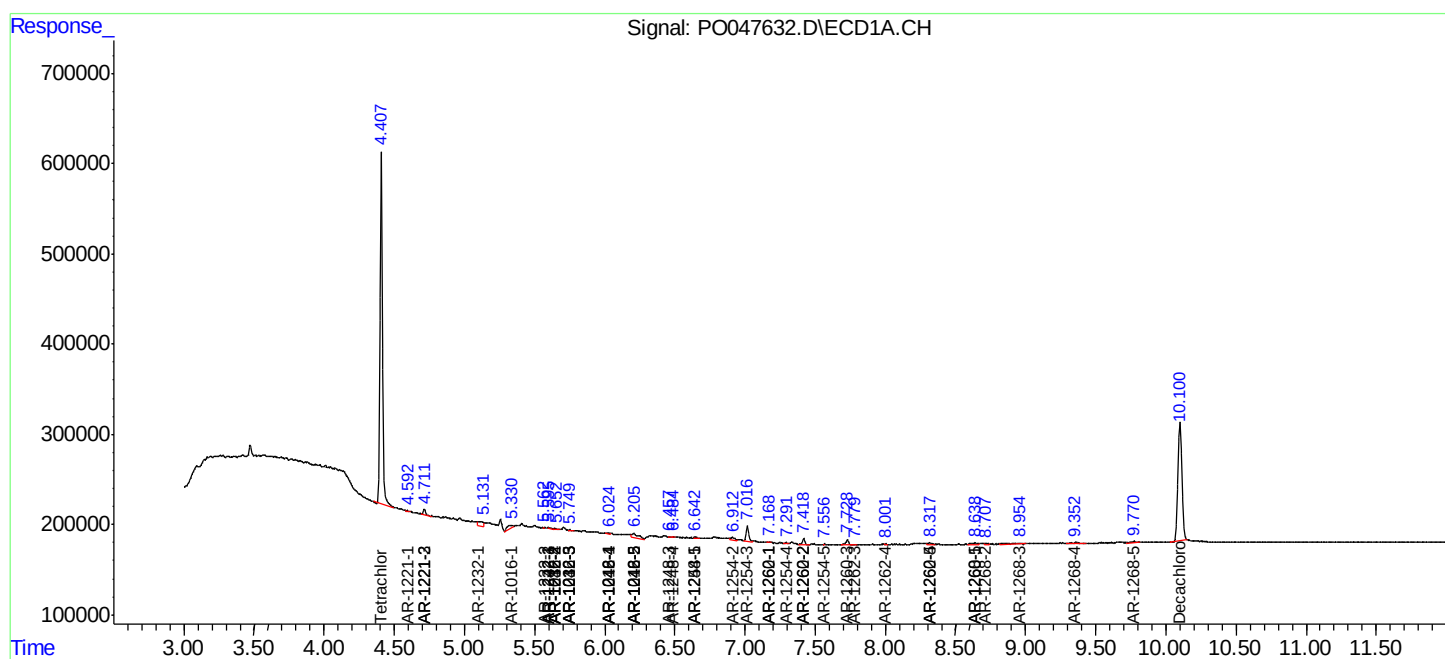


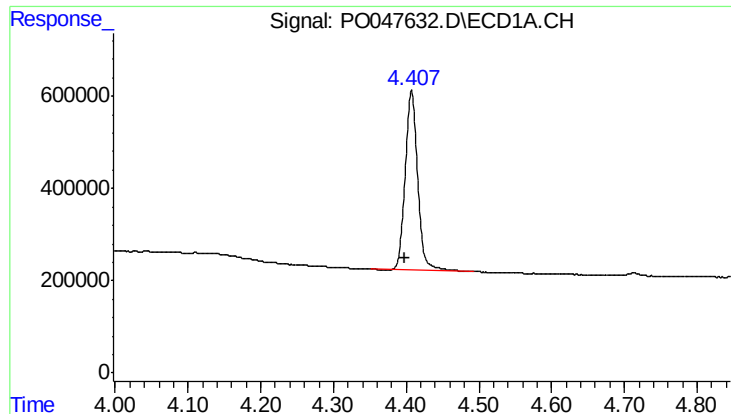

#1 Tetrachloro-m-xylene


R.T.: 4.407 min
Delta R.T.: 0.010 min
Response: 4663000
Conc: 23.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-001-B

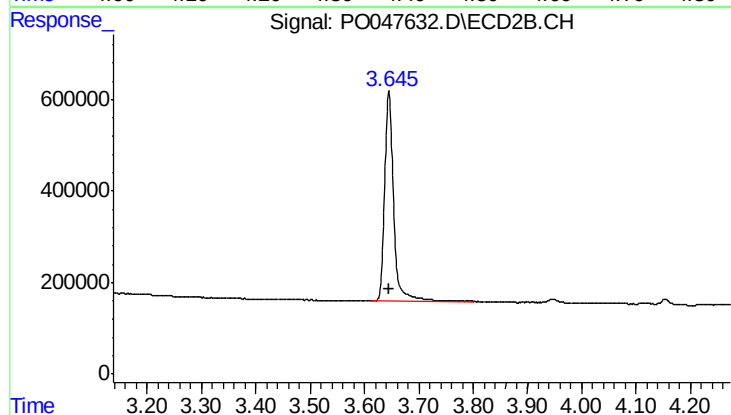


#1 Tetrachloro-m-xylene

R.T.: 3.645 min
Delta R.T.: 0.000 min
Response: 5245968
Conc: 21.35 ng/ml

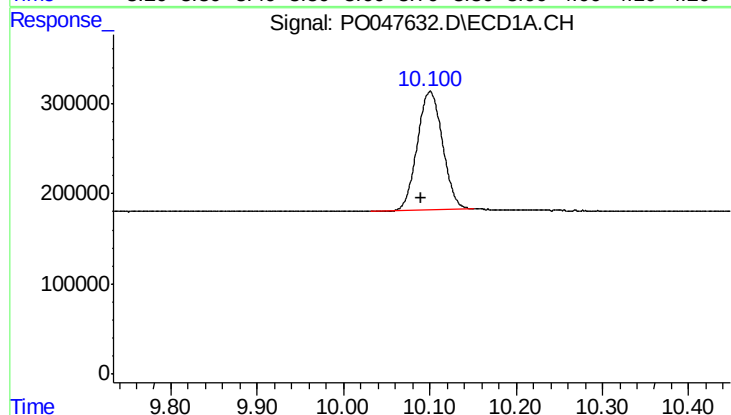


#2 Decachlorobiphenyl

R.T.: 10.100 min
Delta R.T.: 0.010 min
Response: 2665158
Conc: 16.34 ng/ml

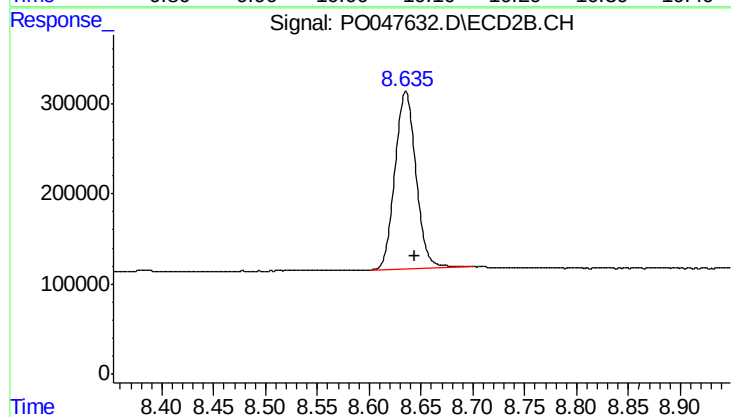

#2 Decachlorobiphenyl


R.T.: 8.635 min
Delta R.T.: -0.009 min
Response: 2772687
Conc: 17.64 ng/ml

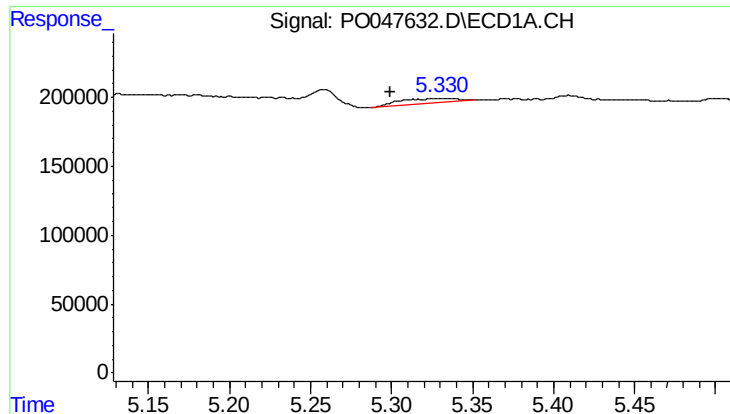

#3 AR-1016-1


R.T.: 5.330 min
Delta R.T.: 0.030 min
Response: 83634
Conc: 17.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-001-B

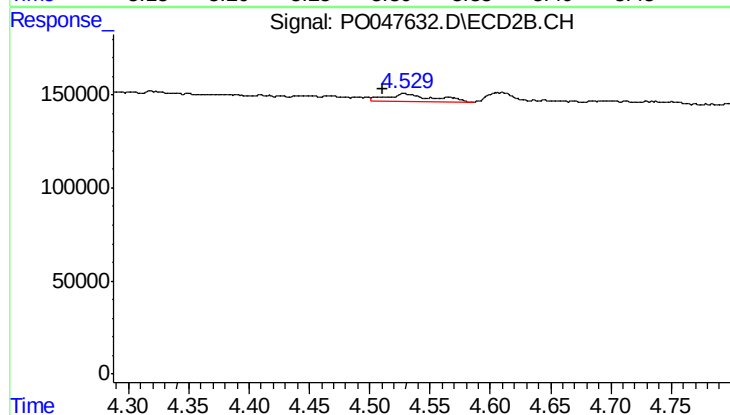


#3 AR-1016-1

R.T.: 4.530 min
Delta R.T.: 0.018 min
Response: 115828
Conc: 20.26 ng/ml

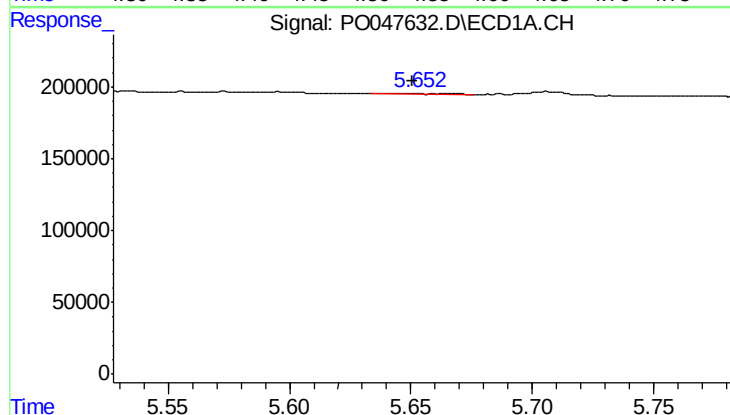


#4 AR-1016-2

R.T.: 5.644 min
Delta R.T.: -0.006 min
Response: 13683
Conc: 2.32 ng/ml

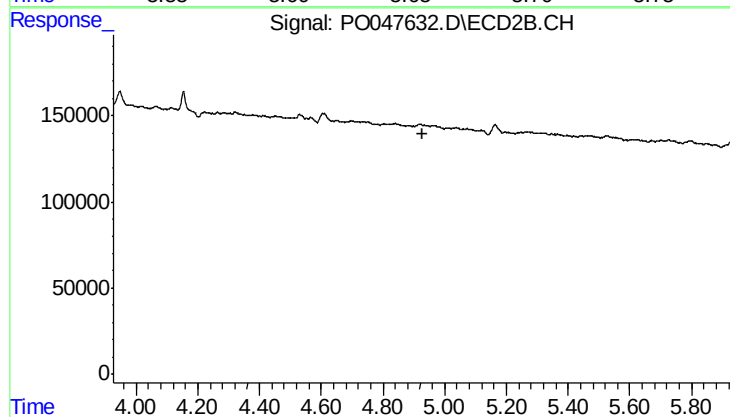

#4 AR-1016-2


R.T.: 0.000 min
Exp R.T.: 4.926 min
Response: 0
Conc: N.D.

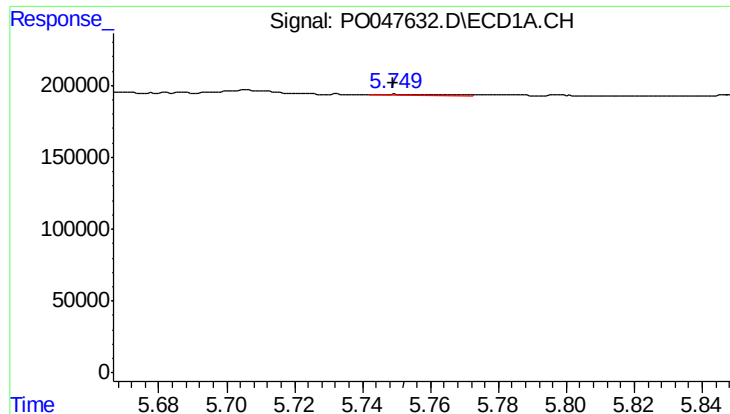

#5 AR-1016-3


R.T.: 5.749 min
Delta R.T.: 0.000 min
Response: 6580
Conc: 1.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-001-B

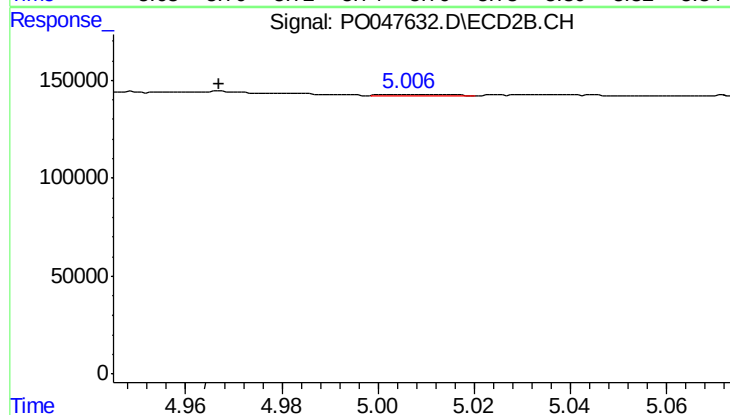


#5 AR-1016-3

R.T.: 5.006 min
Delta R.T.: 0.039 min
Response: 6757
Conc: 1.54 ng/ml

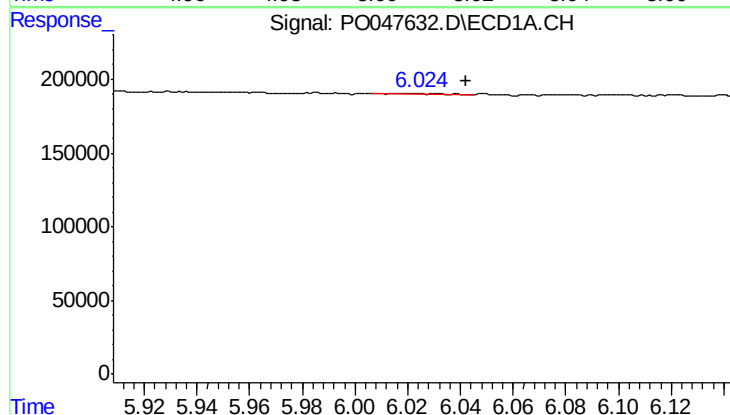


#6 AR-1016-4

R.T.: 6.024 min
Delta R.T.: -0.018 min
Response: 12447
Conc: 2.68 ng/ml

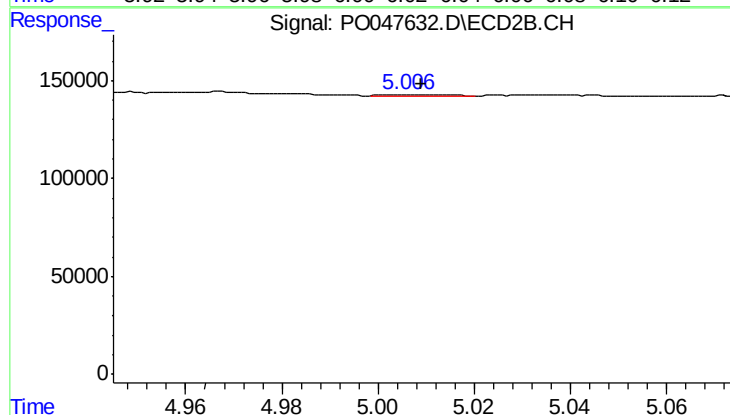

#6 AR-1016-4


R.T.: 5.006 min
Delta R.T.: -0.003 min
Response: 6757
Conc: 1.30 ng/ml

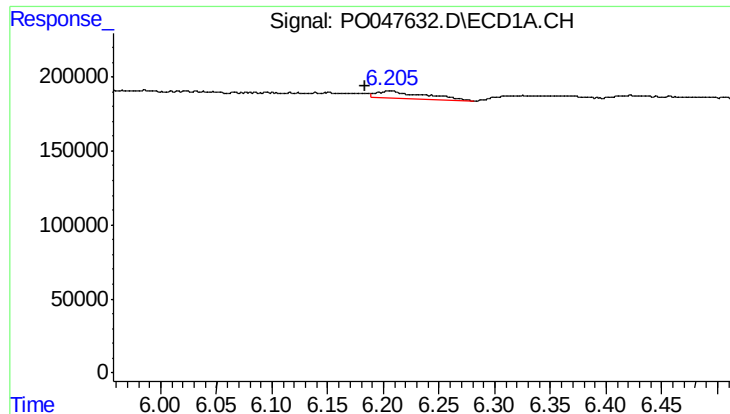

#7 AR-1016-5


R.T.: 6.206 min
Delta R.T.: 0.022 min
Response: 150045
Conc: 28.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-001-B

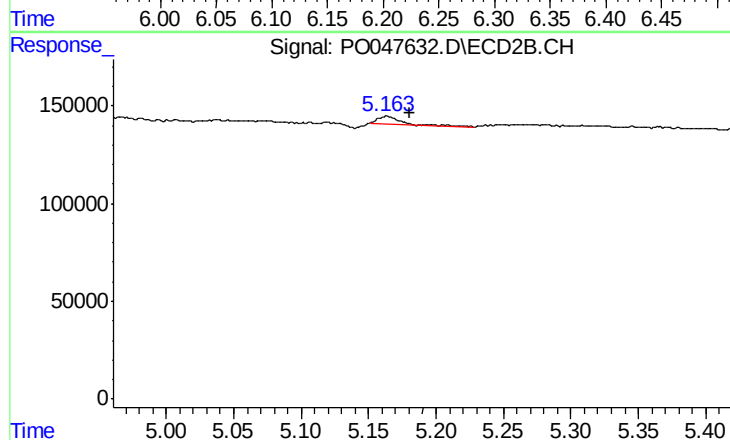


#7 AR-1016-5

R.T.: 5.164 min
Delta R.T.: -0.017 min
Response: 39147
Conc: 6.67 ng/ml

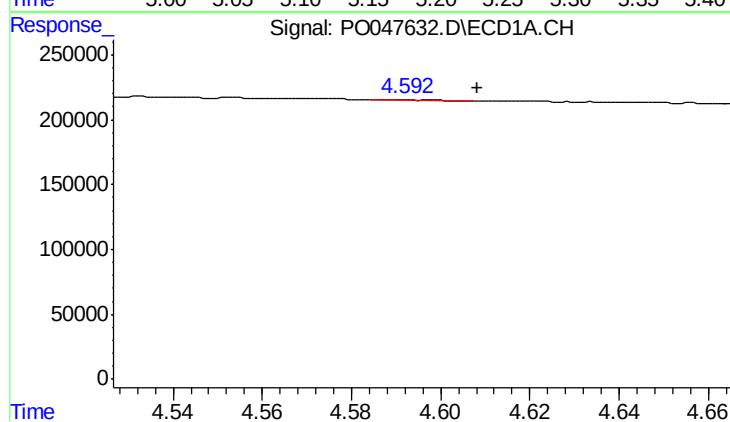


#8 AR-1221-1

R.T.: 4.592 min
Delta R.T.: -0.017 min
Response: 3086
Conc: 1.40 ng/ml

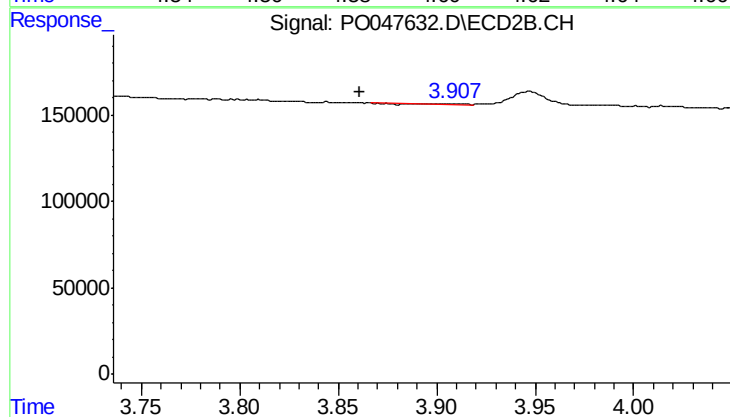

#8 AR-1221-1


R.T.: 3.908 min
Delta R.T.: 0.047 min
Response: 6589
Conc: 2.79 ng/ml

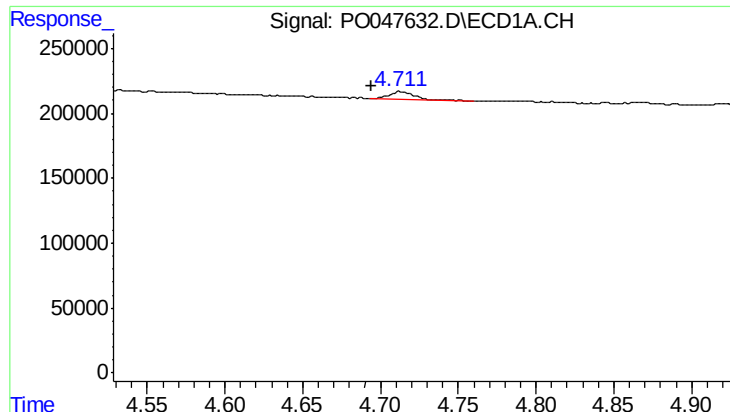

#9 AR-1221-2


R.T.: 4.713 min
Delta R.T.: 0.019 min
Response: 65553
Conc: 40.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-001-B

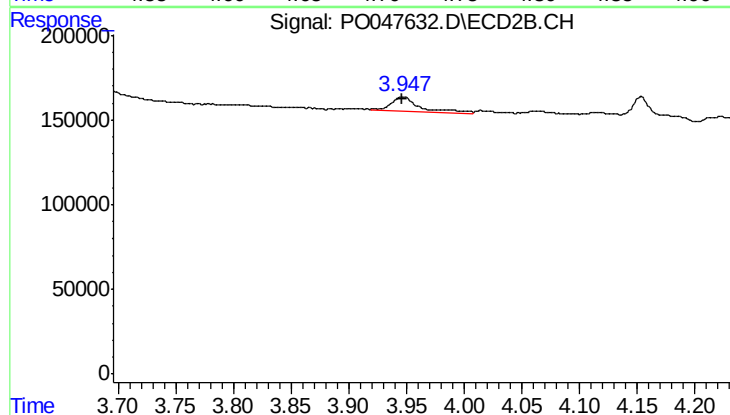


#9 AR-1221-2

R.T.: 3.947 min
Delta R.T.: 0.000 min
Response: 151600
Conc: 83.57 ng/ml

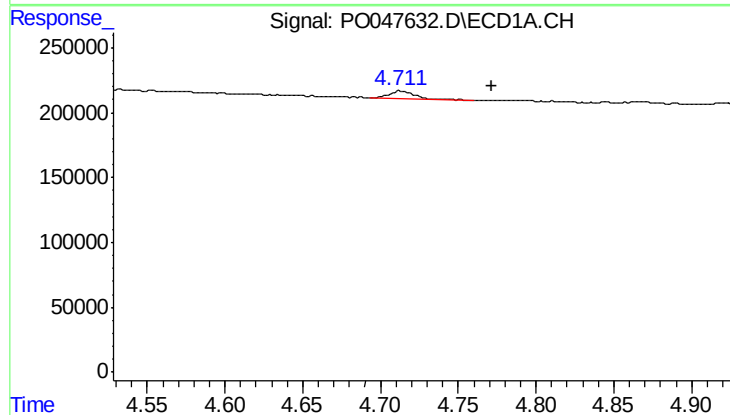


#10 AR-1221-3

R.T.: 4.713 min
Delta R.T.: -0.058 min
Response: 65553
Conc: 12.70 ng/ml

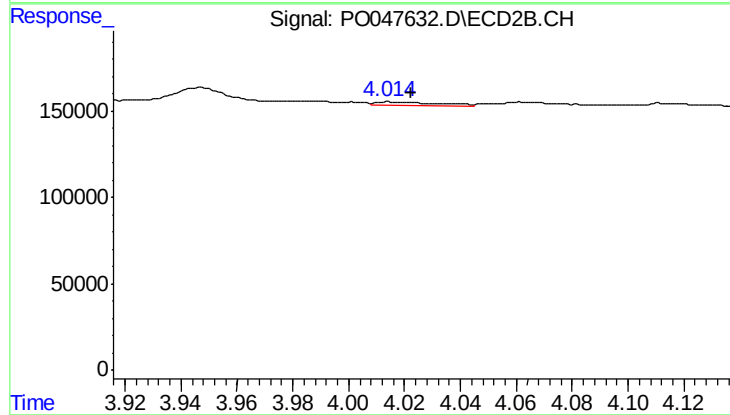

#10 AR-1221-3


R.T.: 4.016 min
Delta R.T.: -0.006 min
Response: 32289
Conc: 5.59 ng/ml

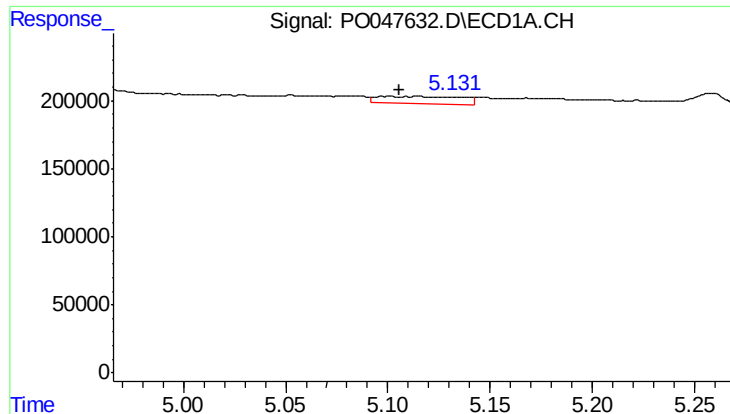

#11 AR-1232-1


R.T.: 5.101 min
Delta R.T.: -0.004 min
Response: 144920
Conc: 67.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-001-B

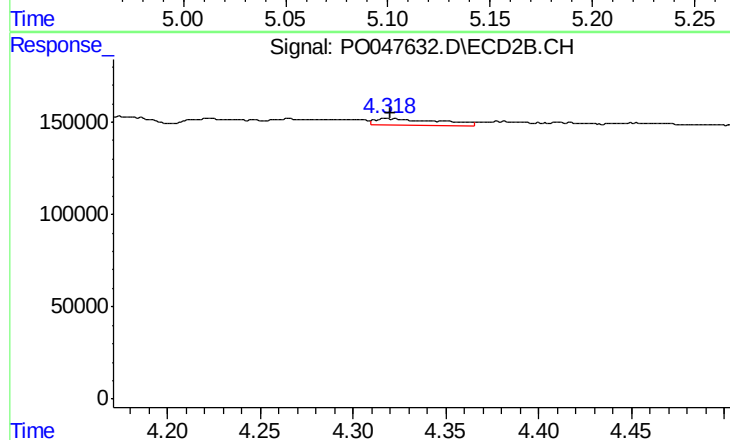


#11 AR-1232-1

R.T.: 4.320 min
Delta R.T.: 0.000 min
Response: 94074
Conc: 40.00 ng/ml

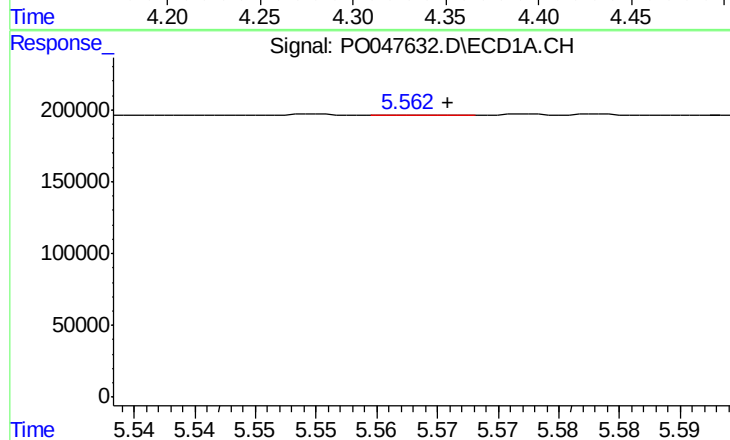


#12 AR-1232-2

R.T.: 5.564 min
Delta R.T.: -0.002 min
Response: 2287
Conc: 0.78 ng/ml

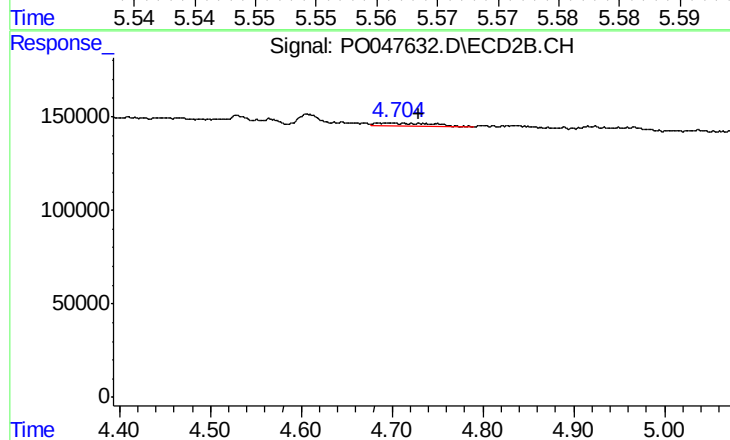

#12 AR-1232-2


R.T.: 4.701 min
Delta R.T.: -0.029 min
Response: 74591
Conc: 24.41 ng/ml

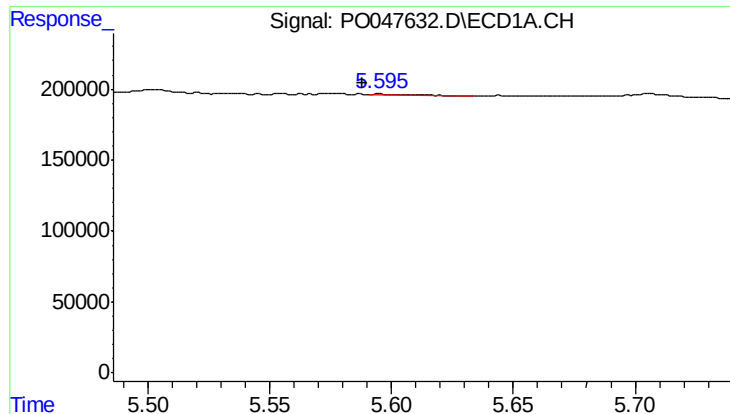

#13 AR-1232-3


R.T.: 5.595 min
Delta R.T.: 0.007 min
Response: 12090
Conc: 2.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-001-B

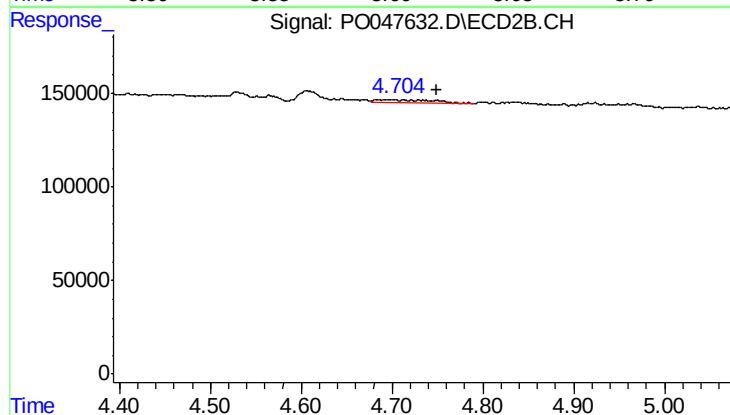


#13 AR-1232-3

R.T.: 4.701 min
Delta R.T.: -0.049 min
Response: 74591
Conc: 16.15 ng/ml

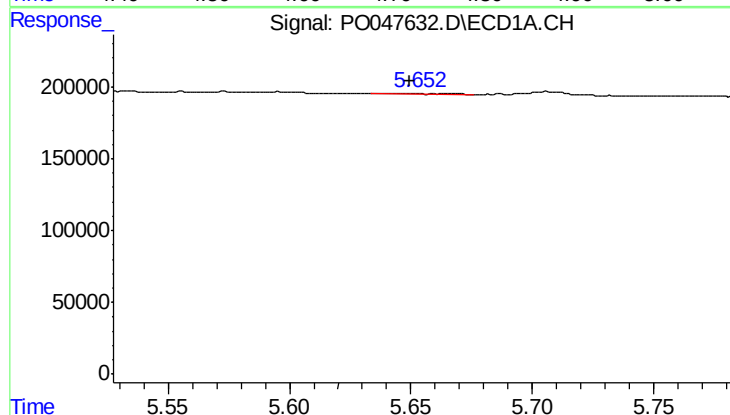


#14 AR-1232-4

R.T.: 5.644 min
Delta R.T.: -0.006 min
Response: 13683
Conc: 4.94 ng/ml

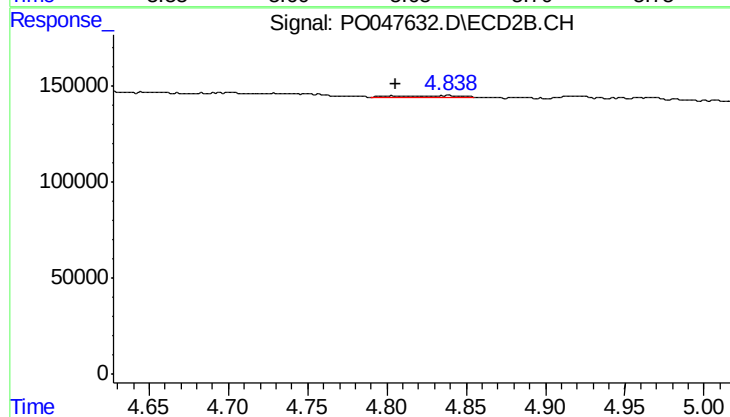

#14 AR-1232-4


R.T.: 4.810 min
Delta R.T.: 0.005 min
Response: 14218
Conc: 4.60 ng/ml

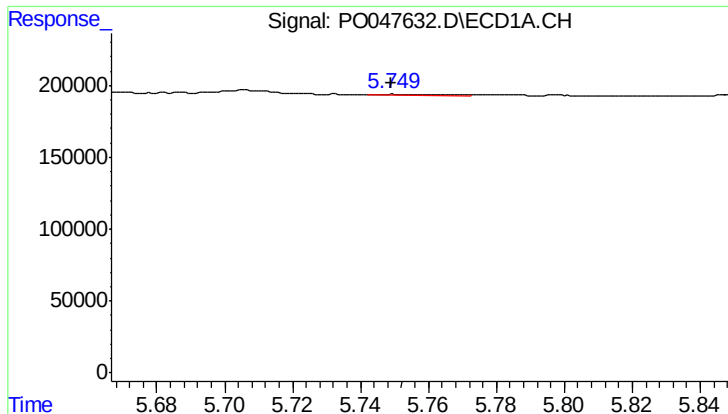

#15 AR-1232-5


R.T.: 5.749 min
Delta R.T.: 0.000 min
Response: 6580
Conc: 2.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-001-B

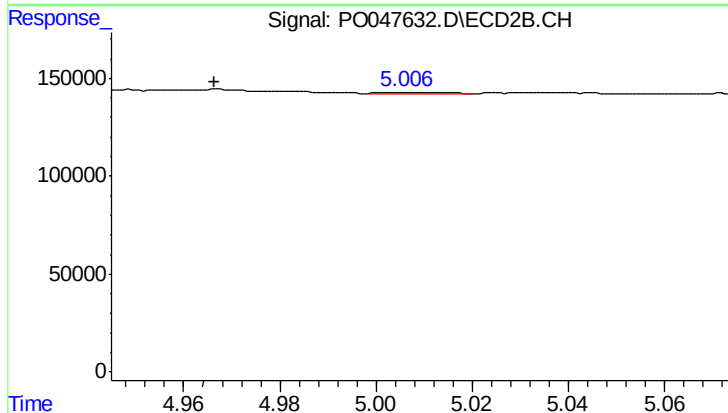


#15 AR-1232-5

R.T.: 5.006 min
Delta R.T.: 0.040 min
Response: 6757
Conc: 3.78 ng/ml

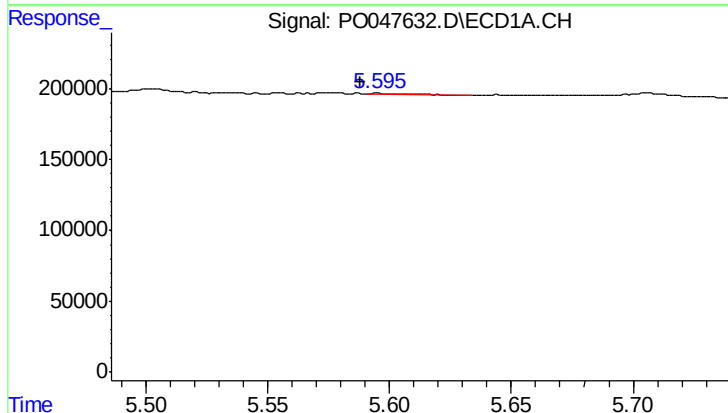


#16 AR-1242-1

R.T.: 5.595 min
Delta R.T.: 0.007 min
Response: 12090
Conc: 1.64 ng/ml

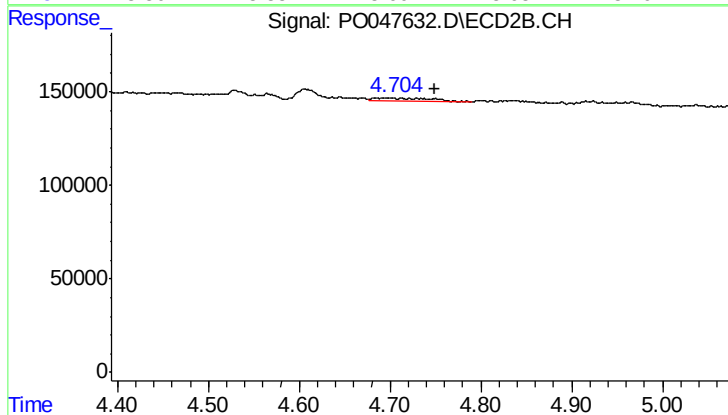

#16 AR-1242-1


R.T.: 4.701 min
Delta R.T.: -0.048 min
Response: 74591
Conc: 9.31 ng/ml

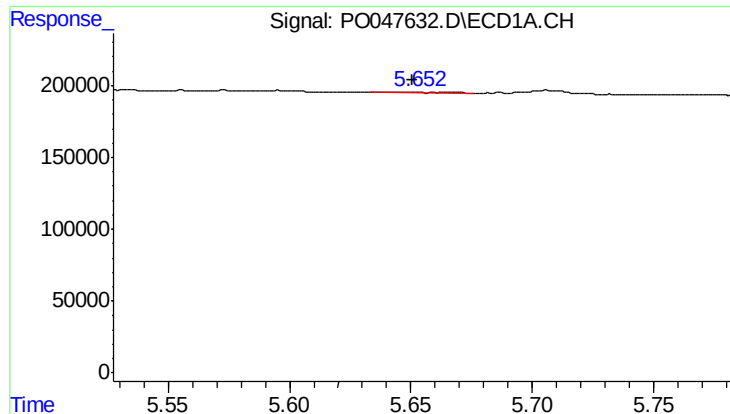

#17 AR-1242-2


R.T.: 5.644 min
Delta R.T.: -0.006 min
Response: 13683
Conc: 2.96 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-001-B

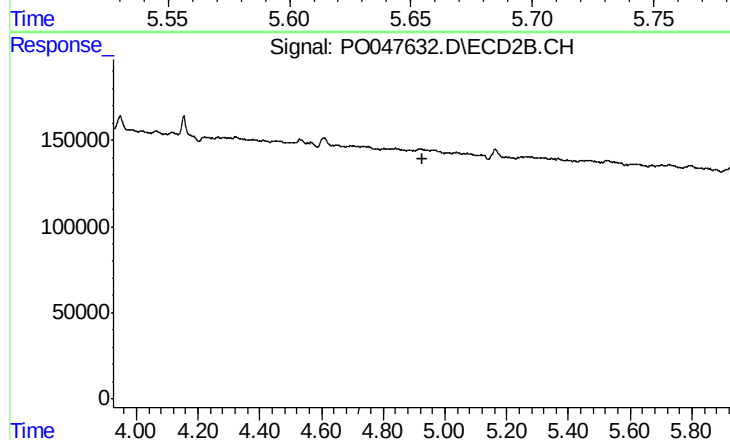


#17 AR-1242-2

R.T.: 0.000 min
Exp R.T.: 4.926 min
Response: 0
Conc: N.D.

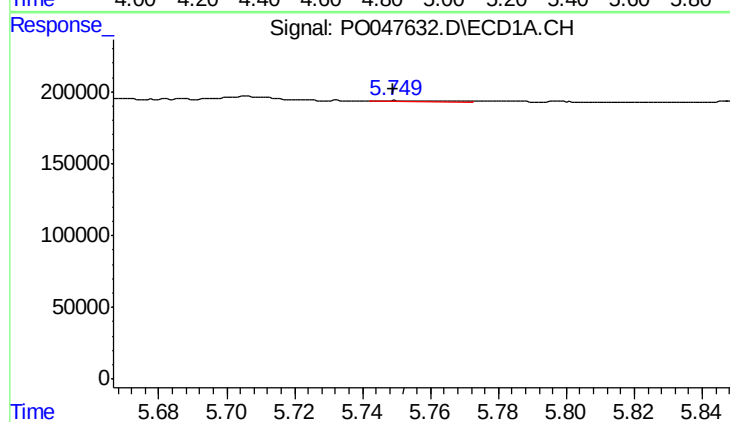


#18 AR-1242-3

R.T.: 5.749 min
Delta R.T.: 0.000 min
Response: 6580
Conc: 1.71 ng/ml

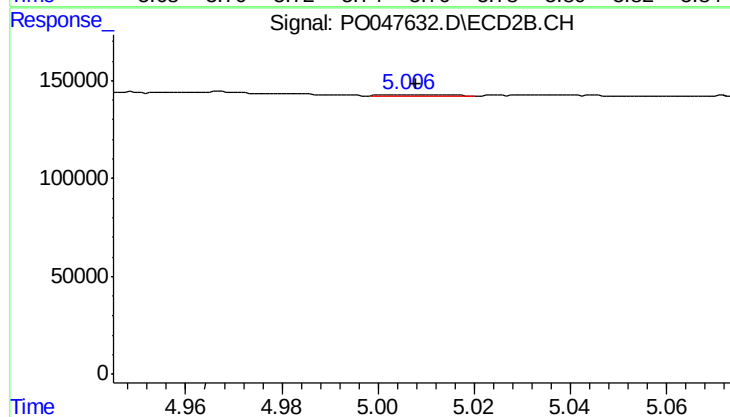

#18 AR-1242-3


R.T.: 5.006 min
Delta R.T.: -0.002 min
Response: 6757
Conc: 1.61 ng/ml

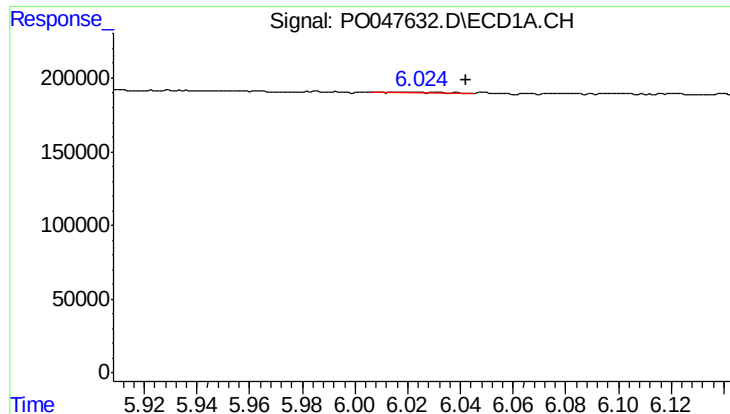

#19 AR-1242-4


R.T.: 6.024 min
Delta R.T.: -0.018 min
Response: 12447
Conc: 3.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-001-B

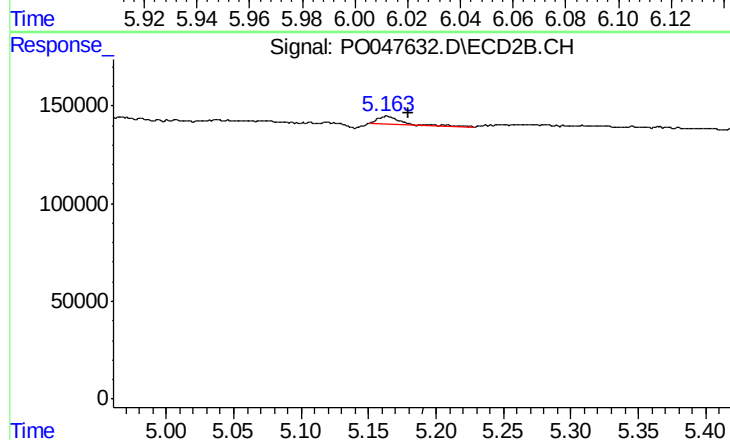


#19 AR-1242-4

R.T.: 5.164 min
Delta R.T.: -0.016 min
Response: 39147
Conc: 8.29 ng/ml

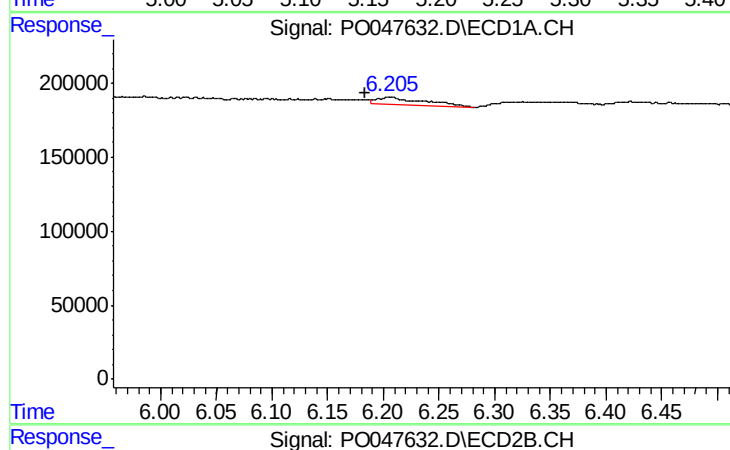


#20 AR-1242-5

R.T.: 6.206 min
Delta R.T.: 0.023 min
Response: 150045
Conc: 35.05 ng/ml

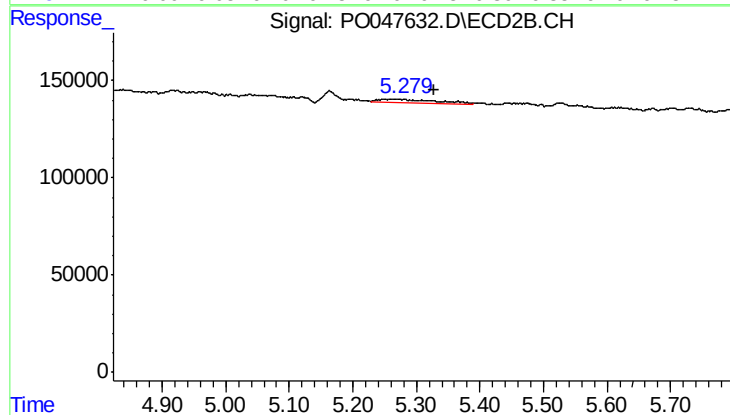

#20 AR-1242-5


R.T.: 5.279 min
Delta R.T.: -0.050 min
Response: 111389
Conc: 28.77 ng/ml

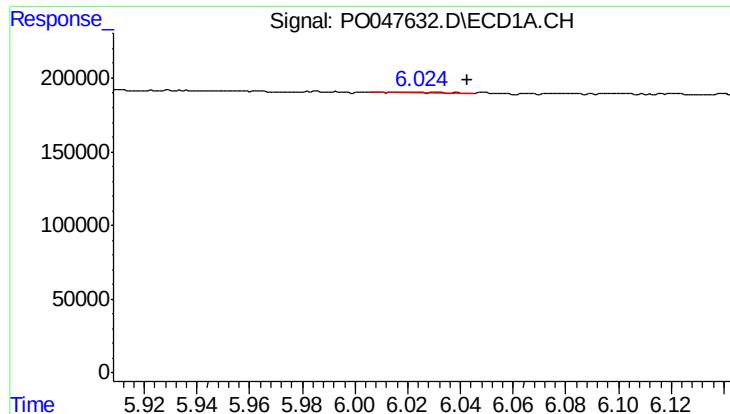

#21 AR-1248-1


R.T.: 6.024 min
Delta R.T.: -0.019 min
Response: 12447
Conc: 1.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-001-B

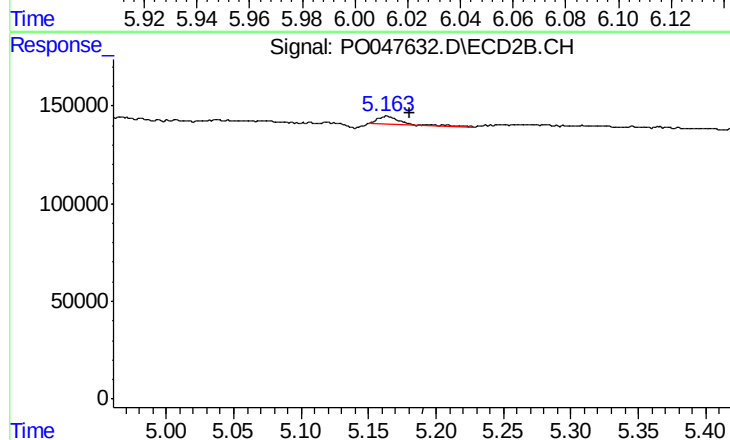


#21 AR-1248-1

R.T.: 5.164 min
Delta R.T.: -0.017 min
Response: 39147
Conc: 5.25 ng/ml

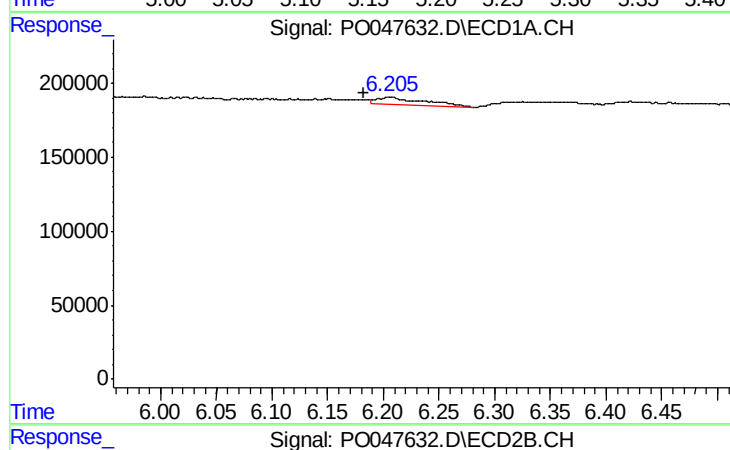


#22 AR-1248-2

R.T.: 6.206 min
Delta R.T.: 0.024 min
Response: 150045
Conc: 27.54 ng/ml

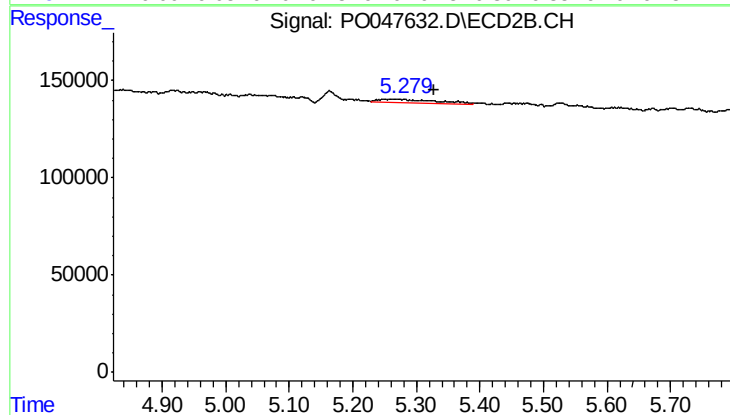

#22 AR-1248-2


R.T.: 5.279 min
Delta R.T.: -0.049 min
Response: 111389
Conc: 20.82 ng/ml

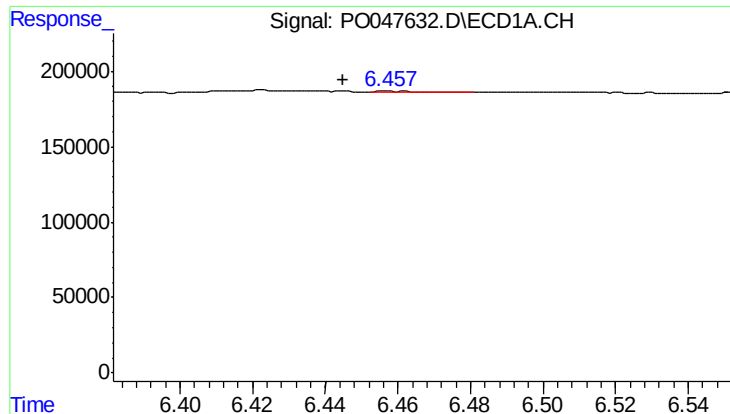

#23 AR-1248-3


R.T.: 6.457 min
Delta R.T.: 0.013 min
Response: 11328
Conc: 1.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-001-B

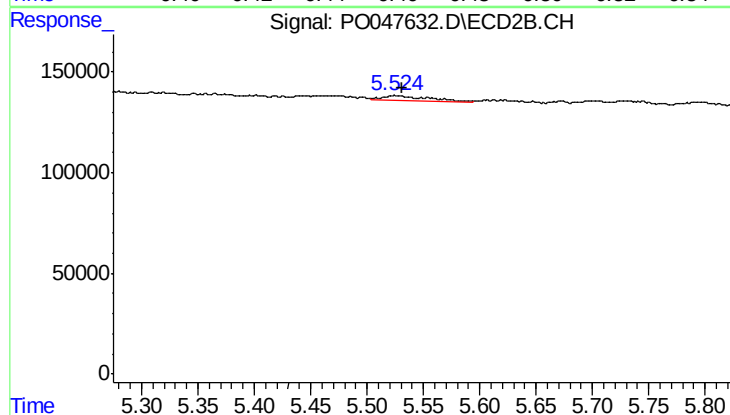


#23 AR-1248-3

R.T.: 5.526 min
Delta R.T.: -0.005 min
Response: 67474
Conc: 6.78 ng/ml

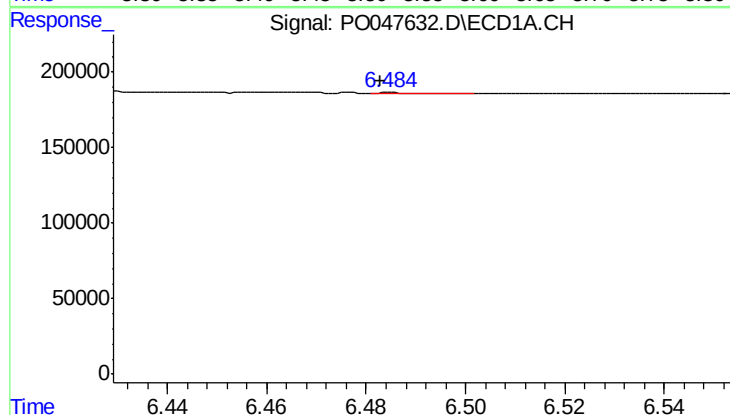


#24 AR-1248-4

R.T.: 6.485 min
Delta R.T.: 0.002 min
Response: 4176
Conc: 0.62 ng/ml

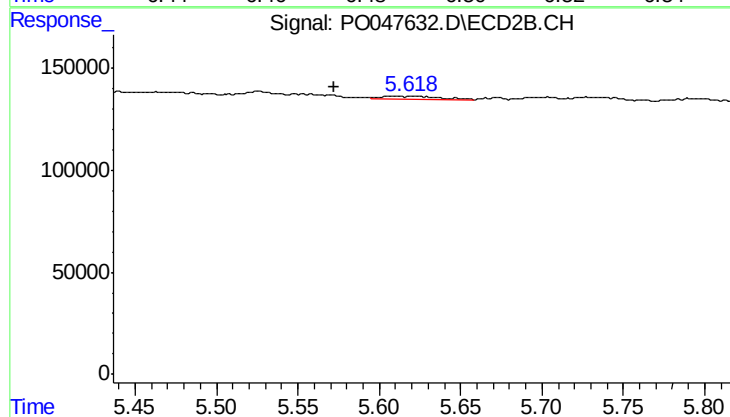

#24 AR-1248-4


R.T.: 5.609 min
Delta R.T.: 0.036 min
Response: 26422
Conc: 3.77 ng/ml

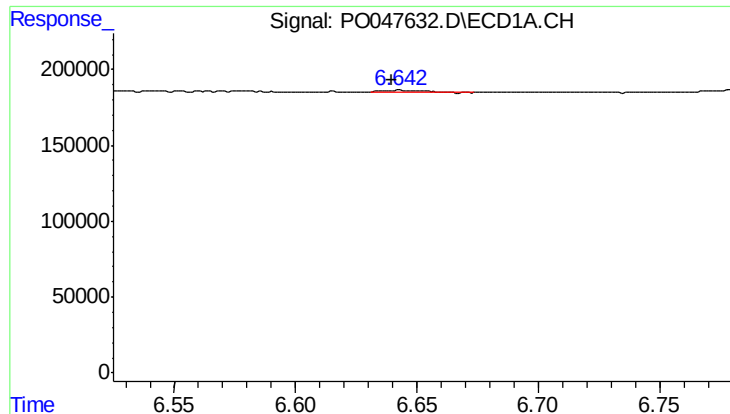

#25 AR-1248-5


R.T.: 6.643 min
Delta R.T.: 0.003 min
Response: 20235
Conc: 2.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-001-B

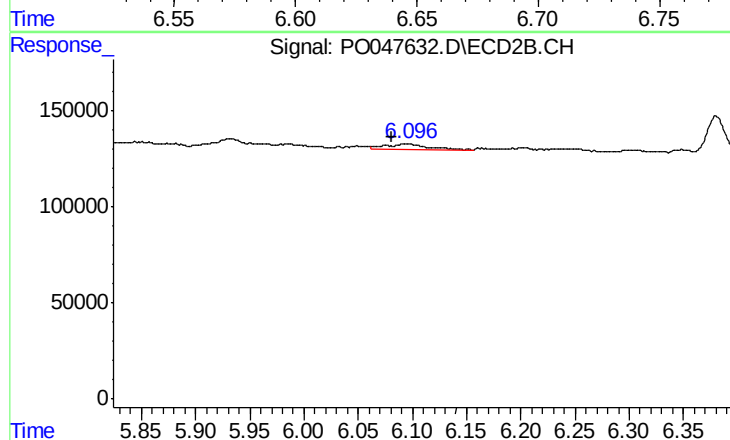


#25 AR-1248-5

R.T.: 6.095 min
Delta R.T.: 0.013 min
Response: 89526
Conc: 18.79 ng/ml

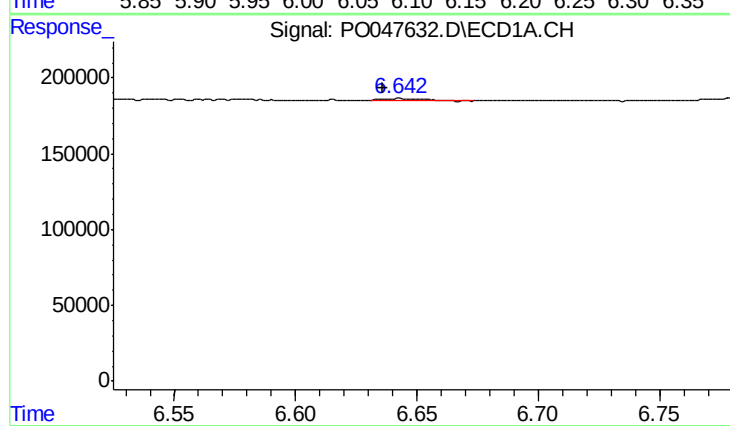


#26 AR-1254-1

R.T.: 6.643 min
Delta R.T.: 0.007 min
Response: 20235
Conc: 1.65 ng/ml

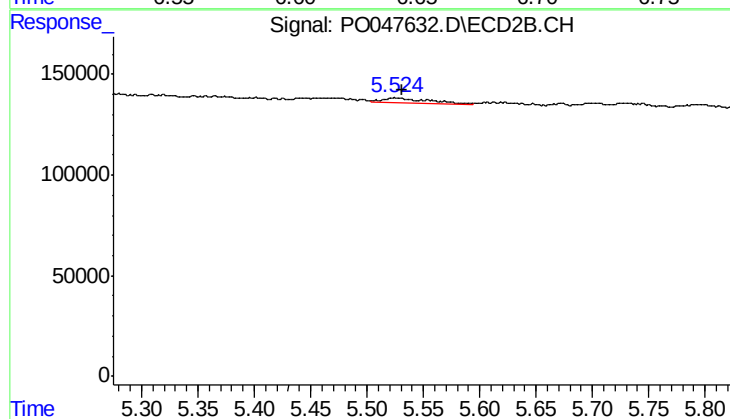

#26 AR-1254-1


R.T.: 5.526 min
Delta R.T.: -0.006 min
Response: 67474
Conc: 5.48 ng/ml

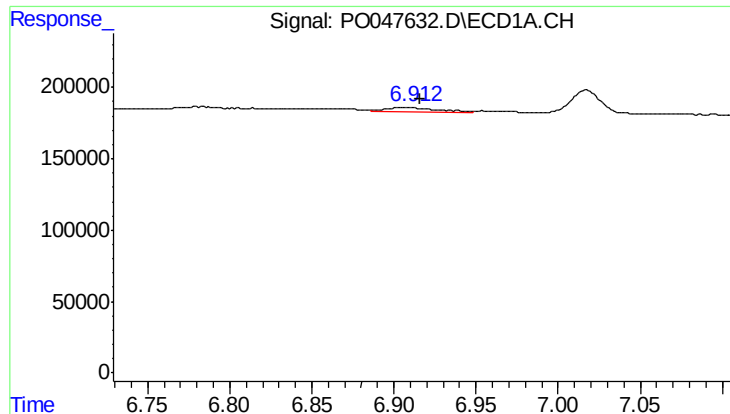

#27 AR-1254-2


R.T.: 6.911 min
Delta R.T.: -0.005 min
Response: 74681
Conc: 10.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-001-B

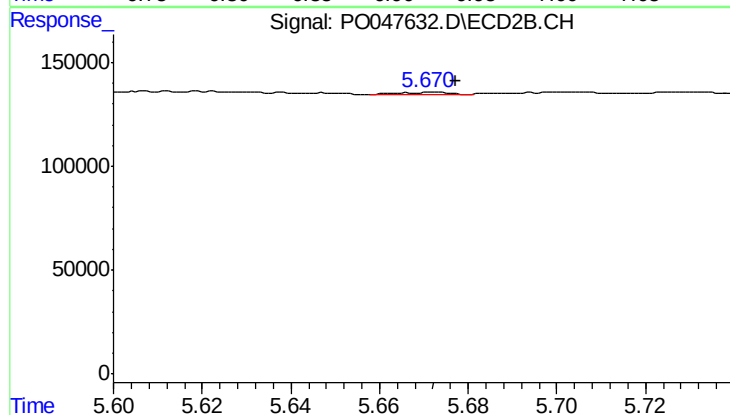


#27 AR-1254-2

R.T.: 5.672 min
Delta R.T.: -0.005 min
Response: 6433
Conc: 0.62 ng/ml

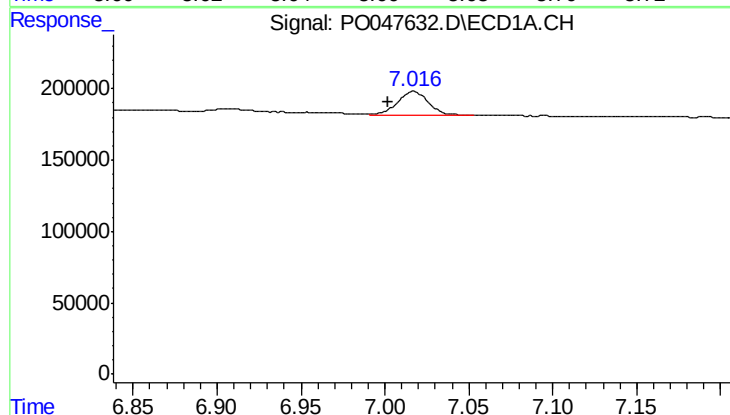


#28 AR-1254-3

R.T.: 7.017 min
Delta R.T.: 0.015 min
Response: 211834
Conc: 16.24 ng/ml

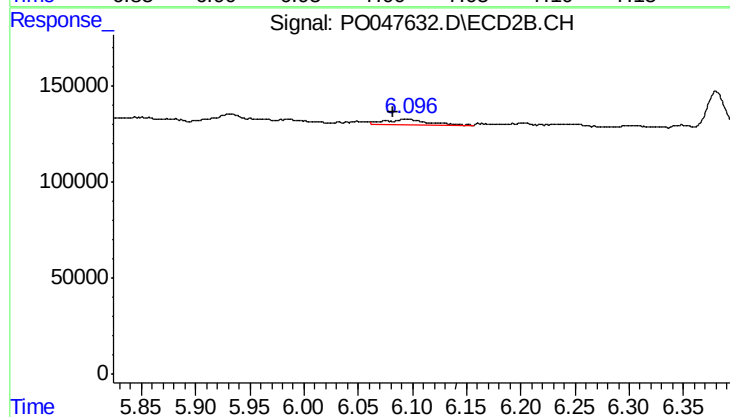

#28 AR-1254-3


R.T.: 6.095 min
Delta R.T.: 0.013 min
Response: 89526
Conc: 5.16 ng/ml

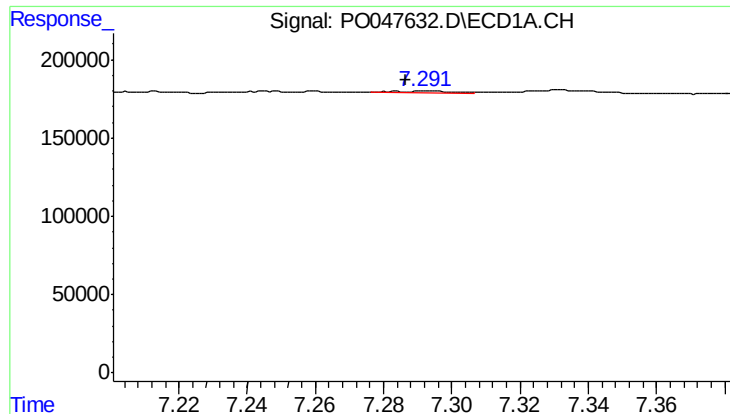

#29 AR-1254-4


R.T.: 7.292 min
Delta R.T.: 0.006 min
Response: 11793
Conc: 1.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-001-B

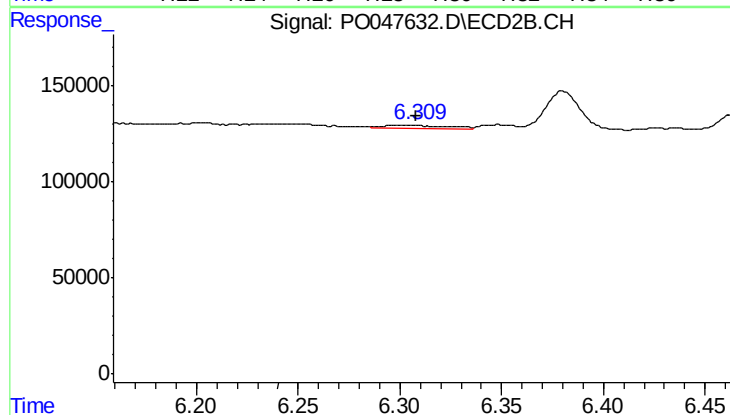


#29 AR-1254-4

R.T.: 6.307 min
Delta R.T.: -0.001 min
Response: 34932
Conc: 3.22 ng/ml

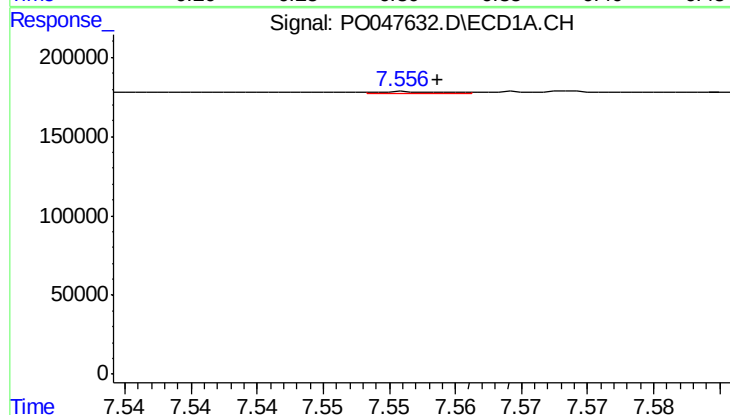


#30 AR-1254-5

R.T.: 7.557 min
Delta R.T.: -0.002 min
Response: 3771
Conc: 0.51 ng/ml

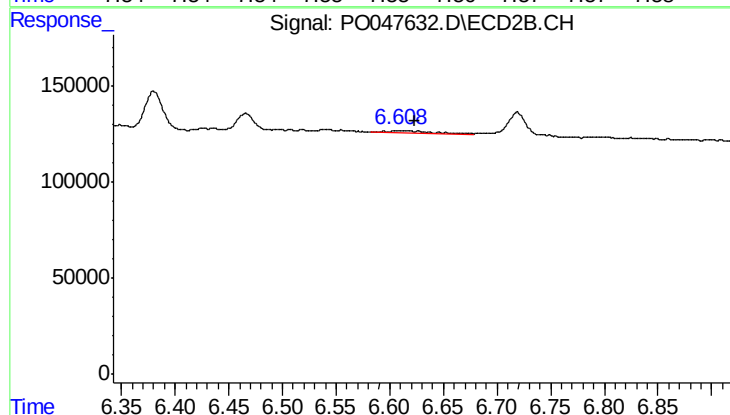

#30 AR-1254-5


R.T.: 6.609 min
Delta R.T.: -0.014 min
Response: 54020
Conc: 7.06 ng/ml

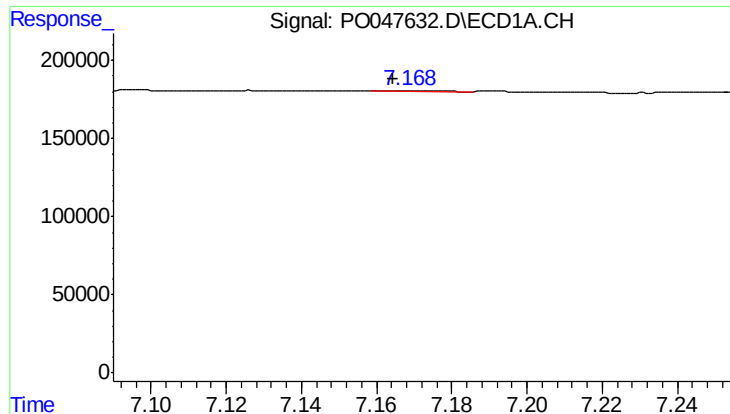

#31 AR-1260-1


R.T.: 7.168 min
Delta R.T.: 0.003 min
Response: 6603
Conc: 0.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-001-B

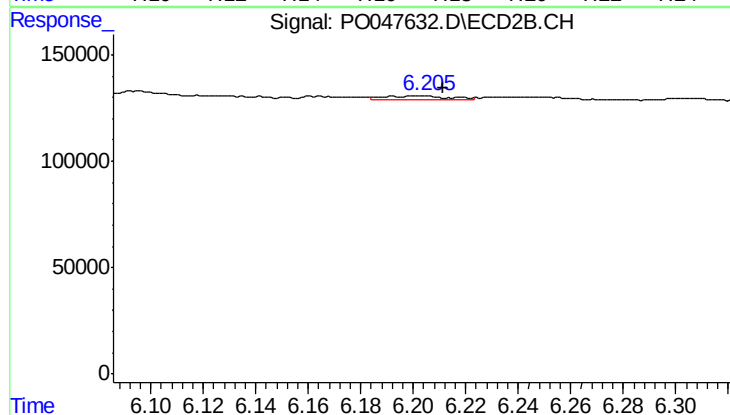


#31 AR-1260-1

R.T.: 6.203 min
Delta R.T.: -0.008 min
Response: 32790
Conc: 2.97 ng/ml

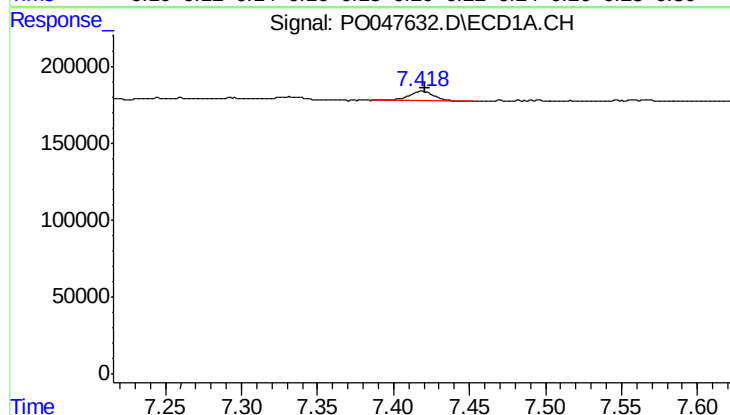


#32 AR-1260-2

R.T.: 7.418 min
Delta R.T.: -0.003 min
Response: 78140
Conc: 7.01 ng/ml

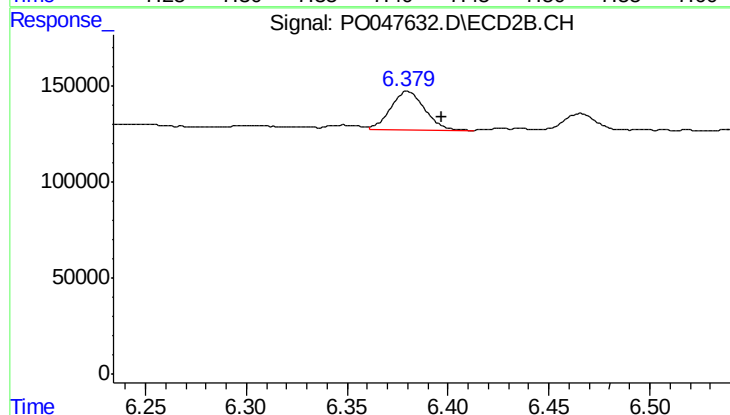

#32 AR-1260-2


R.T.: 6.380 min
Delta R.T.: -0.017 min
Response: 235713
Conc: 17.58 ng/ml

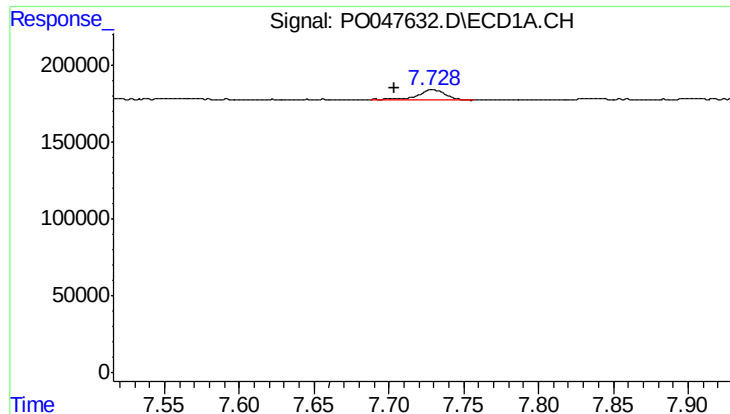

#33 AR-1260-3


R.T.: 7.729 min
Delta R.T.: 0.026 min
Response: 98395
Conc: 7.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-001-B

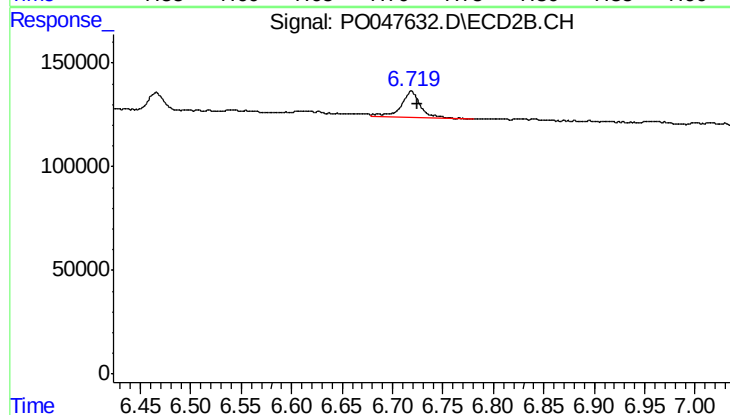


#33 AR-1260-3

R.T.: 6.719 min
Delta R.T.: -0.006 min
Response: 169757
Conc: 11.68 ng/ml

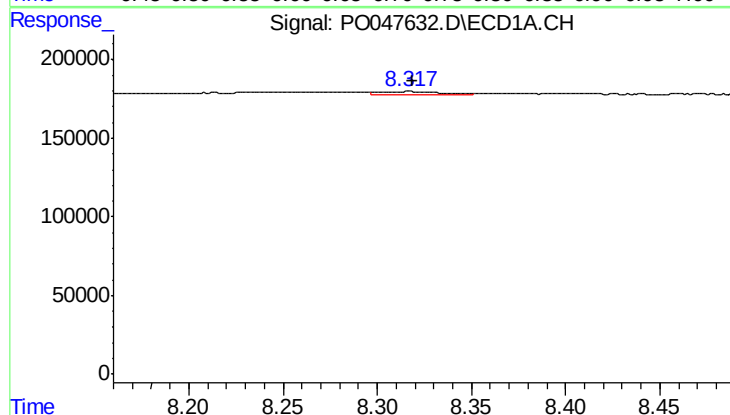


#34 AR-1260-4

R.T.: 8.317 min
Delta R.T.: -0.002 min
Response: 46450
Conc: 2.61 ng/ml

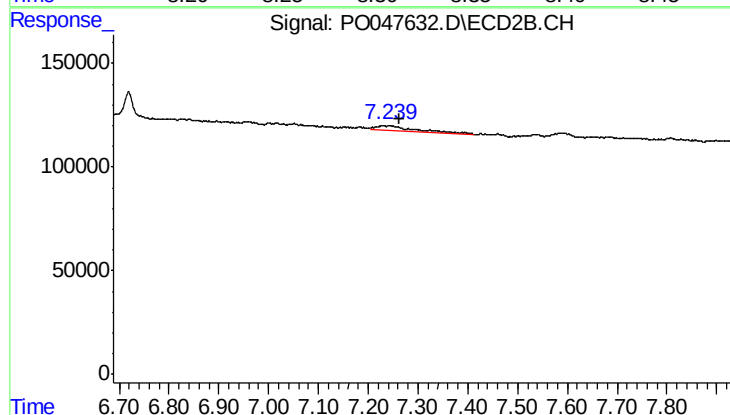

#34 AR-1260-4


R.T.: 7.231 min
Delta R.T.: -0.031 min
Response: 109882
Conc: 4.99 ng/ml

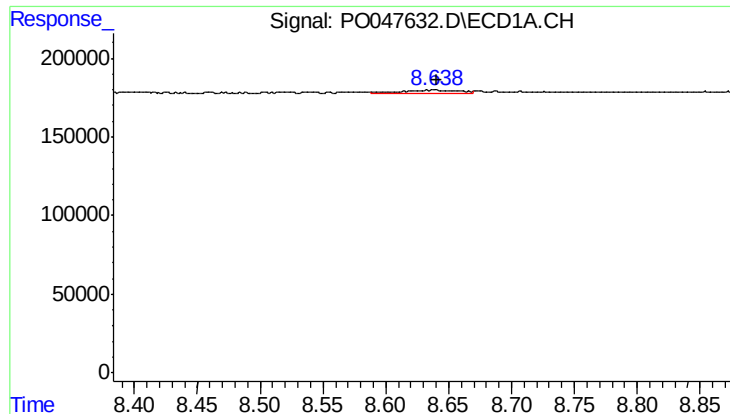

#35 AR-1260-5


R.T.: 8.638 min
Delta R.T.: -0.002 min
Response: 53948
Conc: 4.72 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-001-B

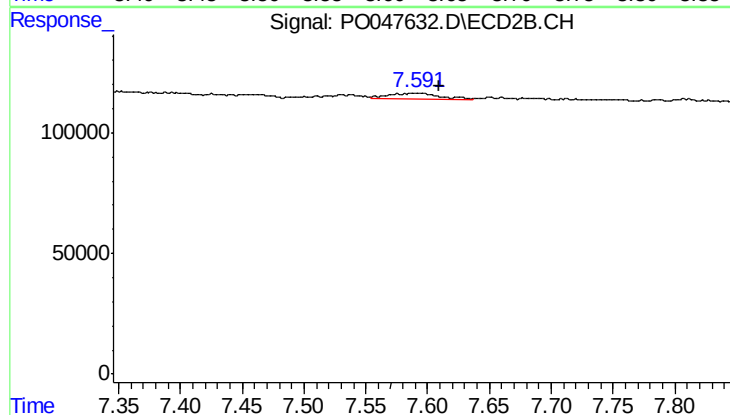


#35 AR-1260-5

R.T.: 7.592 min
Delta R.T.: -0.017 min
Response: 81645
Conc: 5.23 ng/ml

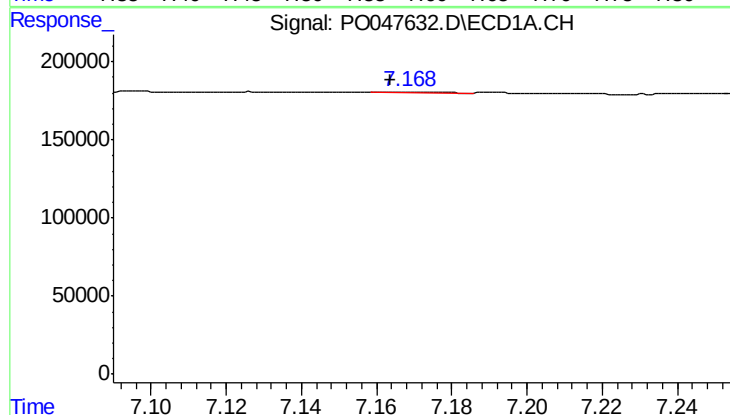


#36 AR-1262-1

R.T.: 7.168 min
Delta R.T.: 0.004 min
Response: 6603
Conc: 0.80 ng/ml

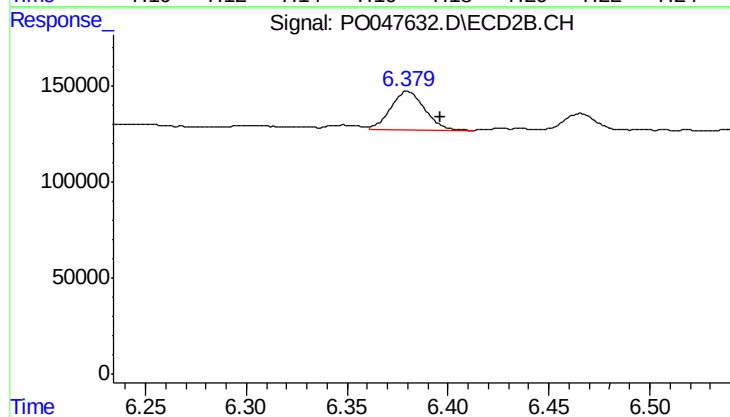

#36 AR-1262-1


R.T.: 6.380 min
Delta R.T.: -0.016 min
Response: 235713
Conc: 20.79 ng/ml

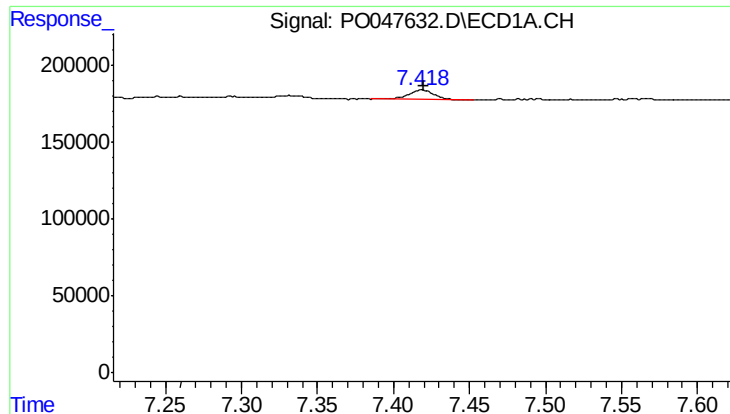

#37 AR-1262-2


R.T.: 7.418 min
Delta R.T.: -0.001 min
Response: 78140
Conc: 8.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-001-B

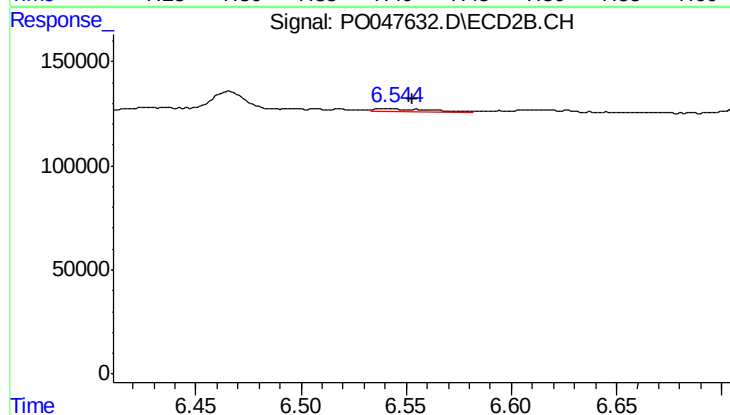


#37 AR-1262-2

R.T.: 6.541 min
Delta R.T.: -0.012 min
Response: 21008
Conc: 1.86 ng/ml

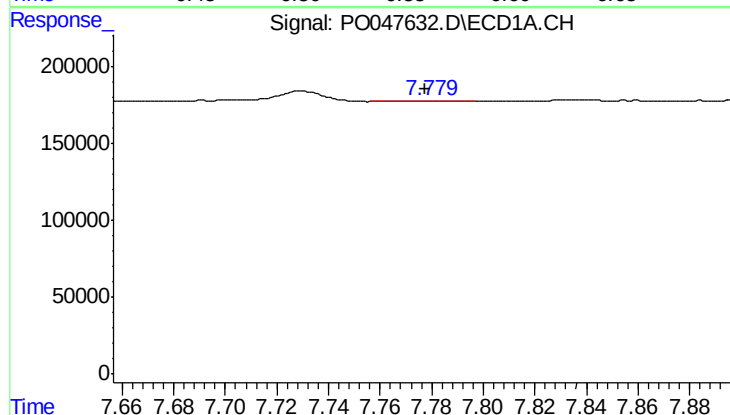


#38 AR-1262-3

R.T.: 7.780 min
Delta R.T.: 0.002 min
Response: 6518
Conc: 0.53 ng/ml

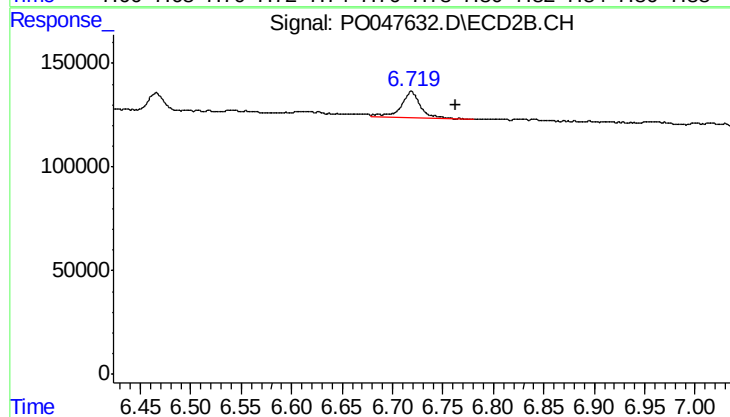

#38 AR-1262-3


R.T.: 6.719 min
Delta R.T.: -0.044 min
Response: 169757
Conc: 11.25 ng/ml

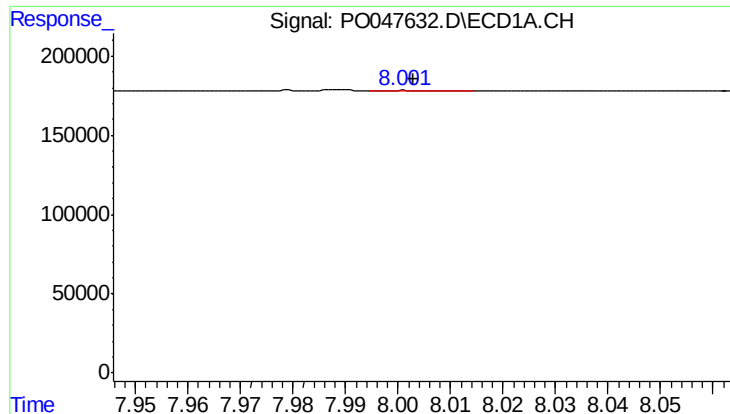

#39 AR-1262-4


R.T.: 8.000 min
Delta R.T.: -0.003 min
Response: 7100
Conc: 0.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-001-B

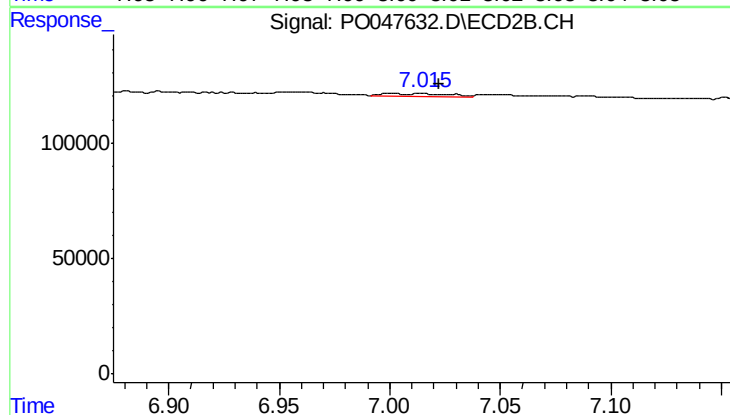


#39 AR-1262-4

R.T.: 7.015 min
Delta R.T.: -0.007 min
Response: 22326
Conc: 1.70 ng/ml

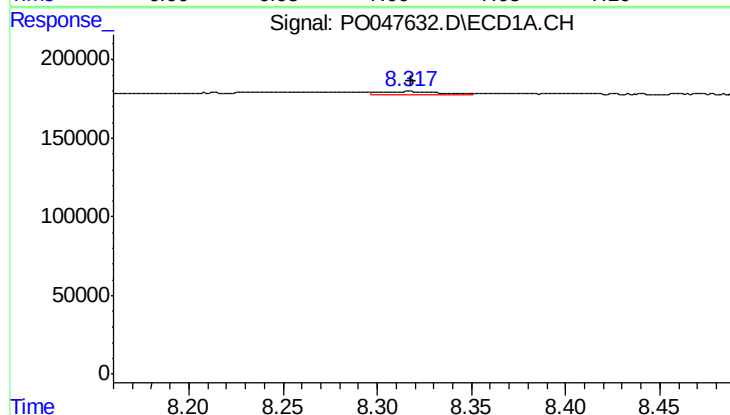


#40 AR-1262-5

R.T.: 8.317 min
Delta R.T.: -0.001 min
Response: 46450
Conc: 2.16 ng/ml

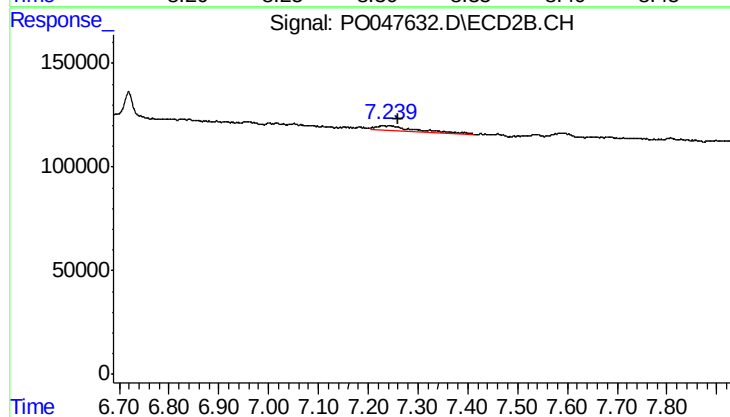

#40 AR-1262-5


R.T.: 7.231 min
Delta R.T.: -0.030 min
Response: 109882
Conc: 4.25 ng/ml

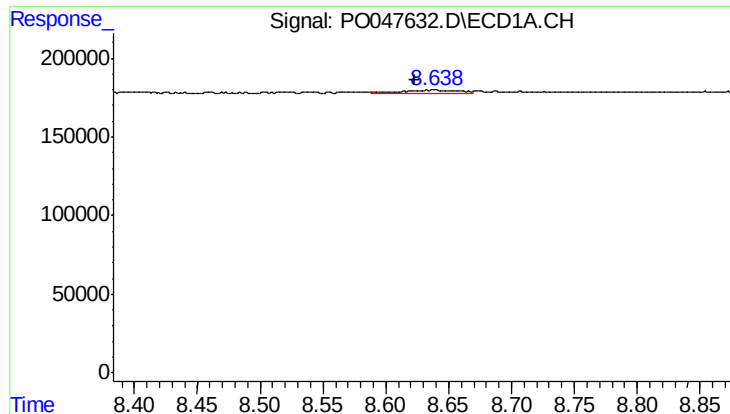

#41 AR-1268-1


R.T.: 8.638 min
Delta R.T.: 0.016 min
Response: 53948
Conc: 2.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-001-B

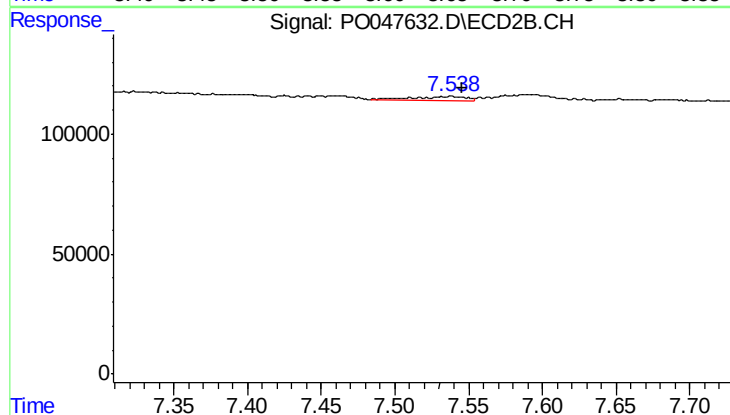


#41 AR-1268-1

R.T.: 7.538 min
Delta R.T.: -0.008 min
Response: 38991
Conc: 1.50 ng/ml

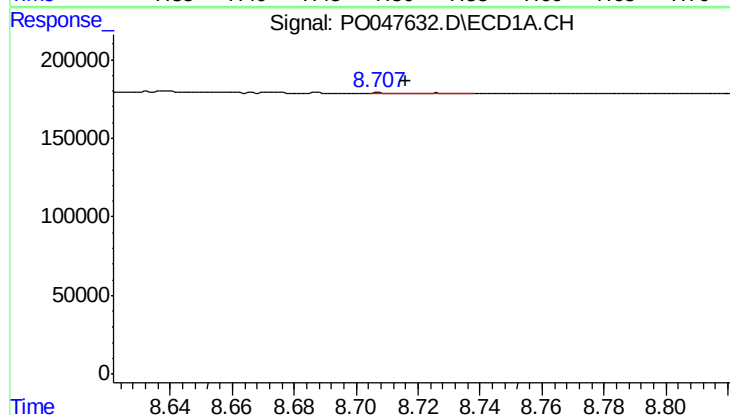


#42 AR-1268-2

R.T.: 8.707 min
Delta R.T.: -0.009 min
Response: 11183
Conc: 0.52 ng/ml

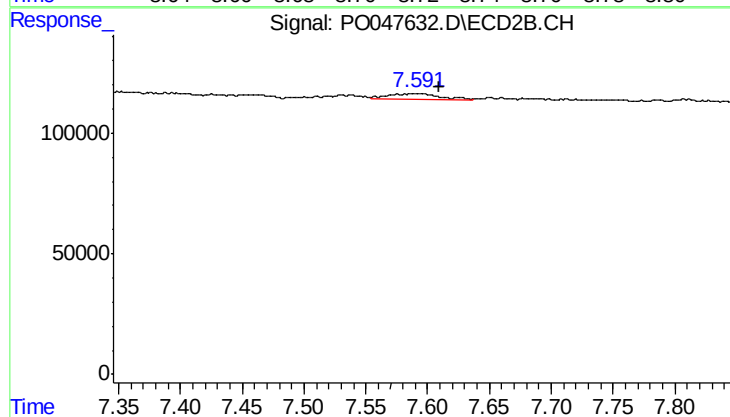

#42 AR-1268-2


R.T.: 7.592 min
Delta R.T.: -0.018 min
Response: 81645
Conc: 3.28 ng/ml

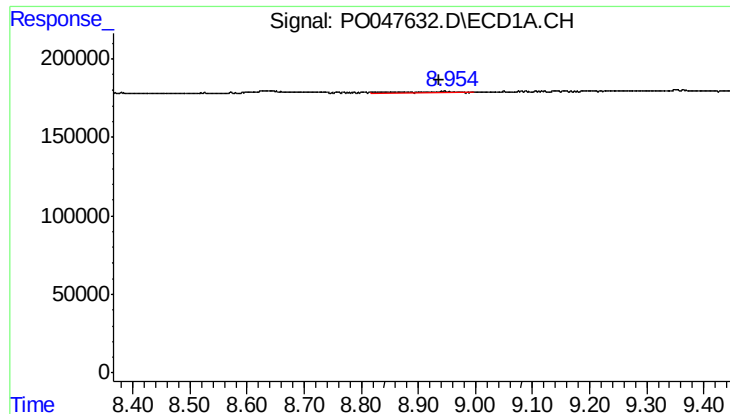

#43 AR-1268-3


R.T.: 8.945 min
Delta R.T.: 0.007 min
Response: 44555
Conc: 2.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-001-B

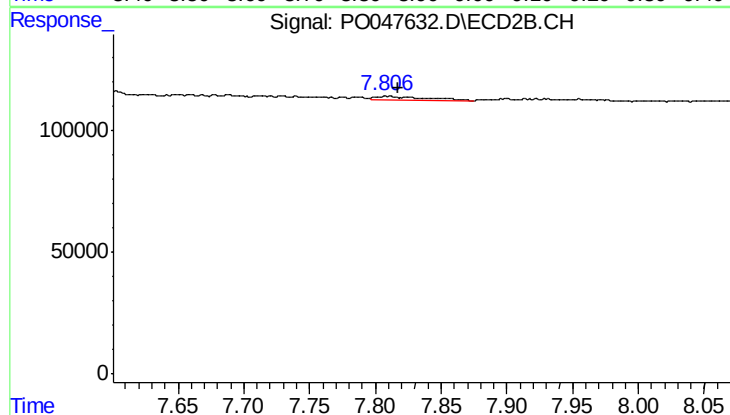


#43 AR-1268-3

R.T.: 7.808 min
Delta R.T.: -0.009 min
Response: 36237
Conc: 1.84 ng/ml

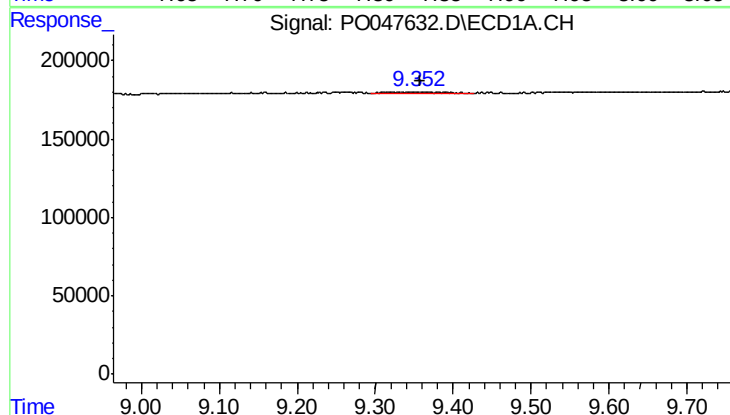


#44 AR-1268-4

R.T.: 9.352 min
Delta R.T.: -0.006 min
Response: 53461
Conc: 6.70 ng/ml

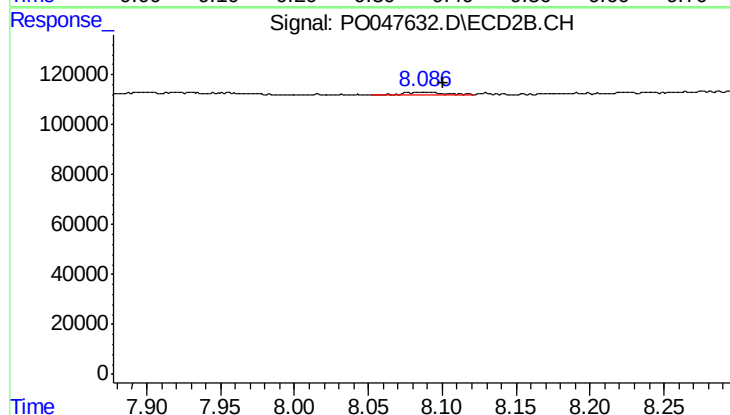

#44 AR-1268-4


R.T.: 8.087 min
Delta R.T.: -0.013 min
Response: 21021
Conc: 2.51 ng/ml

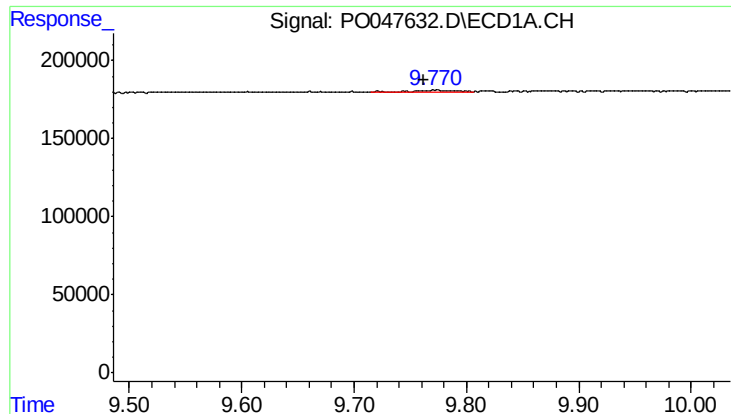

#45 AR-1268-5

R.T.: 9.773 min
Delta R.T.: 0.010 min
Response: 37287
Conc: 0.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-001-B

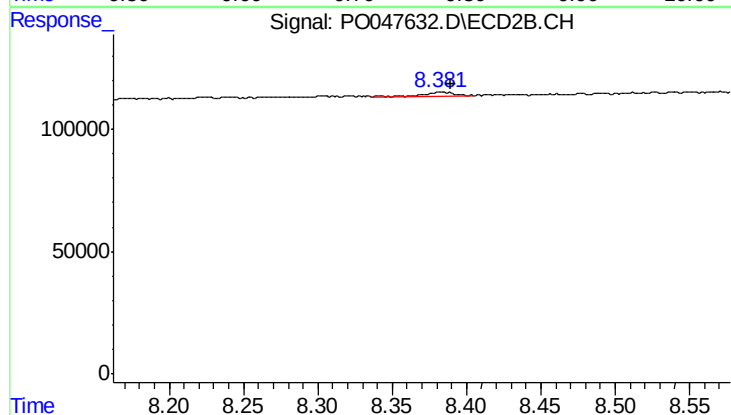

#45 AR-1268-5

R.T.: 8.383 min
Delta R.T.: -0.007 min
Response: 23123
Conc: 0.42 ng/ml