

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0080318\
Data File : P0047659.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Aug 2018 22:22
Operator : SM/SJ
Sample : J4310-01
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
C-1

Manual Integrations
APPROVED

Sohil
8/6/2018 12:41:09 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 04:27:06 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 27 02:33:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.398	3.643	3646163	4392450	18.059m	17.876
2) SA Decachlor...	10.088	8.630	2026419	2080730	12.424	13.237

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0080318\
Data File : P0047659.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Aug 2018 22:22
Operator : SM/SJ
Sample : J4310-01
Misc :
ALS Vial : 37 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
C-1


Manual Integrations
APPROVED

Sohil
8/6/2018 12:41:09 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 04:27:06 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 27 02:33:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

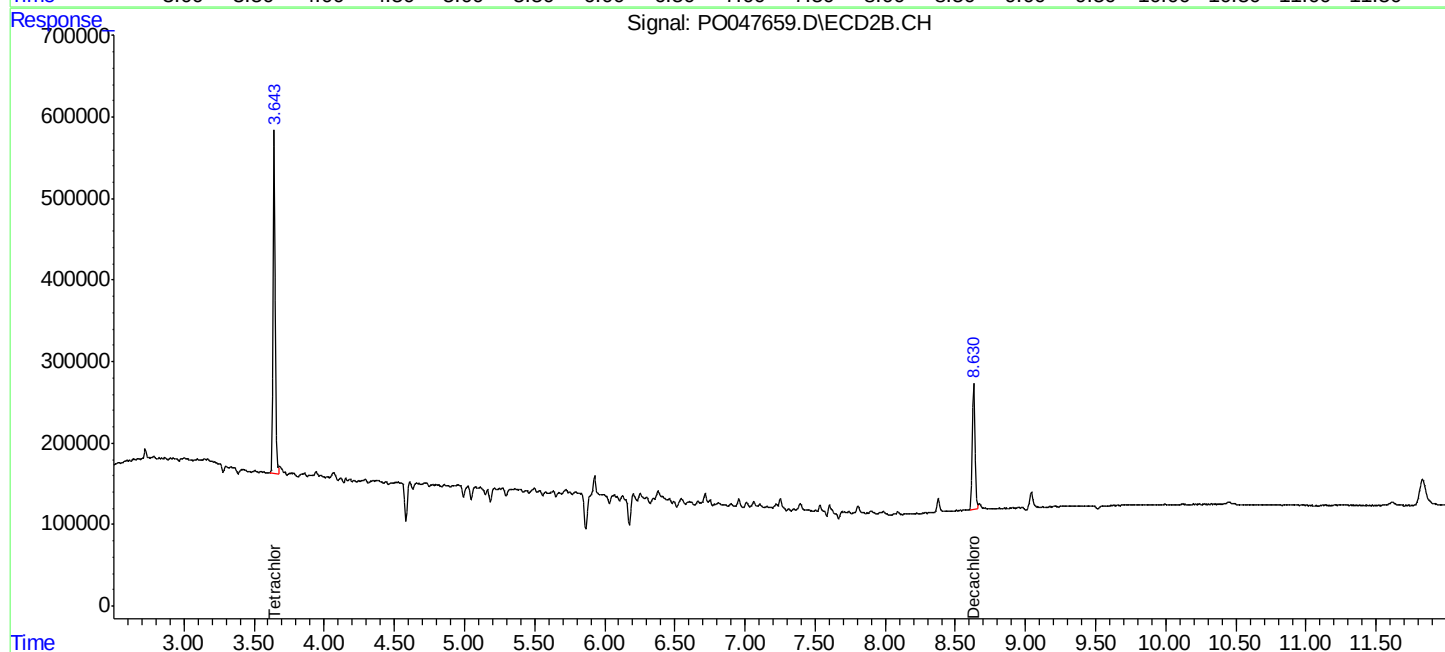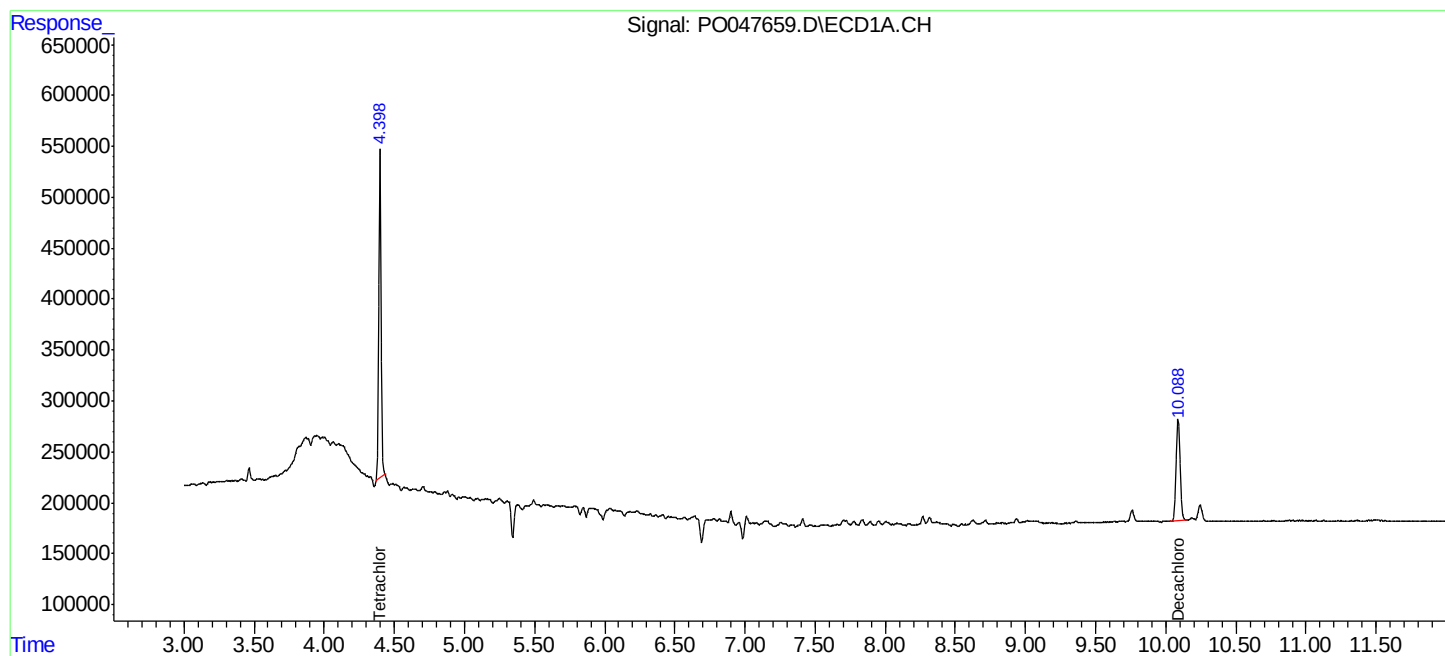

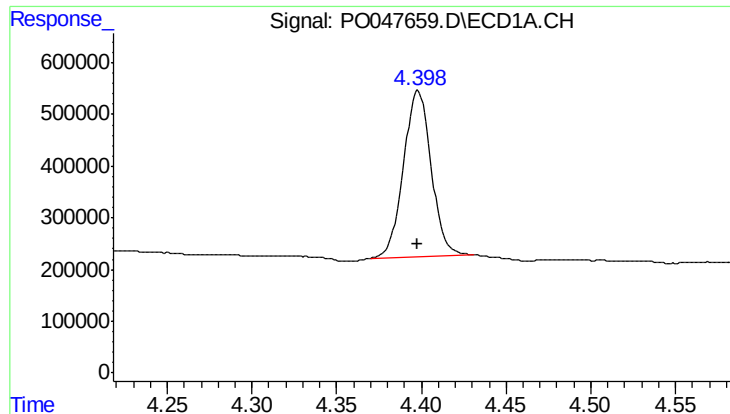


#1 Tetrachloro-m-xylene

R.T.: 4.398 min
Delta R.T.: 0.000 min
Response: 3646163
Conc: 18.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
C-1


Manual Integrations
APPROVED

Sohil
8/6/2018 12:41:09 PM

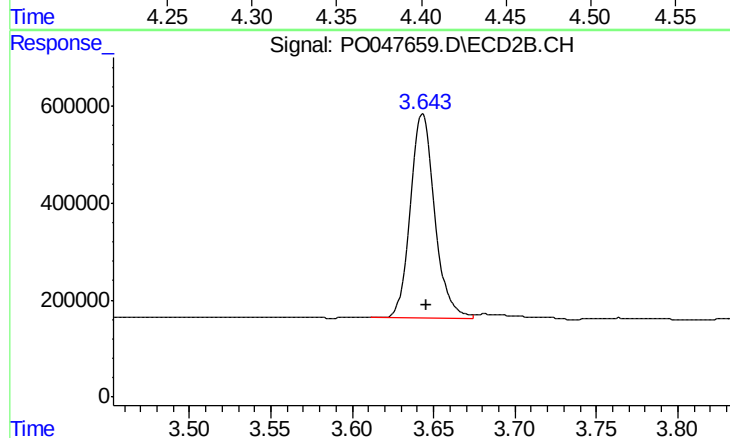


#1 Tetrachloro-m-xylene

R.T.: 3.643 min
Delta R.T.: -0.002 min
Response: 4392450
Conc: 17.88 ng/ml

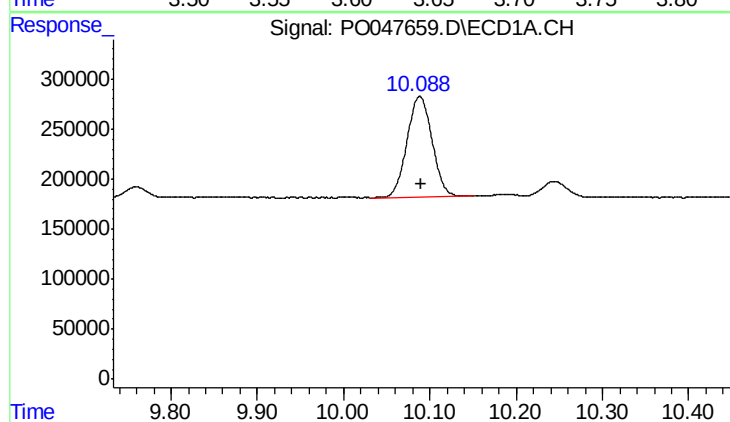

#2 Decachlorobiphenyl

R.T.: 10.088 min
Delta R.T.: -0.002 min
Response: 2026419
Conc: 12.42 ng/ml

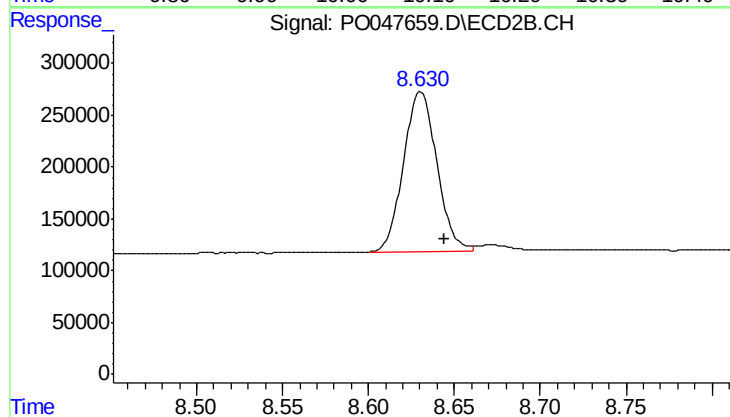

#2 Decachlorobiphenyl

R.T.: 8.630 min
Delta R.T.: -0.014 min
Response: 2080730
Conc: 13.24 ng/ml